

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 16:06
 Operator : AJ\SJ
 Sample : PB115762TB
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB115762TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:01:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	125.4E6	64466995	20.446	21.751
28)	SA Decachlor...	8.202	9.231	129.0E6	58606369	19.761	22.467
Target Compounds							
2)	A alpha-BHC	3.896	4.452f	4376531	357203	0.463	0.079 #
6)	B beta-BHC	0.000	4.902f	0	4312545	N.D.	2.547 #
7)	B delta-BHC	0.000	5.157	0	49500021	N.D.	11.518 #
8)	B Heptachlo...	0.000	5.991	0	50289058	N.D.	13.262 #
9)	A Endosulfan I	0.000	6.366	0	924366	N.D.	0.272 #
11)	B alpha-Chl...	0.000	6.299	0	269411	N.D.	0.075 #
15)	B Endosulfa...	6.228f	0.000	8754807	0	1.316	N.D. #
23)	Chlordane-1	4.363	5.157	2712600	49500021	10.095	350.237 #
26)	Chlordane-4	0.000	6.299	0	269411	N.D.	0.472 #
27)	Chlordane-5	6.228	0.000	8754807	0	36.500	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 16:06
Operator : AJ\SJ
Sample : PB115762TB
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB115762TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:01:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

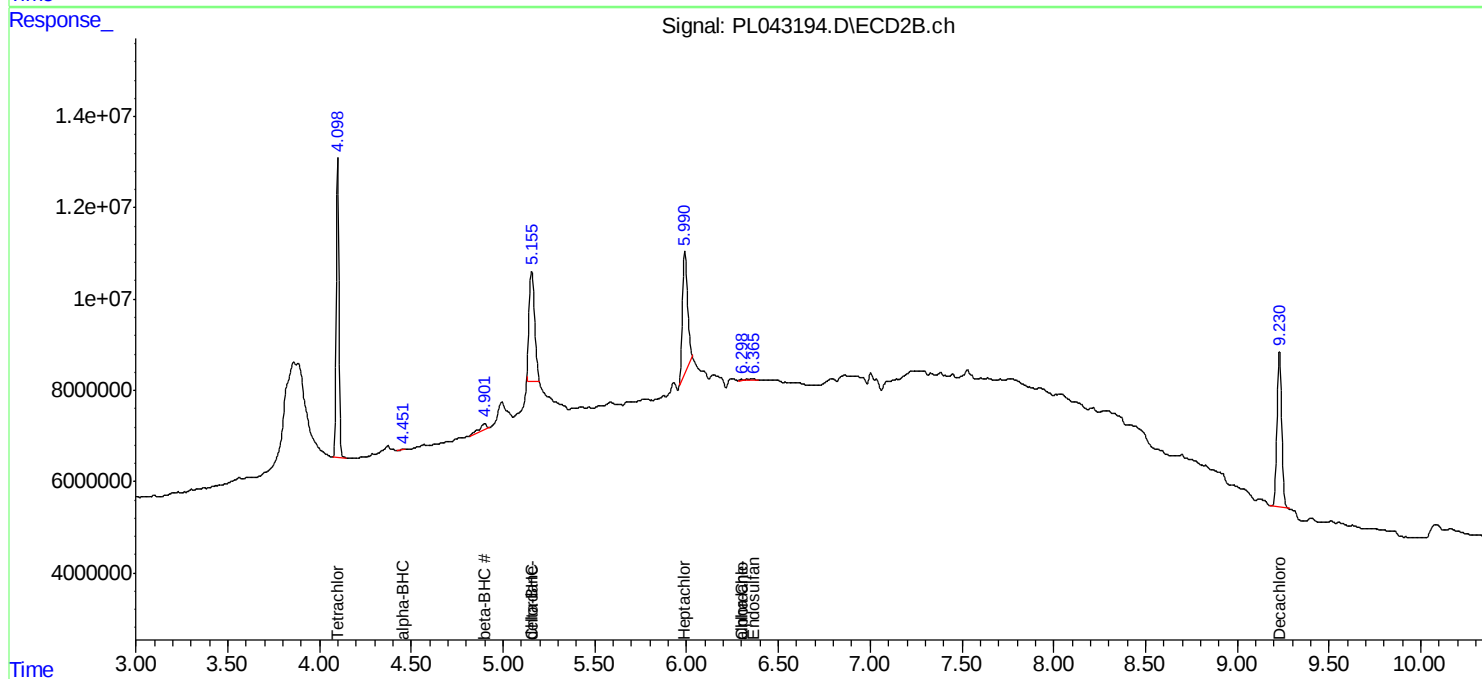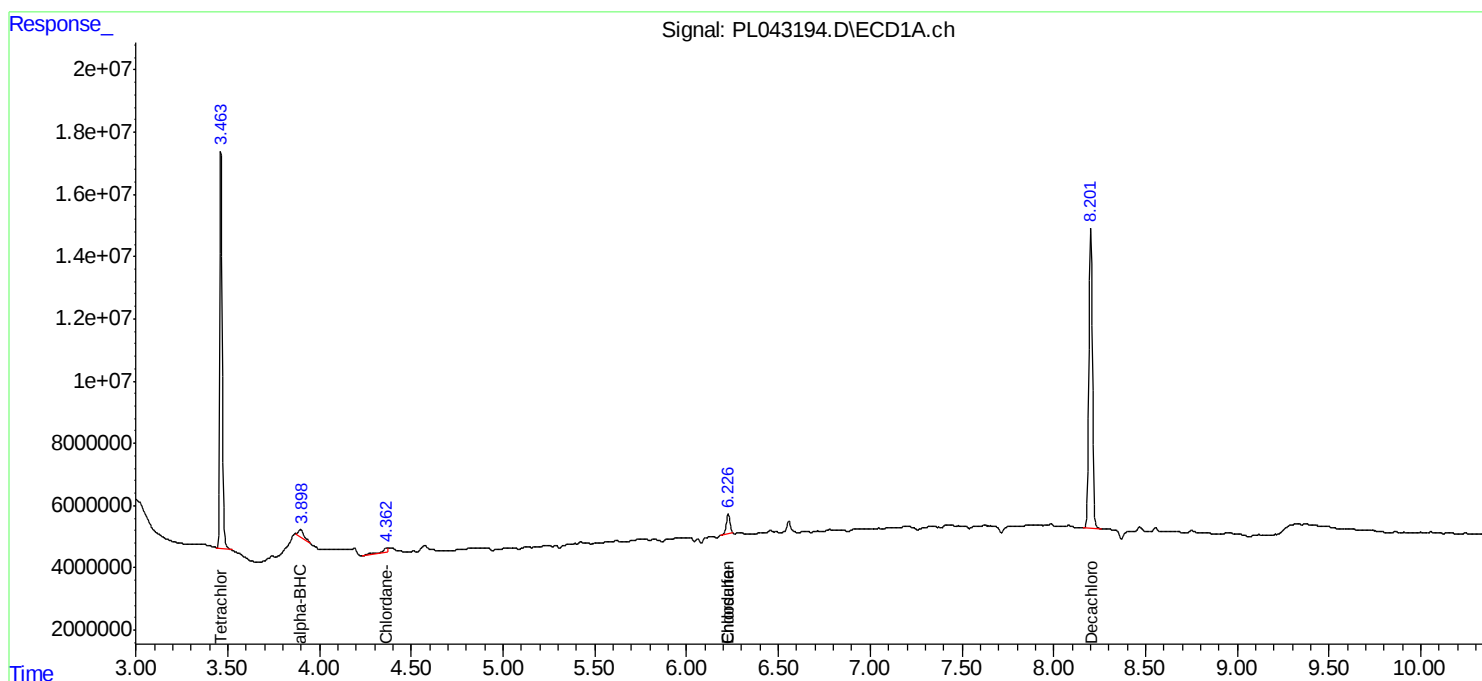


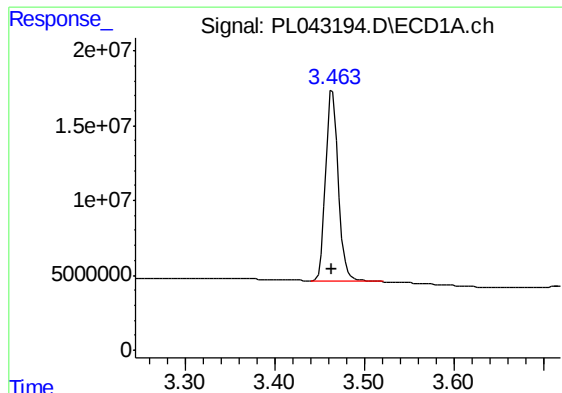

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 125394138
Conc: 20.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB115762TB

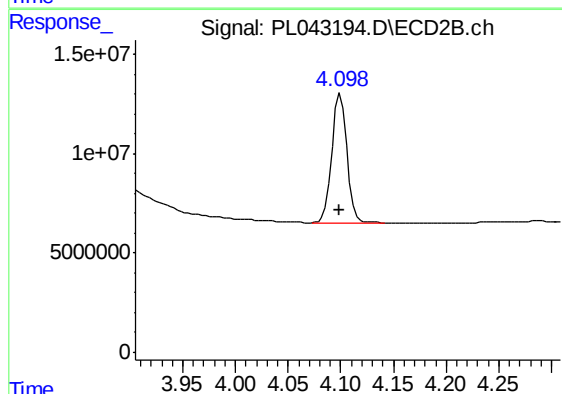


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 64466995
Conc: 21.75 ng/ml

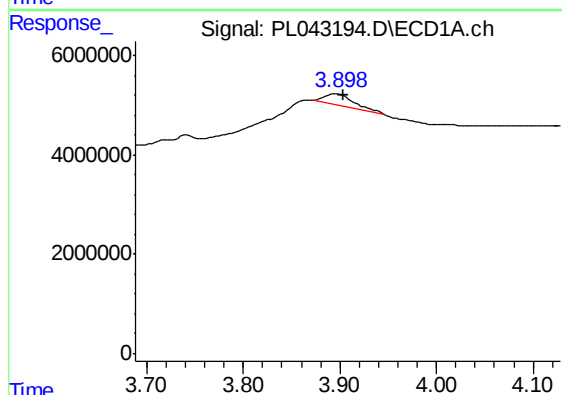


#2 alpha-BHC

R.T.: 3.896 min
Delta R.T.: -0.008 min
Response: 4376531
Conc: 0.46 ng/ml

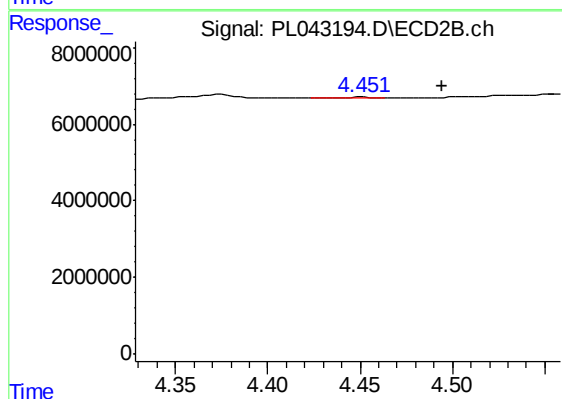

#2 alpha-BHC


R.T.: 4.452 min
Delta R.T.: -0.042 min
Response: 357203
Conc: 0.08 ng/ml

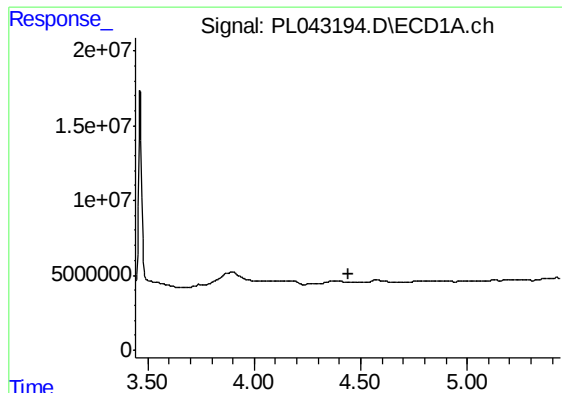

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.441 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB115762TB

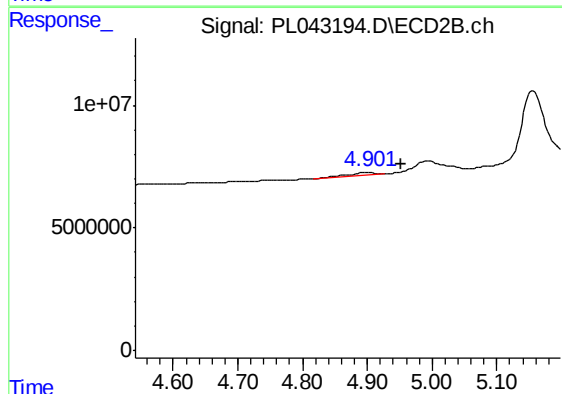


#6 beta-BHC

R.T.: 4.902 min
Delta R.T.: -0.050 min
Response: 4312545
Conc: 2.55 ng/ml

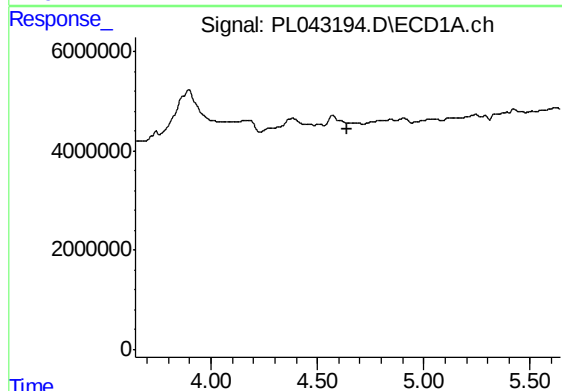


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

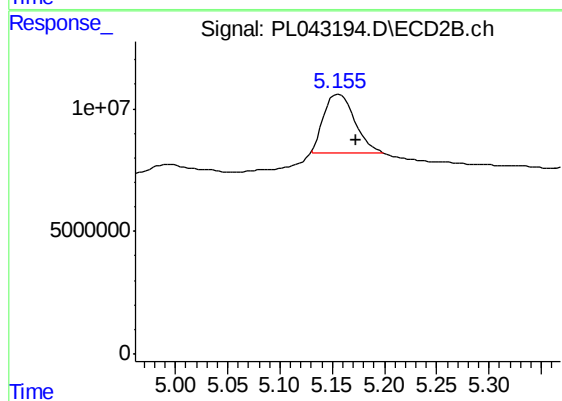

#7 delta-BHC


R.T.: 5.157 min
Delta R.T.: -0.016 min
Response: 49500021
Conc: 11.52 ng/ml

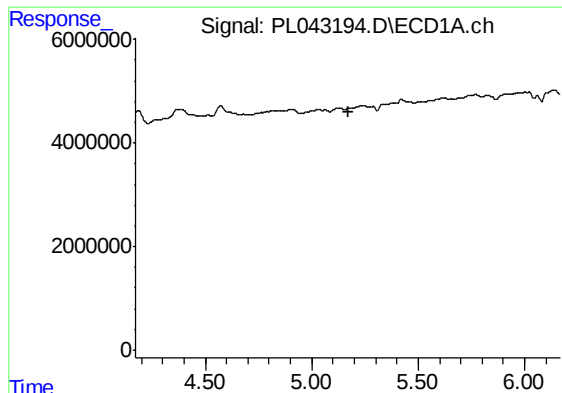

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB115762TB

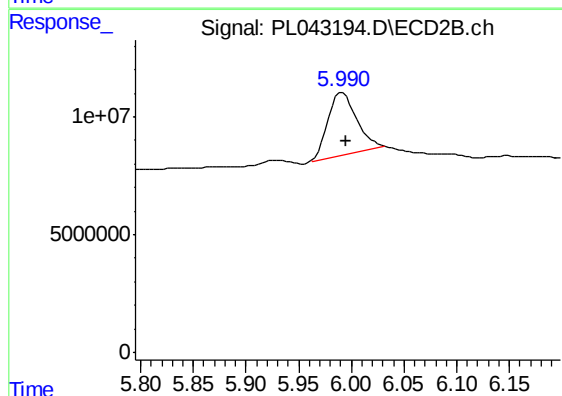


#8 Heptachlor epoxide

R.T.: 5.991 min
Delta R.T.: -0.004 min
Response: 50289058
Conc: 13.26 ng/ml

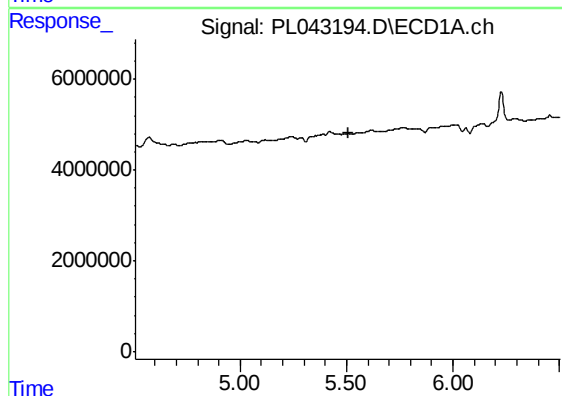


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

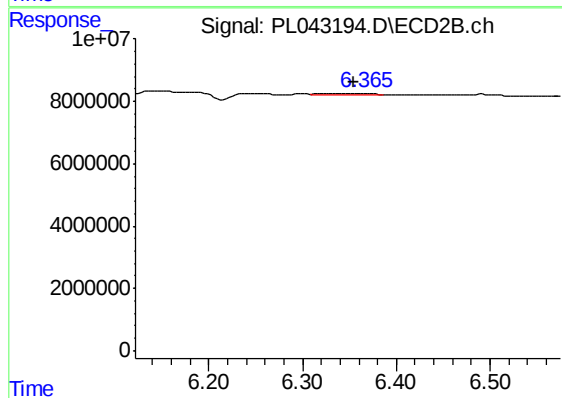

#9 Endosulfan I


R.T.: 6.366 min
Delta R.T.: 0.012 min
Response: 924366
Conc: 0.27 ng/ml

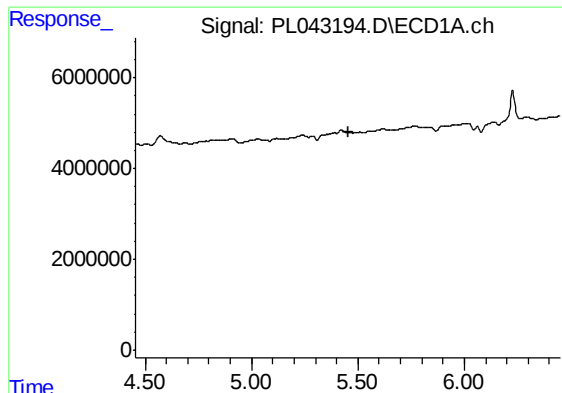

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB115762TB

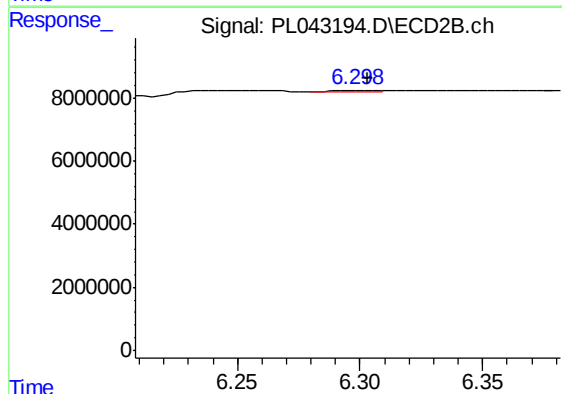


#11 alpha-Chlordane

R.T.: 6.299 min
Delta R.T.: -0.004 min
Response: 269411
Conc: 0.07 ng/ml

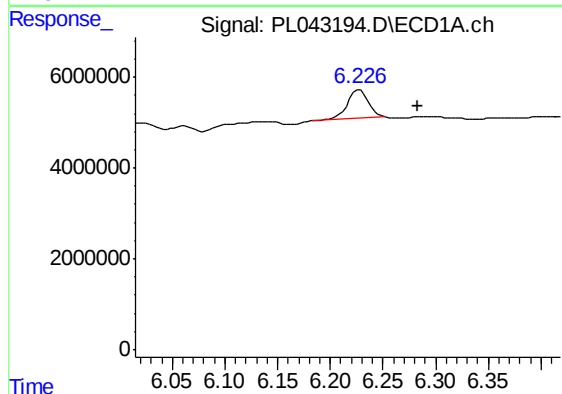


#15 Endosulfan II

R.T.: 6.228 min
Delta R.T.: -0.055 min
Response: 8754807
Conc: 1.32 ng/ml

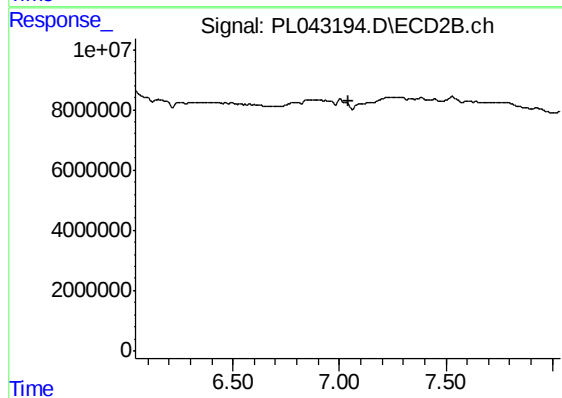

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

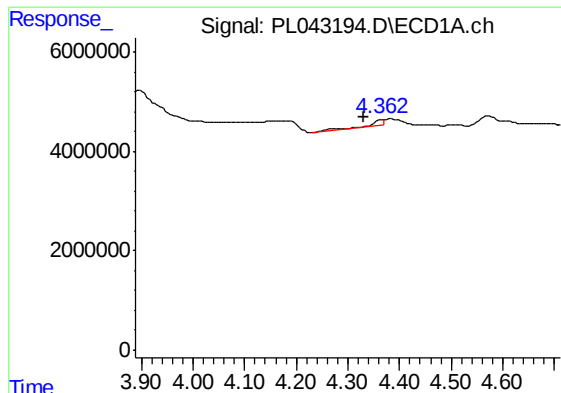

#23 Chlordane-1


R.T.: 4.363 min
Delta R.T.: 0.031 min
Response: 2712600
Conc: 10.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB115762TB

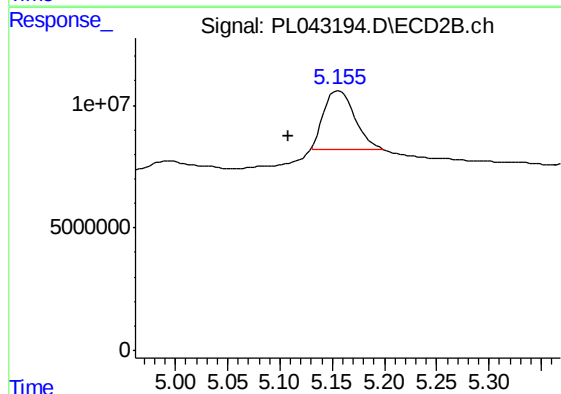


#23 Chlordane-1

R.T.: 5.157 min
Delta R.T.: 0.048 min
Response: 49500021
Conc: 350.24 ng/ml

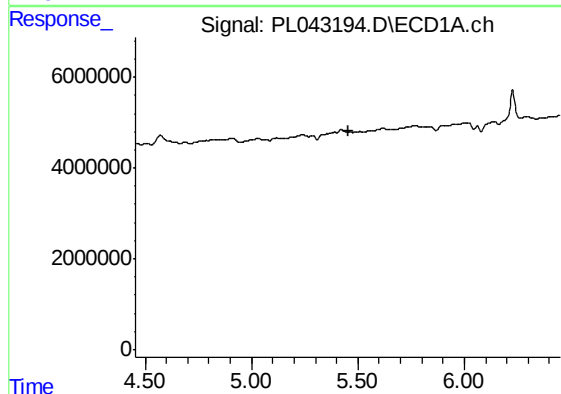


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

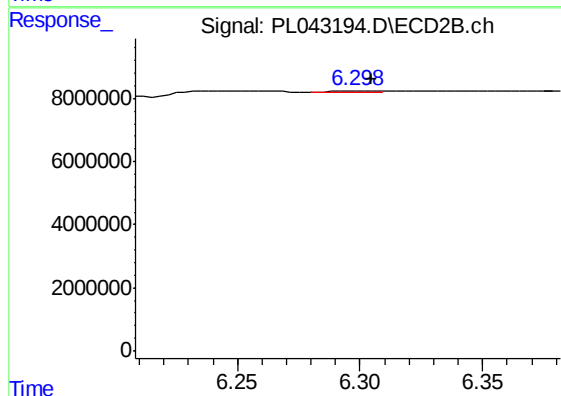

#26 Chlordane-4


R.T.: 6.299 min
Delta R.T.: -0.006 min
Response: 269411
Conc: 0.47 ng/ml

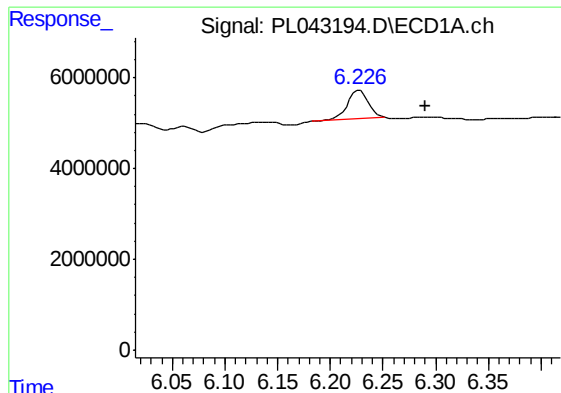

#27 Chlordane-5


R.T.: 6.228 min
Delta R.T.: -0.062 min
Response: 8754807
Conc: 36.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB115762TB

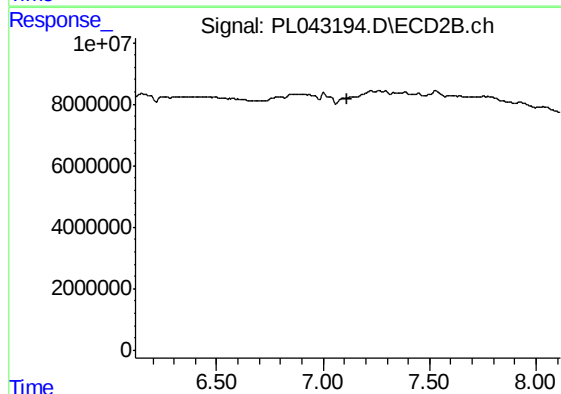


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

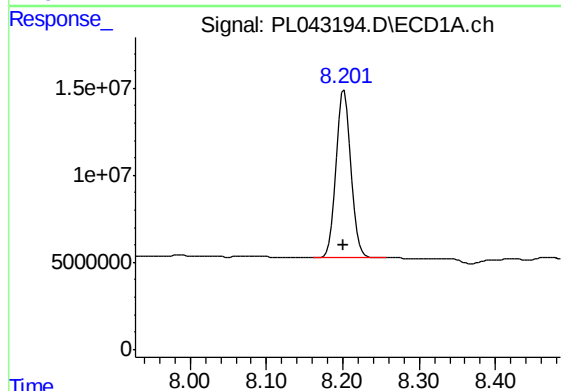

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 129039735
Conc: 19.76 ng/ml

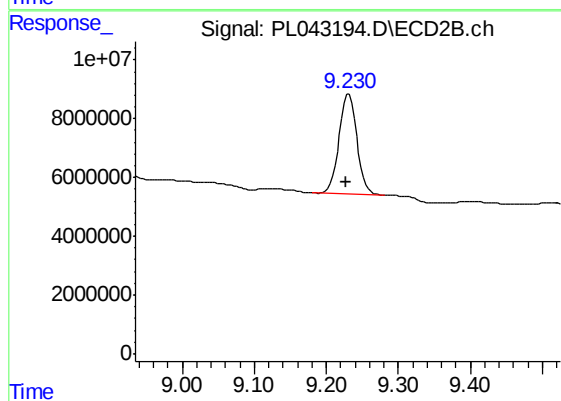

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.004 min
Response: 58606369
Conc: 22.47 ng/ml