

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 17:31
 Operator : AJ\SJ
 Sample : J6403-16
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:03:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.100	123.8E6	63952315	20.187	21.577
28)	SA Decachlor...	8.202	9.231	127.3E6	55342397	19.490	21.216
Target Compounds							
6)	B beta-BHC	4.398f	0.000	8982146	0	2.435	N.D. #
7)	B delta-BHC	0.000	5.158	0	29765398	N.D.	6.926 #
8)	B Heptachlo...	0.000	5.993	0	27631370	N.D.	7.287 #
9)	A Endosulfan I	0.000	6.331	0	640462	N.D.	0.189 #
11)	B alpha-Chl...	0.000	6.331	0	640462	N.D.	0.178 #
14)	MA Endrin	6.064f	6.793f	1034782	2567979	0.144	0.823 #
15)	B Endosulfa...	6.227f	0.000	6420295	0	0.965	N.D. #
23)	Chlordane-1	4.398	5.158	8982146	29765398	33.427	210.605 #
26)	Chlordane-4	0.000	6.331	0	640462	N.D.	1.122 #
27)	Chlordane-5	6.227	0.000	6420295	0	26.767	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 17:31
Operator : AJ\SJ
Sample : J6403-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-2-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:03:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

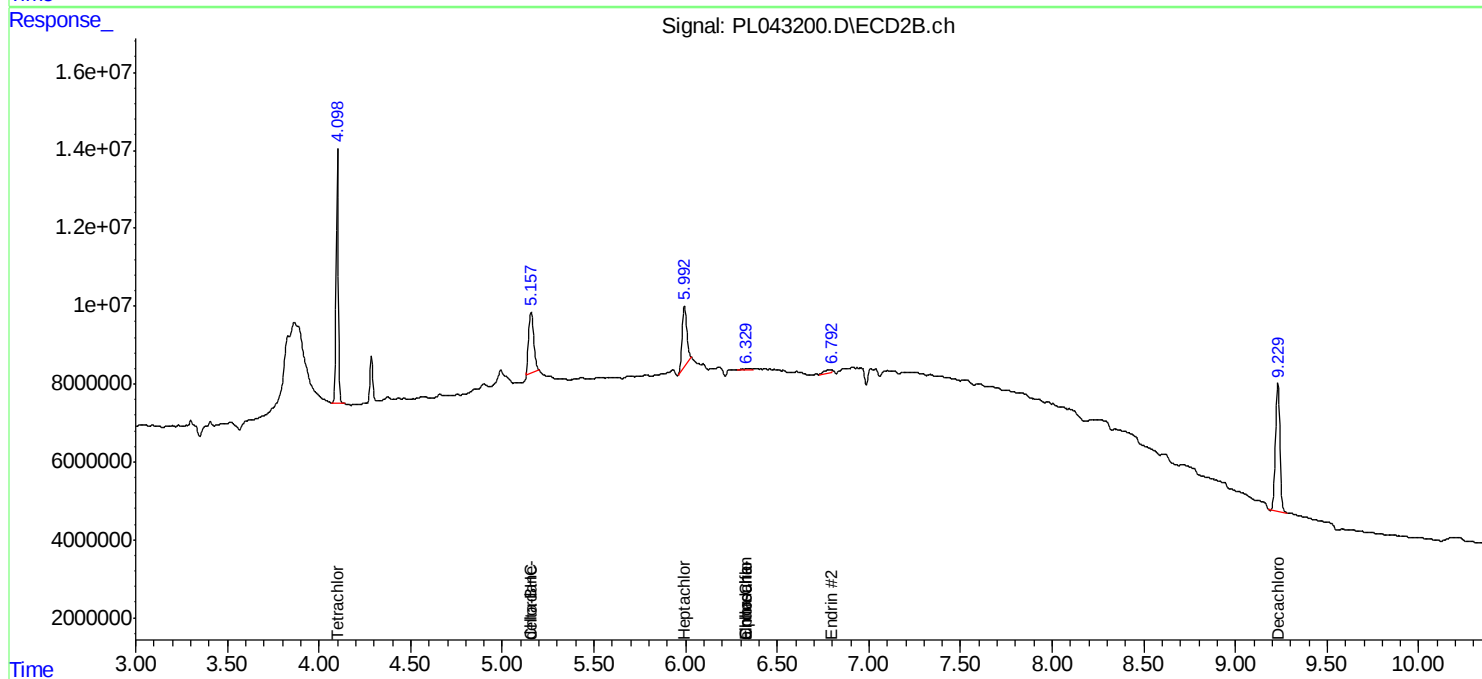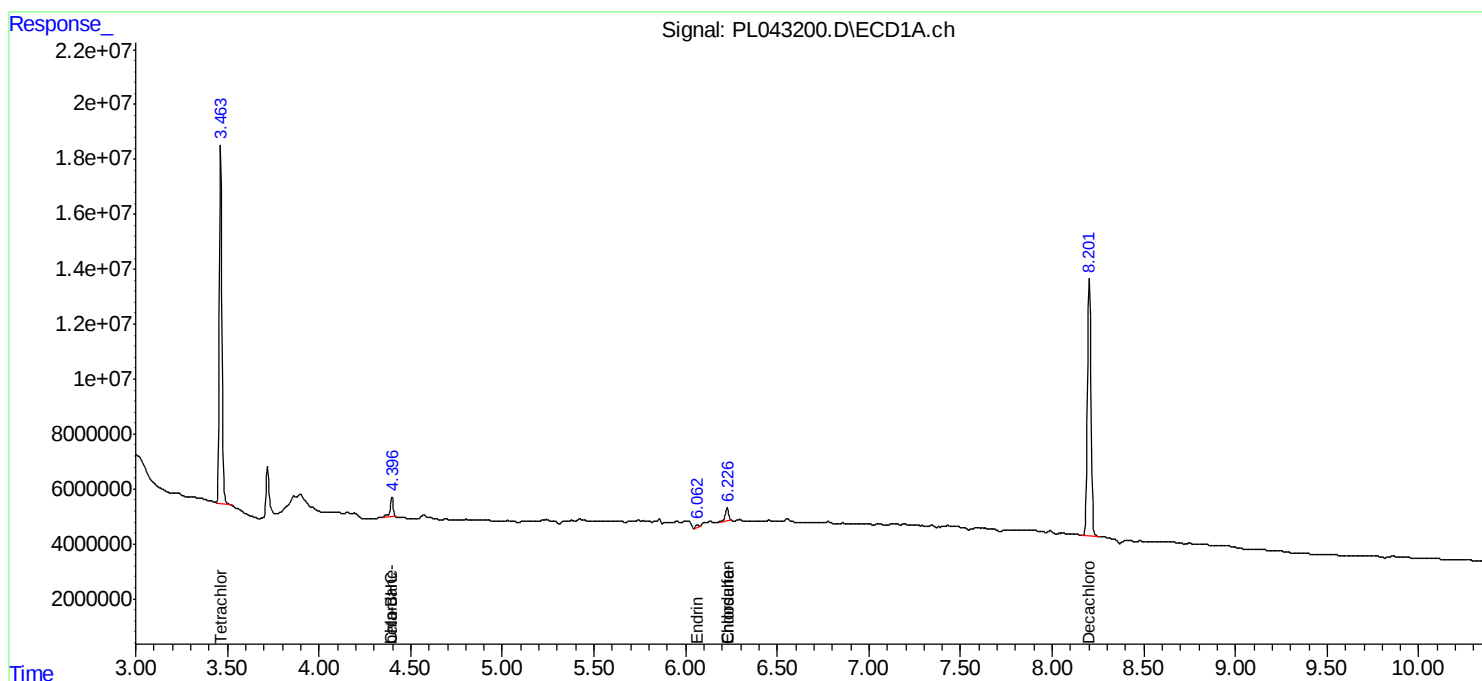


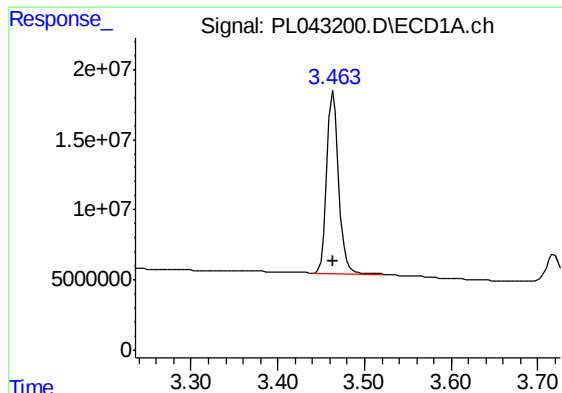

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 123803560
Conc: 20.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-B

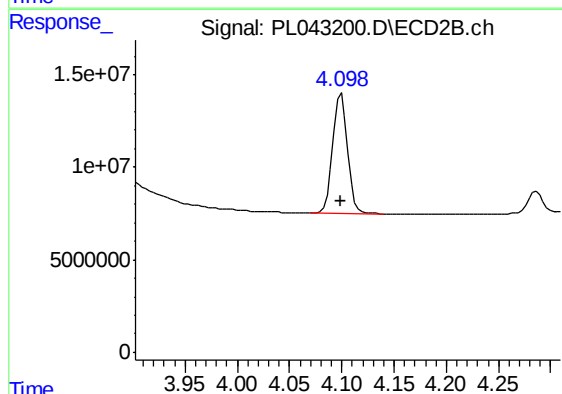


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 63952315
Conc: 21.58 ng/ml

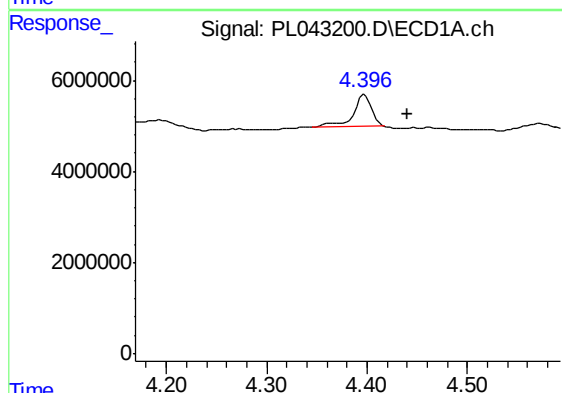


#6 beta-BHC

R.T.: 4.398 min
Delta R.T.: -0.043 min
Response: 8982146
Conc: 2.44 ng/ml

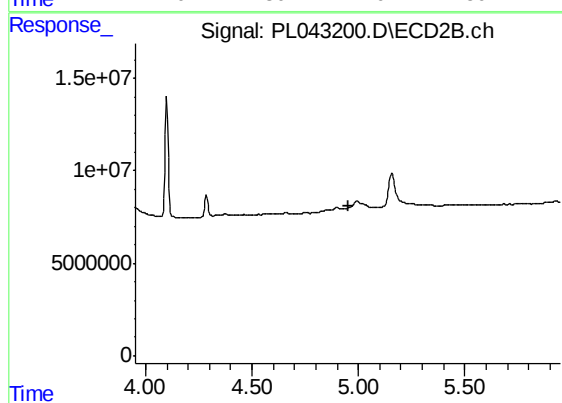

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

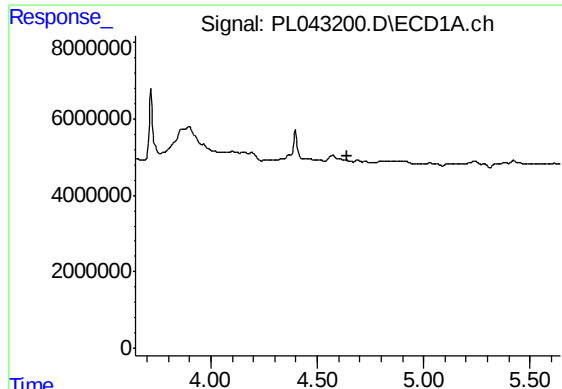

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2-B

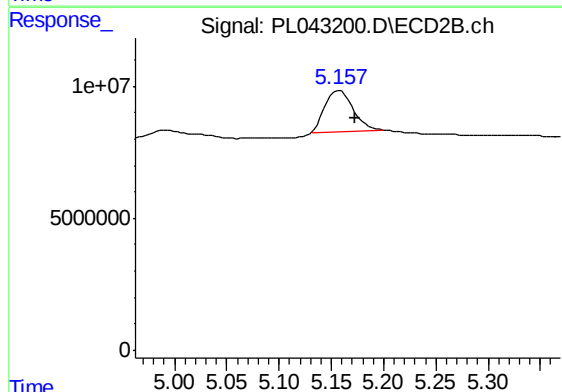


#7 delta-BHC

R.T.: 5.158 min
Delta R.T.: -0.015 min
Response: 29765398
Conc: 6.93 ng/ml

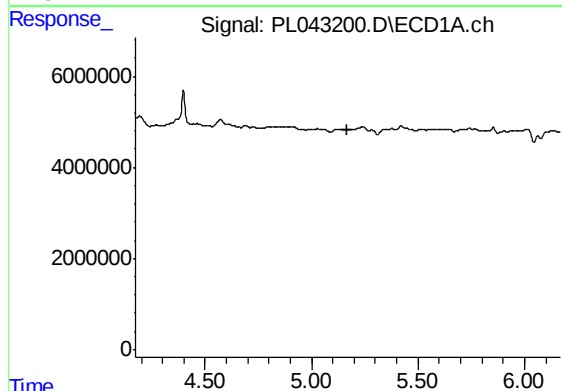


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

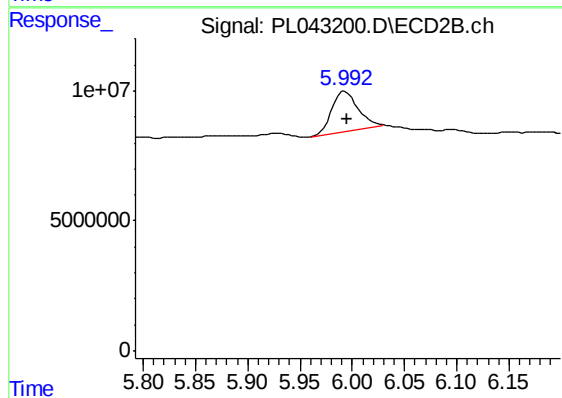

#8 Heptachlor epoxide


R.T.: 5.993 min
Delta R.T.: -0.002 min
Response: 27631370
Conc: 7.29 ng/ml

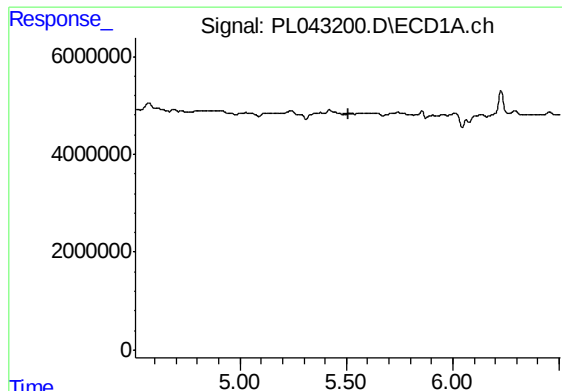

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2-B

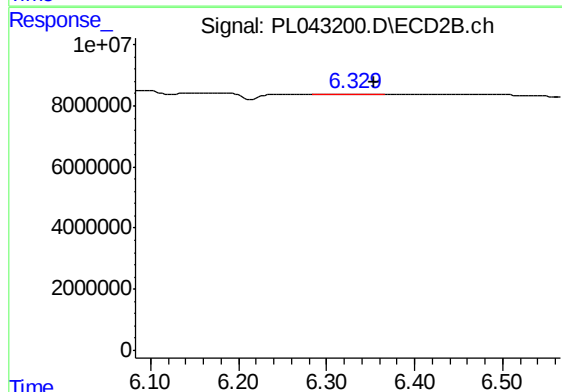


#9 Endosulfan I

R.T.: 6.331 min
Delta R.T.: -0.023 min
Response: 640462
Conc: 0.19 ng/ml

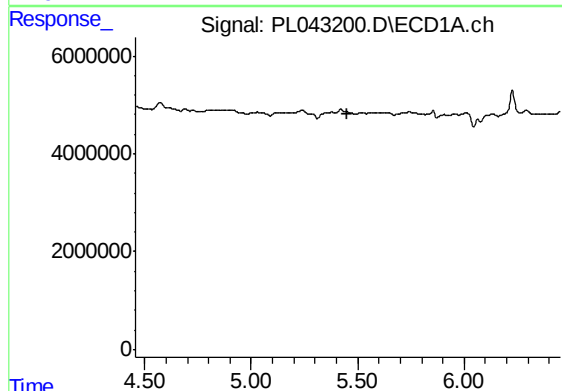


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.454 min
Response: 0
Conc: N.D.

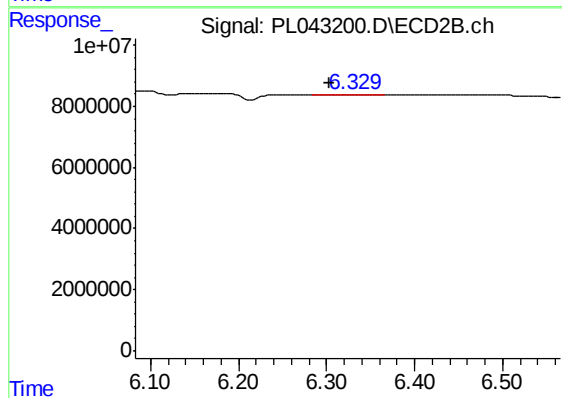

#11 alpha-Chlordane


R.T.: 6.331 min
Delta R.T.: 0.028 min
Response: 640462
Conc: 0.18 ng/ml

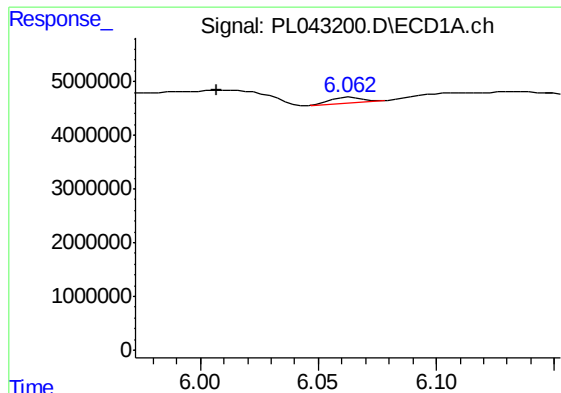

#14 Endrin


R.T.: 6.064 min
Delta R.T.: 0.057 min
Response: 1034782
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-B

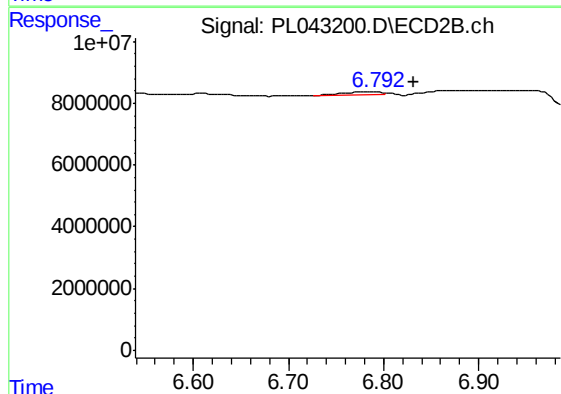


#14 Endrin

R.T.: 6.793 min
Delta R.T.: -0.040 min
Response: 2567979
Conc: 0.82 ng/ml

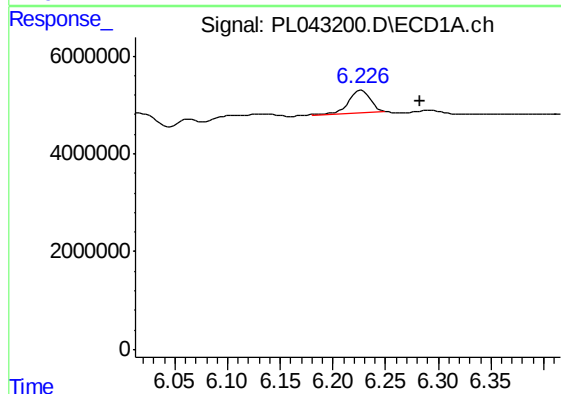


#15 Endosulfan II

R.T.: 6.227 min
Delta R.T.: -0.055 min
Response: 6420295
Conc: 0.97 ng/ml

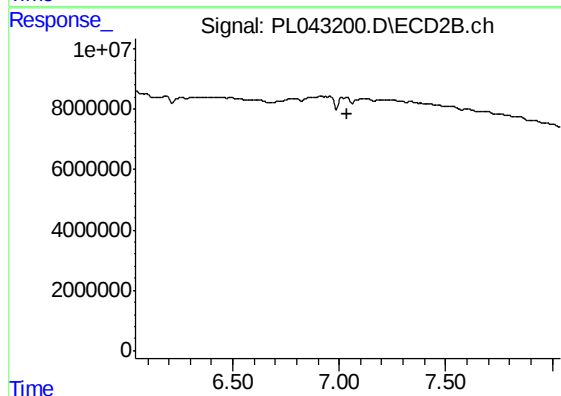

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

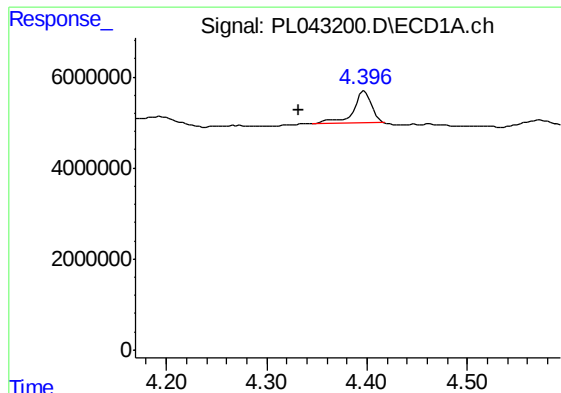

#23 Chlordane-1


R.T.: 4.398 min
Delta R.T.: 0.065 min
Response: 8982146
Conc: 33.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-B

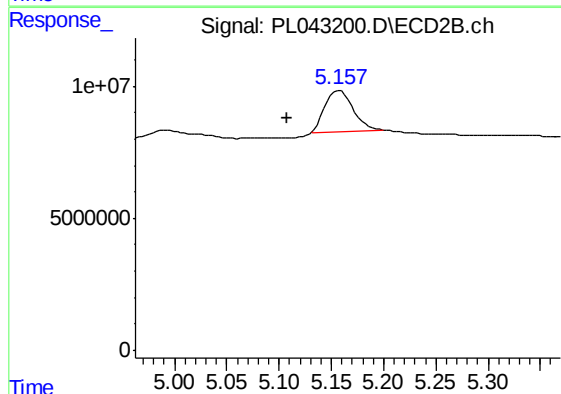


#23 Chlordane-1

R.T.: 5.158 min
Delta R.T.: 0.050 min
Response: 29765398
Conc: 210.60 ng/ml

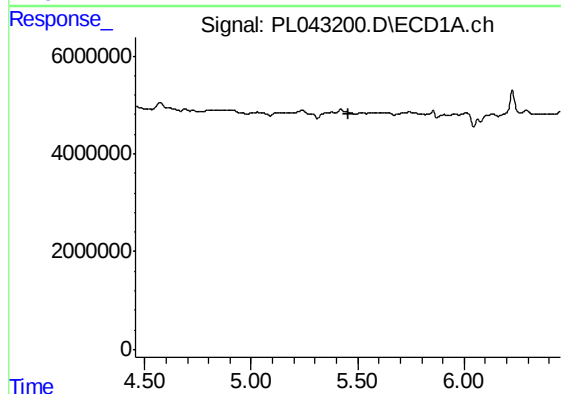


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

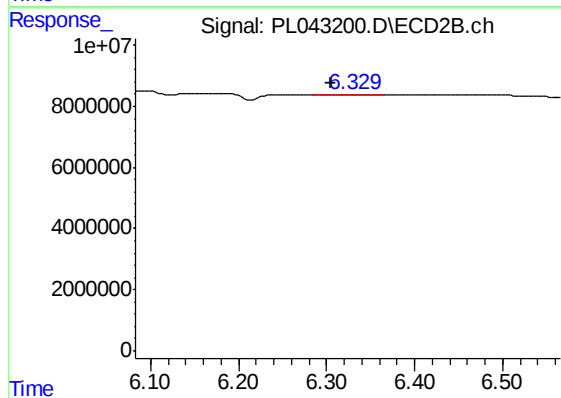

#26 Chlordane-4


R.T.: 6.331 min
Delta R.T.: 0.026 min
Response: 640462
Conc: 1.12 ng/ml

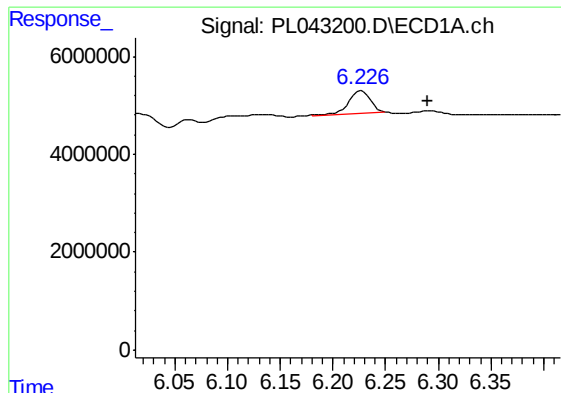

#27 Chlordane-5


R.T.: 6.227 min
Delta R.T.: -0.063 min
Response: 6420295
Conc: 26.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-B

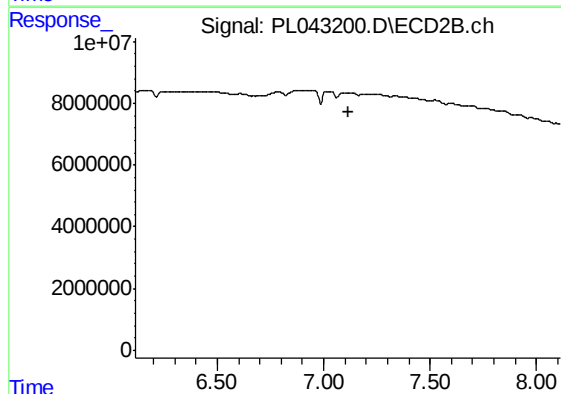


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

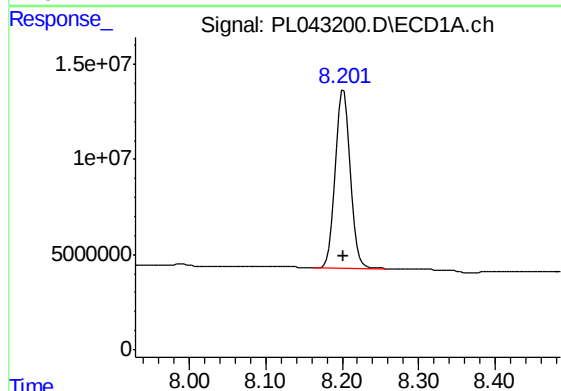

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 127267843
Conc: 19.49 ng/ml

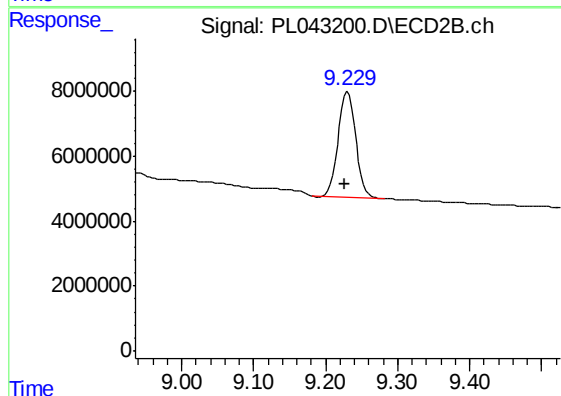

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.004 min
Response: 55342397
Conc: 21.22 ng/ml