

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 18:13
 Operator : AJ\SJ
 Sample : J6403-28
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:04:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	126.3E6	62067884	20.590	20.941
28)	SA Decachlor...	8.202	9.231	128.4E6	53356226	19.663	20.455
Target Compounds							
2)	A alpha-BHC	3.900	0.000	5595569	0	0.592	N.D. #
6)	B beta-BHC	4.398f	0.000	1801332	0	0.488	N.D. #
8)	B Heptachlo...	5.117f	5.993	2818293	8427652	0.356	2.222 #
9)	A Endosulfan I	0.000	6.314f	0	1690315	N.D.	0.498 #
11)	B alpha-Chl...	0.000	6.314	0	1690315	N.D.	0.470 #
14)	MA Endrin	6.064f	0.000	1183051	0	0.164	N.D. #
15)	B Endosulfa...	6.228f	0.000	4848904	0	0.729	N.D. #
23)	Chlordane-1	4.398	0.000	1801332	0	6.704	N.D. #
26)	Chlordane-4	0.000	6.314	0	1690315	N.D.	2.962 #
27)	Chlordane-5	6.228	0.000	4848904	0	20.216	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 18:13
Operator : AJ\SJ
Sample : J6403-28
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-4-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:04:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

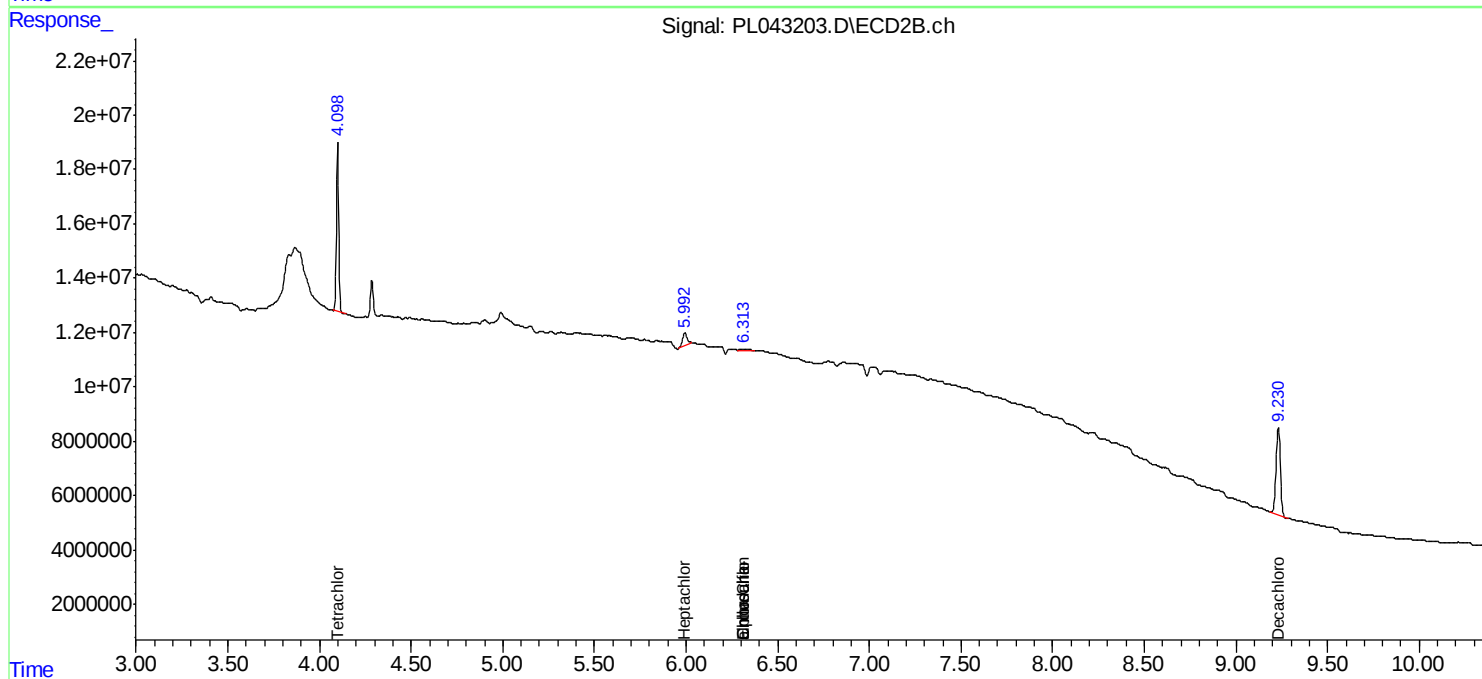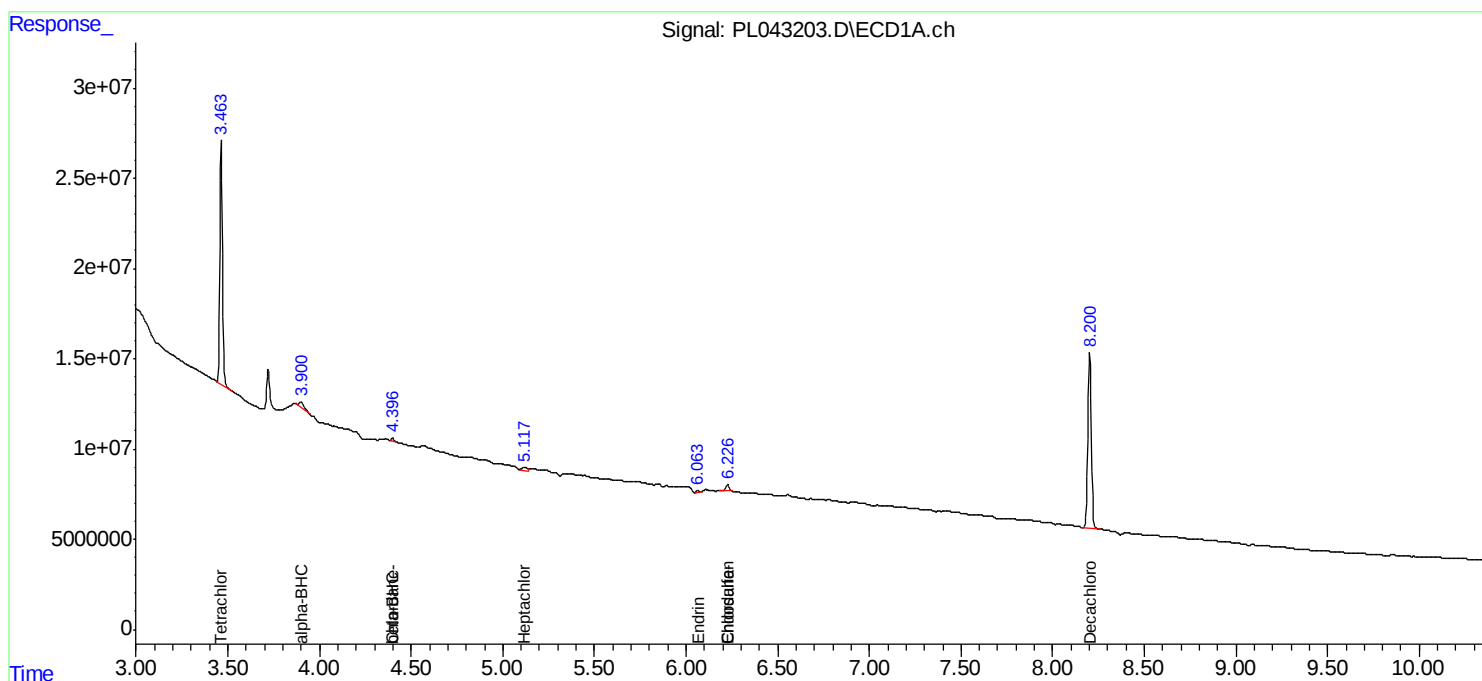


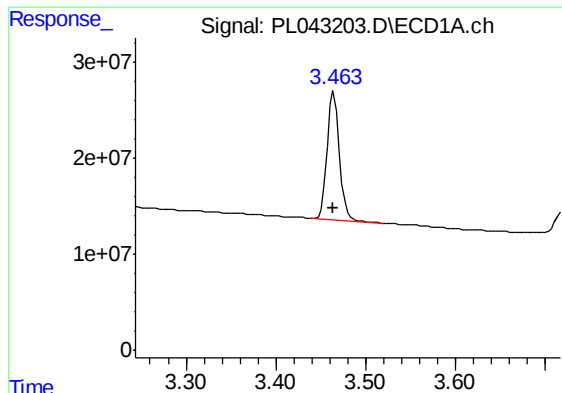

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 126273742
Conc: 20.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-A

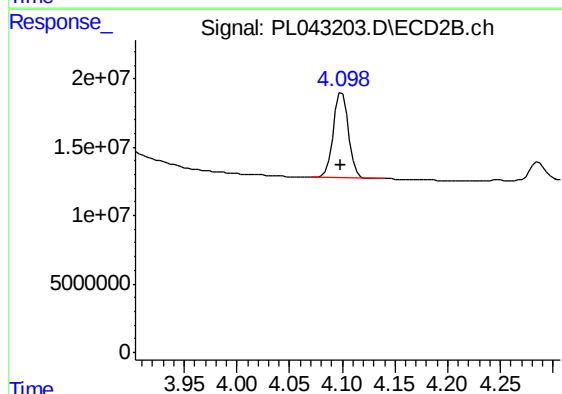


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 62067884
Conc: 20.94 ng/ml

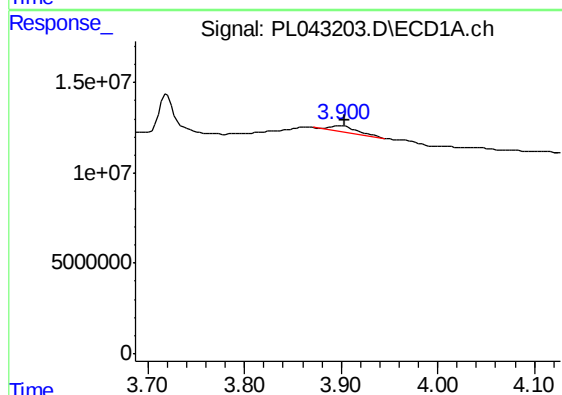


#2 alpha-BHC

R.T.: 3.900 min
Delta R.T.: -0.004 min
Response: 5595569
Conc: 0.59 ng/ml

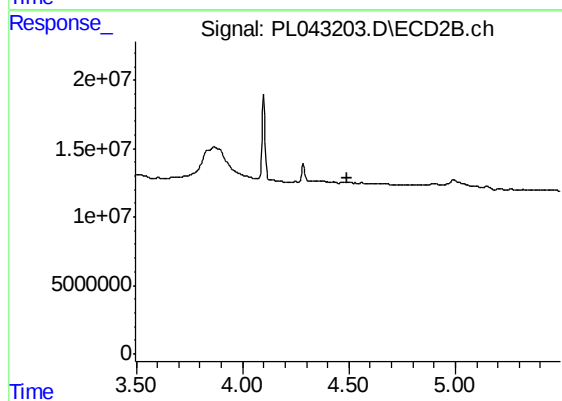

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.494 min
Response: 0
Conc: N.D.

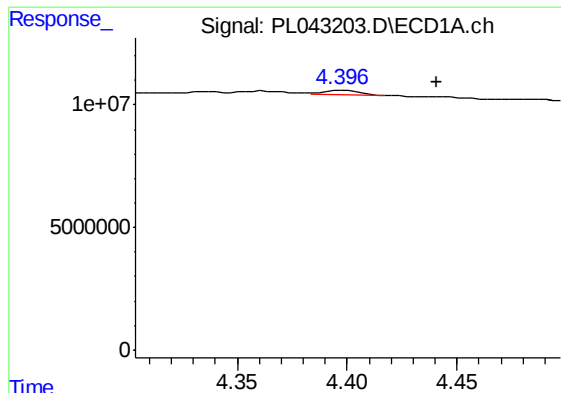

#6 beta-BHC


R.T.: 4.398 min
Delta R.T.: -0.043 min
Response: 1801332
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-A

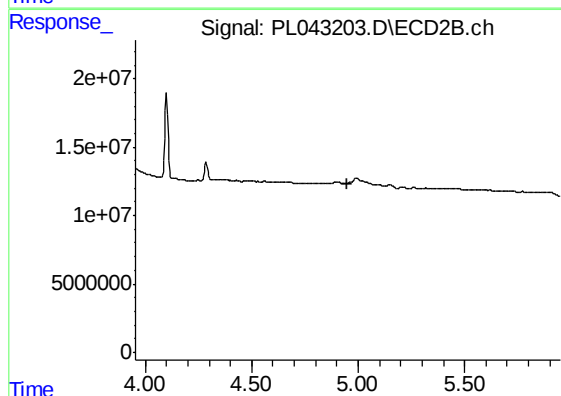


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

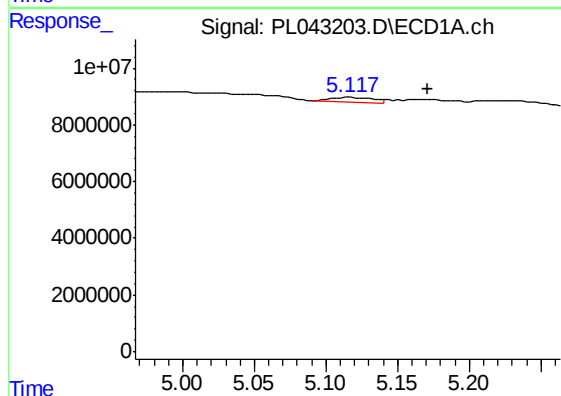


#8 Heptachlor epoxide

R.T.: 5.117 min
Delta R.T.: -0.053 min
Response: 2818293
Conc: 0.36 ng/ml

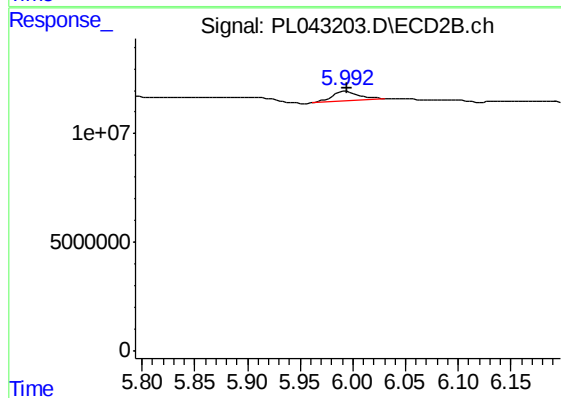

#8 Heptachlor epoxide


R.T.: 5.993 min
Delta R.T.: -0.002 min
Response: 8427652
Conc: 2.22 ng/ml

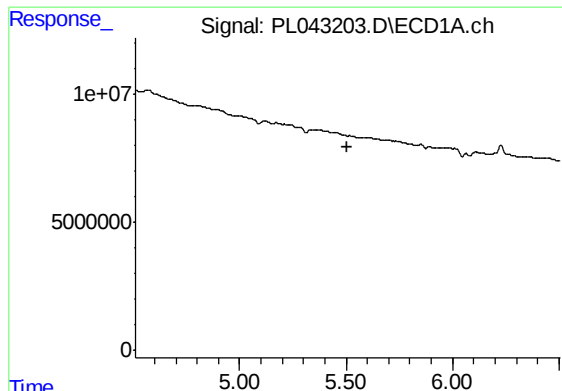

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-4-A

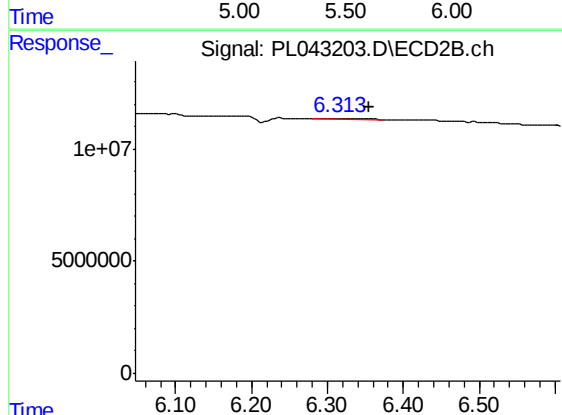


#9 Endosulfan I

R.T.: 6.314 min
Delta R.T.: -0.040 min
Response: 1690315
Conc: 0.50 ng/ml

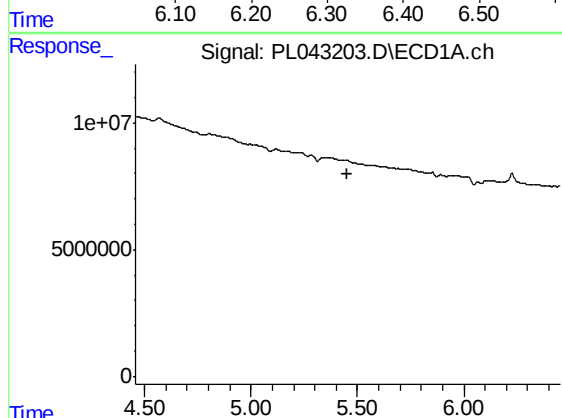


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.454 min
Response: 0
Conc: N.D.

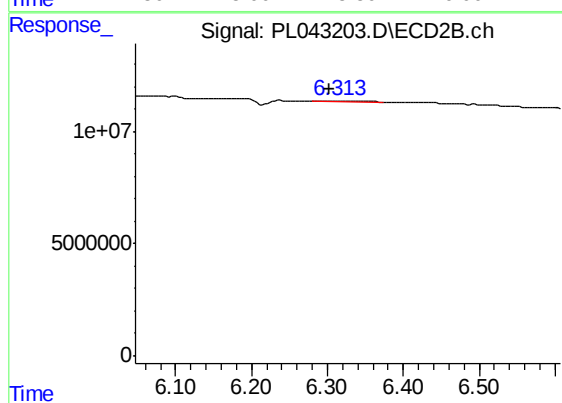

#11 alpha-Chlordane


R.T.: 6.314 min
Delta R.T.: 0.011 min
Response: 1690315
Conc: 0.47 ng/ml

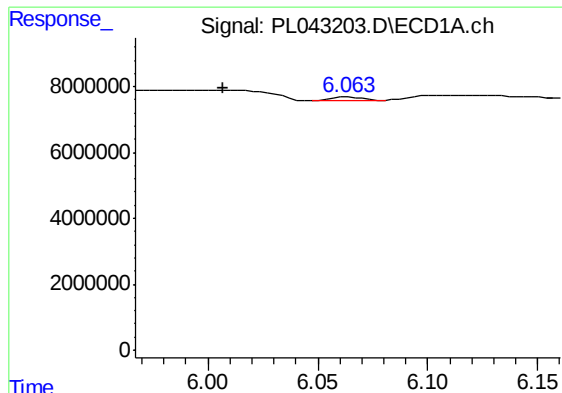

#14 Endrin


R.T.: 6.064 min
Delta R.T.: 0.057 min
Response: 1183051
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-A

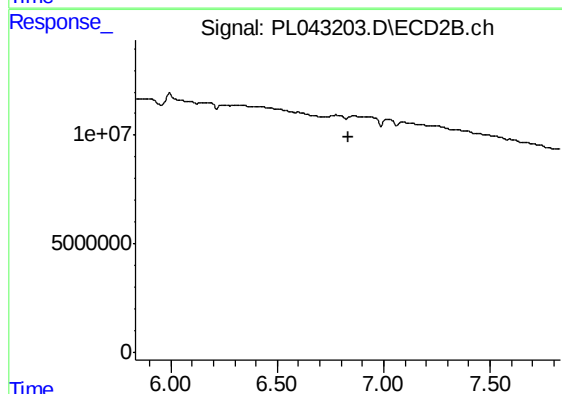


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

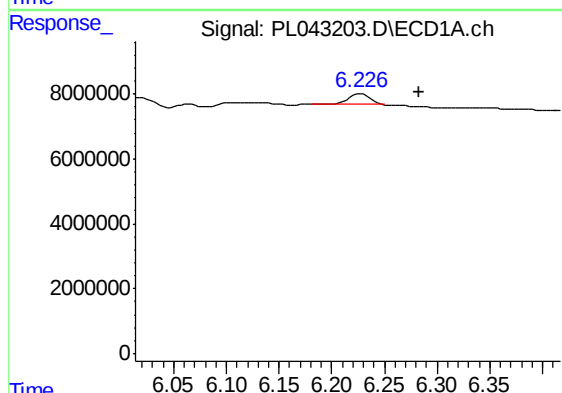


#15 Endosulfan II

R.T.: 6.228 min
Delta R.T.: -0.055 min
Response: 4848904
Conc: 0.73 ng/ml

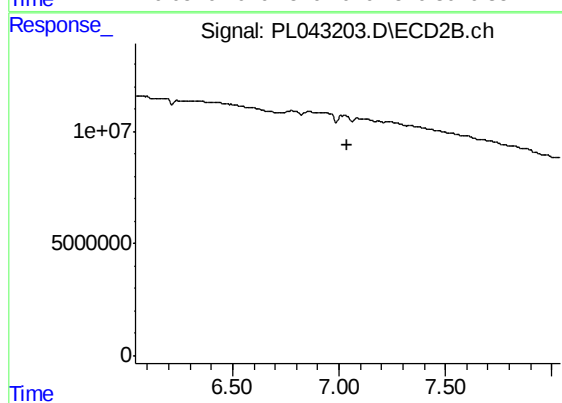

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

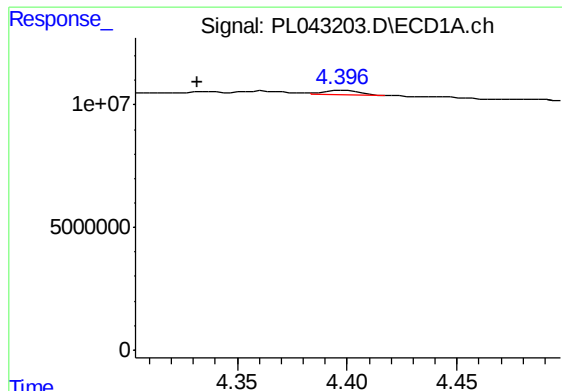

#23 Chlordane-1


R.T.: 4.398 min
Delta R.T.: 0.066 min
Response: 1801332
Conc: 6.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-A

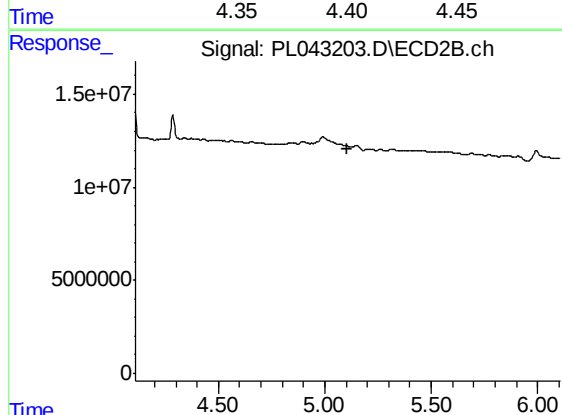


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

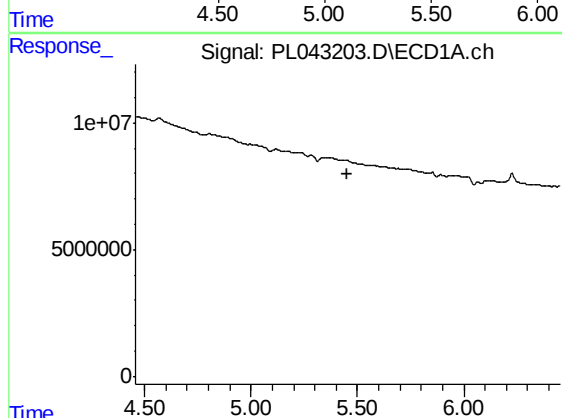


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

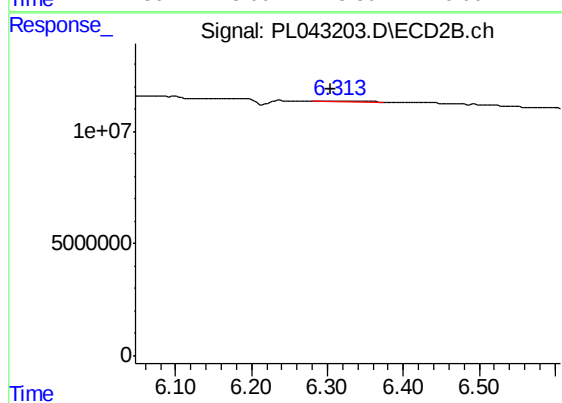

#26 Chlordane-4


R.T.: 6.314 min
Delta R.T.: 0.009 min
Response: 1690315
Conc: 2.96 ng/ml

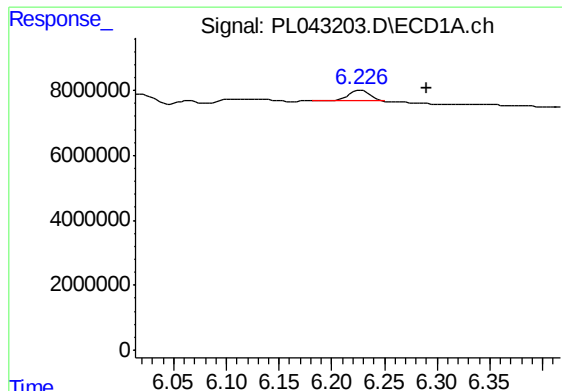

#27 Chlordane-5


R.T.: 6.228 min
Delta R.T.: -0.062 min
Response: 4848904
Conc: 20.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-A

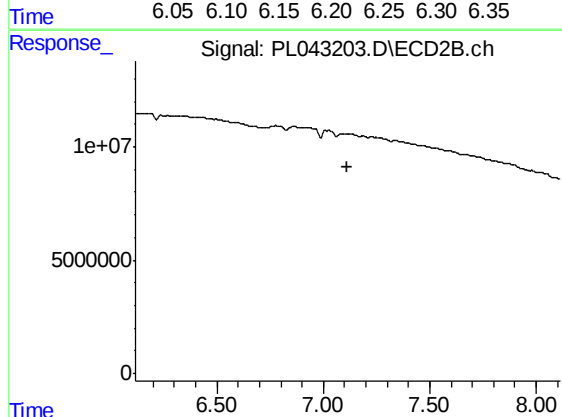


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

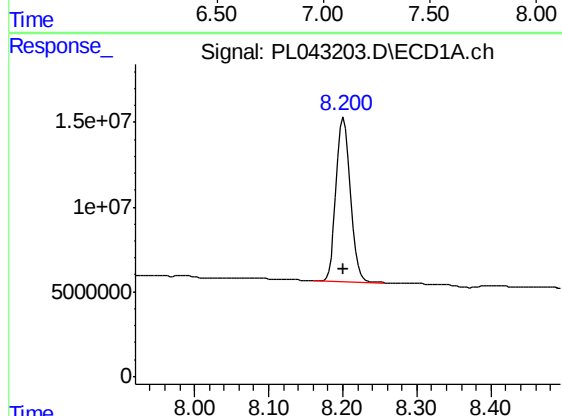

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 128398896
Conc: 19.66 ng/ml

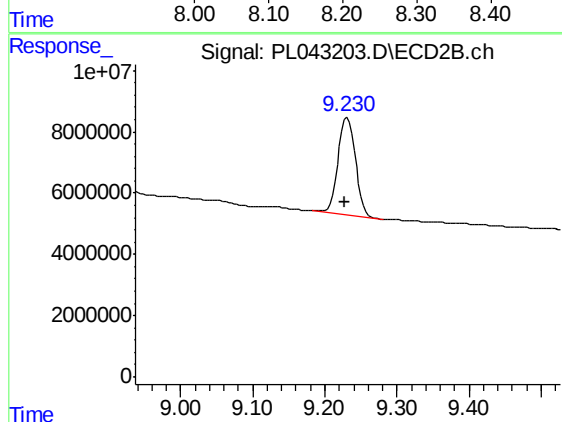

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.004 min
Response: 53356226
Conc: 20.45 ng/ml