

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 18:27
 Operator : AJ\SJ
 Sample : J6403-32
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:04:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	132.2E6	67250144	21.554	22.690
28)	SA Decachlor...	8.202	9.231	140.0E6	61497042	21.438	23.576
Target Compounds							
3)	MA gamma-BHC...	0.000	4.745f	0	958179	N.D.	0.228 #
6)	B beta-BHC	4.398f	0.000	3124815	0	0.847	N.D. #
7)	B delta-BHC	0.000	5.160	0	23566932	N.D.	5.484 #
8)	B Heptachlo...	0.000	5.994	0	23511301	N.D.	6.200 #
14)	MA Endrin	6.066f	0.000	1101954	0	0.153	N.D. #
15)	B Endosulfa...	6.227f	0.000	5693245	0	0.856	N.D. #
16)	A 4,4'-DDD	6.066f	0.000	1101954	0	0.194	N.D. #
23)	Chlordane-1	4.361	5.160	1564018	23566932	5.821	166.748 #
27)	Chlordane-5	6.227	0.000	5693245	0	23.736	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 18:27
Operator : AJ\SJ
Sample : J6403-32
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-4-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:04:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

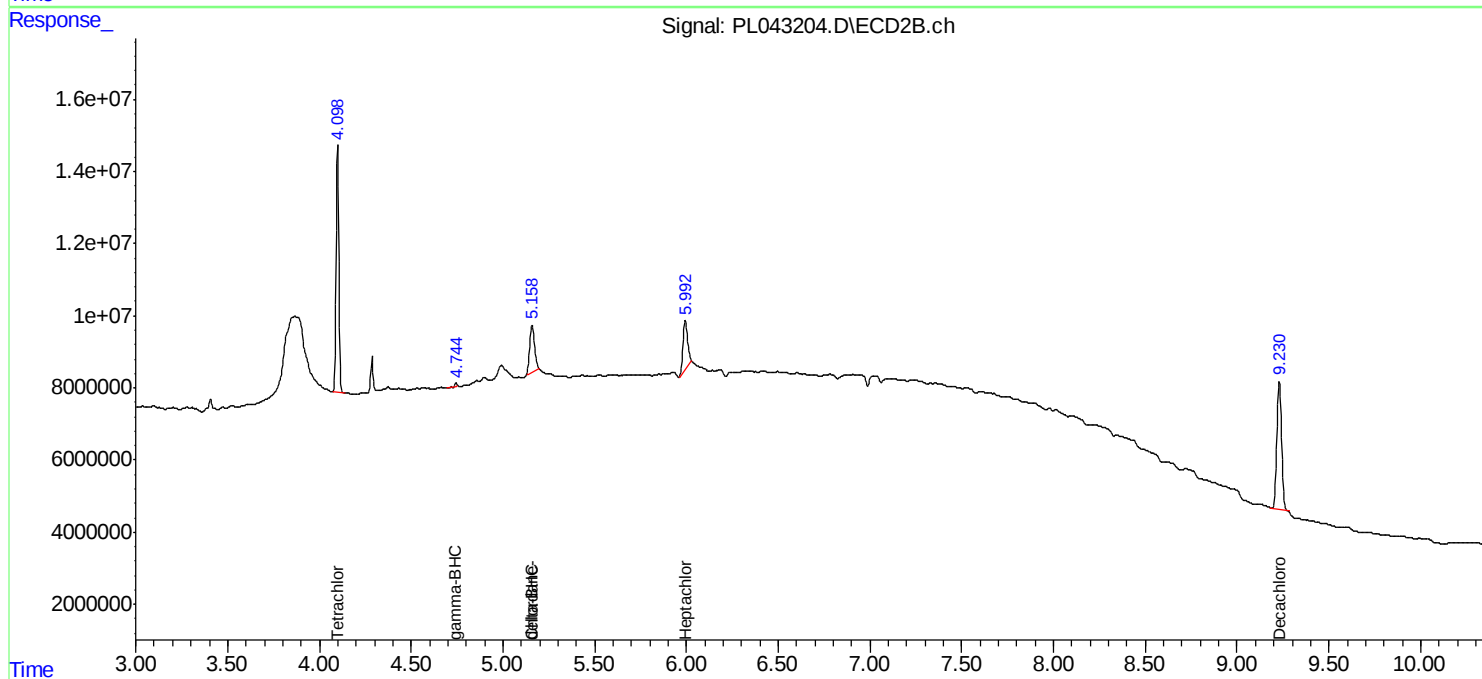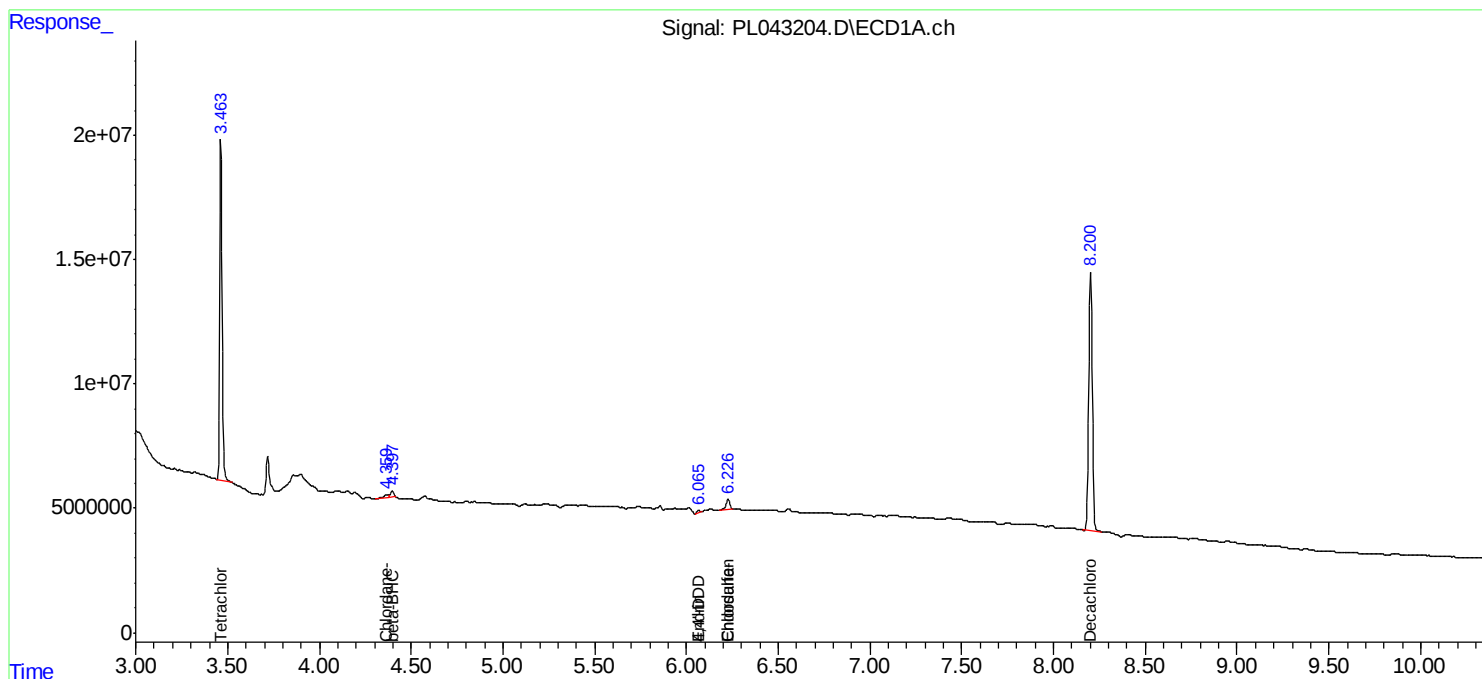


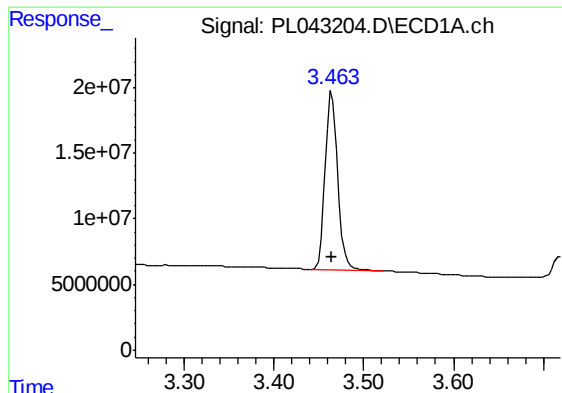

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 132186881
Conc: 21.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

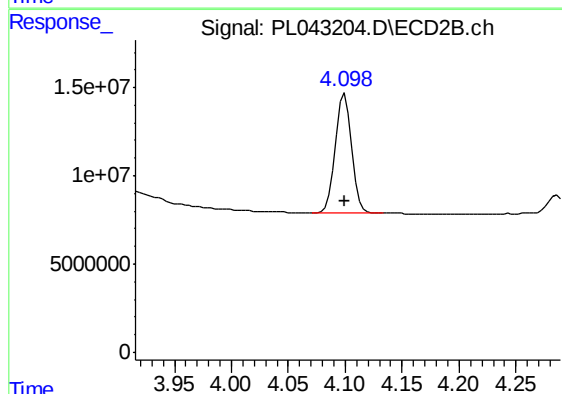


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 67250144
Conc: 22.69 ng/ml

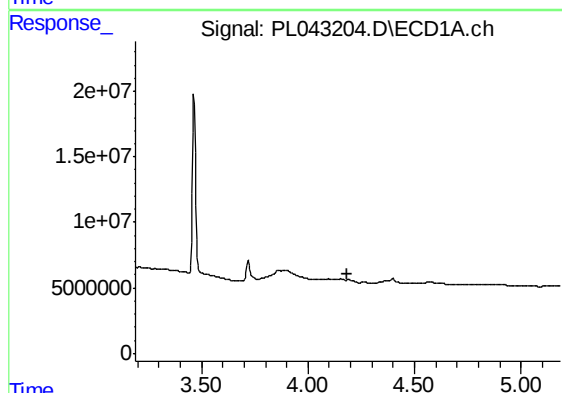


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

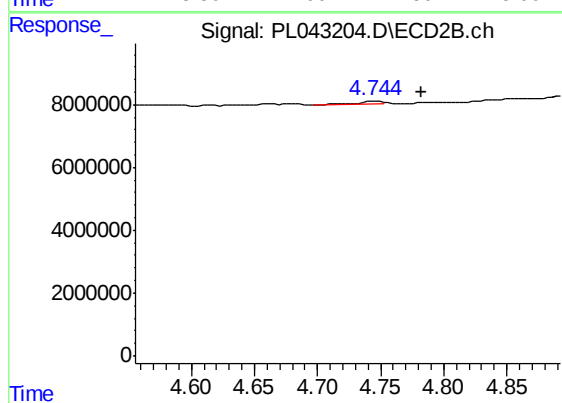

#3 gamma-BHC (Lindane)


R.T.: 4.745 min
Delta R.T.: -0.038 min
Response: 958179
Conc: 0.23 ng/ml

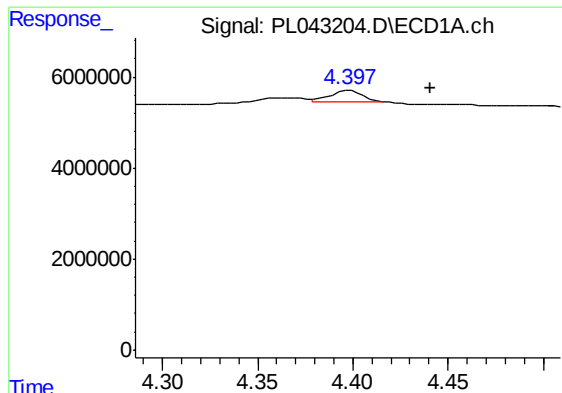

#6 beta-BHC


R.T.: 4.398 min
Delta R.T.: -0.042 min
Response: 3124815
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

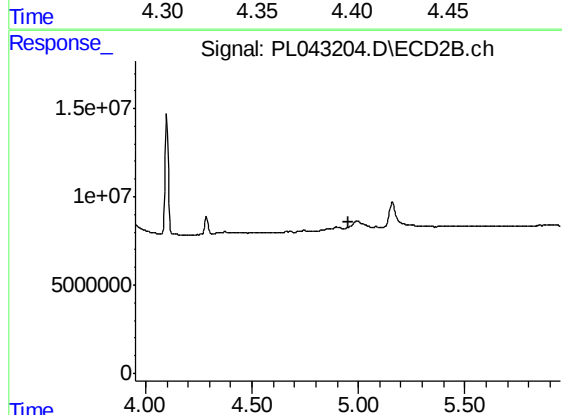


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

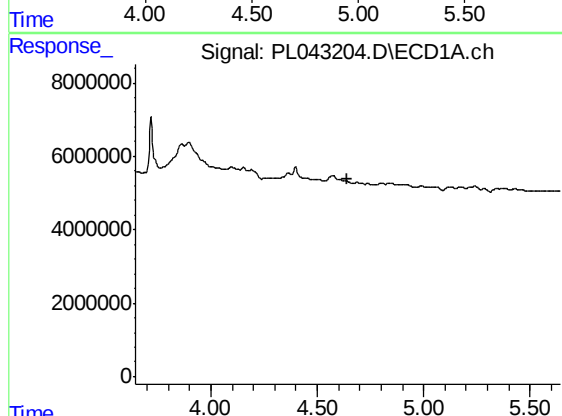


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

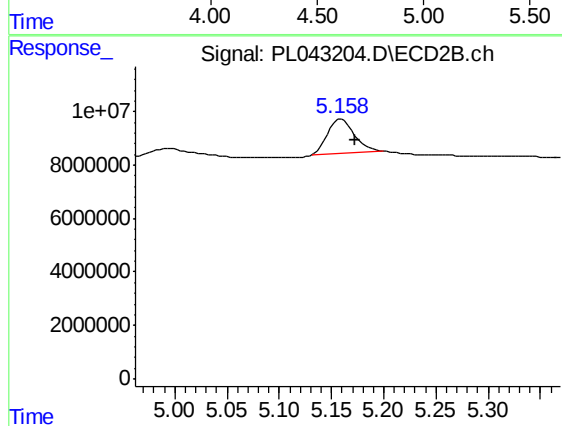

#7 delta-BHC


R.T.: 5.160 min
Delta R.T.: -0.013 min
Response: 23566932
Conc: 5.48 ng/ml

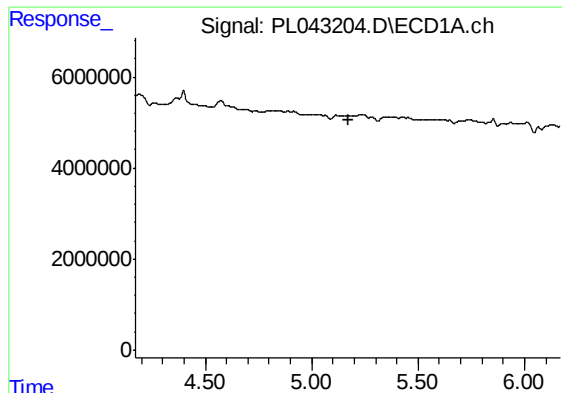

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-4-B

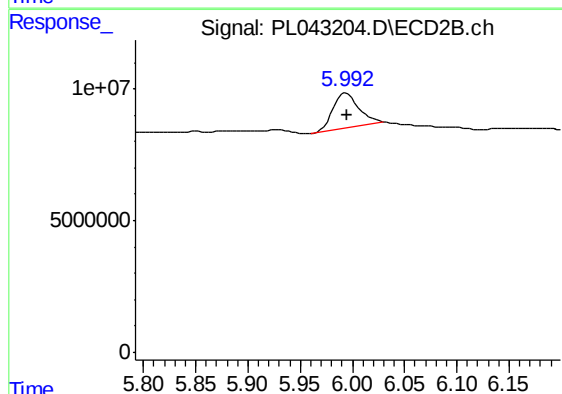


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.001 min
Response: 23511301
Conc: 6.20 ng/ml

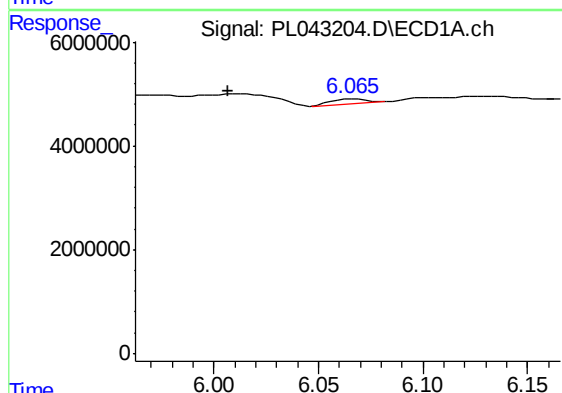


#14 Endrin

R.T.: 6.066 min
Delta R.T.: 0.059 min
Response: 1101954
Conc: 0.15 ng/ml

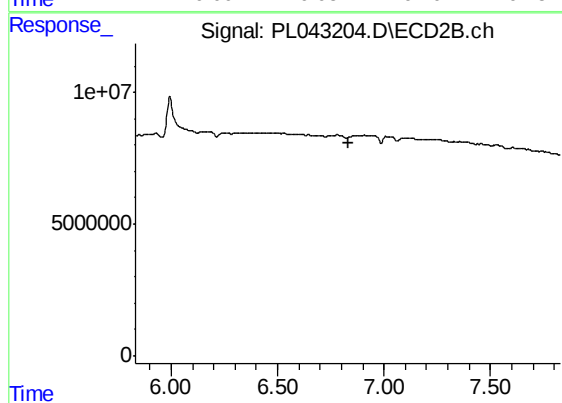

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

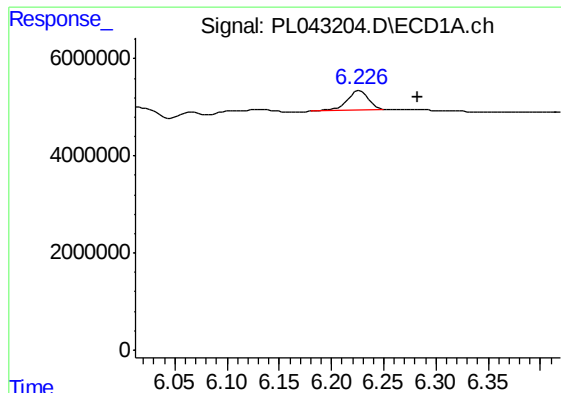

#15 Endosulfan II


R.T.: 6.227 min
Delta R.T.: -0.055 min
Response: 5693245
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

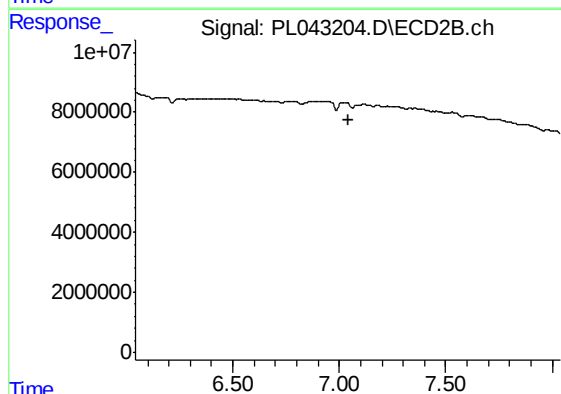


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

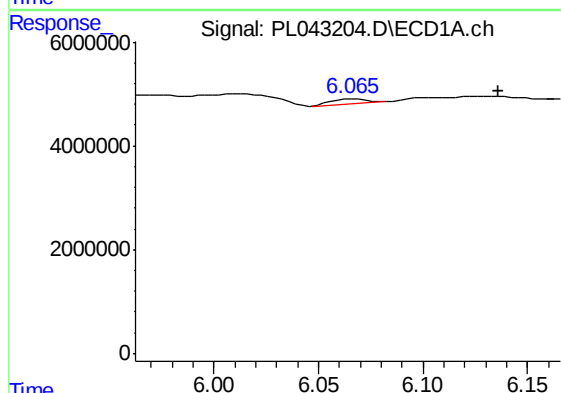


#16 4,4'-DDD

R.T.: 6.066 min
Delta R.T.: -0.070 min
Response: 1101954
Conc: 0.19 ng/ml

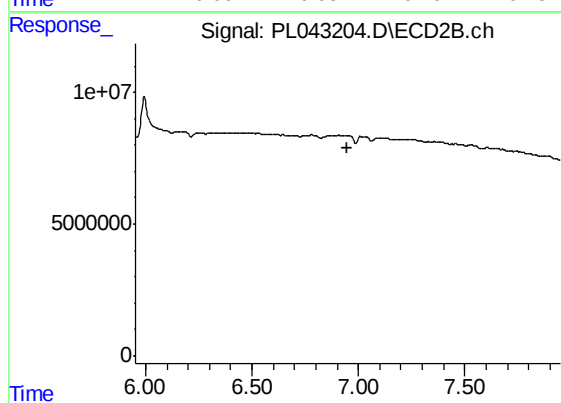

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

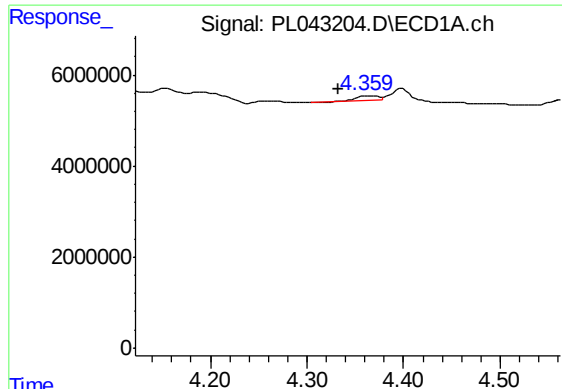

#23 Chlordane-1


R.T.: 4.361 min
Delta R.T.: 0.029 min
Response: 1564018
Conc: 5.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

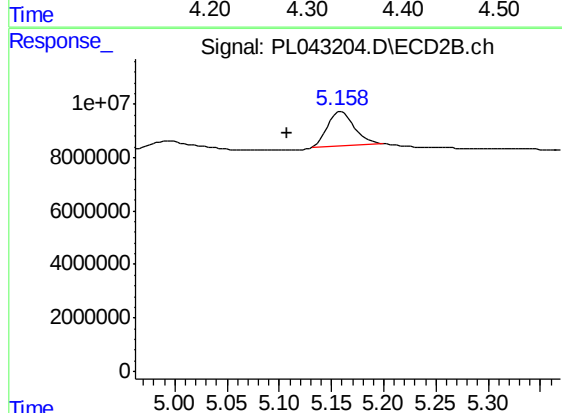


#23 Chlordane-1

R.T.: 5.160 min
Delta R.T.: 0.051 min
Response: 23566932
Conc: 166.75 ng/ml

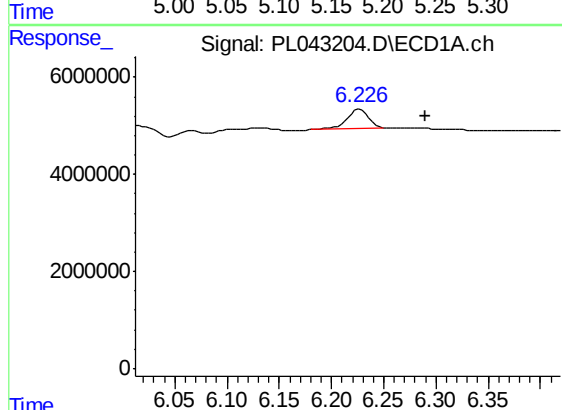


#27 Chlordane-5

R.T.: 6.227 min
Delta R.T.: -0.063 min
Response: 5693245
Conc: 23.74 ng/ml

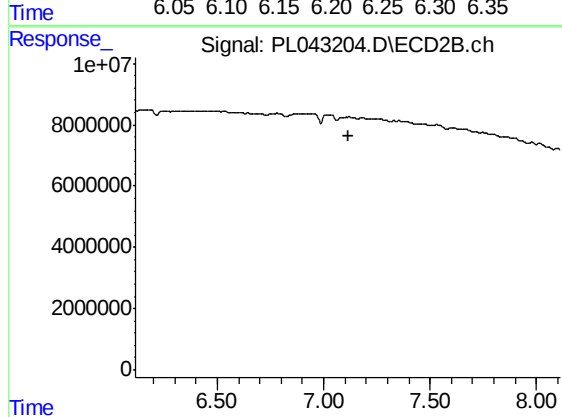

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

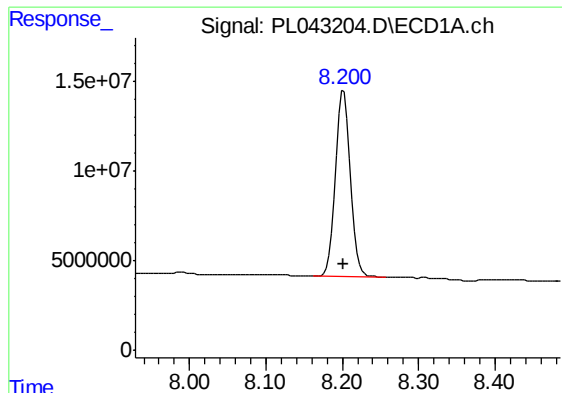

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 139987487
Conc: 21.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

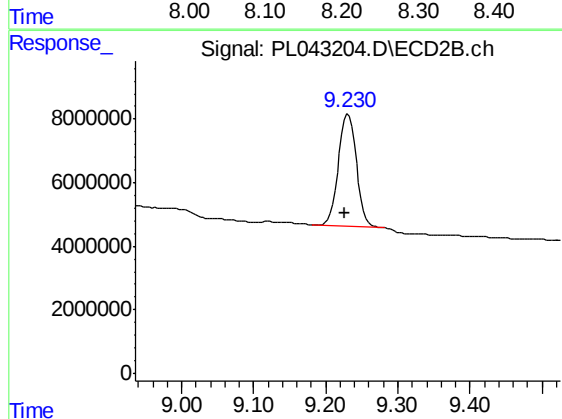

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.004 min
Response: 61497042
Conc: 23.58 ng/ml