

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043206.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 18:55
 Operator : AJ\SJ
 Sample : J6403-40
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-5-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:05:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	127.0E6	64498165	20.709	21.761
28)	SA Decachlor...	8.202	9.232	131.8E6	53474912	20.191	20.500
Target Compounds							
6)	B beta-BHC	4.398f	0.000	3662270	0	0.993	N.D. #
7)	B delta-BHC	0.000	5.158	0	13908447	N.D.	3.236 #
8)	B Heptachlo...	0.000	5.993	0	15471909	N.D.	4.080 #
14)	MA Endrin	6.066f	0.000	1054431	0	0.146	N.D. #
15)	B Endosulfa...	6.228f	0.000	4928185	0	0.741	N.D. #
16)	A 4,4'-DDD	6.066f	0.000	1054431	0	0.186	N.D. #
23)	Chlordane-1	4.365	5.158	1878690	13908447	6.992	98.409 #
27)	Chlordane-5	6.228	0.000	4928185	0	20.547	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043206.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 18:55
Operator : AJ\SJ
Sample : J6403-40
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-5-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:05:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

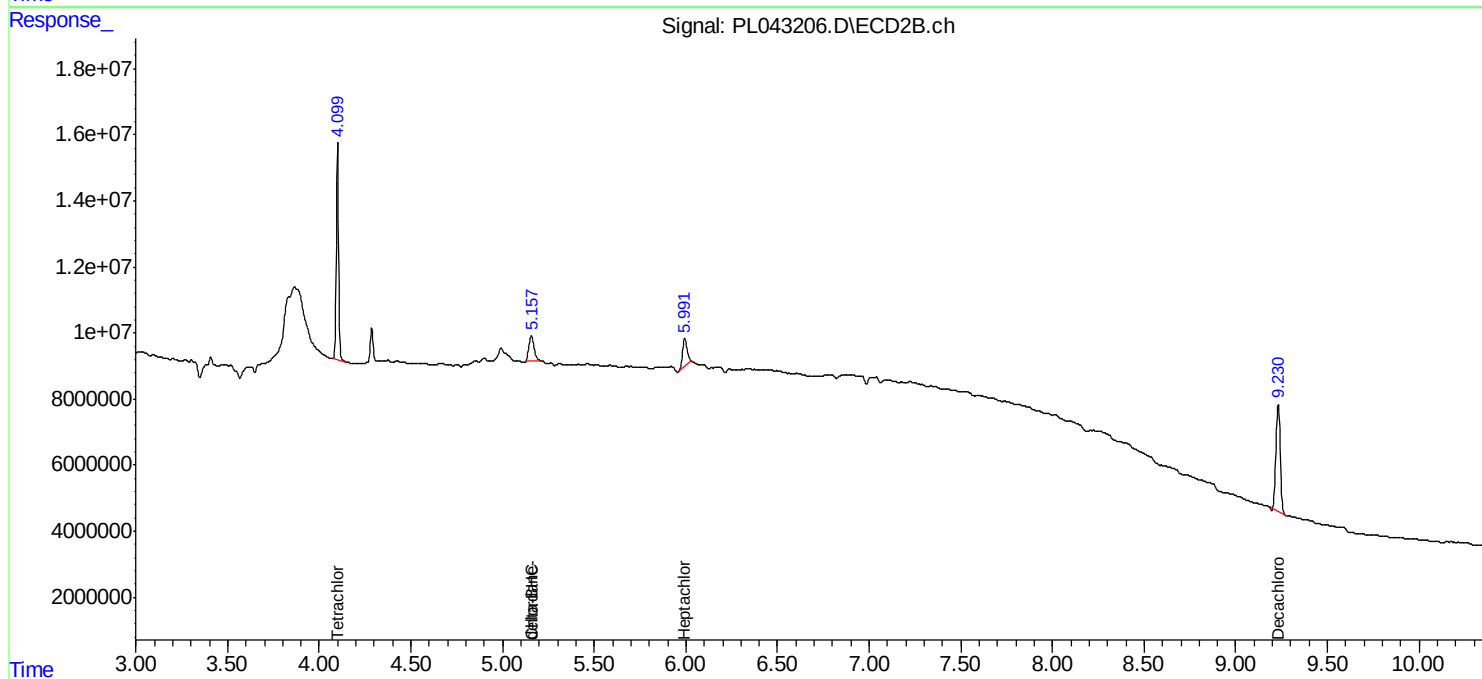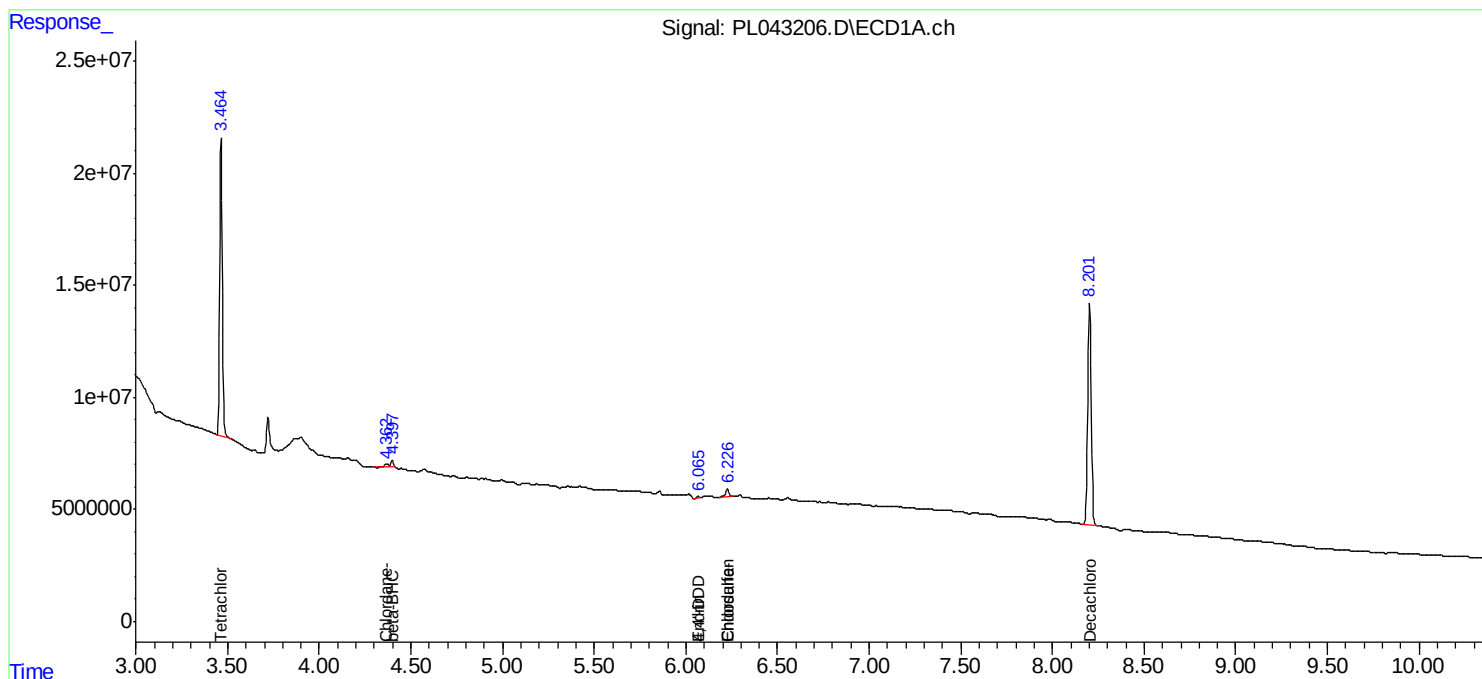


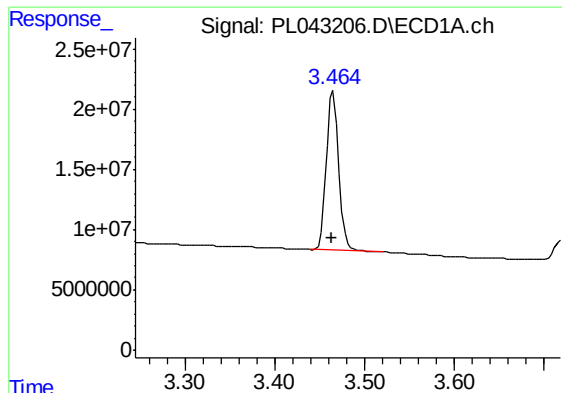

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 127007072
Conc: 20.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-B

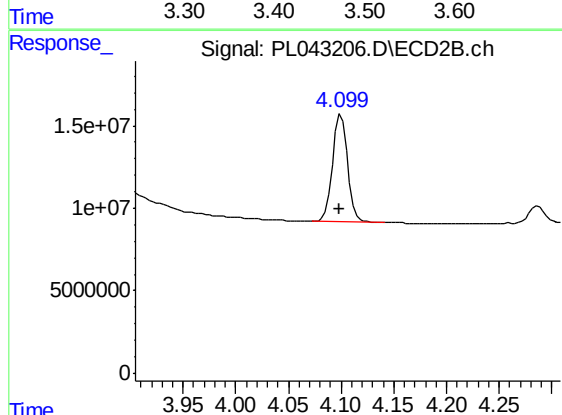


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.001 min
Response: 64498165
Conc: 21.76 ng/ml

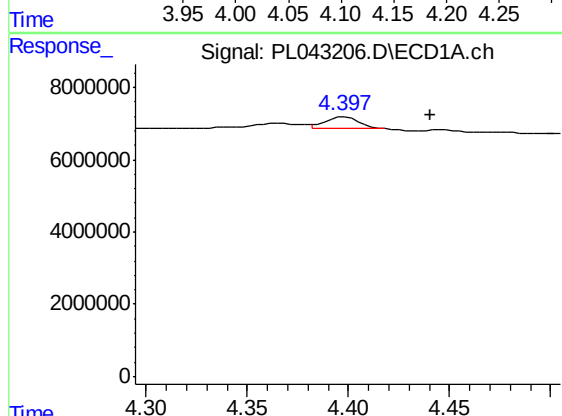


#6 beta-BHC

R.T.: 4.398 min
Delta R.T.: -0.043 min
Response: 3662270
Conc: 0.99 ng/ml

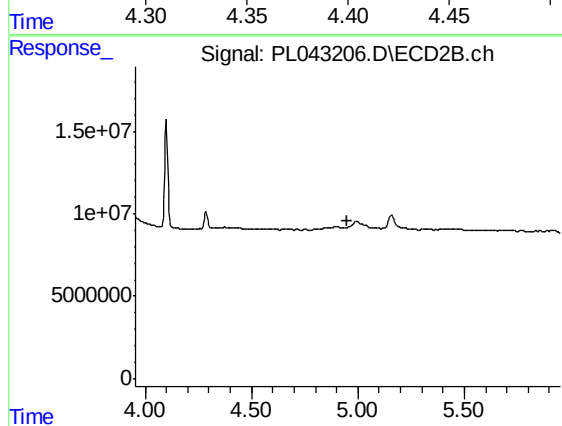

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

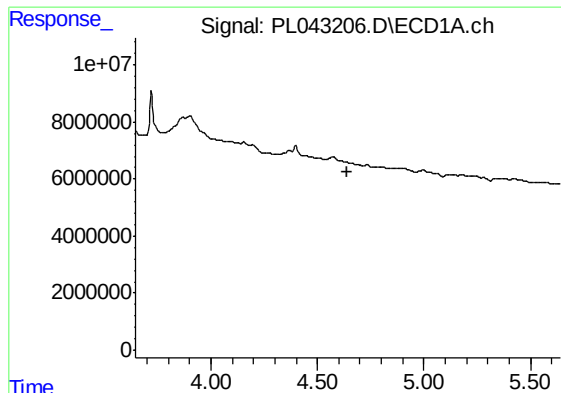

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-5-B

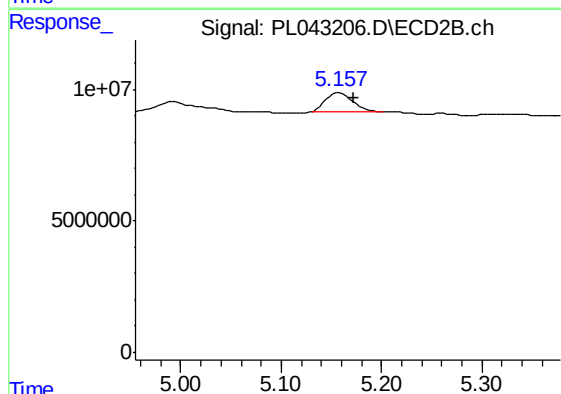


#7 delta-BHC

R.T.: 5.158 min
Delta R.T.: -0.015 min
Response: 13908447
Conc: 3.24 ng/ml

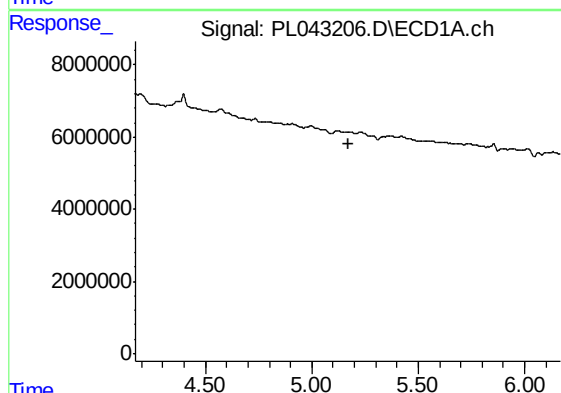


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

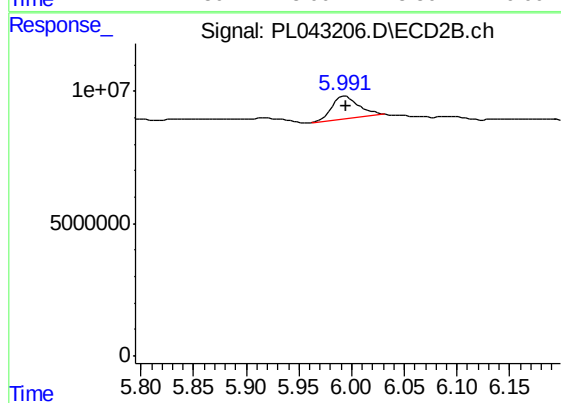

#8 Heptachlor epoxide


R.T.: 5.993 min
Delta R.T.: -0.001 min
Response: 15471909
Conc: 4.08 ng/ml

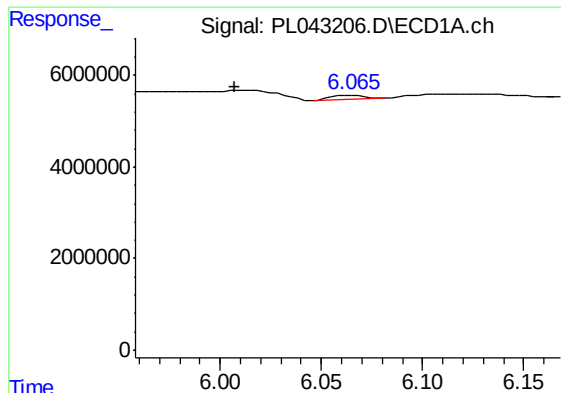

#14 Endrin


R.T.: 6.066 min
Delta R.T.: 0.059 min
Response: 1054431
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-B

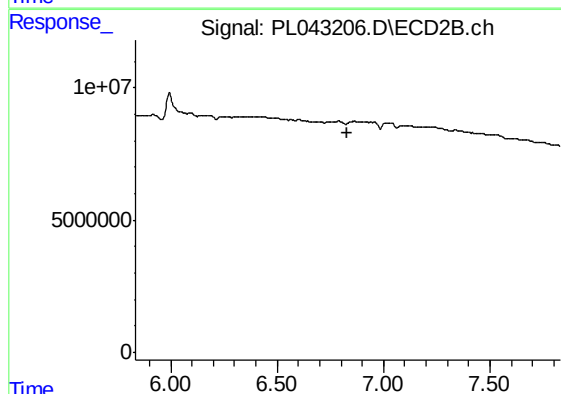


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

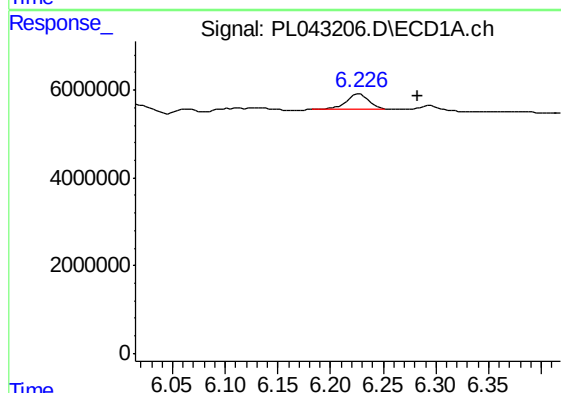


#15 Endosulfan II

R.T.: 6.228 min
Delta R.T.: -0.055 min
Response: 4928185
Conc: 0.74 ng/ml

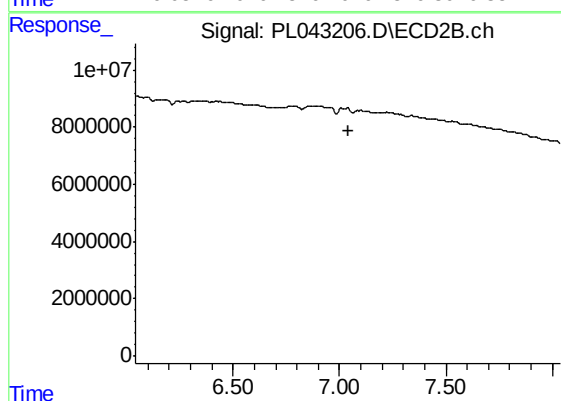

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

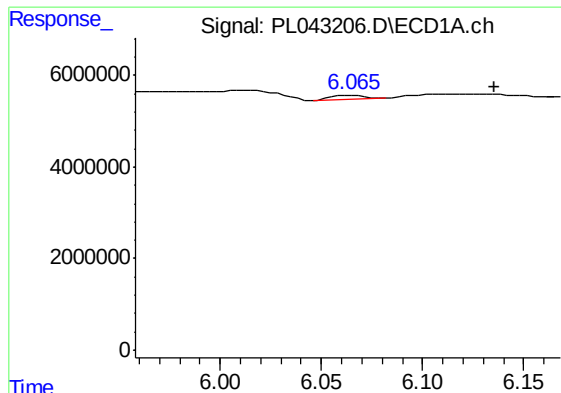

#16 4,4'-DDD


R.T.: 6.066 min
Delta R.T.: -0.070 min
Response: 1054431
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-B

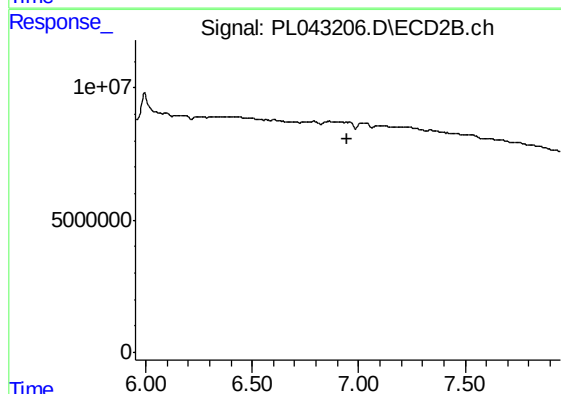


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

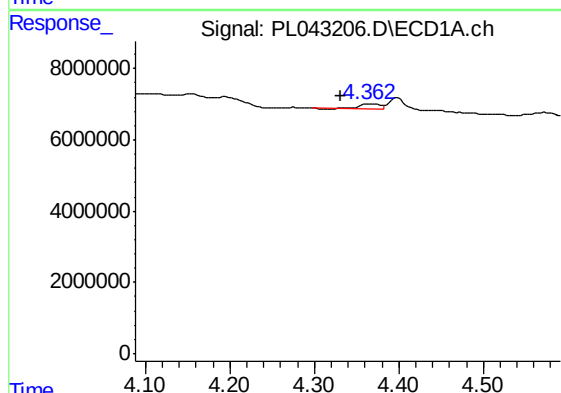


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.032 min
Response: 1878690
Conc: 6.99 ng/ml

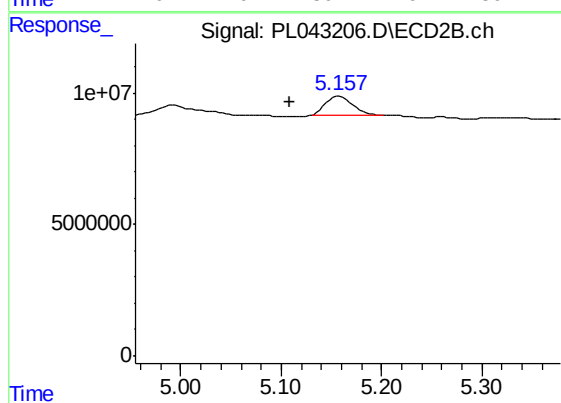

#23 Chlordane-1


R.T.: 5.158 min
Delta R.T.: 0.050 min
Response: 13908447
Conc: 98.41 ng/ml

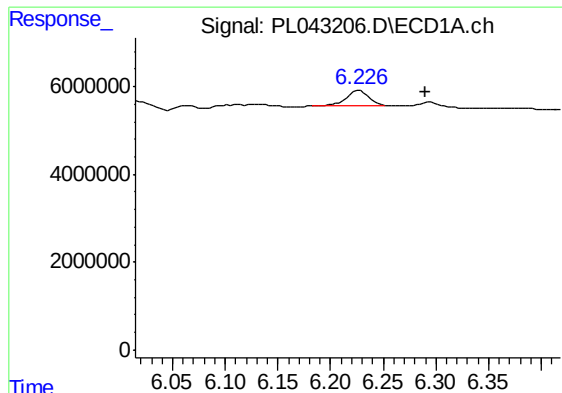

#27 Chlordane-5


R.T.: 6.228 min
Delta R.T.: -0.062 min
Response: 4928185
Conc: 20.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-B

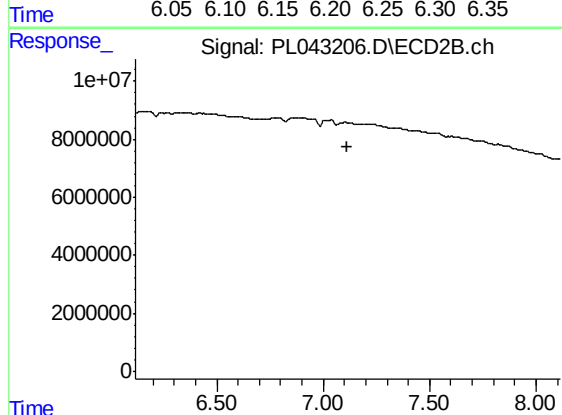


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

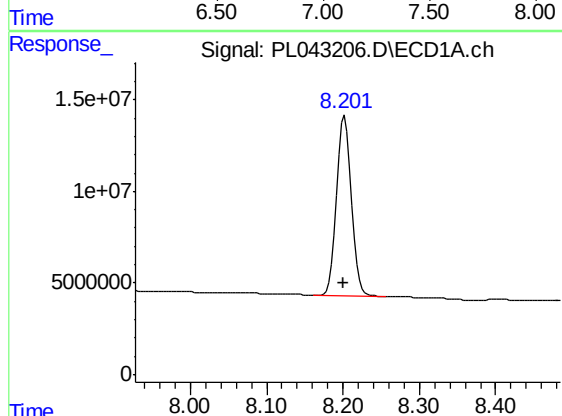

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.001 min
Response: 131849217
Conc: 20.19 ng/ml

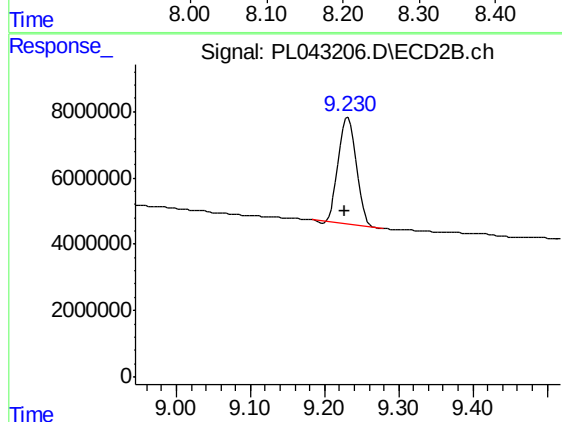

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.005 min
Response: 53474912
Conc: 20.50 ng/ml