

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043209.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 19:38
 Operator : AJ\SJ
 Sample : J6403-44
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:06:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	133.5E6	67559116	21.764	22.794
28)	SA Decachlor...	8.202	9.232	137.0E6	58477636	20.973	22.418
Target Compounds							
6)	B beta-BHC	4.398f	0.000	4625399	0	1.254	N.D. #
7)	B delta-BHC	0.000	5.160	0	19792453	N.D.	4.606 #
8)	B Heptachlo...	0.000	5.995	0	18195039	N.D.	4.798 #
14)	MA Endrin	6.067f	0.000	1231304	0	0.171	N.D. #
15)	B Endosulfa...	6.228f	0.000	4774510	0	0.718	N.D. #
16)	A 4,4'-DDD	6.067f	0.000	1231304	0	0.217	N.D. #
23)	Chlordane-1	4.362	5.160	1629090	19792453	6.063	140.041 #
27)	Chlordane-5	6.228	0.000	4774510	0	19.906	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043209.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 19:38
Operator : AJ\SJ
Sample : J6403-44
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-6-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:06:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

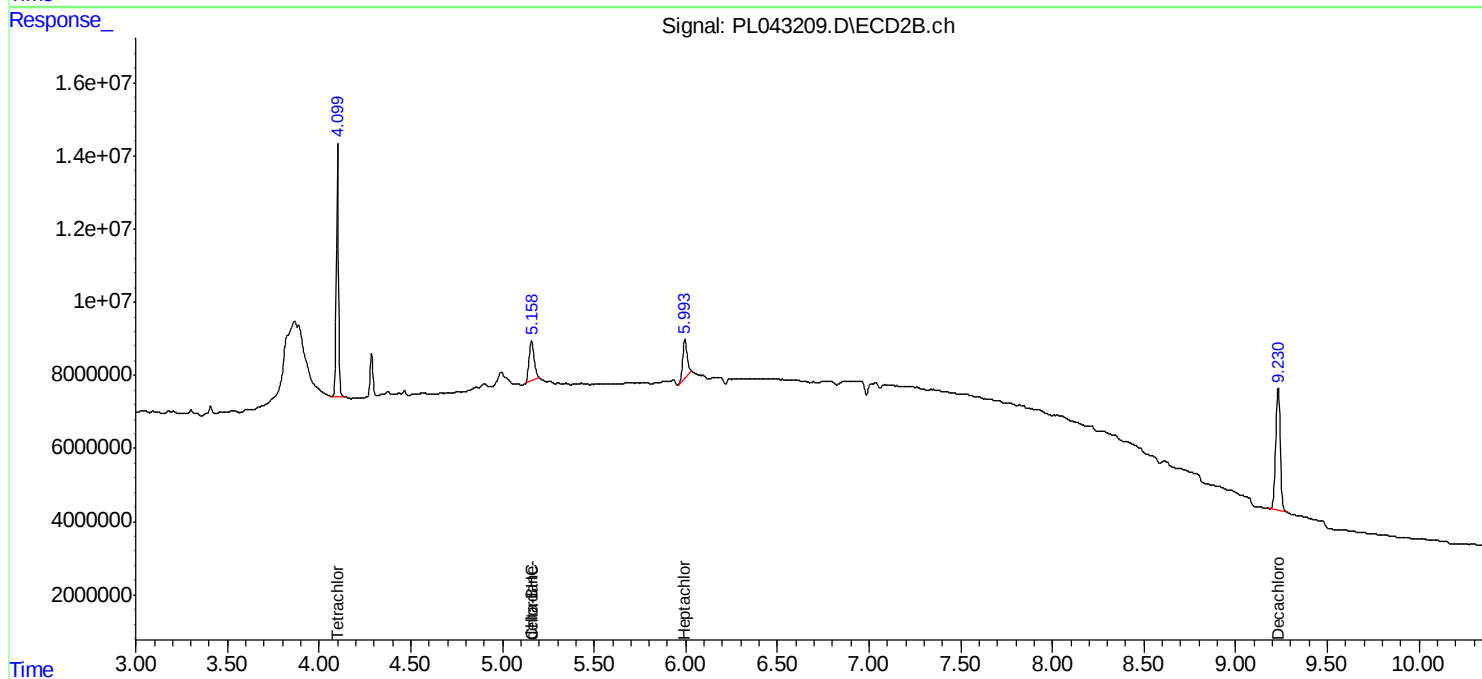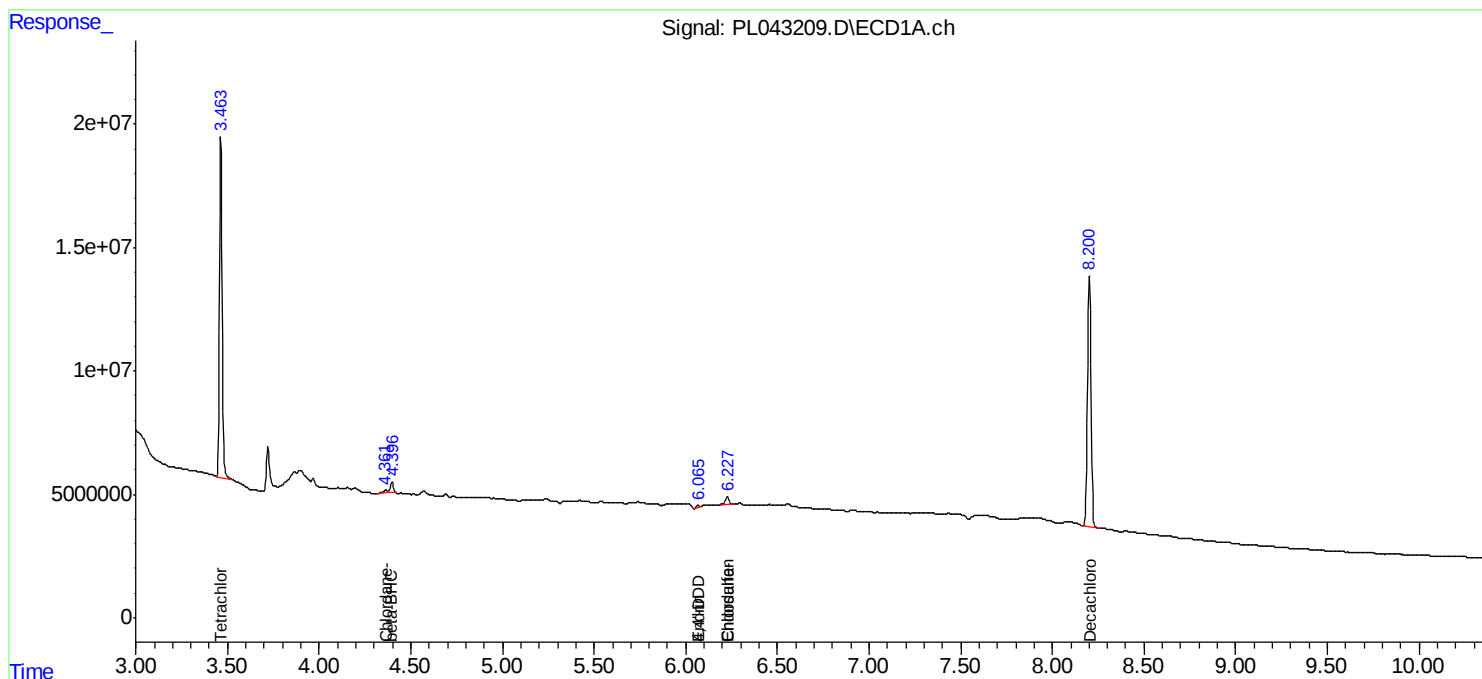


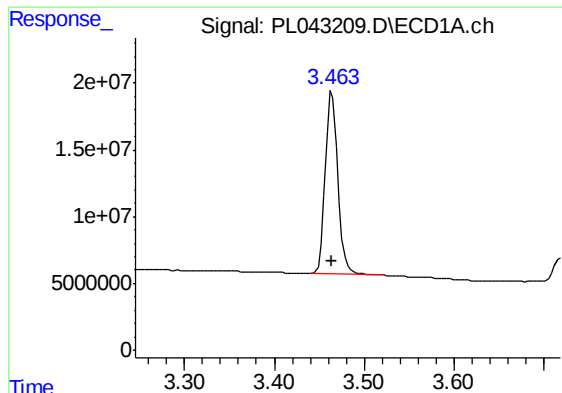

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 133475545
Conc: 21.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-A

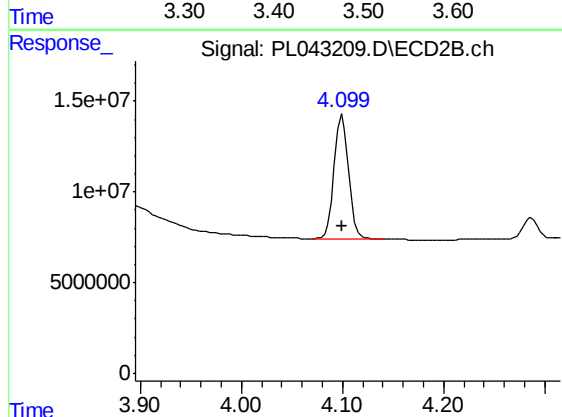


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.001 min
Response: 67559116
Conc: 22.79 ng/ml

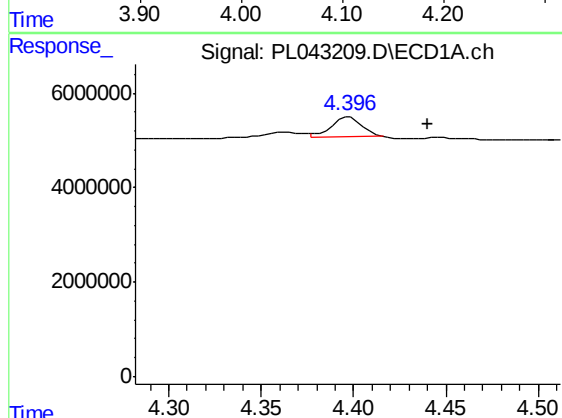


#6 beta-BHC

R.T.: 4.398 min
Delta R.T.: -0.043 min
Response: 4625399
Conc: 1.25 ng/ml

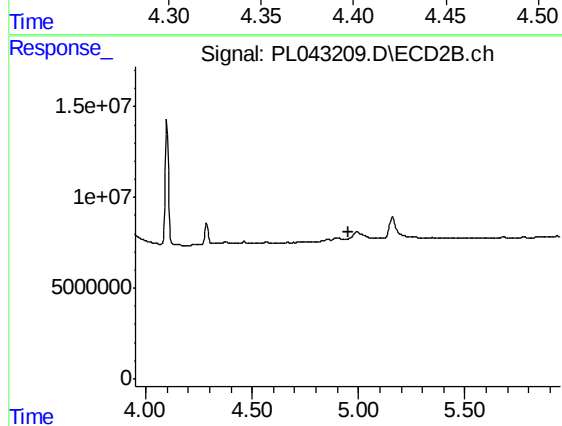

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

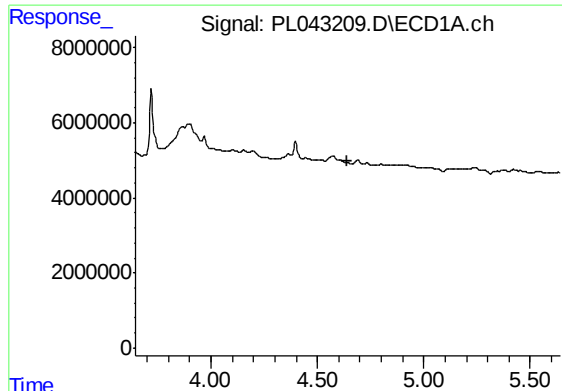

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-6-A

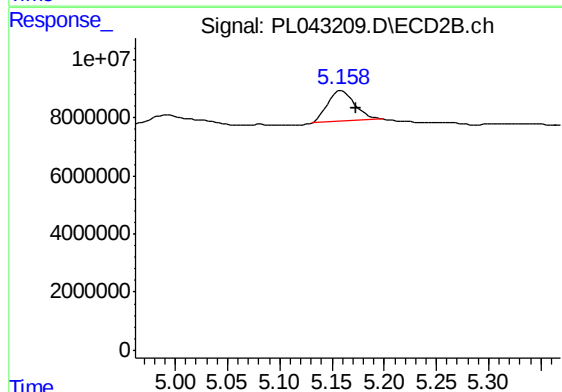


#7 delta-BHC

R.T.: 5.160 min
Delta R.T.: -0.013 min
Response: 19792453
Conc: 4.61 ng/ml

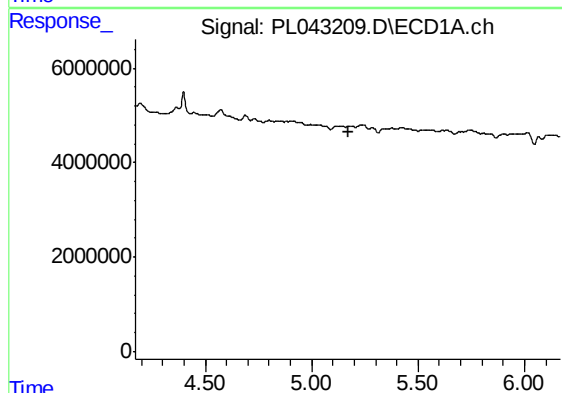


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

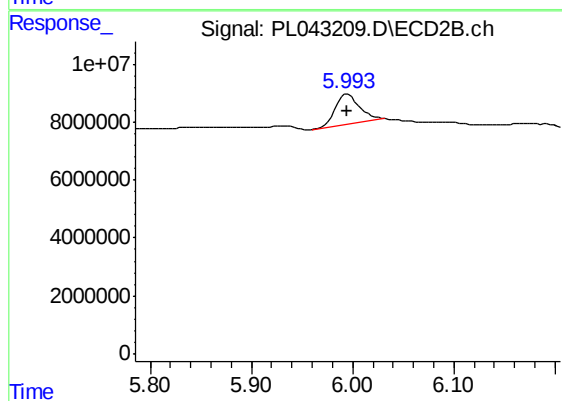

#8 Heptachlor epoxide


R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 18195039
Conc: 4.80 ng/ml

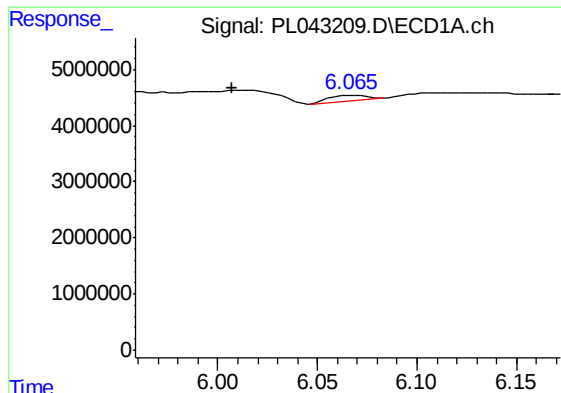

#14 Endrin


R.T.: 6.067 min
Delta R.T.: 0.060 min
Response: 1231304
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-A

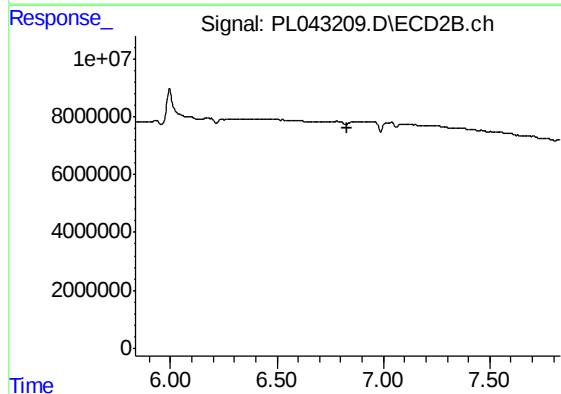


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

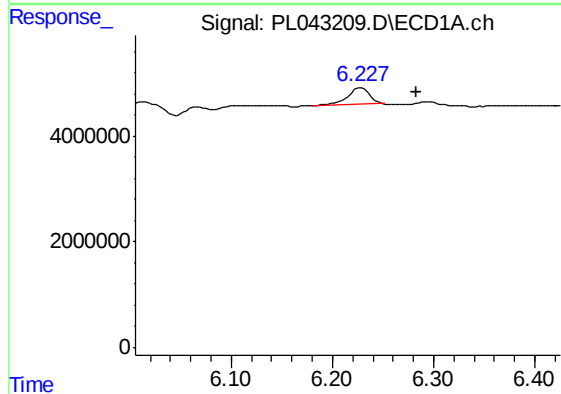


#15 Endosulfan II

R.T.: 6.228 min
Delta R.T.: -0.054 min
Response: 4774510
Conc: 0.72 ng/ml

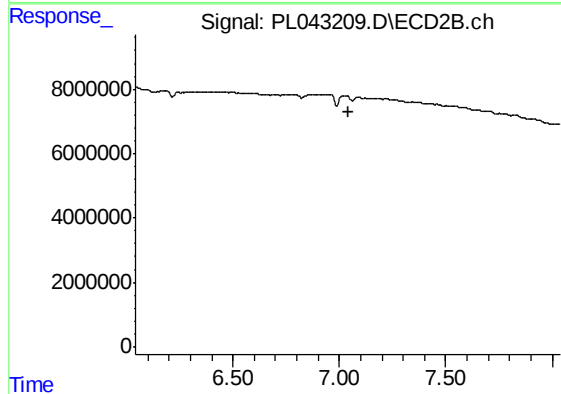

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

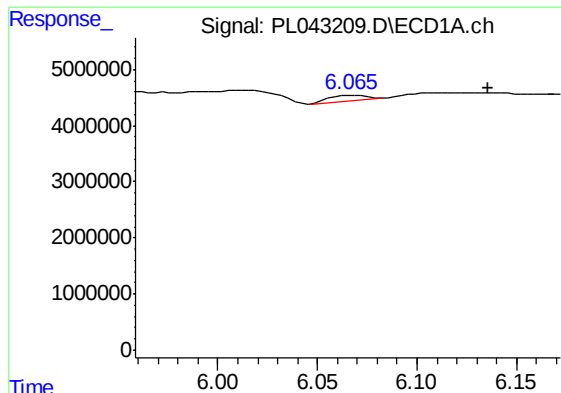

#16 4,4'-DDD


R.T.: 6.067 min
Delta R.T.: -0.069 min
Response: 1231304
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-A

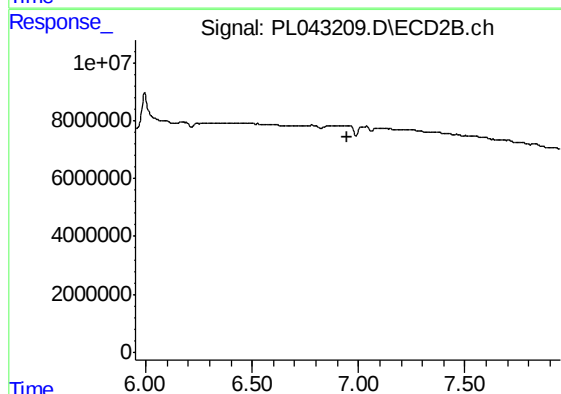


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

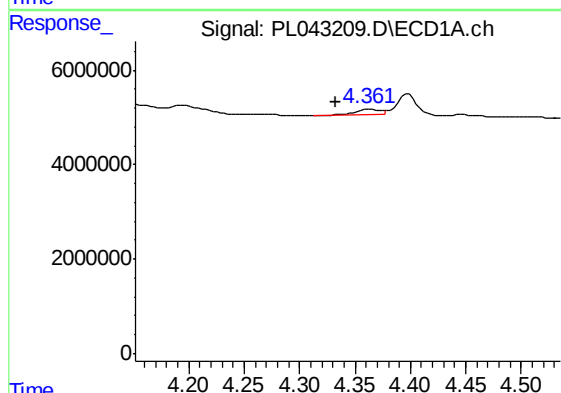


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.030 min
Response: 1629090
Conc: 6.06 ng/ml

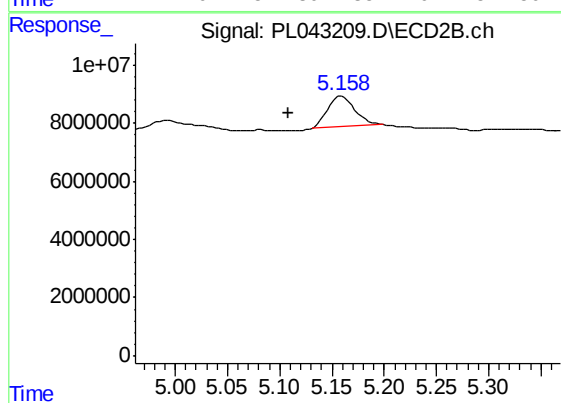

#23 Chlordane-1


R.T.: 5.160 min
Delta R.T.: 0.051 min
Response: 19792453
Conc: 140.04 ng/ml

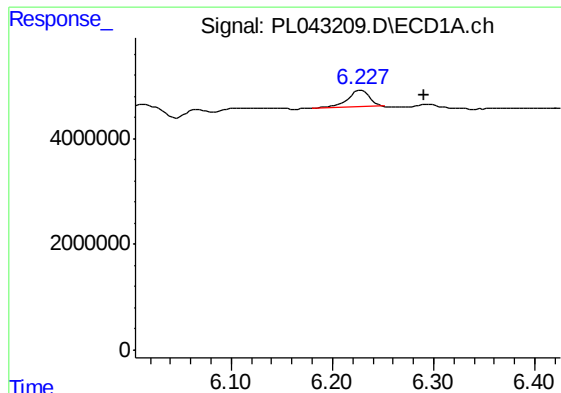

#27 Chlordane-5


R.T.: 6.228 min
Delta R.T.: -0.062 min
Response: 4774510
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-A

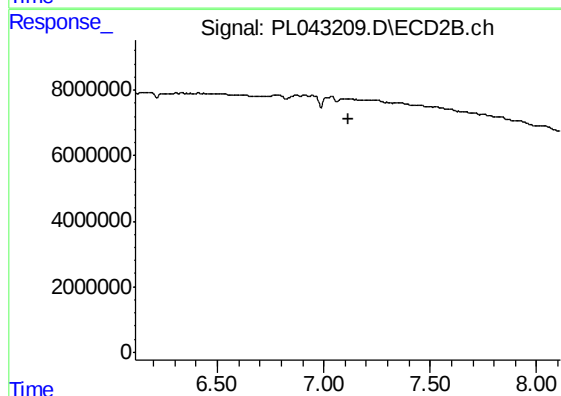


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

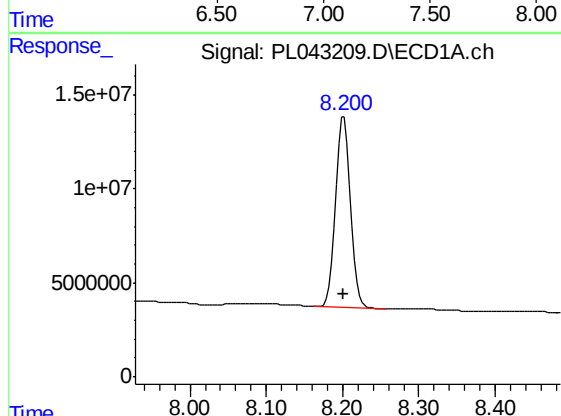

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 136950503
Conc: 20.97 ng/ml

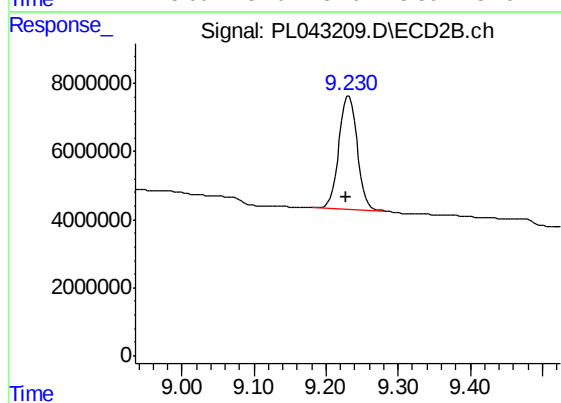

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.005 min
Response: 58477636
Conc: 22.42 ng/ml