

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 19:52
 Operator : AJ\SJ
 Sample : J6403-48
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:06:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	134.3E6	66106406	21.891	22.304
28)	SA Decachlor...	8.203	9.231	137.2E6	58095625	21.016	22.272
Target Compounds							
3)	MA gamma-BHC...	4.197	0.000	3403001	0	0.394	N.D. #
6)	B beta-BHC	4.398f	4.902f	4067184	2570532	1.103	1.518 #
7)	B delta-BHC	0.000	5.161	0	19213733	N.D.	4.471 #
8)	B Heptachlo...	0.000	5.995	0	15730052	N.D.	4.148 #
13)	MA Dieldrin	5.739	0.000	2536600	0	0.326	N.D. #
14)	MA Endrin	6.068f	0.000	1065604	0	0.148	N.D. #
15)	B Endosulfa...	6.227f	0.000	4133327	0	0.621	N.D. #
16)	A 4,4'-DDD	6.068f	0.000	1065604	0	0.188	N.D. #
23)	Chlordane-1	4.362	5.161	1977697	19213733	7.360	135.947 #
27)	Chlordane-5	6.227	0.000	4133327	0	17.233	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 19:52
Operator : AJ\SJ
Sample : J6403-48
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-6-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:06:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

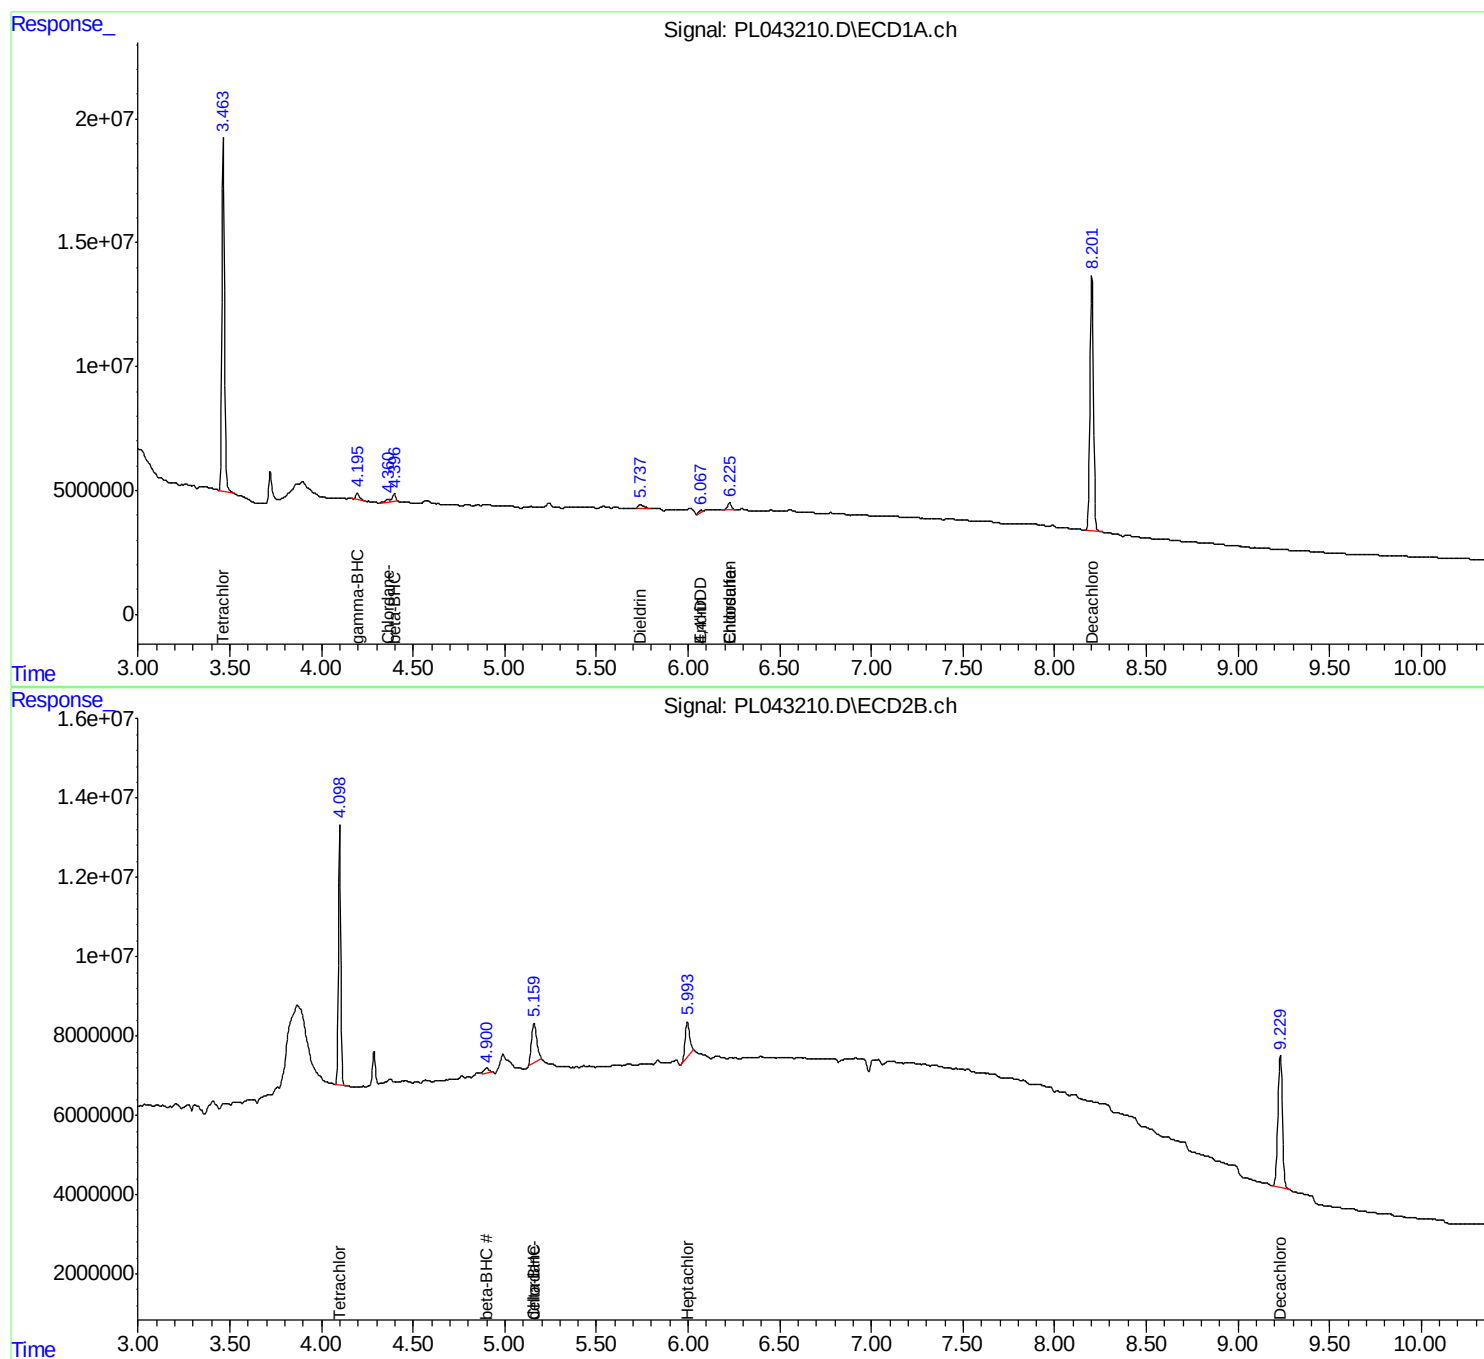


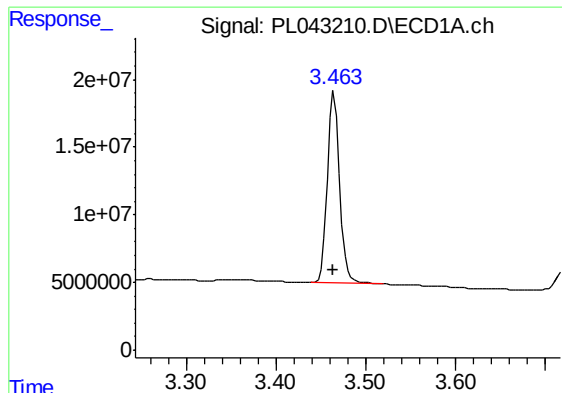

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 134256011
Conc: 21.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-B

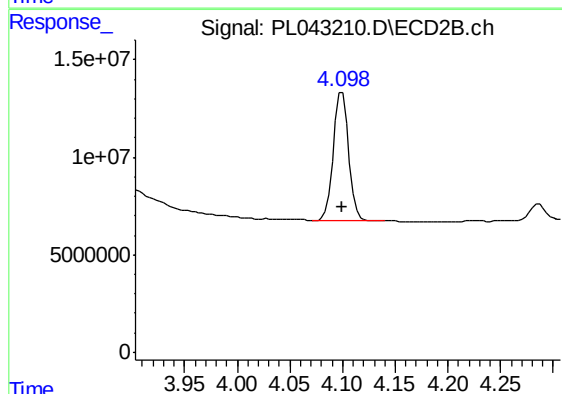


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 66106406
Conc: 22.30 ng/ml

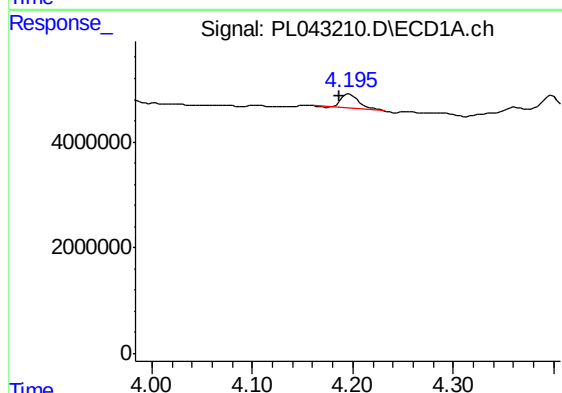


#3 gamma-BHC (Lindane)

R.T.: 4.197 min
Delta R.T.: 0.010 min
Response: 3403001
Conc: 0.39 ng/ml

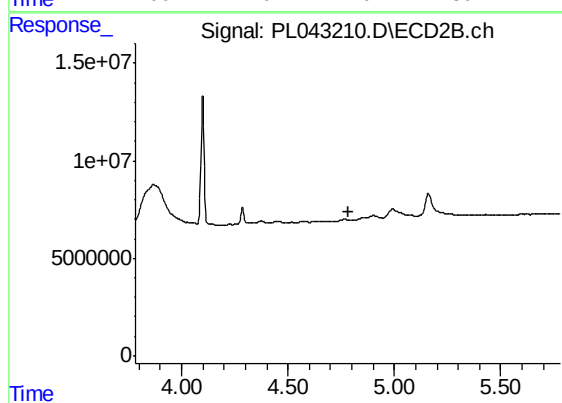

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.783 min
Response: 0
Conc: N.D.

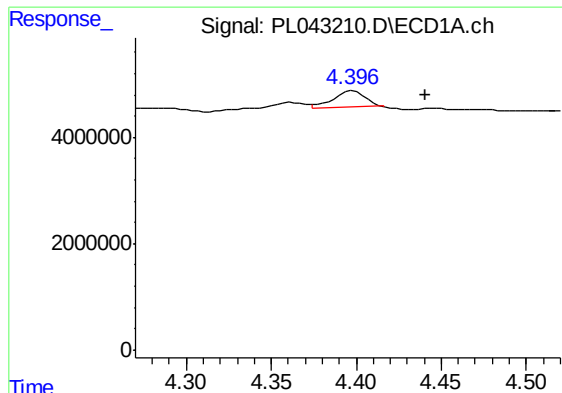

#6 beta-BHC


R.T.: 4.398 min
Delta R.T.: -0.043 min
Response: 4067184
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-B

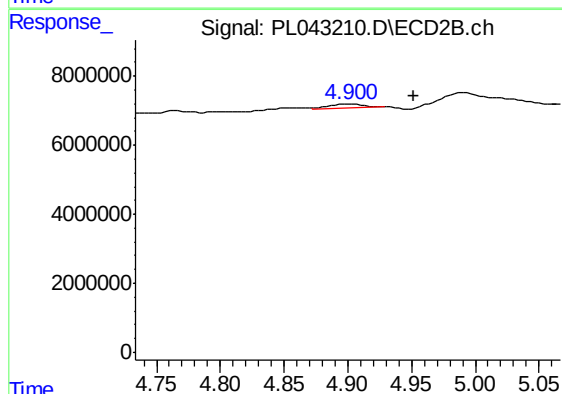


#6 beta-BHC

R.T.: 4.902 min
Delta R.T.: -0.050 min
Response: 2570532
Conc: 1.52 ng/ml

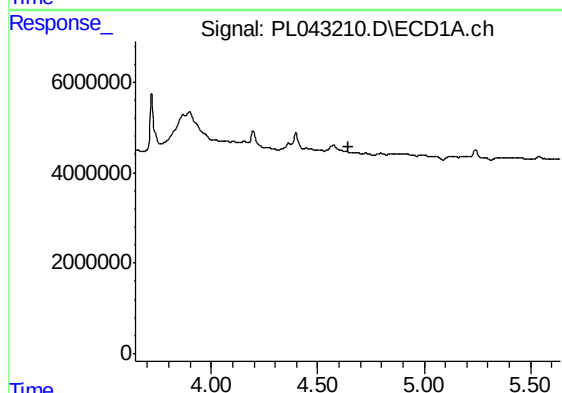


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

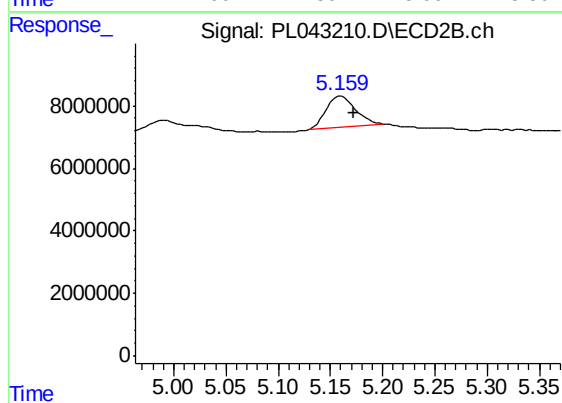

#7 delta-BHC


R.T.: 5.161 min
Delta R.T.: -0.012 min
Response: 19213733
Conc: 4.47 ng/ml

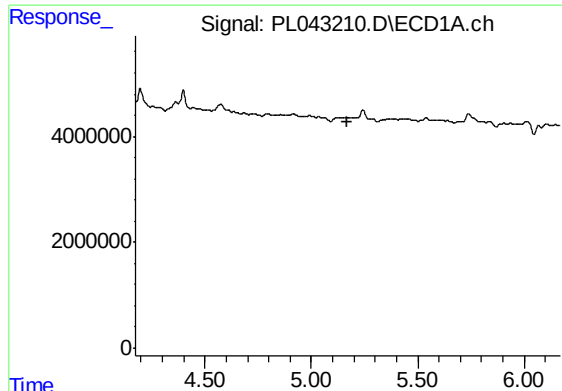

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-6-B

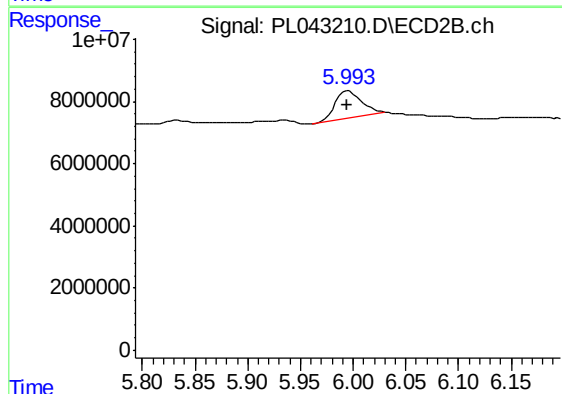


#8 Heptachlor epoxide

R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 15730052
Conc: 4.15 ng/ml

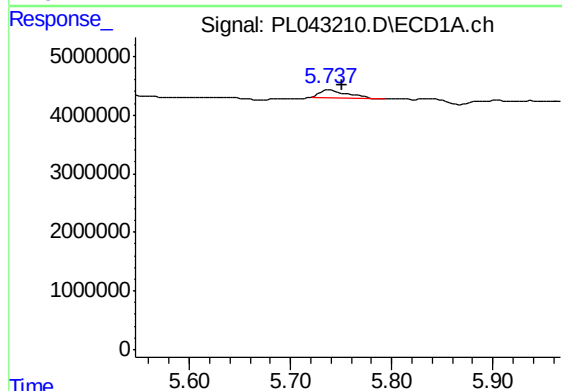


#13 Dieldrin

R.T.: 5.739 min
Delta R.T.: -0.012 min
Response: 2536600
Conc: 0.33 ng/ml

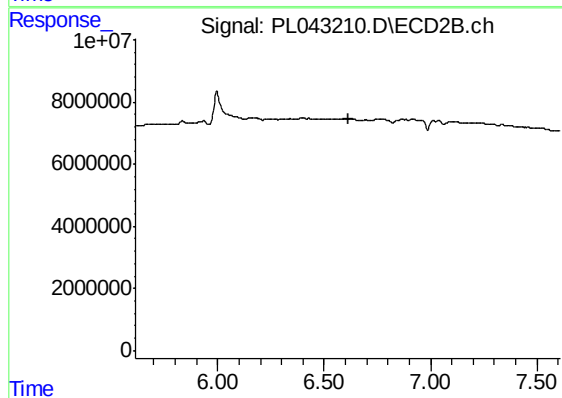

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.613 min
Response: 0
Conc: N.D.

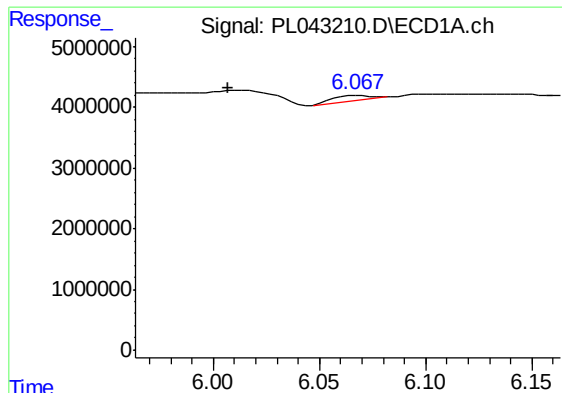

#14 Endrin


R.T.: 6.068 min
Delta R.T.: 0.061 min
Response: 1065604
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-B

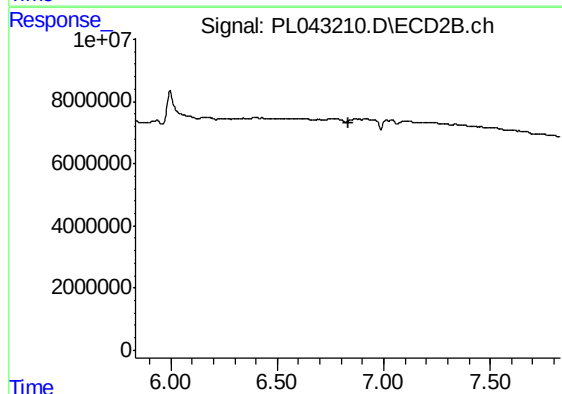


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

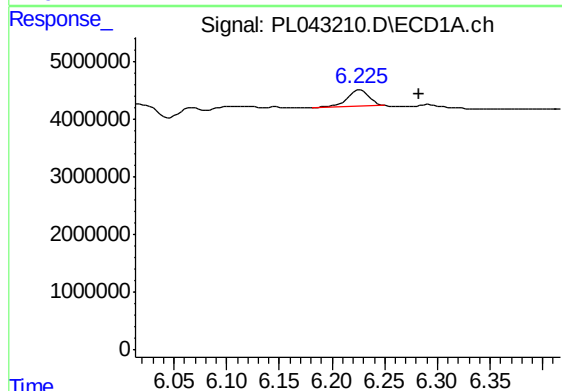


#15 Endosulfan II

R.T.: 6.227 min
Delta R.T.: -0.056 min
Response: 4133327
Conc: 0.62 ng/ml

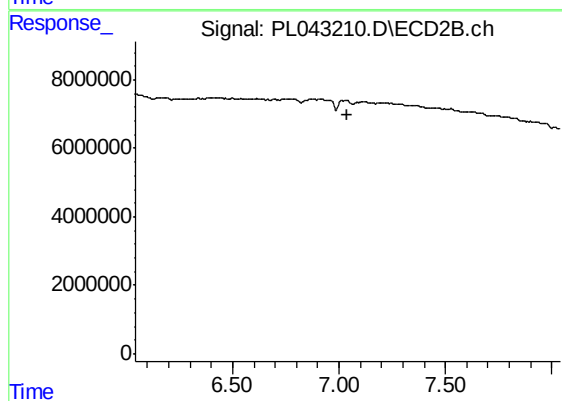

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

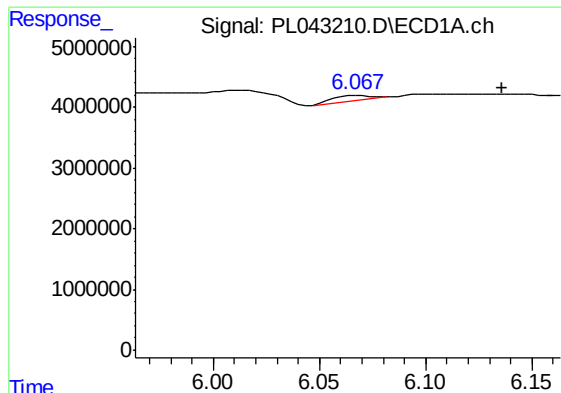

#16 4,4'-DDD


R.T.: 6.068 min
Delta R.T.: -0.068 min
Response: 1065604
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-B

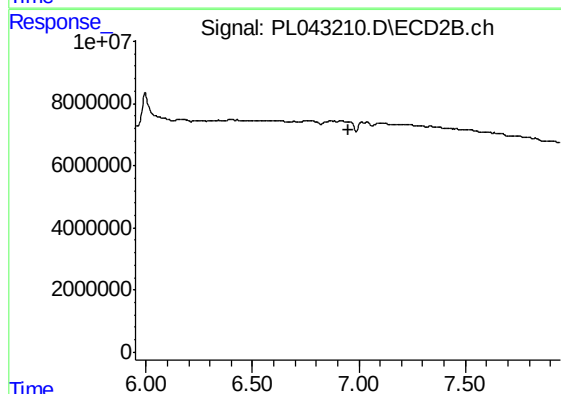


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

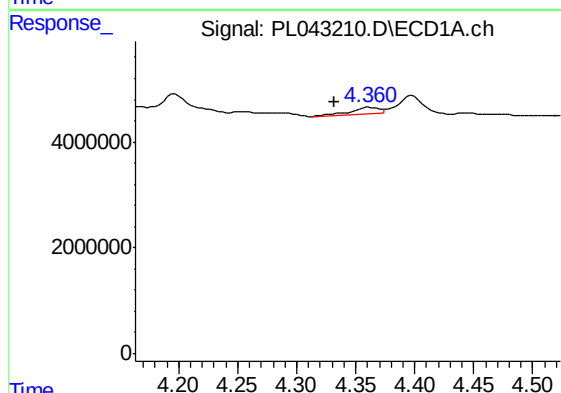


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.030 min
Response: 1977697
Conc: 7.36 ng/ml

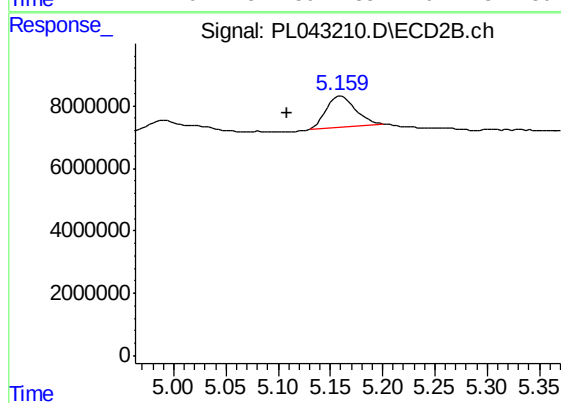

#23 Chlordane-1


R.T.: 5.161 min
Delta R.T.: 0.053 min
Response: 19213733
Conc: 135.95 ng/ml

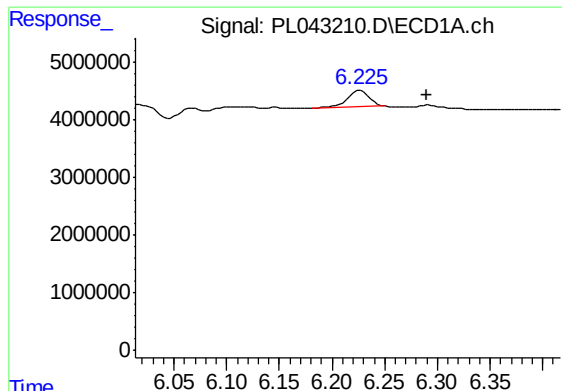

#27 Chlordane-5


R.T.: 6.227 min
Delta R.T.: -0.063 min
Response: 4133327
Conc: 17.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-B

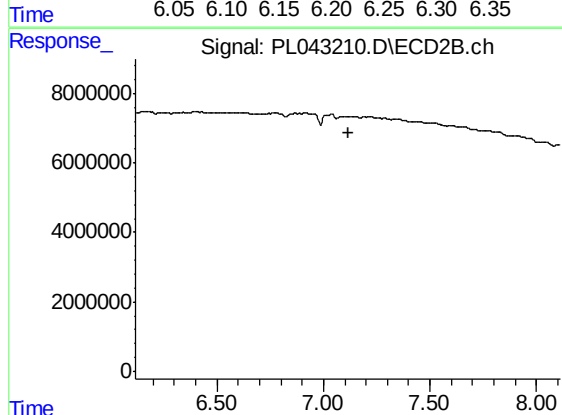


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

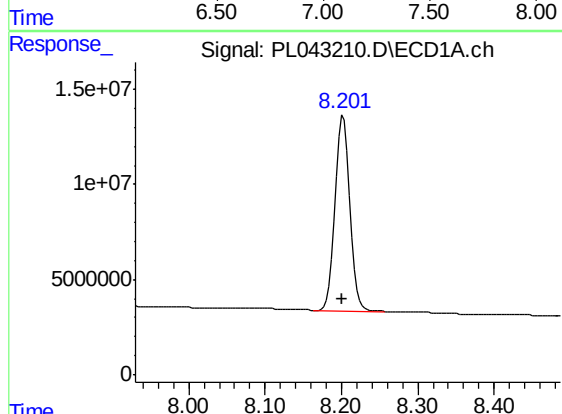

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.001 min
Response: 137236780
Conc: 21.02 ng/ml

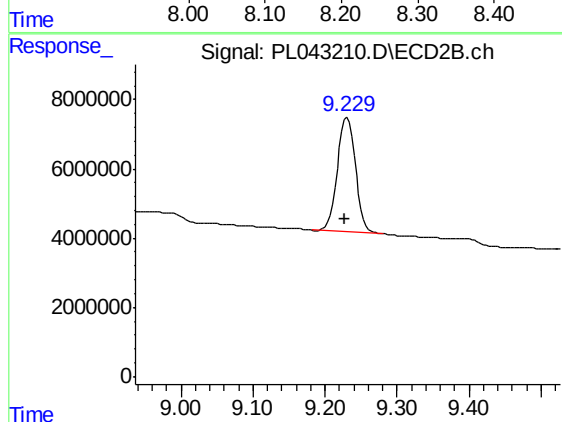

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.004 min
Response: 58095625
Conc: 22.27 ng/ml