

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
 Data File : PL043211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 20:06
 Operator : AJ\SJ
 Sample : J6403-60
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-8-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:06:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	123.2E6	64069959	20.096	21.617
28)	SA Decachlor...	8.202	9.232	138.4E6	59877226	21.193	22.955
Target Compounds							
3)	MA gamma-BHC...	4.197	4.766	8764899	1887755	1.015	0.450 #
6)	B beta-BHC	4.398f	4.903f	2105253	2044289	0.571	1.208 #
7)	B delta-BHC	4.642	5.160	1168875	10221390	0.144	2.378 #
8)	B Heptachlo...	0.000	5.995	0	12526283	N.D.	3.303 #
9)	A Endosulfan I	5.540	0.000	1690441	0	0.231	N.D. #
13)	MA Dieldrin	5.739	0.000	807588	0	0.104	N.D. #
14)	MA Endrin	6.012	6.859	5577770	-1383845	0.775	N.D. #
15)	B Endosulfa...	6.228f	0.000	3607388	0	0.542	N.D. #
23)	Chlordane-1	4.377	5.160	-688581	10221390	N.D.	72.321
27)	Chlordane-5	6.228	0.000	3607388	0	15.040	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121718\
Data File : PL043211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 20:06
Operator : AJ\SJ
Sample : J6403-60
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-8-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:06:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

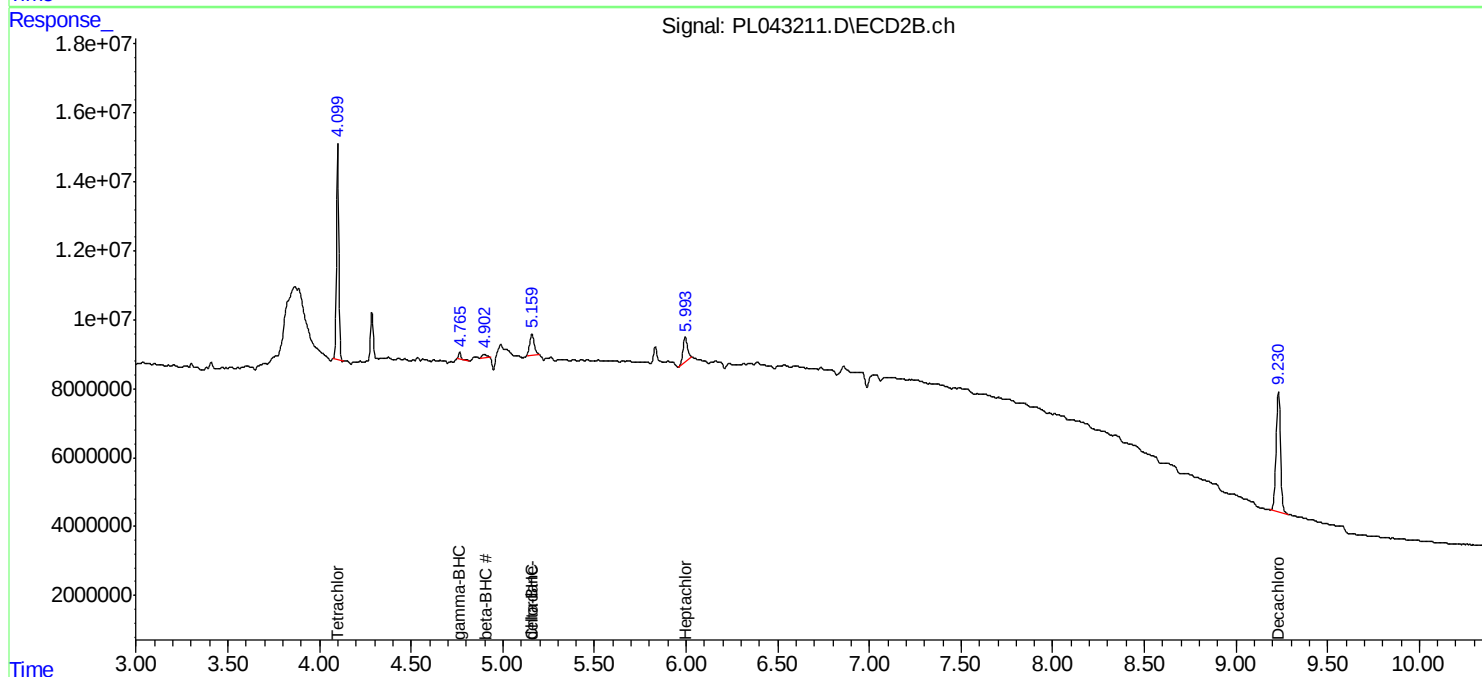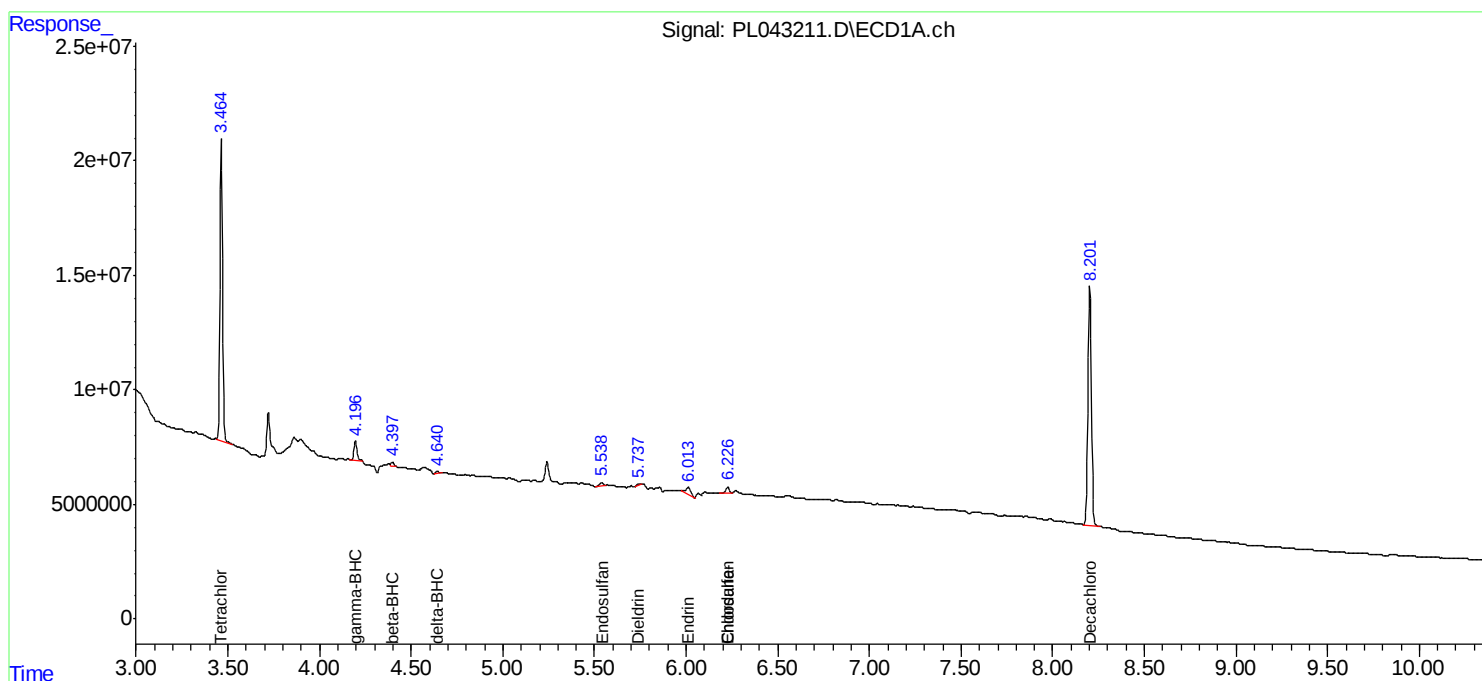


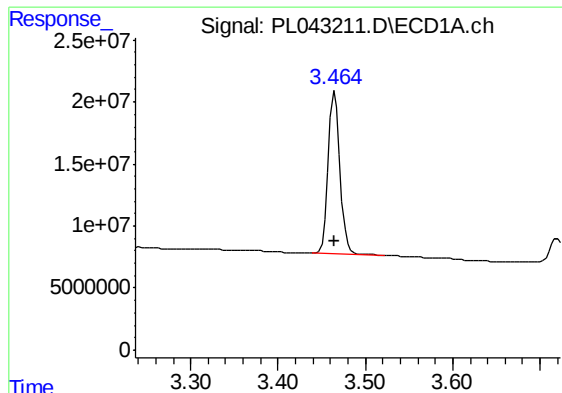

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 123244614
Conc: 20.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8-A

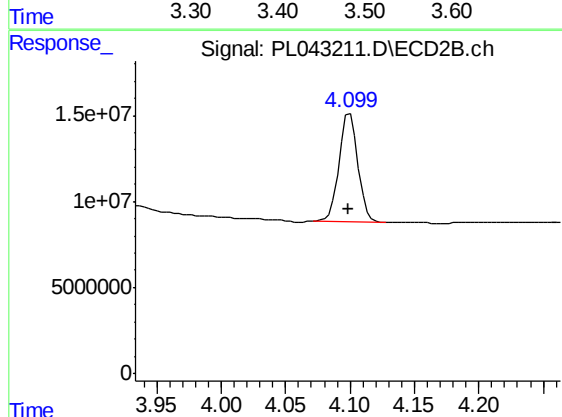


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.001 min
Response: 64069959
Conc: 21.62 ng/ml

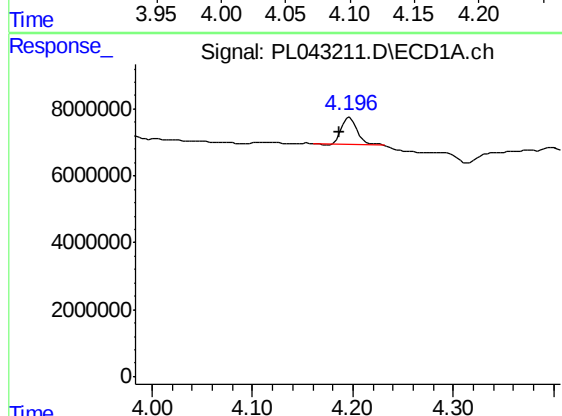


#3 gamma-BHC (Lindane)

R.T.: 4.197 min
Delta R.T.: 0.010 min
Response: 8764899
Conc: 1.02 ng/ml

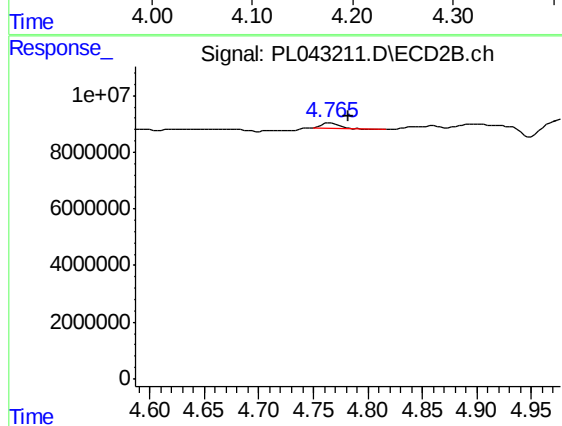

#3 gamma-BHC (Lindane)


R.T.: 4.766 min
Delta R.T.: -0.017 min
Response: 1887755
Conc: 0.45 ng/ml

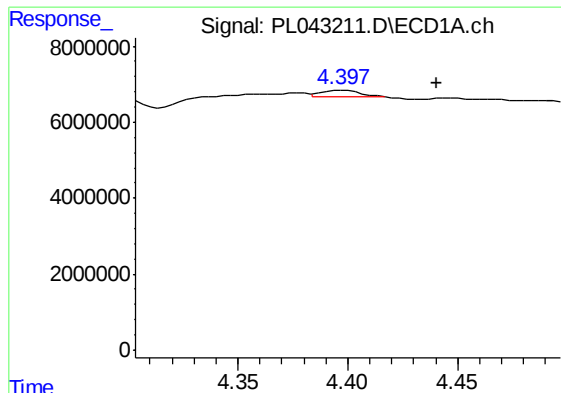

#6 beta-BHC


R.T.: 4.398 min
Delta R.T.: -0.042 min
Response: 2105253
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8-A

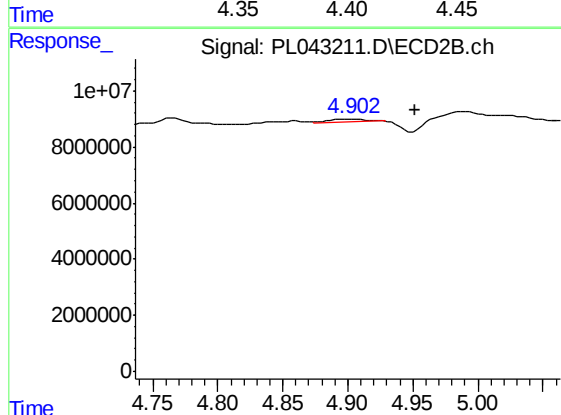


#6 beta-BHC

R.T.: 4.903 min
Delta R.T.: -0.049 min
Response: 2044289
Conc: 1.21 ng/ml

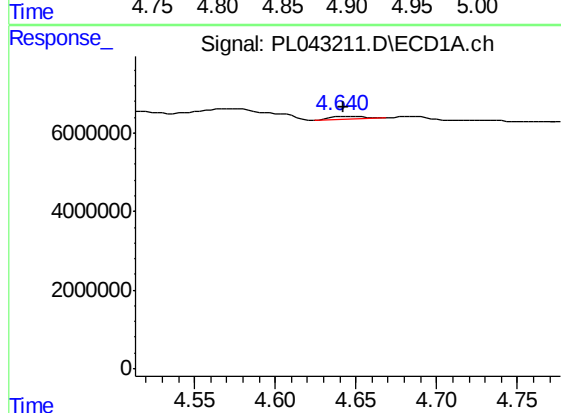


#7 delta-BHC

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 1168875
Conc: 0.14 ng/ml

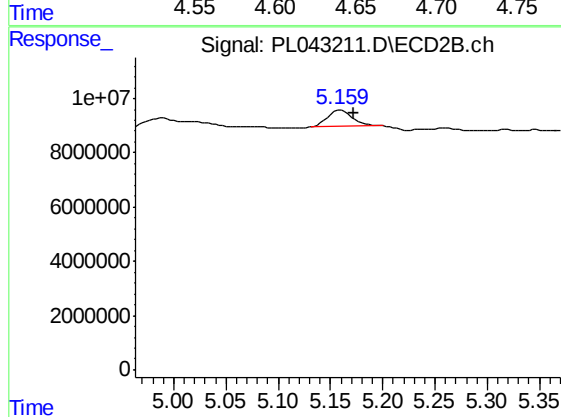

#7 delta-BHC


R.T.: 5.160 min
Delta R.T.: -0.013 min
Response: 10221390
Conc: 2.38 ng/ml

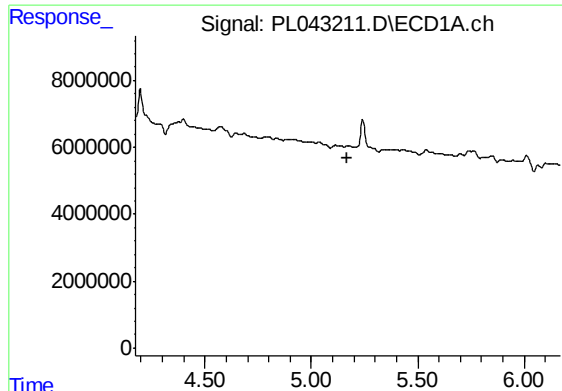

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-8-A

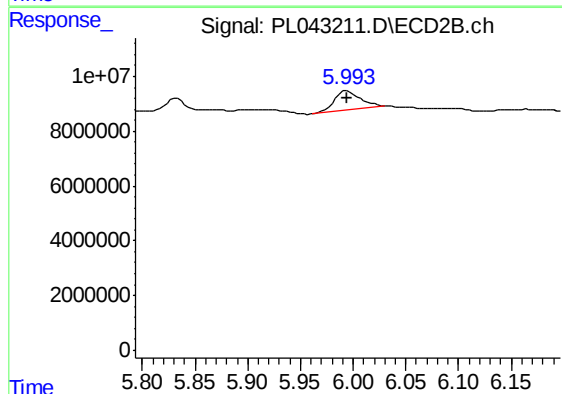


#8 Heptachlor epoxide

R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 12526283
Conc: 3.30 ng/ml

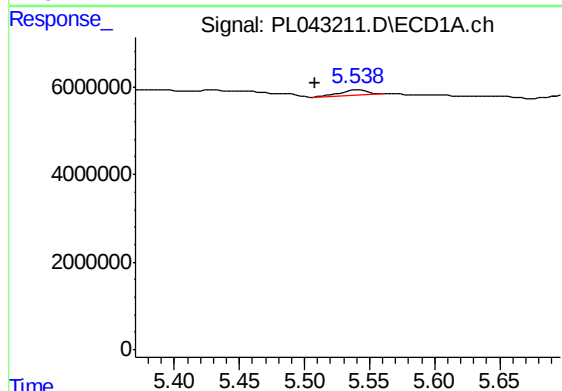


#9 Endosulfan I

R.T.: 5.540 min
Delta R.T.: 0.032 min
Response: 1690441
Conc: 0.23 ng/ml

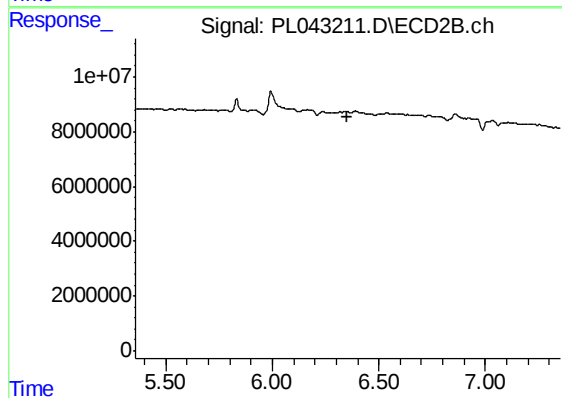

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

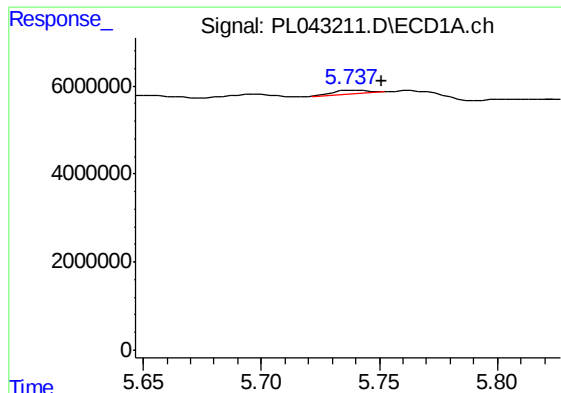

#13 Dielddrin


R.T.: 5.739 min
Delta R.T.: -0.012 min
Response: 807588
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8-A

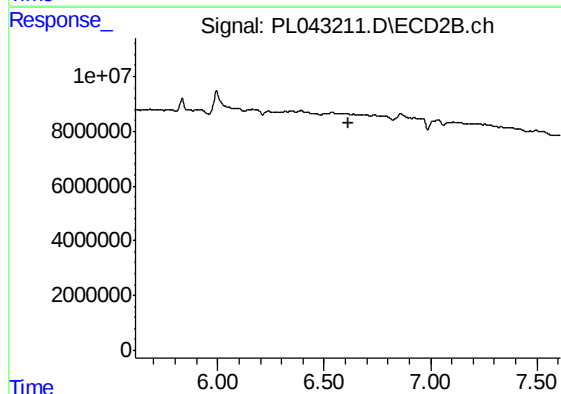


#13 Dielddrin

R.T.: 0.000 min
Exp R.T. : 6.613 min
Response: 0
Conc: N.D.

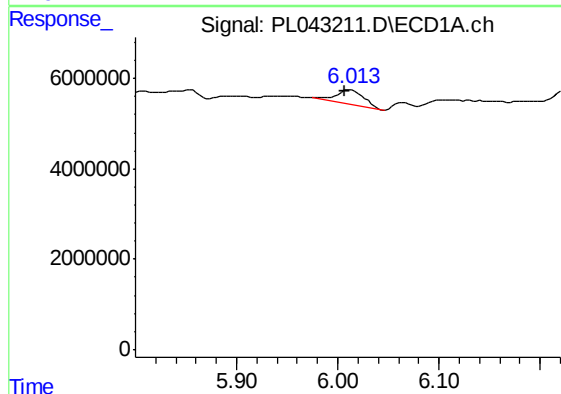


#14 Endrin

R.T.: 6.012 min
Delta R.T.: 0.005 min
Response: 5577770
Conc: 0.77 ng/ml

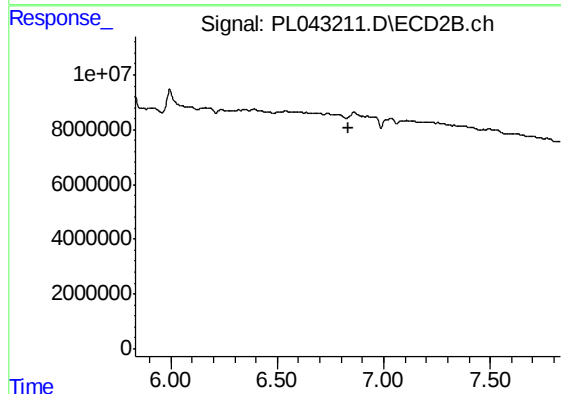

#14 Endrin


R.T.: 6.859 min
Delta R.T.: 0.027 min
Response: -1383845
Conc: N.D.

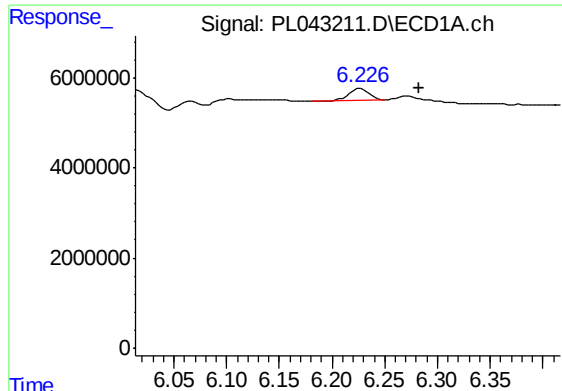

#15 Endosulfan II


R.T.: 6.228 min
Delta R.T.: -0.055 min
Response: 3607388
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8-A

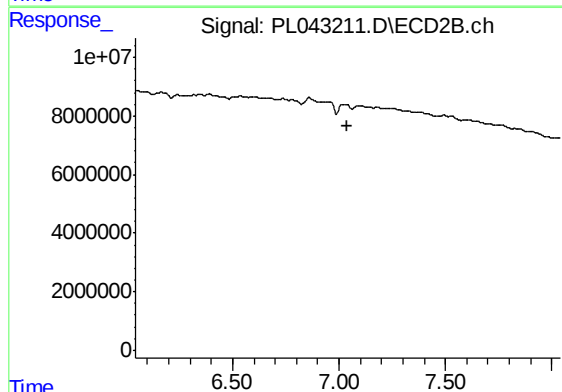


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

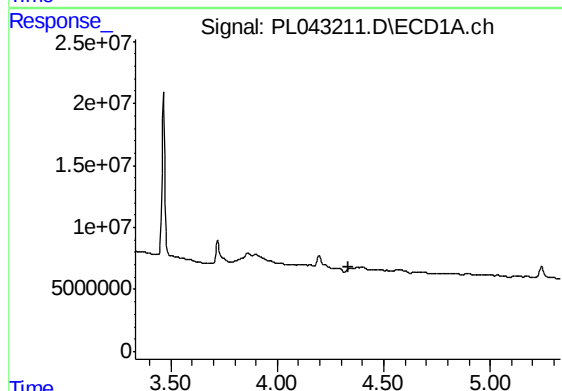


#23 Chlordane-1

R.T.: 4.377 min
Delta R.T.: 0.044 min
Response: -688581
Conc: N.D.

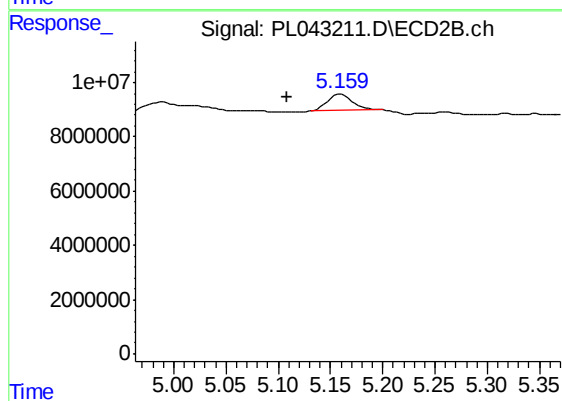

#23 Chlordane-1


R.T.: 5.160 min
Delta R.T.: 0.052 min
Response: 10221390
Conc: 72.32 ng/ml

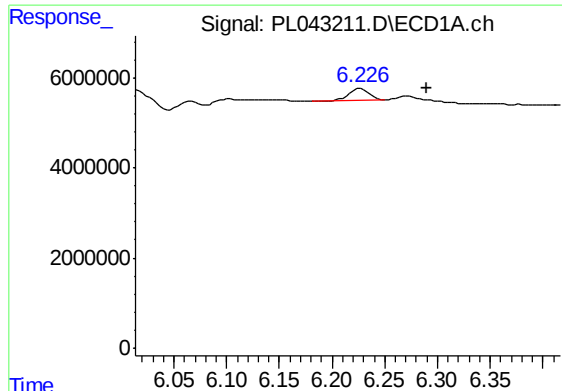

#27 Chlordane-5


R.T.: 6.228 min
Delta R.T.: -0.063 min
Response: 3607388
Conc: 15.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8-A

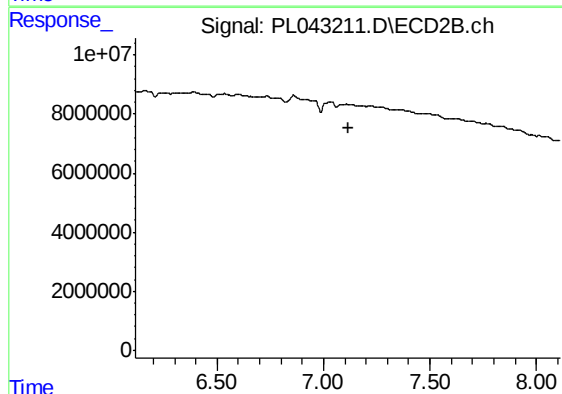


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

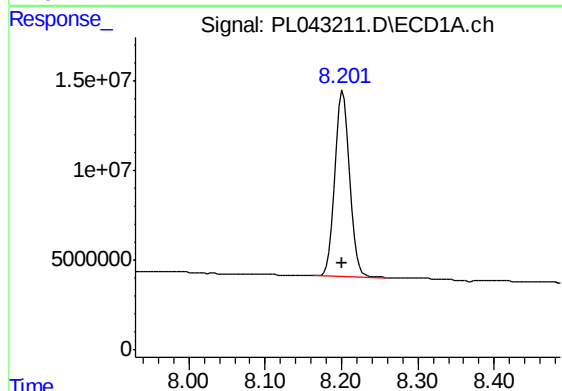

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 138388444
Conc: 21.19 ng/ml

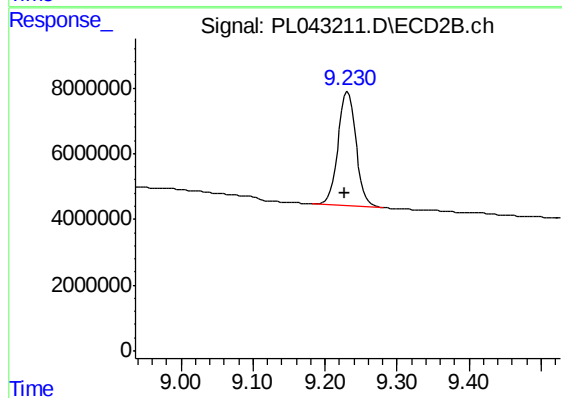

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.005 min
Response: 59877226
Conc: 22.95 ng/ml