

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
 Data File : PL055029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 13:30
 Operator : SG\AJ
 Sample : K6294-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 03:39:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.050	219.0E6	56617914	18.822	22.187
28)	SA Decachlor...	8.318	9.152	181.8E6	46750553	18.989	19.500
Target Compounds							
9)	A Endosulfan I	5.624	0.000	29551380	0	2.167	N.D. #
15)	B Endosulfa...	0.000	6.983	0	1637129	N.D.	0.696 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
Data File : PL055029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 13:30
Operator : SG\AJ
Sample : K6294-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 03:39:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

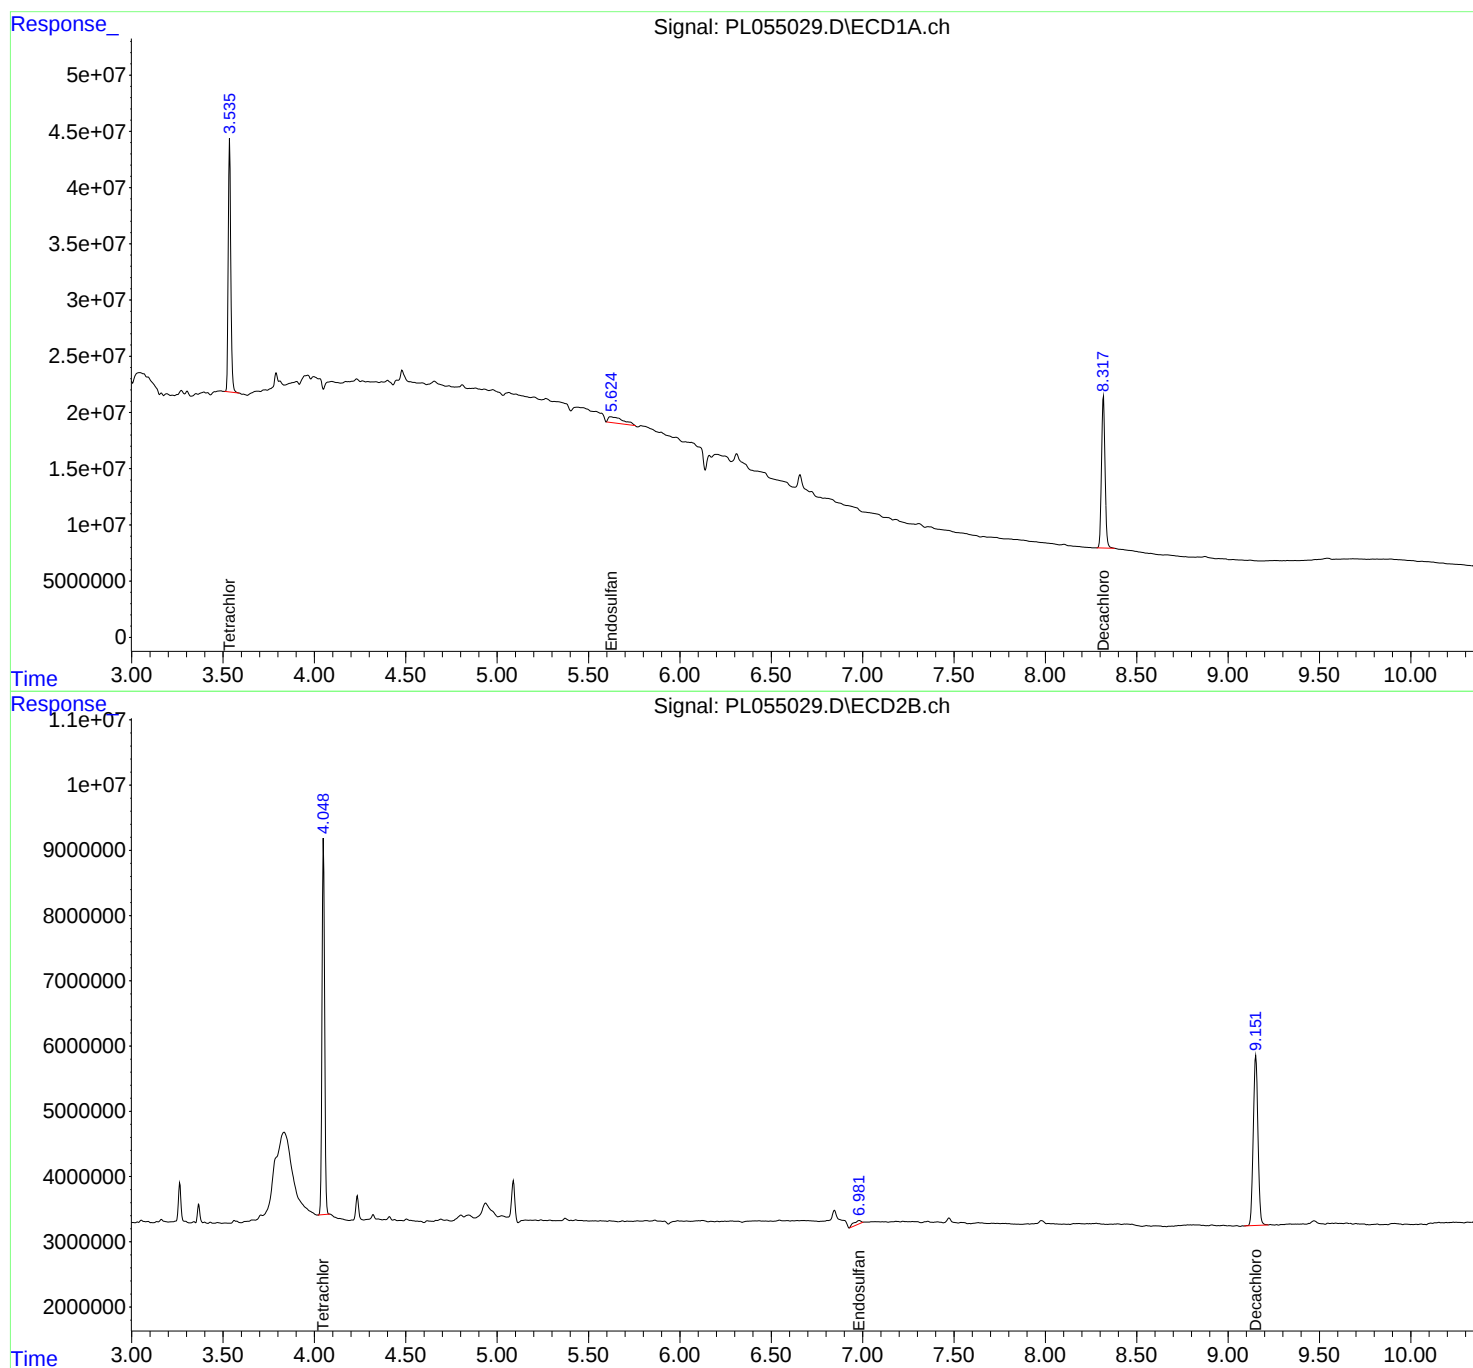


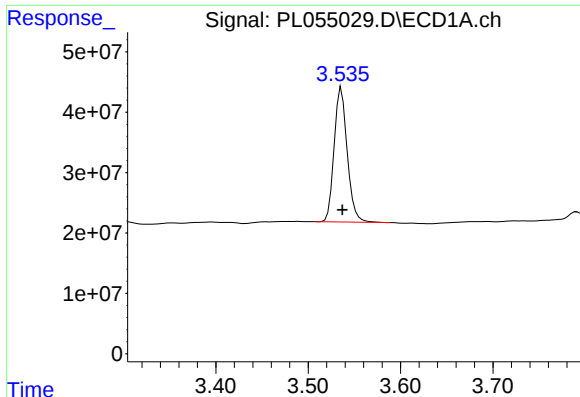

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: -0.001 min
Response: 218974580
Conc: 18.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

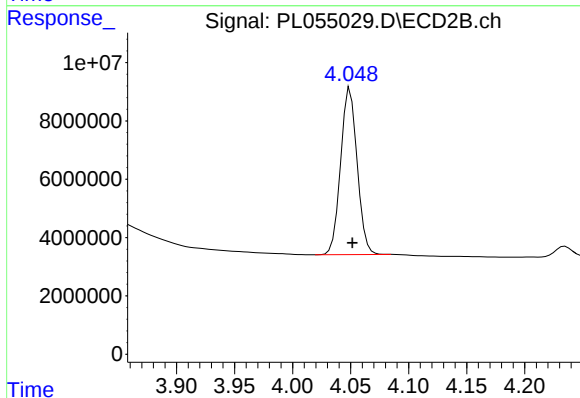


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 56617914
Conc: 22.19 ng/ml

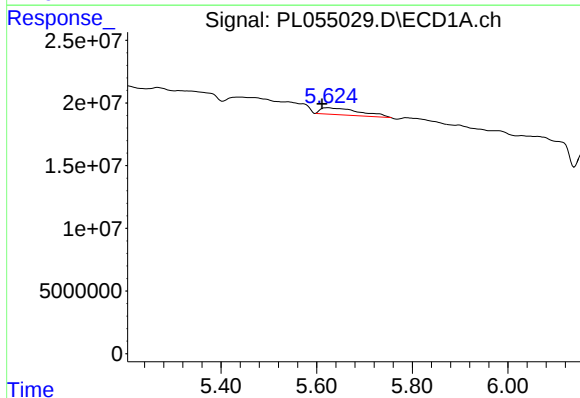


#9 Endosulfan I

R.T.: 5.624 min
Delta R.T.: 0.013 min
Response: 29551380
Conc: 2.17 ng/ml

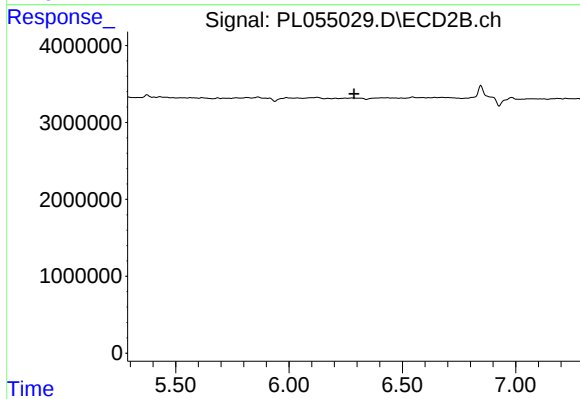

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.288 min
Response: 0
Conc: N.D.

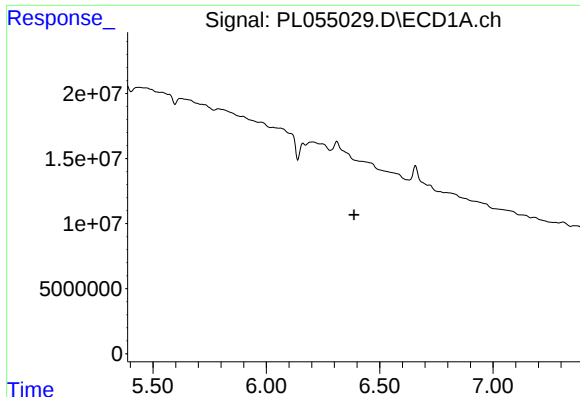

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.388 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

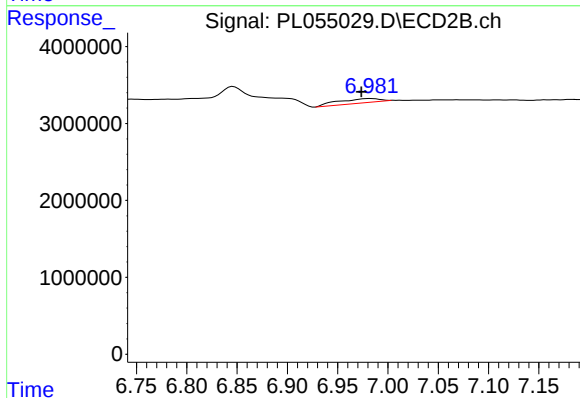


#15 Endosulfan II

R.T.: 6.983 min
Delta R.T.: 0.009 min
Response: 1637129
Conc: 0.70 ng/ml

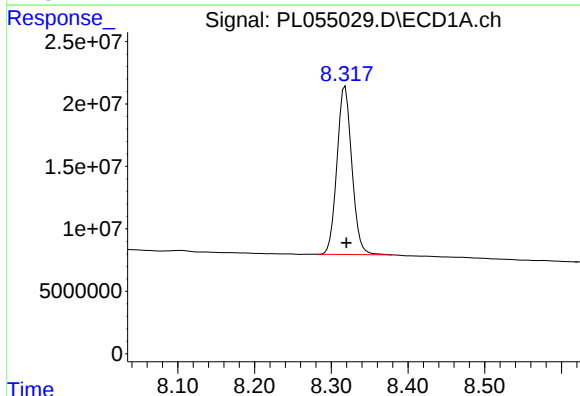

#28 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: -0.002 min
Response: 181836848
Conc: 18.99 ng/ml

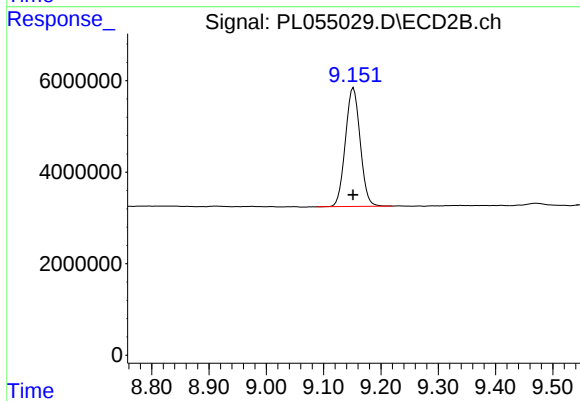

#28 Decachlorobiphenyl

R.T.: 9.152 min
Delta R.T.: 0.000 min
Response: 46750553
Conc: 19.50 ng/ml