

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
 Data File : PL055033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 14:26
 Operator : SG\AJ
 Sample : PB125519TB
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 03:40:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.050	213.0E6	54966897	18.308	21.540
28)	SA Decachlor...	8.318	9.153	181.2E6	46978487	18.927	19.595
Target Compounds							
3)	MA gamma-BHC...	4.297f	0.000	4466394	0	0.262	N.D. #
6)	B beta-BHC	4.540f	0.000	11731275	0	1.582	N.D. #
9)	A Endosulfan I	5.625	0.000	30778060	0	2.257	N.D. #
11)	B alpha-Chl...	5.544	0.000	33868519	0	2.297	N.D. #
12)	B 4,4'-DDE	5.707	0.000	7226878	0	0.543	N.D. #
19)	B Endosulfa...	6.779	0.000	12242081	0	1.143	N.D. #
23)	Chlordane-1	4.445f	0.000	4992132	0	12.650	N.D. #
26)	Chlordane-4	5.544	0.000	33868519	0	32.064	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
Data File : PL055033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 14:26
Operator : SG\AJ
Sample : PB125519TB
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 03:40:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

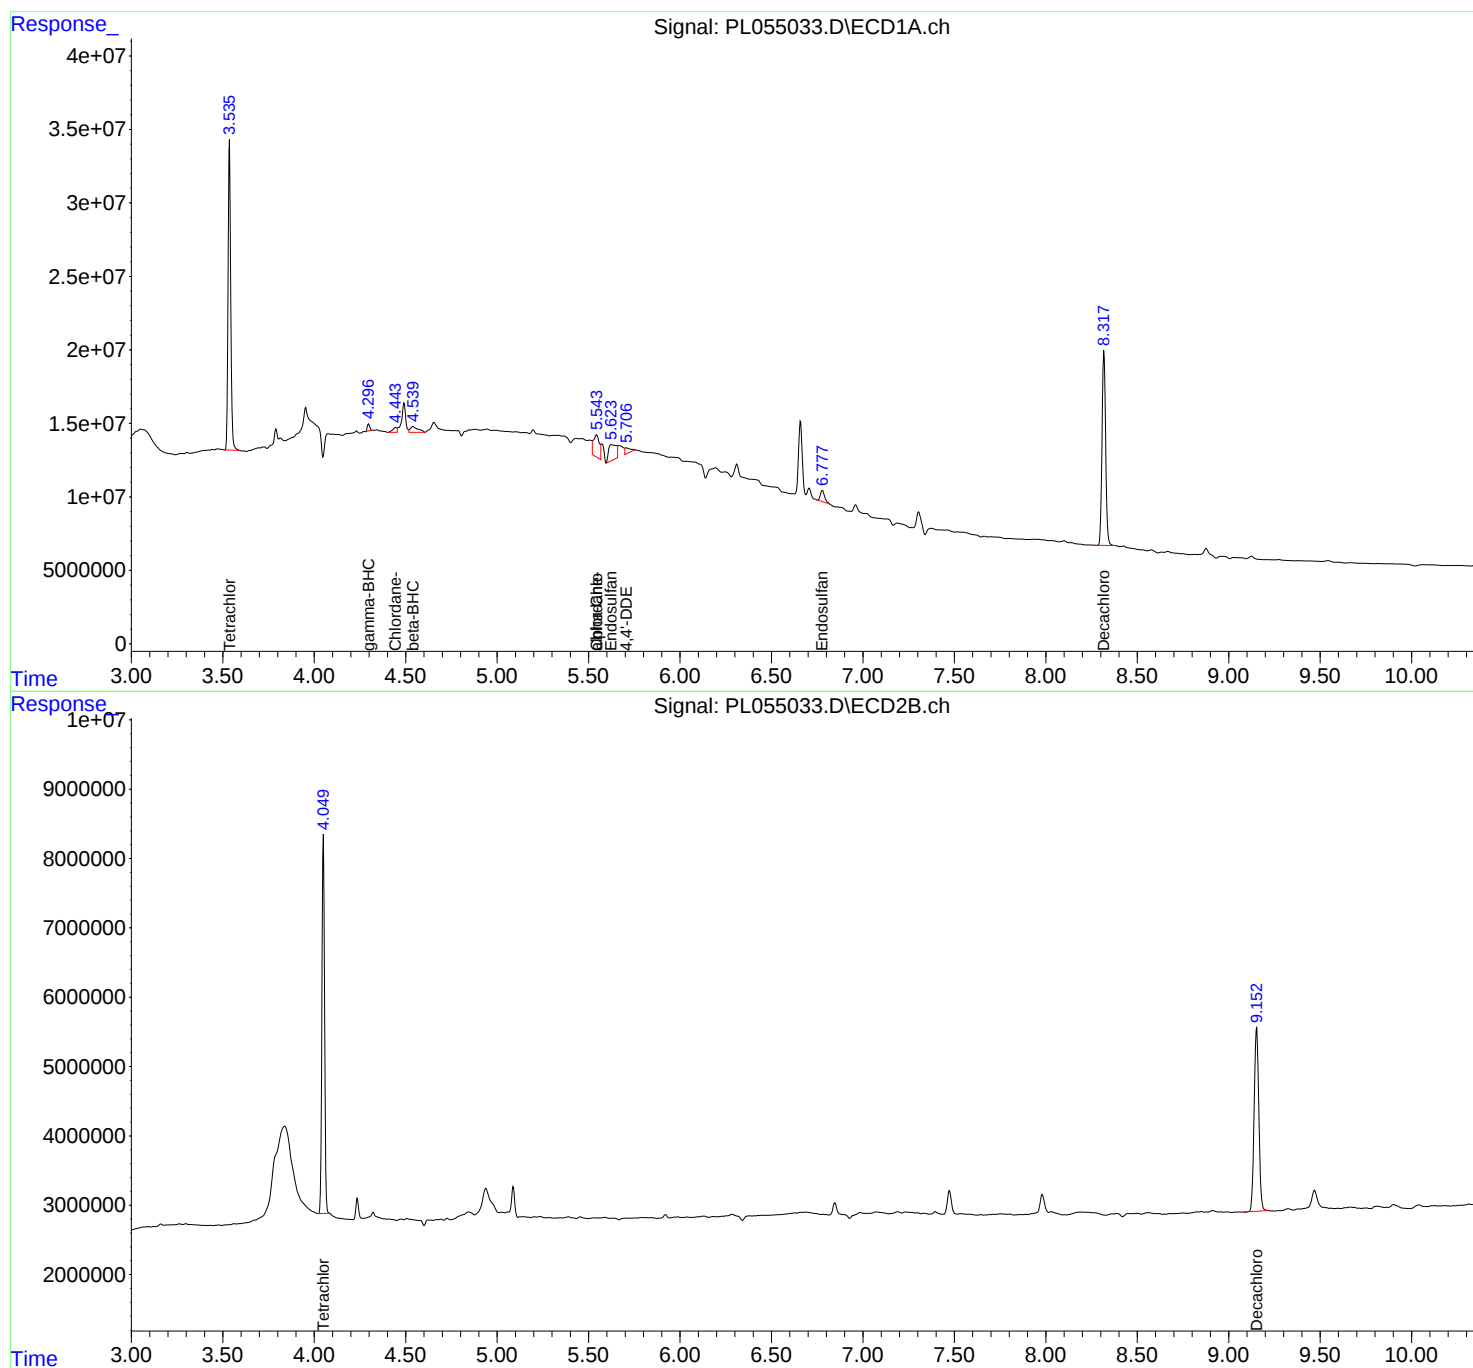


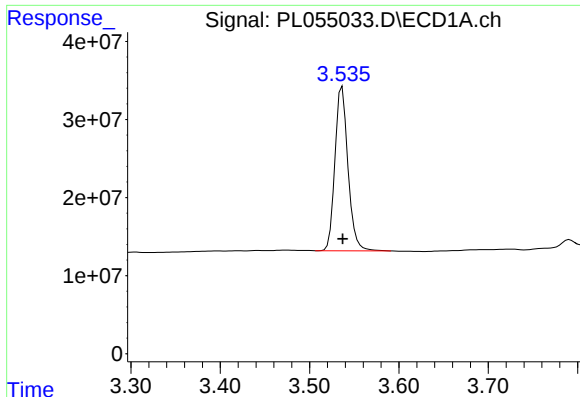

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 21300830
Conc: 18.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

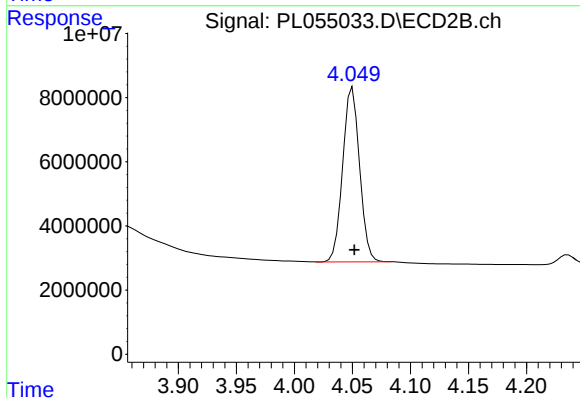


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.001 min
Response: 54966897
Conc: 21.54 ng/ml

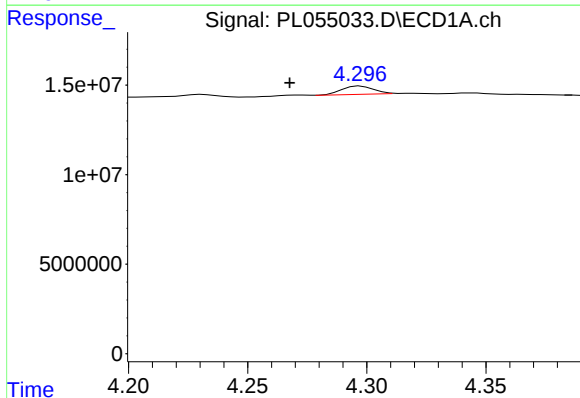


#3 gamma-BHC (Lindane)

R.T.: 4.297 min
Delta R.T.: 0.030 min
Response: 4466394
Conc: 0.26 ng/ml

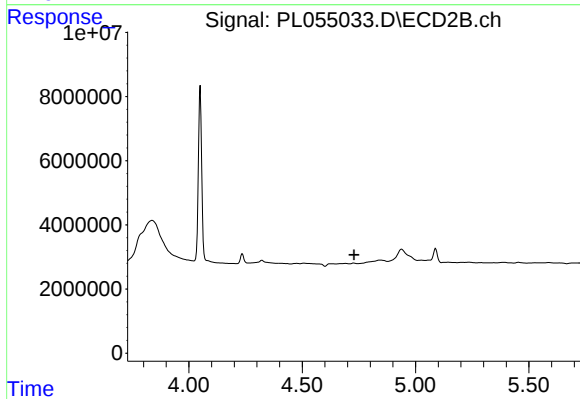

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.729 min
Response: 0
Conc: N.D.

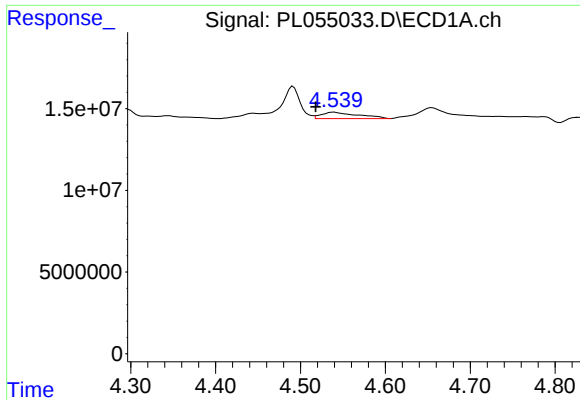

#6 beta-BHC


R.T.: 4.540 min
Delta R.T.: 0.022 min
Response: 11731275
Conc: 1.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

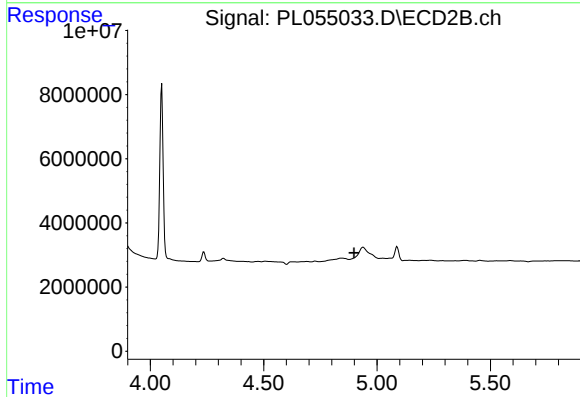


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.899 min
Response: 0
Conc: N.D.

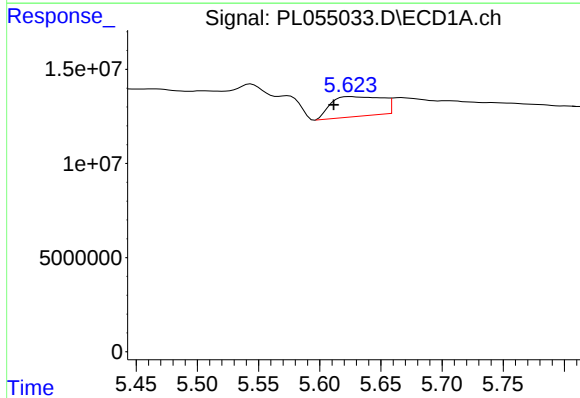


#9 Endosulfan I

R.T.: 5.625 min
Delta R.T.: 0.013 min
Response: 30778060
Conc: 2.26 ng/ml

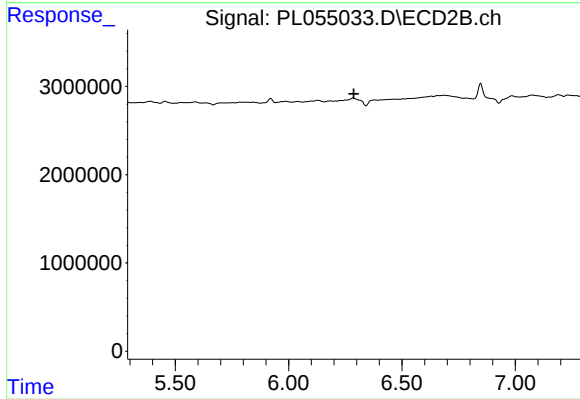

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

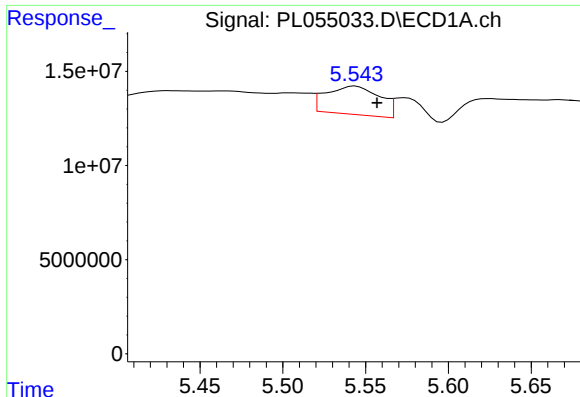

#11 alpha-Chlordane


R.T.: 5.544 min
Delta R.T.: -0.013 min
Response: 33868519
Conc: 2.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

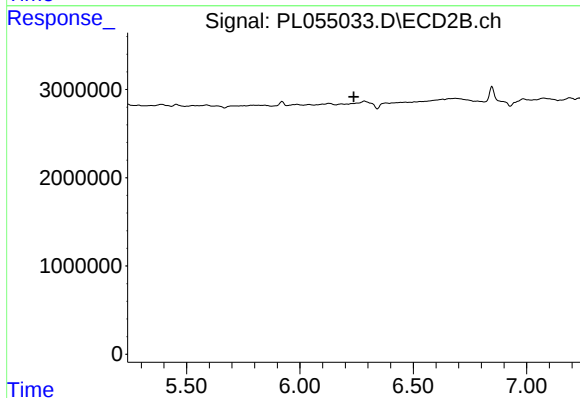


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

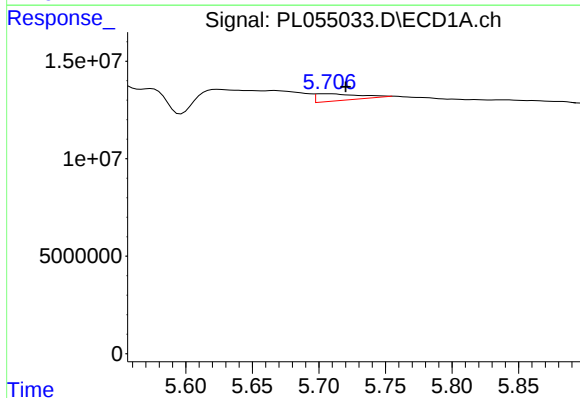


#12 4,4'-DDE

R.T.: 5.707 min
Delta R.T.: -0.013 min
Response: 7226878
Conc: 0.54 ng/ml

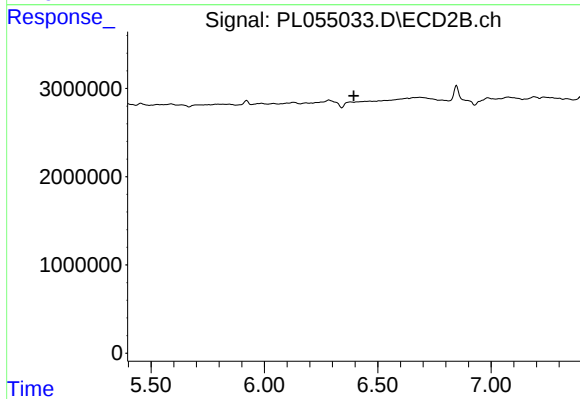

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

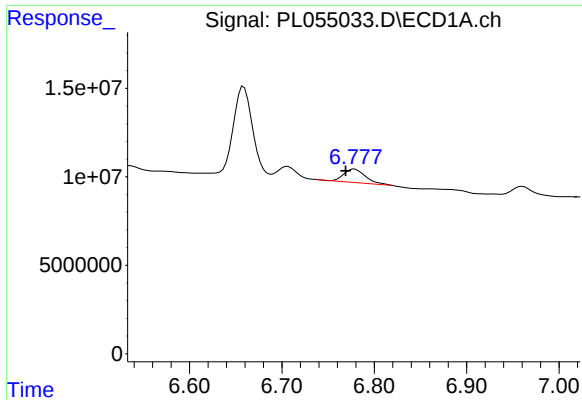

#19 Endosulfan Sulfate


R.T.: 6.779 min
Delta R.T.: 0.009 min
Response: 12242081
Conc: 1.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

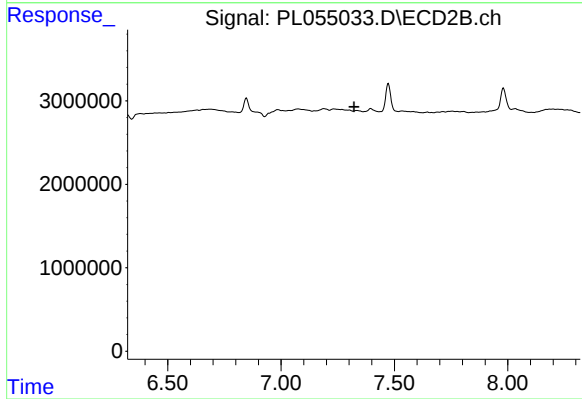


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.322 min
Response: 0
Conc: N.D.

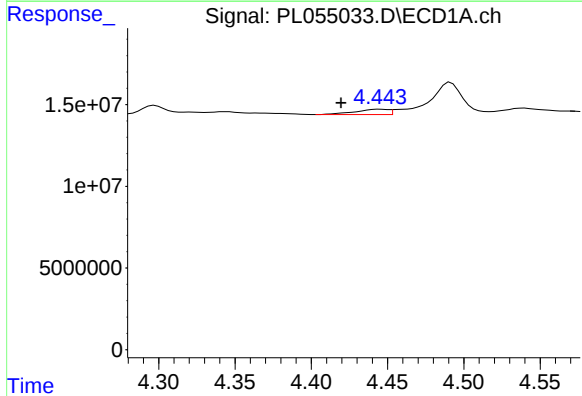


#23 Chlordane-1

R.T.: 4.445 min
Delta R.T.: 0.025 min
Response: 4992132
Conc: 12.65 ng/ml

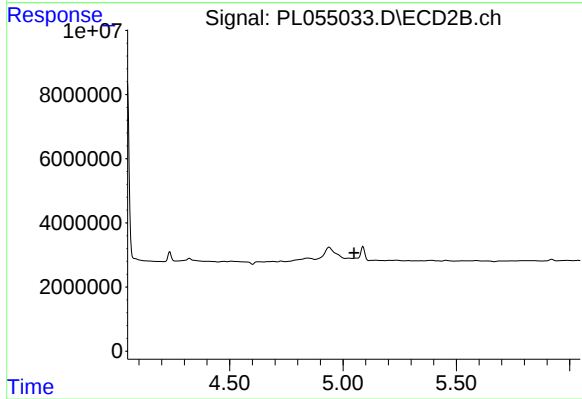

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

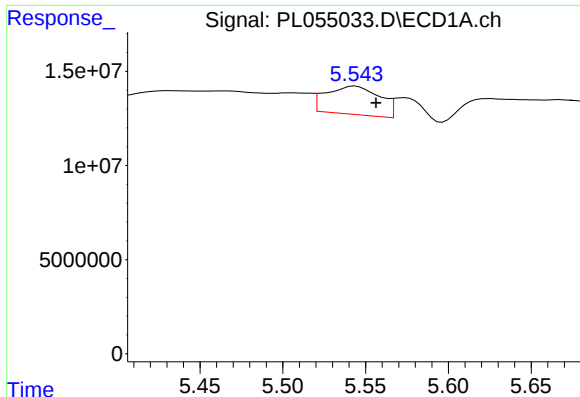

#26 Chlordane-4


R.T.: 5.544 min
Delta R.T.: -0.012 min
Response: 33868519
Conc: 32.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

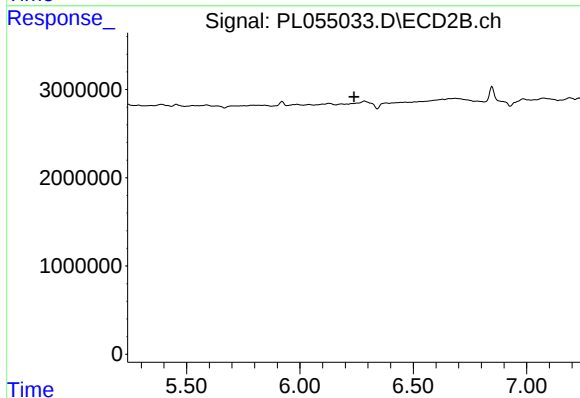


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

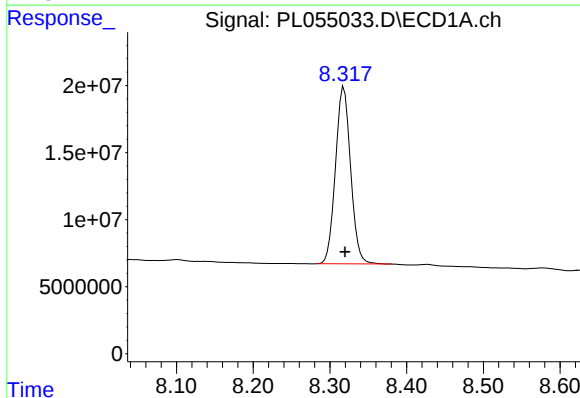

#28 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: -0.001 min
Response: 181244480
Conc: 18.93 ng/ml

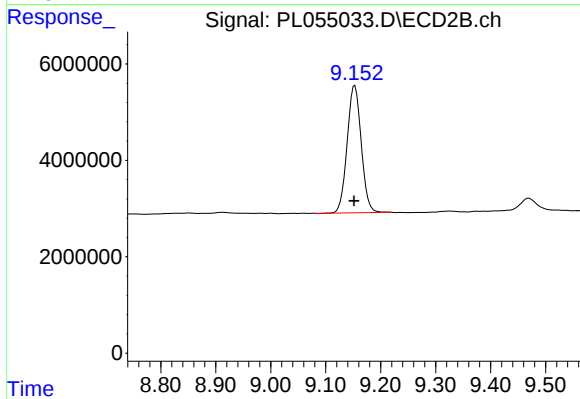

#28 Decachlorobiphenyl

R.T.: 9.153 min
Delta R.T.: 0.001 min
Response: 46978487
Conc: 19.60 ng/ml