

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
 Data File : PL055035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 14:56
 Operator : SG\AJ
 Sample : PB125528BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 03:40:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.050	218.8E6	58169836	18.806	22.796
28)	SA Decachlor...	8.319	9.153	190.0E6	49233378	19.840	20.536
Target Compounds							
2)	A alpha-BHC	3.974	0.000	11365734	0	0.599	N.D. #
11)	B alpha-Chl...	5.547	0.000	11092970	0	0.752	N.D. #
23)	Chlordane-1	4.448f	0.000	9323917	0	23.627	N.D. #
26)	Chlordane-4	5.547	0.000	11092970	0	10.502	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
Data File : PL055035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 14:56
Operator : SG\AJ
Sample : PB125528BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 03:40:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

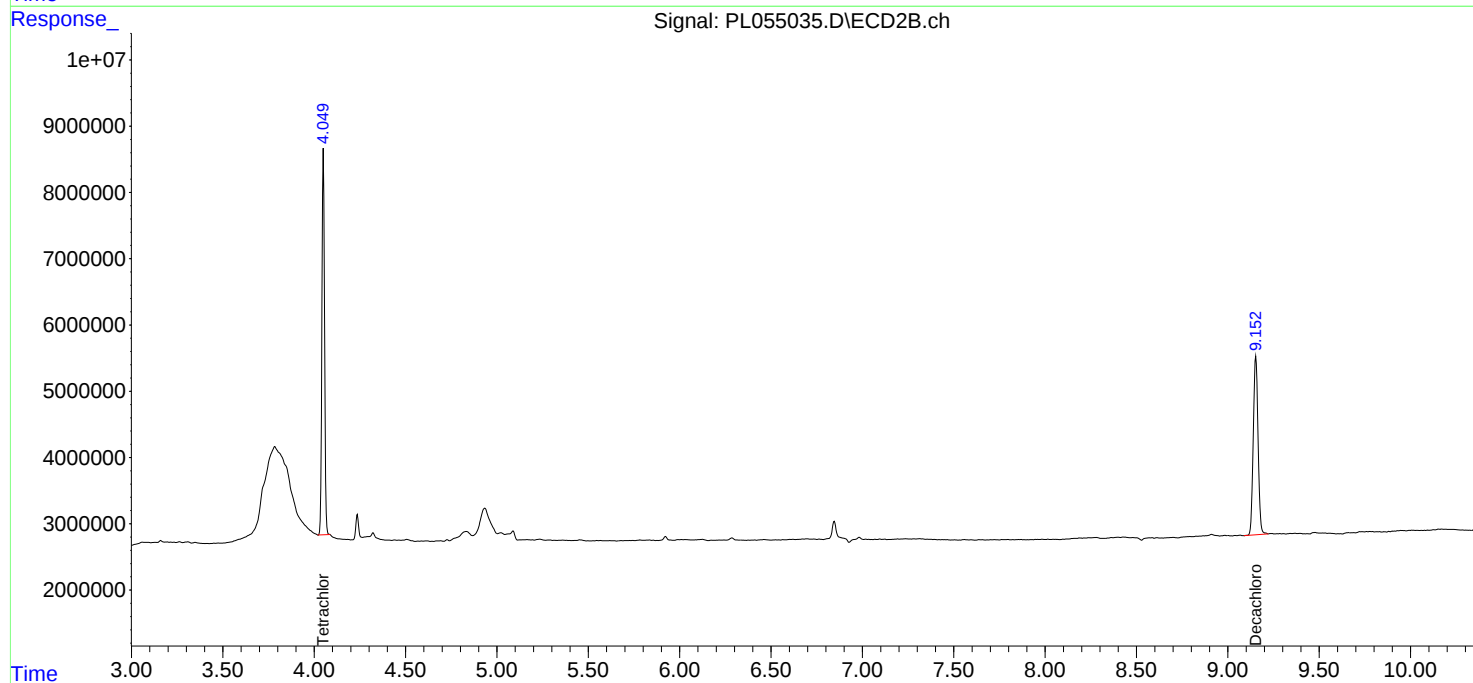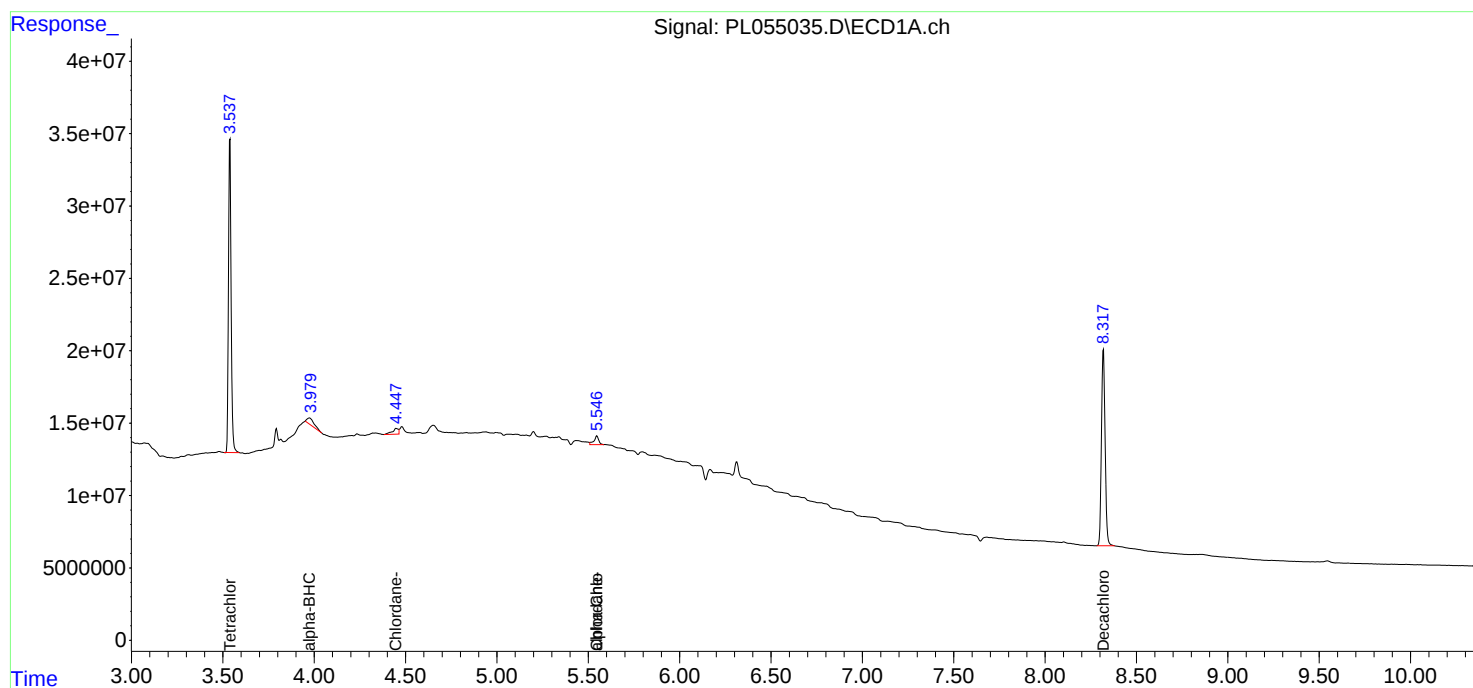


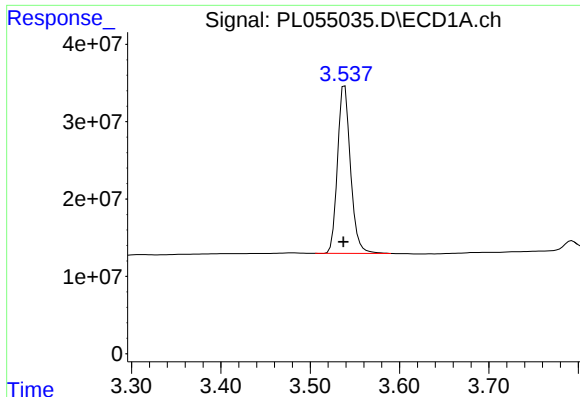

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.002 min
Response: 218796109
Conc: 18.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

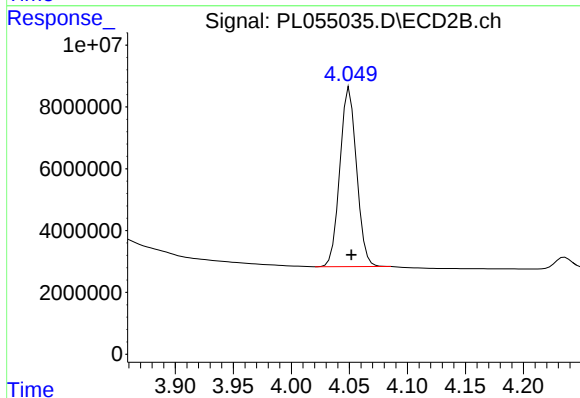


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.001 min
Response: 58169836
Conc: 22.80 ng/ml

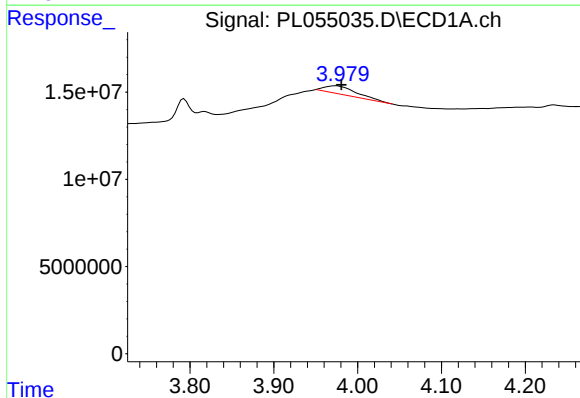


#2 alpha-BHC

R.T.: 3.974 min
Delta R.T.: -0.007 min
Response: 11365734
Conc: 0.60 ng/ml

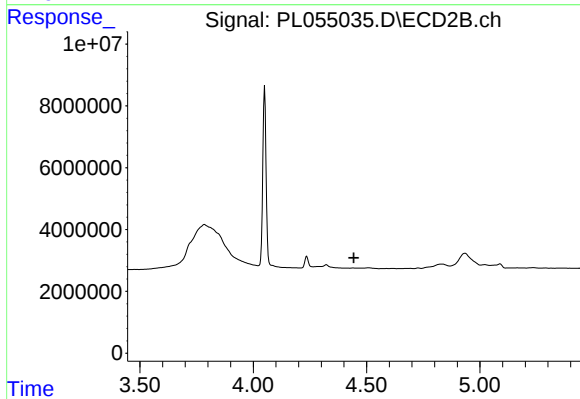

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.443 min
Response: 0
Conc: N.D.

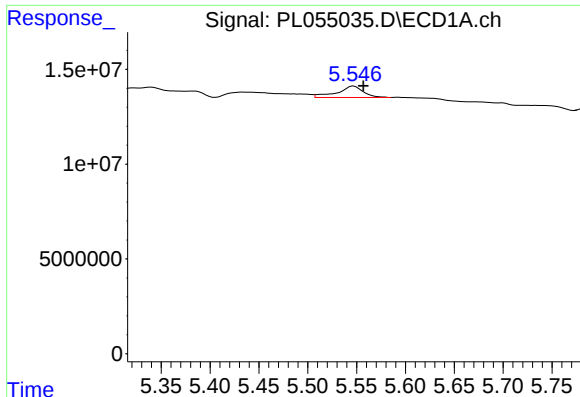

#11 alpha-Chlordane


R.T.: 5.547 min
Delta R.T.: -0.010 min
Response: 11092970
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

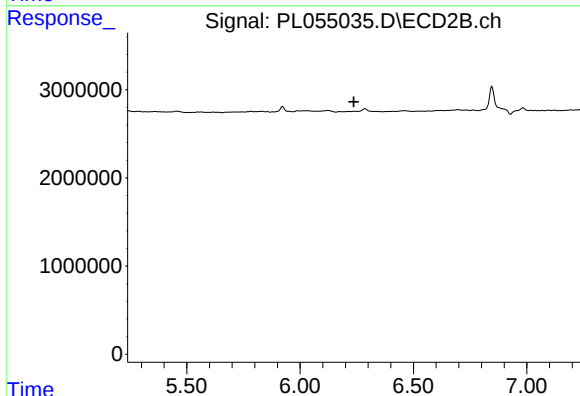


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

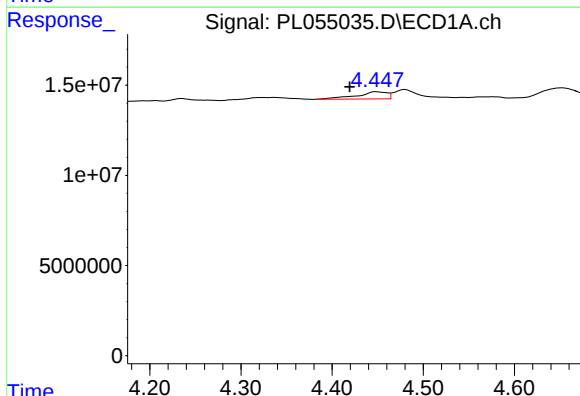


#23 Chlordane-1

R.T.: 4.448 min
Delta R.T.: 0.029 min
Response: 9323917
Conc: 23.63 ng/ml

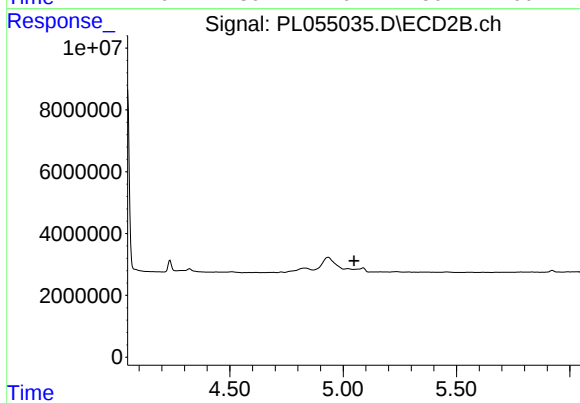

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

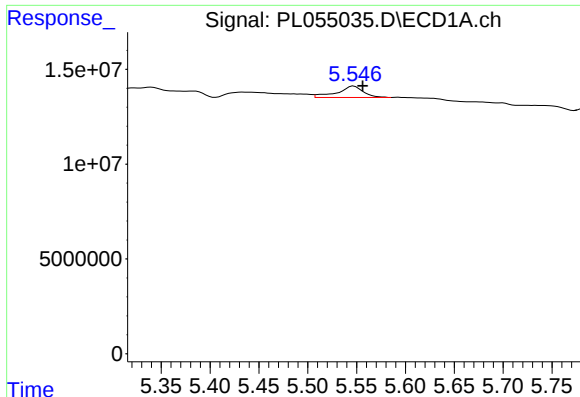

#26 Chlordane-4


R.T.: 5.547 min
Delta R.T.: -0.009 min
Response: 11092970
Conc: 10.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

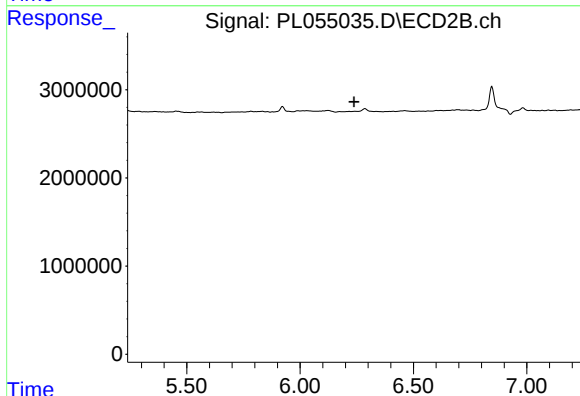


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

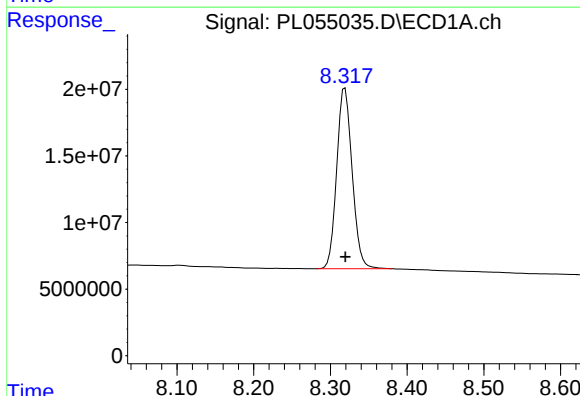

#28 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.000 min
Response: 189986340
Conc: 19.84 ng/ml

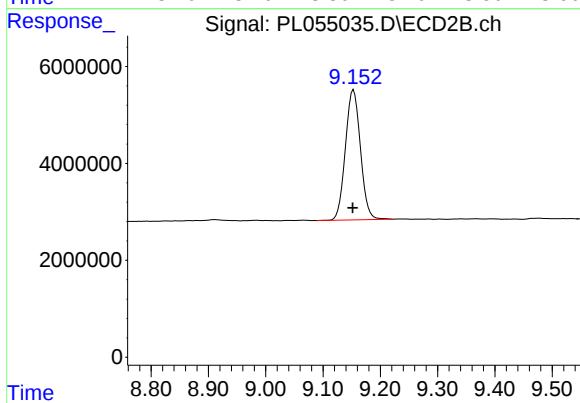

#28 Decachlorobiphenyl

R.T.: 9.153 min
Delta R.T.: 0.002 min
Response: 49233378
Conc: 20.54 ng/ml