

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
 Data File : PL055042.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 17:10
 Operator : SG\AJ
 Sample : K6318-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 03:42:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.050	136.4E6	36748385	11.725	14.401
28)	SA Decachlor...	8.318	9.151	138.3E6	34775643	14.444	14.505
Target Compounds							
4)	MA Heptachlor	4.585	0.000	9627974	0	0.546	N.D. #
7)	B delta-BHC	4.701f	0.000	7889230	0	0.485	N.D. #
11)	B alpha-Chl...	5.546	0.000	11065464	0	0.750	N.D. #
12)	B 4,4'-DDE	5.718	6.392	6320786	1530180	0.475	0.618 #
17)	MA 4,4'-DDT	6.475	0.000	3516222	0	0.336	N.D. #
20)	A Methoxychlor	7.009f	0.000	4483733	0	0.895	N.D. #
23)	Chlordane-1	4.434	0.000	9061826	0	22.962	N.D. #
26)	Chlordane-4	5.546	0.000	11065464	0	10.476	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
Data File : PL055042.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 17:10
Operator : SG\AJ
Sample : K6318-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 03:42:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

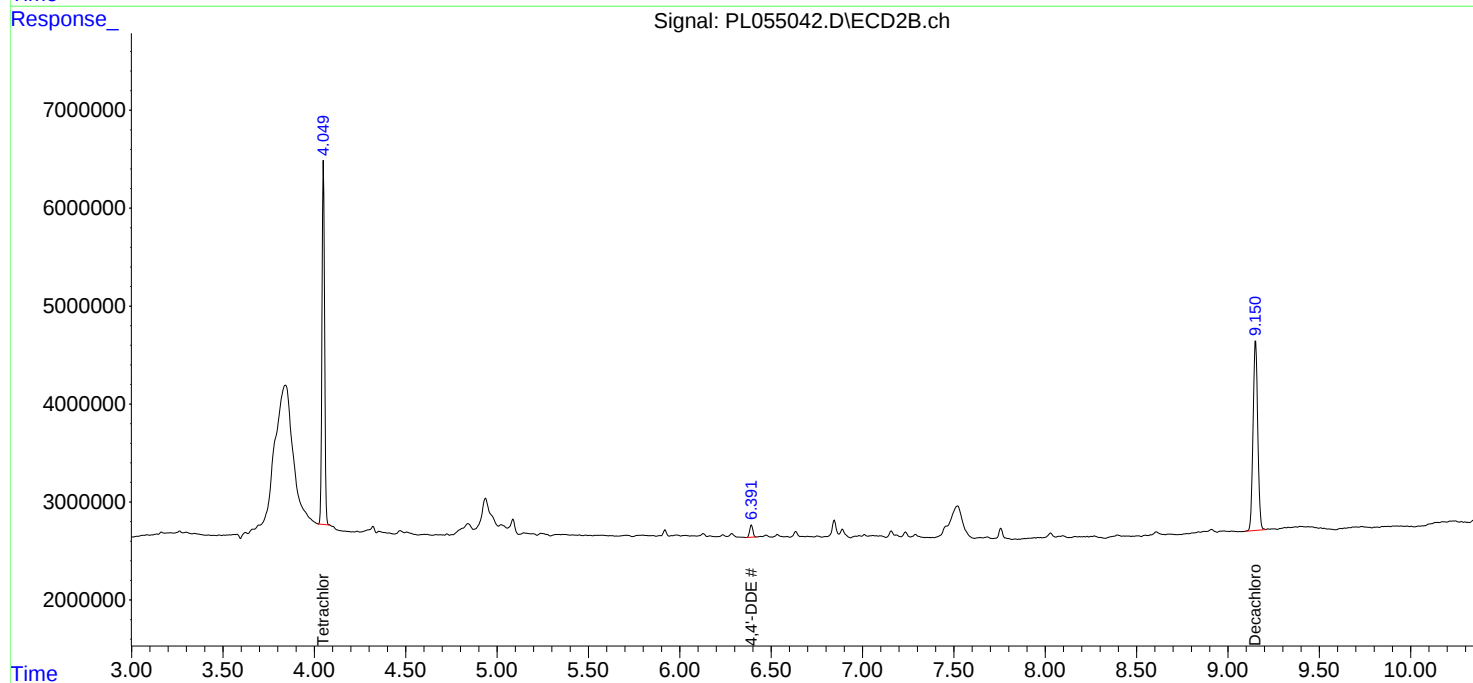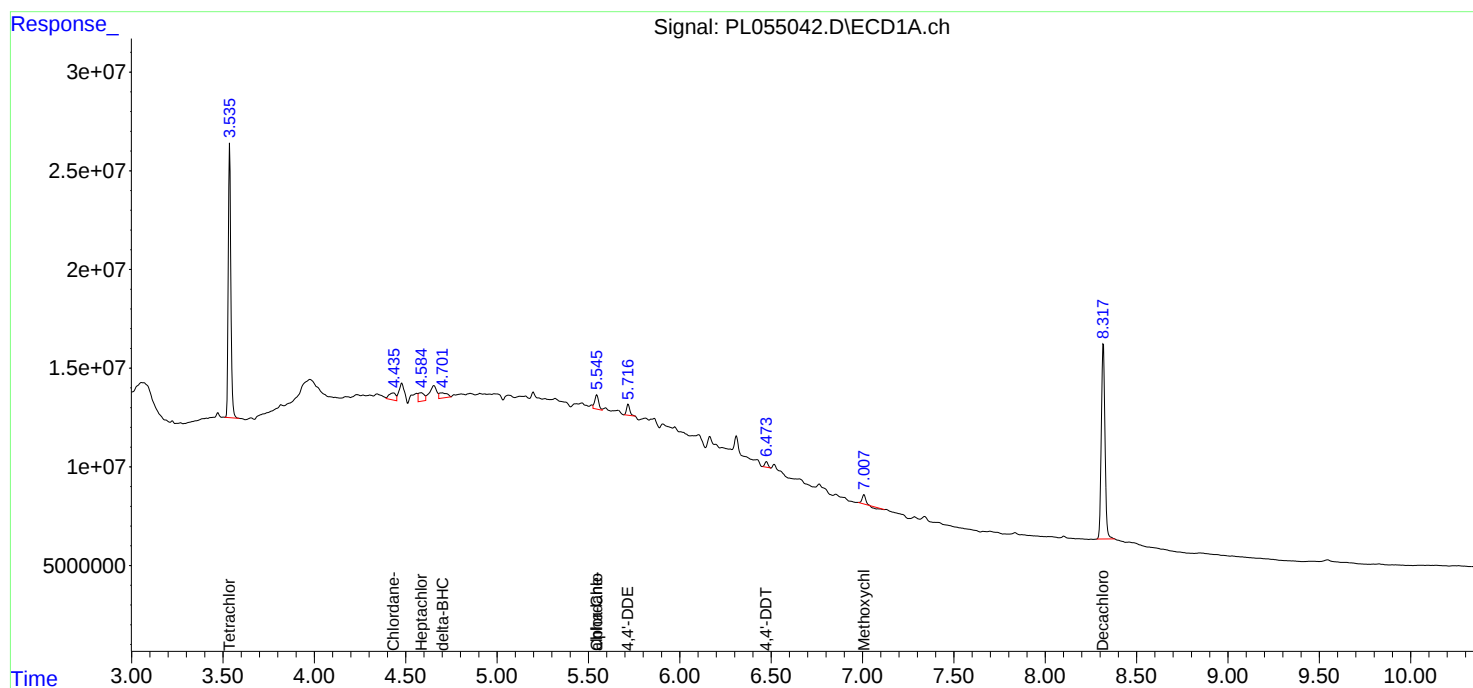


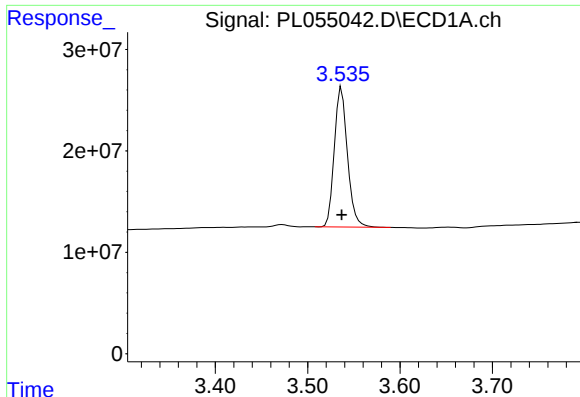

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 136415478
Conc: 11.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

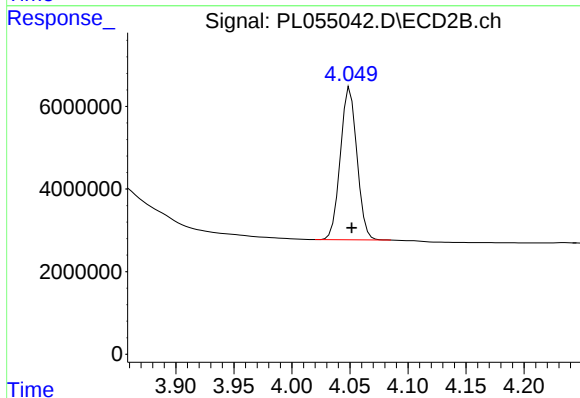


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.001 min
Response: 36748385
Conc: 14.40 ng/ml

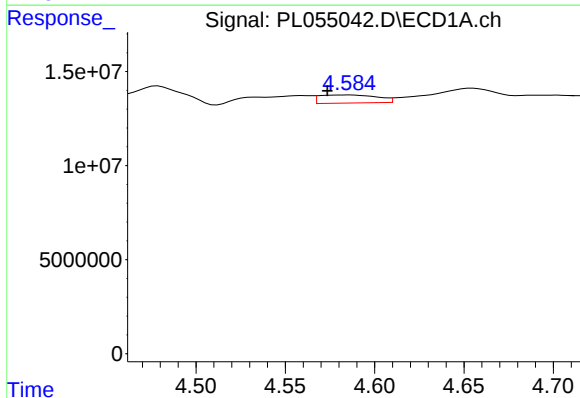


#4 Heptachlor

R.T.: 4.585 min
Delta R.T.: 0.012 min
Response: 9627974
Conc: 0.55 ng/ml

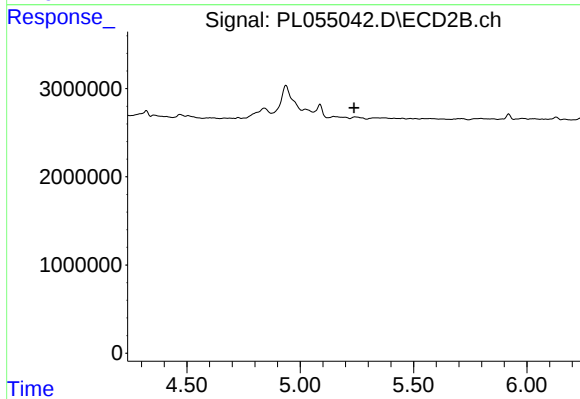

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.238 min
Response: 0
Conc: N.D.

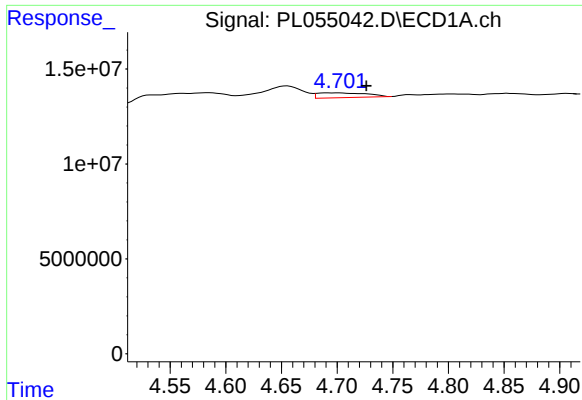

#7 delta-BHC


R.T.: 4.701 min
Delta R.T.: -0.025 min
Response: 7889230
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

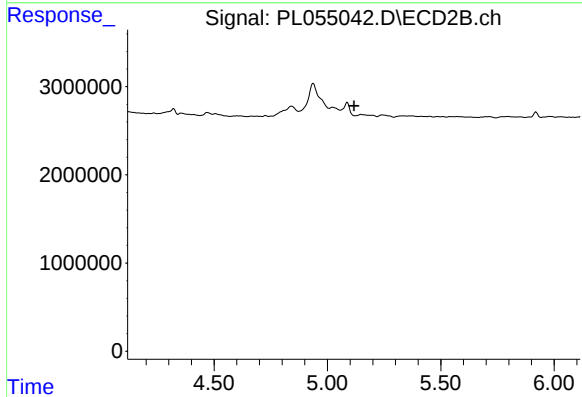


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 5.117 min
Response: 0
Conc: N.D.

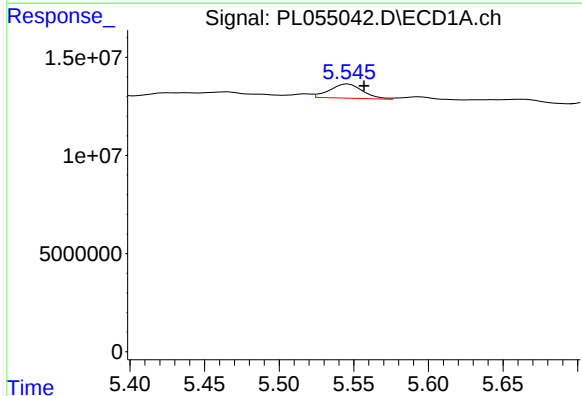


#11 alpha-Chlordane

R.T.: 5.546 min
Delta R.T.: -0.011 min
Response: 11065464
Conc: 0.75 ng/ml

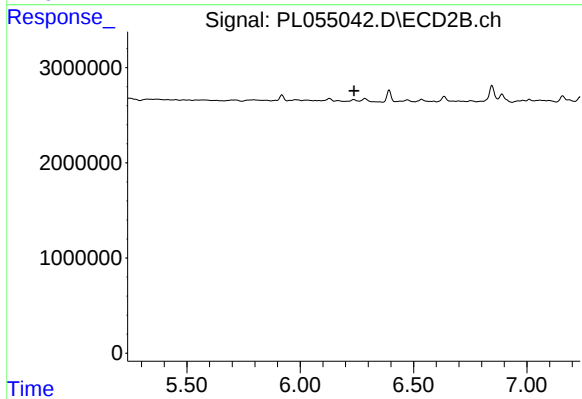

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

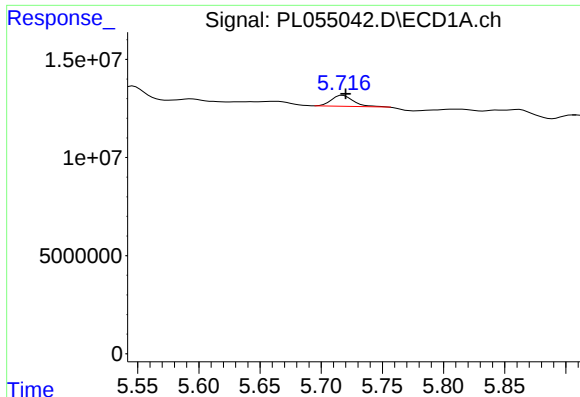

#12 4,4'-DDE


R.T.: 5.718 min
Delta R.T.: -0.002 min
Response: 6320786
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

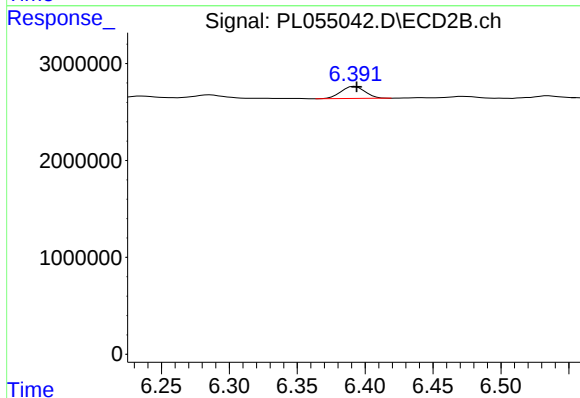


#12 4,4'-DDE

R.T.: 6.392 min
Delta R.T.: -0.001 min
Response: 1530180
Conc: 0.62 ng/ml

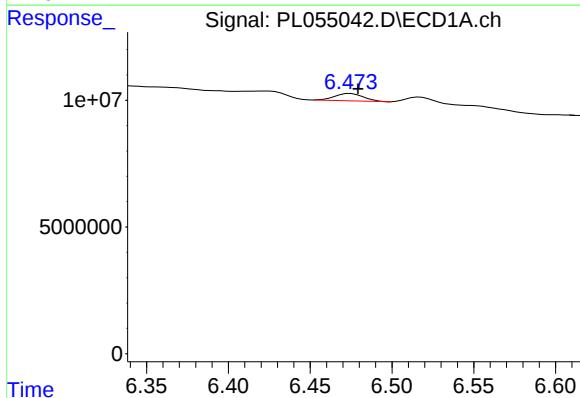


#17 4,4'-DDT

R.T.: 6.475 min
Delta R.T.: -0.005 min
Response: 3516222
Conc: 0.34 ng/ml

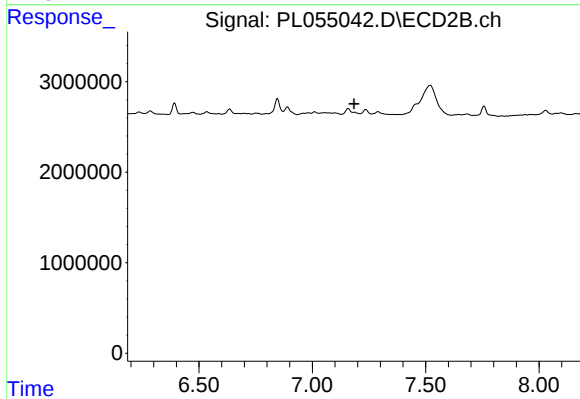

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.185 min
Response: 0
Conc: N.D.

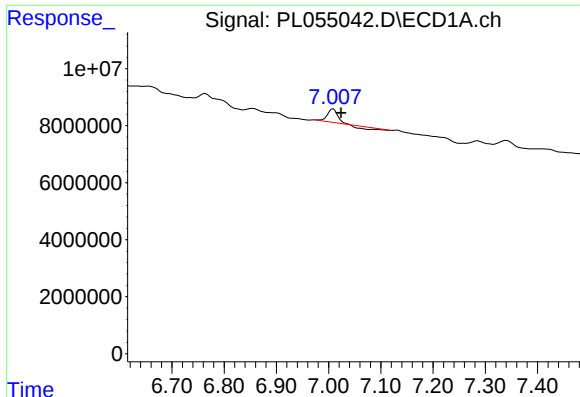

#20 Methoxychlor


R.T.: 7.009 min
Delta R.T.: -0.016 min
Response: 4483733
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

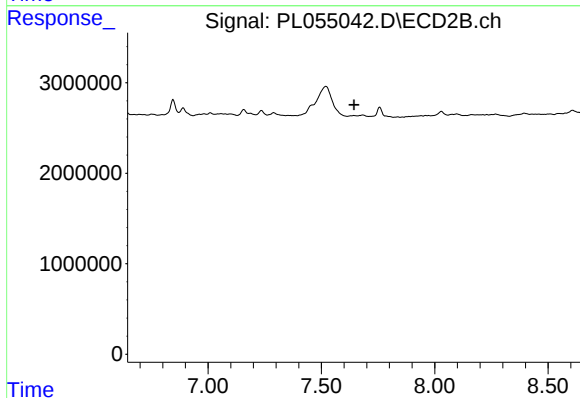


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.645 min
Response: 0
Conc: N.D.

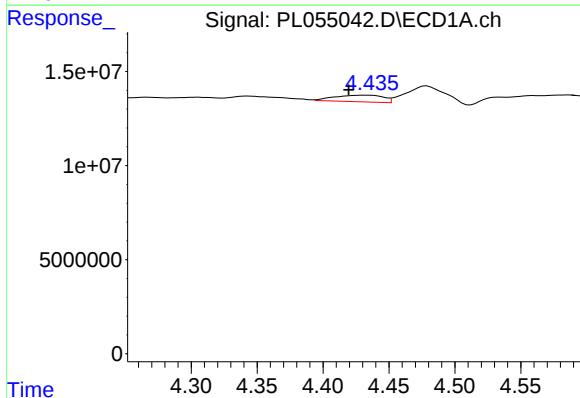


#23 Chlordane-1

R.T.: 4.434 min
Delta R.T.: 0.014 min
Response: 9061826
Conc: 22.96 ng/ml

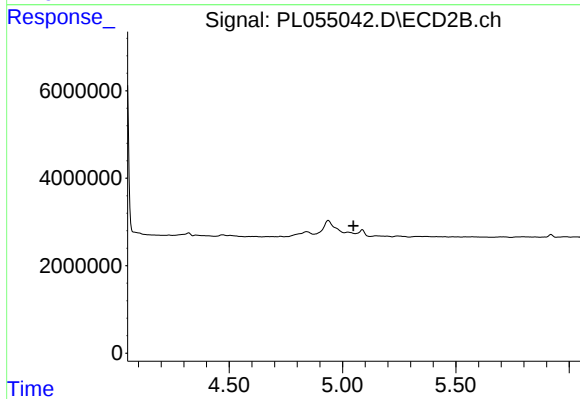

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

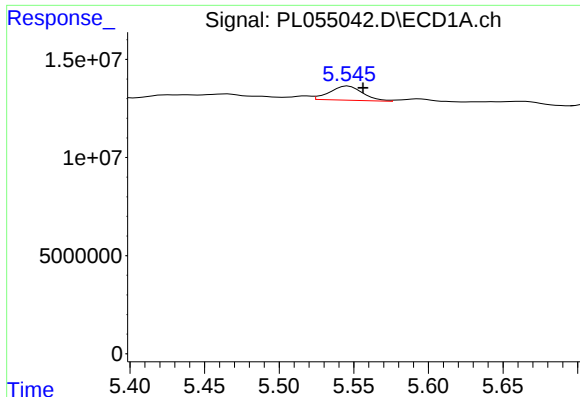

#26 Chlordane-4


R.T.: 5.546 min
Delta R.T.: -0.010 min
Response: 11065464
Conc: 10.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

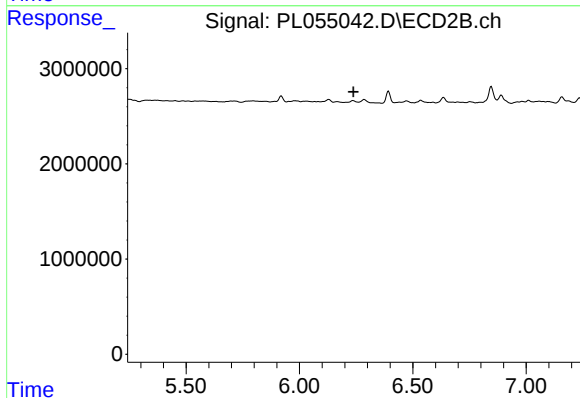


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

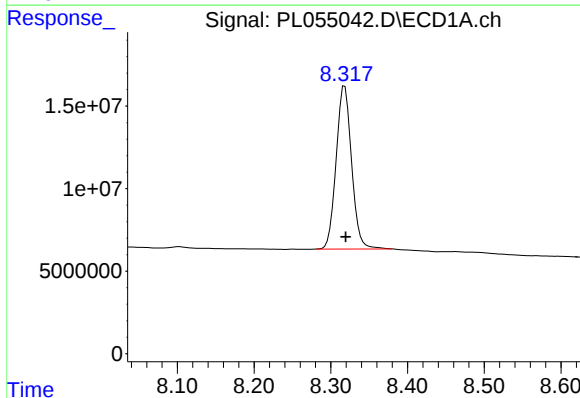

#28 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: -0.002 min
Response: 138313217
Conc: 14.44 ng/ml

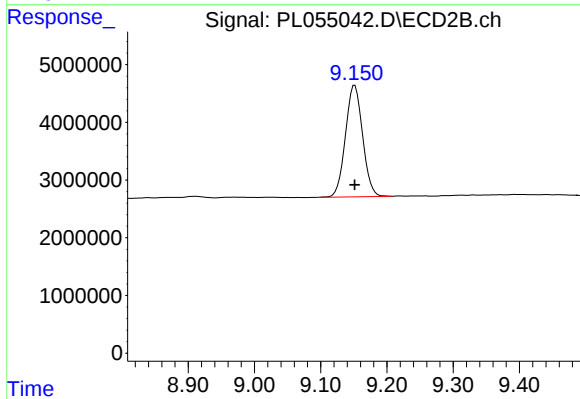

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 34775643
Conc: 14.51 ng/ml