

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
 Data File : PL055052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 19:30
 Operator : SG\AJ
 Sample : K6335-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-4BD

Manual Integrations
 APPROVED

Ankita
 12/18/2019 3:23:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 13:23:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.050	125.0E6	33922298	10.742	13.293
28)	SA Decachlor...	8.317	9.151	145.2E6	36812165	15.164	15.355
Target Compounds							
23)	Chlordane-1	4.418	5.047	127.0E6	39152414	321.722	491.164 #
24)	Chlordane-2	4.923	5.516	130.9E6	39768502	301.370m	443.726 #
25)	Chlordane-3	5.504	6.162	318.8E6	199.1E6	248.293m	641.563 #
26)	Chlordane-4	5.557	6.238	661.9E6	158.3E6	626.661	420.644 #
27)	Chlordane-5	6.397	7.046	111.3E6	29945428	295.567	444.179 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
Data File : PL055052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 19:30
Operator : SG\AJ
Sample : K6335-02
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-4BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:23:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 13:23:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

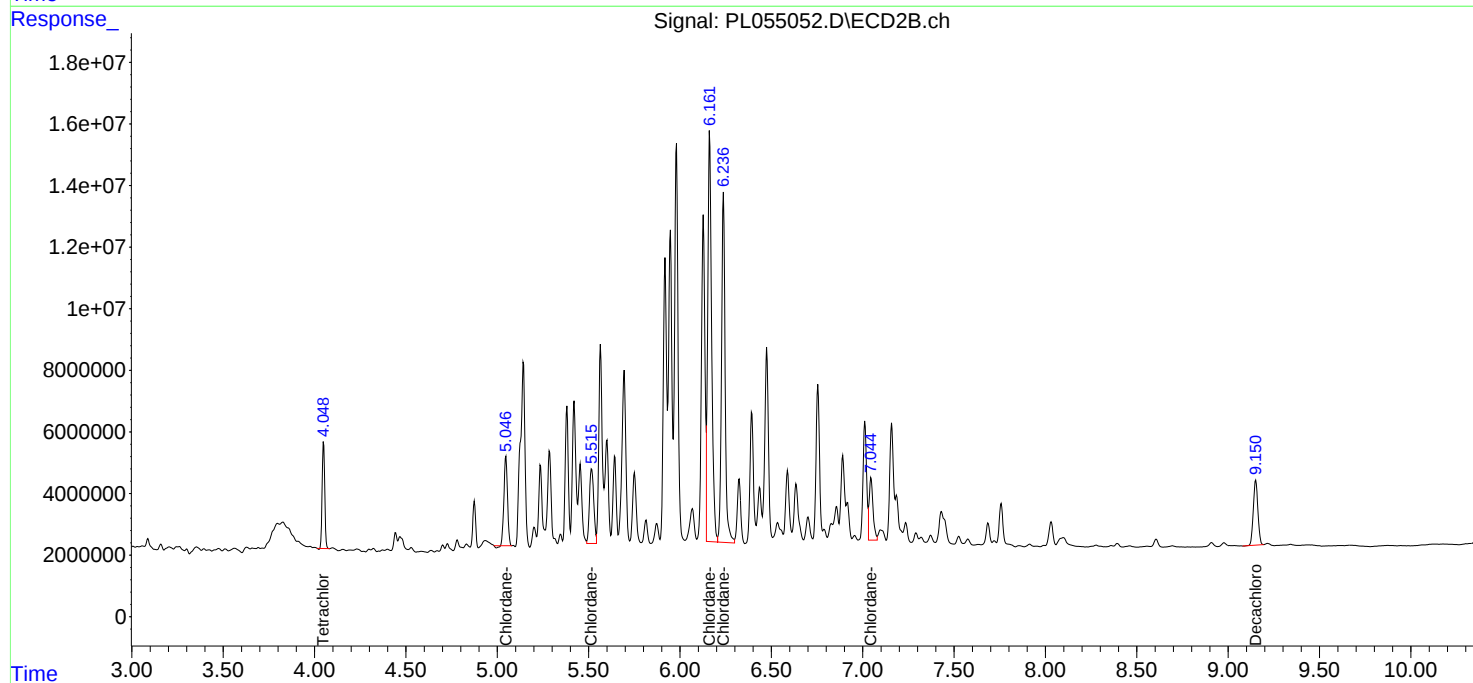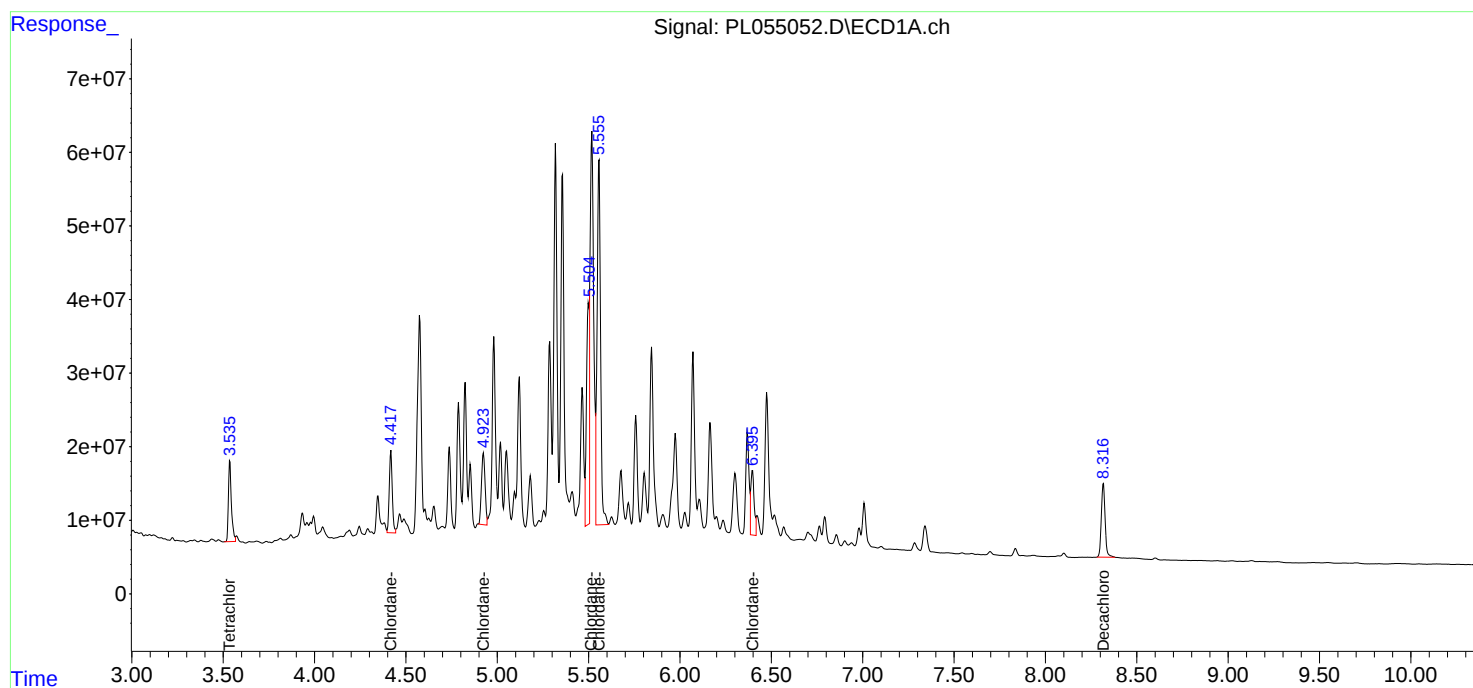

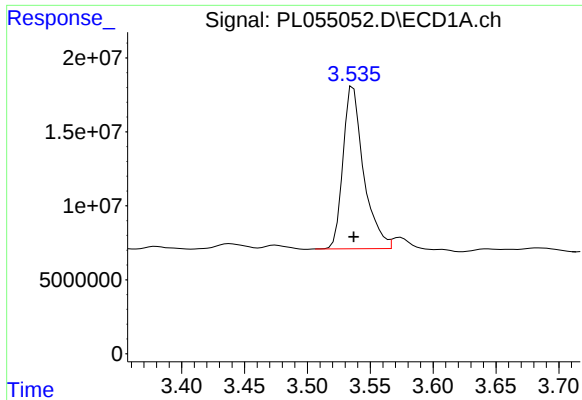


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 124976324
Conc: 10.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-4BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:23:59 PM

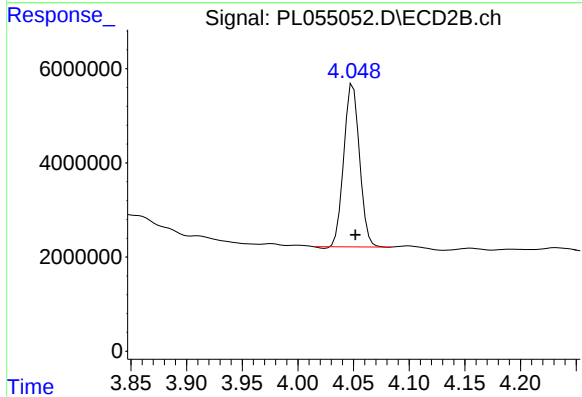


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 33922298
Conc: 13.29 ng/ml

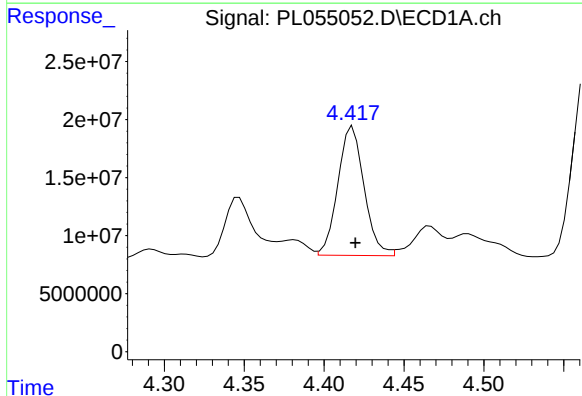


#23 Chlordane-1

R.T.: 4.418 min
Delta R.T.: -0.002 min
Response: 126963076
Conc: 321.72 ng/ml

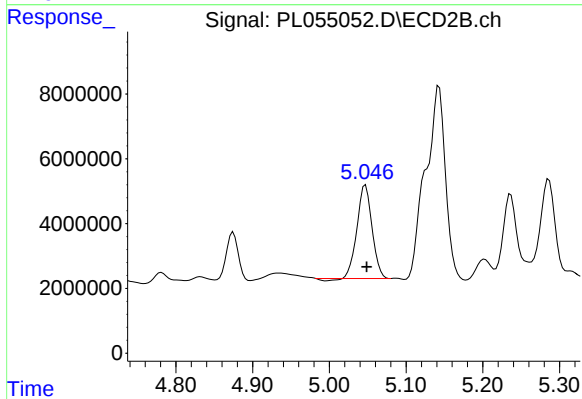

#23 Chlordane-1

R.T.: 5.047 min
Delta R.T.: -0.002 min
Response: 39152414
Conc: 491.16 ng/ml

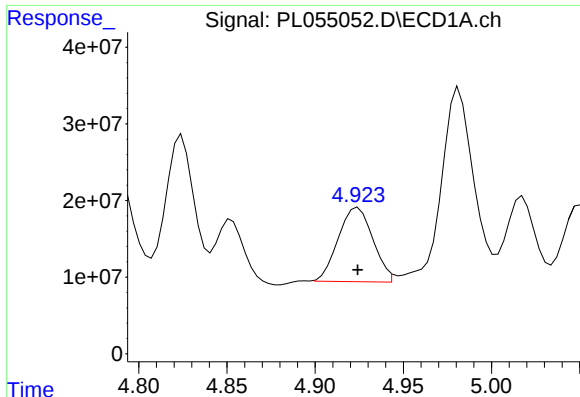


#24 Chlordane-2

R.T.: 4.923 min
Delta R.T.: -0.001 min
Response: 130871967
Conc: 301.37 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-4BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:23:59 PM

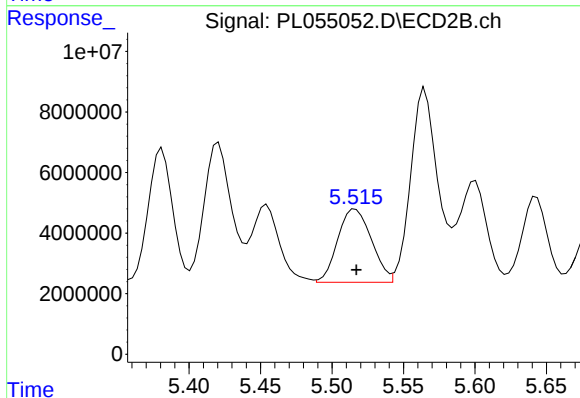


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: 0.000 min
Response: 39768502
Conc: 443.73 ng/ml

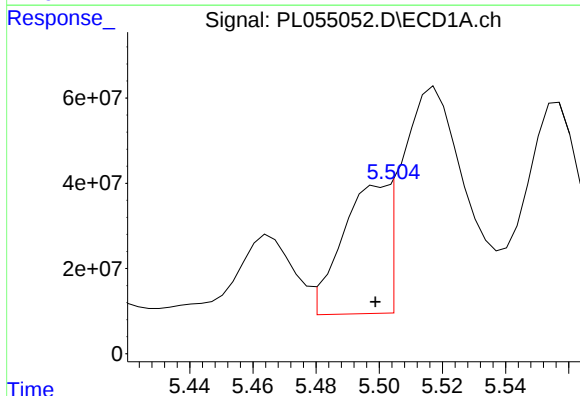


#25 Chlordane-3

R.T.: 5.504 min
Delta R.T.: 0.005 min
Response: 318840540
Conc: 248.29 ng/ml m

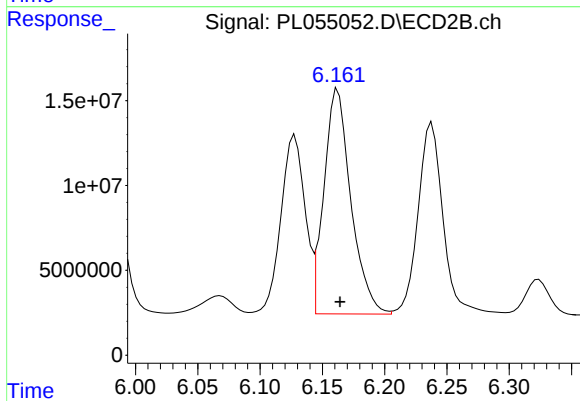

#25 Chlordane-3

R.T.: 6.162 min
Delta R.T.: -0.002 min
Response: 199141636
Conc: 641.56 ng/ml

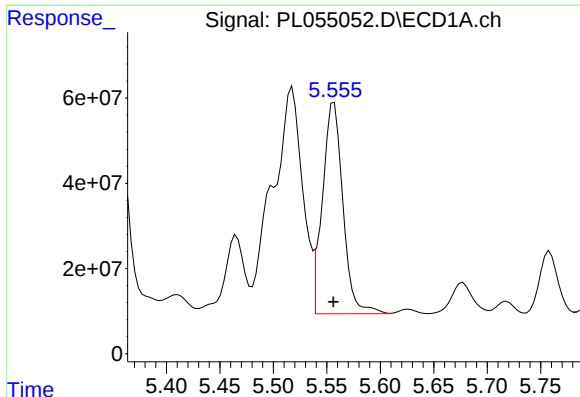


#26 Chlordane-4

R.T.: 5.557 min
Delta R.T.: 0.000 min
Response: 661935022
Conc: 626.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-4BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:23:59 PM

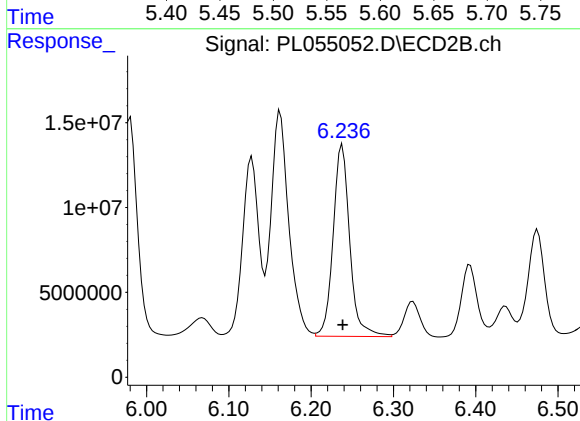


#26 Chlordane-4

R.T.: 6.238 min
Delta R.T.: 0.000 min
Response: 158283765
Conc: 420.64 ng/ml

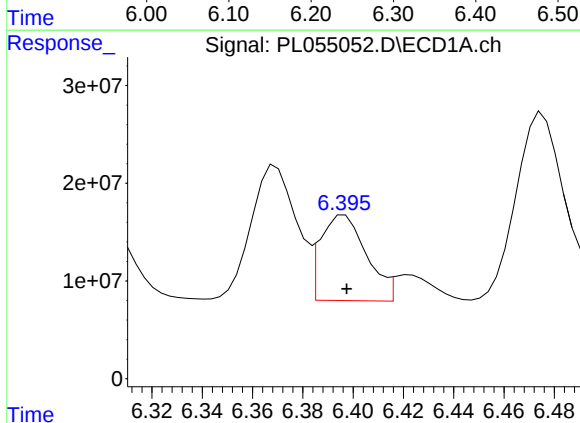


#27 Chlordane-5

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 111281439
Conc: 295.57 ng/ml

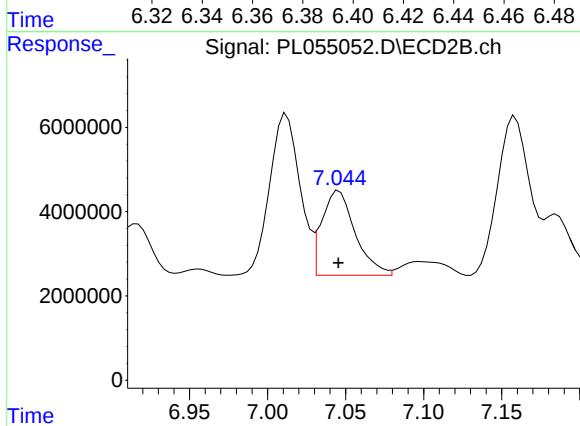

#27 Chlordane-5

R.T.: 7.046 min
Delta R.T.: 0.000 min
Response: 29945428
Conc: 444.18 ng/ml

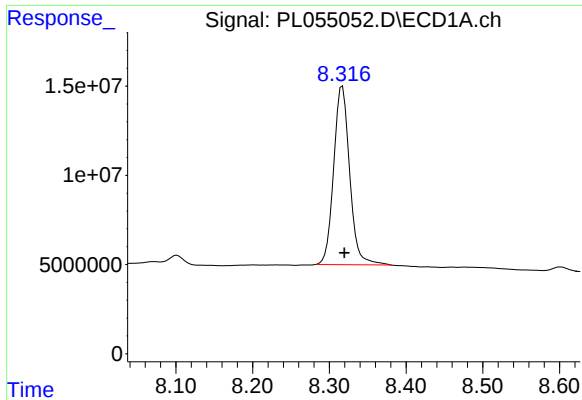


#28 Decachlorobiphenyl

R.T.: 8.317 min
Delta R.T.: -0.003 min
Response: 145212014
Conc: 15.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-4BD

Manual Integrations
APPROVED

Ankita
12/18/2019 3:23:59 PM

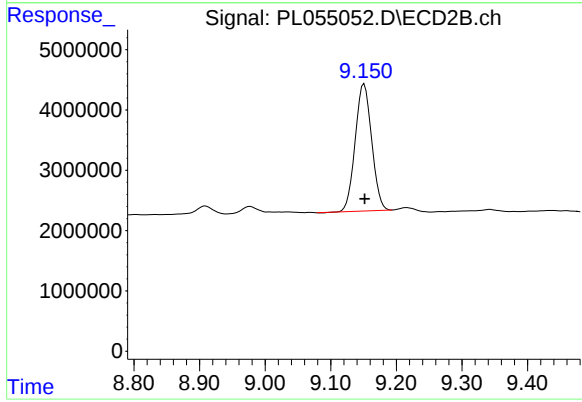

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 36812165
Conc: 15.35 ng/ml