

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
 Data File : PL055053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 19:44
 Operator : SG\AJ
 Sample : K6335-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-6BD

Manual Integrations
 APPROVED

Ankita
 12/18/2019 3:24:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 13:24:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.050	133.6E6	35277388	11.479	13.824
28)	SA Decachlor...	8.318	9.152	148.0E6	39067992	15.450	16.296
Target Compounds							
23)	Chlordane-1	4.418	5.047	137.1E6	40718020	347.451	510.805 #
24)	Chlordane-2	4.922	5.516	145.0E6	42522264	333.794m	474.452 #
25)	Chlordane-3	5.499	6.163	316.2E6	200.1E6	246.234	644.576 #
26)	Chlordane-4	5.557	6.238	675.9E6	172.3E6	639.880	457.986 #
27)	Chlordane-5	6.396	7.046	126.3E6	32211525	335.565	477.792 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
Data File : PL055053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 19:44
Operator : SG\AJ
Sample : K6335-03
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-6BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 13:24:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

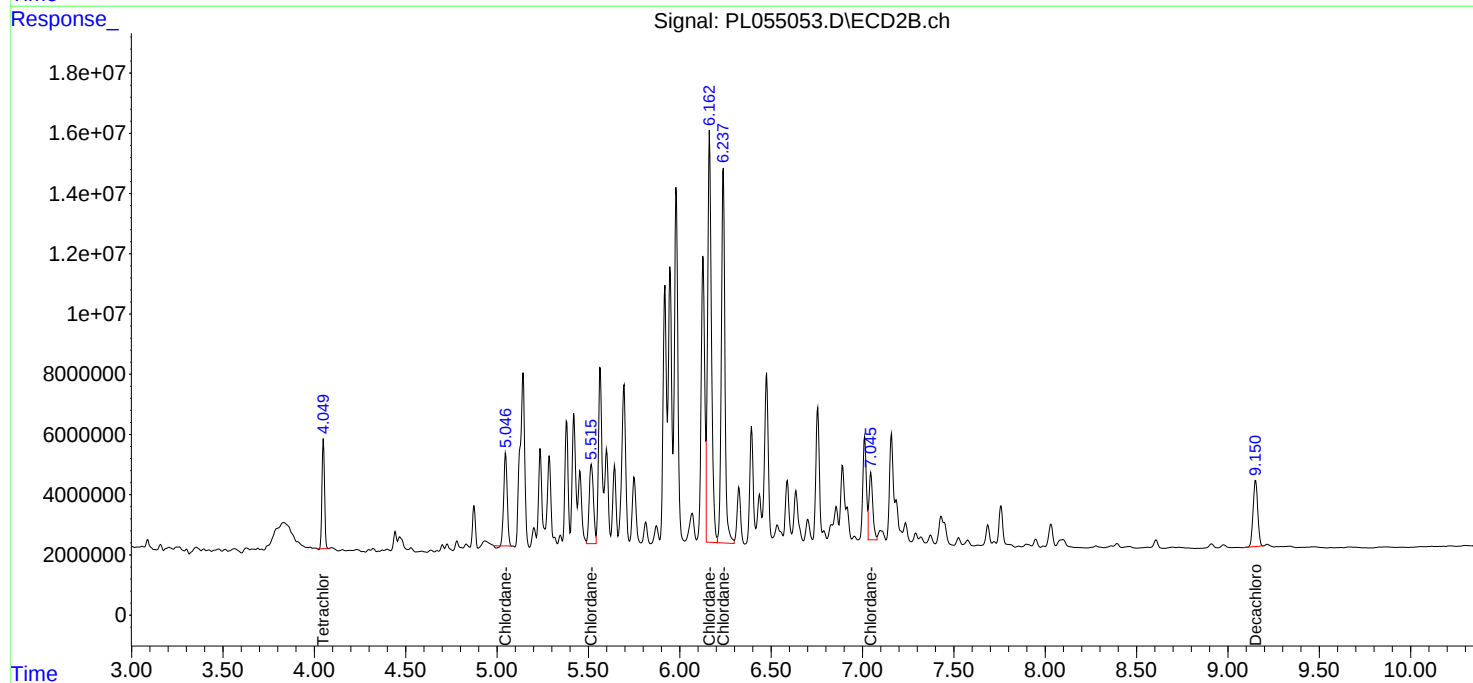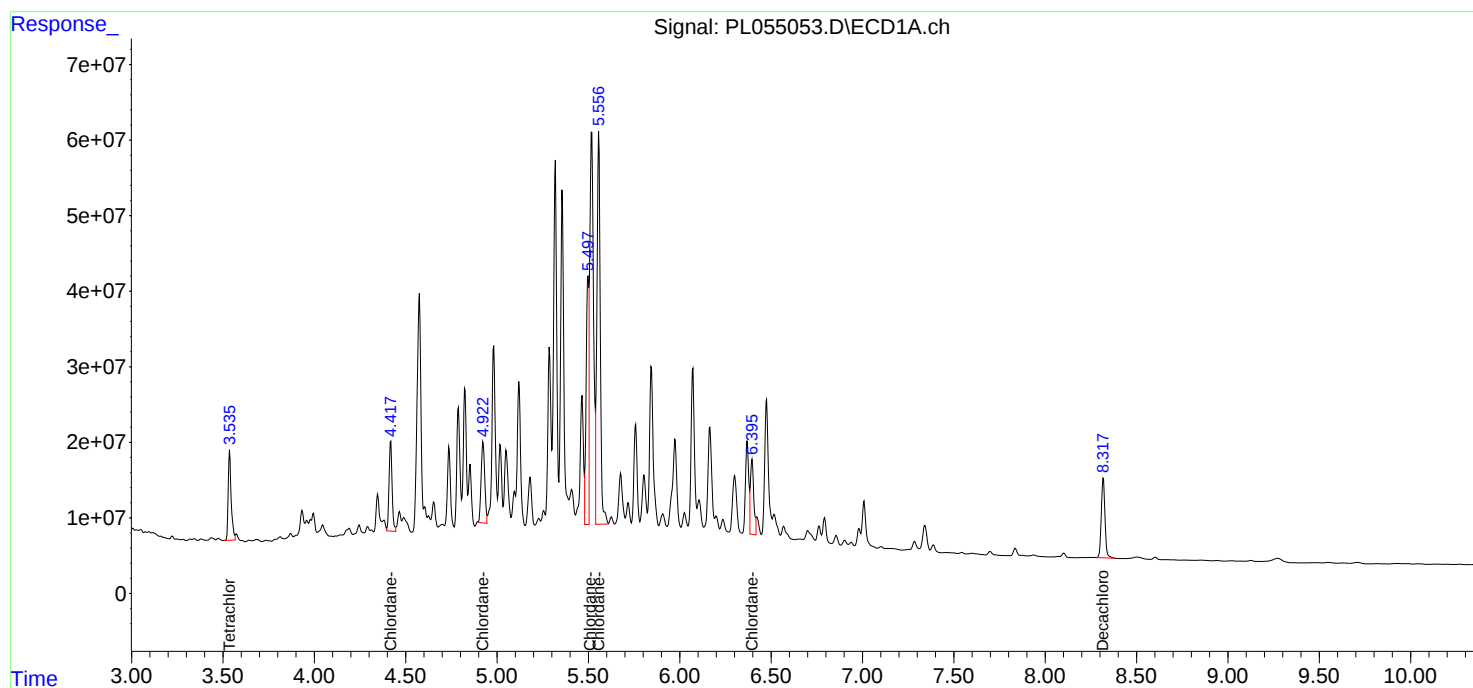

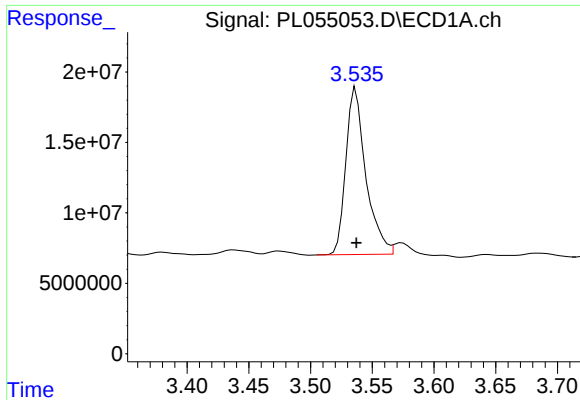


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 133550856
Conc: 11.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:01 PM

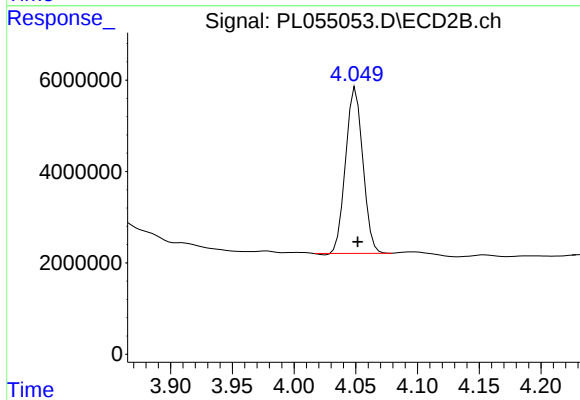


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 35277388
Conc: 13.82 ng/ml

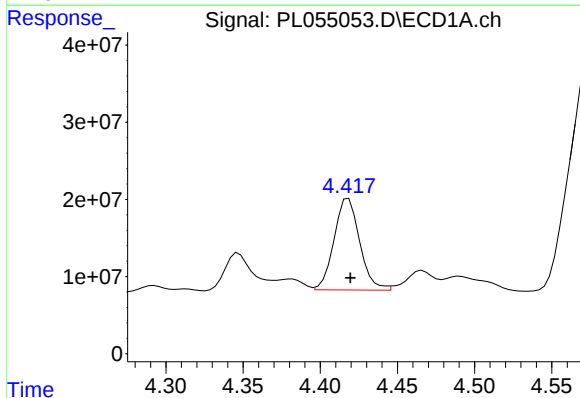


#23 Chlordane-1

R.T.: 4.418 min
Delta R.T.: -0.001 min
Response: 137116640
Conc: 347.45 ng/ml

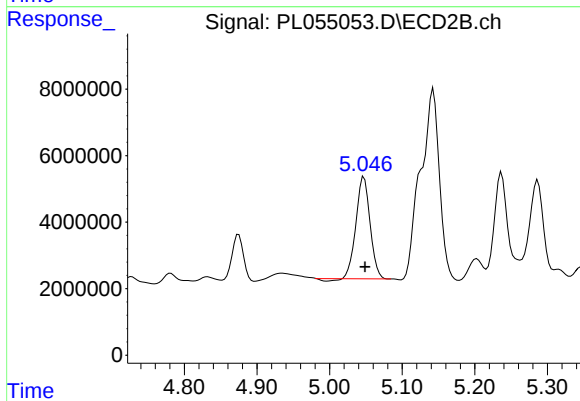

#23 Chlordane-1

R.T.: 5.047 min
Delta R.T.: -0.001 min
Response: 40718020
Conc: 510.80 ng/ml

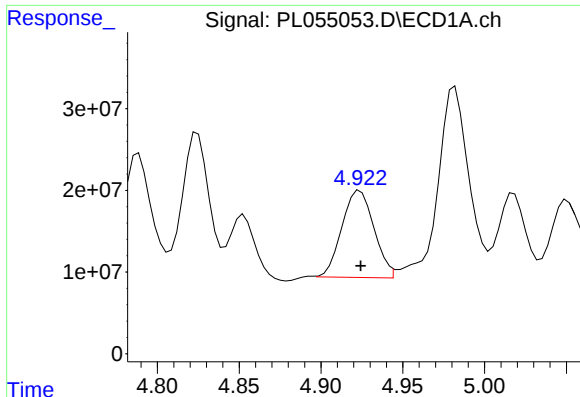


#24 Chlordane-2

R.T.: 4.922 min
Delta R.T.: -0.002 min
Response: 144952517
Conc: 333.79 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-6BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:01 PM

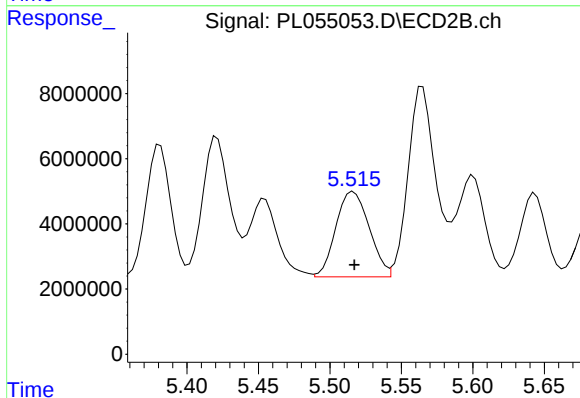


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: 0.000 min
Response: 42522264
Conc: 474.45 ng/ml

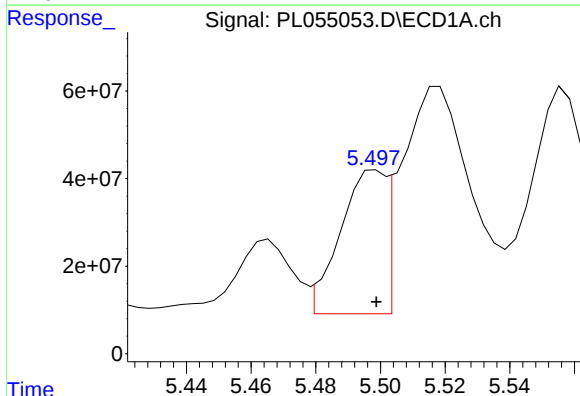


#25 Chlordane-3

R.T.: 5.499 min
Delta R.T.: 0.000 min
Response: 316196307
Conc: 246.23 ng/ml

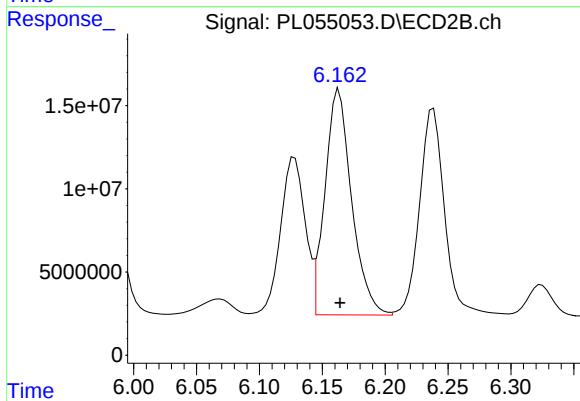

#25 Chlordane-3

R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 200077061
Conc: 644.58 ng/ml

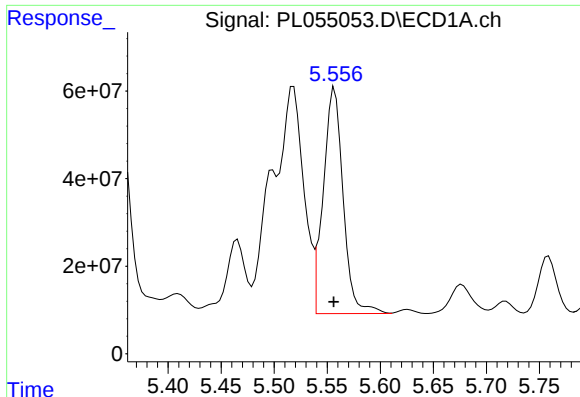


#26 Chlordane-4

R.T.: 5.557 min
Delta R.T.: 0.000 min
Response: 675898867
Conc: 639.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:01 PM

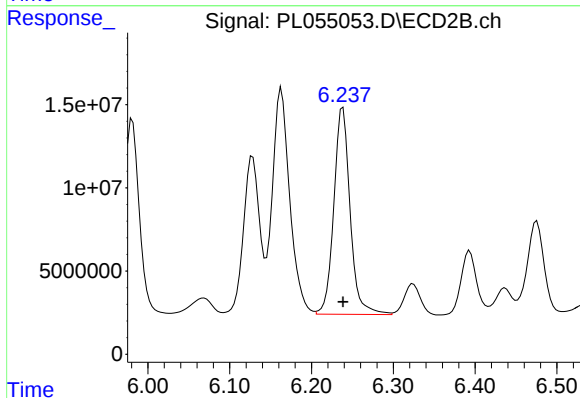


#26 Chlordane-4

R.T.: 6.238 min
Delta R.T.: 0.000 min
Response: 172335298
Conc: 457.99 ng/ml

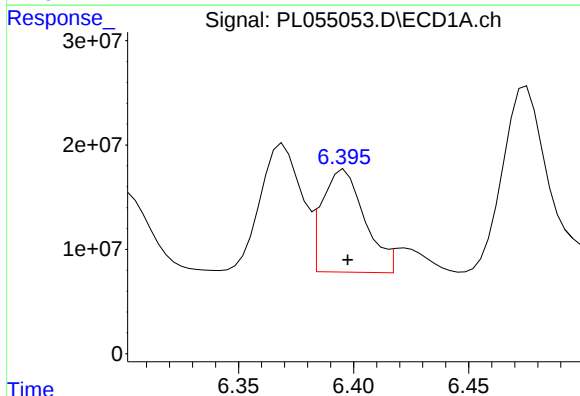


#27 Chlordane-5

R.T.: 6.396 min
Delta R.T.: -0.001 min
Response: 126340894
Conc: 335.57 ng/ml

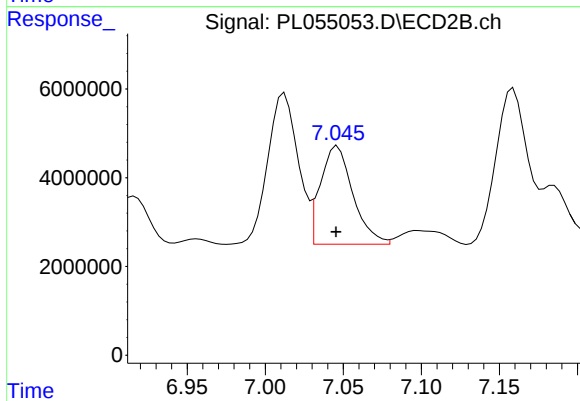

#27 Chlordane-5

R.T.: 7.046 min
Delta R.T.: 0.000 min
Response: 32211525
Conc: 477.79 ng/ml

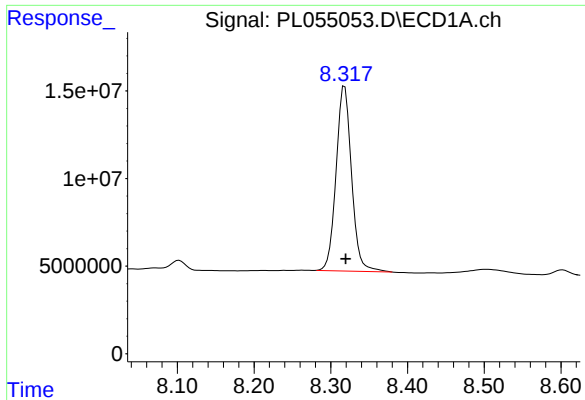


#28 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: -0.002 min
Response: 147951455
Conc: 15.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6BD

Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:01 PM

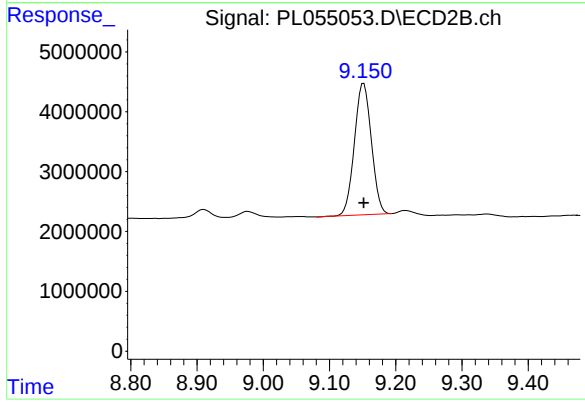

#28 Decachlorobiphenyl

R.T.: 9.152 min
Delta R.T.: 0.000 min
Response: 39067992
Conc: 16.30 ng/ml