

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
 Data File : PL055054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 19:58
 Operator : SG\AJ
 Sample : K6335-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-7BD

Manual Integrations
 APPROVED

Ankita
 12/18/2019 3:24:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 13:25:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.050	129.9E6	35732880	11.163	14.003 #
28)	SA Decachlor...	8.318	9.152	146.1E6	41807477	15.260	17.438
Target Compounds							
23)	Chlordane-1	4.418	5.048	121.5E6	35889130	307.793	450.226 #
24)	Chlordane-2	4.922	5.516	133.2E6	40167092	306.675m	448.173 #
25)	Chlordane-3	5.498	6.162	279.4E6	166.9E6	217.567	537.668 #
26)	Chlordane-4	5.556	6.238	542.0E6	156.9E6	513.105	417.030
27)	Chlordane-5	6.396	7.045	135.5E6	29999336	359.870	444.979

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
Data File : PL055054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 19:58
Operator : SG\AJ
Sample : K6335-04
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-7BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 13:25:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

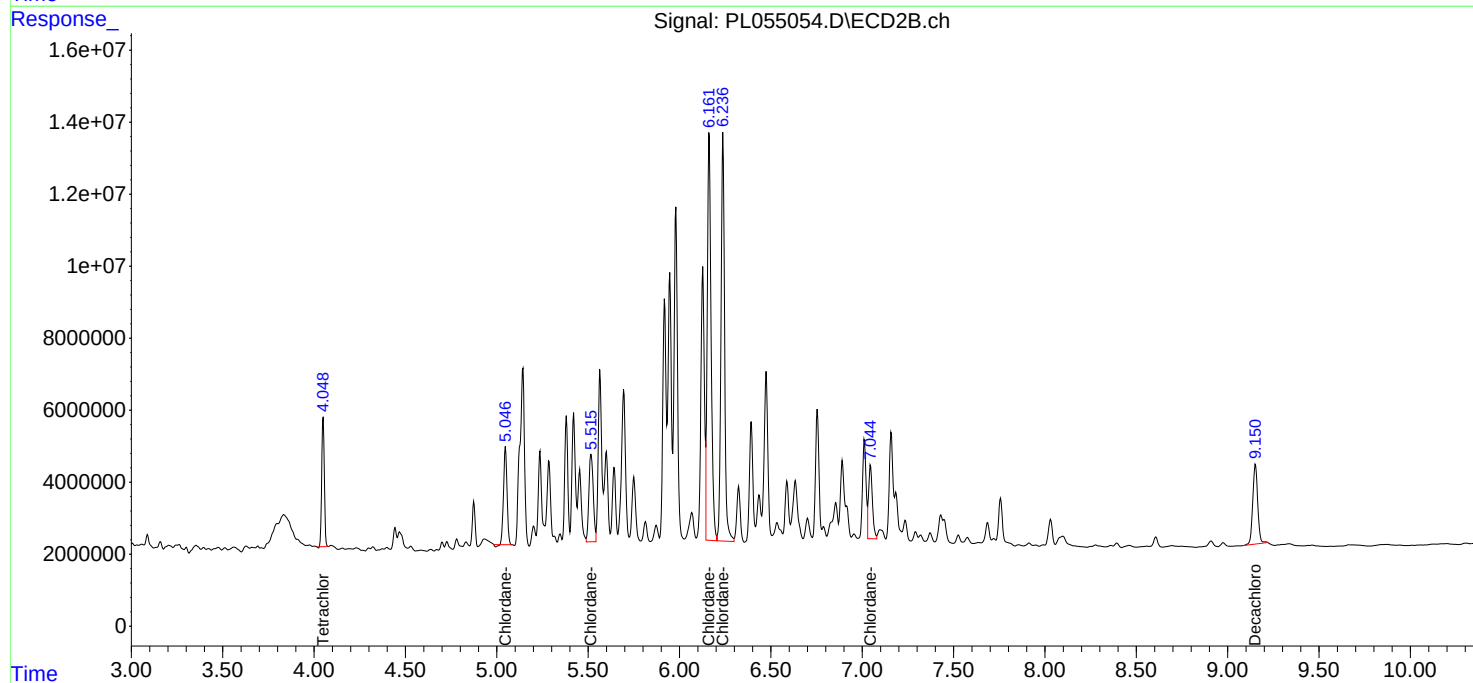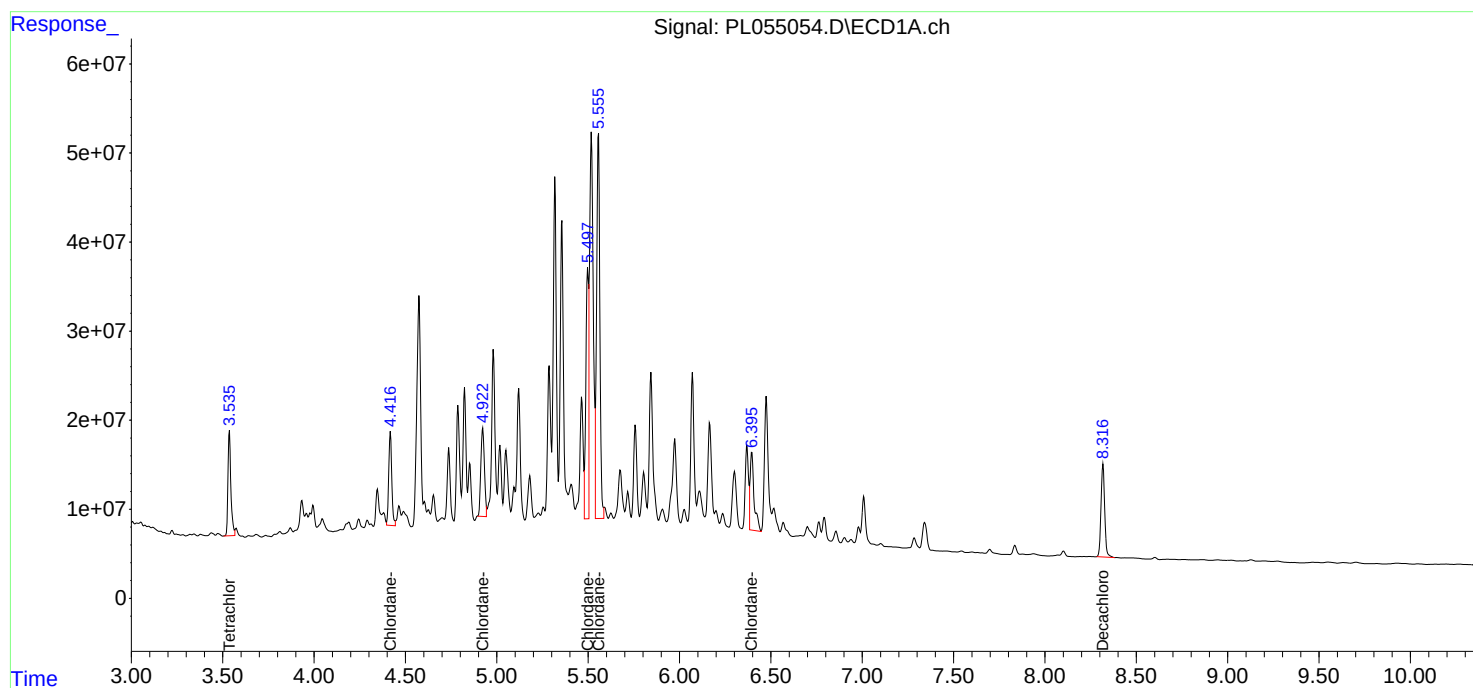

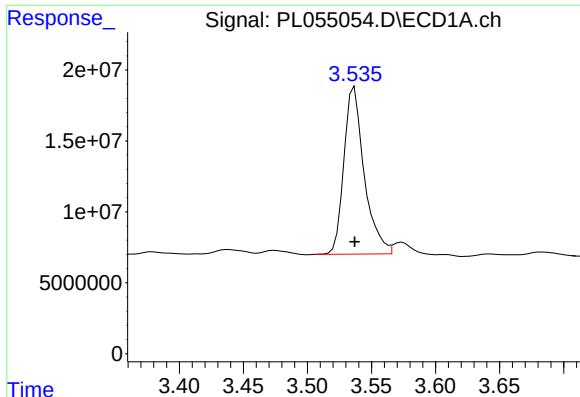


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 129870475
Conc: 11.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:02 PM

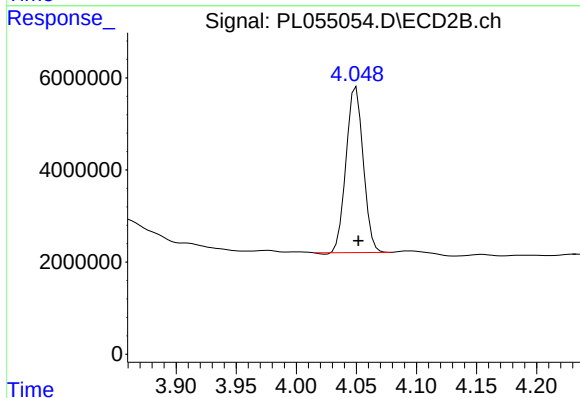


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 35732880
Conc: 14.00 ng/ml

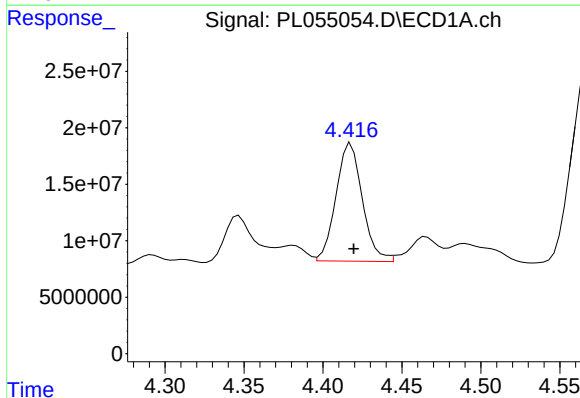


#23 Chlordane-1

R.T.: 4.418 min
Delta R.T.: -0.002 min
Response: 121466307
Conc: 307.79 ng/ml

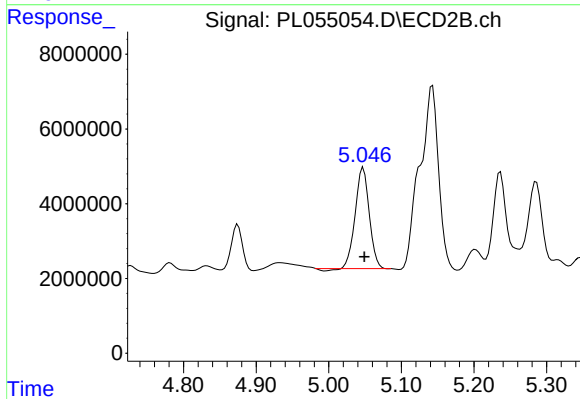

#23 Chlordane-1

R.T.: 5.048 min
Delta R.T.: -0.001 min
Response: 35889130
Conc: 450.23 ng/ml

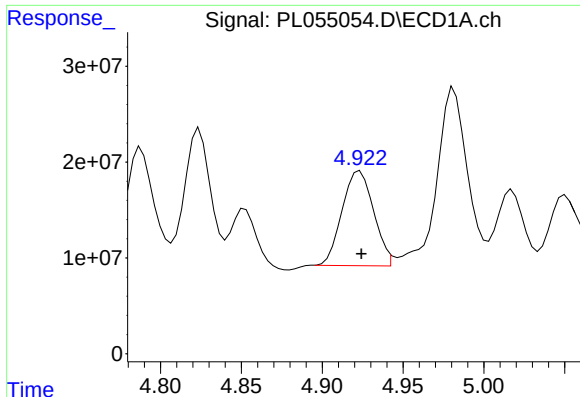


#24 Chlordane-2

R.T.: 4.922 min
Delta R.T.: -0.002 min
Response: 133175627
Conc: 306.67 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-7BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:02 PM

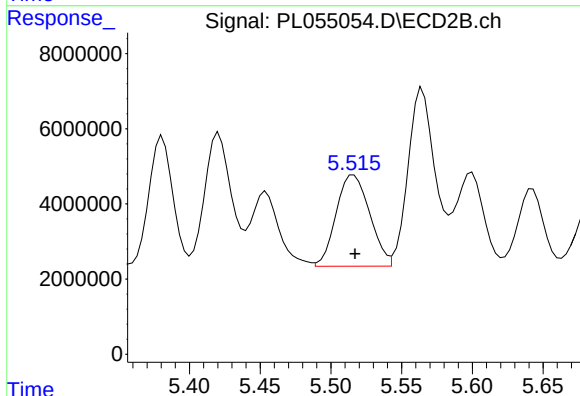


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: -0.001 min
Response: 40167092
Conc: 448.17 ng/ml

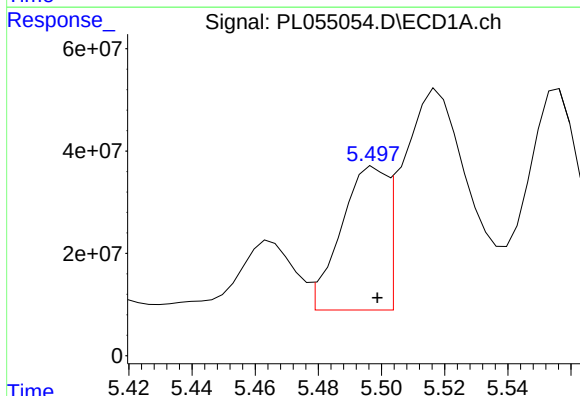


#25 Chlordane-3

R.T.: 5.498 min
Delta R.T.: 0.000 min
Response: 279384543
Conc: 217.57 ng/ml

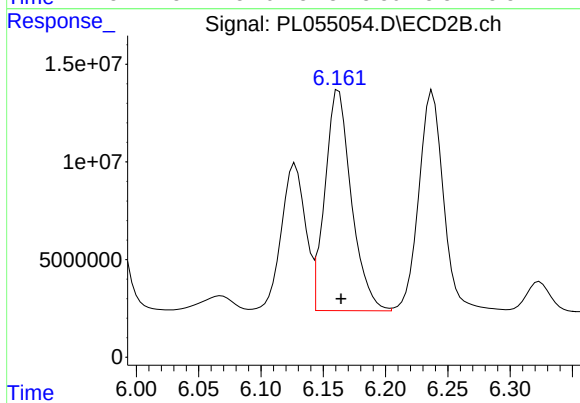

#25 Chlordane-3

R.T.: 6.162 min
Delta R.T.: -0.002 min
Response: 166892609
Conc: 537.67 ng/ml

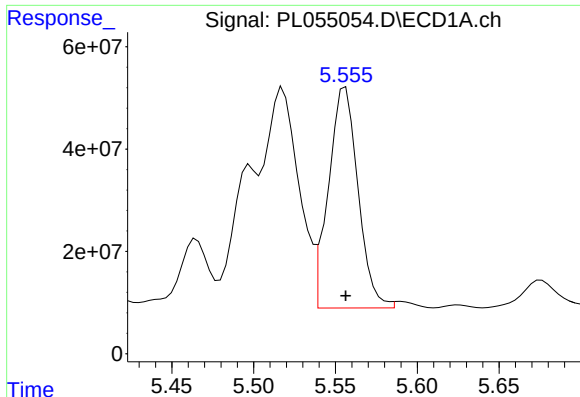


#26 Chlordane-4

R.T.: 5.556 min
Delta R.T.: 0.000 min
Response: 541987616
Conc: 513.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7BD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:02 PM

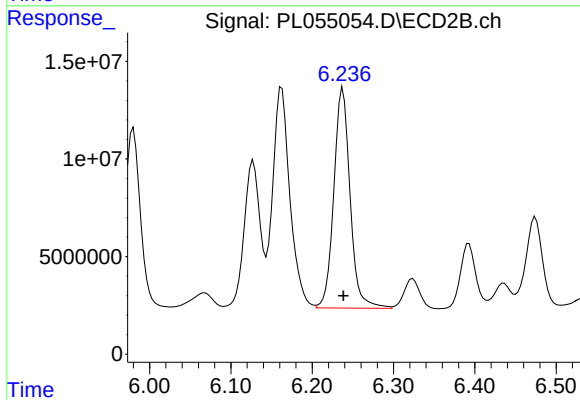


#26 Chlordane-4

R.T.: 6.238 min
Delta R.T.: 0.000 min
Response: 156923660
Conc: 417.03 ng/ml

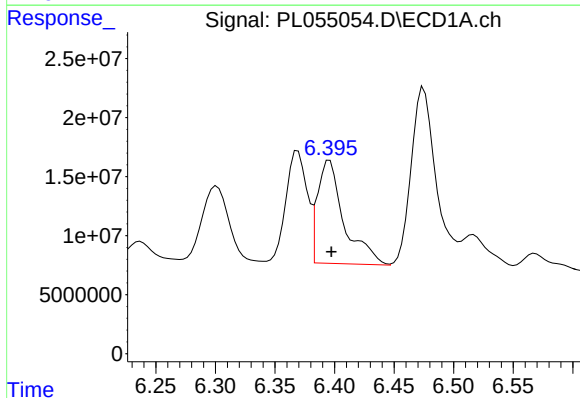


#27 Chlordane-5

R.T.: 6.396 min
Delta R.T.: -0.001 min
Response: 135491858
Conc: 359.87 ng/ml

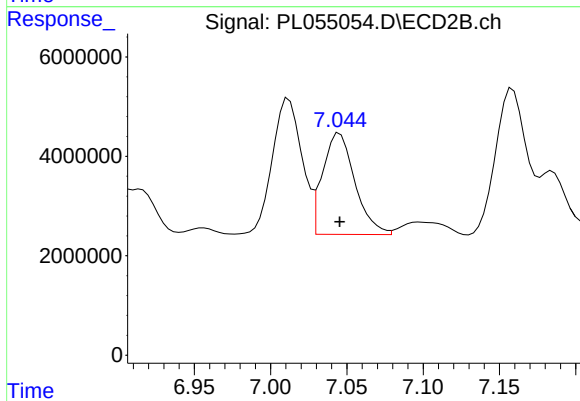

#27 Chlordane-5

R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 29999336
Conc: 444.98 ng/ml

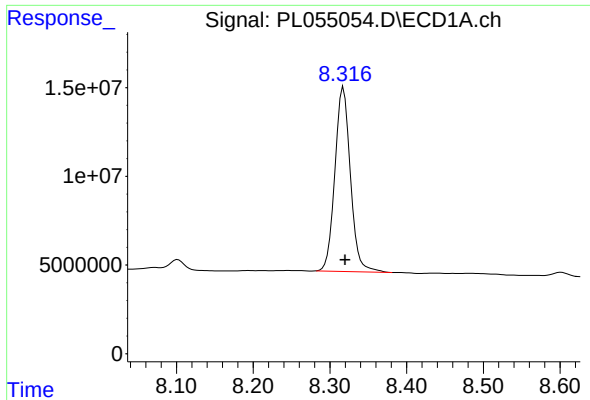

#28 Decachlorobiphenyl

R.T.: 8.318 min

Delta R.T.: -0.002 min


Response: 146128407

Conc: 15.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7BD

Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:02 PM

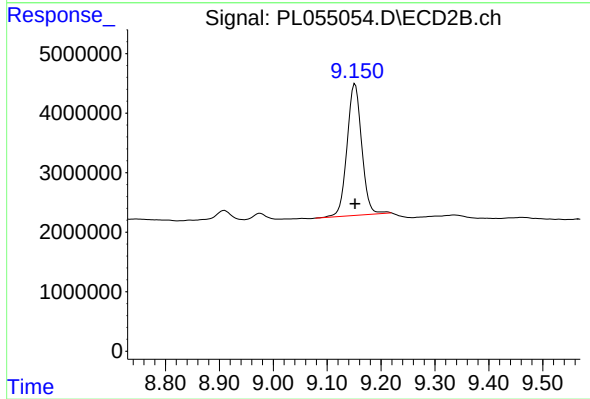

#28 Decachlorobiphenyl

R.T.: 9.152 min

Delta R.T.: 0.000 min

Response: 41807477

Conc: 17.44 ng/ml