

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
 Data File : PL055055.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 20:12
 Operator : SG\AJ
 Sample : K6335-05
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-1AD

Manual Integrations
 APPROVED

Ankita
 12/18/2019 3:24:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 13:25:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.050	130.2E6	35200318	11.194	13.794
28)	SA Decachlor...	8.316	9.151	141.7E6	38354712	14.794	15.998
Target Compounds							
23)	Chlordane-1	4.418	5.046	120.8E6	43576772	306.167	546.667 #
24)	Chlordane-2	4.923	5.515	131.9E6	38285503	303.803m	427.179 #
25)	Chlordane-3	5.498	6.162	259.5E6	169.9E6	202.071	547.510 #
26)	Chlordane-4	5.556	6.237	573.9E6	157.7E6	543.291	419.158
27)	Chlordane-5	6.395	7.045	107.3E6	29663421	284.924	439.996 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121719\
Data File : PL055055.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 20:12
Operator : SG\AJ
Sample : K6335-05
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-1AD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 13:25:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

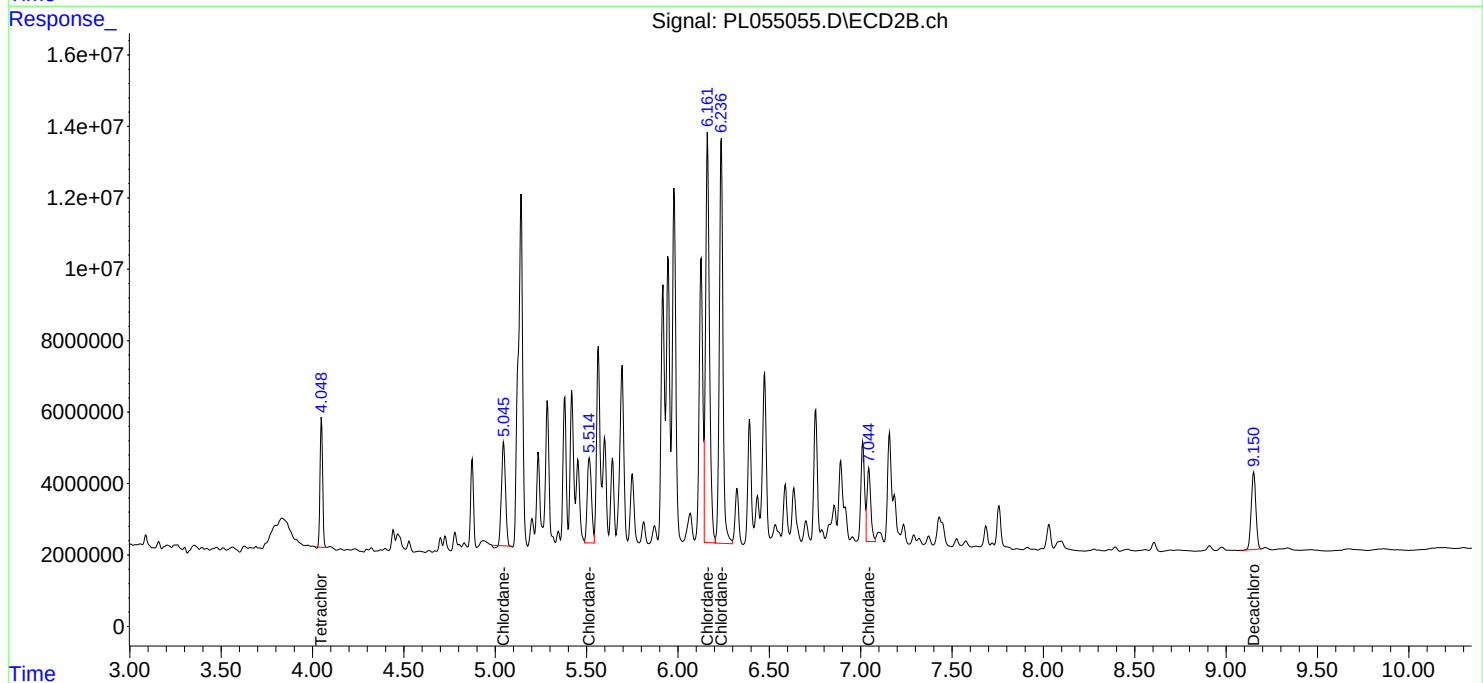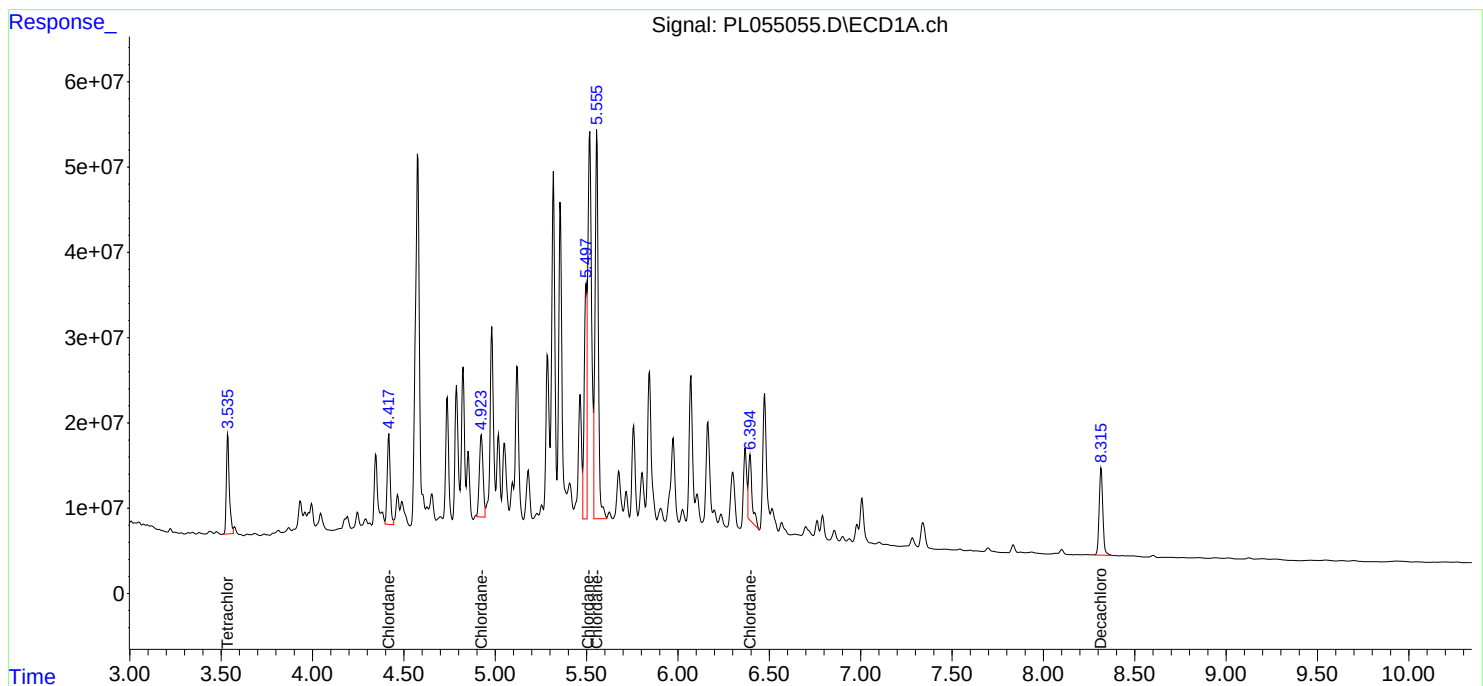

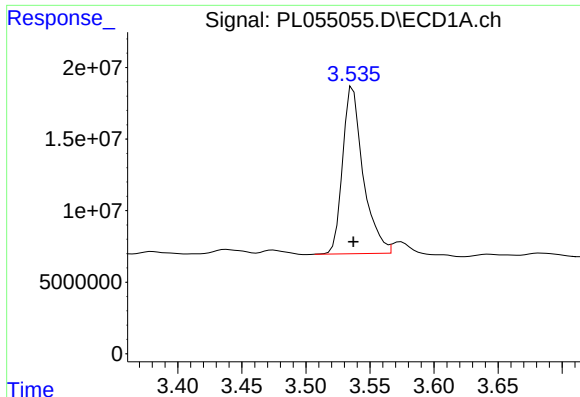


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 130228286
Conc: 11.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-1AD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:04 PM

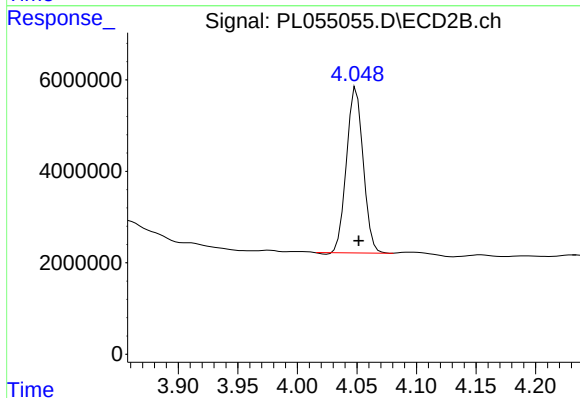


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 35200318
Conc: 13.79 ng/ml

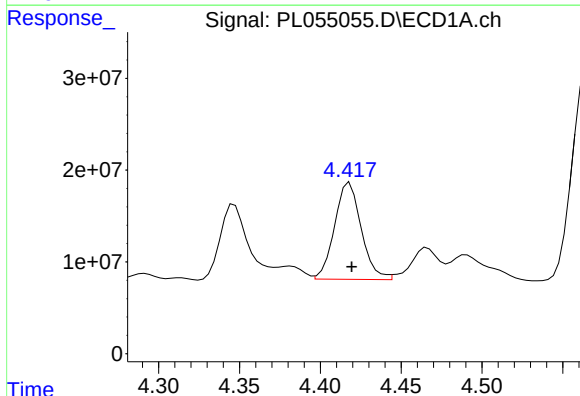


#23 Chlordane-1

R.T.: 4.418 min
Delta R.T.: -0.001 min
Response: 120824646
Conc: 306.17 ng/ml

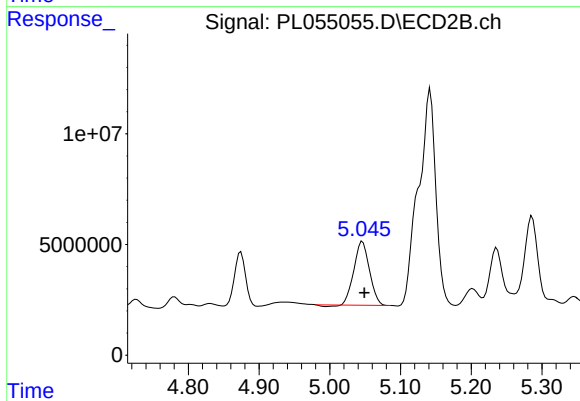

#23 Chlordane-1

R.T.: 5.046 min
Delta R.T.: -0.003 min
Response: 43576772
Conc: 546.67 ng/ml

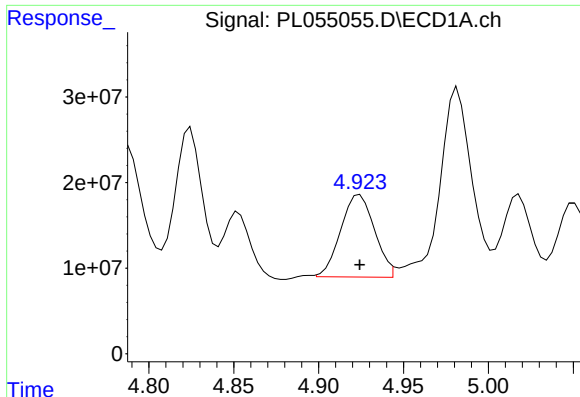


#24 Chlordane-2

R.T.: 4.923 min
Delta R.T.: -0.001 min
Response: 131928744
Conc: 303.80 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-1AD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:04 PM

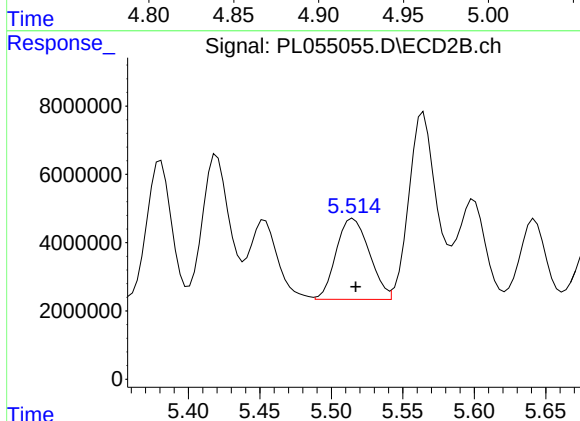


#24 Chlordane-2

R.T.: 5.515 min
Delta R.T.: -0.002 min
Response: 38285503
Conc: 427.18 ng/ml

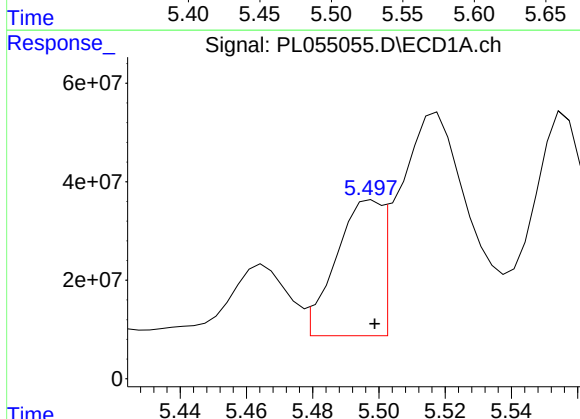


#25 Chlordane-3

R.T.: 5.498 min
Delta R.T.: 0.000 min
Response: 259485798
Conc: 202.07 ng/ml

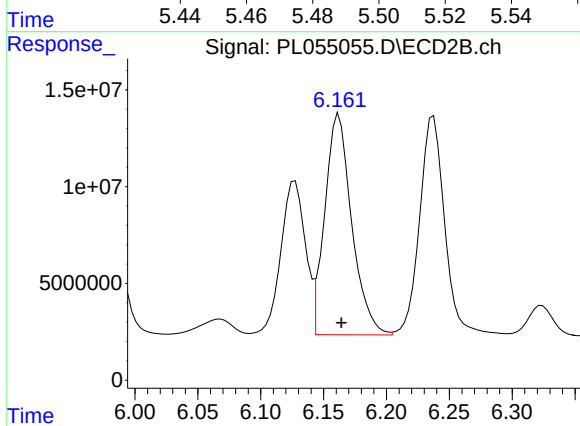

#25 Chlordane-3

R.T.: 6.162 min
Delta R.T.: -0.002 min
Response: 169947747
Conc: 547.51 ng/ml

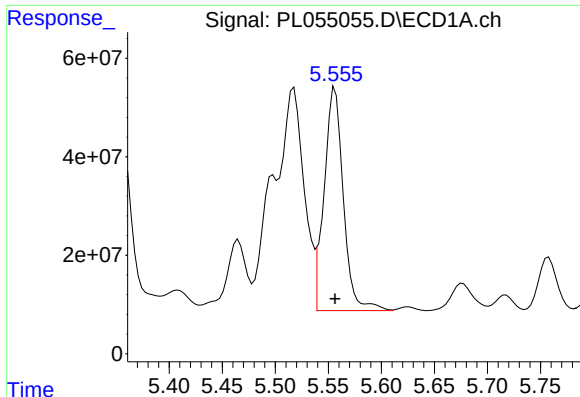


#26 Chlordane-4

R.T.: 5.556 min
Delta R.T.: 0.000 min
Response: 573872434
Conc: 543.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-1AD


Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:04 PM

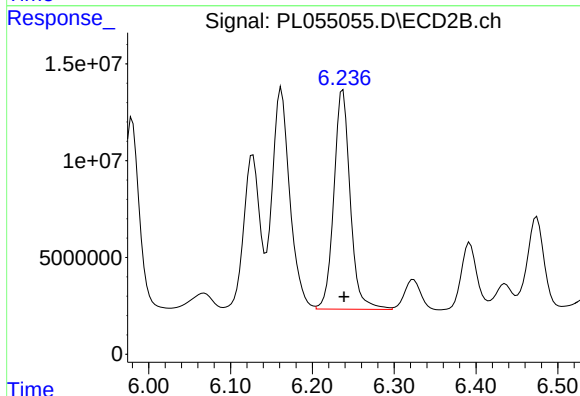


#26 Chlordane-4

R.T.: 6.237 min
Delta R.T.: -0.001 min
Response: 157724529
Conc: 419.16 ng/ml

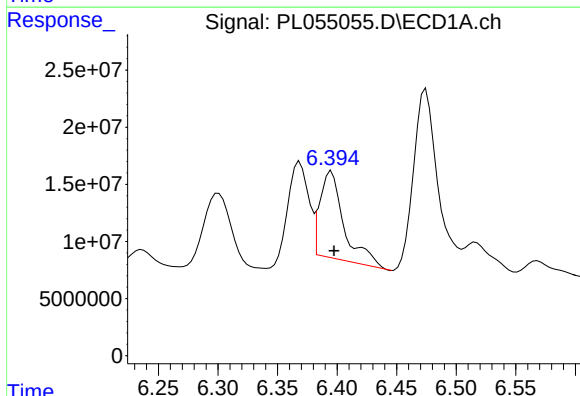


#27 Chlordane-5

R.T.: 6.395 min
Delta R.T.: -0.002 min
Response: 107274216
Conc: 284.92 ng/ml

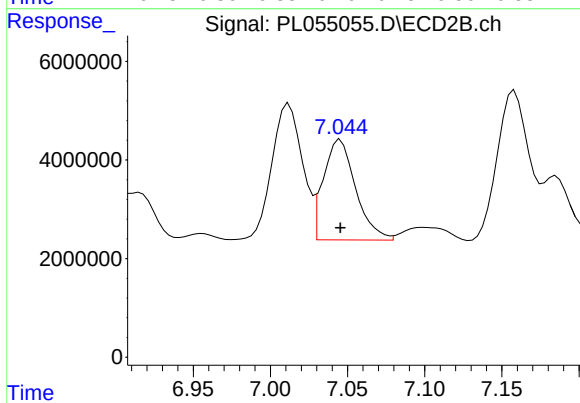

#27 Chlordane-5

R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 29663421
Conc: 440.00 ng/ml

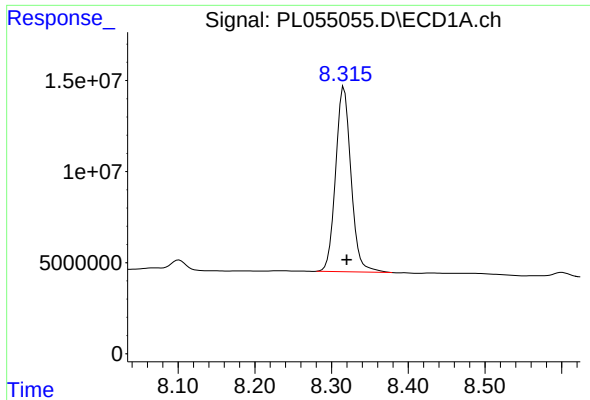


#28 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: -0.003 min
Response: 141673369
Conc: 14.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-1AD

Manual Integrations
APPROVED

Ankita
12/18/2019 3:24:04 PM

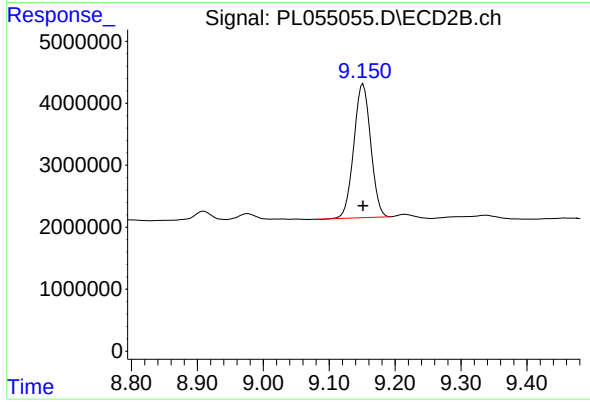

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 38354712
Conc: 16.00 ng/ml