

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121720\
 Data File : PL063654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 12:37
 Operator : DD\AJ
 Sample : PB133608BS
 Misc : CHLOR BLANK SPIKE
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB133608BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 13:31:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 09:38:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	4.149	43609091	63725137	21.440	19.977
28)	SA Decachlor...	8.232	9.341	46076547	51715180	21.090	19.303
Target Compounds							
23)	Chlordane-1	4.356	5.169	13678156	22168770	181.932	190.811
24)	Chlordane-2	4.856	5.646	17569622	24055279	199.556	193.009
25)	Chlordane-3	5.424	6.303	45464821	84162286	184.819	182.039
26)	Chlordane-4	5.482	6.377	37866471	100.4E6	186.656	183.199
27)	Chlordane-5	6.313	7.200	15667048	16114836	186.510	184.913



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121720\
Data File : PL063654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 12:37
Operator : DD\AJ
Sample : PB133608BS
Misc : CHLOR BLANK SPIKE
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB133608BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 13:31:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 09:38:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

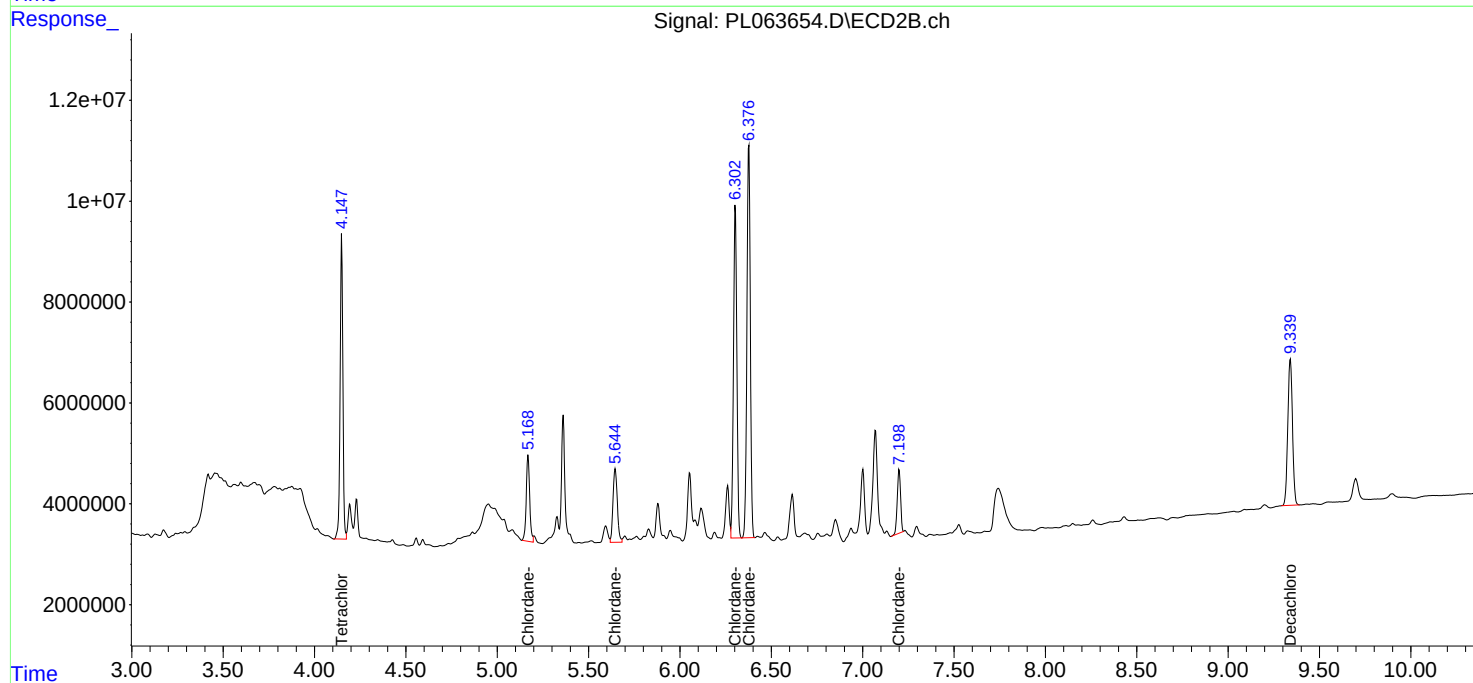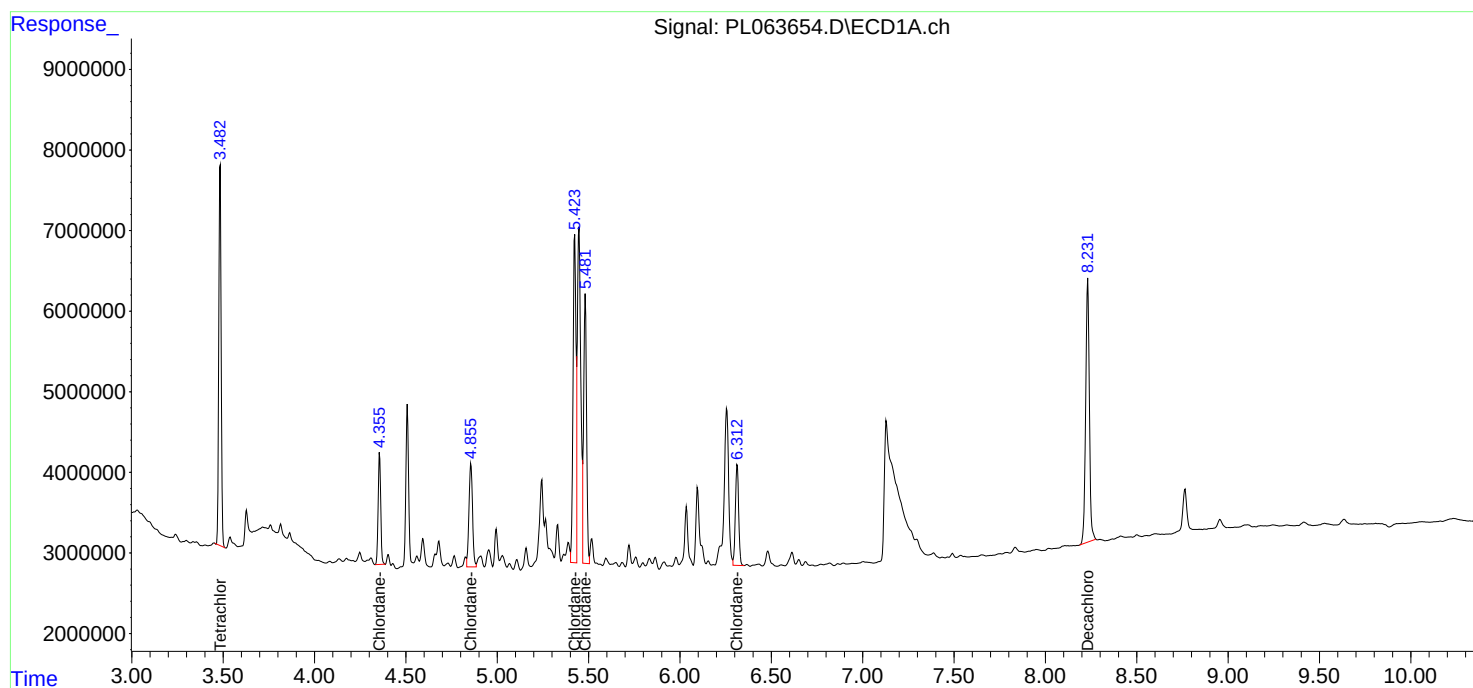


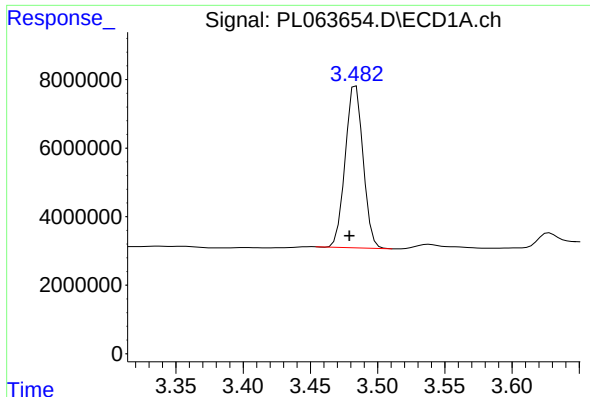

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: 0.005 min
Response: 43609091
Conc: 21.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB133608BS

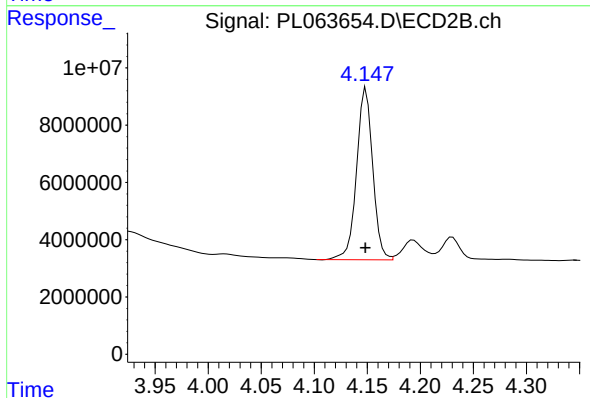


#1 Tetrachloro-m-xylene

R.T.: 4.149 min
Delta R.T.: 0.000 min
Response: 63725137
Conc: 19.98 ng/ml

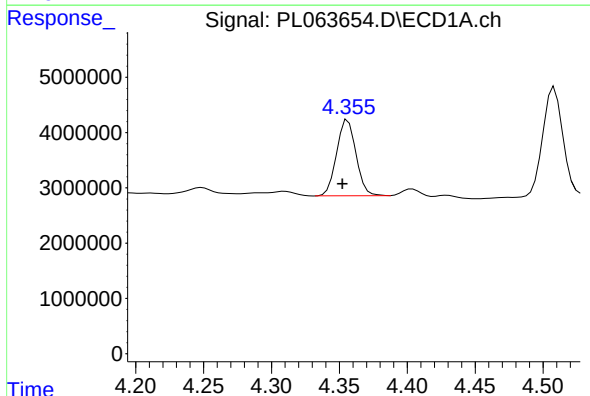


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: 0.004 min
Response: 13678156
Conc: 181.93 ng/ml

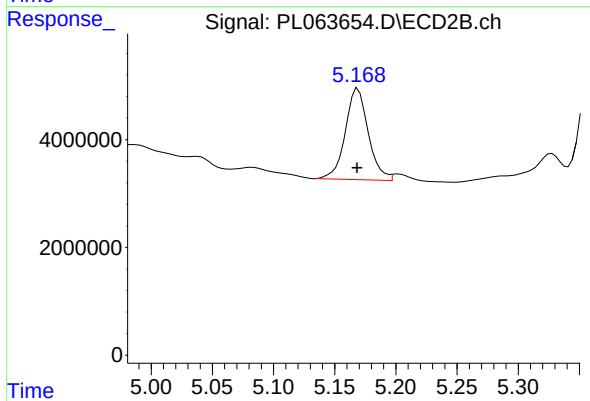

#23 Chlordane-1


R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 22168770
Conc: 190.81 ng/ml

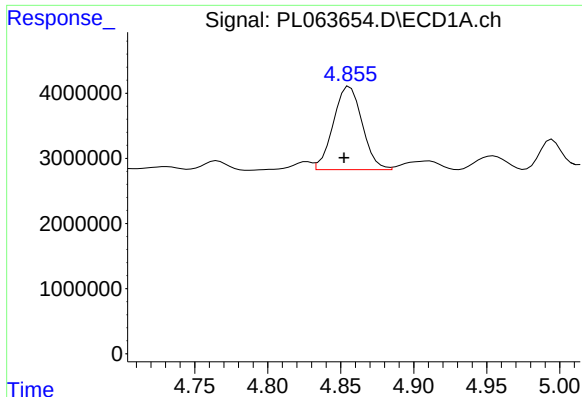

#24 Chlordane-2


R.T.: 4.856 min
Delta R.T.: 0.004 min
Response: 17569622
Conc: 199.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB133608BS

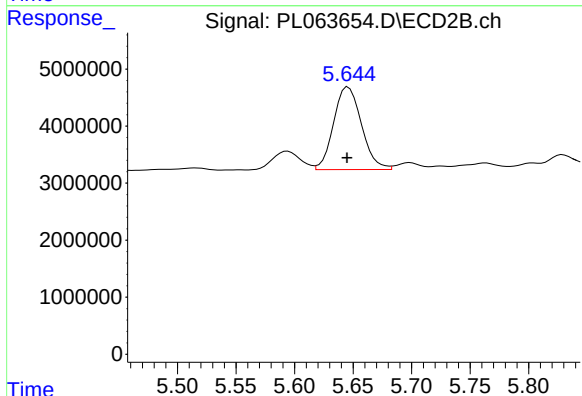


#24 Chlordane-2

R.T.: 5.646 min
Delta R.T.: 0.000 min
Response: 24055279
Conc: 193.01 ng/ml

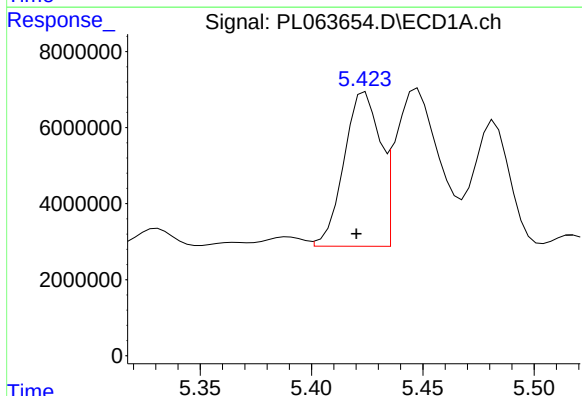


#25 Chlordane-3

R.T.: 5.424 min
Delta R.T.: 0.004 min
Response: 45464821
Conc: 184.82 ng/ml

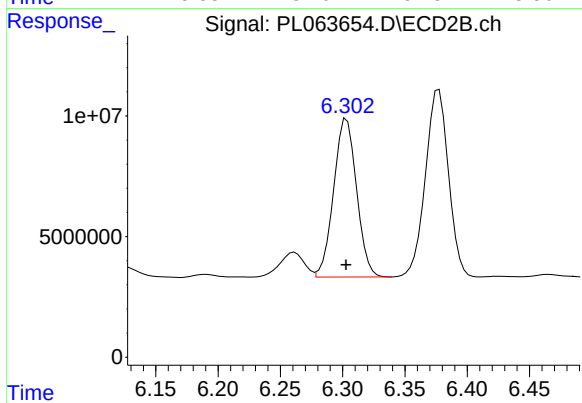

#25 Chlordane-3


R.T.: 6.303 min
Delta R.T.: 0.000 min
Response: 84162286
Conc: 182.04 ng/ml

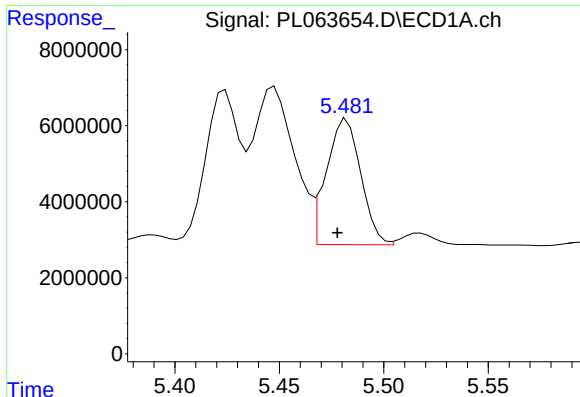

#26 Chlordane-4


R.T.: 5.482 min
Delta R.T.: 0.004 min
Response: 37866471
Conc: 186.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB133608BS

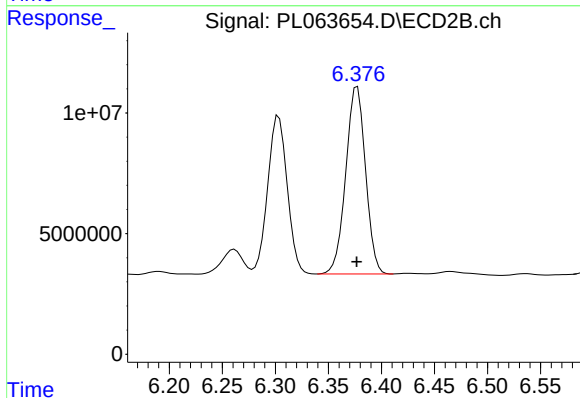


#26 Chlordane-4

R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 100434435
Conc: 183.20 ng/ml

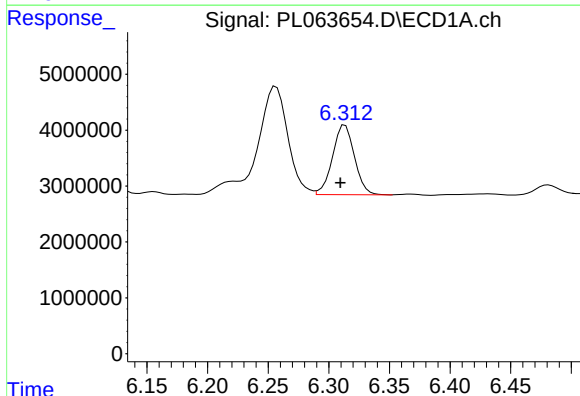


#27 Chlordane-5

R.T.: 6.313 min
Delta R.T.: 0.004 min
Response: 15667048
Conc: 186.51 ng/ml

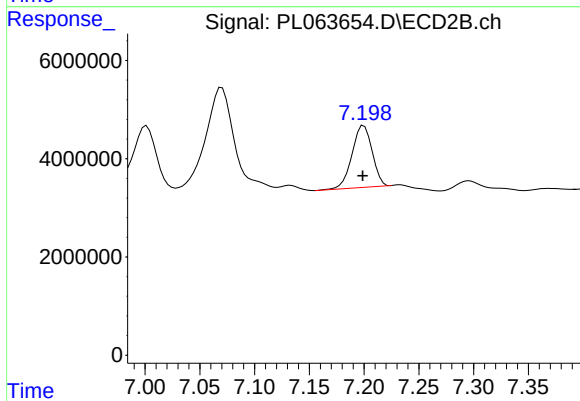

#27 Chlordane-5


R.T.: 7.200 min
Delta R.T.: 0.001 min
Response: 16114836
Conc: 184.91 ng/ml

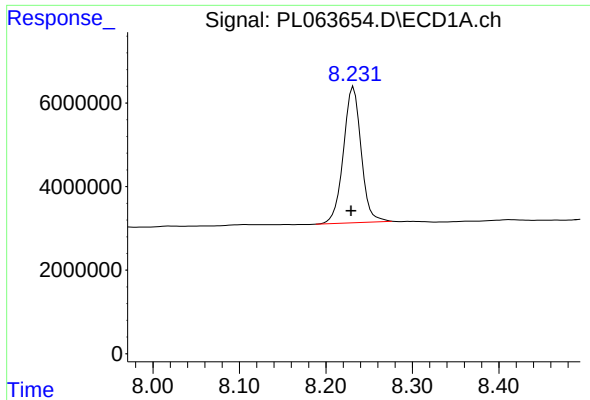

#28 Decachlorobiphenyl

R.T.: 8.232 min
Delta R.T.: 0.003 min
Response: 46076547
Conc: 21.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB133608BS

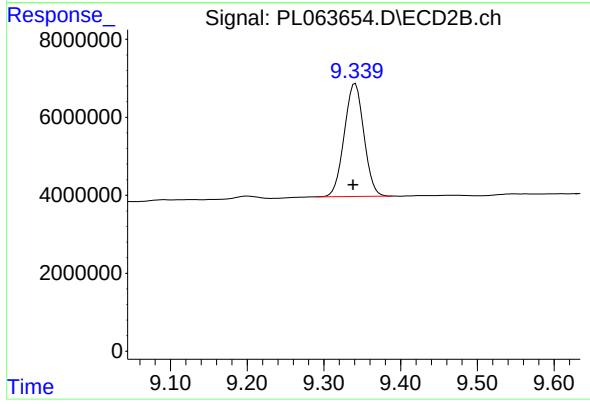

#28 Decachlorobiphenyl

R.T.: 9.341 min
Delta R.T.: 0.003 min
Response: 51715180
Conc: 19.30 ng/ml