

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121720\
 Data File : PL063673.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 17:32
 Operator : DD\AJ
 Sample : L5036-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-9

Manual Integrations
 APPROVED

Ankita
 12/18/2020 3:20:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 01:08:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 09:38:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.479	4.148	27858827	44562782	13.696	13.970
28)	SA Decachlor...	8.224	9.335	84795900	105.9E6	38.812	39.536
Target Compounds							
12)	B 4,4'-DDE	5.639	6.529	5496666	8316253	2.236	2.576m
17)	MA 4,4'-DDT	6.391	7.329	7284123	5358885	3.753	2.205 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121720\
Data File : PL063673.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 17:32
Operator : DD\AJ
Sample : L5036-10
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
B-9


Manual Integrations
APPROVED

Ankita
12/18/2020 3:20:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 01:08:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 09:38:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

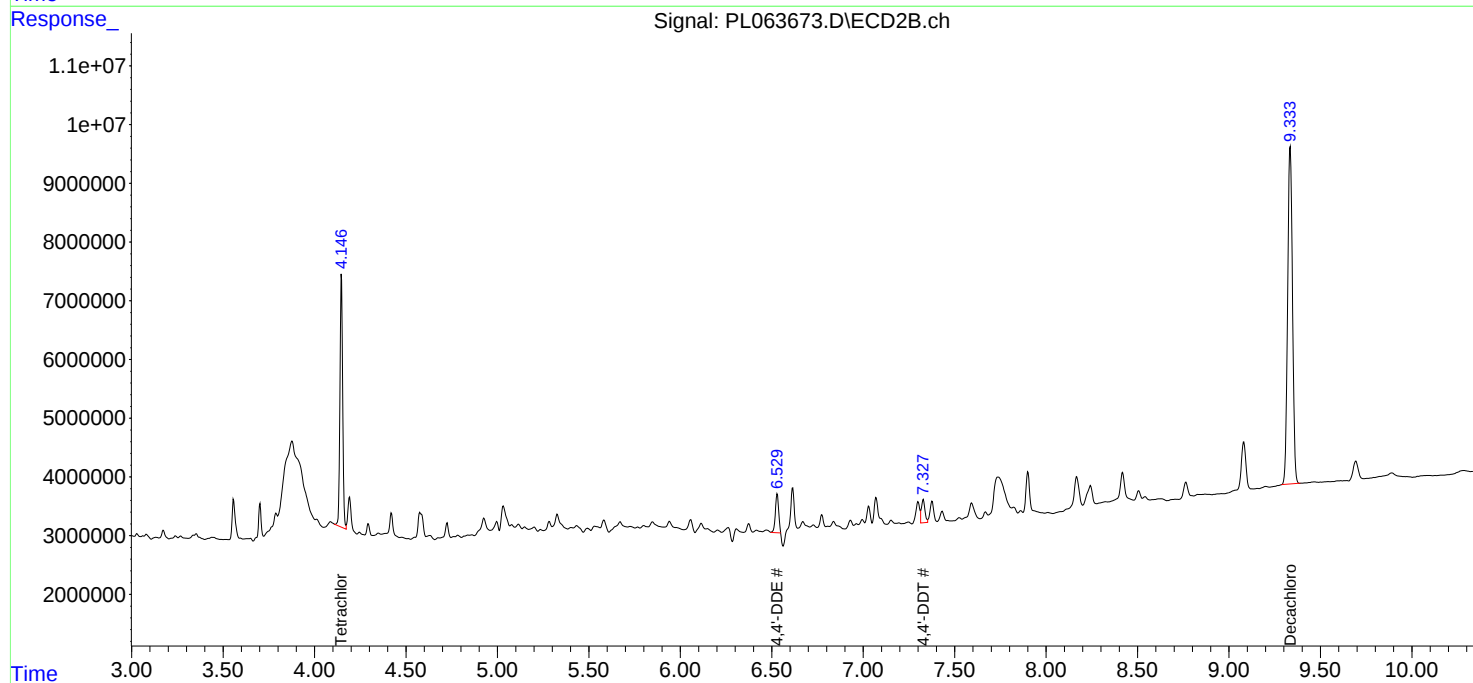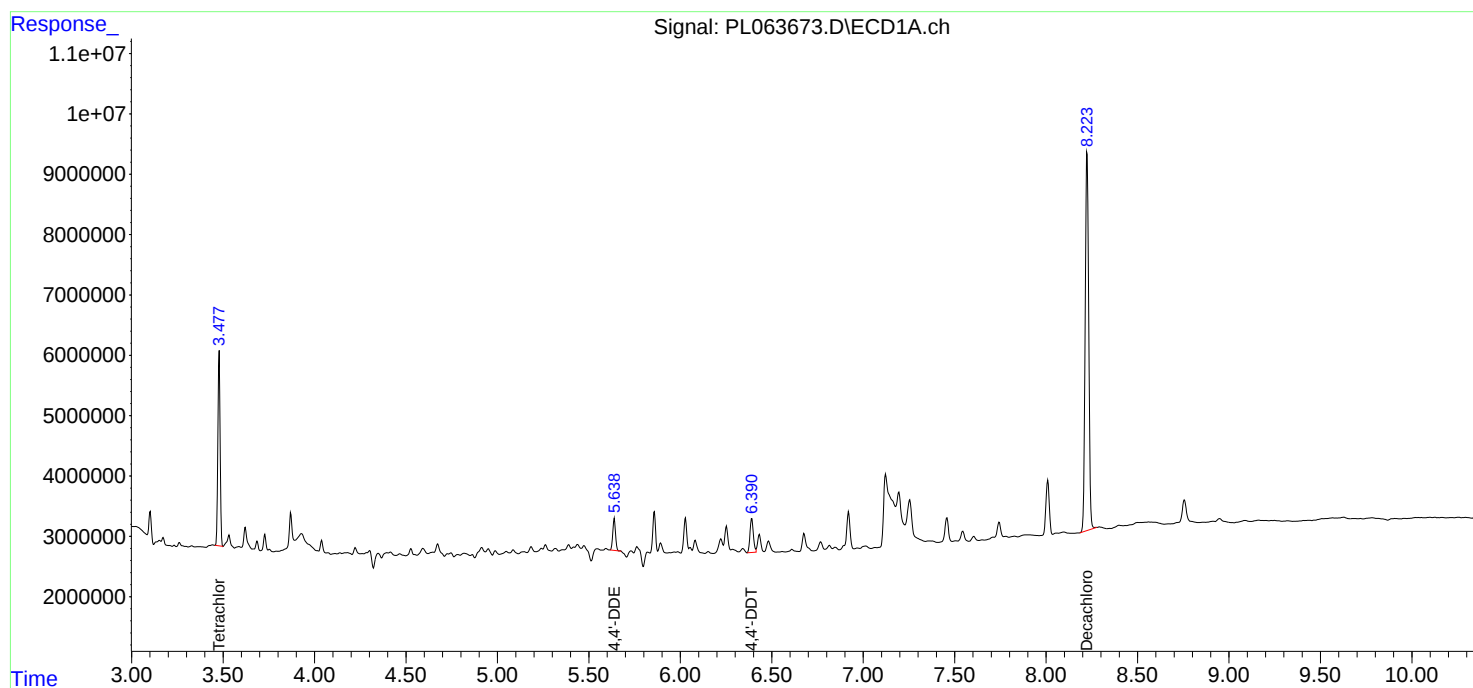

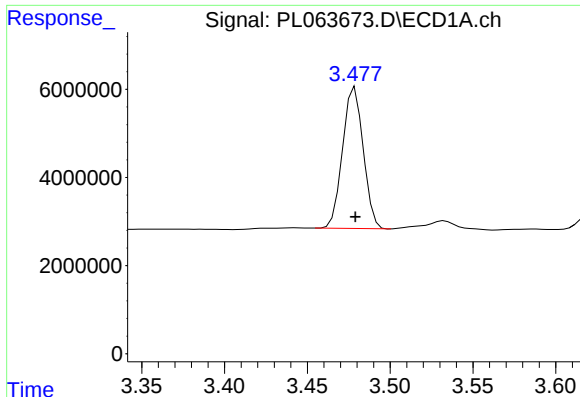


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 27858827
Conc: 13.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-9


Manual Integrations
APPROVED

Ankita
12/18/2020 3:20:34 PM

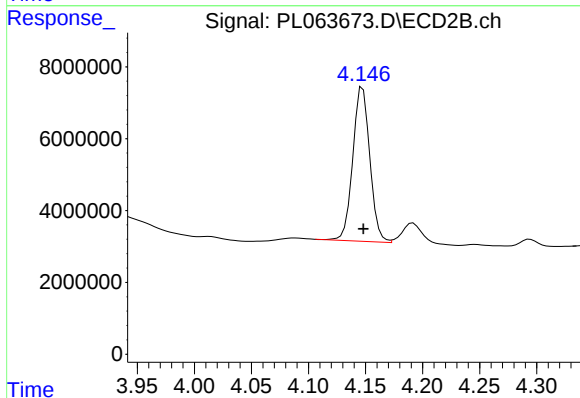


#1 Tetrachloro-m-xylene

R.T.: 4.148 min
Delta R.T.: 0.000 min
Response: 44562782
Conc: 13.97 ng/ml

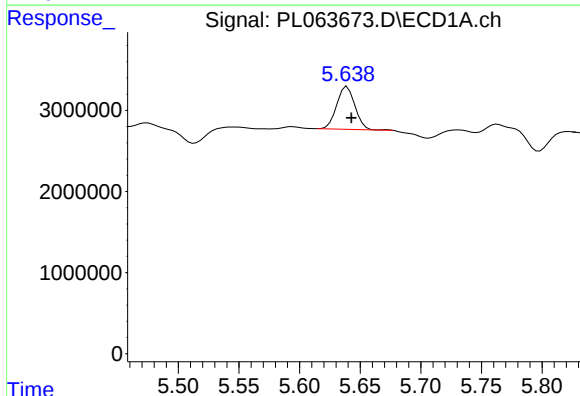


#12 4,4'-DDE

R.T.: 5.639 min
Delta R.T.: -0.003 min
Response: 5496666
Conc: 2.24 ng/ml

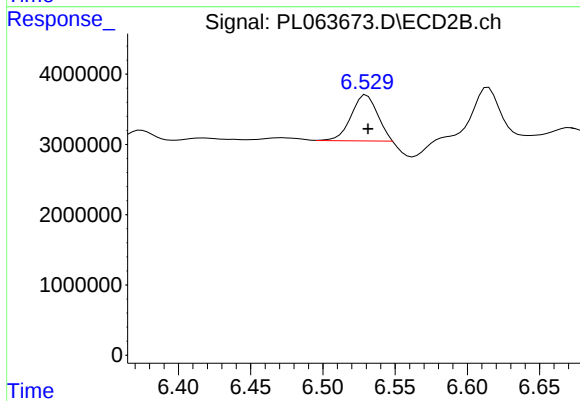

#12 4,4'-DDE

R.T.: 6.529 min
Delta R.T.: -0.003 min
Response: 8316253
Conc: 2.58 ng/ml m

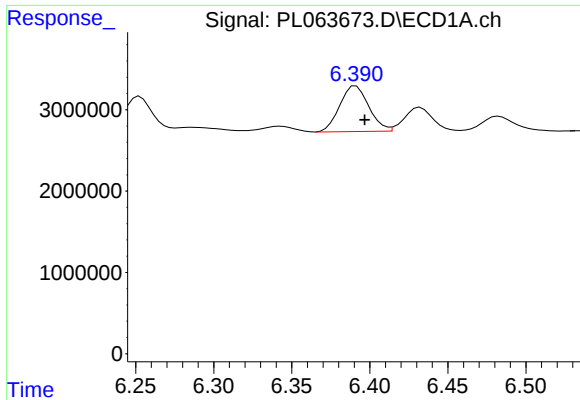


#17 4,4'-DDT

R.T.: 6.391 min
Delta R.T.: -0.006 min
Response: 7284123
Conc: 3.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-9


Manual Integrations
APPROVED

Ankita
12/18/2020 3:20:34 PM

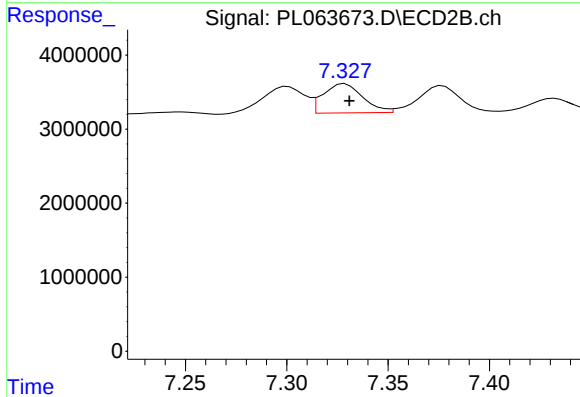


#17 4,4'-DDT

R.T.: 7.329 min
Delta R.T.: -0.002 min
Response: 5358885
Conc: 2.20 ng/ml

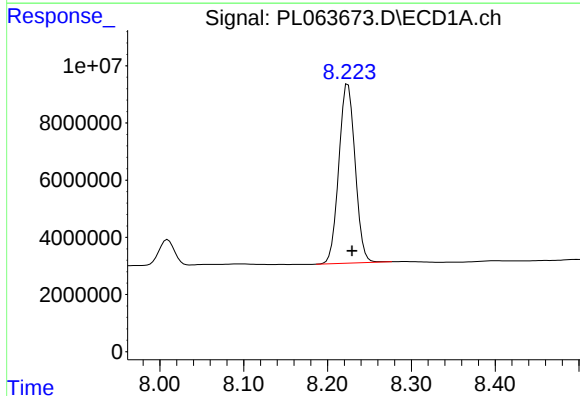

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.005 min
Response: 84795900
Conc: 38.81 ng/ml

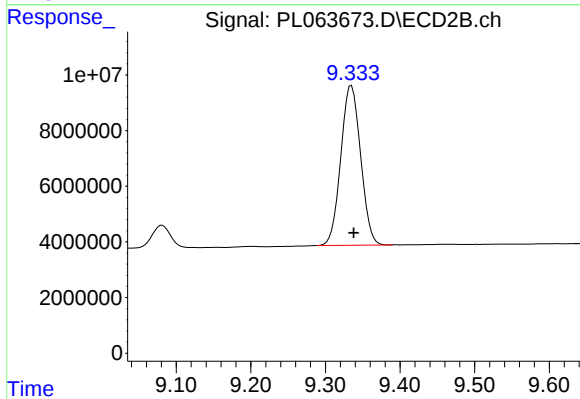

#28 Decachlorobiphenyl

R.T.: 9.335 min
Delta R.T.: -0.003 min
Response: 105922882
Conc: 39.54 ng/ml