

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121721\
 Data File : PL071511.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2021 14:02
 Operator : AR\AJ
 Sample : M5051-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 23:14:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	11.393	0	117258	N.D.	0.108 #
Target Compounds							
7)	B delta-BHC	0.000	7.023f	0	55330	N.D.	0.036 #
9)	A Endosulfan I	0.000	8.348	0	35257	N.D.	0.029 #
10)	B gamma-Chl...	0.000	8.235	0	143399	N.D.	0.111 #
11)	B alpha-Chl...	0.000	8.295	0	29606	N.D.	0.023 #
16)	A 4,4'-DDD	0.000	9.008f	0	25240	N.D.	0.029 #
17)	MA 4,4'-DDT	0.000	9.330f	0	65206	N.D.	0.066 #
18)	B Endrin al...	0.000	9.284f	0	27396	N.D.	0.036 #
25)	Chlordane-3	0.000	8.235	0	143399	N.D.	0.819 #
26)	Chlordane-4	0.000	8.295	0	29606	N.D.	0.141 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121721\
Data File : PL071511.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2021 14:02
Operator : AR\AJ
Sample : M5051-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 23:14:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

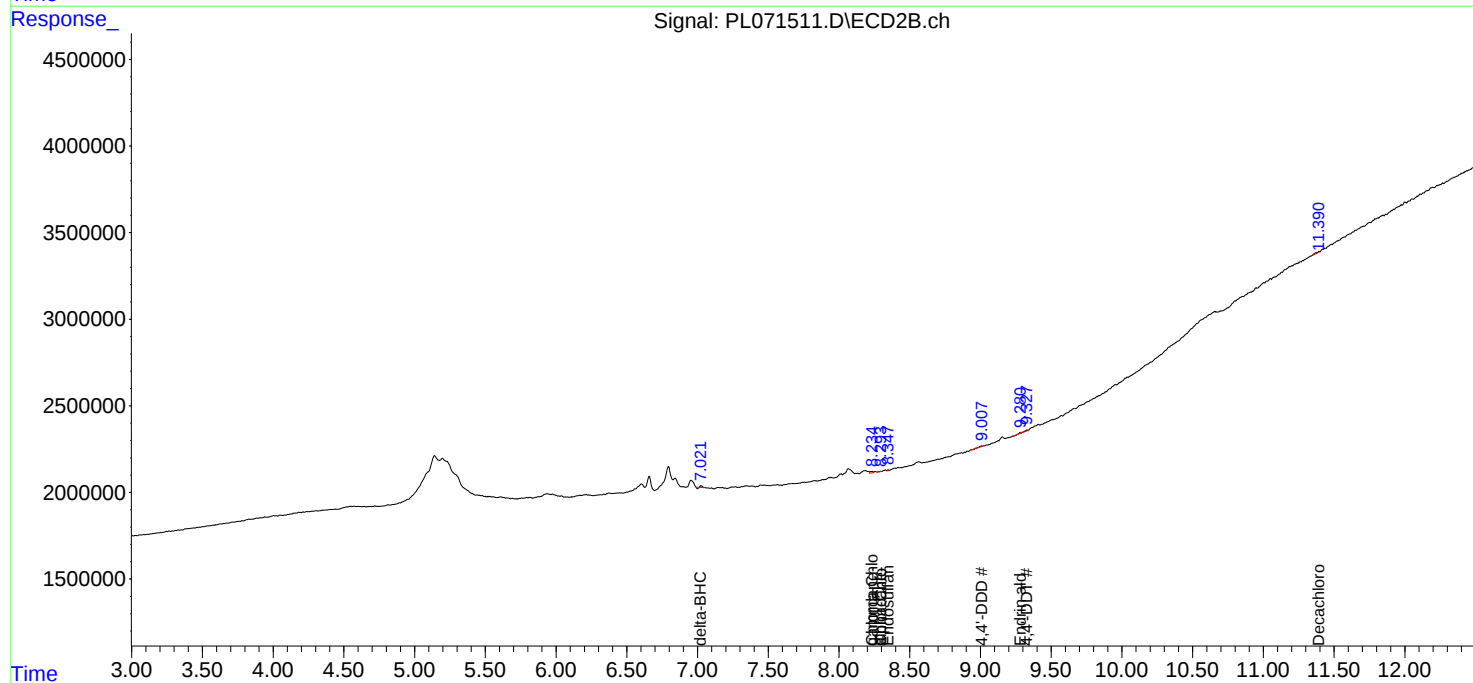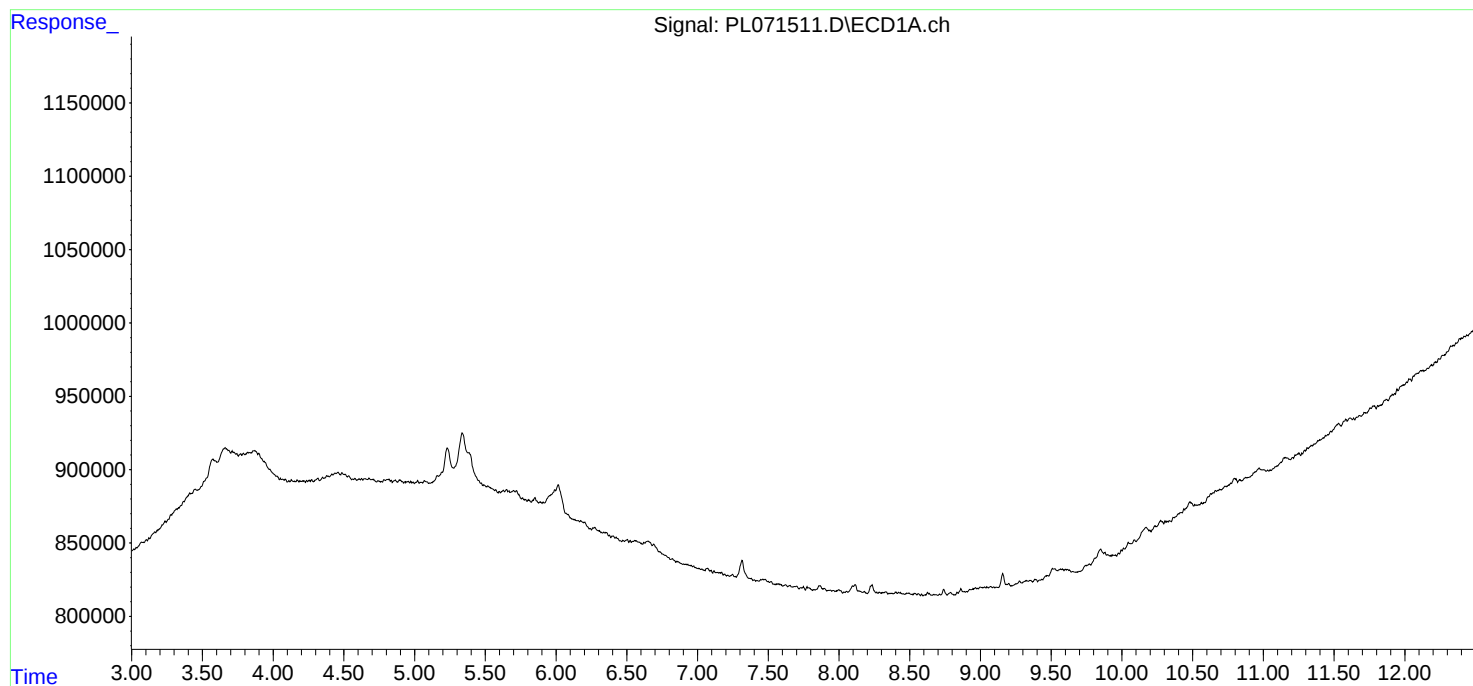


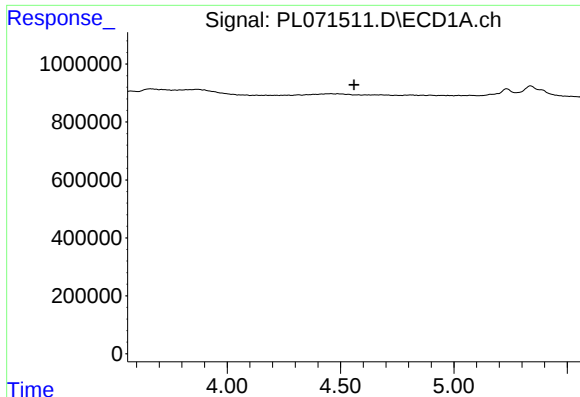

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

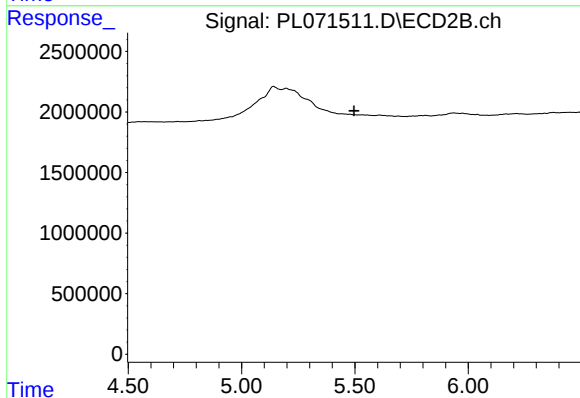


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

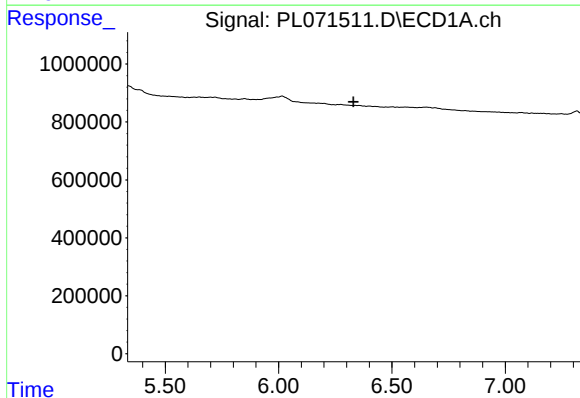


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

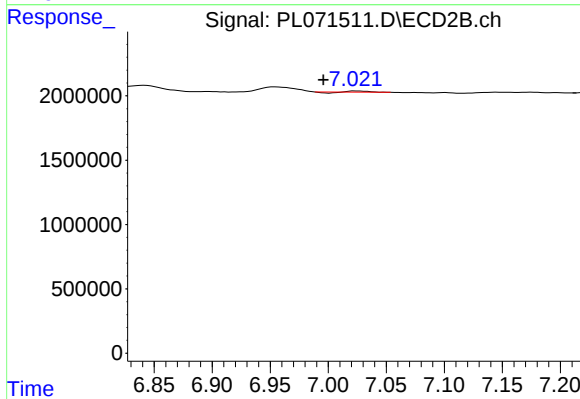

#7 delta-BHC


R.T.: 7.023 min
Delta R.T.: 0.027 min
Response: 55330
Conc: 0.04 ng/ml

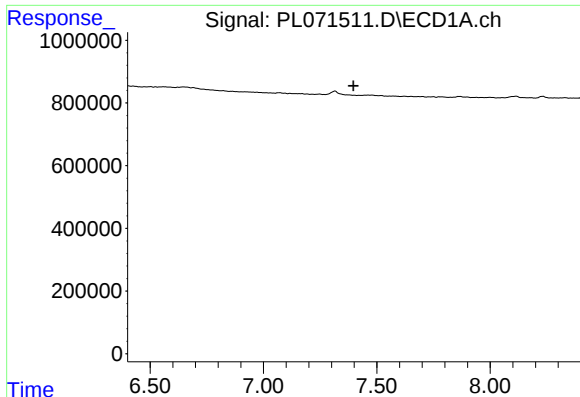

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

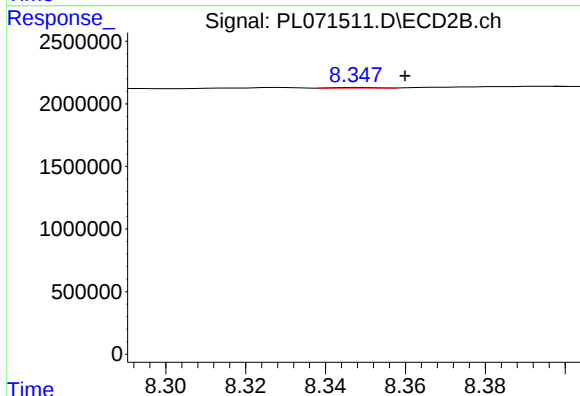


#9 Endosulfan I

R.T.: 8.348 min
Delta R.T.: -0.011 min
Response: 35257
Conc: 0.03 ng/ml

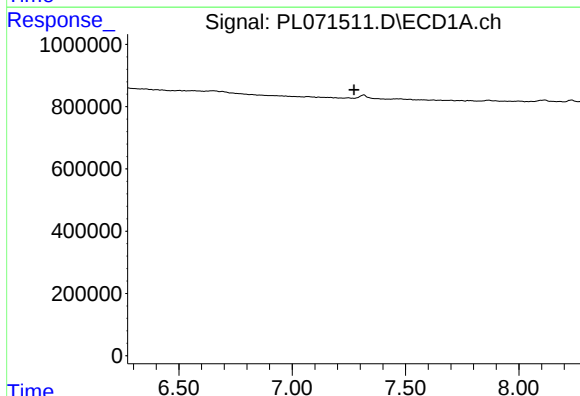


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.273 min
Response: 0
Conc: N.D.

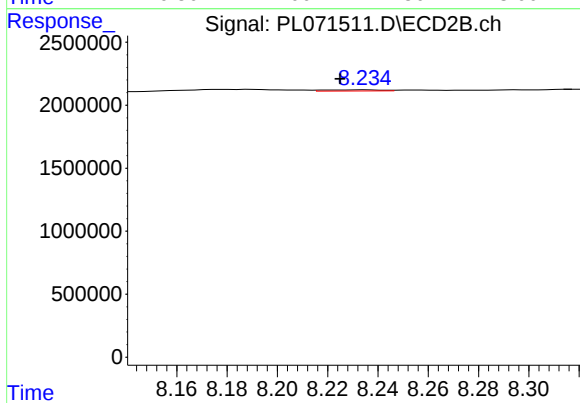

#10 gamma-Chlordane


R.T.: 8.235 min
Delta R.T.: 0.010 min
Response: 143399
Conc: 0.11 ng/ml

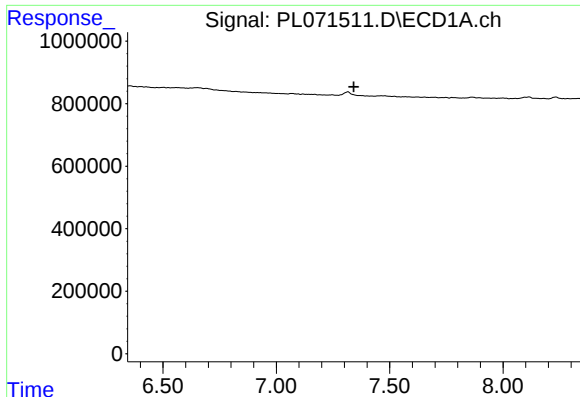

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

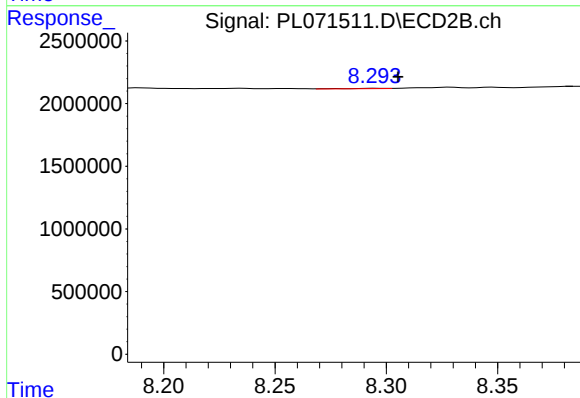


#11 alpha-Chlordane

R.T.: 8.295 min
Delta R.T.: -0.011 min
Response: 29606
Conc: 0.02 ng/ml

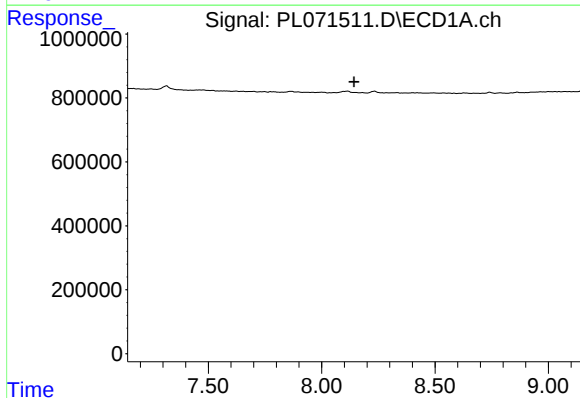


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.143 min
Response: 0
Conc: N.D.

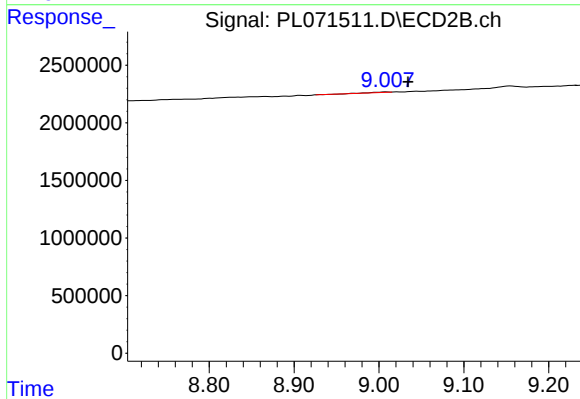

#16 4,4'-DDD


R.T.: 9.008 min
Delta R.T.: -0.026 min
Response: 25240
Conc: 0.03 ng/ml

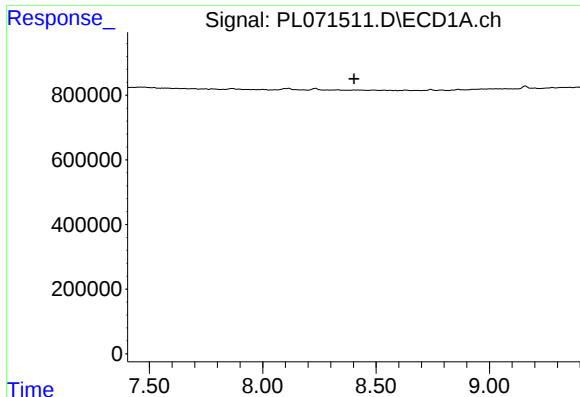

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.403 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

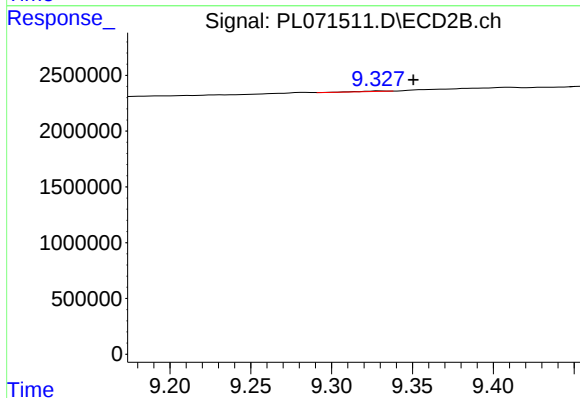


#17 4,4'-DDT

R.T.: 9.330 min
Delta R.T.: -0.021 min
Response: 65206
Conc: 0.07 ng/ml

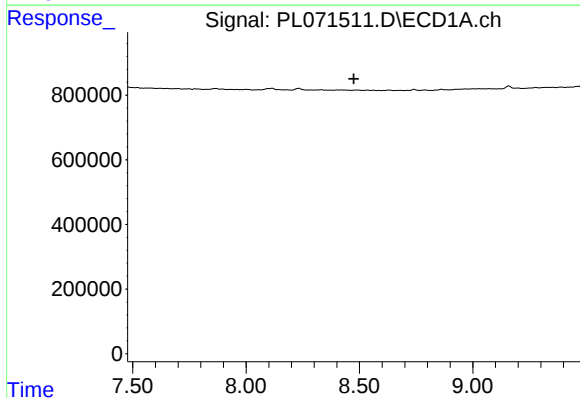


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.476 min
Response: 0
Conc: N.D.

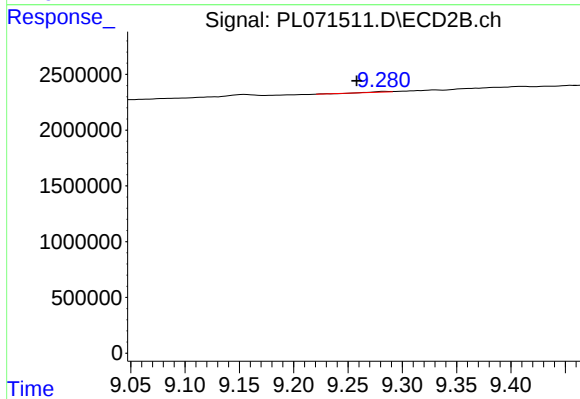

#18 Endrin aldehyde


R.T.: 9.284 min
Delta R.T.: 0.026 min
Response: 27396
Conc: 0.04 ng/ml

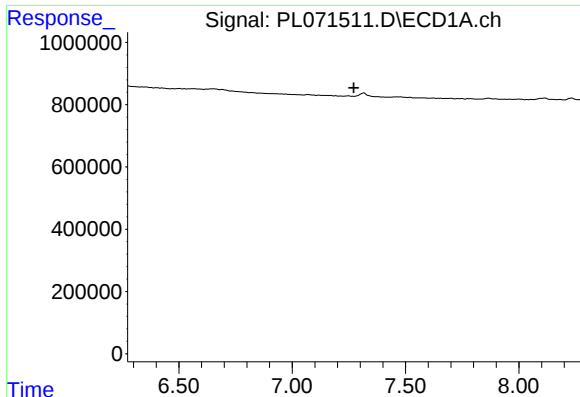

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.272 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

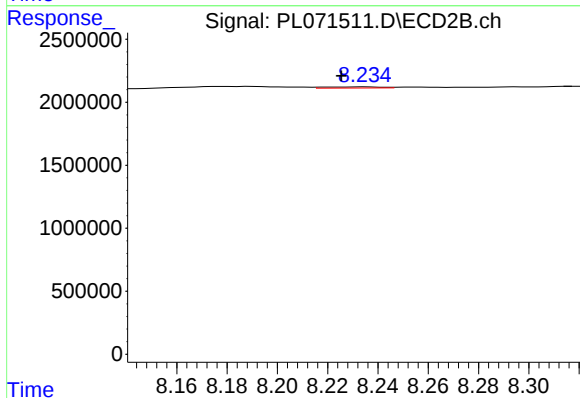


#25 Chlordane-3

R.T.: 8.235 min
Delta R.T.: 0.010 min
Response: 143399
Conc: 0.82 ng/ml

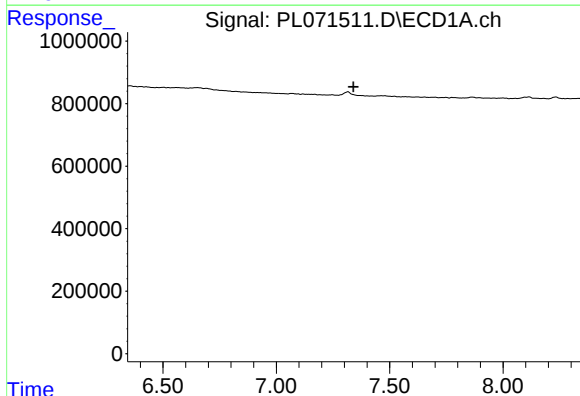


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.340 min
Response: 0
Conc: N.D.

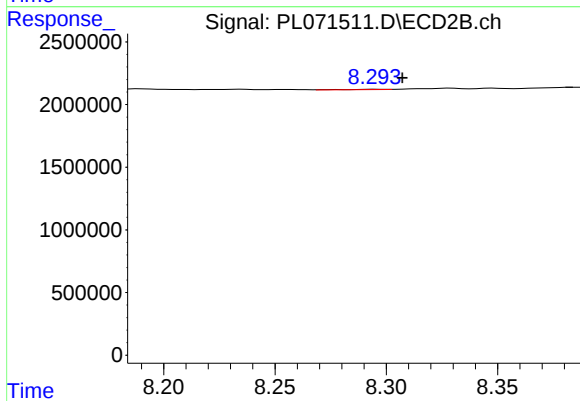

#26 Chlordane-4


R.T.: 8.295 min
Delta R.T.: -0.013 min
Response: 29606
Conc: 0.14 ng/ml

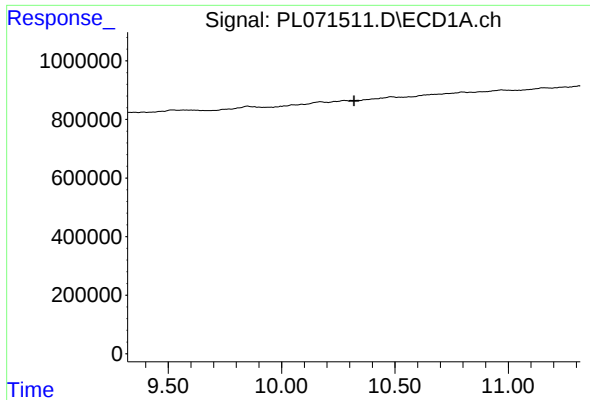

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 10.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

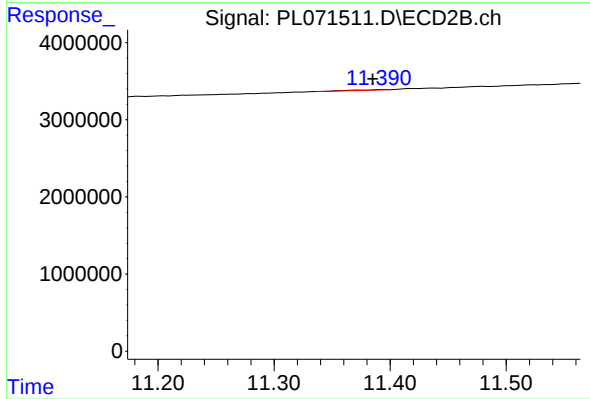

#28 Decachlorobiphenyl

R.T.: 11.393 min
Delta R.T.: 0.008 min
Response: 117258
Conc: 0.11 ng/ml