

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121723\
 Data File : PL087202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2023 10:36
 Operator : AR\AJ
 Sample : 05827-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RT-SB-08-15.5-16.5

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/18/2023
 Supervised By :Ankita Jodhani 12/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:26:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.426	2.683	57514137	24394366	15.282m	14.492
2) SA Decachlor...	8.984	7.874	36863603	16146737	10.811	9.560

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121723\
Data File : PL087202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2023 10:36
Operator : AR\AJ
Sample : 05827-08
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RT-SB-08-15.5-16.5


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/18/2023
Supervised By : Ankita Jodhani 12/18/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:26:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

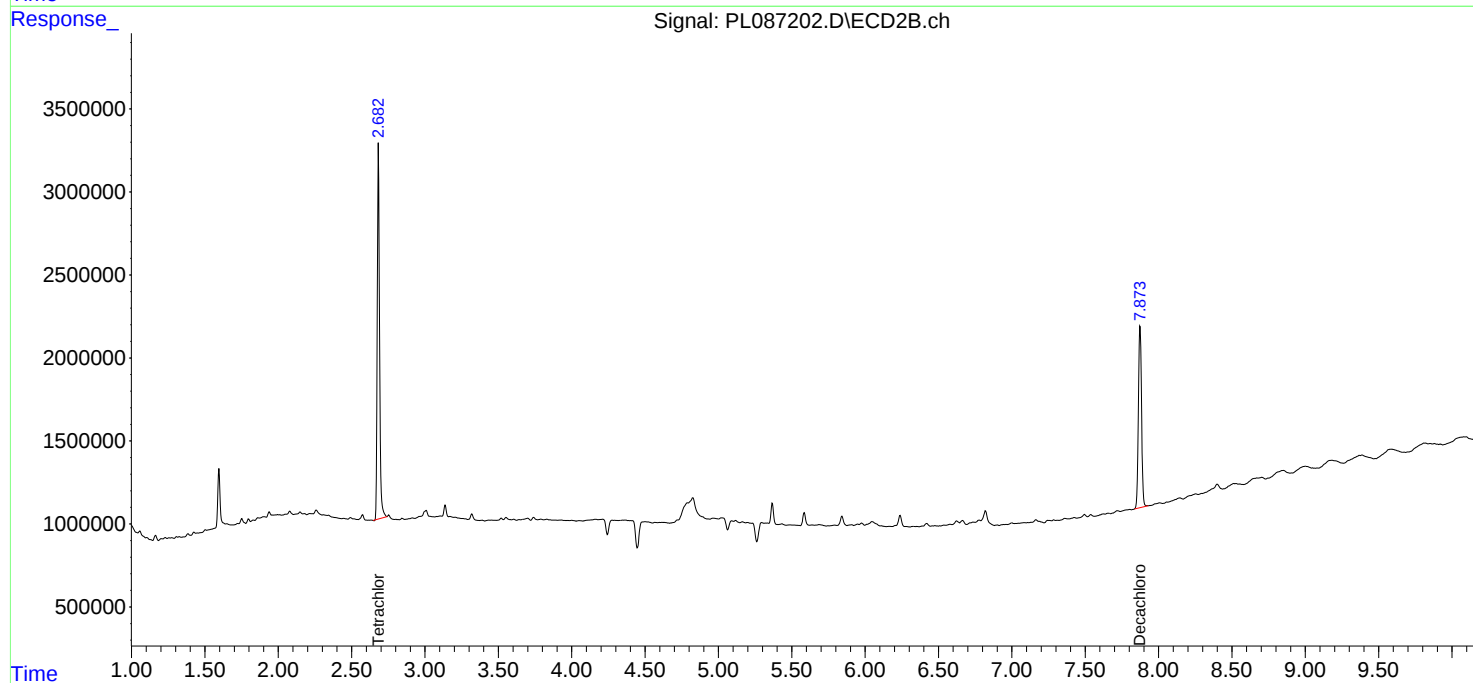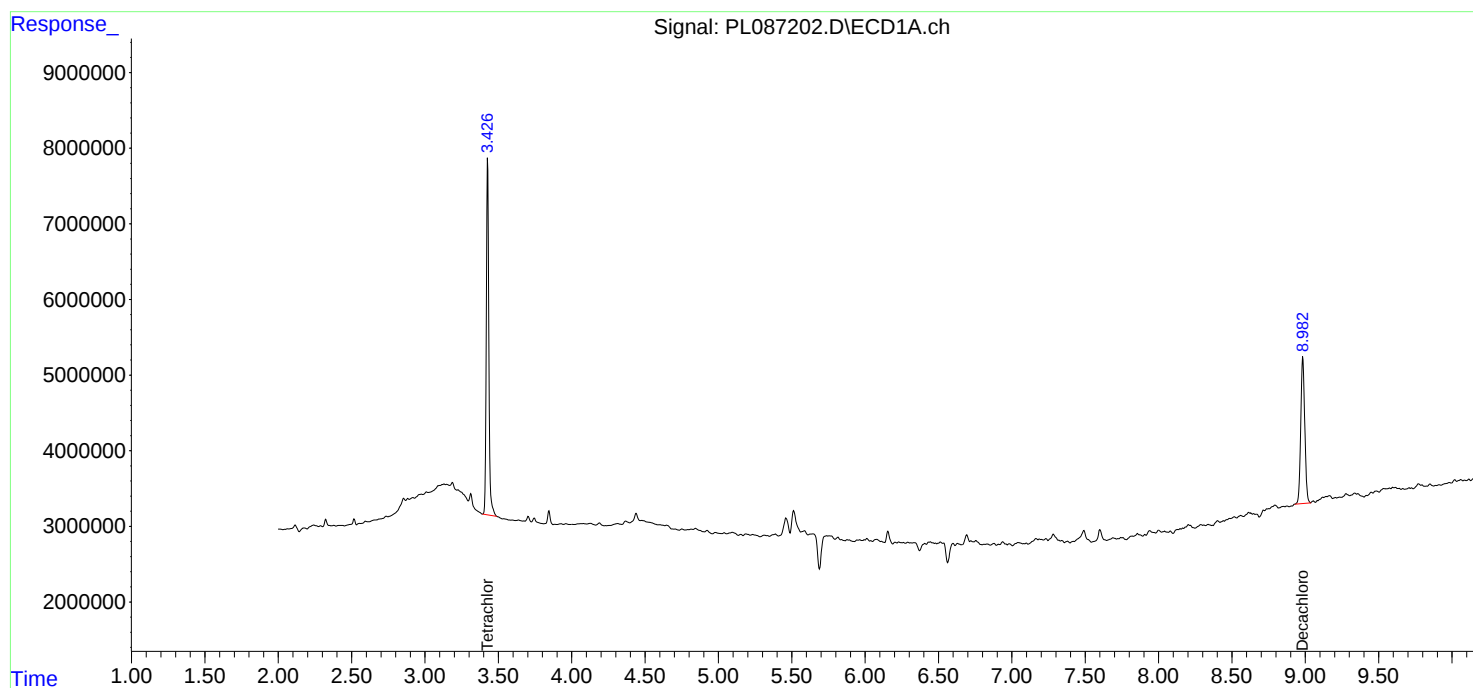

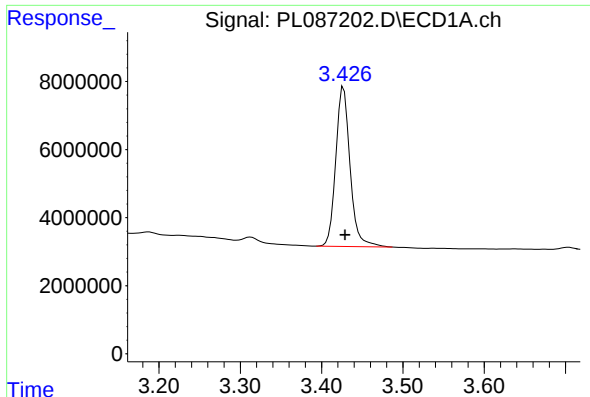


#1 Tetrachloro-m-xylene

R.T.: 3.426 min
Delta R.T.: -0.003 min
Response: 57514137
Conc: 15.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-SB-08-15.5-16.5


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/18/2023
Supervised By :Ankita Jodhani 12/18/2023

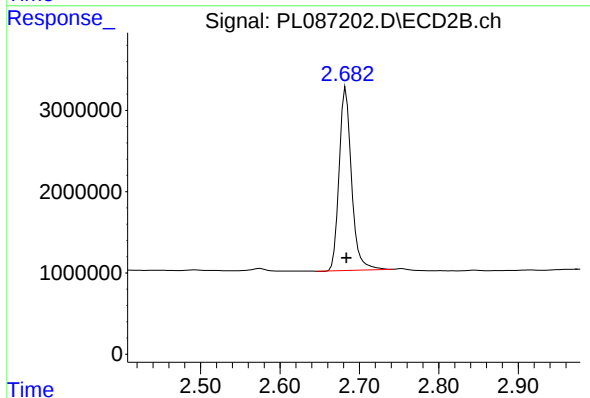


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: 0.000 min
Response: 24394366
Conc: 14.49 ng/ml

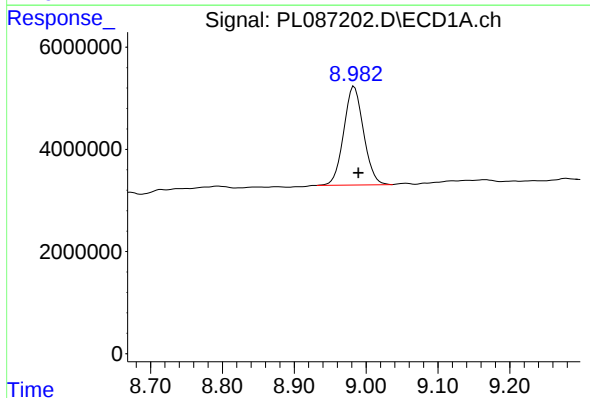

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: -0.006 min
Response: 36863603
Conc: 10.81 ng/ml

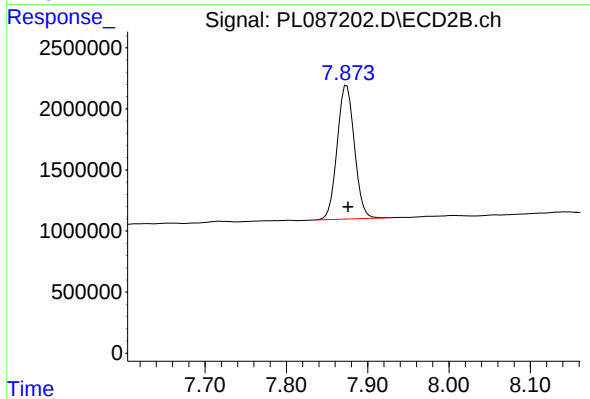

#28 Decachlorobiphenyl

R.T.: 7.874 min
Delta R.T.: -0.001 min
Response: 16146737
Conc: 9.56 ng/ml