

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121723\
 Data File : PL087220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2023 14:53
 Operator : AR\AJ
 Sample : 05831-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-20017

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/18/2023
 Supervised By :Ankita Jodhani 12/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:30:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.446f	2.681	30123411	13226109	8.004	7.857m
28) SA Decachlor...	9.004	7.874	28642341	12384743	8.400m	7.333

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121723\
Data File : PL087220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2023 14:53
Operator : AR\AJ
Sample : 05831-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT-20017


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/18/2023
Supervised By : Ankita Jodhani 12/18/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:30:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

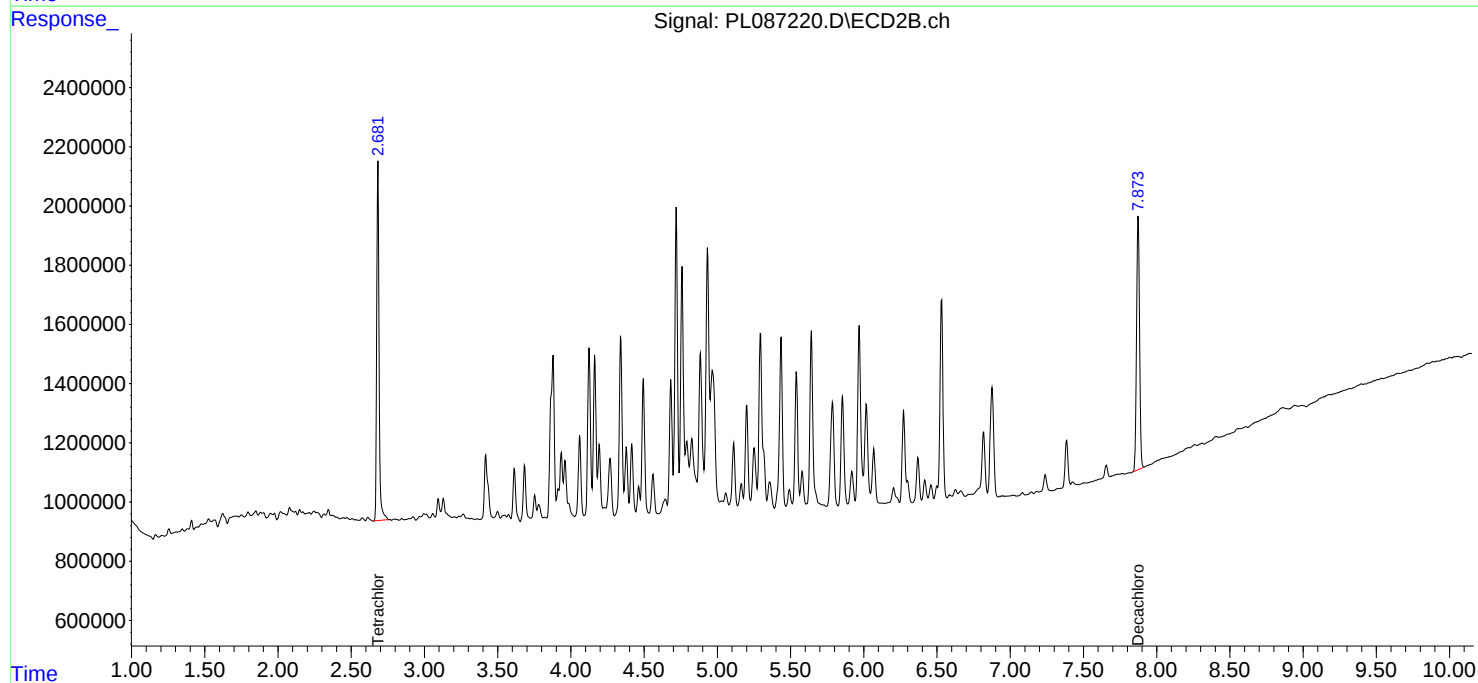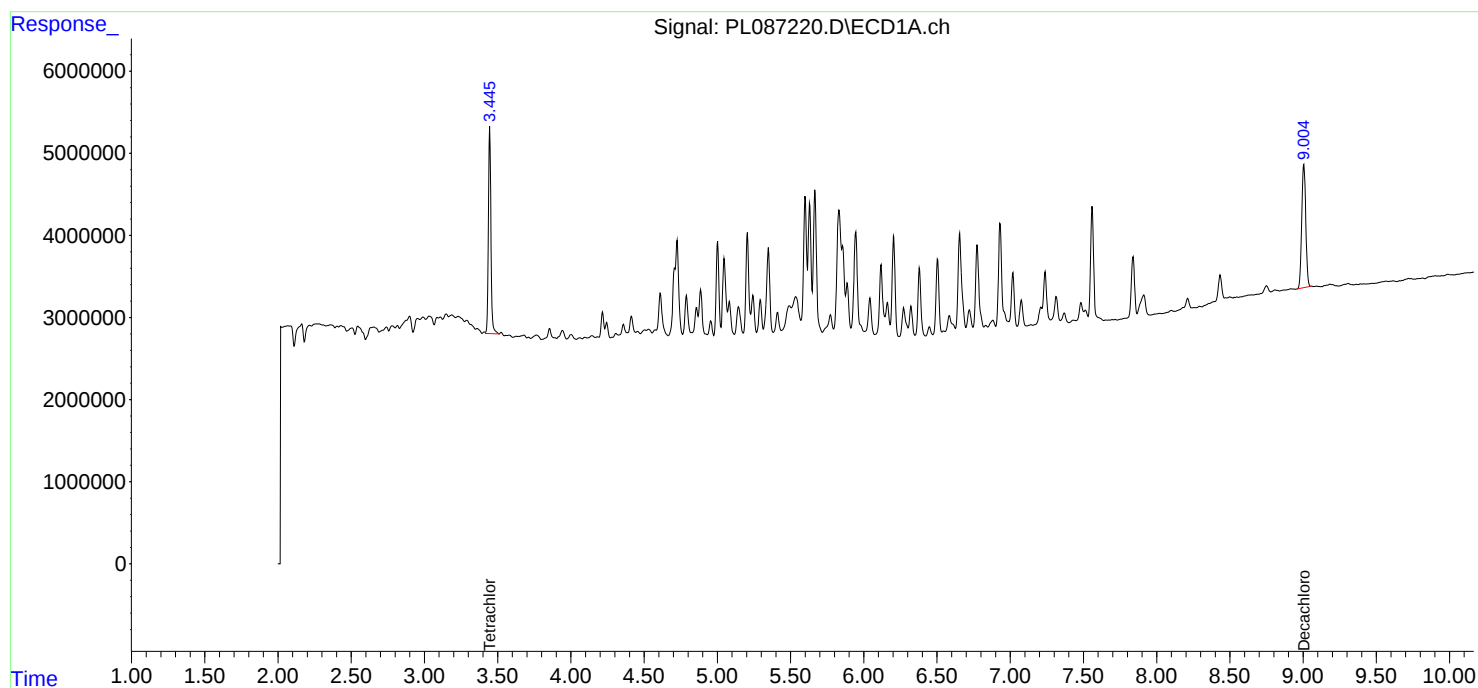

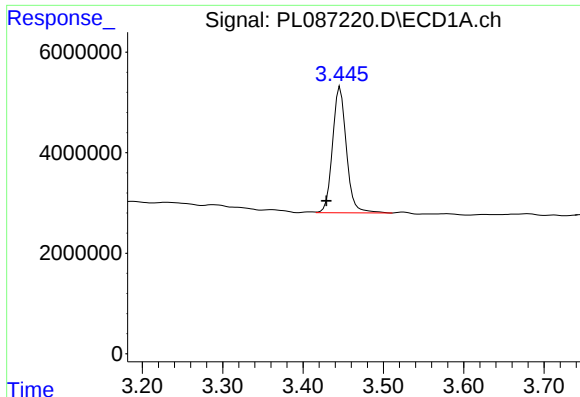


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.017 min
Response: 30123411
Conc: 8.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-20017


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/18/2023
Supervised By :Ankita Jodhani 12/18/2023

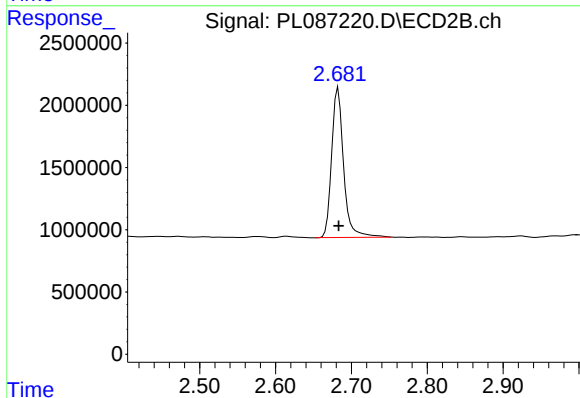


#1 Tetrachloro-m-xylene

R.T.: 2.681 min
Delta R.T.: -0.002 min
Response: 13226109
Conc: 7.86 ng/ml m

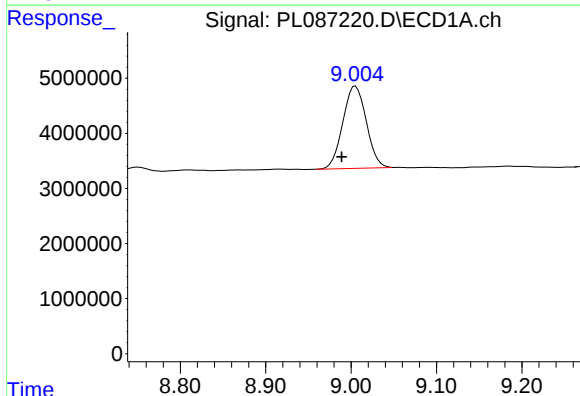

#28 Decachlorobiphenyl

R.T.: 9.004 min
Delta R.T.: 0.015 min
Response: 28642341
Conc: 8.40 ng/ml m

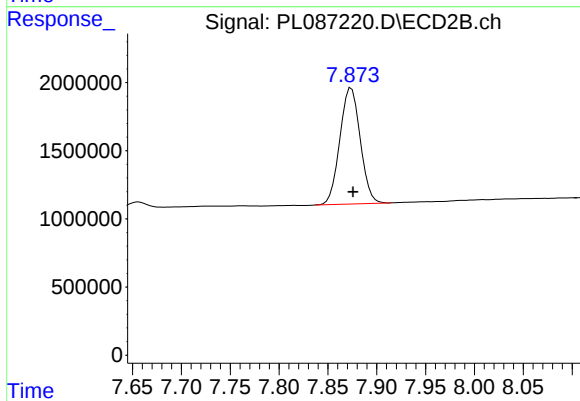

#28 Decachlorobiphenyl

R.T.: 7.874 min
Delta R.T.: -0.002 min
Response: 12384743
Conc: 7.33 ng/ml