

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121724\
 Data File : PL093401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2024 13:05
 Operator : AR\AJ
 Sample : P5301-01 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-01-121624

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/18/2024
 Supervised By : Ankita Jodhani 12/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 23:45:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 15:18:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.537	2.776	5229948	6077035	2.012m	2.107
28) SA Decachlor...	9.055	7.912	3816003	5488895	2.195	1.922

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121724\
Data File : PL093401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2024 13:05
Operator : AR\AJ
Sample : P5301-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HR-01-121624


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/18/2024
Supervised By : Ankita Jodhani 12/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 23:45:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 15:18:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

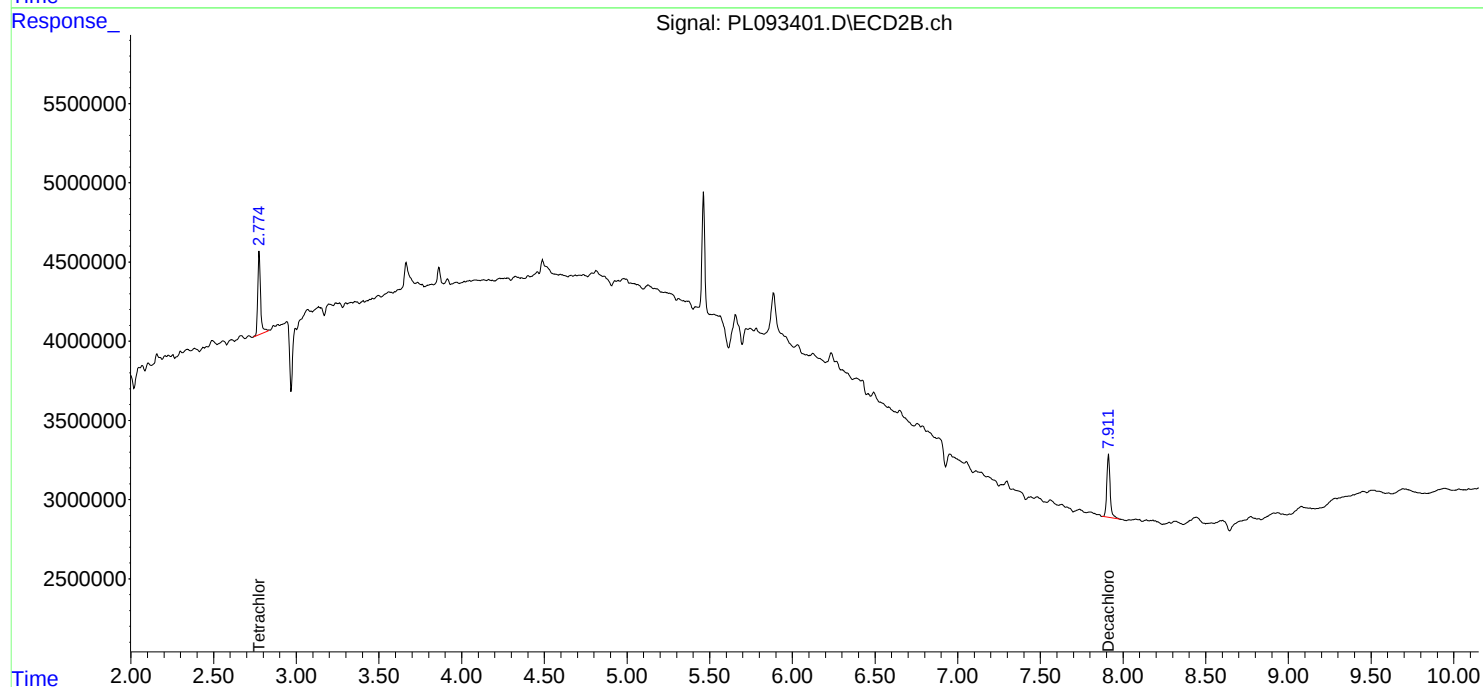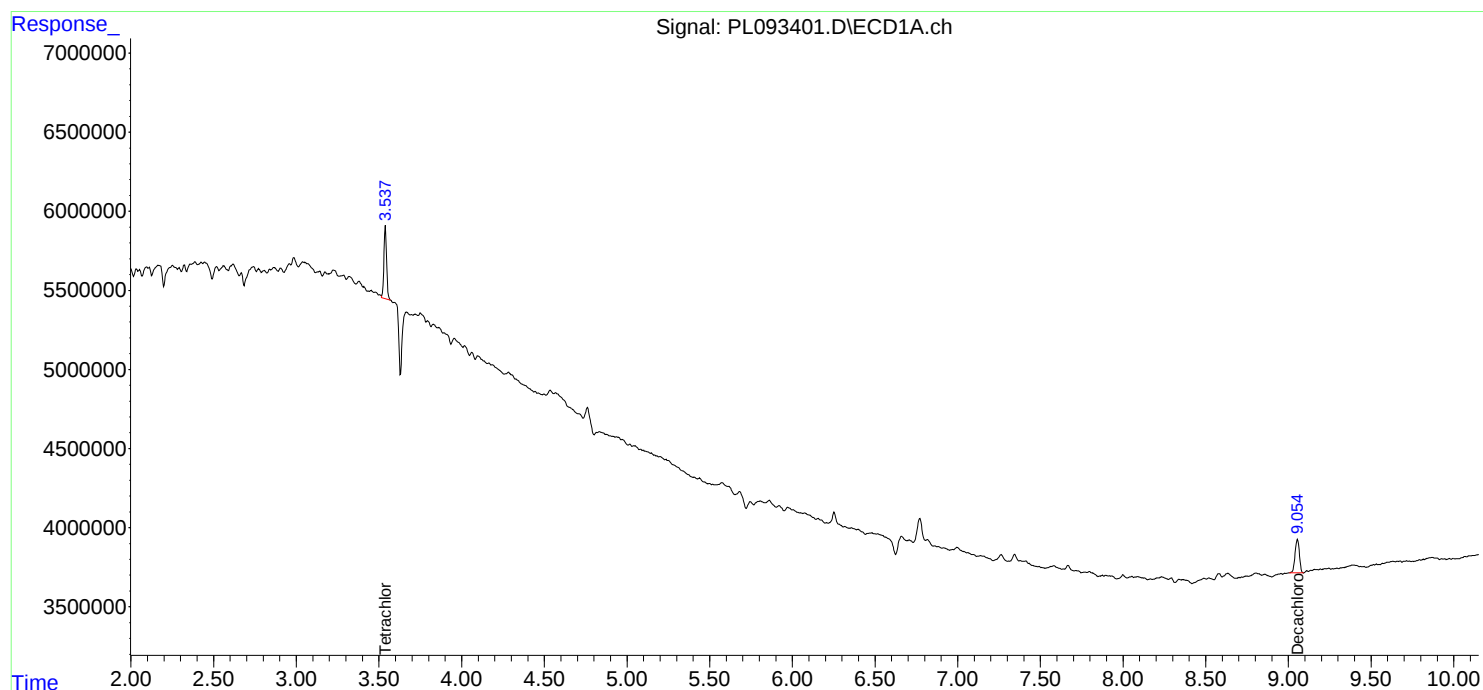

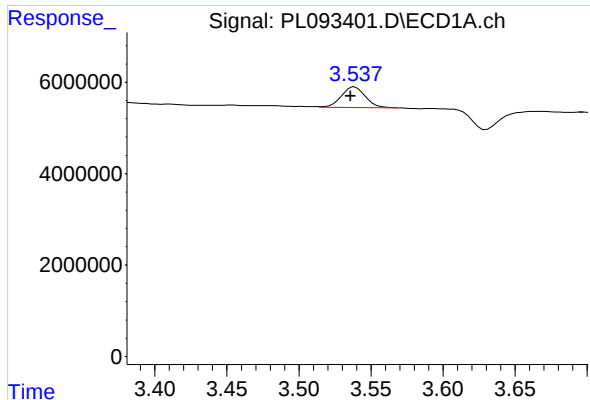


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.001 min
Response: 5229948
Conc: 2.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-121624


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/18/2024
Supervised By :Ankita Jodhani 12/18/2024

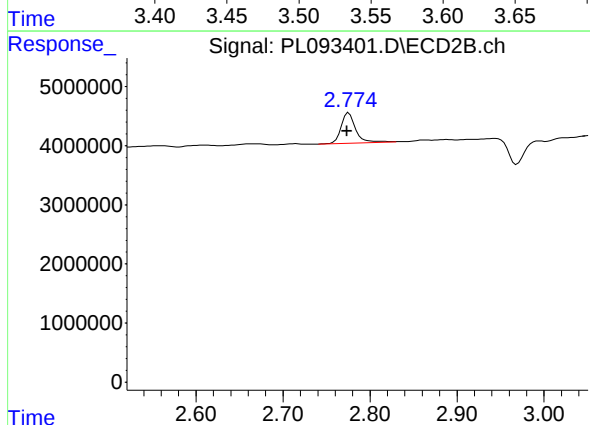


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.002 min
Response: 6077035
Conc: 2.11 ng/ml

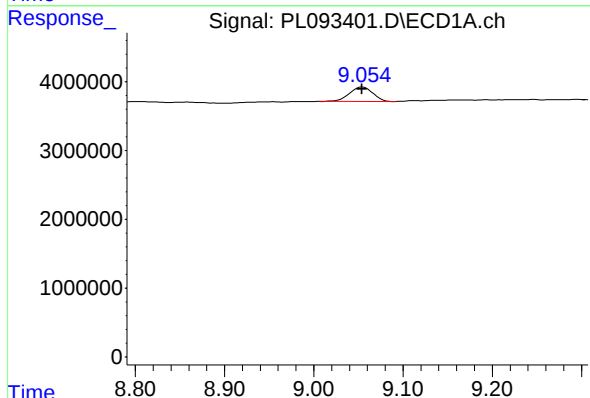

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 3816003
Conc: 2.19 ng/ml

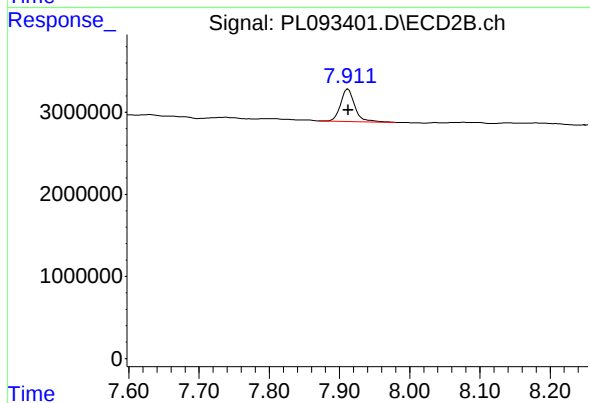

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 5488895
Conc: 1.92 ng/ml