

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121818\
 Data File : PL043264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2018 21:54
 Operator : AJ\SJ
 Sample : PB115795BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:19:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.099	126.5E6	65518618	20.623	22.106
28)	SA Decachlor...	8.199	9.228	140.7E6	59798776	21.543	22.925
Target Compounds							
6)	B beta-BHC	4.396f	0.000	4612476	0	1.251	N.D. #
7)	B delta-BHC	0.000	5.164	0	13936569	N.D.	3.243 #
8)	B Heptachlo...	0.000	5.998	0	9628777	N.D.	2.539 #
15)	B Endosulfa...	6.225f	0.000	2376983	0	0.357	N.D. #
23)	Chlordane-1	4.360	5.164	1319689	13936569	4.911	98.608 #
27)	Chlordane-5	6.225	0.000	2376983	0	9.910	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121818\
Data File : PL043264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2018 21:54
Operator : AJ\SJ
Sample : PB115795BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:19:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

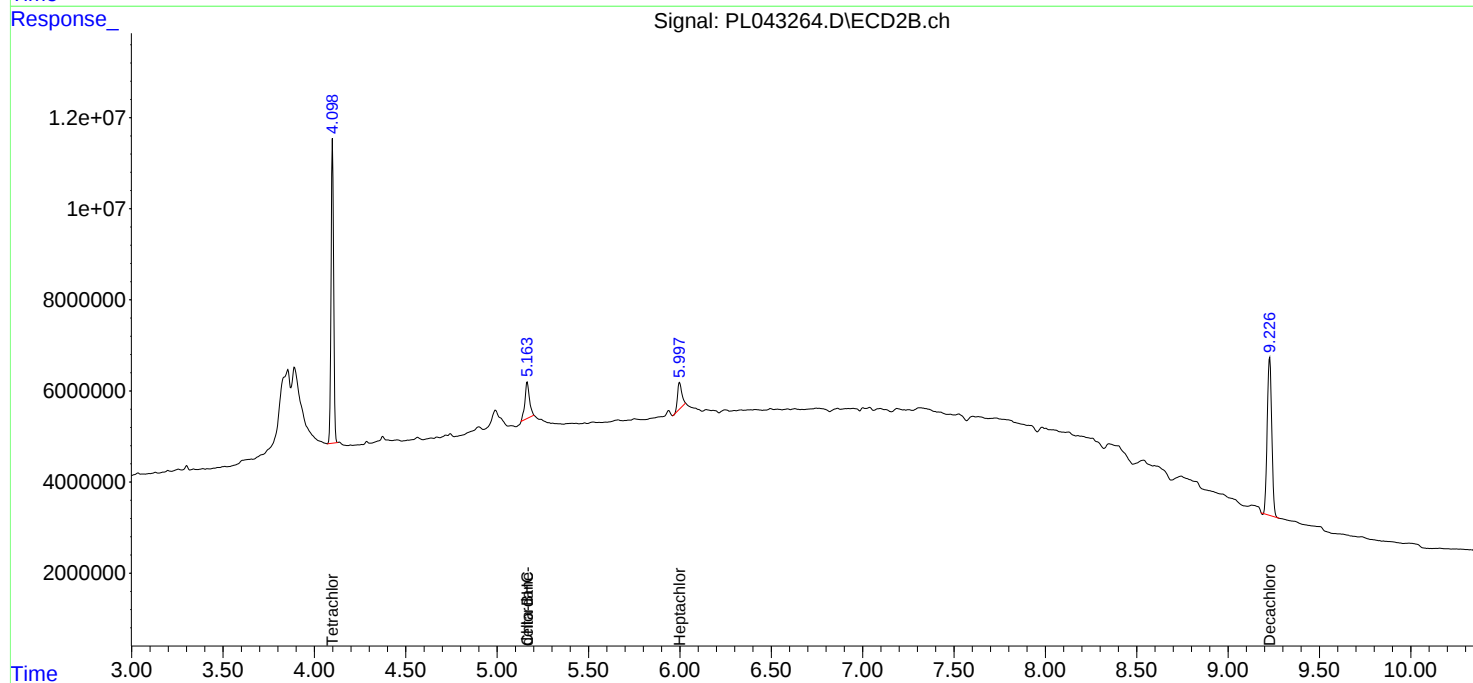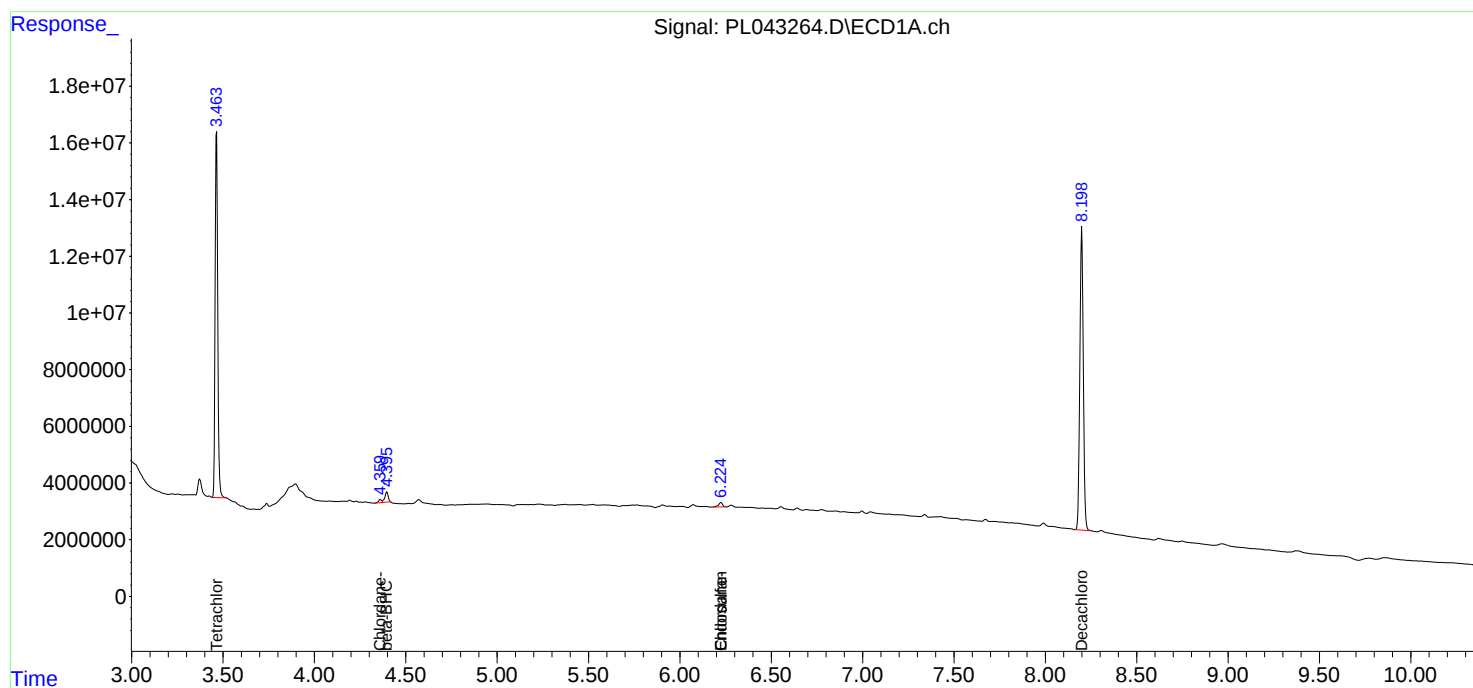


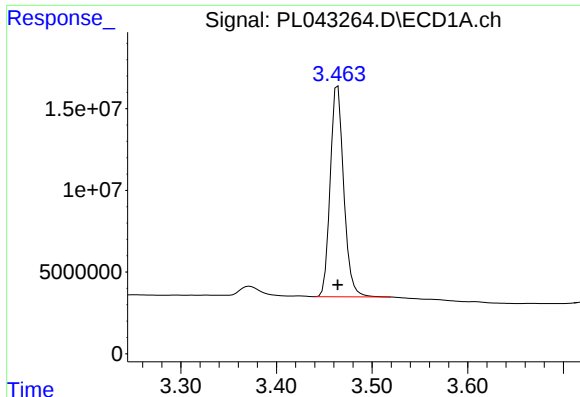

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 126478191
Conc: 20.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

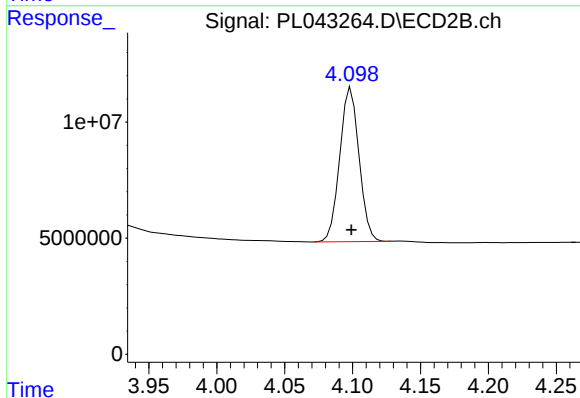


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 65518618
Conc: 22.11 ng/ml

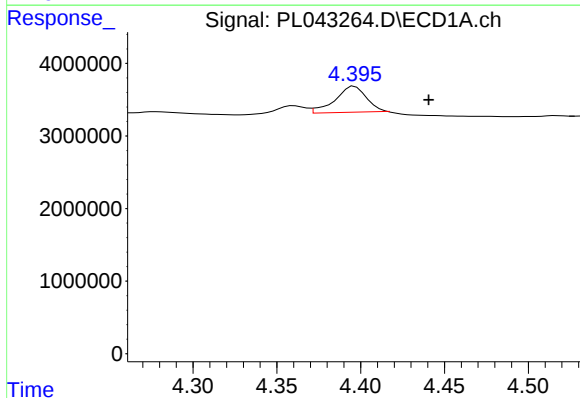


#6 beta-BHC

R.T.: 4.396 min
Delta R.T.: -0.044 min
Response: 4612476
Conc: 1.25 ng/ml

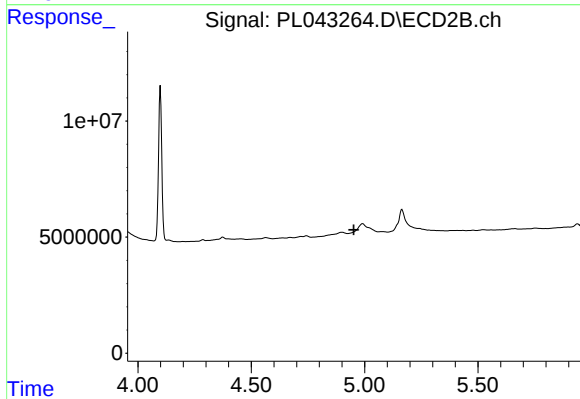

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.952 min
Response: 0
Conc: N.D.

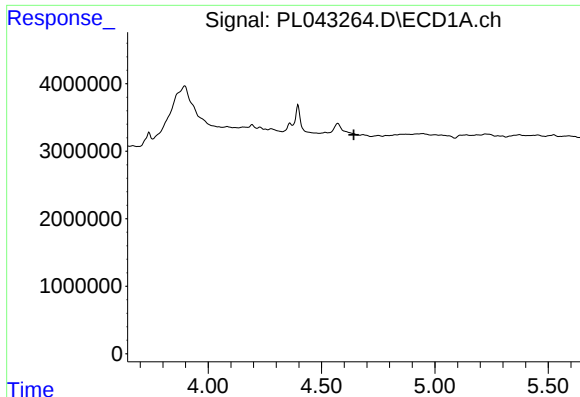

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

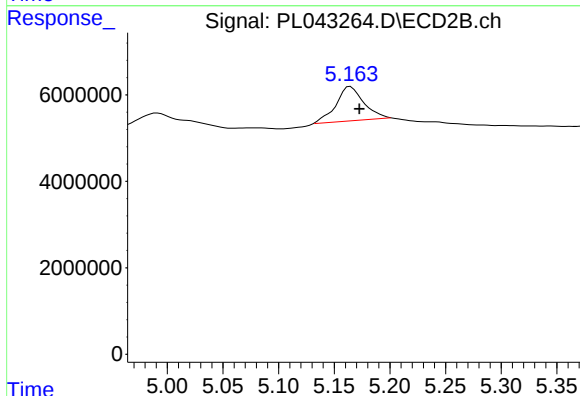


#7 delta-BHC

R.T.: 5.164 min
Delta R.T.: -0.008 min
Response: 13936569
Conc: 3.24 ng/ml

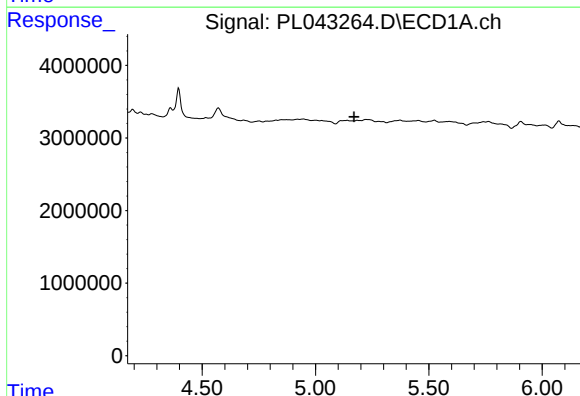


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

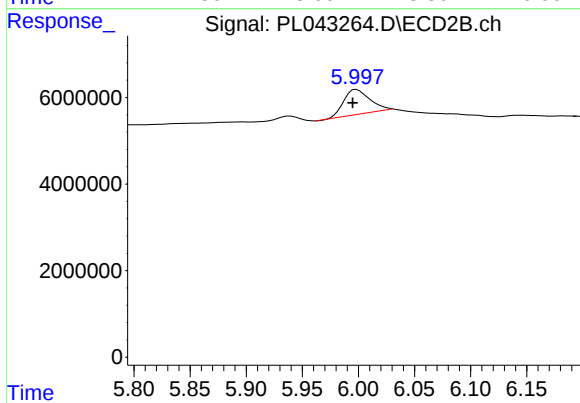

#8 Heptachlor epoxide


R.T.: 5.998 min
Delta R.T.: 0.003 min
Response: 9628777
Conc: 2.54 ng/ml

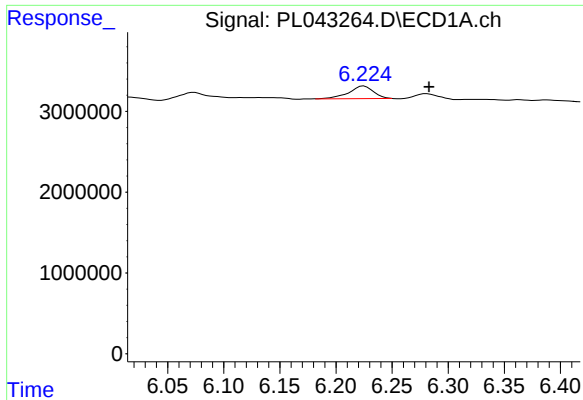

#15 Endosulfan II


R.T.: 6.225 min
Delta R.T.: -0.058 min
Response: 2376983
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

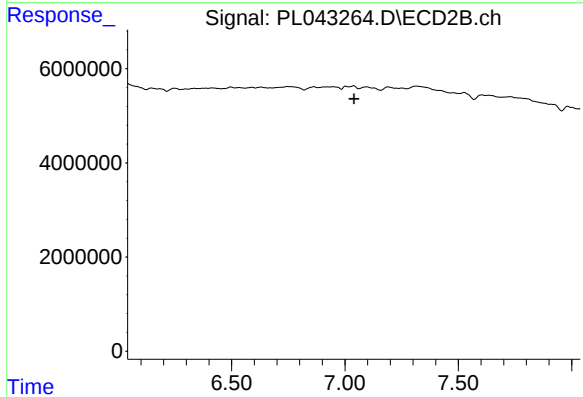


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

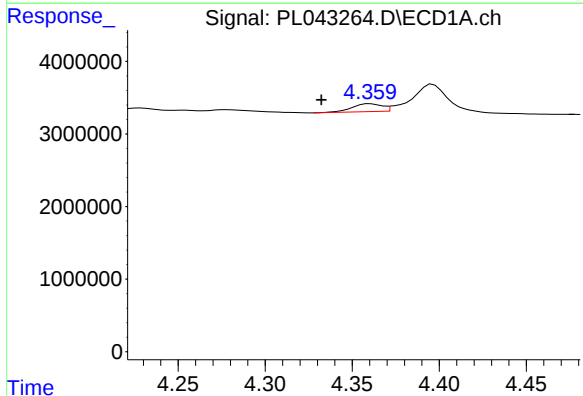


#23 Chlordane-1

R.T.: 4.360 min
Delta R.T.: 0.028 min
Response: 1319689
Conc: 4.91 ng/ml

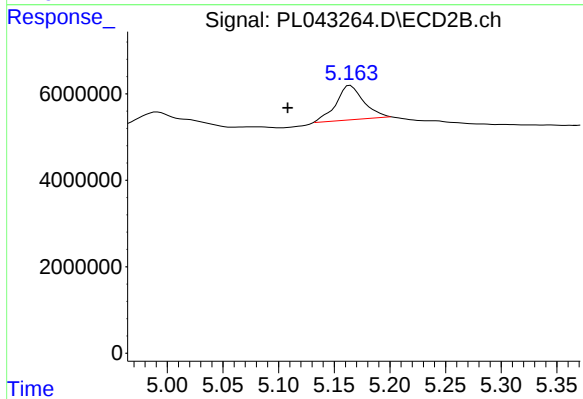

#23 Chlordane-1


R.T.: 5.164 min
Delta R.T.: 0.056 min
Response: 13936569
Conc: 98.61 ng/ml

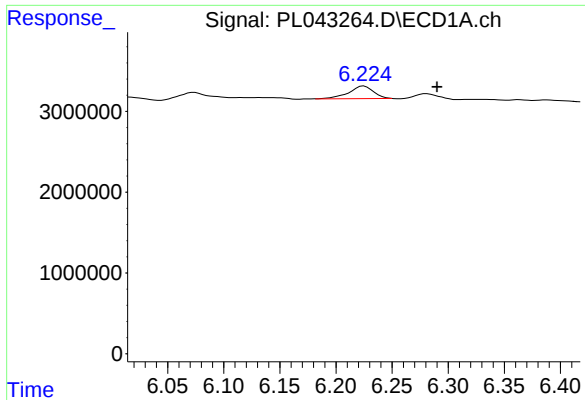

#27 Chlordane-5


R.T.: 6.225 min
Delta R.T.: -0.065 min
Response: 2376983
Conc: 9.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

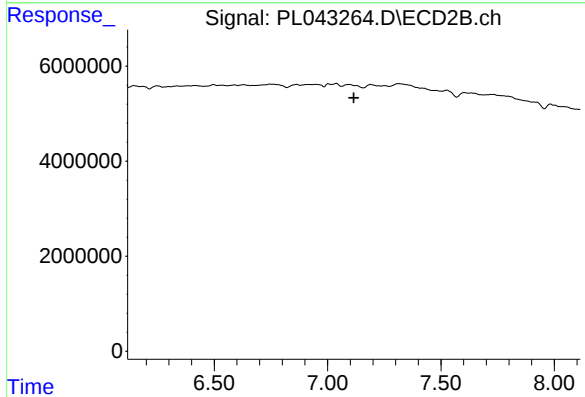


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

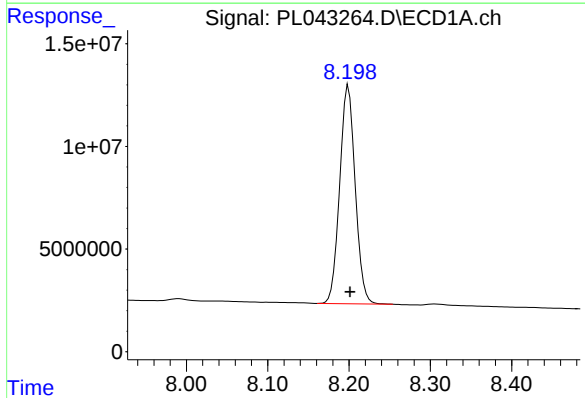

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: -0.002 min
Response: 140673293
Conc: 21.54 ng/ml

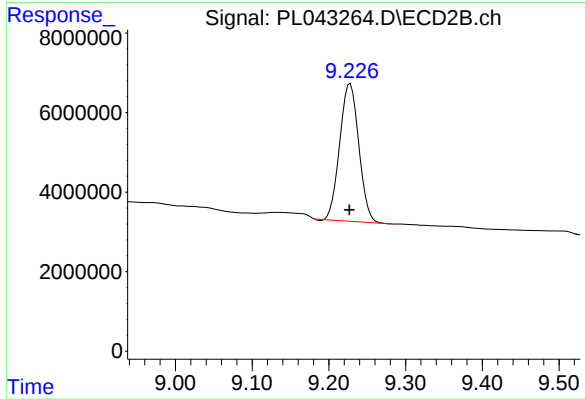

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: 0.000 min
Response: 59798776
Conc: 22.92 ng/ml