

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121818\
 Data File : PL043277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2018 00:57
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 03:11:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.099	143.6E6	71565697	23.421	24.146
28)	SA Decachlor...	8.200	9.229	140.2E6	64158301	21.463	24.596
Target Compounds							
7)	B delta-BHC	0.000	5.165	0	7272843	N.D.	1.692 #
8)	B Heptachlo...	0.000	5.996	0	12550050	N.D.	3.310 #
13)	MA Dieldrin	5.700f	0.000	1491395	0	0.192	N.D. #
14)	MA Endrin	6.019	0.000	994826	0	0.138	N.D. #
15)	B Endosulfa...	6.227f	0.000	753652	0	0.113	N.D. #
16)	A 4,4'-DDD	6.087f	0.000	992883	0	0.175	N.D. #
21)	B Endrin ke...	7.112f	0.000	2651831	0	0.367	N.D. #
23)	Chlordane-1	4.361	5.165	503395	7272843	1.873	51.459 #
24)	Chlordane-2	0.000	5.519	0	850801	N.D.	5.931 #
27)	Chlordane-5	6.227	0.000	753652	0	3.142	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121818\
Data File : PL043277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2018 00:57
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 03:11:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

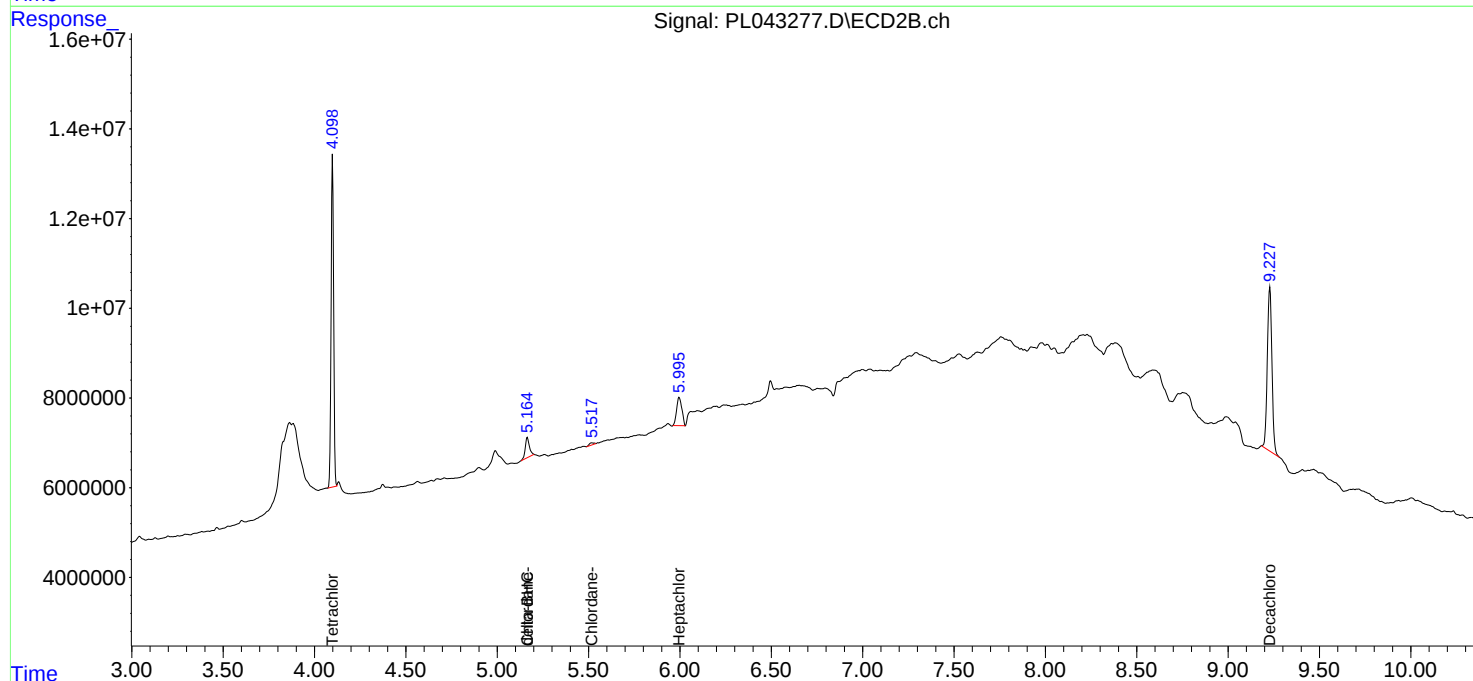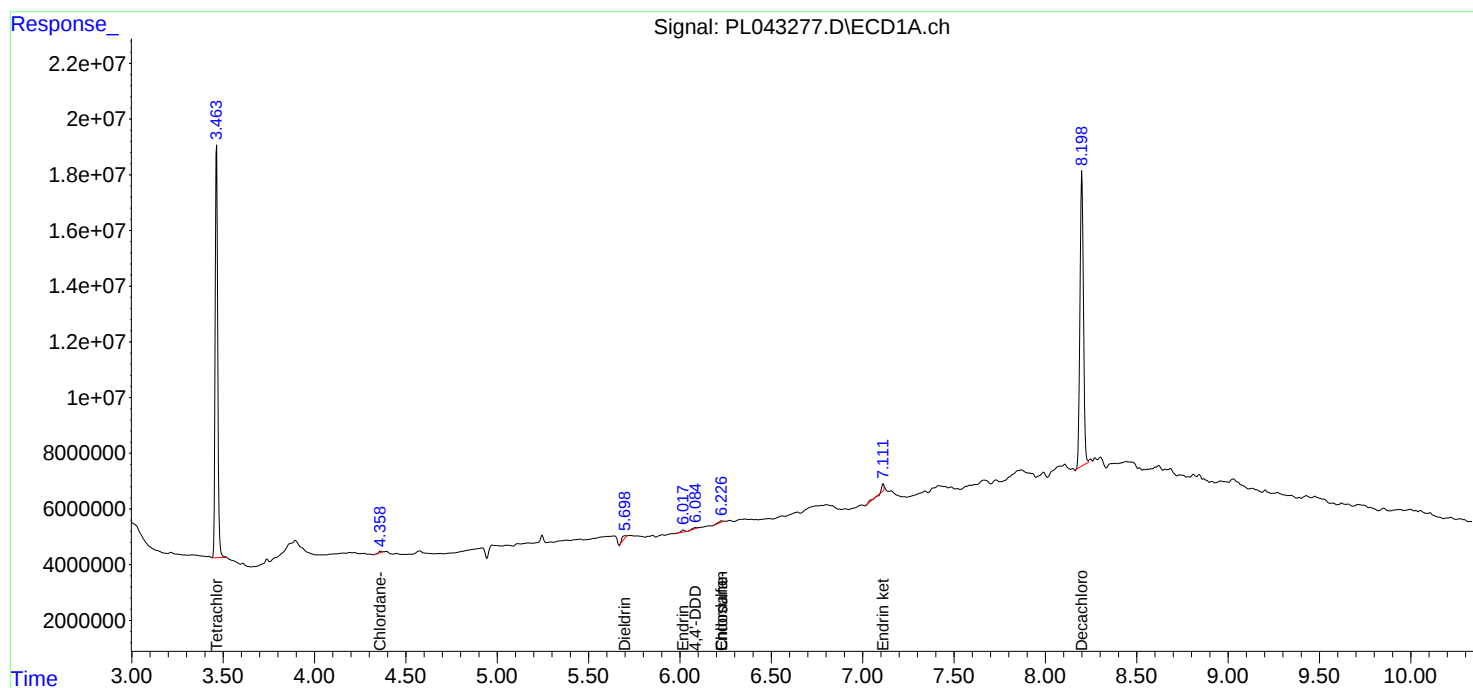


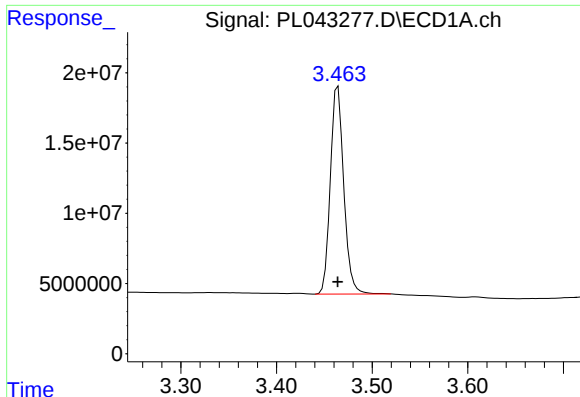

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 143635646
Conc: 23.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

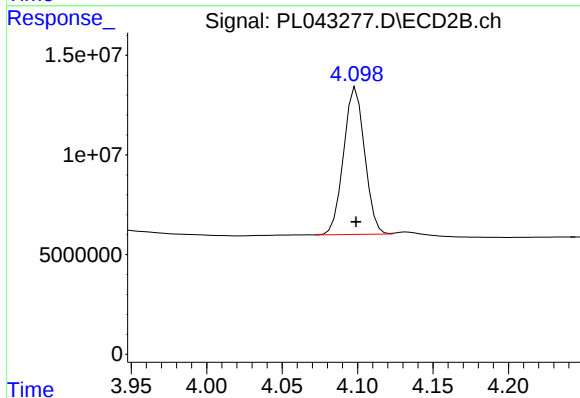


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 71565697
Conc: 24.15 ng/ml

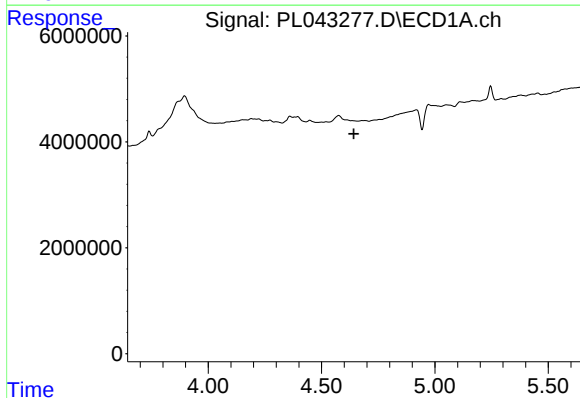


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

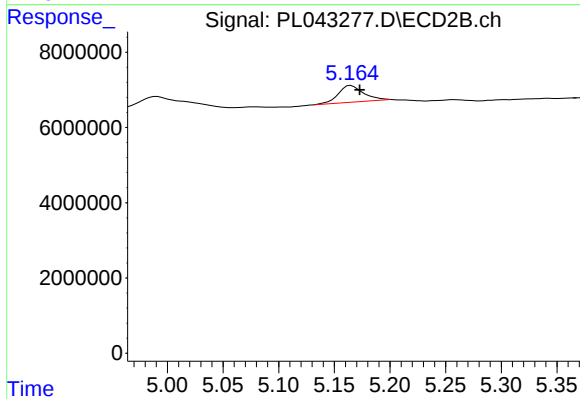

#7 delta-BHC


R.T.: 5.165 min
Delta R.T.: -0.008 min
Response: 7272843
Conc: 1.69 ng/ml

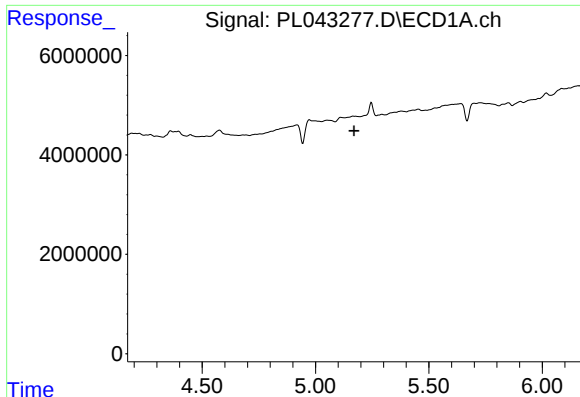

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

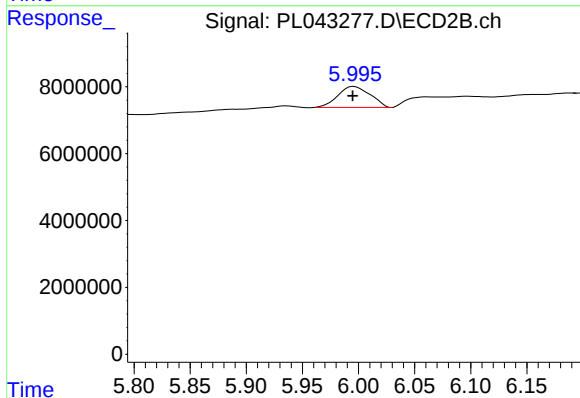


#8 Heptachlor epoxide

R.T.: 5.996 min
Delta R.T.: 0.001 min
Response: 12550050
Conc: 3.31 ng/ml

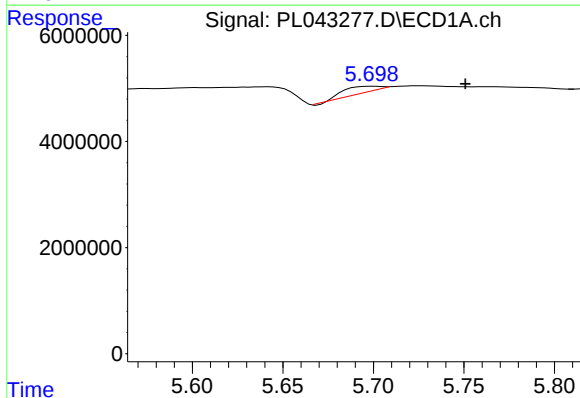


#13 Dieldrin

R.T.: 5.700 min
Delta R.T.: -0.051 min
Response: 1491395
Conc: 0.19 ng/ml

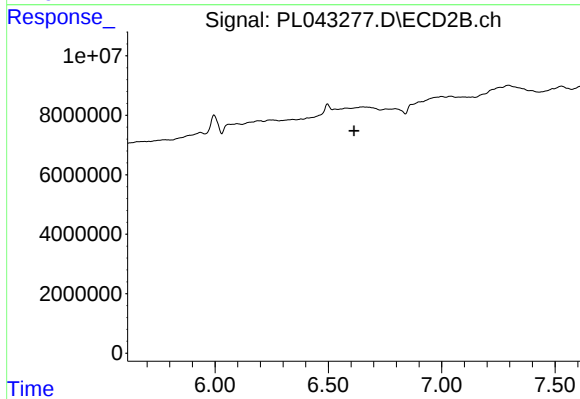

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.613 min
Response: 0
Conc: N.D.

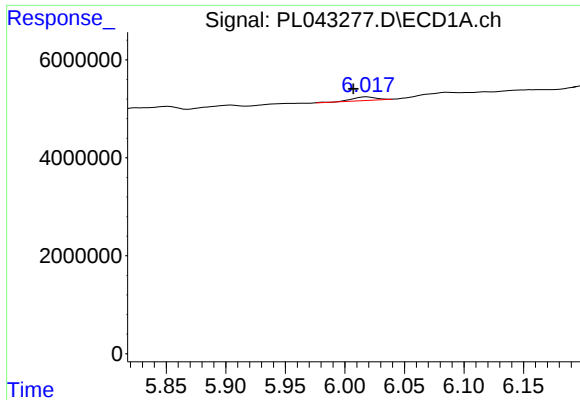

#14 Endrin


R.T.: 6.019 min
Delta R.T.: 0.012 min
Response: 994826
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

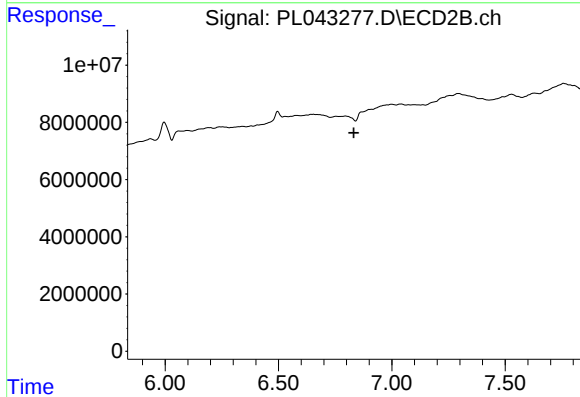


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

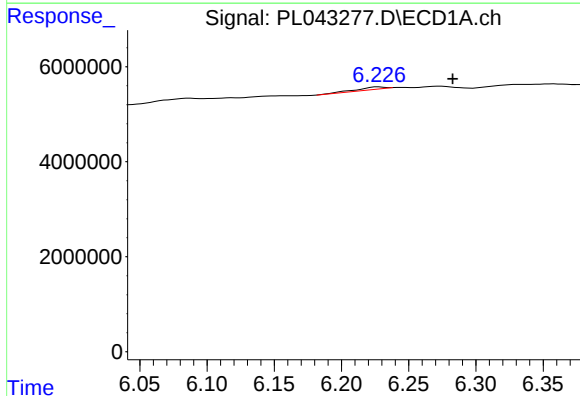


#15 Endosulfan II

R.T.: 6.227 min
Delta R.T.: -0.055 min
Response: 753652
Conc: 0.11 ng/ml

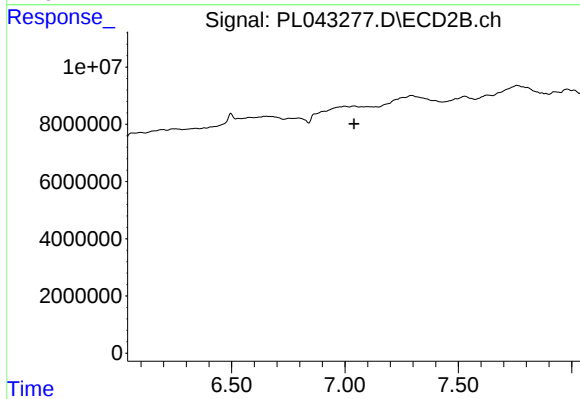

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

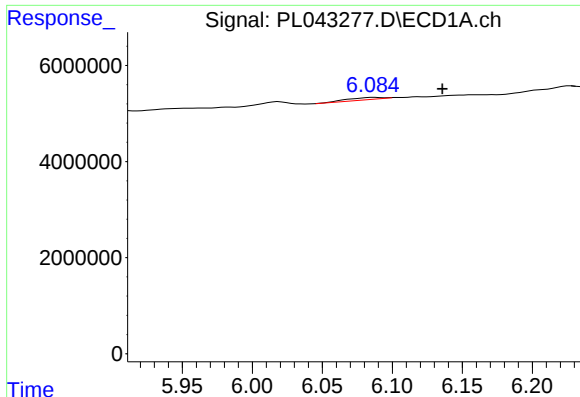

#16 4,4'-DDD


R.T.: 6.087 min
Delta R.T.: -0.049 min
Response: 992883
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

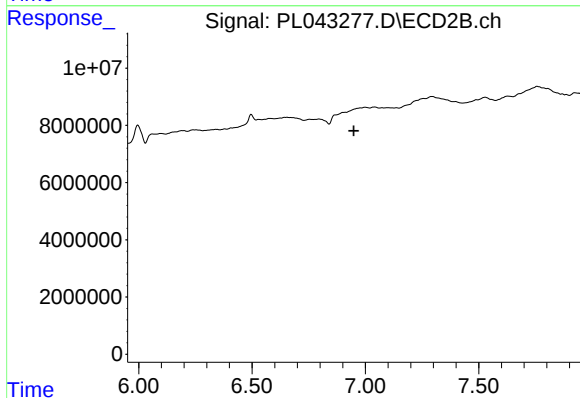


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

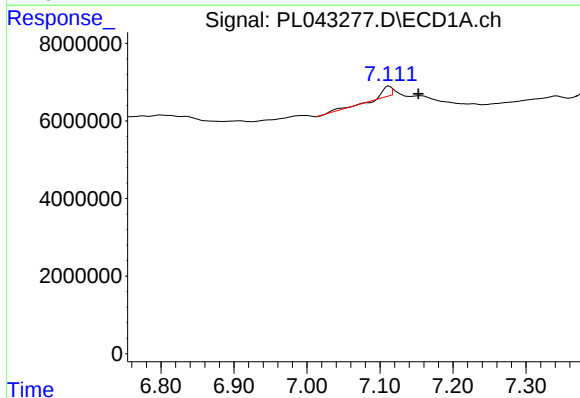


#21 Endrin ketone

R.T.: 7.112 min
Delta R.T.: -0.040 min
Response: 2651831
Conc: 0.37 ng/ml

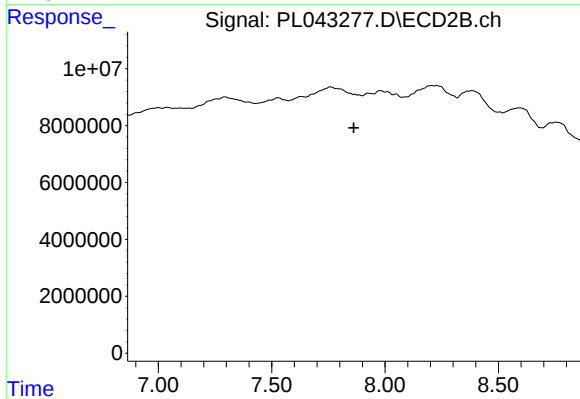

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.863 min
Response: 0
Conc: N.D.

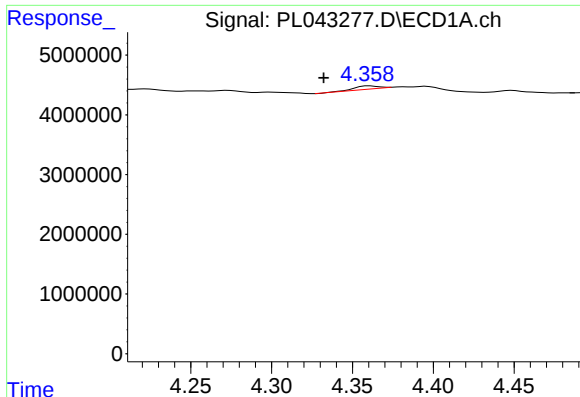

#23 Chlordane-1


R.T.: 4.361 min
Delta R.T.: 0.028 min
Response: 503395
Conc: 1.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

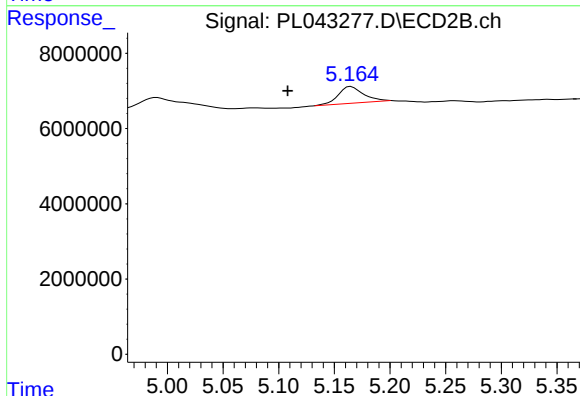


#23 Chlordane-1

R.T.: 5.165 min
Delta R.T.: 0.057 min
Response: 7272843
Conc: 51.46 ng/ml

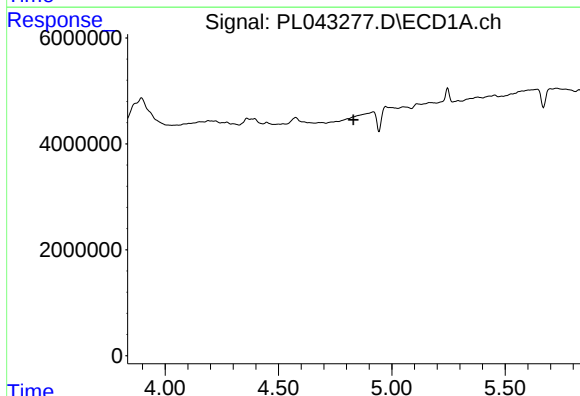


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.832 min
Response: 0
Conc: N.D.

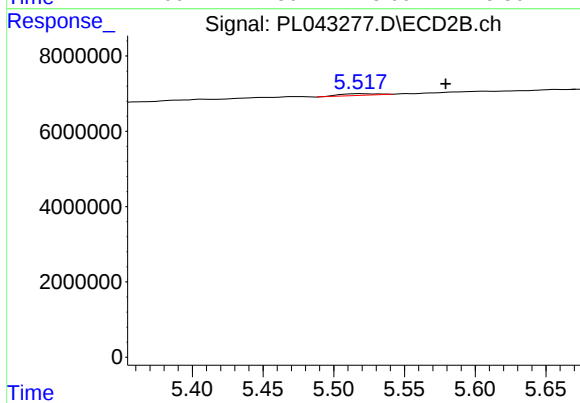

#24 Chlordane-2


R.T.: 5.519 min
Delta R.T.: -0.061 min
Response: 850801
Conc: 5.93 ng/ml

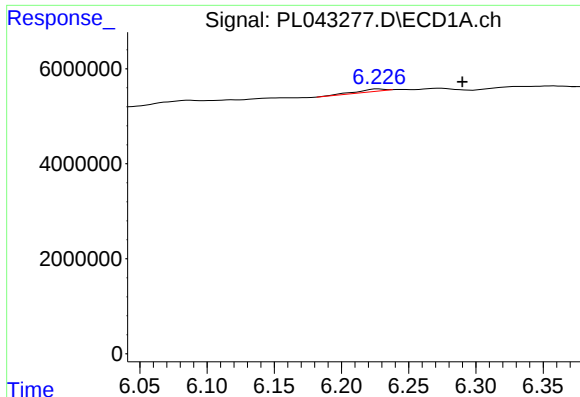

#27 Chlordane-5


R.T.: 6.227 min
Delta R.T.: -0.063 min
Response: 753652
Conc: 3.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

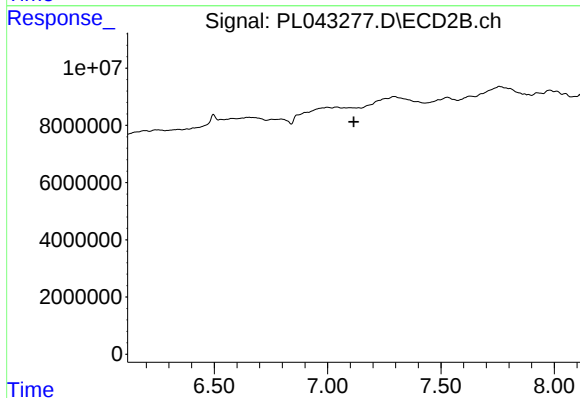


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

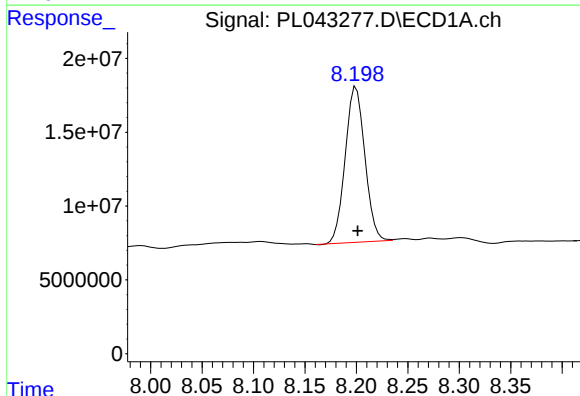

#28 Decachlorobiphenyl

R.T.: 8.200 min
Delta R.T.: -0.001 min
Response: 140150331
Conc: 21.46 ng/ml

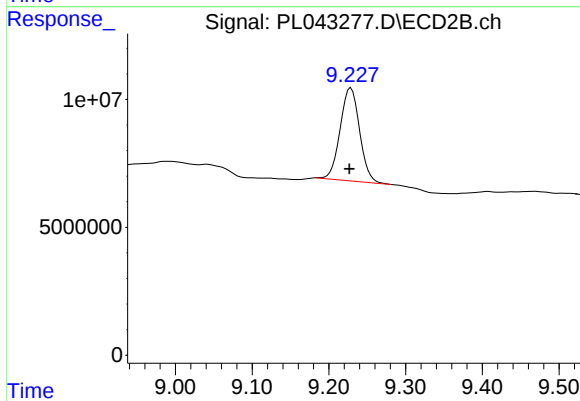

#28 Decachlorobiphenyl

R.T.: 9.229 min
Delta R.T.: 0.002 min
Response: 64158301
Conc: 24.60 ng/ml