

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
 Data File : PL055057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 09:20
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 13:36:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	4.488f	0.000	6441124	0	0.868	N.D.	#
8) B	Heptachlo...	5.271	0.000	67008792	0	4.430	N.D.	#
12) B	4,4'-DDE	5.740f	0.000	989962	0	0.074	N.D.	#
15) B	Endosulfa...	6.405f	0.000	4159299	0	0.344	N.D.	#
27)	Chlordane-5	6.405	0.000	4159299	0	11.047	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
Data File : PL055057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 09:20
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 13:36:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

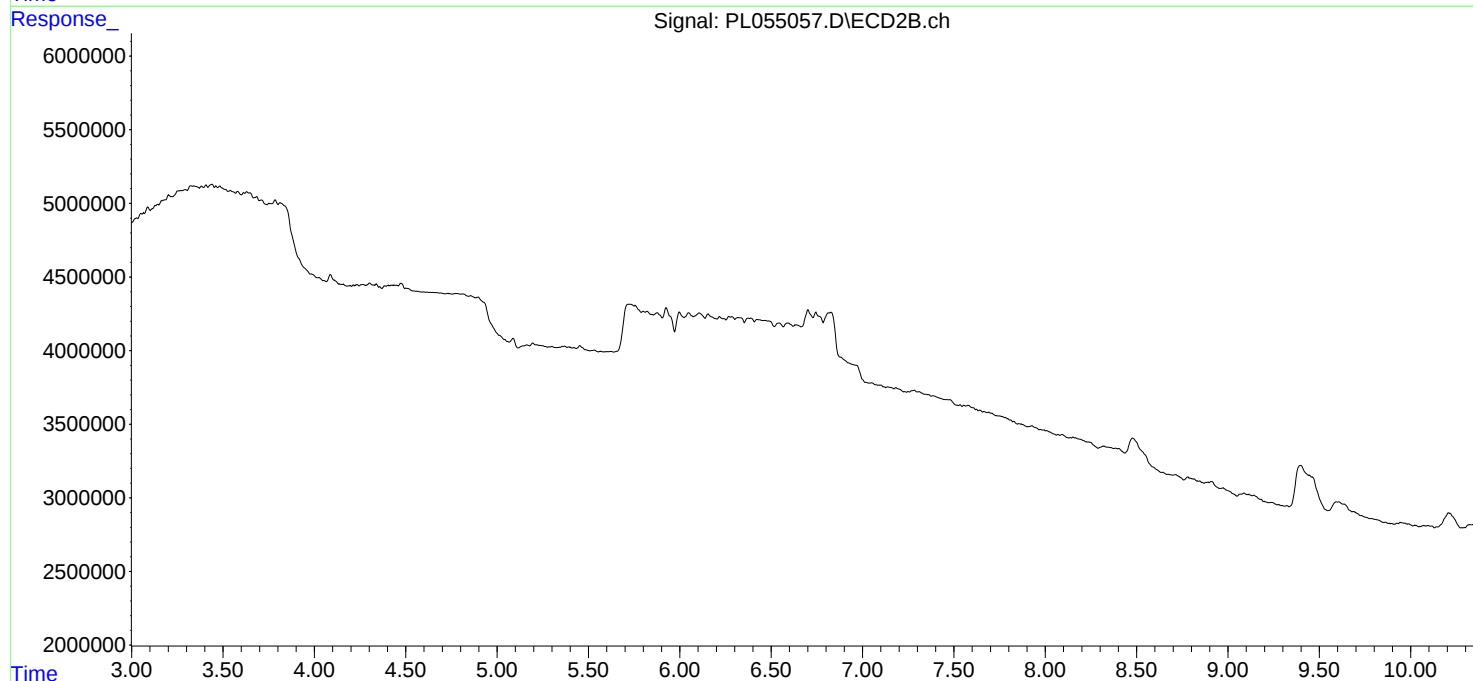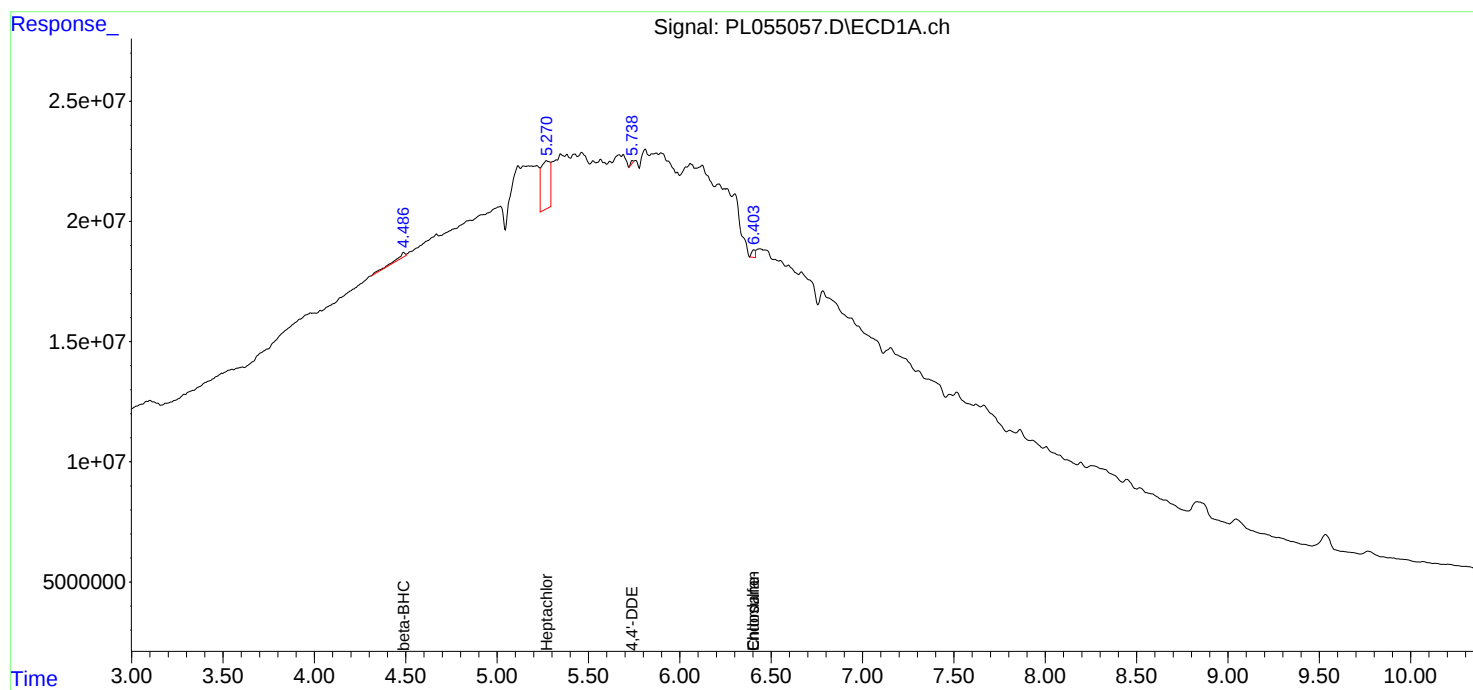


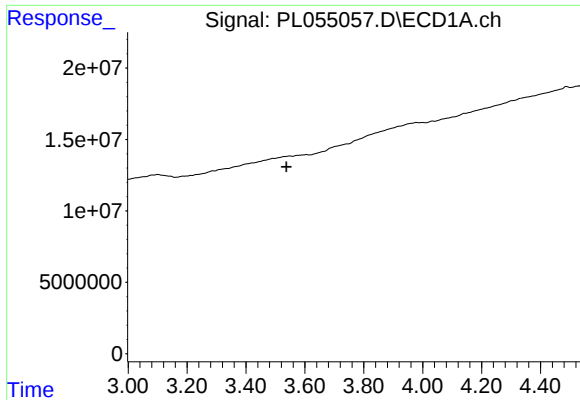

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

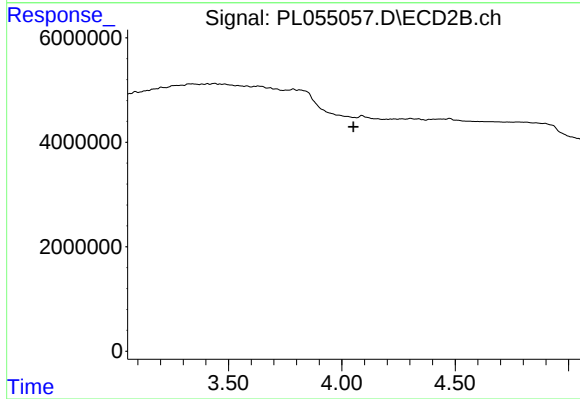


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.052 min
Response: 0
Conc: N.D.

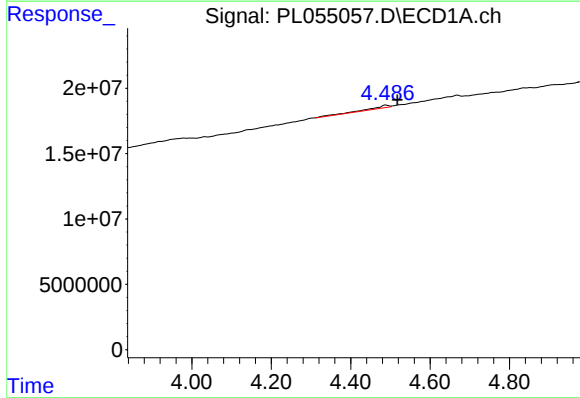


#6 beta-BHC

R.T.: 4.488 min
Delta R.T.: -0.030 min
Response: 6441124
Conc: 0.87 ng/ml

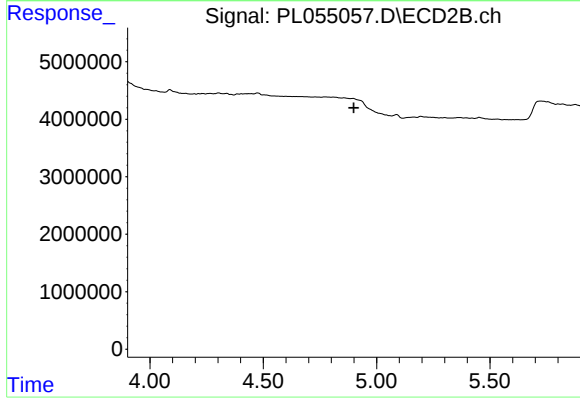

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.899 min
Response: 0
Conc: N.D.

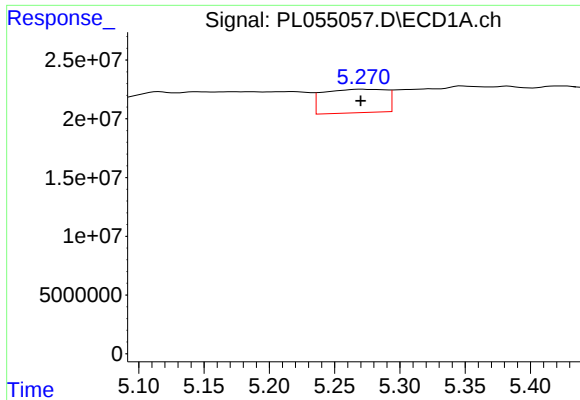

#8 Heptachlor epoxide


R.T.: 5.271 min
Delta R.T.: 0.001 min
Response: 67008792
Conc: 4.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

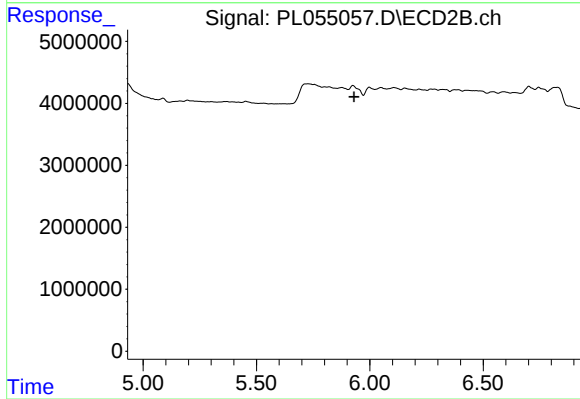


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.930 min
Response: 0
Conc: N.D.

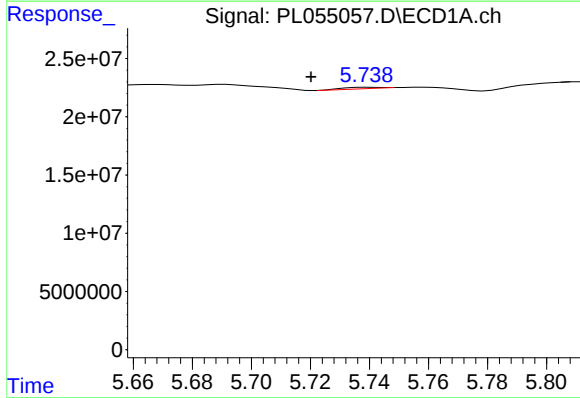


#12 4,4'-DDE

R.T.: 5.740 min
Delta R.T.: 0.020 min
Response: 989962
Conc: 0.07 ng/ml

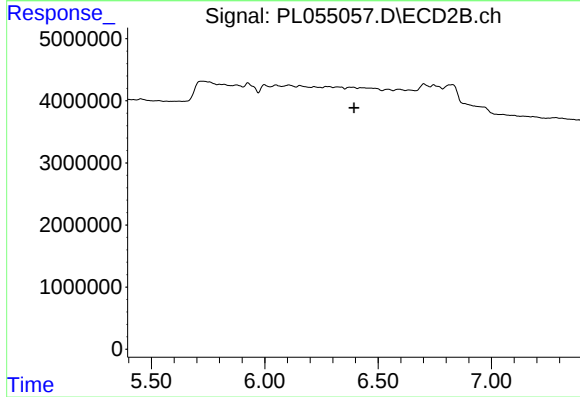

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

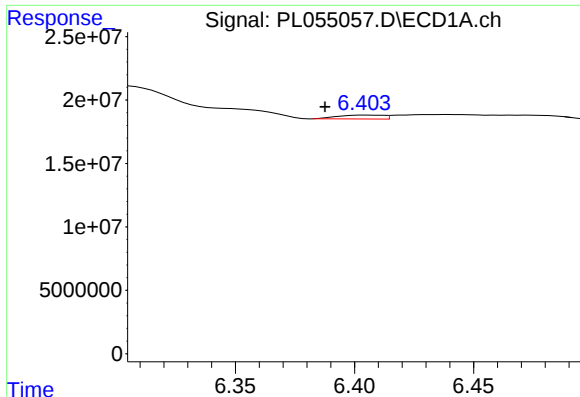

#15 Endosulfan II


R.T.: 6.405 min
Delta R.T.: 0.017 min
Response: 4159299
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

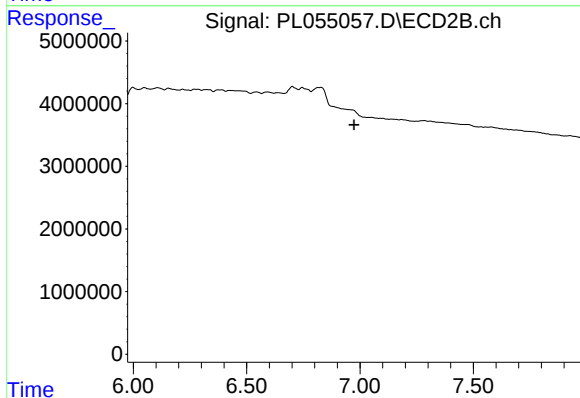


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.974 min
Response: 0
Conc: N.D.

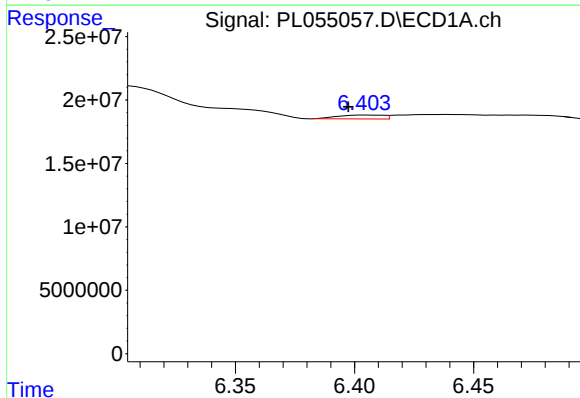


#27 Chlordane-5

R.T.: 6.405 min
Delta R.T.: 0.007 min
Response: 4159299
Conc: 11.05 ng/ml

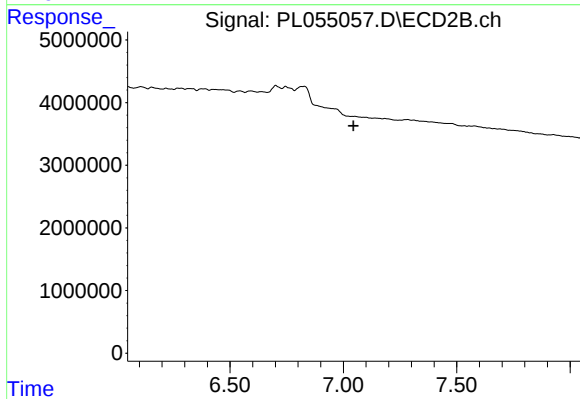

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.045 min
Response: 0
Conc: N.D.

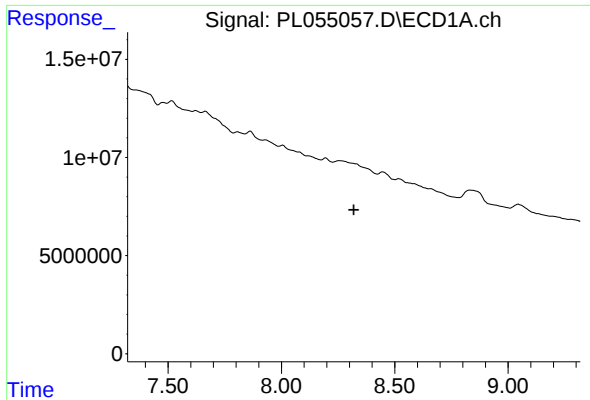

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

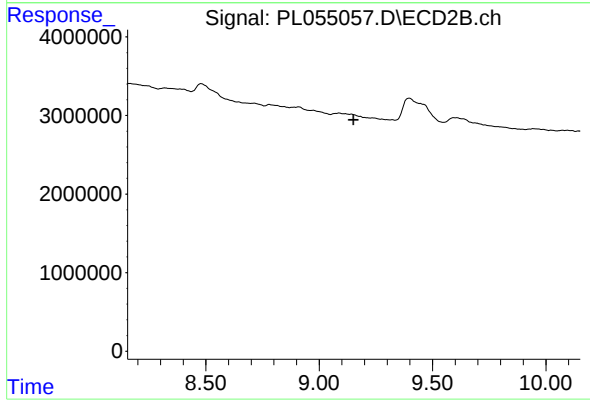

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.152 min
Response: 0
Conc: N.D.