

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
 Data File : PL055064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 13:17
 Operator : SG\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 14:01:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:00:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.049	1345.7E6	269.5E6	98.663	95.247
28)	SA Decachlor...	8.317	9.151	876.0E6	211.5E6	96.343	92.940
Target Compounds							
23)	Chlordane-1	4.418	5.046	424.9E6	96508275	986.997	915.443
24)	Chlordane-2	4.924	5.515	447.4E6	98576443	958.634	920.066
25)	Chlordane-3	5.498	6.163	1361.1E6	353.5E6	983.691	964.107
26)	Chlordane-4	5.555	6.237	1119.2E6	415.1E6	970.328	953.042
27)	Chlordane-5	6.396	7.044	395.2E6	74023035	1001.619	939.405



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
Data File : PL055064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 13:17
Operator : SG\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 14:01:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:00:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

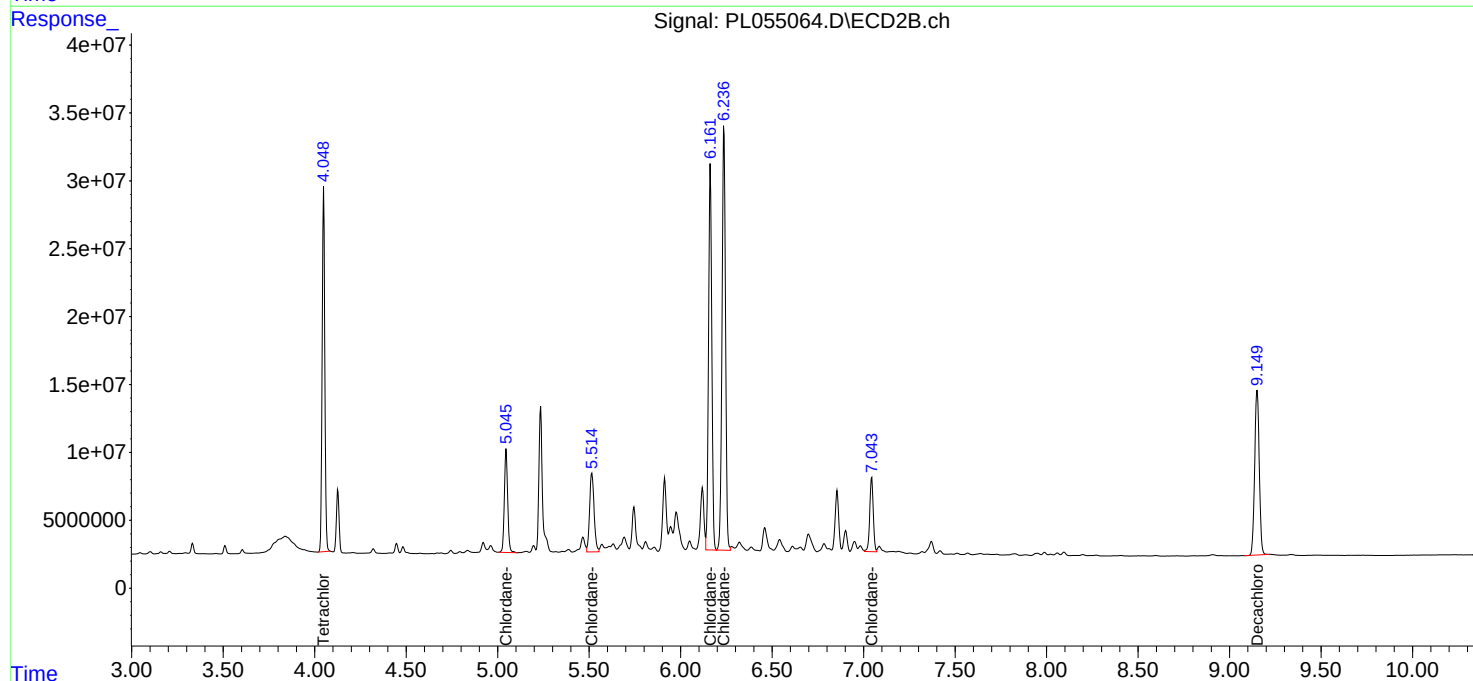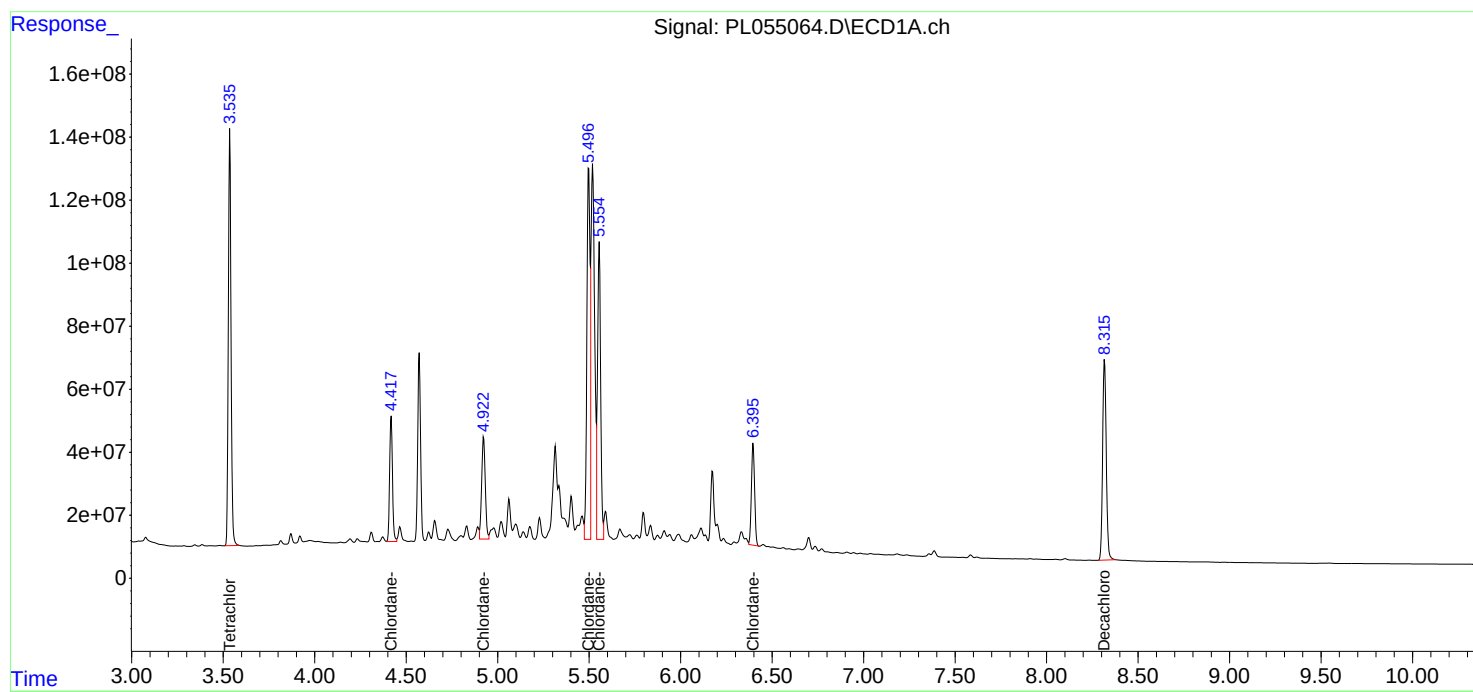


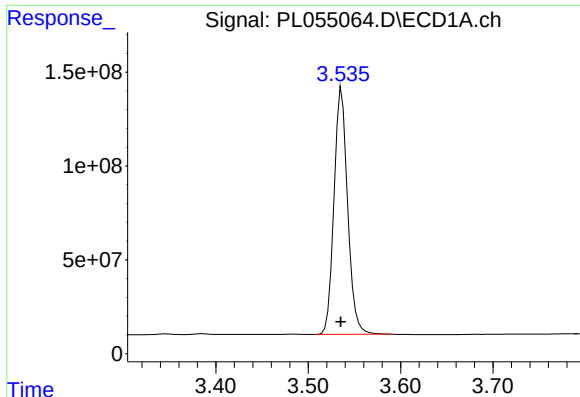

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: 0.001 min
Response: 1345692084
Conc: 98.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

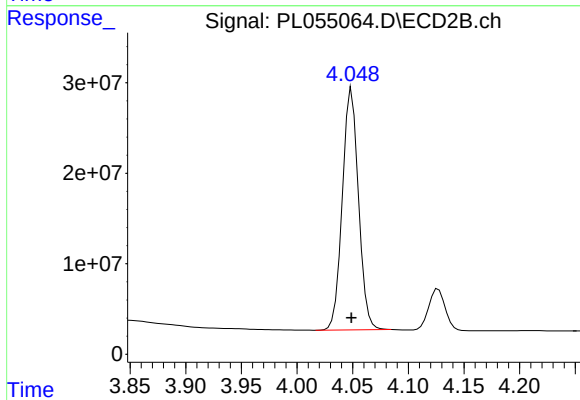


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.000 min
Response: 269489749
Conc: 95.25 ng/ml

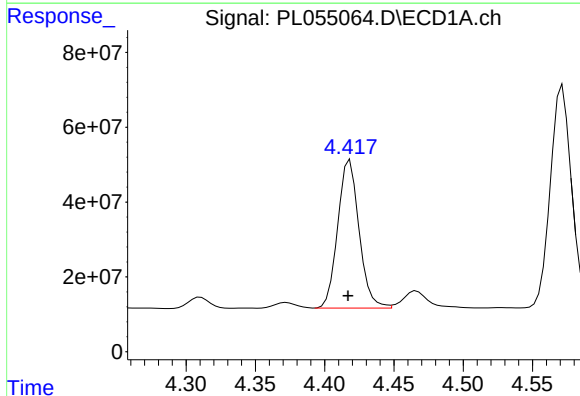


#23 Chlordane-1

R.T.: 4.418 min
Delta R.T.: 0.001 min
Response: 424901345
Conc: 987.00 ng/ml

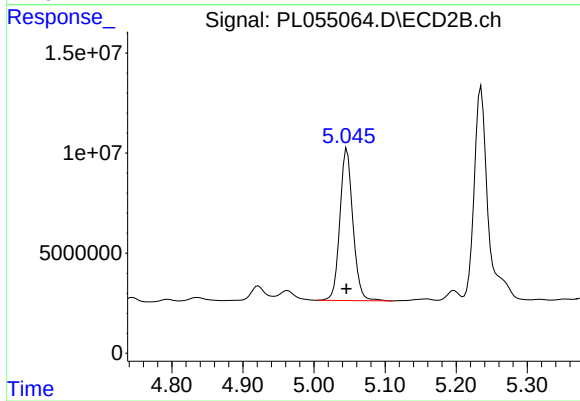

#23 Chlordane-1


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 96508275
Conc: 915.44 ng/ml

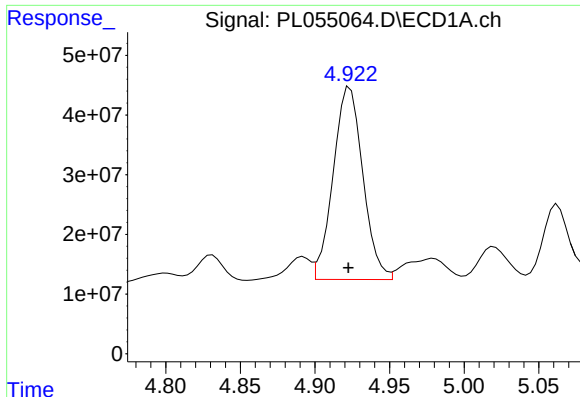

#24 Chlordane-2


R.T.: 4.924 min
Delta R.T.: 0.001 min
Response: 447395941
Conc: 958.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

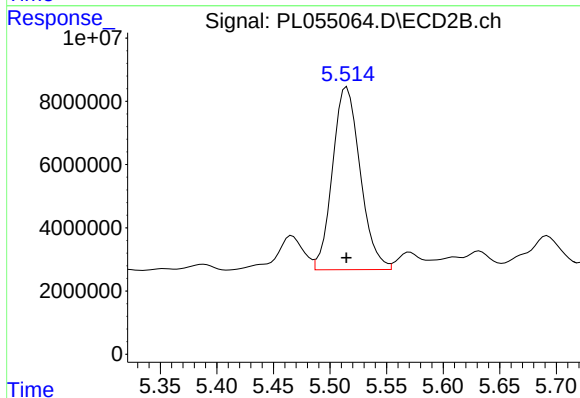


#24 Chlordane-2

R.T.: 5.515 min
Delta R.T.: 0.000 min
Response: 98576443
Conc: 920.07 ng/ml

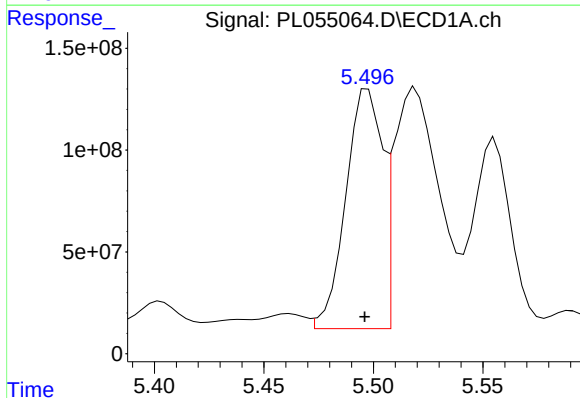


#25 Chlordane-3

R.T.: 5.498 min
Delta R.T.: 0.002 min
Response: 1361107792
Conc: 983.69 ng/ml

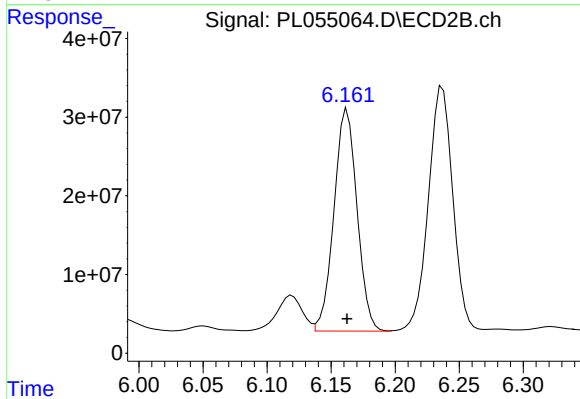

#25 Chlordane-3


R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 353451971
Conc: 964.11 ng/ml

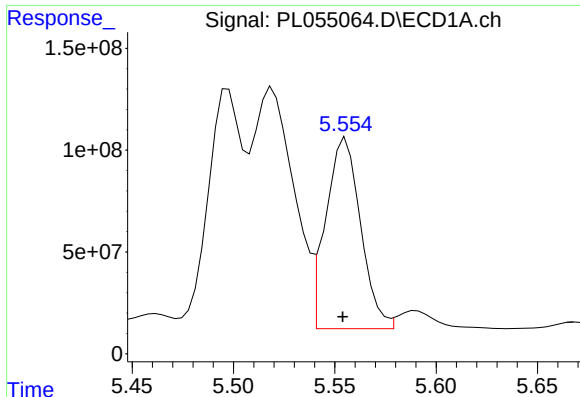

#26 Chlordane-4


R.T.: 5.555 min
Delta R.T.: 0.002 min
Response: 1119198757
Conc: 970.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

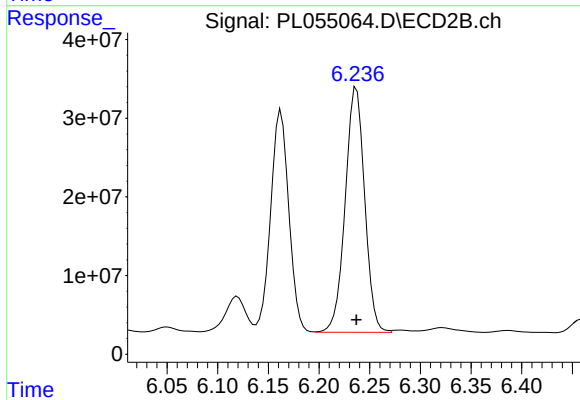


#26 Chlordane-4

R.T.: 6.237 min
Delta R.T.: 0.000 min
Response: 415142861
Conc: 953.04 ng/ml

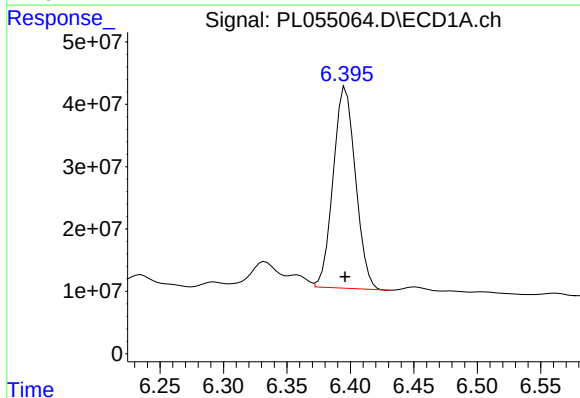


#27 Chlordane-5

R.T.: 6.396 min
Delta R.T.: 0.000 min
Response: 395155273
Conc: 1001.62 ng/ml

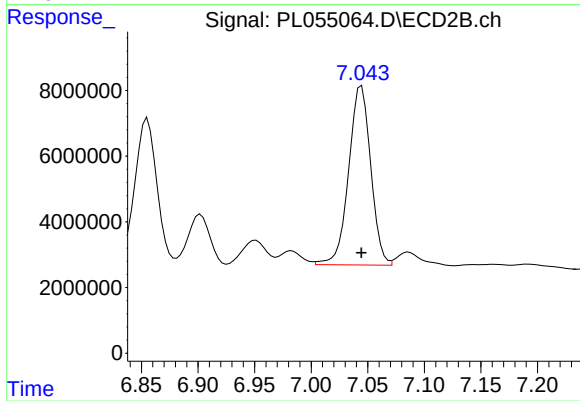

#27 Chlordane-5


R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 74023035
Conc: 939.41 ng/ml

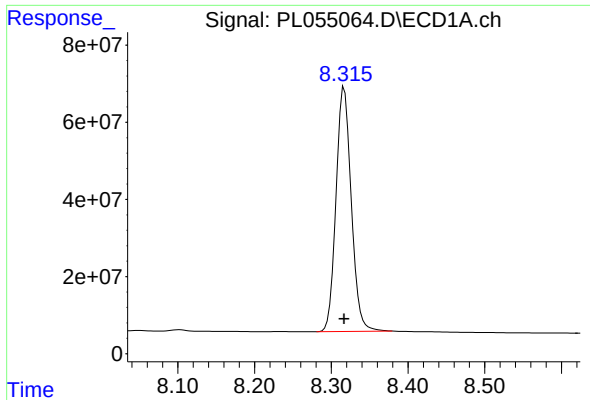

#28 Decachlorobiphenyl

R.T.: 8.317 min
Delta R.T.: 0.000 min
Response: 876011276
Conc: 96.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

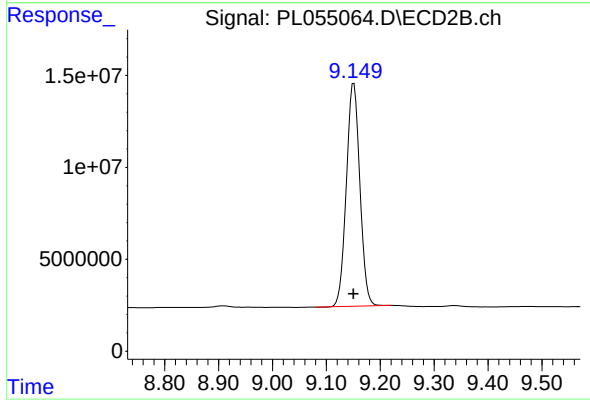

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 211487251
Conc: 92.94 ng/ml