

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
 Data File : PL055065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 13:31
 Operator : SG\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 14:01:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:00:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	999.8E6	203.9E6	73.306	72.072
28)	SA Decachlor...	8.316	9.151	653.6E6	161.3E6	71.883	70.872
Target Compounds							
23)	Chlordane-1	4.418	5.046	314.2E6	75114211	729.909	712.507
24)	Chlordane-2	4.922	5.514	336.4E6	76066130	720.797	709.965
25)	Chlordane-3	5.496	6.162	1024.3E6	265.8E6	740.281	725.112
26)	Chlordane-4	5.554	6.237	835.0E6	314.2E6	723.900	721.377
27)	Chlordane-5	6.395	7.045	291.5E6	56401335	738.885	715.773


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
Data File : PL055065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 13:31
Operator : SG\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 14:01:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:00:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

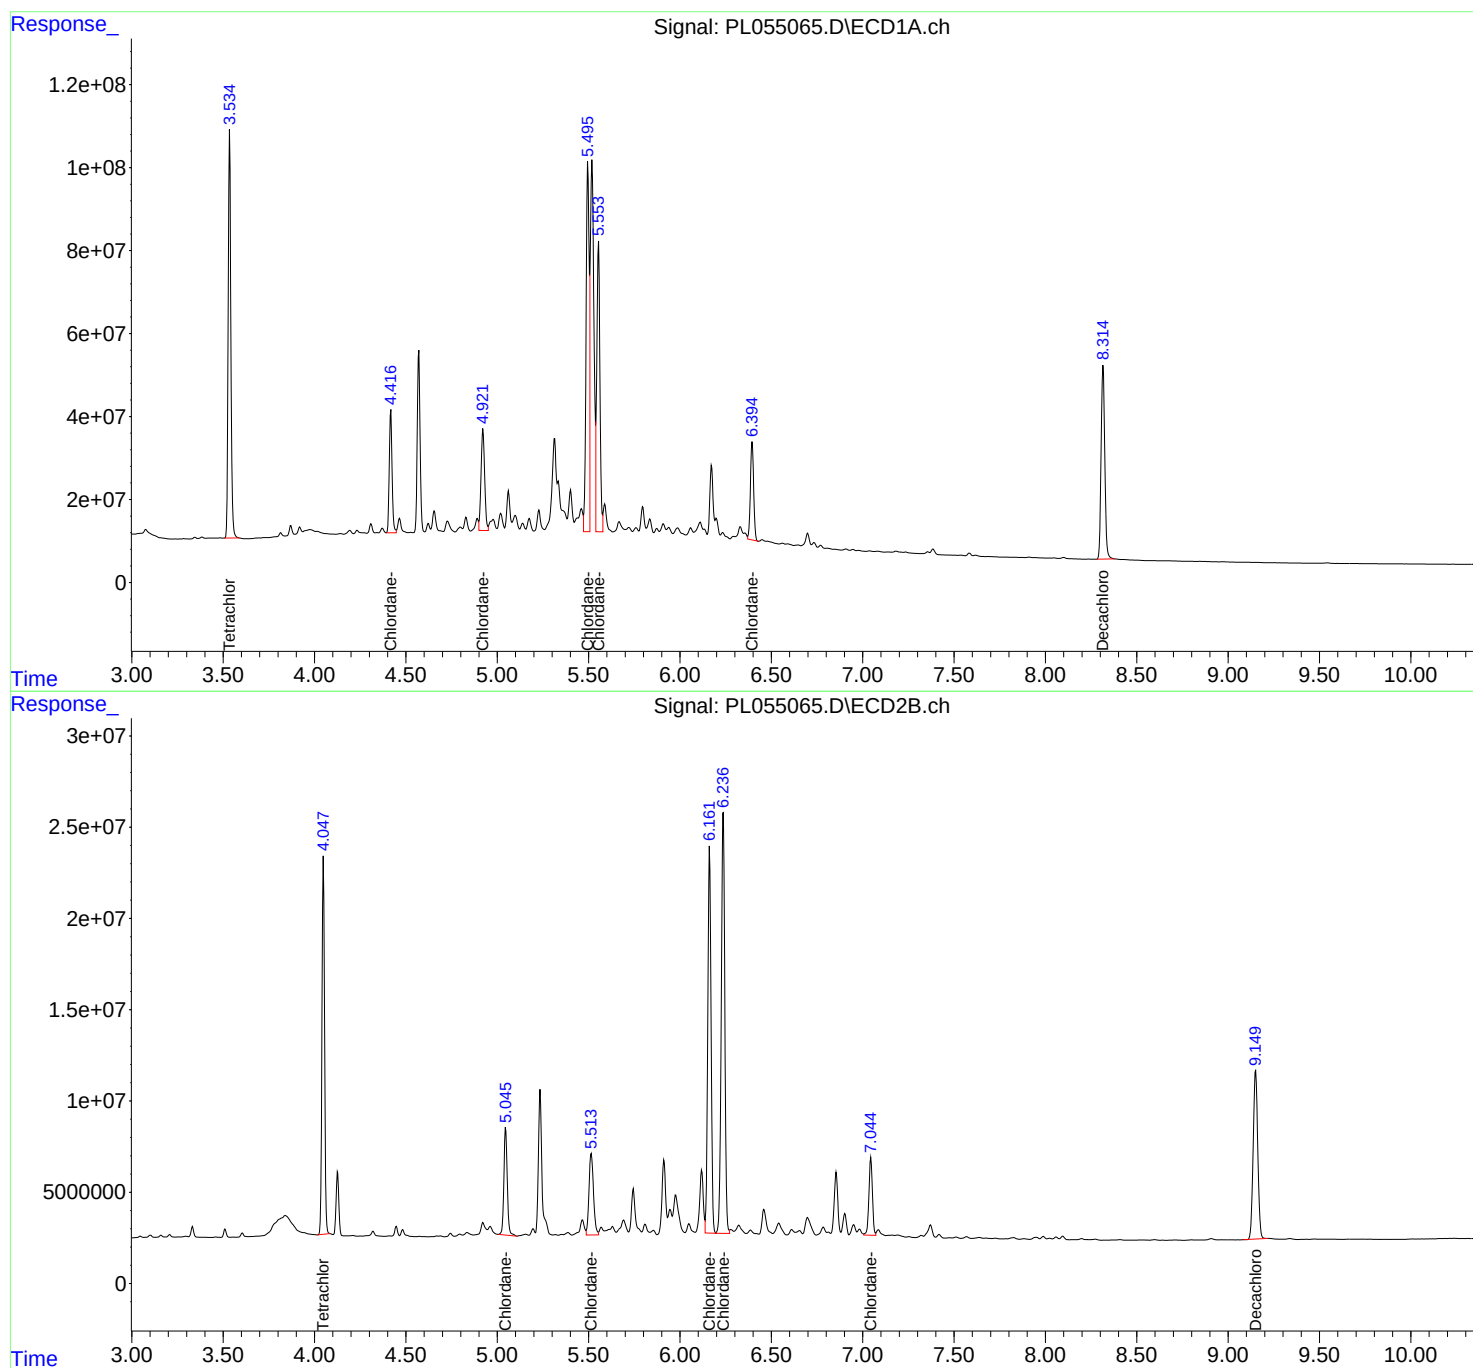


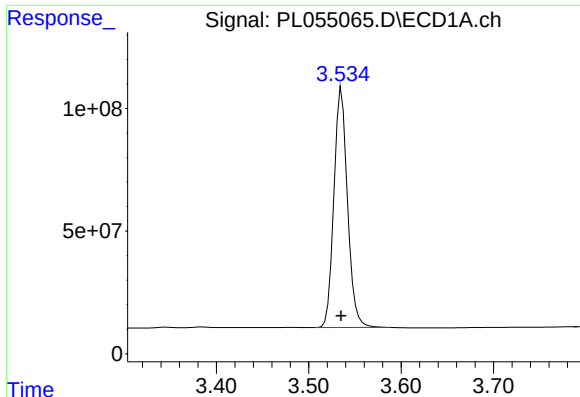

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 999847983
Conc: 73.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

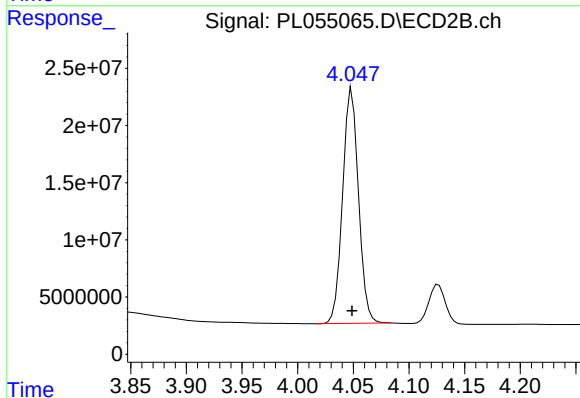


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.000 min
Response: 203918736
Conc: 72.07 ng/ml

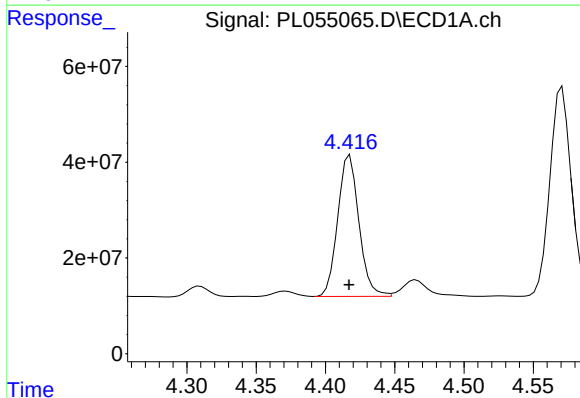


#23 Chlordane-1

R.T.: 4.418 min
Delta R.T.: 0.000 min
Response: 314225012
Conc: 729.91 ng/ml

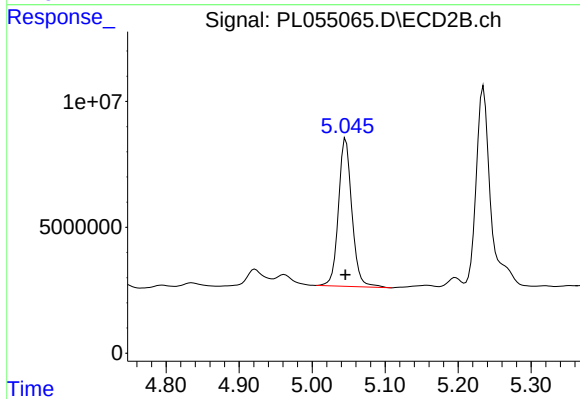

#23 Chlordane-1


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 75114211
Conc: 712.51 ng/ml

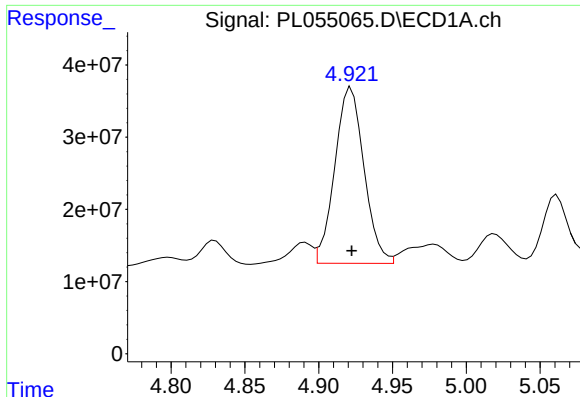

#24 Chlordane-2


R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 336397152
Conc: 720.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

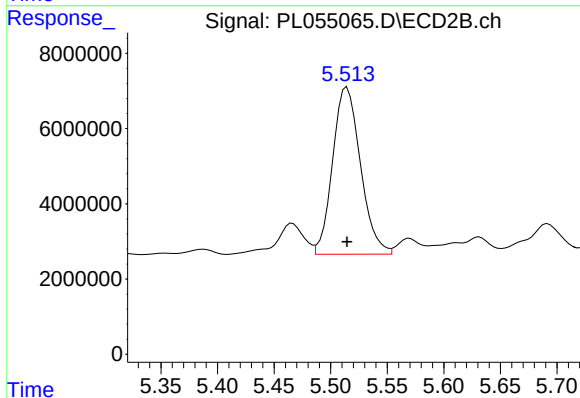


#24 Chlordane-2

R.T.: 5.514 min
Delta R.T.: 0.000 min
Response: 76066130
Conc: 709.97 ng/ml

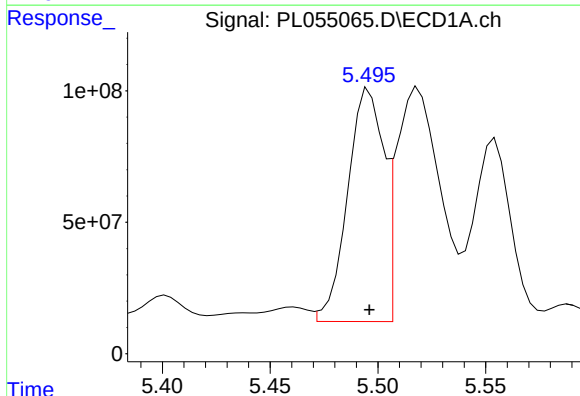


#25 Chlordane-3

R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 1024308382
Conc: 740.28 ng/ml

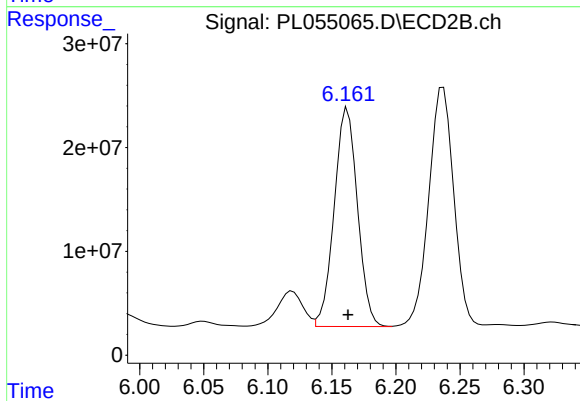

#25 Chlordane-3


R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 265833902
Conc: 725.11 ng/ml

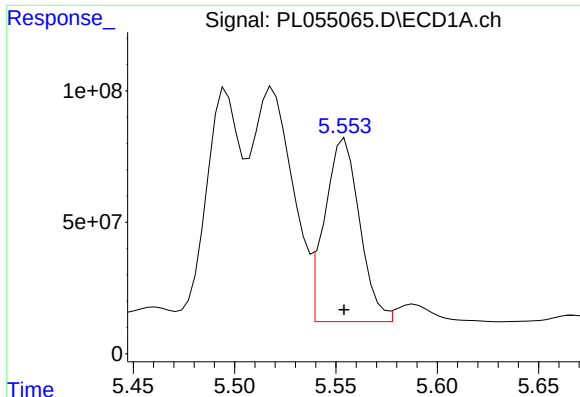

#26 Chlordane-4


R.T.: 5.554 min
Delta R.T.: 0.000 min
Response: 834963051
Conc: 723.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

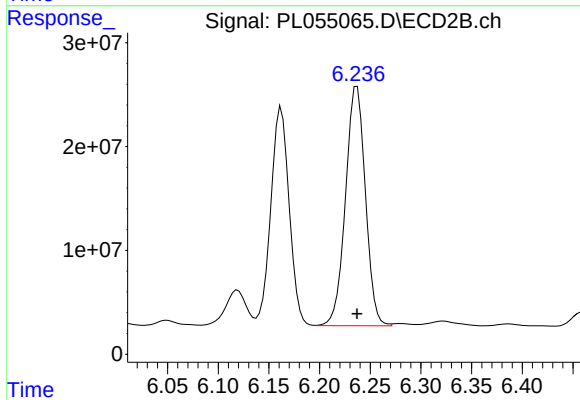


#26 Chlordane-4

R.T.: 6.237 min
Delta R.T.: 0.000 min
Response: 314230373
Conc: 721.38 ng/ml

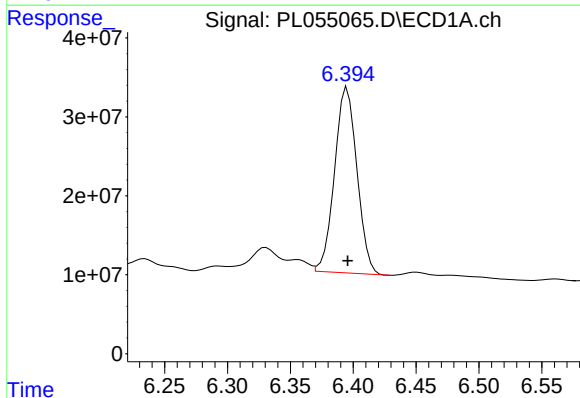


#27 Chlordane-5

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 291502068
Conc: 738.88 ng/ml

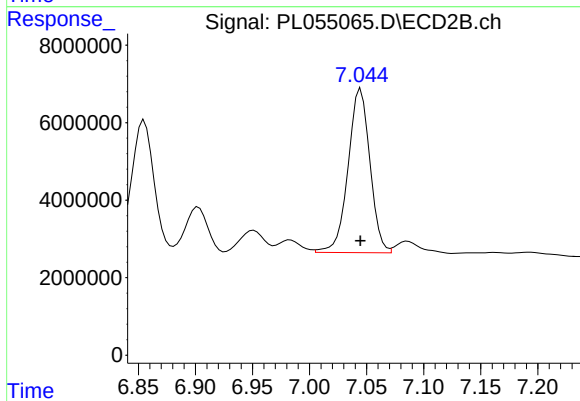

#27 Chlordane-5


R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 56401335
Conc: 715.77 ng/ml

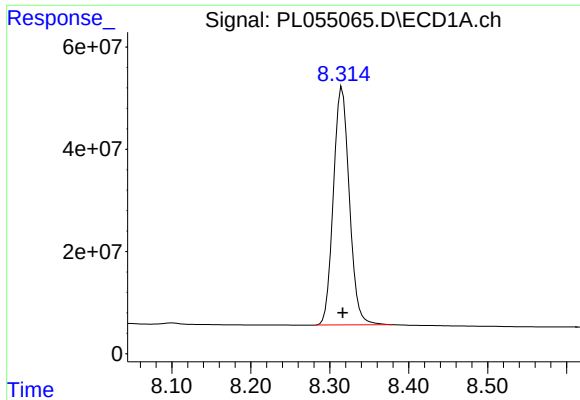

#28 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 653607117
Conc: 71.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

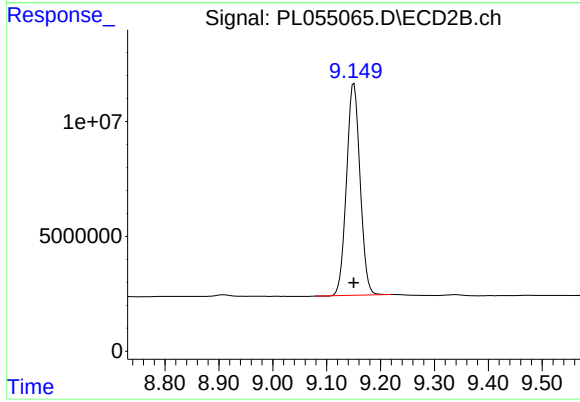

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 161271551
Conc: 70.87 ng/ml