

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
 Data File : PL055066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 13:45
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 14:00:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:00:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	682.0E6	141.5E6	50.000	50.000
28)	SA Decachlor...	8.316	9.150	454.6E6	113.8E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.417	5.046	215.2E6	52711218	500.000	500.000
24)	Chlordane-2	4.922	5.514	233.4E6	53570329	500.000	500.000
25)	Chlordane-3	5.496	6.163	691.8E6	183.3E6	500.000	500.000
26)	Chlordane-4	5.554	6.237	576.7E6	217.8E6	500.000	500.000
27)	Chlordane-5	6.396	7.044	197.3E6	39398885	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
Data File : PL055066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 13:45
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 14:00:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:00:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

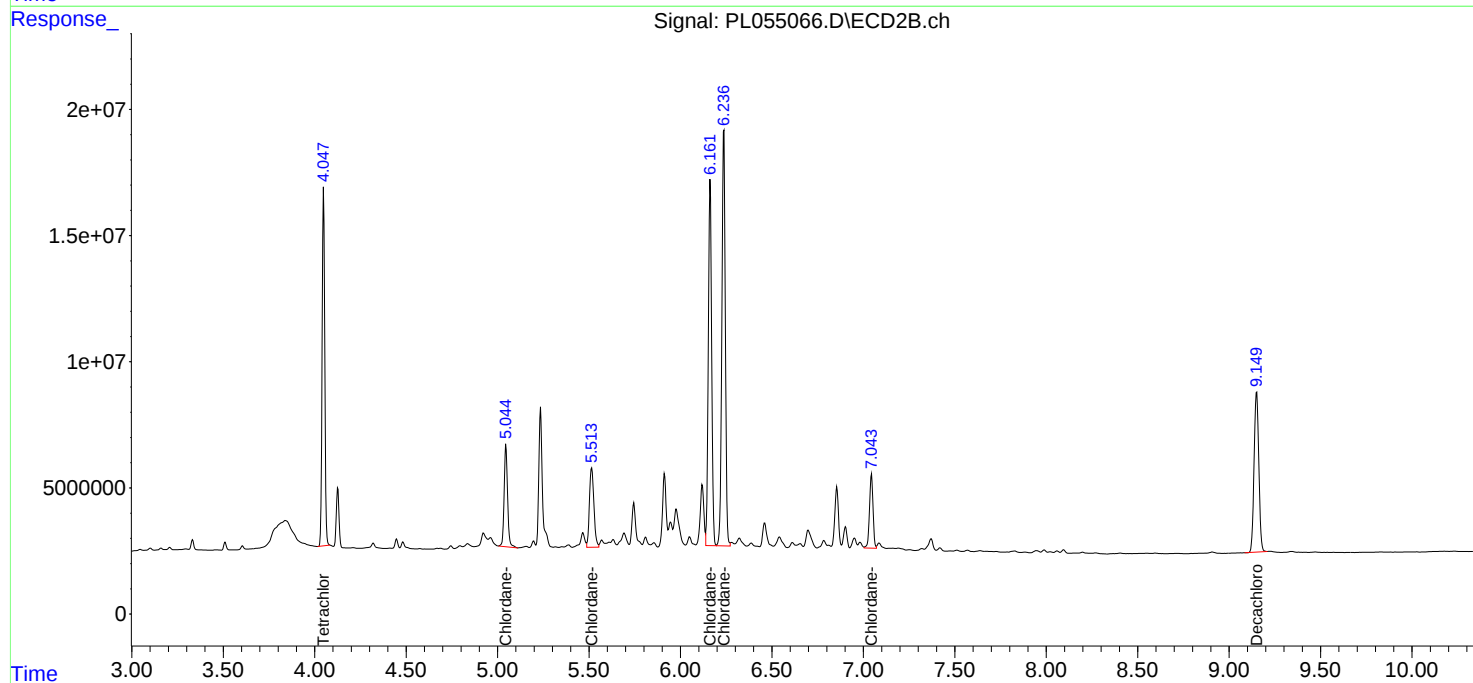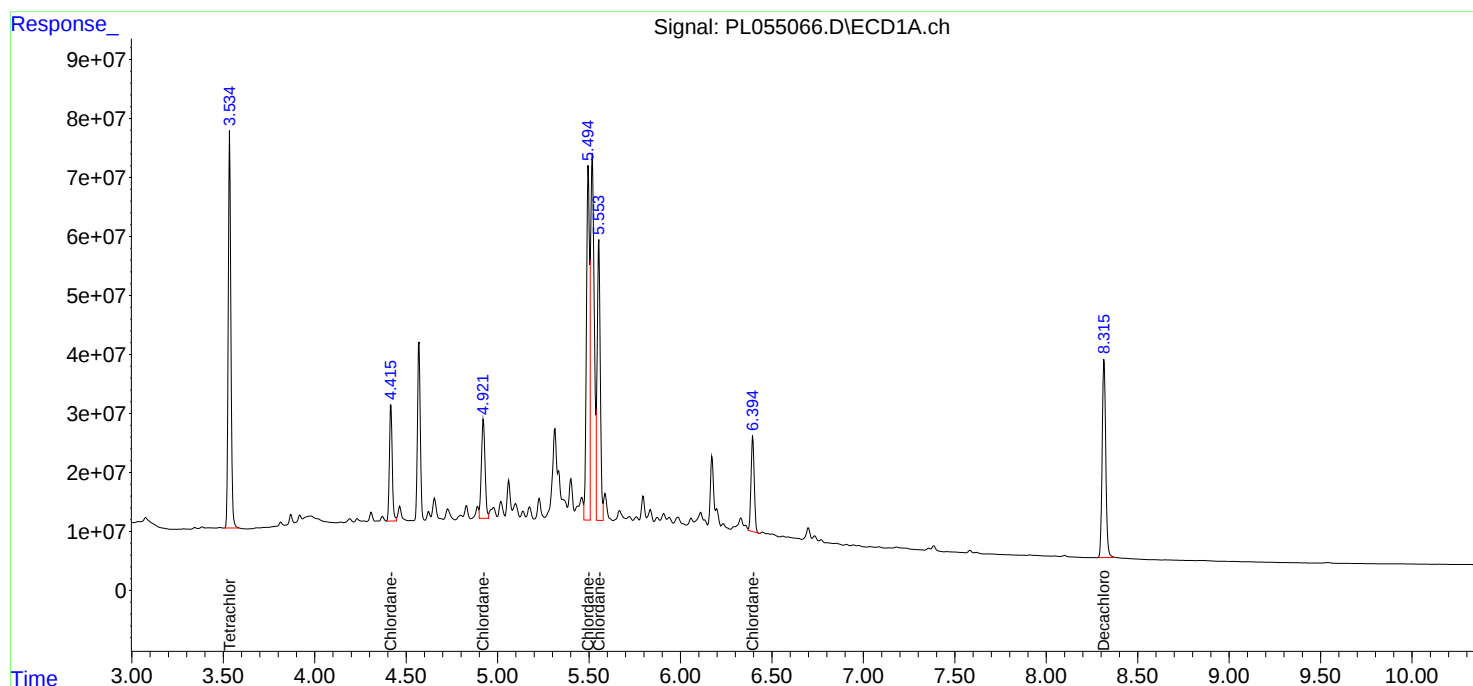


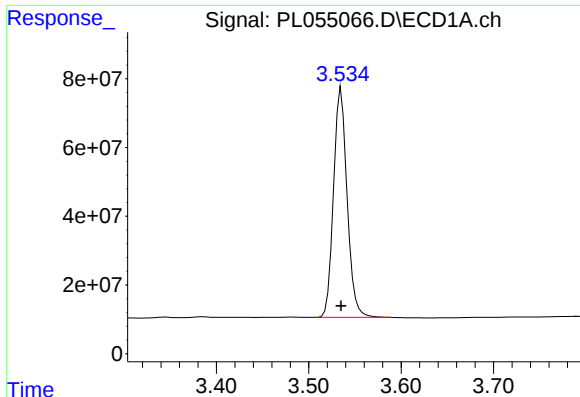

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 681964127
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

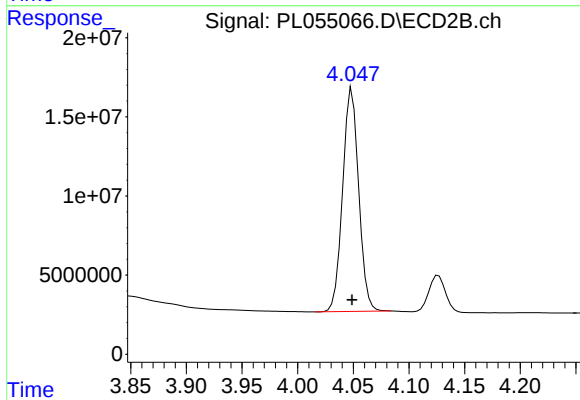


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.000 min
Response: 141469377
Conc: 50.00 ng/ml

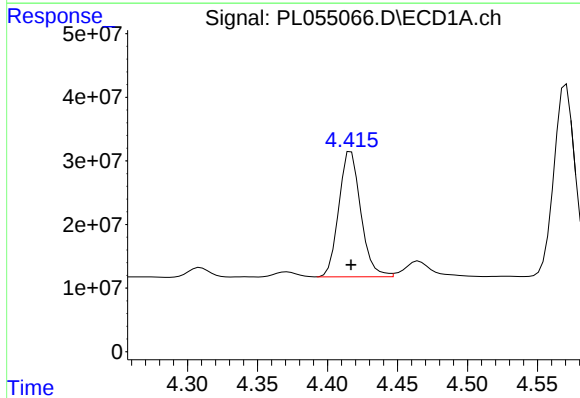


#23 Chlordane-1

R.T.: 4.417 min
Delta R.T.: 0.000 min
Response: 215249578
Conc: 500.00 ng/ml

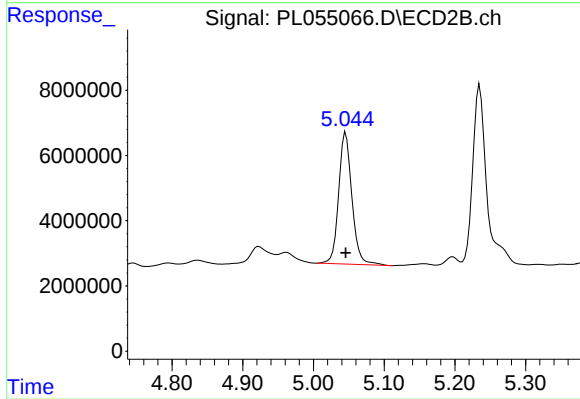

#23 Chlordane-1


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 52711218
Conc: 500.00 ng/ml

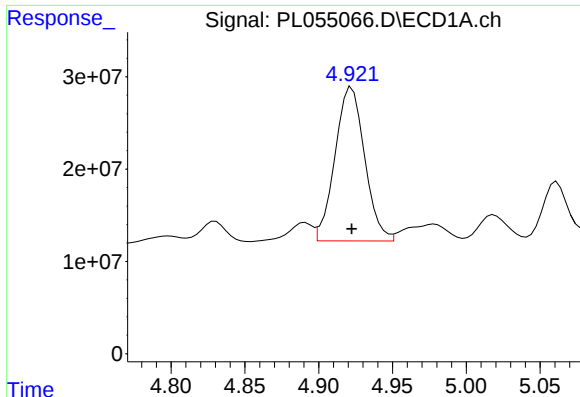

#24 Chlordane-2


R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 233350738
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

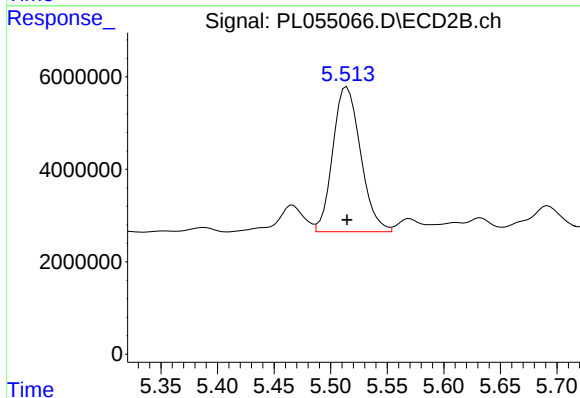


#24 Chlordane-2

R.T.: 5.514 min
Delta R.T.: 0.000 min
Response: 53570329
Conc: 500.00 ng/ml

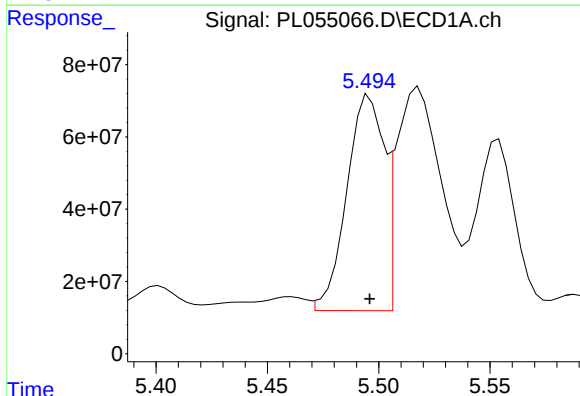


#25 Chlordane-3

R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 691837210
Conc: 500.00 ng/ml

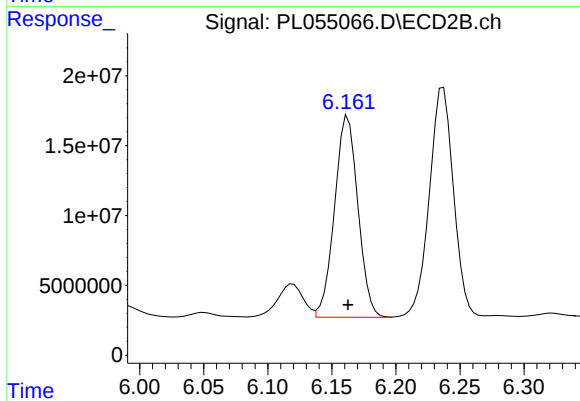

#25 Chlordane-3


R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 183305342
Conc: 500.00 ng/ml

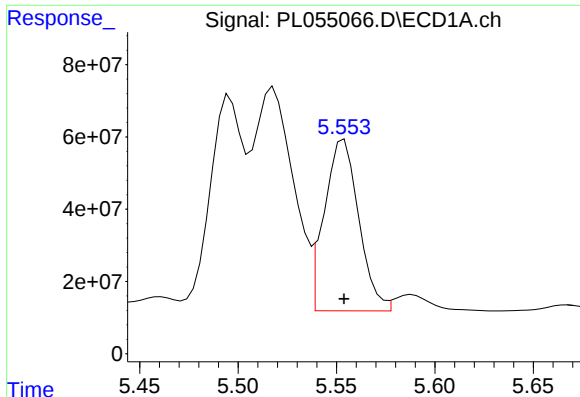

#26 Chlordane-4


R.T.: 5.554 min
Delta R.T.: 0.000 min
Response: 576711766
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

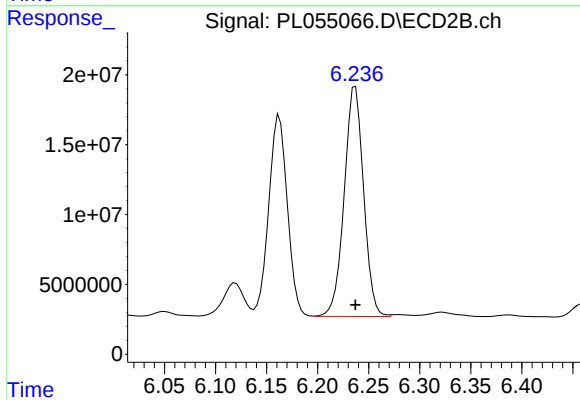


#26 Chlordane-4

R.T.: 6.237 min
Delta R.T.: 0.000 min
Response: 217798876
Conc: 500.00 ng/ml

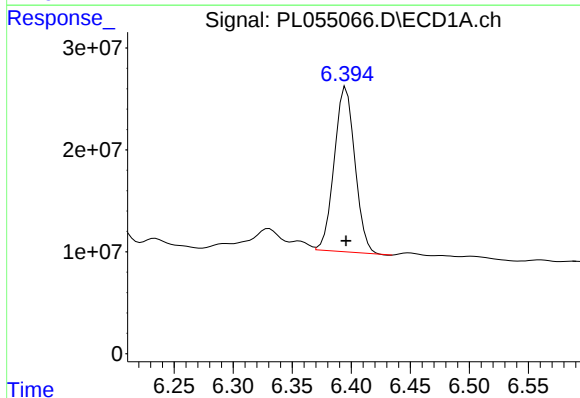


#27 Chlordane-5

R.T.: 6.396 min
Delta R.T.: 0.000 min
Response: 197258192
Conc: 500.00 ng/ml

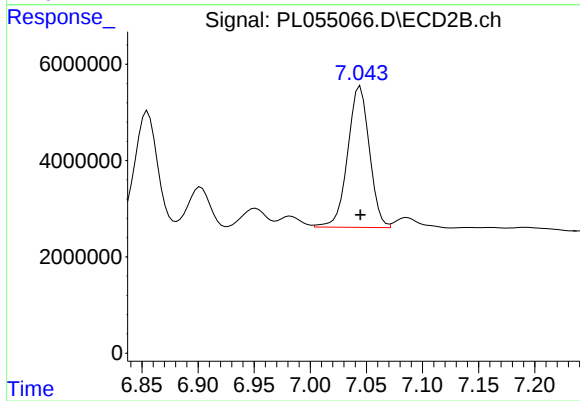

#27 Chlordane-5


R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 39398885
Conc: 500.00 ng/ml

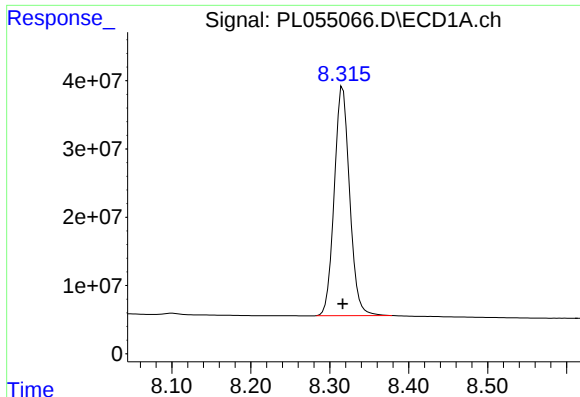

#28 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 454630292
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

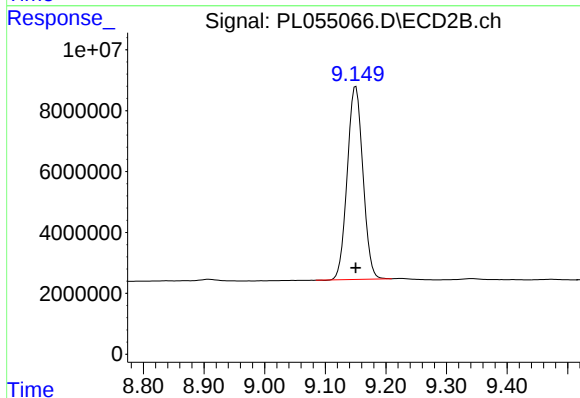

#28 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: 0.000 min
Response: 113776648
Conc: 50.00 ng/ml