

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
 Data File : PL055067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 13:59
 Operator : SG\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 14:11:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:00:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.048	324.2E6	69021690	24.058	25.119
28)	SA Decachlor...	8.316	9.149	227.6E6	57209498	25.698	26.240
Target Compounds							
23)	Chlordane-1	4.417	5.046	102.8E6	26745369	241.954	265.609
24)	Chlordane-2	4.921	5.514	115.6E6	26908555	254.517	262.831
25)	Chlordane-3	5.496	6.162	334.7E6	88778096	244.249	247.866
26)	Chlordane-4	5.554	6.236	274.8E6	106.4E6	243.460	251.361
27)	Chlordane-5	6.395	7.044	90322640	18039053	229.957	237.332



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
Data File : PL055067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 13:59
Operator : SG\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 14:11:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:00:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

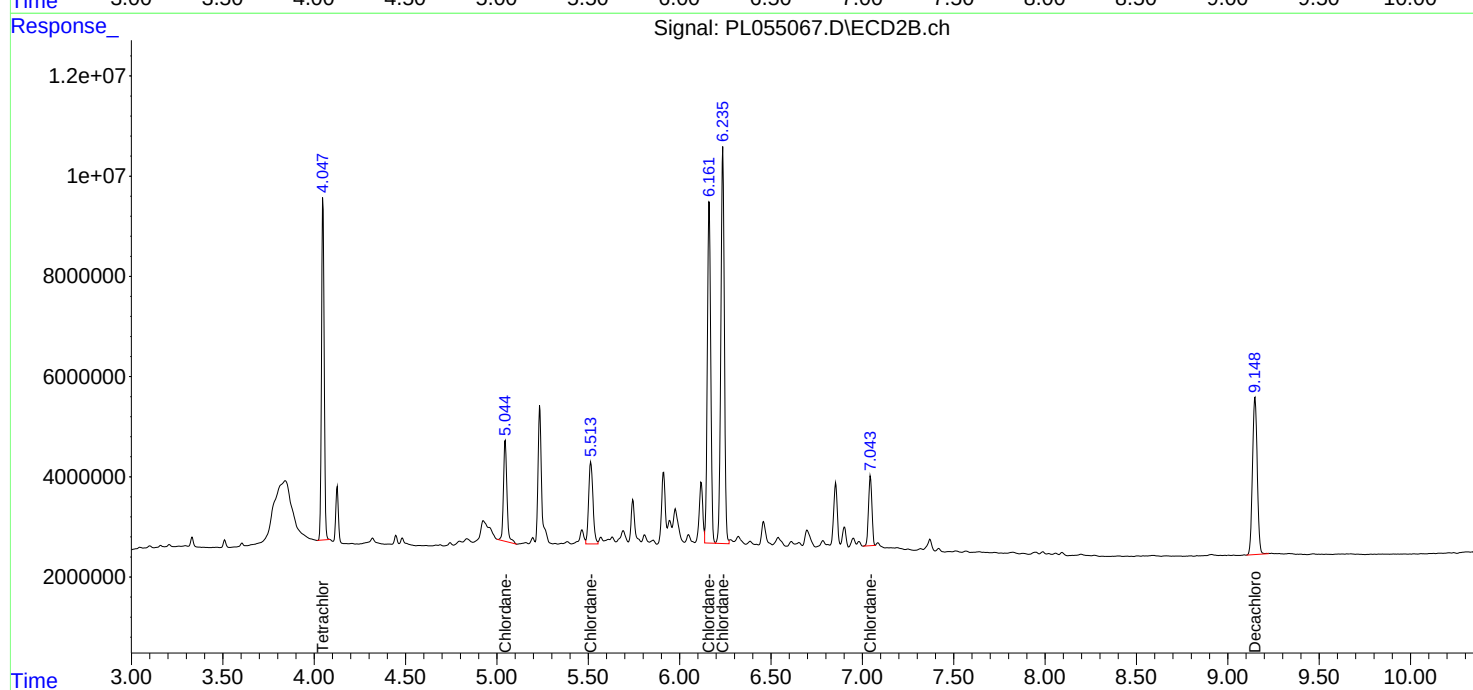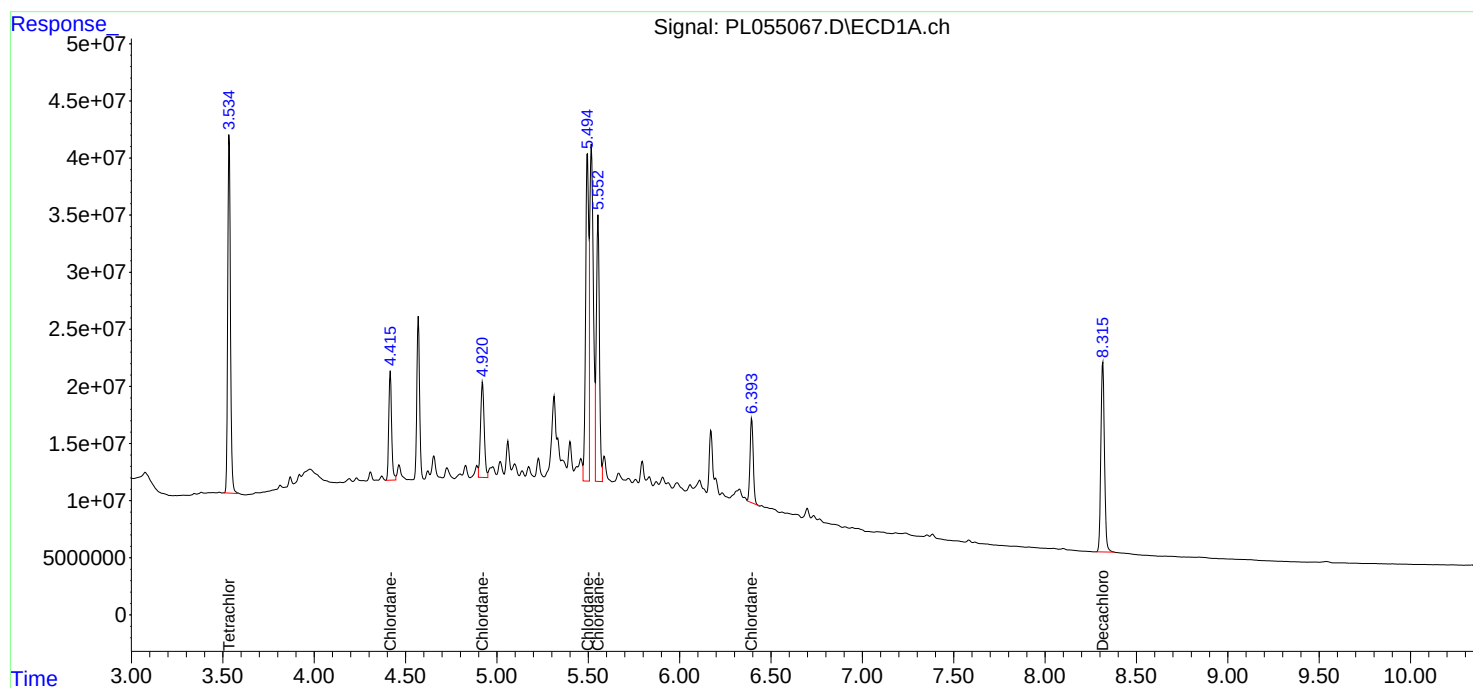


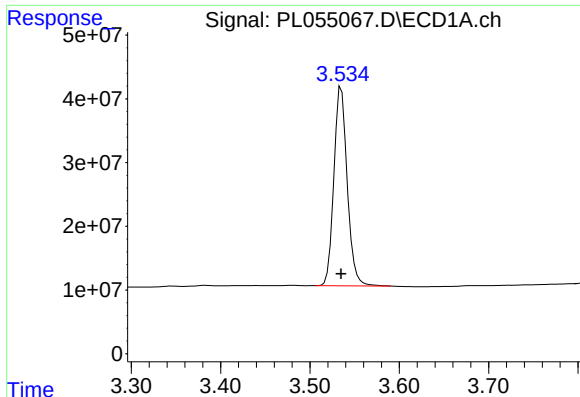

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 324202318
Conc: 24.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

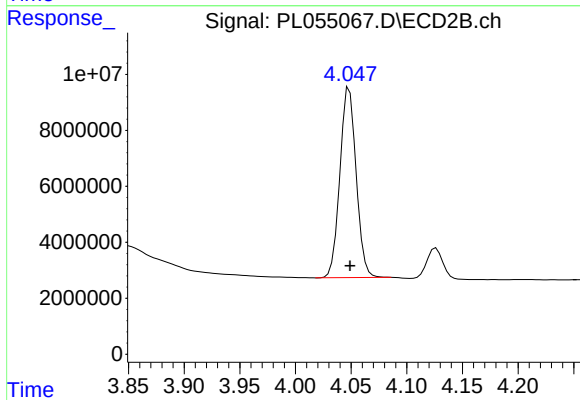


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 69021690
Conc: 25.12 ng/ml

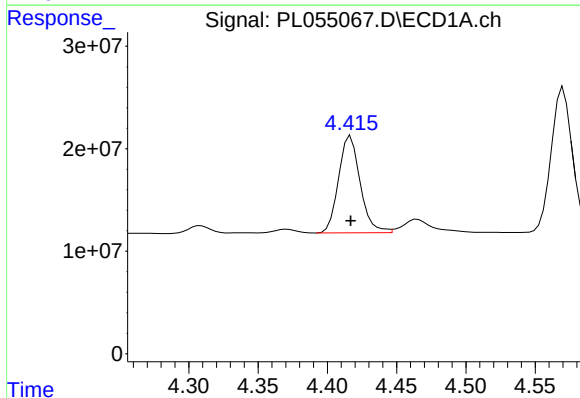


#23 Chlordane-1

R.T.: 4.417 min
Delta R.T.: 0.000 min
Response: 102779618
Conc: 241.95 ng/ml

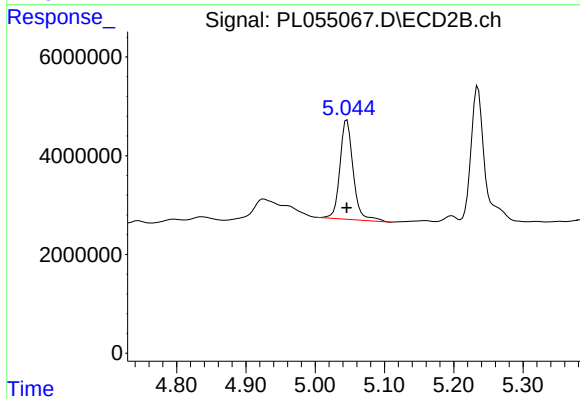

#23 Chlordane-1


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 26745369
Conc: 265.61 ng/ml

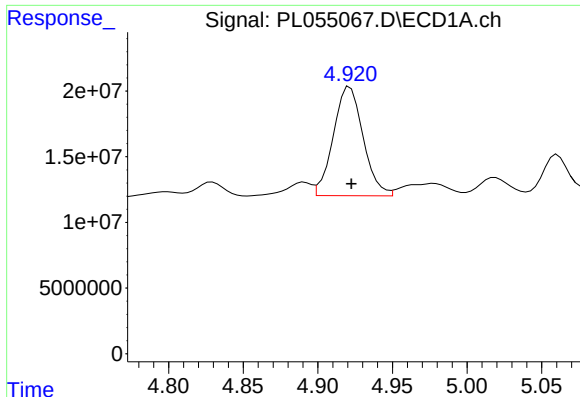

#24 Chlordane-2


R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 115603986
Conc: 254.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

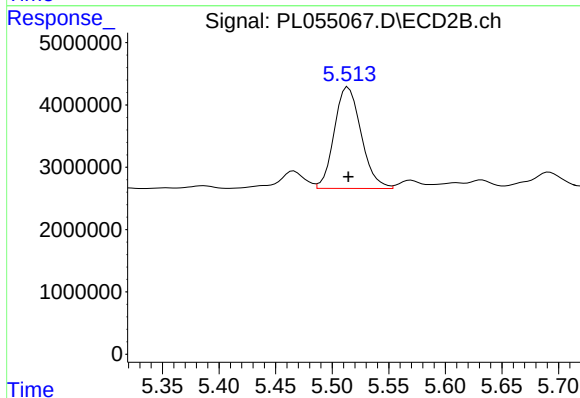


#24 Chlordane-2

R.T.: 5.514 min
Delta R.T.: 0.000 min
Response: 26908555
Conc: 262.83 ng/ml

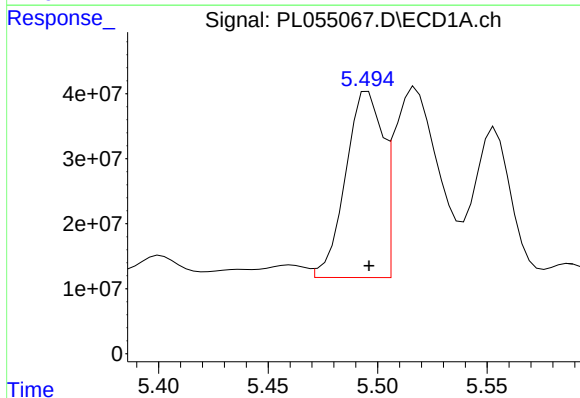


#25 Chlordane-3

R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 334664625
Conc: 244.25 ng/ml

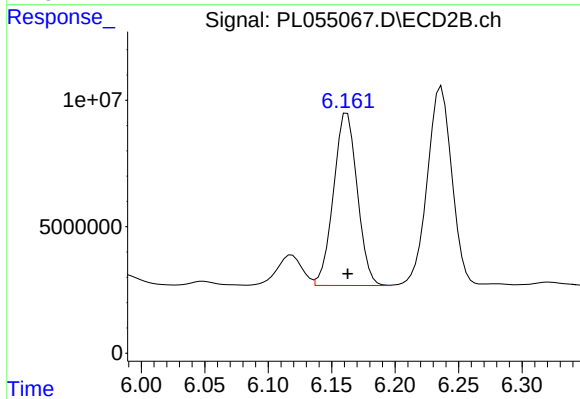

#25 Chlordane-3


R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 88778096
Conc: 247.87 ng/ml

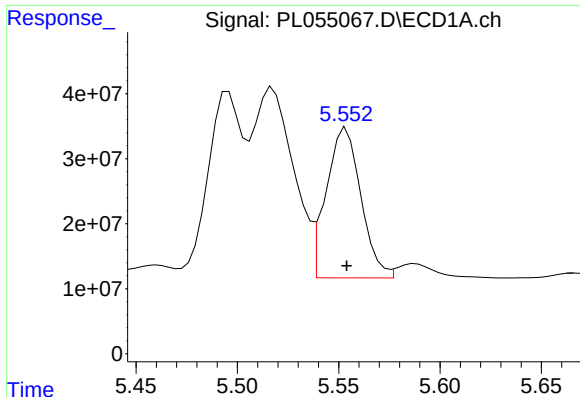

#26 Chlordane-4


R.T.: 5.554 min
Delta R.T.: 0.000 min
Response: 274777990
Conc: 243.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

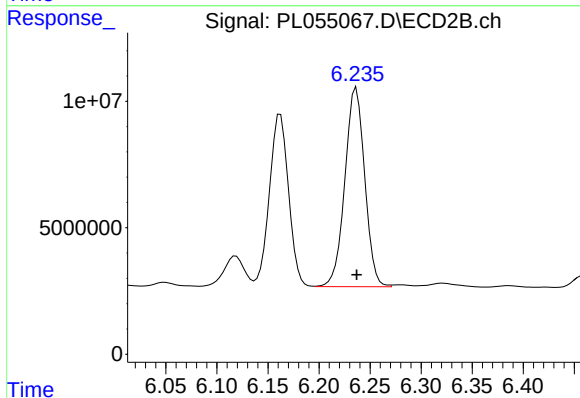


#26 Chlordane-4

R.T.: 6.236 min
Delta R.T.: 0.000 min
Response: 106385639
Conc: 251.36 ng/ml

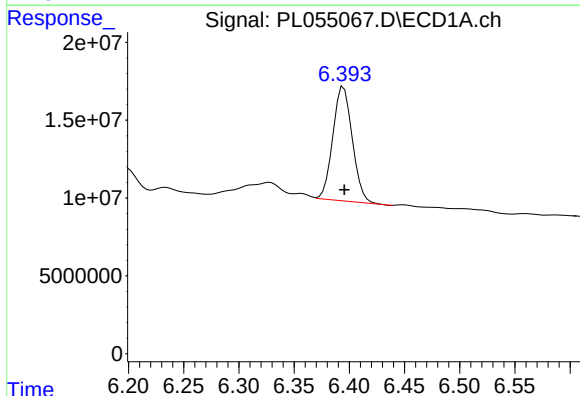


#27 Chlordane-5

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 90322640
Conc: 229.96 ng/ml

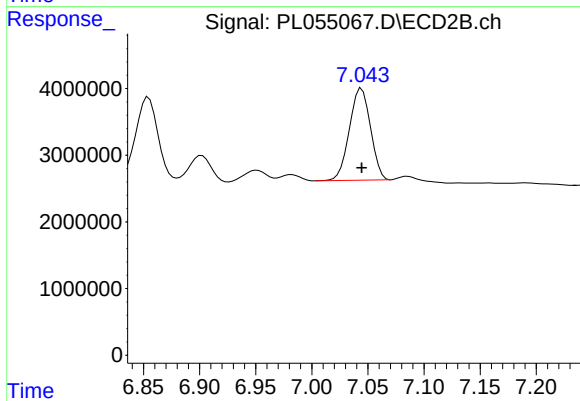

#27 Chlordane-5


R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 18039053
Conc: 237.33 ng/ml

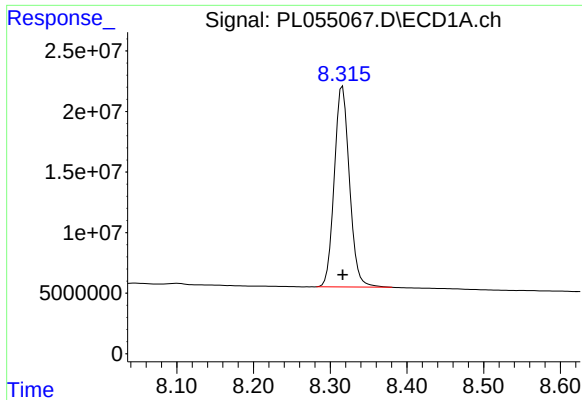

#28 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 227578987
Conc: 25.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

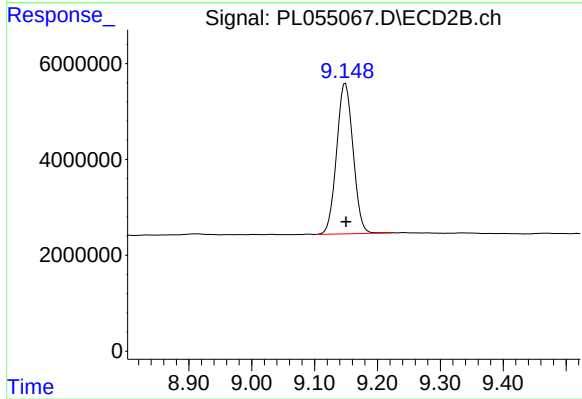

#28 Decachlorobiphenyl

R.T.: 9.149 min
Delta R.T.: -0.001 min
Response: 57209498
Conc: 26.24 ng/ml