

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
 Data File : PL055073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 15:24
 Operator : SG\AJ
 Sample : K6335-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-2BD

Manual Integrations
 APPROVED

Ankita
 12/19/2019 11:41:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 15:35:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:58:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.049	125.4E6	33948497	10.779	13.304
28)	SA Decachlor...	8.316	9.149	153.9E6	39091465	16.071	16.306
Target Compounds							
23)	Chlordane-1	4.417	5.046	111.8E6	34863410	260.629	339.588 #
24)	Chlordane-2	4.921	5.515	128.5E6	37481467	273.873m	352.748 #
25)	Chlordane-3	5.496	6.162	348.3E6	184.9E6	258.430m	504.356 #
26)	Chlordane-4	5.556	6.237	621.0E6	153.7E6	560.139	353.335 #
27)	Chlordane-5	6.393	7.044	102.0E6	28708922	275.895m	379.880 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
Data File : PL055073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 15:24
Operator : SG\AJ
Sample : K6335-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-2BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 15:35:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:58:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

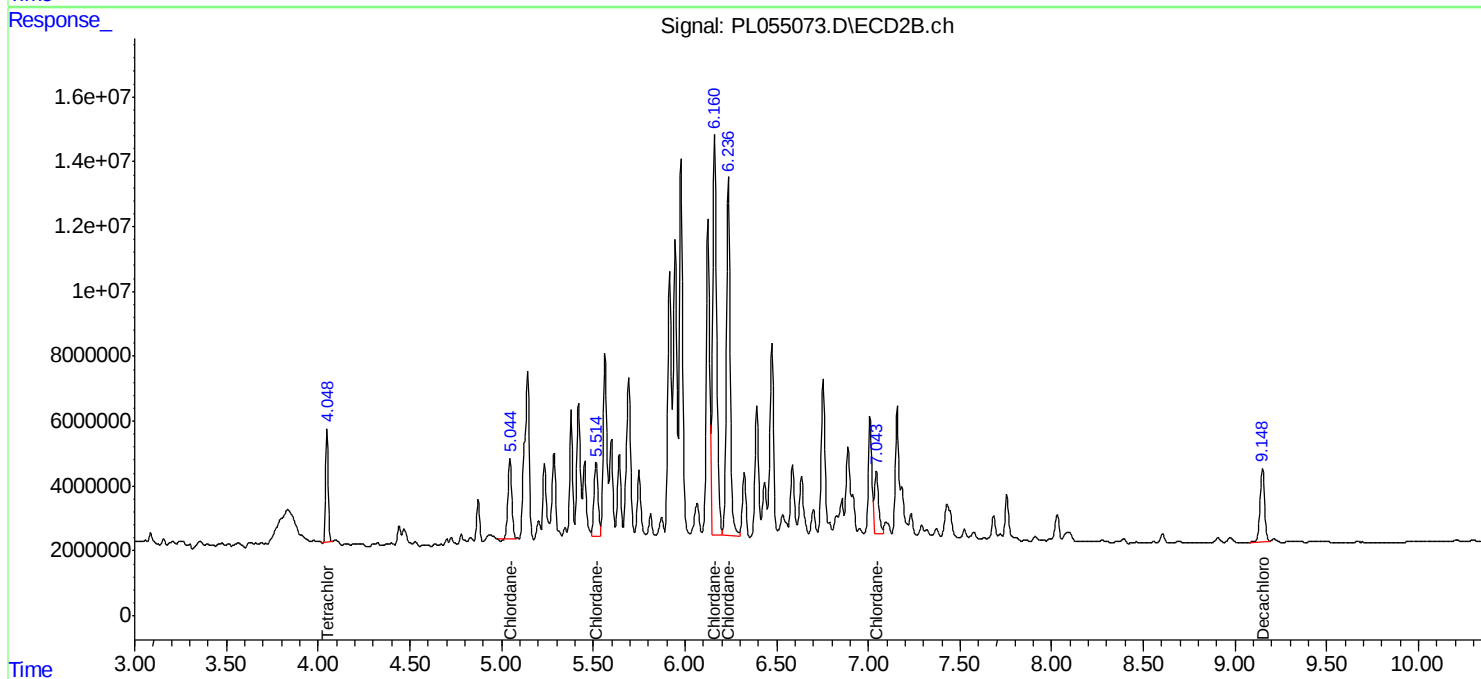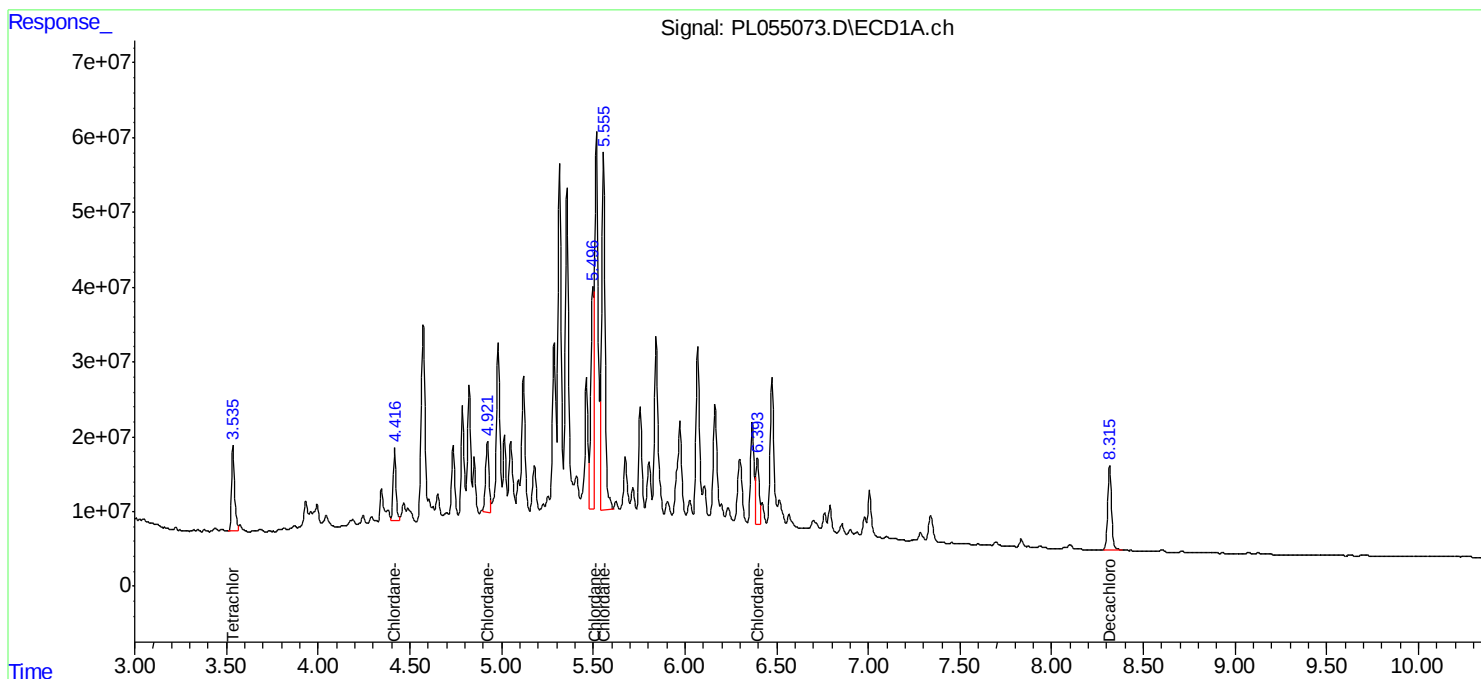

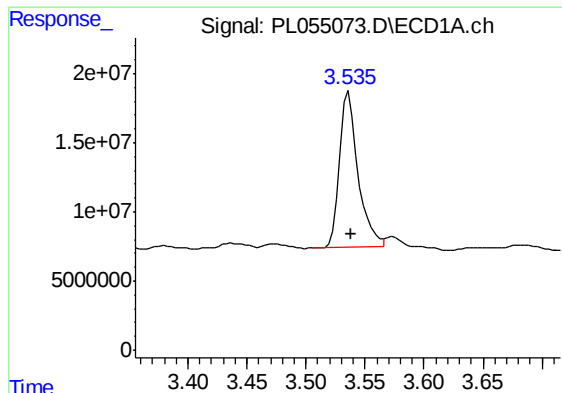


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 125399299
Conc: 10.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-2BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:49 AM

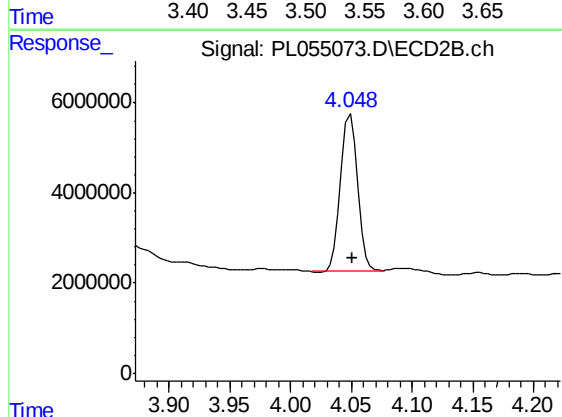


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.002 min
Response: 33948497
Conc: 13.30 ng/ml

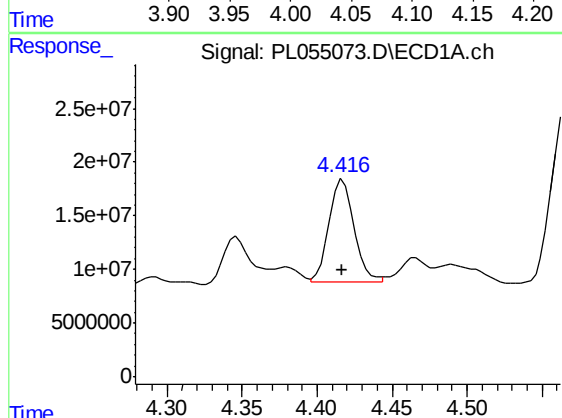


#23 Chlordane-1

R.T.: 4.417 min
Delta R.T.: 0.000 min
Response: 111845052
Conc: 260.63 ng/ml

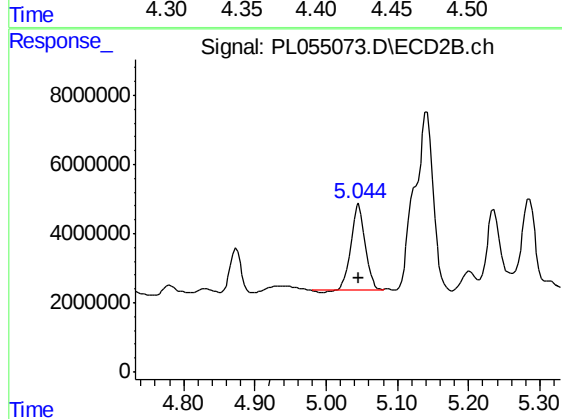

#23 Chlordane-1

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 34863410
Conc: 339.59 ng/ml

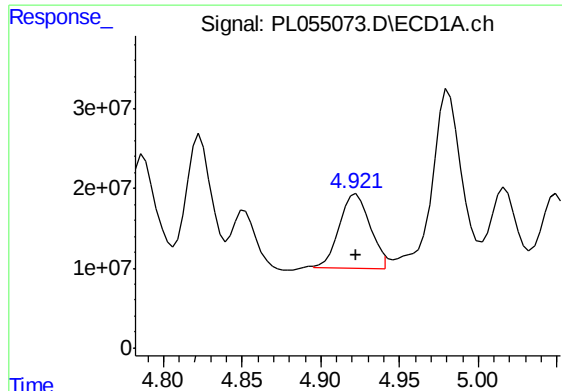


#24 Chlordane-2

R.T.: 4.921 min
Delta R.T.: -0.001 min
Response: 128532457
Conc: 273.87 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-2BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:49 AM

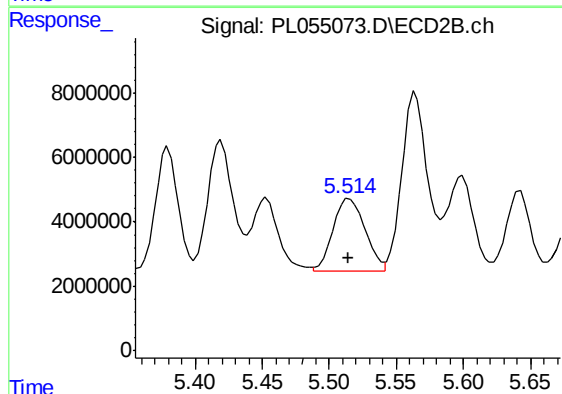


#24 Chlordane-2

R.T.: 5.515 min
Delta R.T.: 0.000 min
Response: 37481467
Conc: 352.75 ng/ml

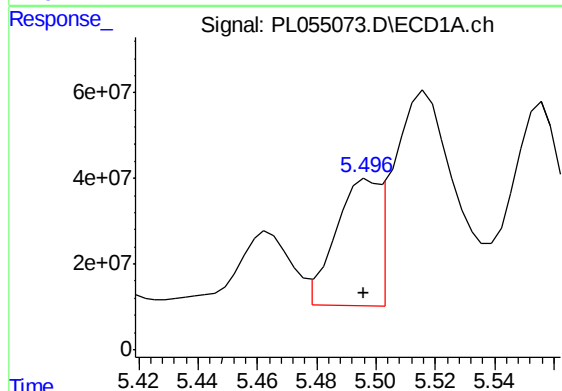


#25 Chlordane-3

R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 348296757
Conc: 258.43 ng/ml m

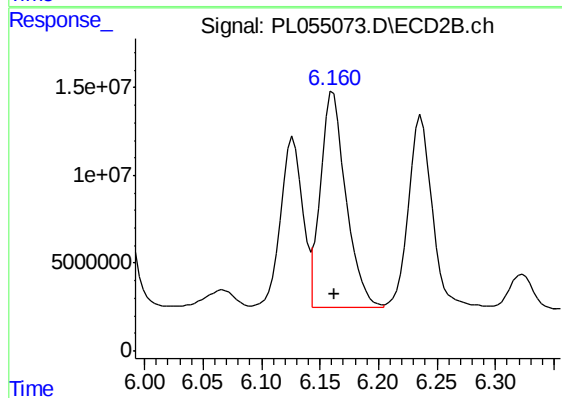

#25 Chlordane-3

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 184917093
Conc: 504.36 ng/ml

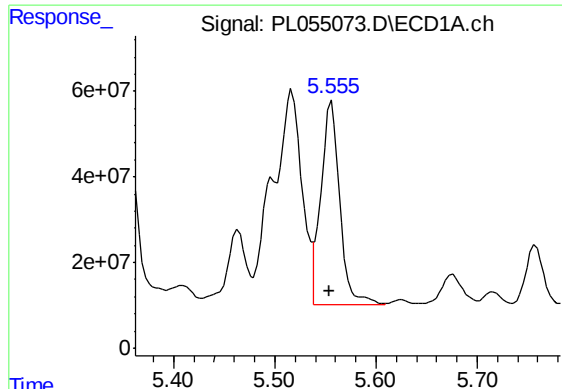


#26 Chlordane-4

R.T.: 5.556 min
Delta R.T.: 0.002 min
Response: 621032404
Conc: 560.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-2BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:49 AM

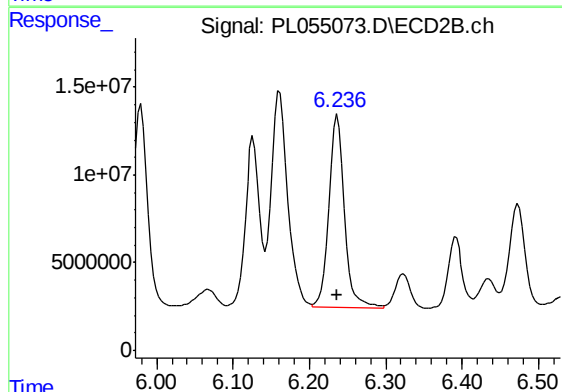


#26 Chlordane-4

R.T.: 6.237 min
Delta R.T.: 0.000 min
Response: 153659046
Conc: 353.33 ng/ml

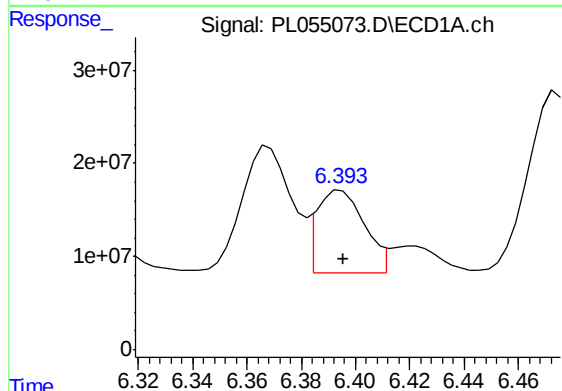


#27 Chlordane-5

R.T.: 6.393 min
Delta R.T.: -0.002 min
Response: 102034878
Conc: 275.89 ng/ml m

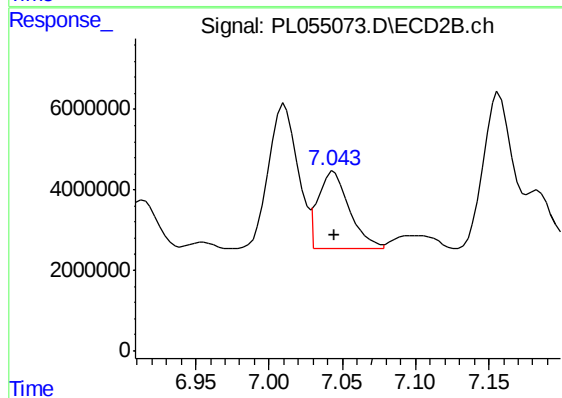

#27 Chlordane-5

R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 28708922
Conc: 379.88 ng/ml

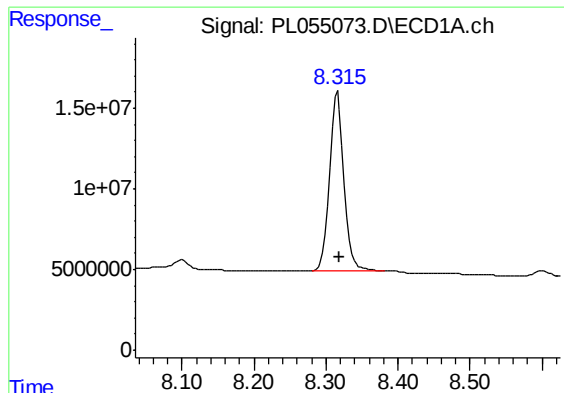


#28 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: -0.003 min
Response: 153900543
Conc: 16.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-2BD

Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:49 AM

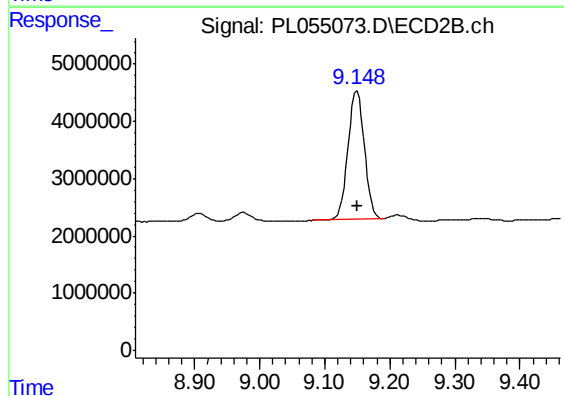

#28 Decachlorobiphenyl

R.T.: 9.149 min
Delta R.T.: -0.002 min
Response: 39091465
Conc: 16.31 ng/ml