

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
 Data File : PL055075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 15:54
 Operator : SG\AJ
 Sample : K6335-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-6BD

Manual Integrations
 APPROVED

Ankita
 12/19/2019 11:41:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 16:05:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:58:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.050	133.7E6	36118889	11.496	14.154
28)	SA Decachlor...	8.318	9.151	148.5E6	39556201	15.512	16.499
Target Compounds							
23)	Chlordane-1	4.420	5.047	140.5E6	42996063	327.294	418.805 #
24)	Chlordane-2	4.923	5.517	139.5E6	42948285	297.254m	404.197 #
25)	Chlordane-3	5.500	6.163	312.6E6	202.4E6	231.935	552.032 #
26)	Chlordane-4	5.558	6.238	688.1E6	174.6E6	620.632	401.493 #
27)	Chlordane-5	6.397	7.046	128.8E6	32817423	348.338	434.245

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
Data File : PL055075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 15:54
Operator : SG\AJ
Sample : K6335-03
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-6BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 16:05:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:58:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

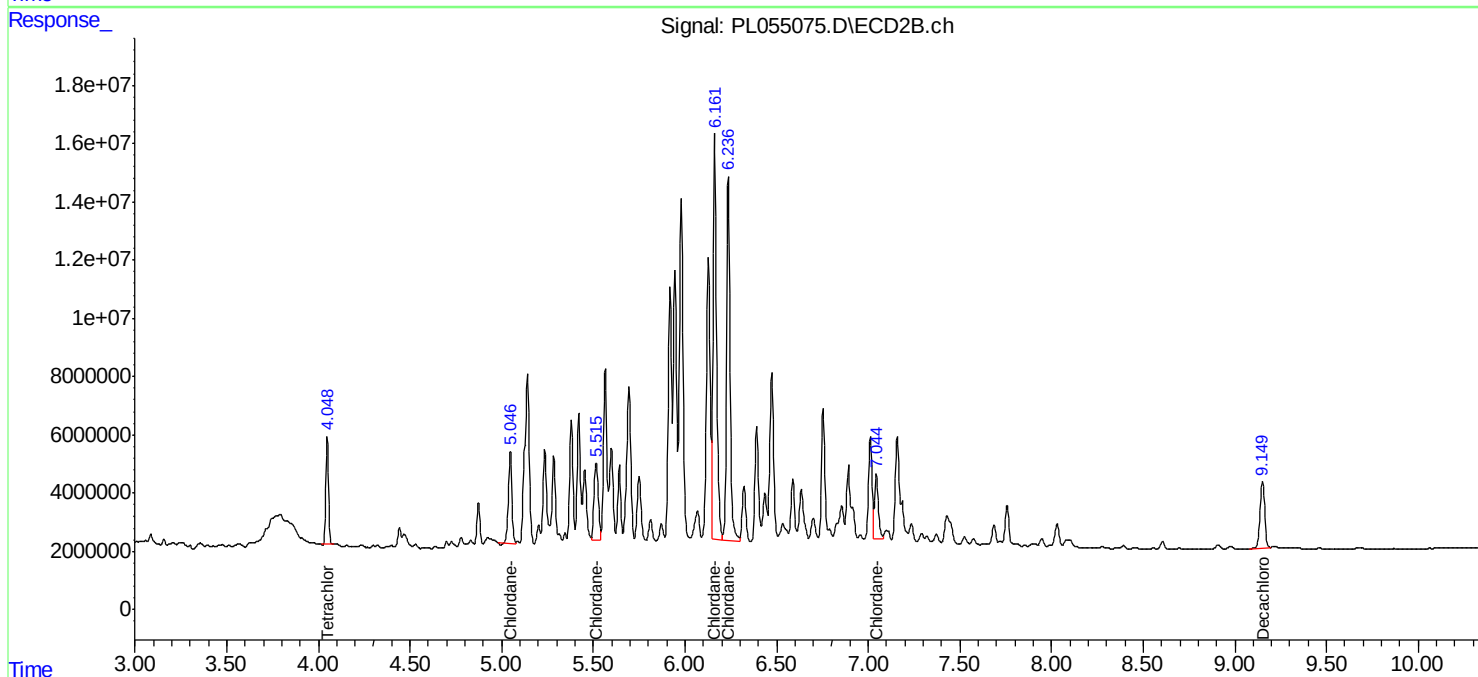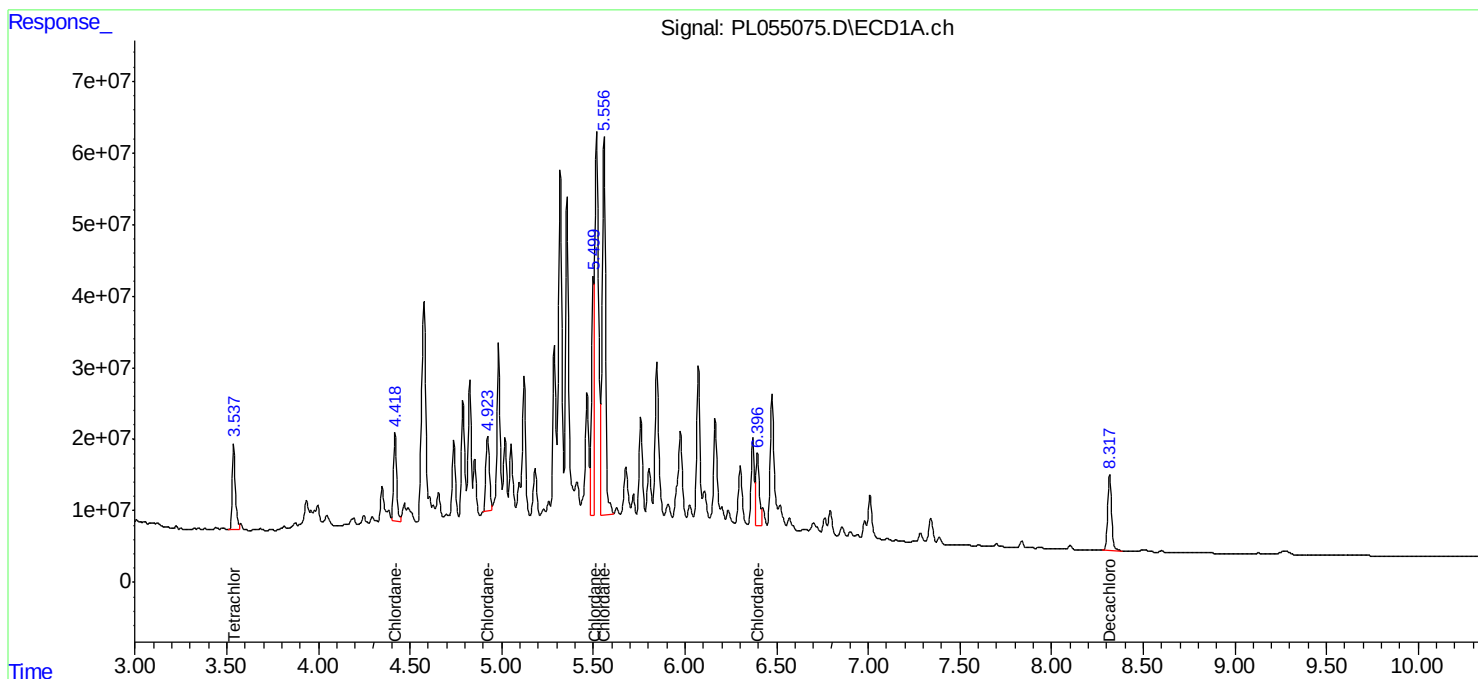

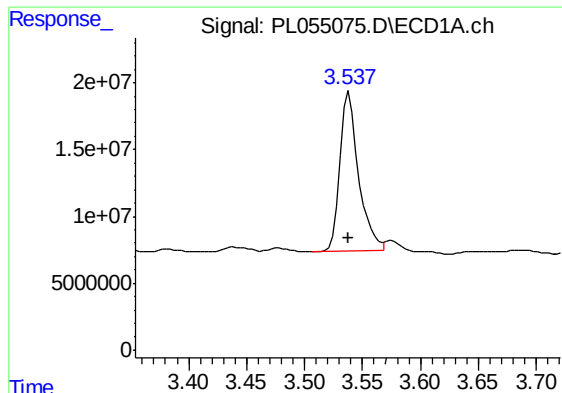


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 133748226
Conc: 11.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:53 AM

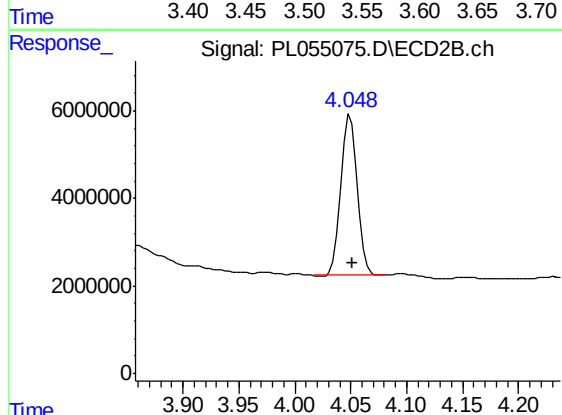


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 36118889
Conc: 14.15 ng/ml

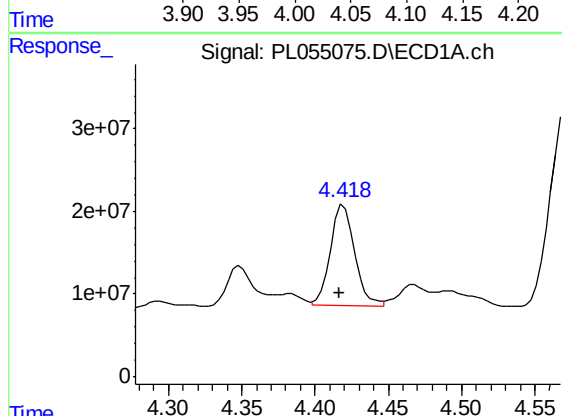


#23 Chlordane-1

R.T.: 4.420 min
Delta R.T.: 0.003 min
Response: 140453531
Conc: 327.29 ng/ml

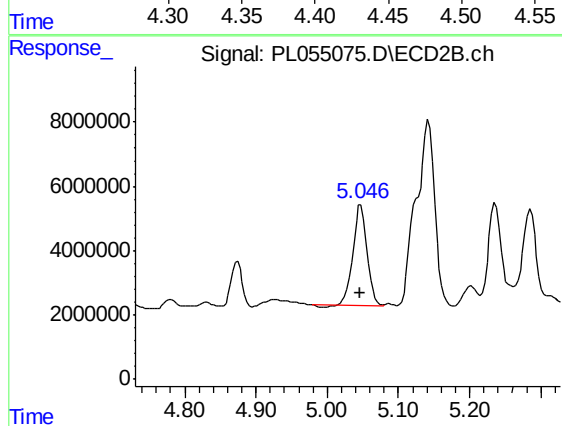

#23 Chlordane-1

R.T.: 5.047 min
Delta R.T.: 0.002 min
Response: 42996063
Conc: 418.80 ng/ml

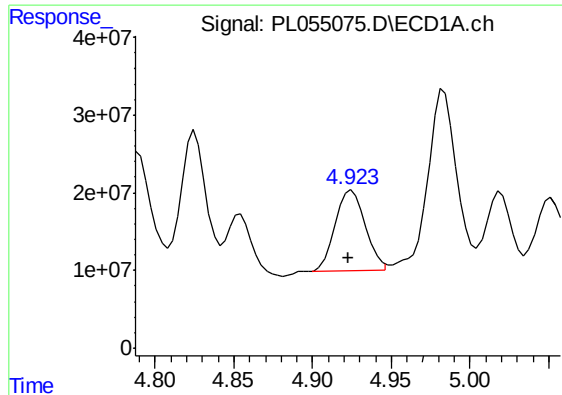


#24 Chlordane-2

R.T.: 4.923 min
Delta R.T.: 0.001 min
Response: 139505650
Conc: 297.25 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-6BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:53 AM

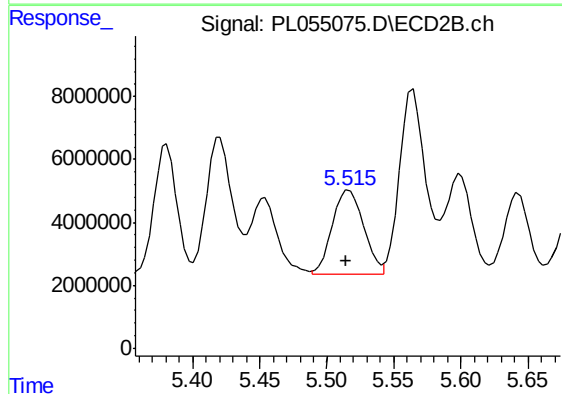


#24 Chlordane-2

R.T.: 5.517 min
Delta R.T.: 0.002 min
Response: 42948285
Conc: 404.20 ng/ml

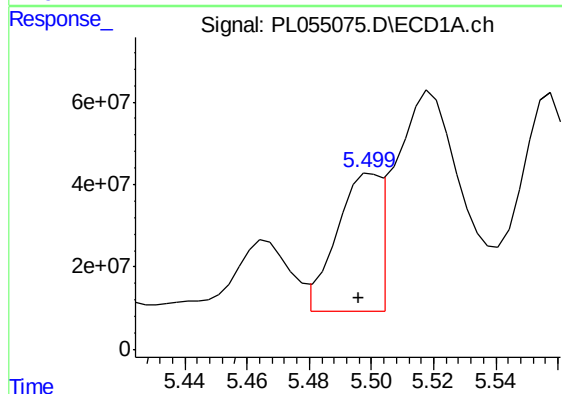


#25 Chlordane-3

R.T.: 5.500 min
Delta R.T.: 0.004 min
Response: 312588095
Conc: 231.94 ng/ml

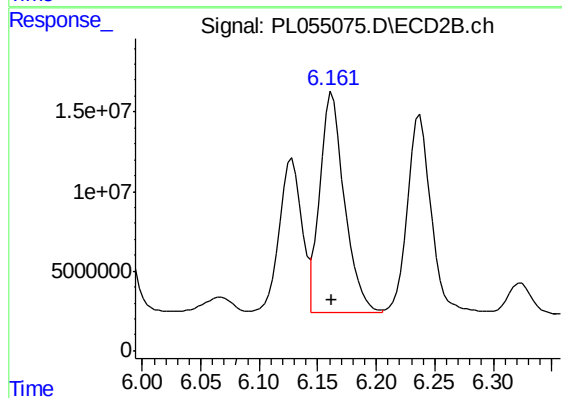

#25 Chlordane-3

R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 202397013
Conc: 552.03 ng/ml

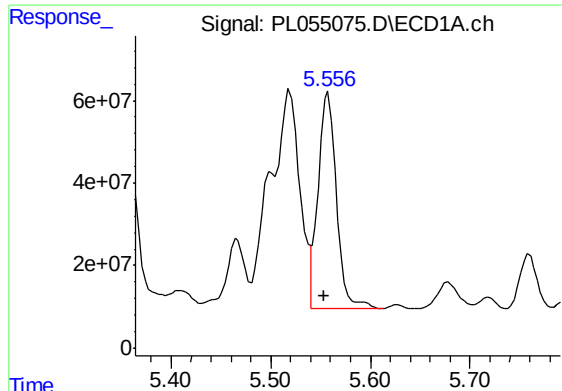


#26 Chlordane-4

R.T.: 5.558 min
Delta R.T.: 0.004 min
Response: 688102379
Conc: 620.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:53 AM

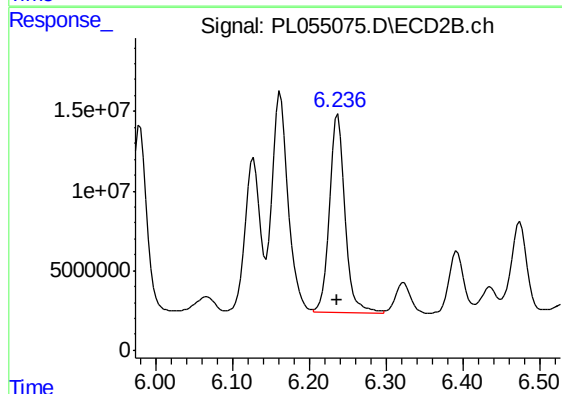


#26 Chlordane-4

R.T.: 6.238 min
Delta R.T.: 0.000 min
Response: 174602140
Conc: 401.49 ng/ml

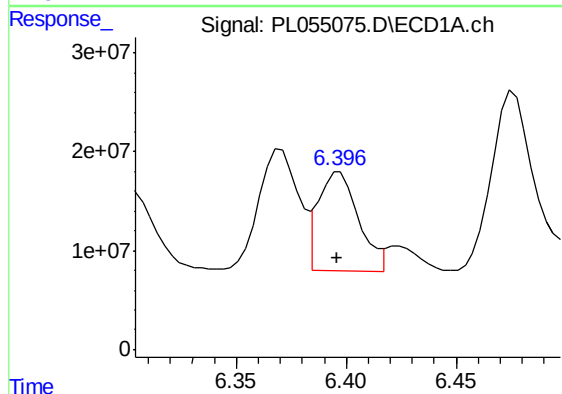


#27 Chlordane-5

R.T.: 6.397 min
Delta R.T.: 0.001 min
Response: 128826688
Conc: 348.34 ng/ml

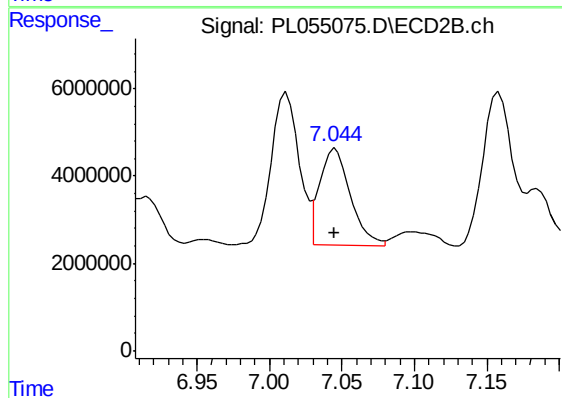

#27 Chlordane-5

R.T.: 7.046 min
Delta R.T.: 0.001 min
Response: 32817423
Conc: 434.24 ng/ml

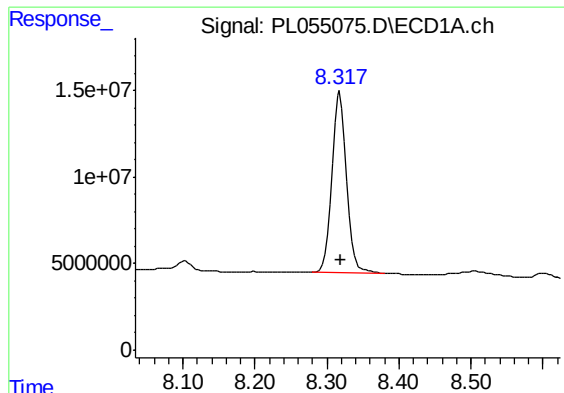


#28 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: 0.000 min
Response: 148547452
Conc: 15.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6BD

Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:53 AM

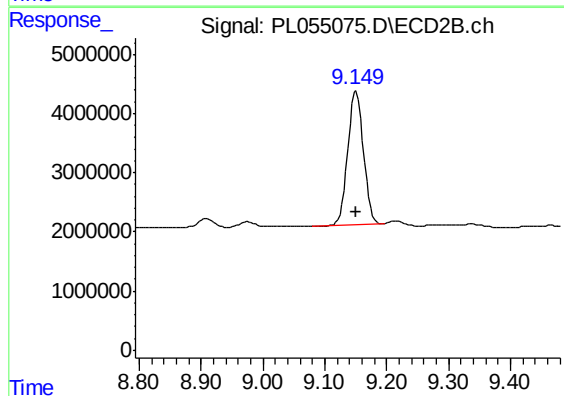

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 39556201
Conc: 16.50 ng/ml