

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
 Data File : PL055076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 16:08
 Operator : SG\AJ
 Sample : K6335-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-7BD

Manual Integrations
 APPROVED

Ankita
 12/19/2019 11:41:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 16:27:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:58:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.049	129.3E6	35507963	11.111	13.915 #
28)	SA Decachlor...	8.316	9.150	146.1E6	40405760	15.254	16.854
Target Compounds							
23)	Chlordane-1	4.418	5.046	122.4E6	36292731	285.127	353.511
24)	Chlordane-2	4.922	5.515	144.0E6	39996251	306.864m	376.415
25)	Chlordane-3	5.498	6.162	276.6E6	165.9E6	205.262	452.406 #
26)	Chlordane-4	5.556	6.237	559.4E6	156.2E6	504.516	359.229 #
27)	Chlordane-5	6.395	7.045	115.5E6	29973925	312.276	396.619 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
Data File : PL055076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 16:08
Operator : SG\AJ
Sample : K6335-04
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-7BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 16:27:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:58:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

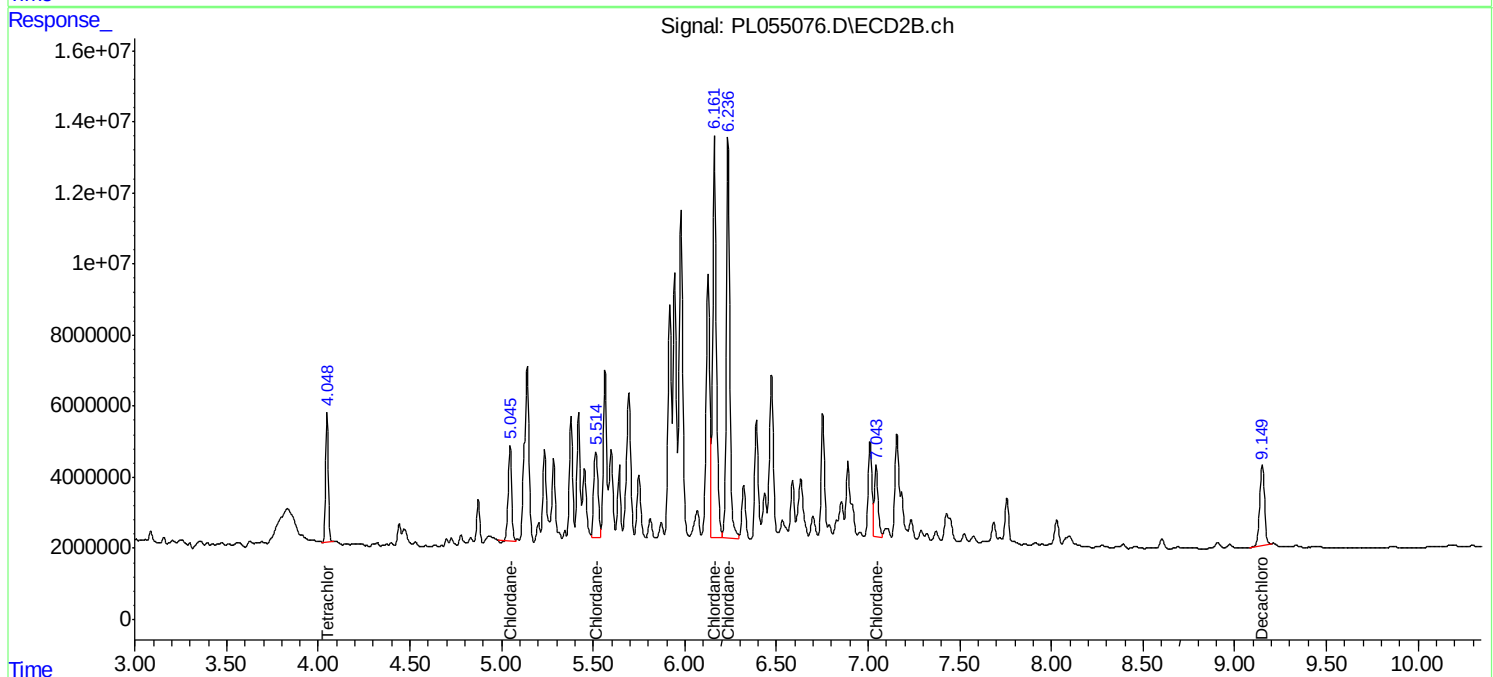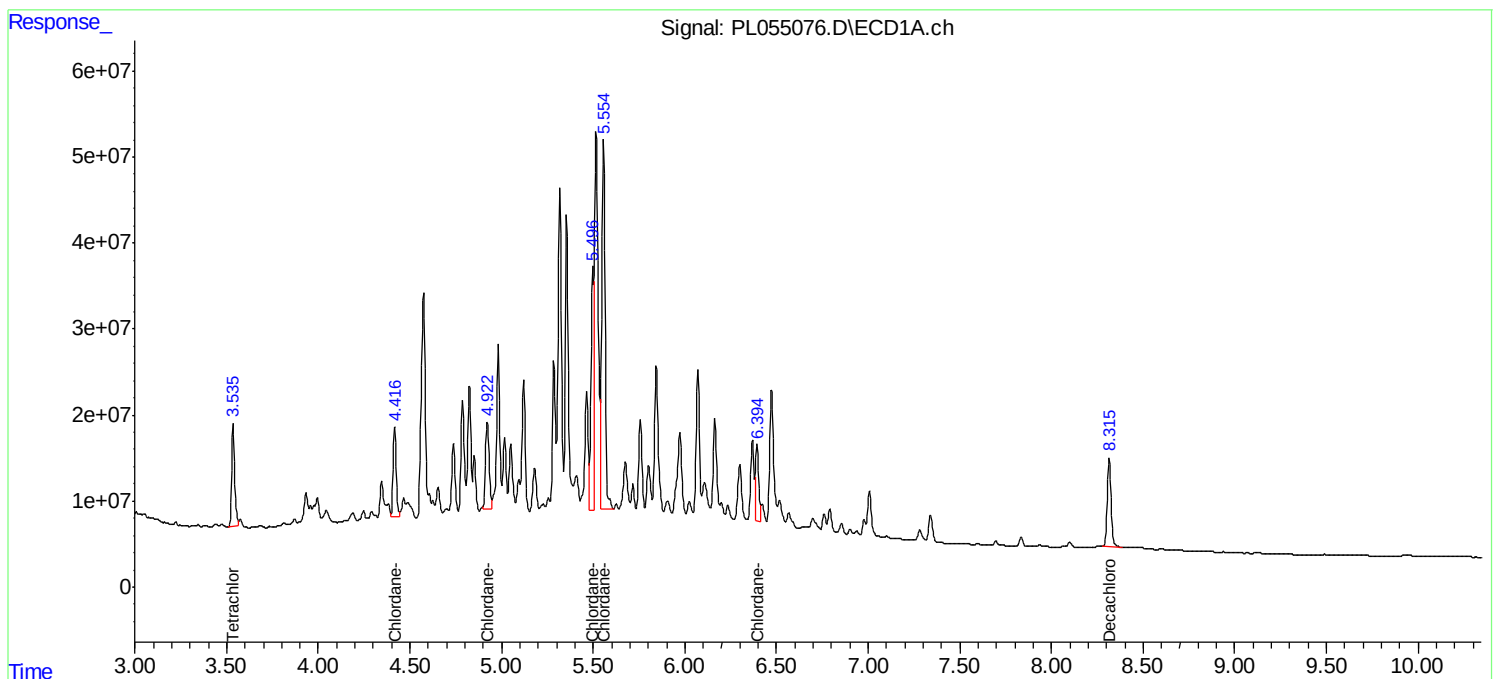

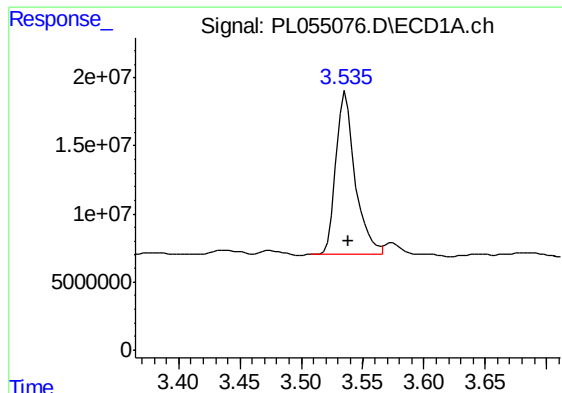


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 129269791
Conc: 11.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:55 AM

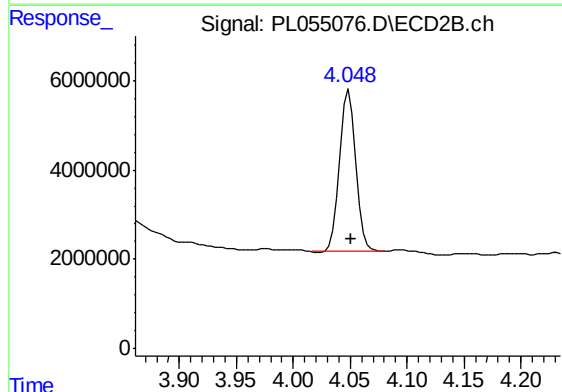


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.002 min
Response: 35507963
Conc: 13.91 ng/ml

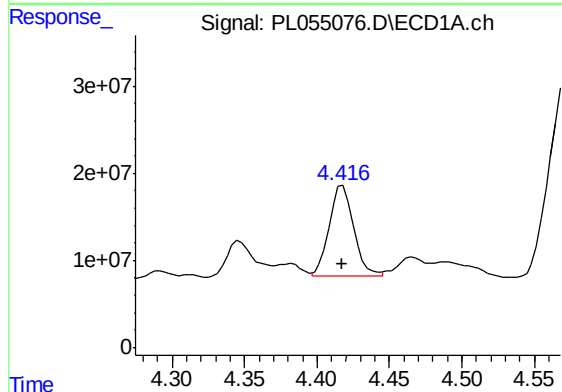


#23 Chlordane-1

R.T.: 4.418 min
Delta R.T.: 0.000 min
Response: 122357953
Conc: 285.13 ng/ml

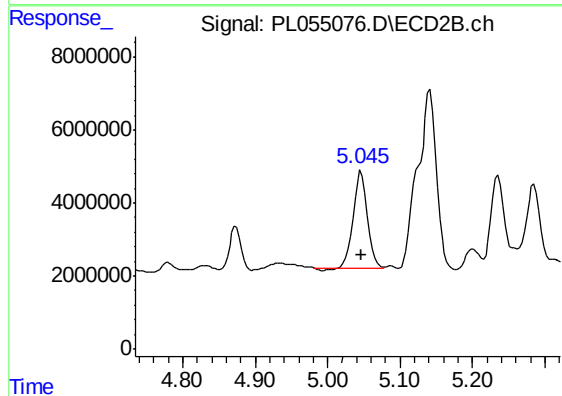

#23 Chlordane-1

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 36292731
Conc: 353.51 ng/ml

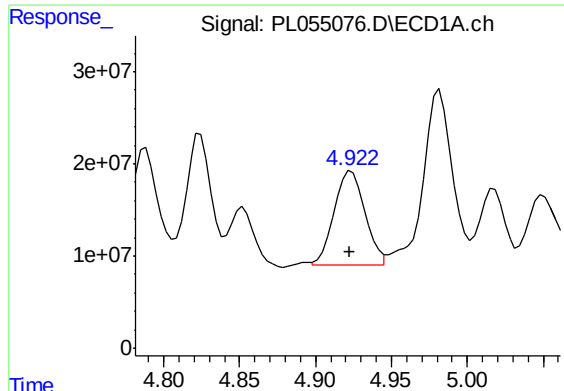


#24 Chlordane-2

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 144015665
Conc: 306.86 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-7BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:55 AM

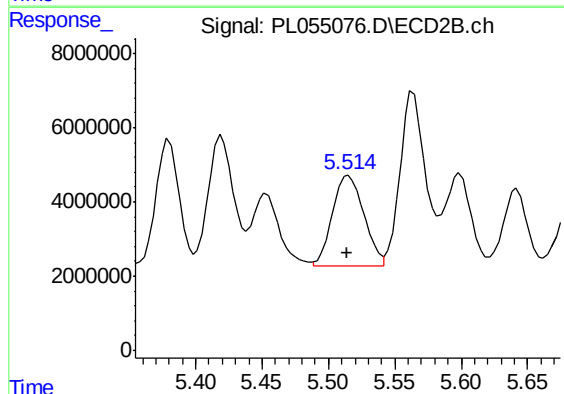


#24 Chlordane-2

R.T.: 5.515 min
Delta R.T.: 0.000 min
Response: 39996251
Conc: 376.41 ng/ml

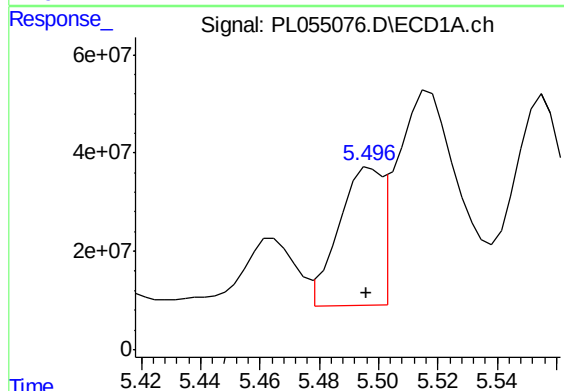


#25 Chlordane-3

R.T.: 5.498 min
Delta R.T.: 0.002 min
Response: 276640136
Conc: 205.26 ng/ml

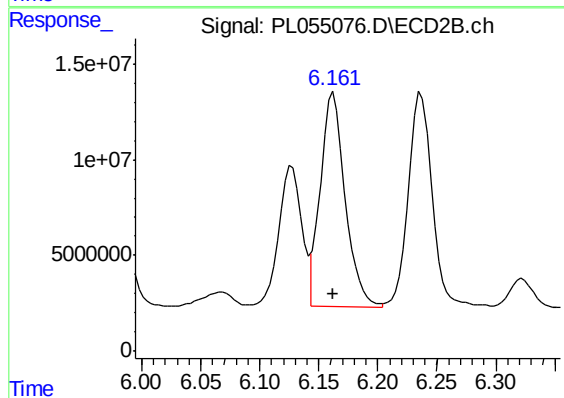

#25 Chlordane-3

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 165870197
Conc: 452.41 ng/ml

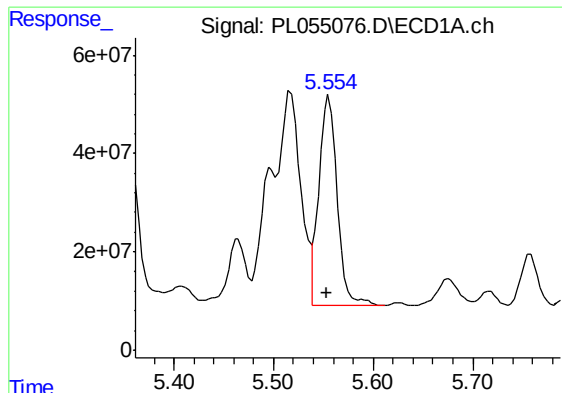


#26 Chlordane-4

R.T.: 5.556 min
Delta R.T.: 0.002 min
Response: 559362392
Conc: 504.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7BD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:55 AM

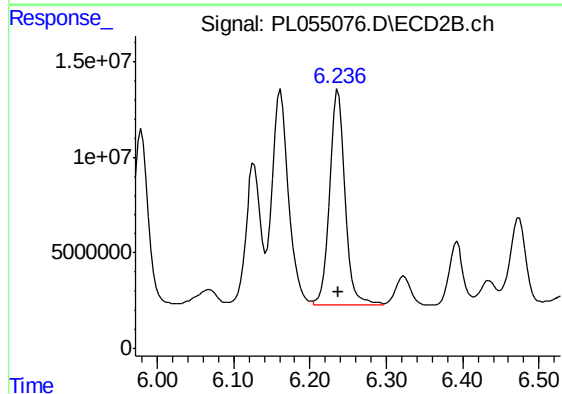


#26 Chlordane-4

R.T.: 6.237 min
Delta R.T.: 0.000 min
Response: 156222411
Conc: 359.23 ng/ml

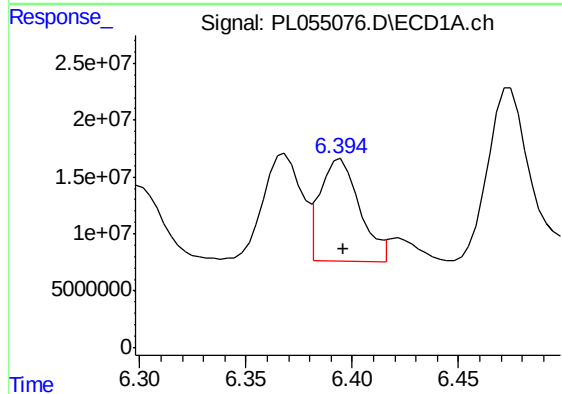


#27 Chlordane-5

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 115489922
Conc: 312.28 ng/ml

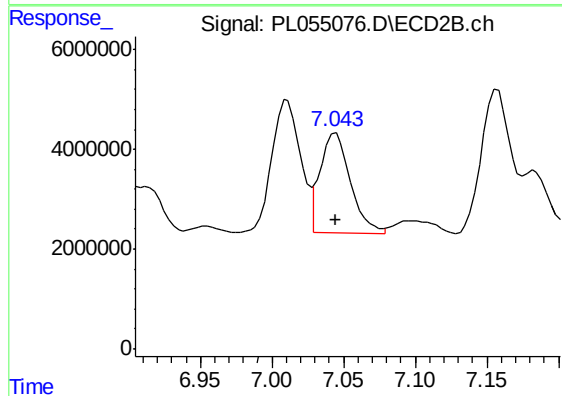

#27 Chlordane-5

R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 29973925
Conc: 396.62 ng/ml

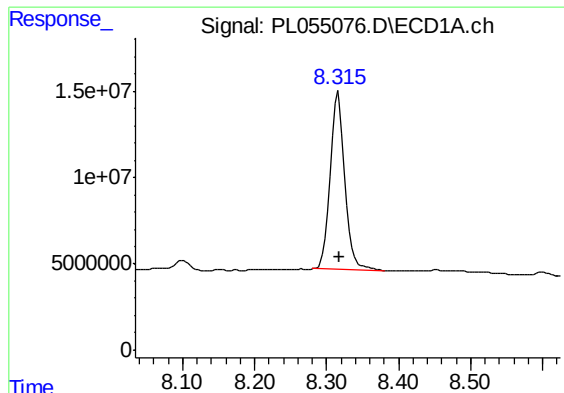


#28 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: -0.003 min
Response: 146073734
Conc: 15.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7BD

Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:55 AM

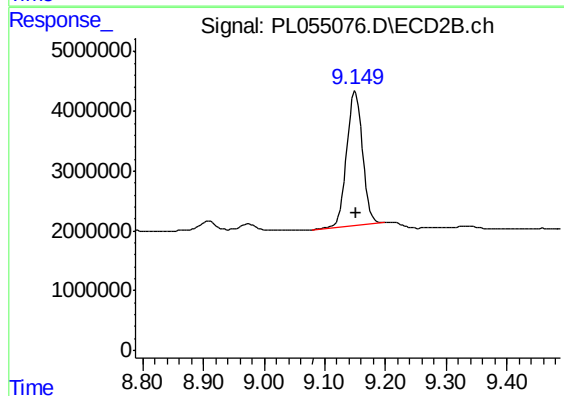

#28 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: 0.000 min
Response: 40405760
Conc: 16.85 ng/ml