

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
 Data File : PL055077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 16:22
 Operator : SG\AJ
 Sample : K6335-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-1AD

Manual Integrations
 APPROVED

Ankita
 12/19/2019 11:41:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 16:33:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:58:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.050	128.1E6	34255195	11.010	13.424
28)	SA Decachlor...	8.316	9.150	138.0E6	38141736	14.413	15.909
Target Compounds							
23)	Chlordane-1	4.417	5.047	118.1E6	43714289	275.121	425.801 #
24)	Chlordane-2	4.921	5.516	131.7E6	37340351	280.532m	351.420 #
25)	Chlordane-3	5.498	6.162	266.0E6	165.3E6	197.331	450.957 #
26)	Chlordane-4	5.555	6.237	567.4E6	153.1E6	511.772	352.012 #
27)	Chlordane-5	6.393	7.045	100.9E6	28773171	272.814m	380.730 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121819\
Data File : PL055077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 16:22
Operator : SG\AJ
Sample : K6335-05
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-1AD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 16:33:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:58:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

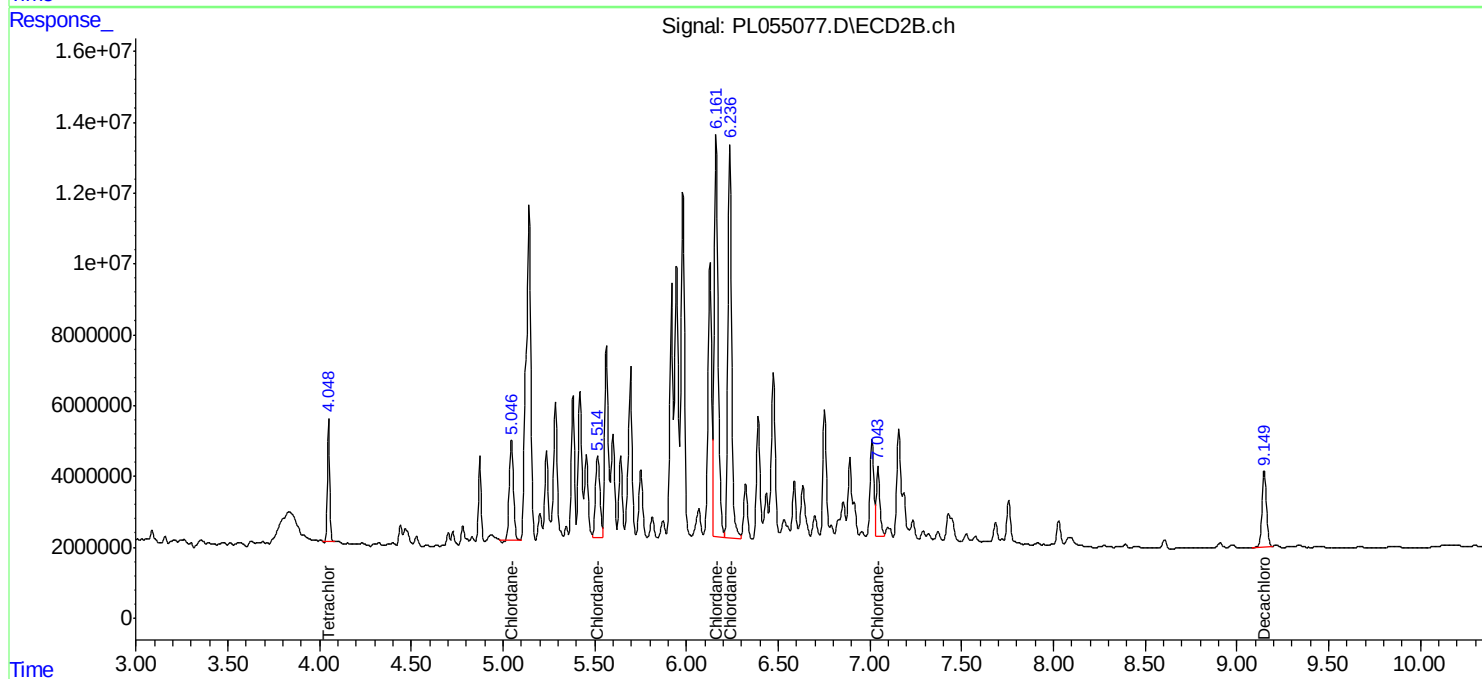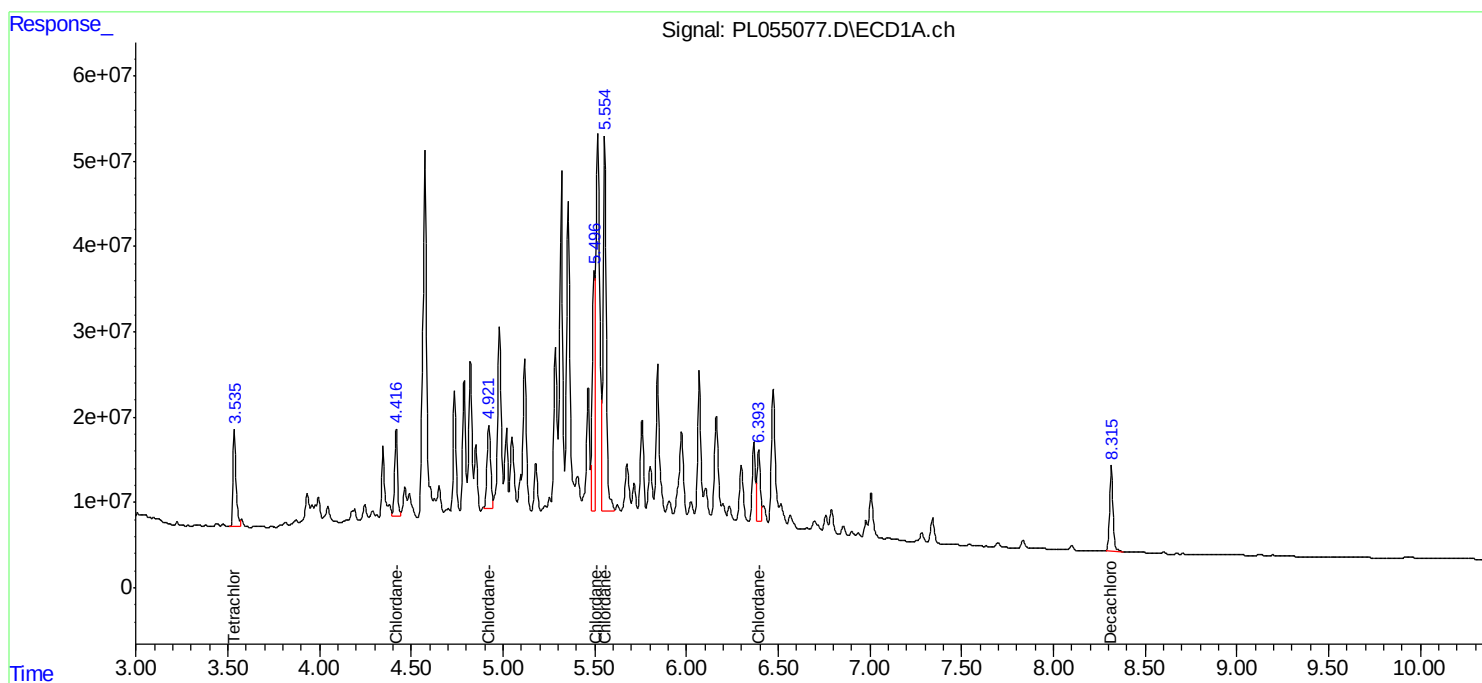

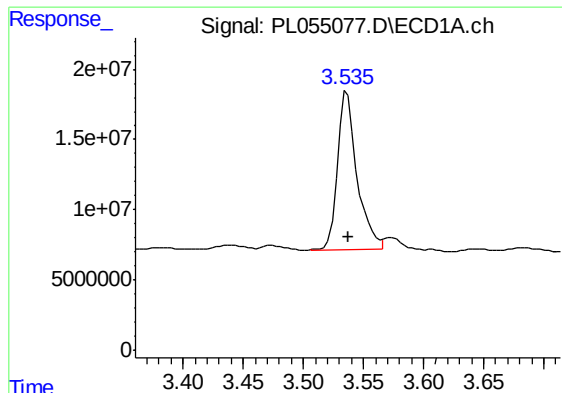


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 128096525
Conc: 11.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-1AD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:56 AM

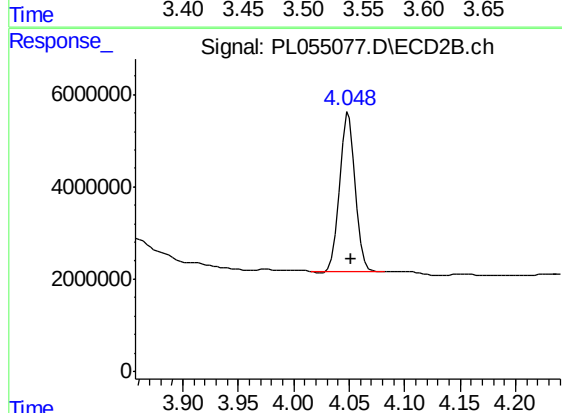


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 34255195
Conc: 13.42 ng/ml

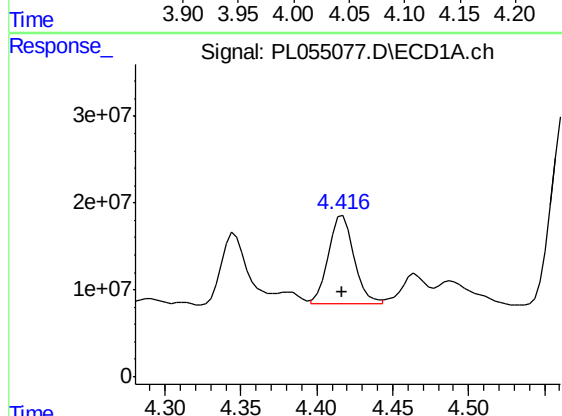


#23 Chlordane-1

R.T.: 4.417 min
Delta R.T.: 0.000 min
Response: 118064180
Conc: 275.12 ng/ml

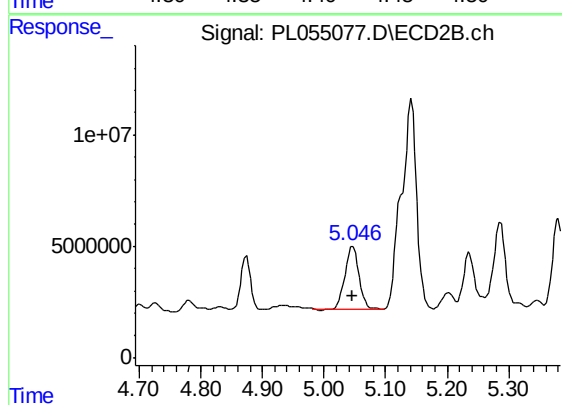

#23 Chlordane-1

R.T.: 5.047 min
Delta R.T.: 0.001 min
Response: 43714289
Conc: 425.80 ng/ml

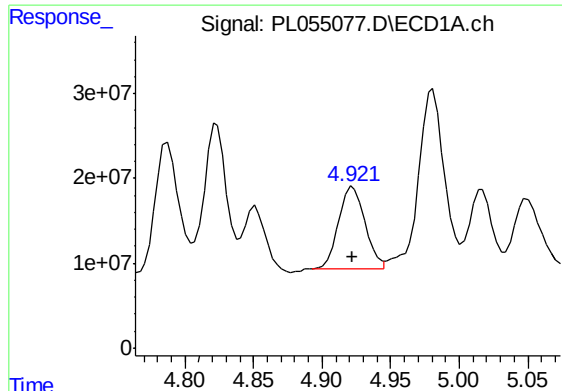


#24 Chlordane-2

R.T.: 4.921 min
Delta R.T.: -0.001 min
Response: 131657446
Conc: 280.53 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-1AD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:56 AM

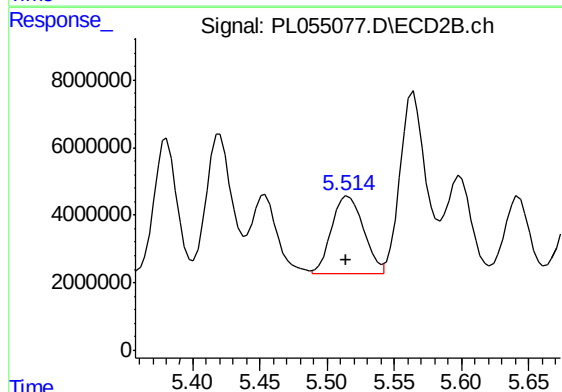


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: 0.001 min
Response: 37340351
Conc: 351.42 ng/ml

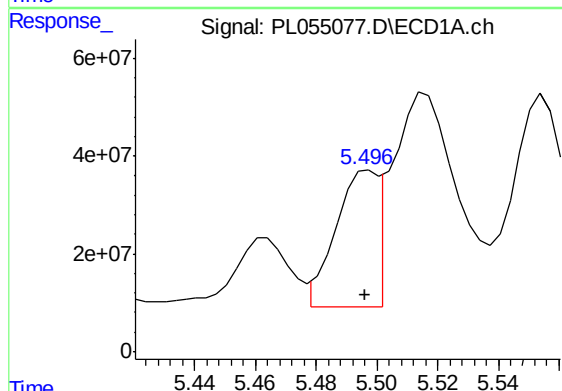


#25 Chlordane-3

R.T.: 5.498 min
Delta R.T.: 0.002 min
Response: 265950326
Conc: 197.33 ng/ml

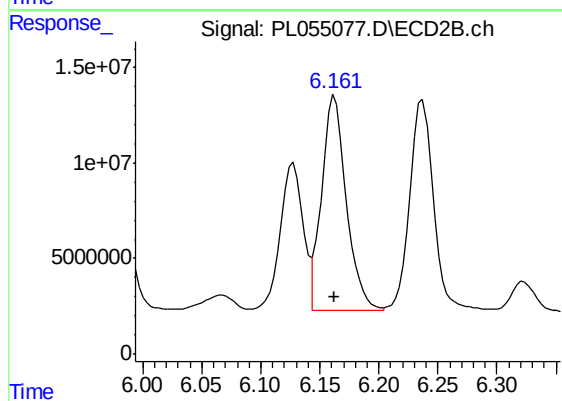

#25 Chlordane-3

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 165338892
Conc: 450.96 ng/ml

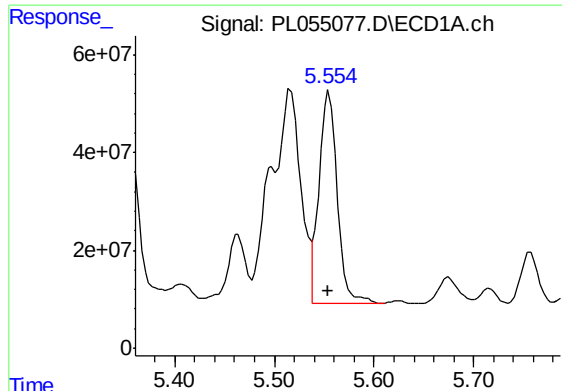


#26 Chlordane-4

R.T.: 5.555 min
Delta R.T.: 0.001 min
Response: 567407797
Conc: 511.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-1AD


Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:56 AM

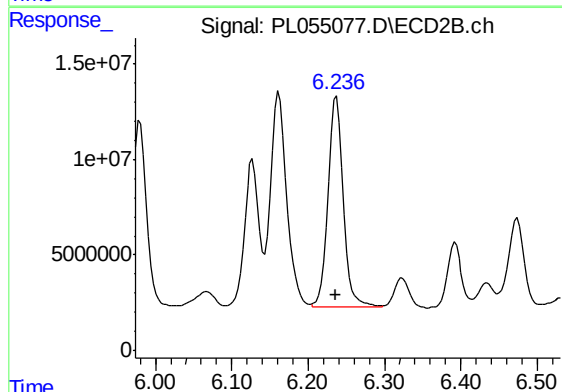


#26 Chlordane-4

R.T.: 6.237 min
Delta R.T.: 0.000 min
Response: 153083985
Conc: 352.01 ng/ml

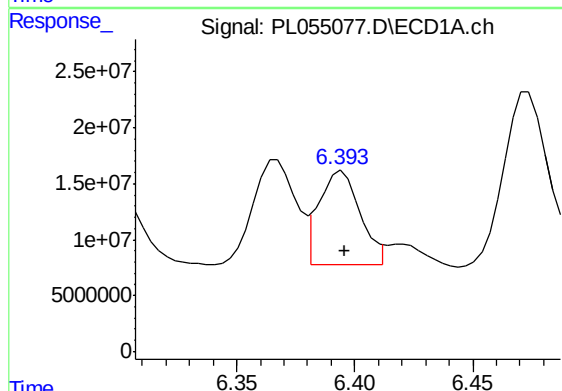


#27 Chlordane-5

R.T.: 6.393 min
Delta R.T.: -0.002 min
Response: 100895637
Conc: 272.81 ng/ml m

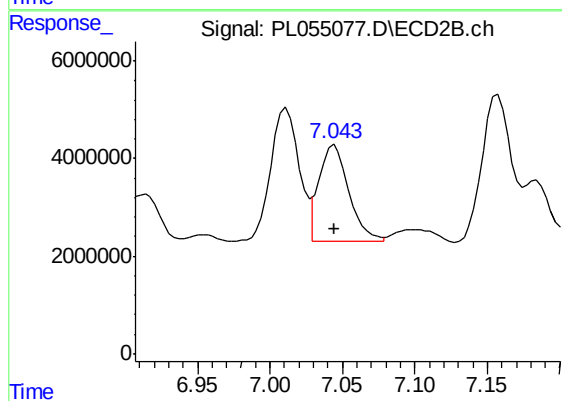

#27 Chlordane-5

R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 28773171
Conc: 380.73 ng/ml

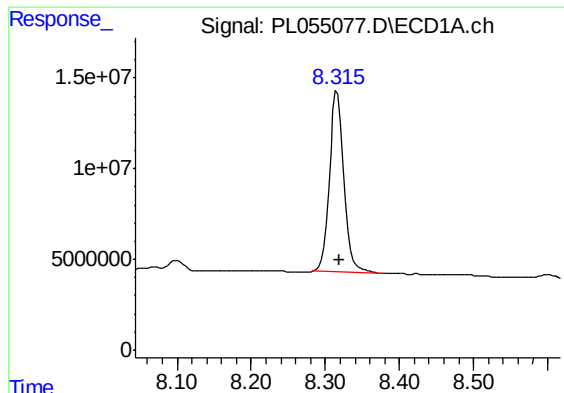


#28 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: -0.002 min
Response: 138023386
Conc: 14.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-1AD

Manual Integrations
APPROVED

Ankita
12/19/2019 11:41:56 AM

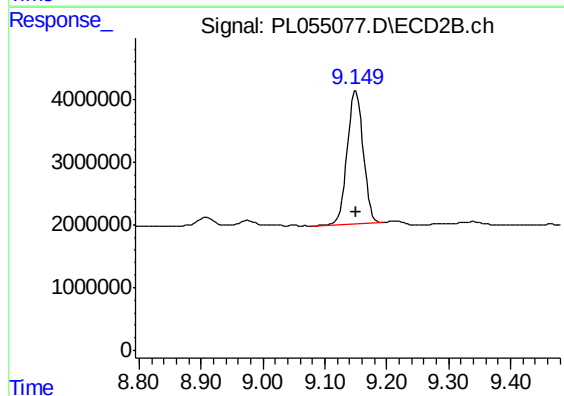

#28 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: 0.000 min
Response: 38141736
Conc: 15.91 ng/ml