

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121824\
 Data File : PL093419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2024 16:32
 Operator : AR\AJ
 Sample : P5312-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CONCRETE-VNJ-222

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/19/2024
 Supervised By : Ankita Jodhani 12/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 04:28:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 15:18:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.538	2.775	58489327	63553576	22.505m	22.036
28) SA Decachlor...	9.054	7.912	43522761	53936988	25.034m	18.882

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121824\
Data File : PL093419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2024 16:32
Operator : AR\AJ
Sample : P5312-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CONCRETE-VNJ-222


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/19/2024
Supervised By : Ankita Jodhani 12/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 04:28:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 15:18:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

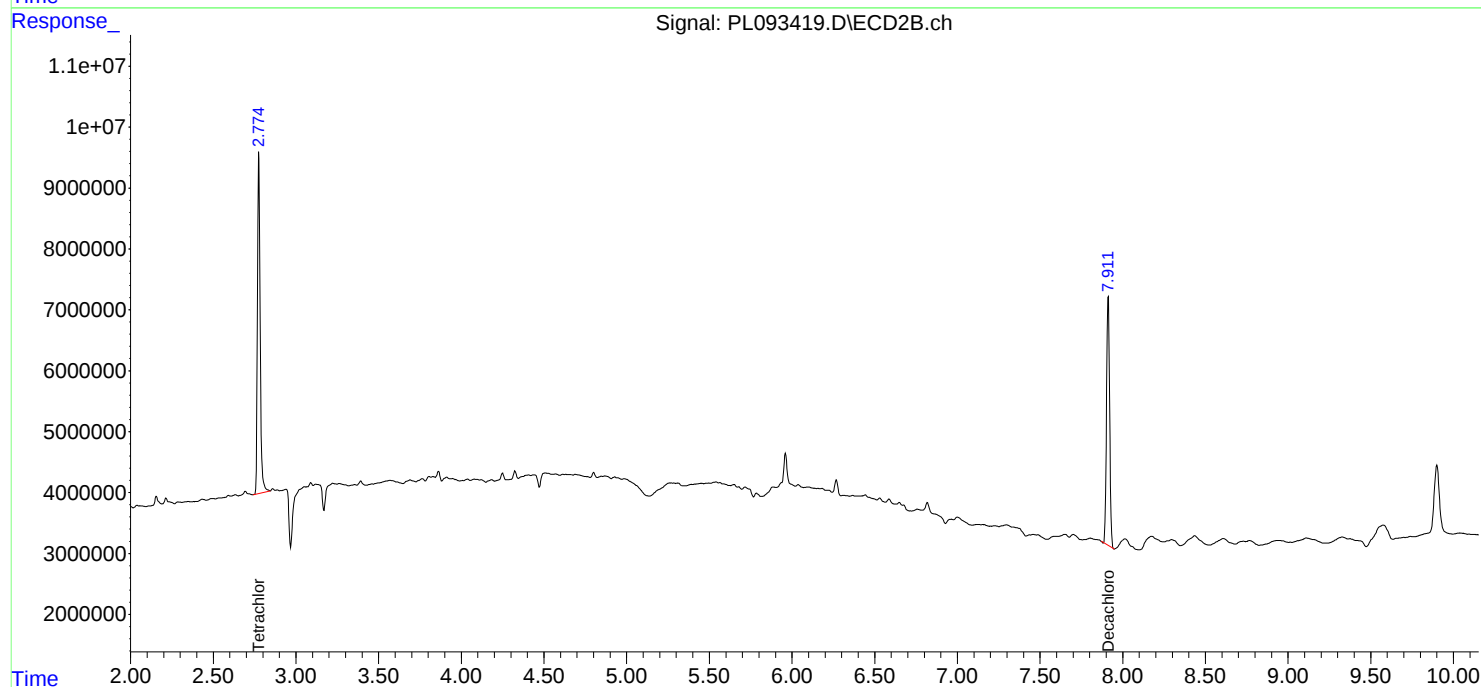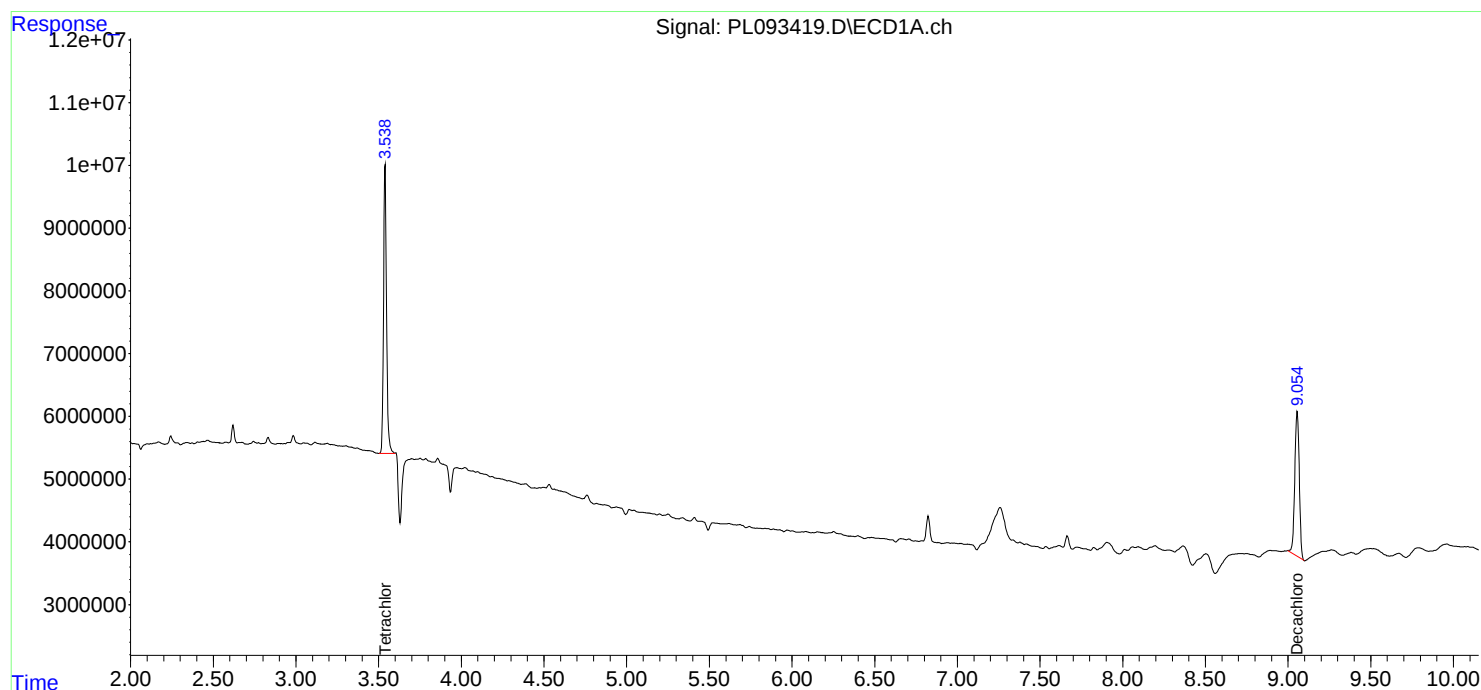

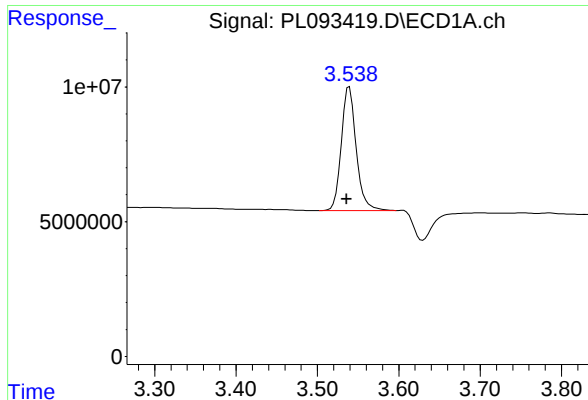

#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.002 min
Response: 58489327
Conc: 22.50 ng/ml

Instrument :


ECD_L

ClientSampleId :

CONCRETE-VNJ-222


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/19/2024
Supervised By :Ankita Jodhani 12/19/2024

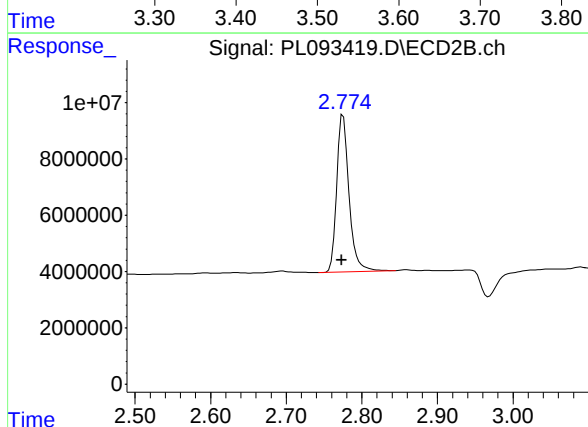


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.002 min
Response: 63553576
Conc: 22.04 ng/ml

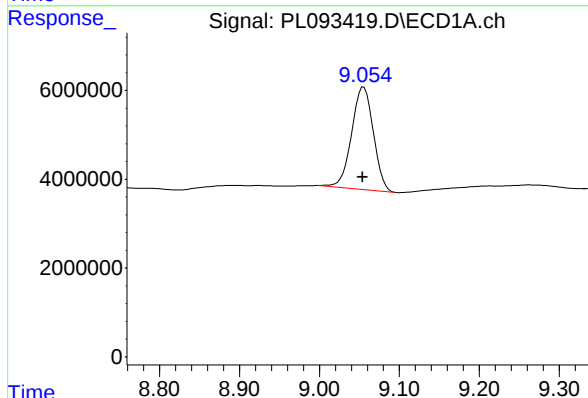

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 43522761
Conc: 25.03 ng/ml m

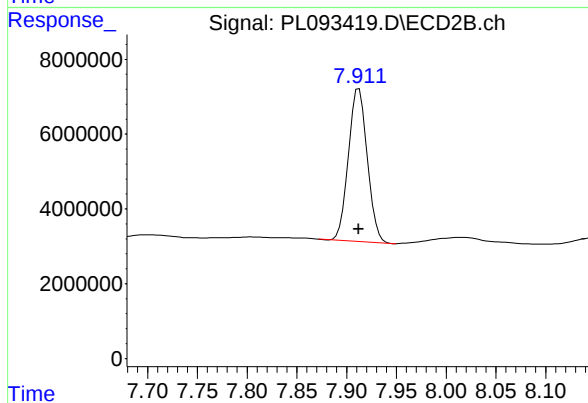

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 53936988
Conc: 18.88 ng/ml