

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121824\
 Data File : PL093420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2024 16:45
 Operator : AR\AJ
 Sample : P5316-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TT-304-IDWSO-20241217-1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/19/2024
 Supervised By :Ankita Jodhani 12/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 04:28:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 15:18:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.537	2.776	44354749	49588982	17.066m	17.194
28) SA Decachlor...	9.055	7.912	29993069	45526386	17.252m	15.938m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121824\
Data File : PL093420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2024 16:45
Operator : AR\AJ
Sample : P5316-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TT-304-IDWSO-20241217-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/19/2024
Supervised By : Ankita Jodhani 12/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 04:28:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 15:18:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

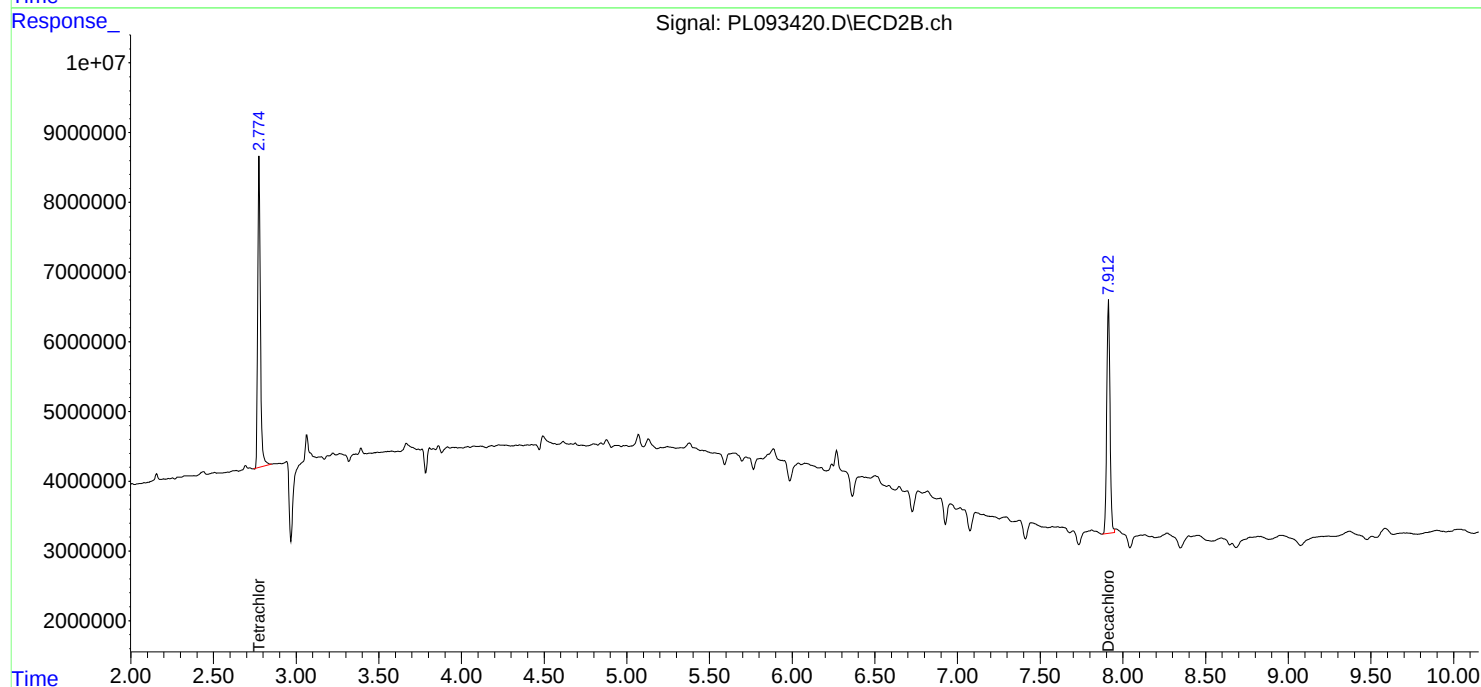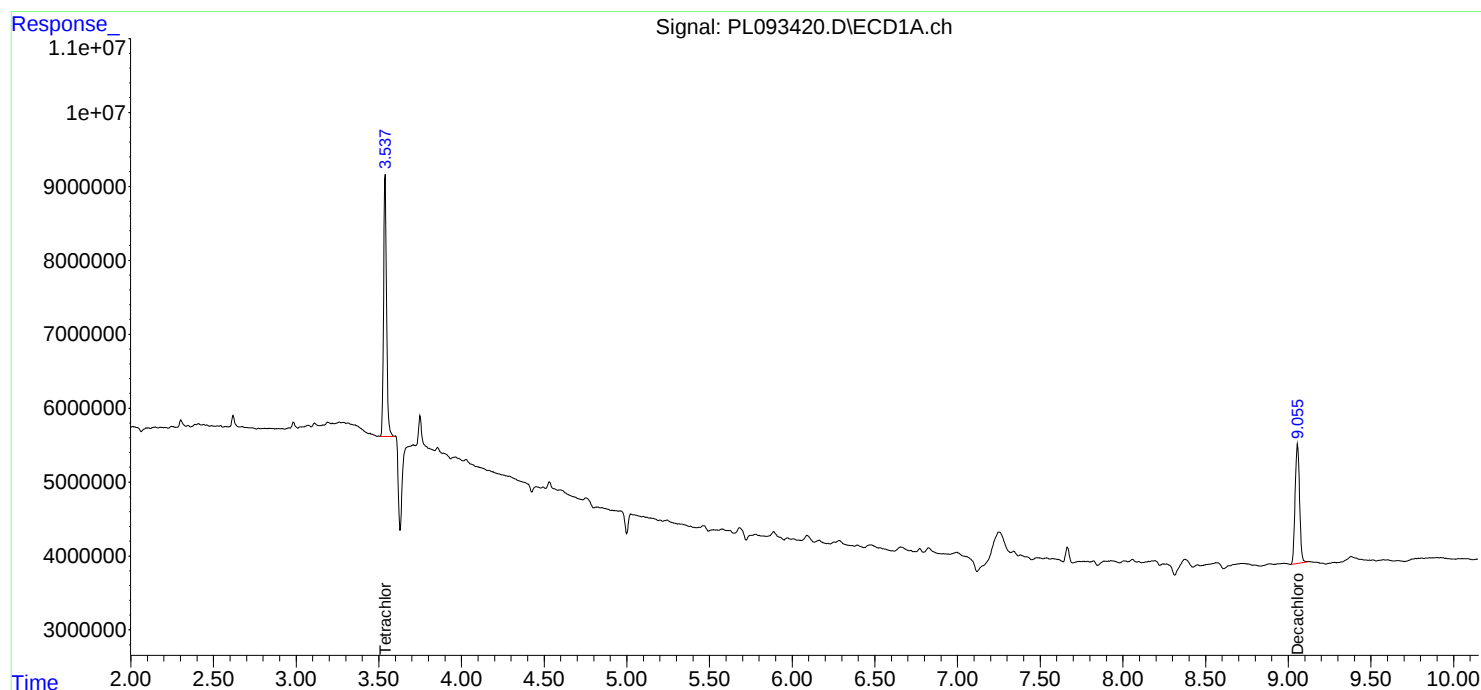

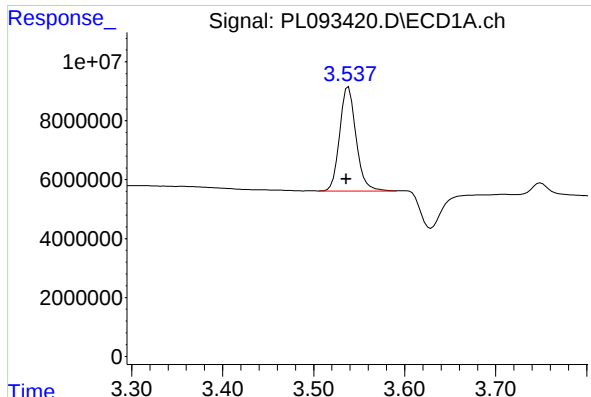


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 44354749
Conc: 17.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
TT-304-IDWSO-20241217-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/19/2024
Supervised By :Ankita Jodhani 12/19/2024

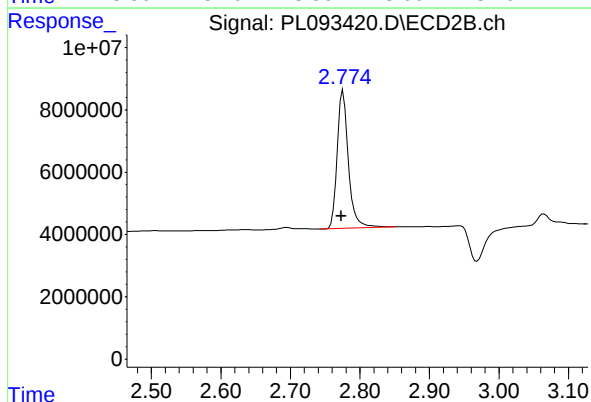


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.002 min
Response: 49588982
Conc: 17.19 ng/ml

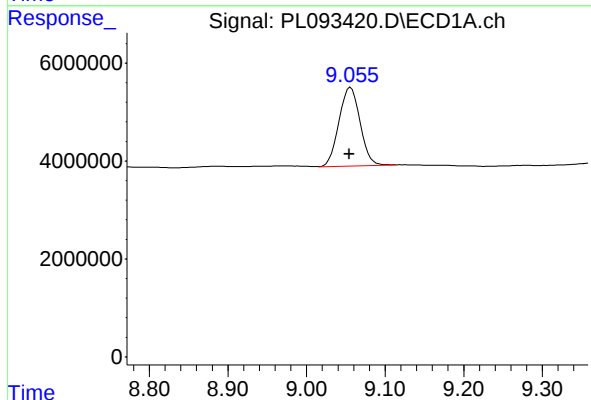

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 29993069
Conc: 17.25 ng/ml m

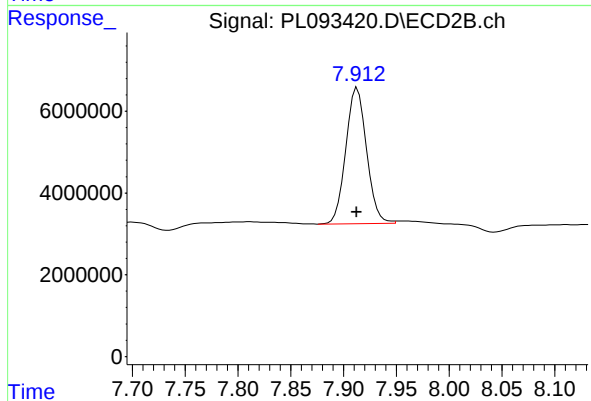

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 45526386
Conc: 15.94 ng/ml m