

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121918\
 Data File : PL043326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2018 22:56
 Operator : AJ\SJ
 Sample : J6453-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 00:36:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.099	125.8E6	65206102	20.507	22.000
28)	SA Decachlor...	8.199	9.228	125.2E6	56352270	19.171	21.603
Target Compounds							
3)	MA gamma-BHC...	0.000	4.745f	0	3927156	N.D.	0.936 #
6)	B beta-BHC	4.396f	4.903f	8959145	1706259	2.429	1.008 #
7)	B delta-BHC	0.000	5.145f	0	1531693	N.D.	0.356 #
8)	B Heptachlo...	0.000	6.001	0	3017032	N.D.	0.796 #
9)	A Endosulfan I	5.540	0.000	1484987	0	0.203	N.D. #
14)	MA Endrin	6.066f	0.000	759314	0	0.105	N.D. #
16)	A 4,4'-DDD	6.066f	0.000	759314	0	0.134	N.D. #
20)	A Methoxychlor	6.919	0.000	2417611	0	0.721	N.D. #
23)	Chlordane-1	4.396	5.145	8959145	1531693	33.342	10.837 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121918\
Data File : PL043326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2018 22:56
Operator : AJ\SJ
Sample : J6453-03
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 00:36:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25 μ m

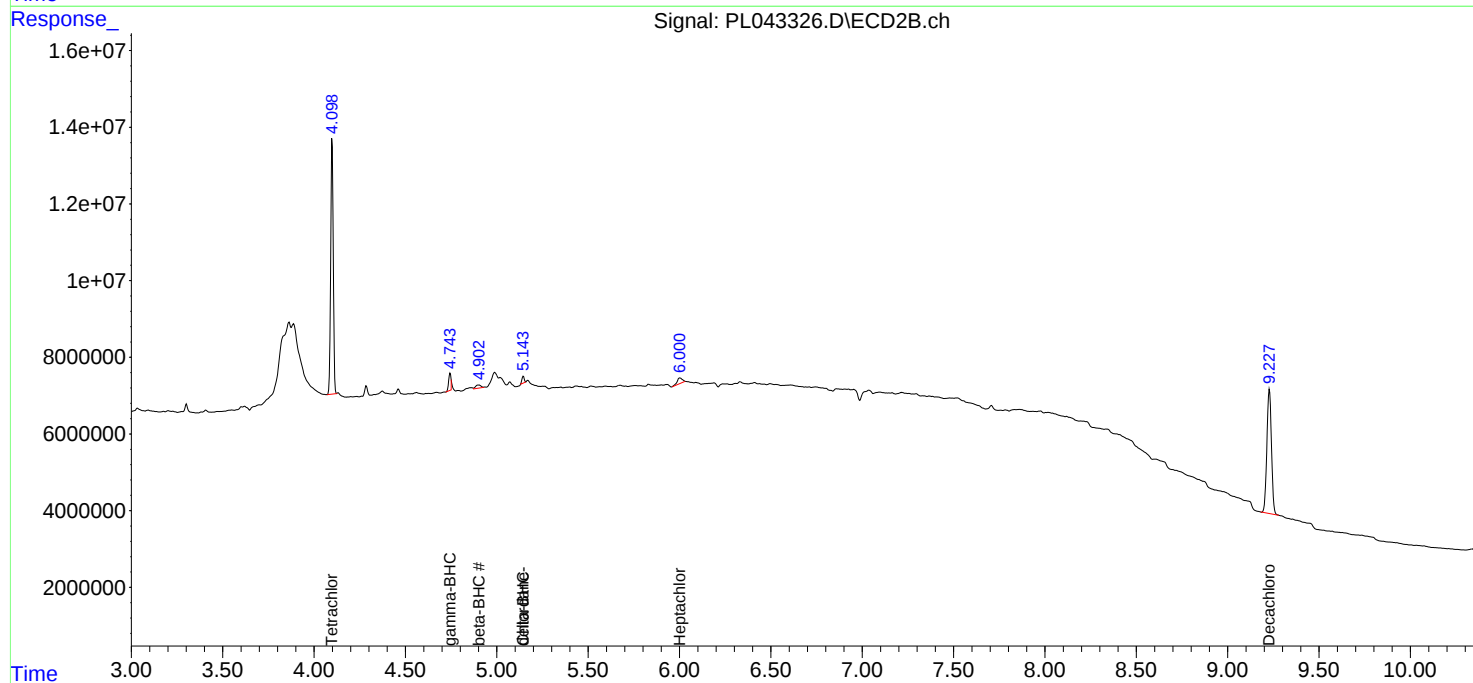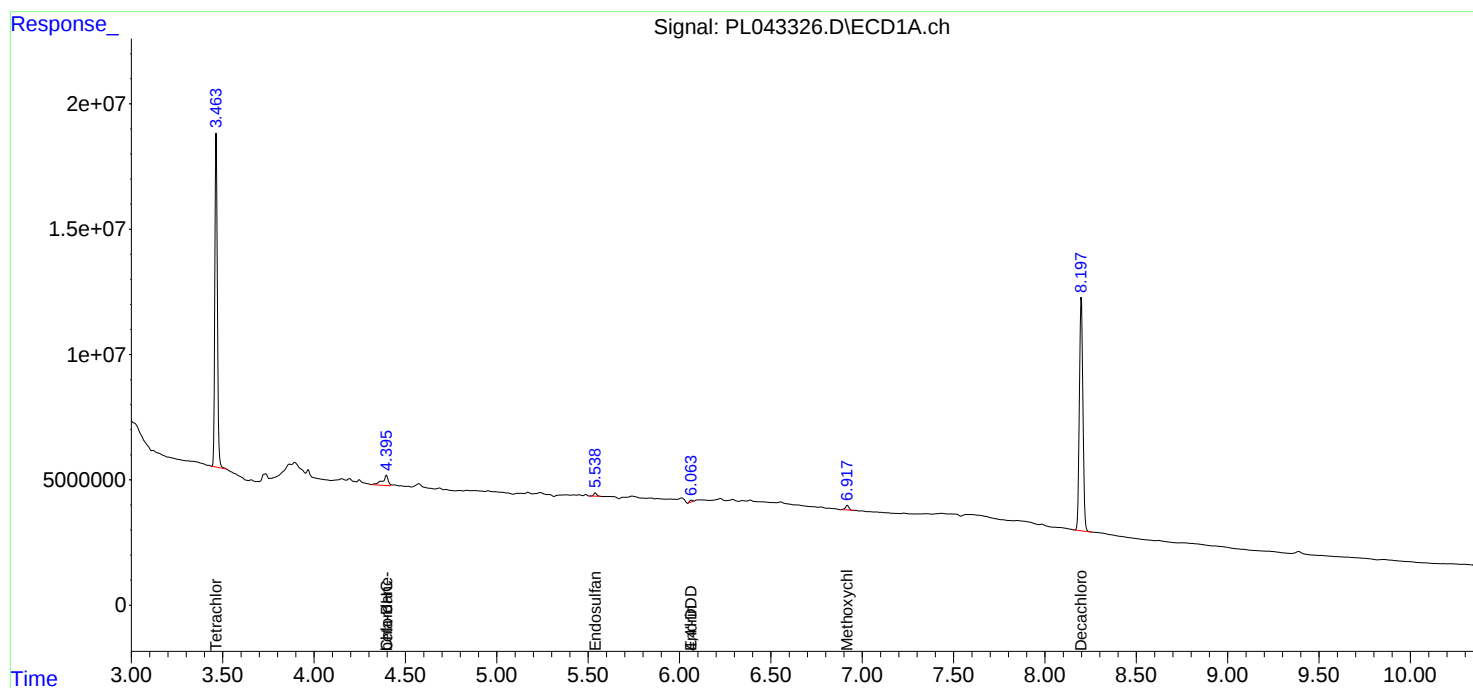


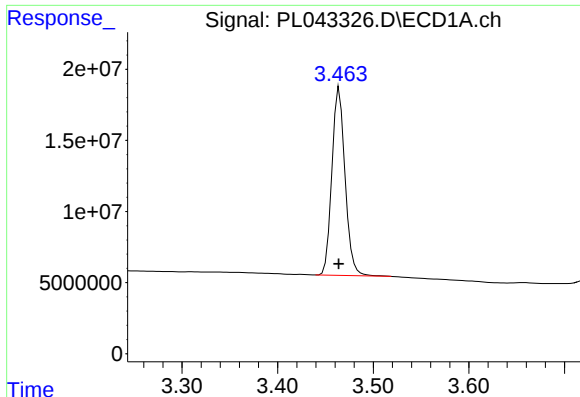

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 125767291
Conc: 20.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

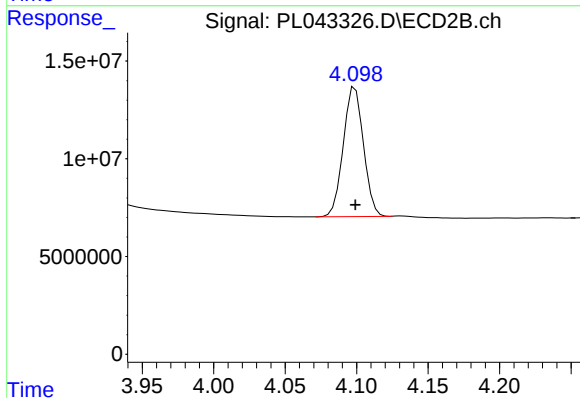


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 65206102
Conc: 22.00 ng/ml

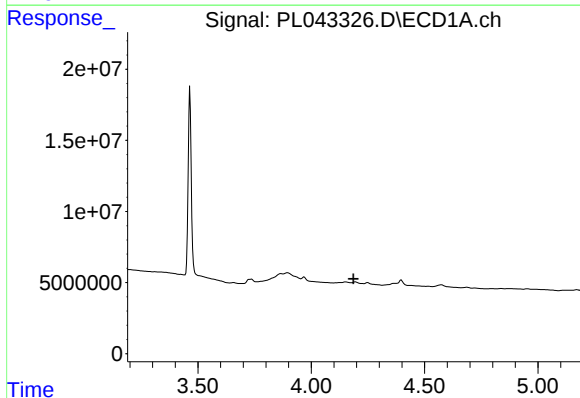


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

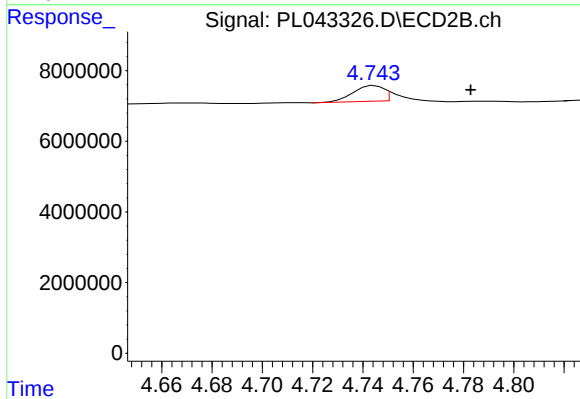

#3 gamma-BHC (Lindane)


R.T.: 4.745 min
Delta R.T.: -0.038 min
Response: 3927156
Conc: 0.94 ng/ml

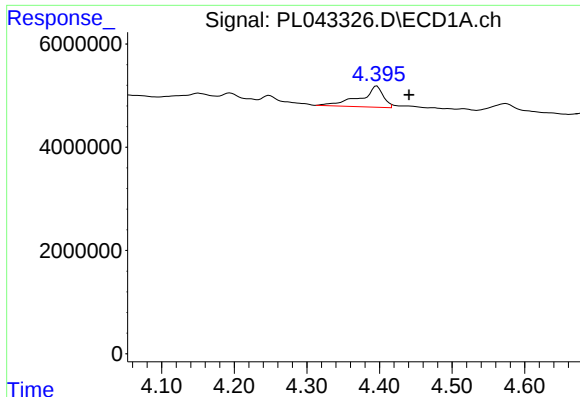

#6 beta-BHC


R.T.: 4.396 min
Delta R.T.: -0.044 min
Response: 8959145
Conc: 2.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

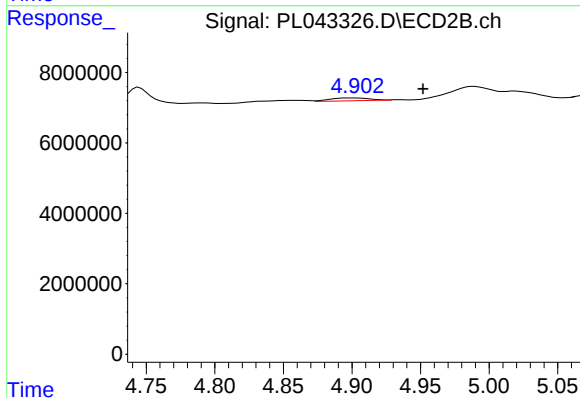


#6 beta-BHC

R.T.: 4.903 min
Delta R.T.: -0.049 min
Response: 1706259
Conc: 1.01 ng/ml

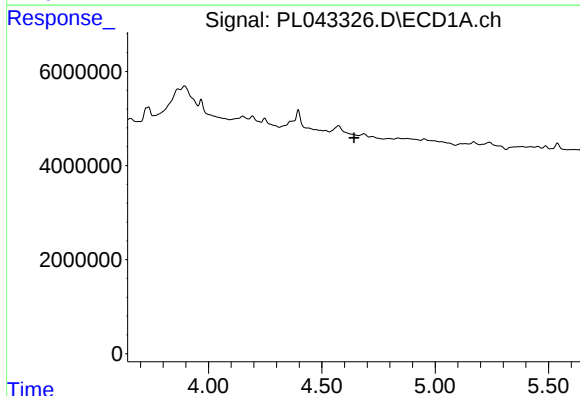


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

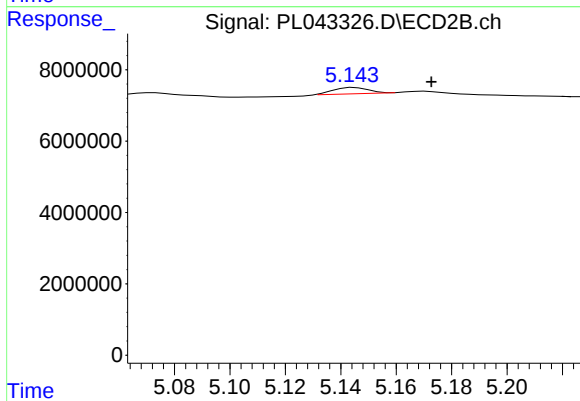

#7 delta-BHC


R.T.: 5.145 min
Delta R.T.: -0.027 min
Response: 1531693
Conc: 0.36 ng/ml

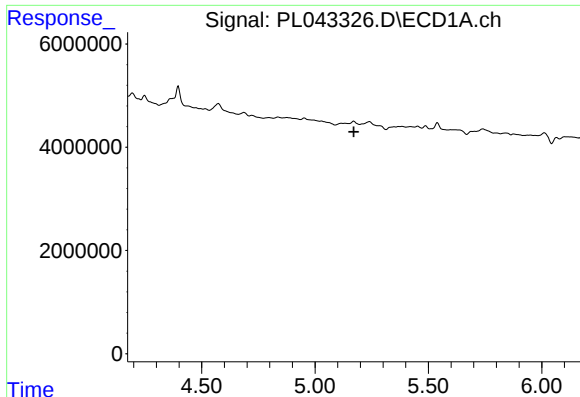

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

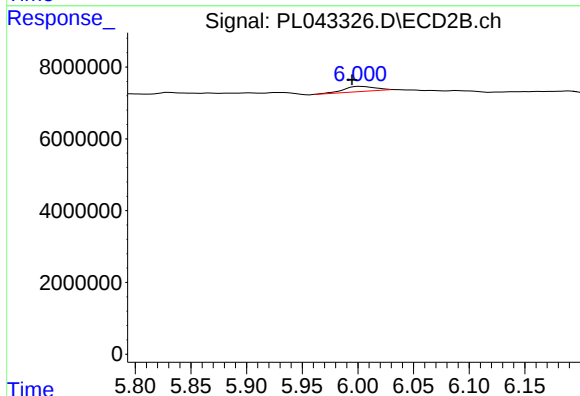


#8 Heptachlor epoxide

R.T.: 6.001 min
Delta R.T.: 0.007 min
Response: 3017032
Conc: 0.80 ng/ml

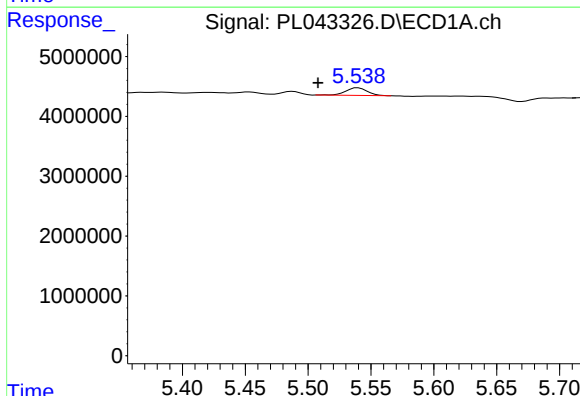


#9 Endosulfan I

R.T.: 5.540 min
Delta R.T.: 0.032 min
Response: 1484987
Conc: 0.20 ng/ml

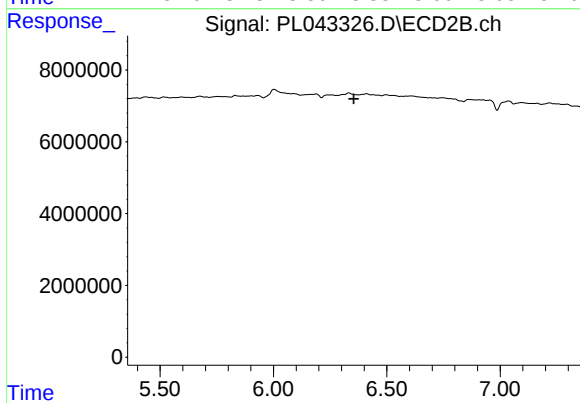

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.354 min
Response: 0
Conc: N.D.

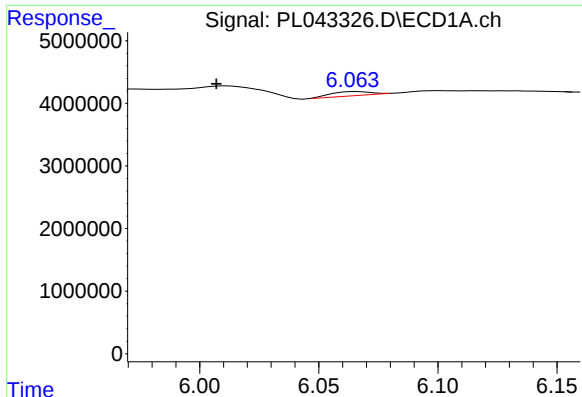

#14 Endrin


R.T.: 6.066 min
Delta R.T.: 0.059 min
Response: 759314
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

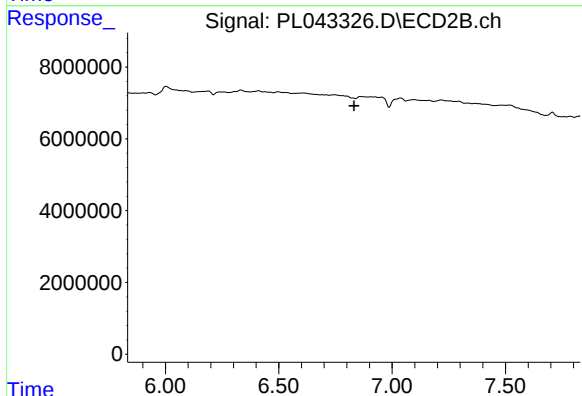


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

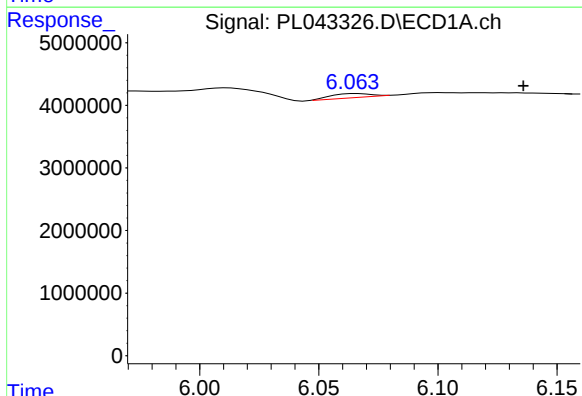


#16 4,4'-DDD

R.T.: 6.066 min
Delta R.T.: -0.070 min
Response: 759314
Conc: 0.13 ng/ml

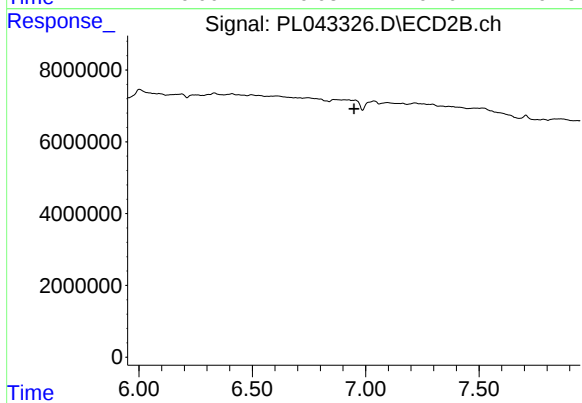

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

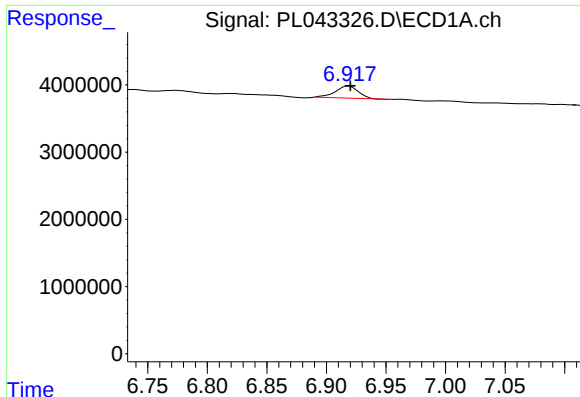

#20 Methoxychlor


R.T.: 6.919 min
Delta R.T.: -0.001 min
Response: 2417611
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

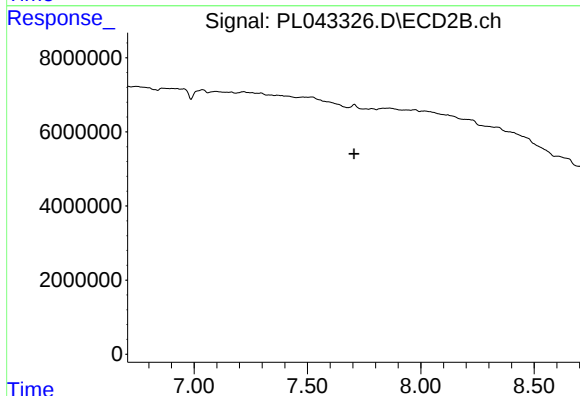


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.705 min
Response: 0
Conc: N.D.

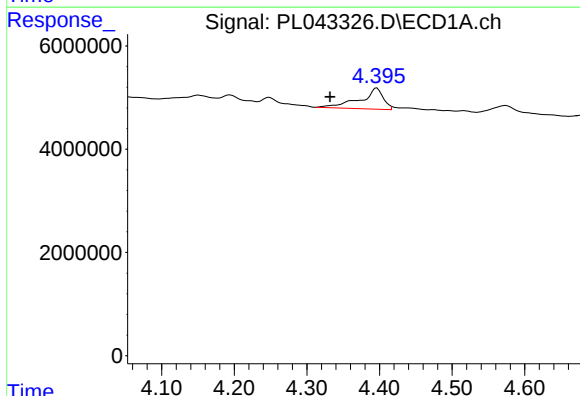


#23 Chlordane-1

R.T.: 4.396 min
Delta R.T.: 0.064 min
Response: 8959145
Conc: 33.34 ng/ml

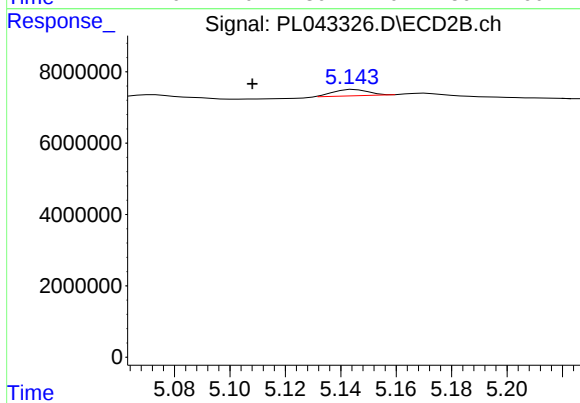

#23 Chlordane-1

R.T.: 5.145 min
Delta R.T.: 0.037 min
Response: 1531693
Conc: 10.84 ng/ml

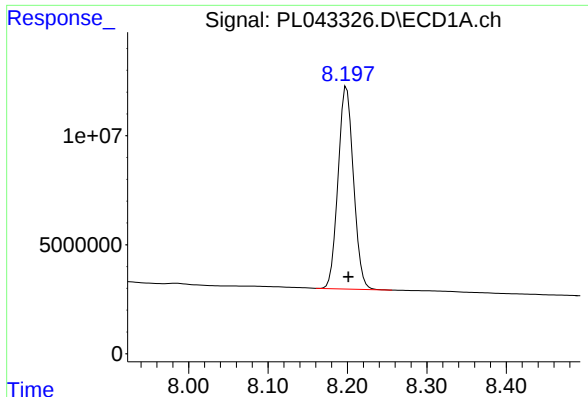

#28 Decachlorobiphenyl


R.T.: 8.199 min

Delta R.T.: -0.002 min

Response: 125183720

Conc: 19.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

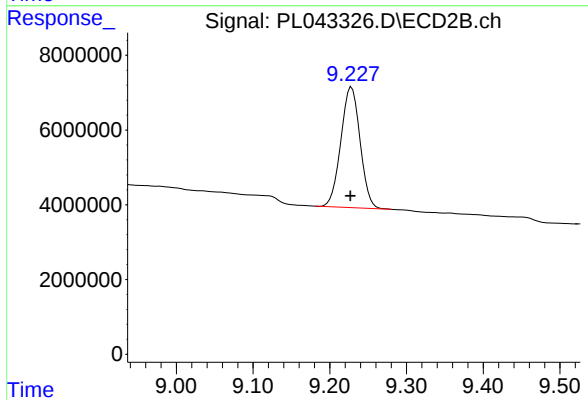

#28 Decachlorobiphenyl

R.T.: 9.228 min

Delta R.T.: 0.001 min

Response: 56352270

Conc: 21.60 ng/ml