

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121919\
 Data File : PL055103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 09:05
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 03:51:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:58:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

7) B	delta-BHC	4.700f	0.000	368264	0	0.023	N.D.	#
8) B	Heptachlo...	5.265	5.922	39098289	4714532	2.585	1.887	#
9) A	Endosulfan I	5.586f	0.000	19130181	0	1.403	N.D.	#
10) B	gamma-Chl...	5.516f	0.000	18603462	0	1.227	N.D.	#
11) B	alpha-Chl...	5.547	0.000	29195290	0	1.980	N.D.	#
15) B	Endosulfa...	6.399	0.000	2233966	0	0.185	N.D.	#
25)	Chlordane-3	5.516f	0.000	18603462	0	13.803	N.D.	#
26)	Chlordane-4	5.547	0.000	29195290	0	26.333	N.D.	#
27)	Chlordane-5	6.399	0.000	2233966	0	6.040	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL1121919\
Data File : PL055103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 09:05
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 03:51:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:58:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

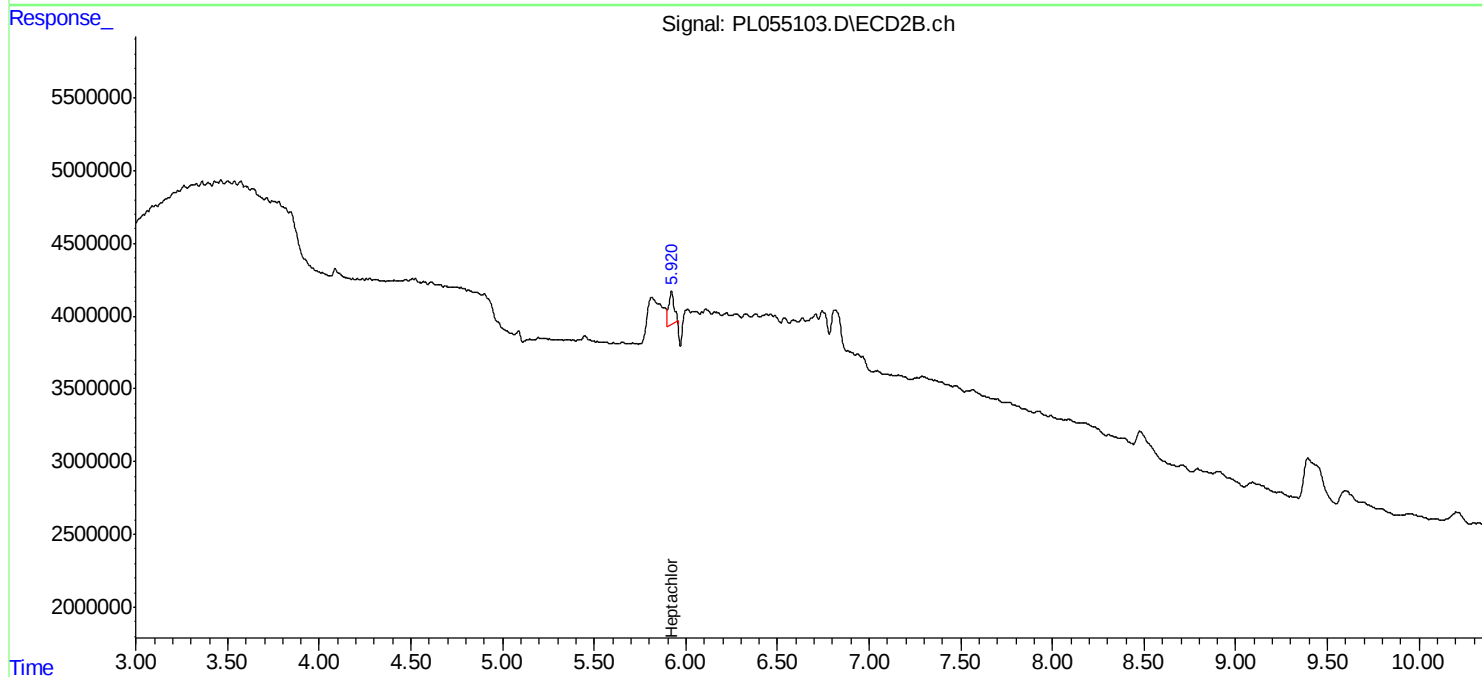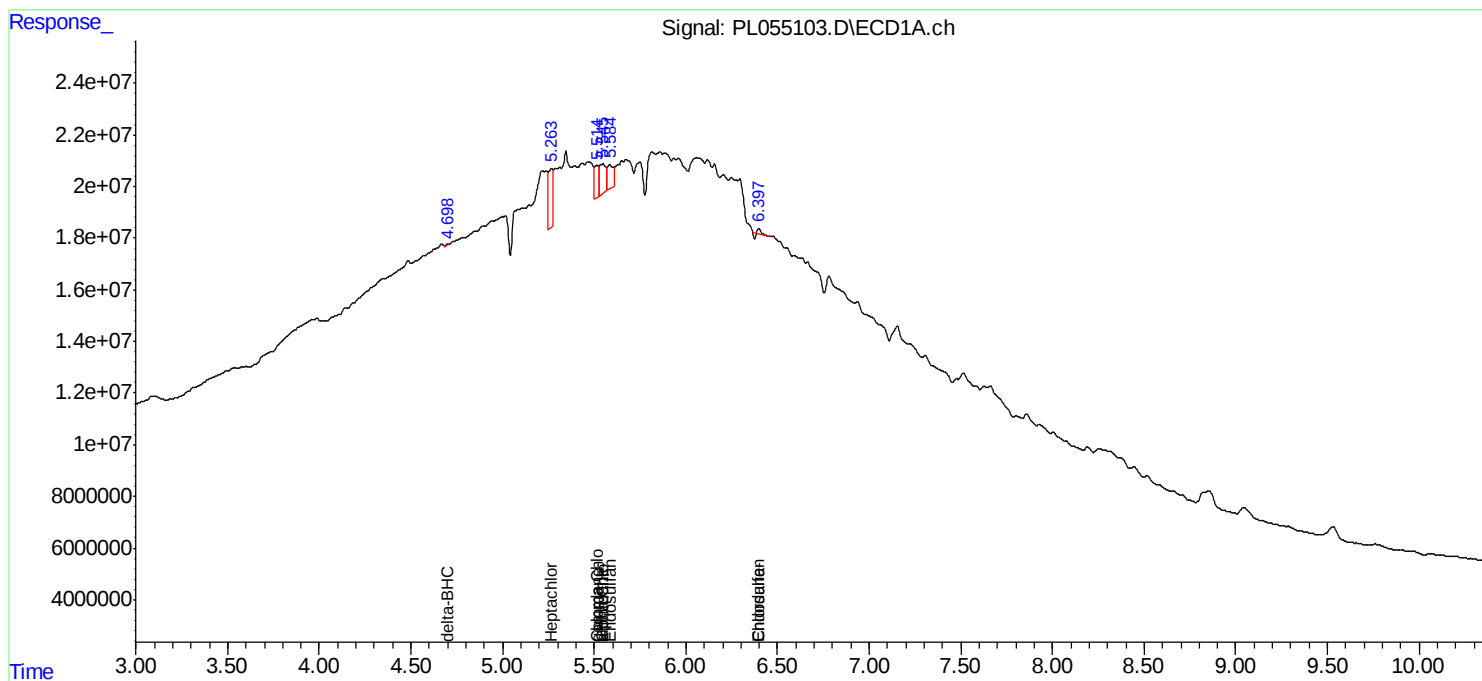


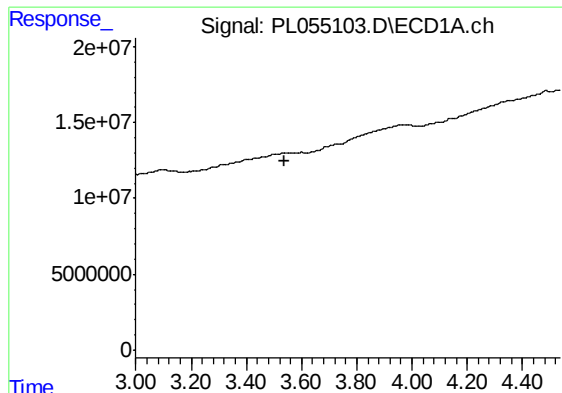

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.538 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

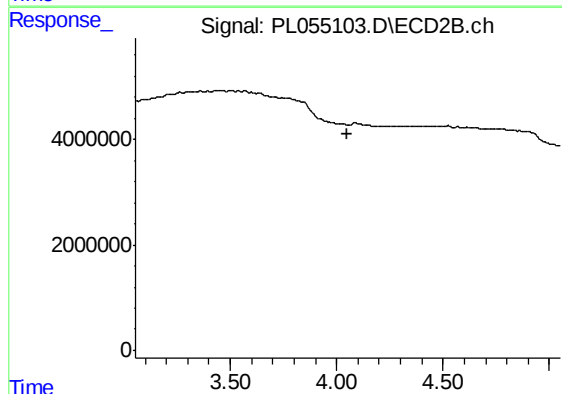


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.051 min
Response: 0
Conc: N.D.

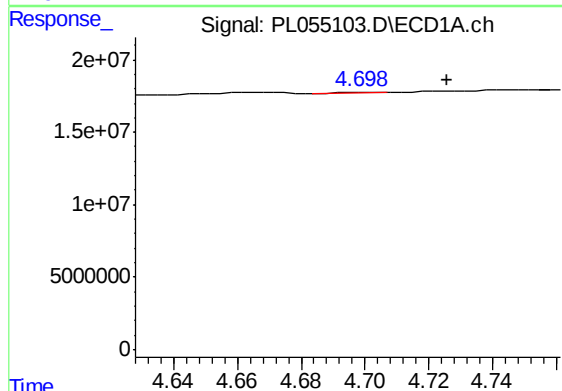


#7 delta-BHC

R.T.: 4.700 min
Delta R.T.: -0.026 min
Response: 368264
Conc: 0.02 ng/ml

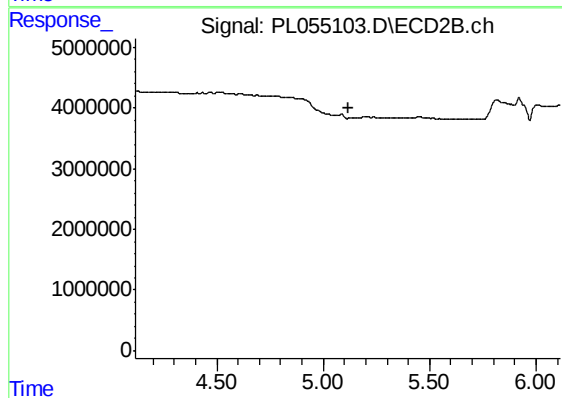

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 5.117 min
Response: 0
Conc: N.D.

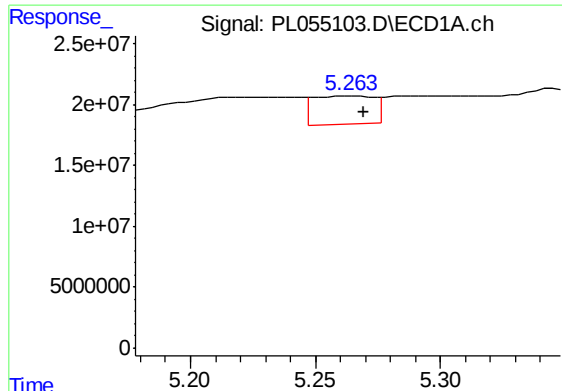

#8 Heptachlor epoxide


R.T.: 5.265 min
Delta R.T.: -0.005 min
Response: 39098289
Conc: 2.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

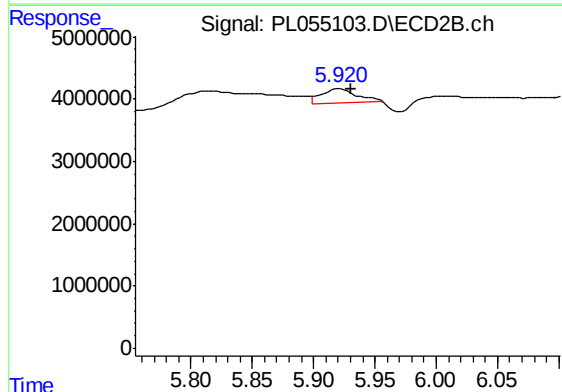


#8 Heptachlor epoxide

R.T.: 5.922 min
Delta R.T.: -0.008 min
Response: 4714532
Conc: 1.89 ng/ml

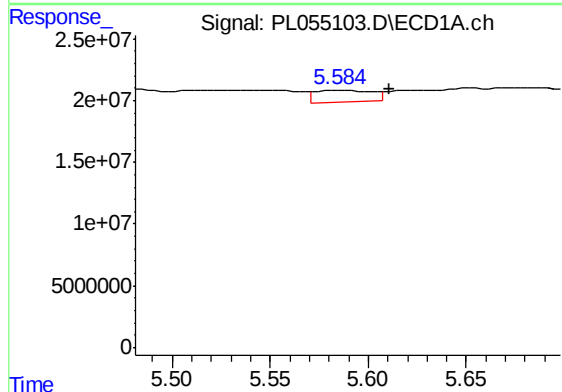


#9 Endosulfan I

R.T.: 5.586 min
Delta R.T.: -0.025 min
Response: 19130181
Conc: 1.40 ng/ml

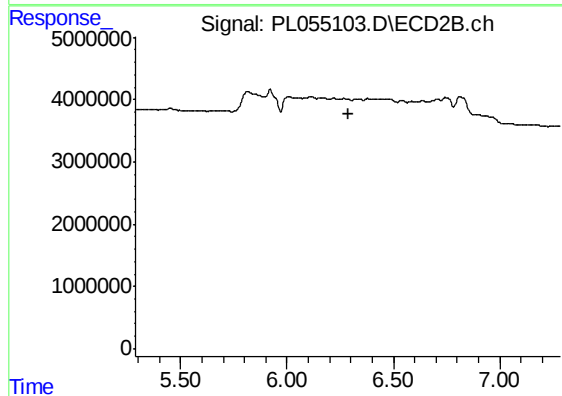

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

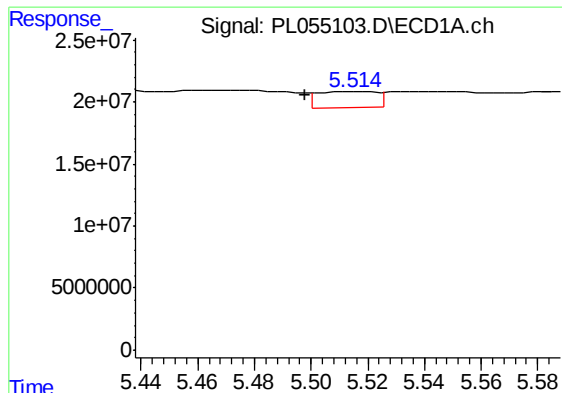

#10 gamma-Chlordane


R.T.: 5.516 min
Delta R.T.: 0.018 min
Response: 18603462
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

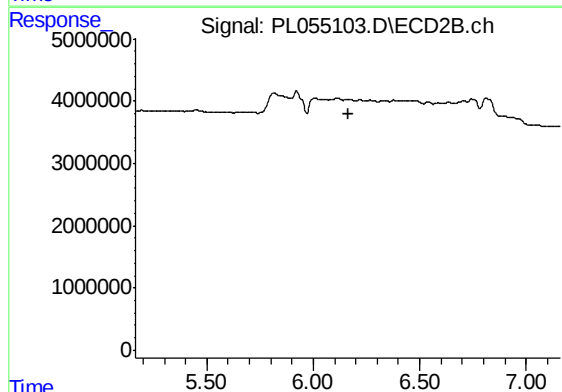


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

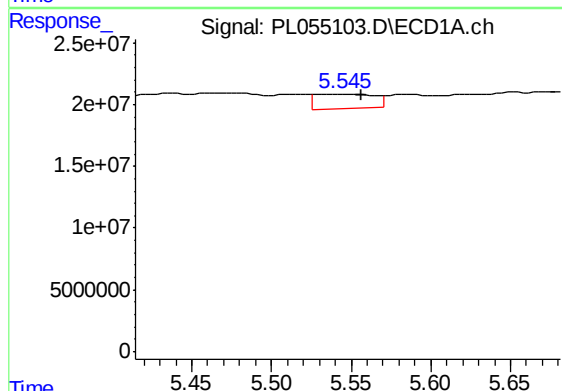


#11 alpha-Chlordane

R.T.: 5.547 min
Delta R.T.: -0.010 min
Response: 29195290
Conc: 1.98 ng/ml

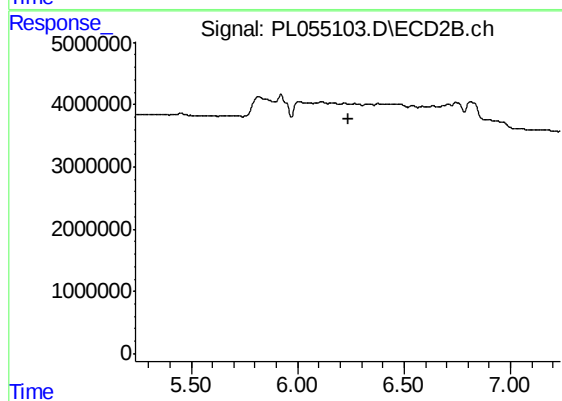

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

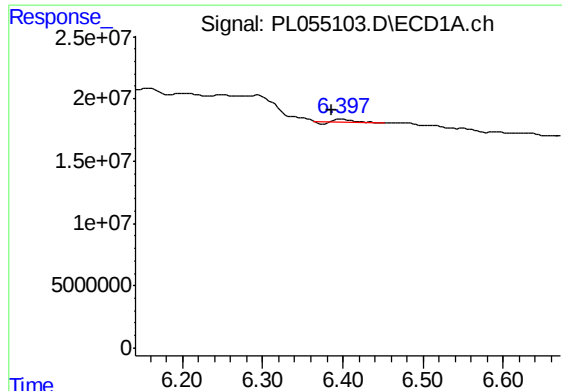

#15 Endosulfan II


R.T.: 6.399 min
Delta R.T.: 0.012 min
Response: 2233966
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

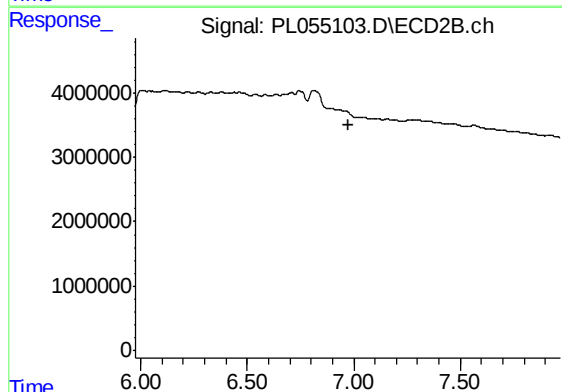


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.973 min
Response: 0
Conc: N.D.

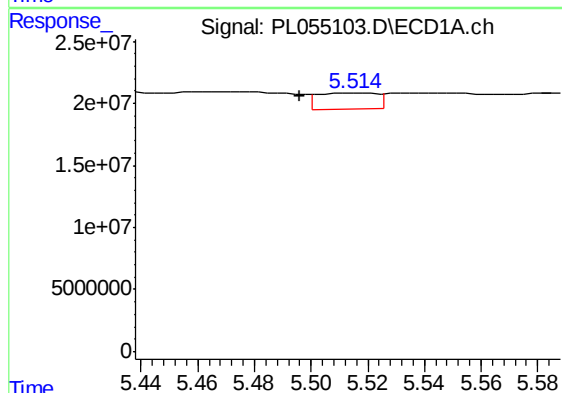


#25 Chlordane-3

R.T.: 5.516 min
Delta R.T.: 0.020 min
Response: 18603462
Conc: 13.80 ng/ml

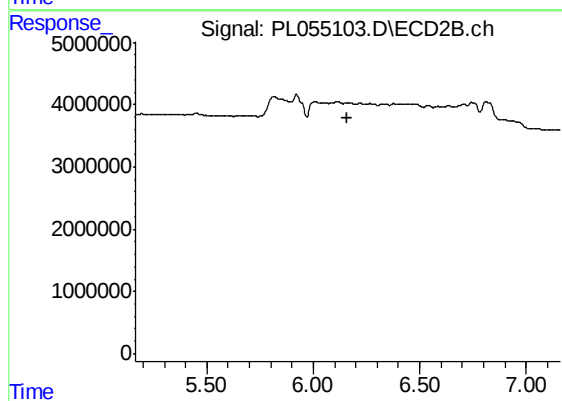

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.163 min
Response: 0
Conc: N.D.

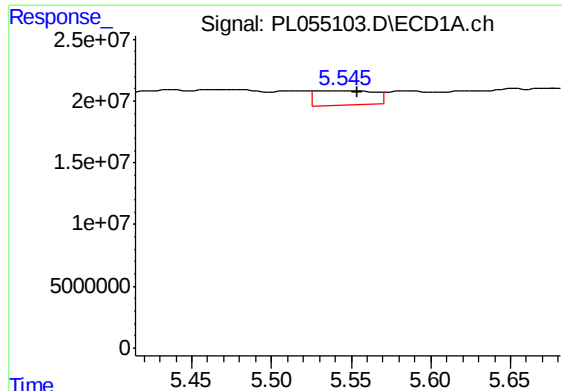

#26 Chlordane-4


R.T.: 5.547 min
Delta R.T.: -0.007 min
Response: 29195290
Conc: 26.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

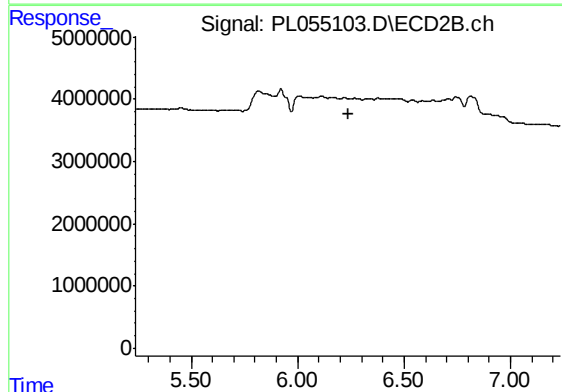


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

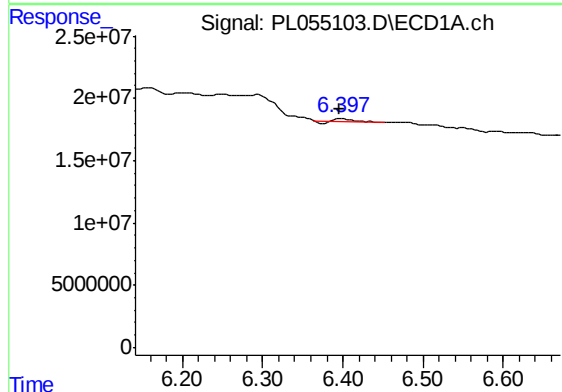


#27 Chlordane-5

R.T.: 6.399 min
Delta R.T.: 0.003 min
Response: 2233966
Conc: 6.04 ng/ml

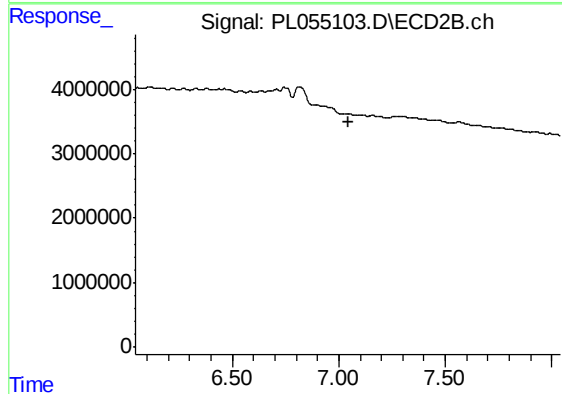

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

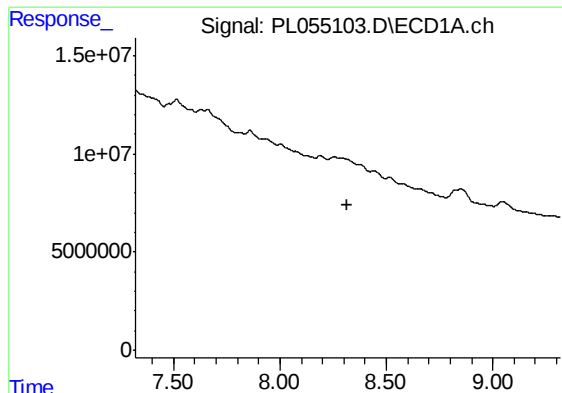

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

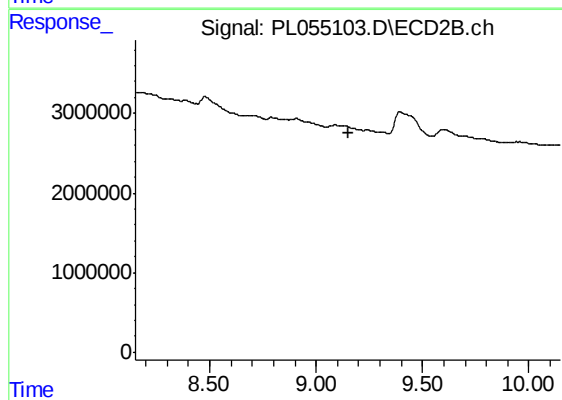

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.151 min
Response: 0
Conc: N.D.