

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121919\
 Data File : PL055113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 11:41
 Operator : SG\AJ
 Sample : K6333-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1A-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 03:54:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:58:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.535	4.048	209.6E6	53931594	18.017	21.135
28) SA Decachlor...	8.313	9.145	189.3E6	48720140	19.764	20.322
Target Compounds						
9) A Endosulfan I	5.616	0.000	18867330	0	1.384	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121919\
Data File : PL055113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 11:41
Operator : SG\AJ
Sample : K6333-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1A-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 03:54:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:58:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

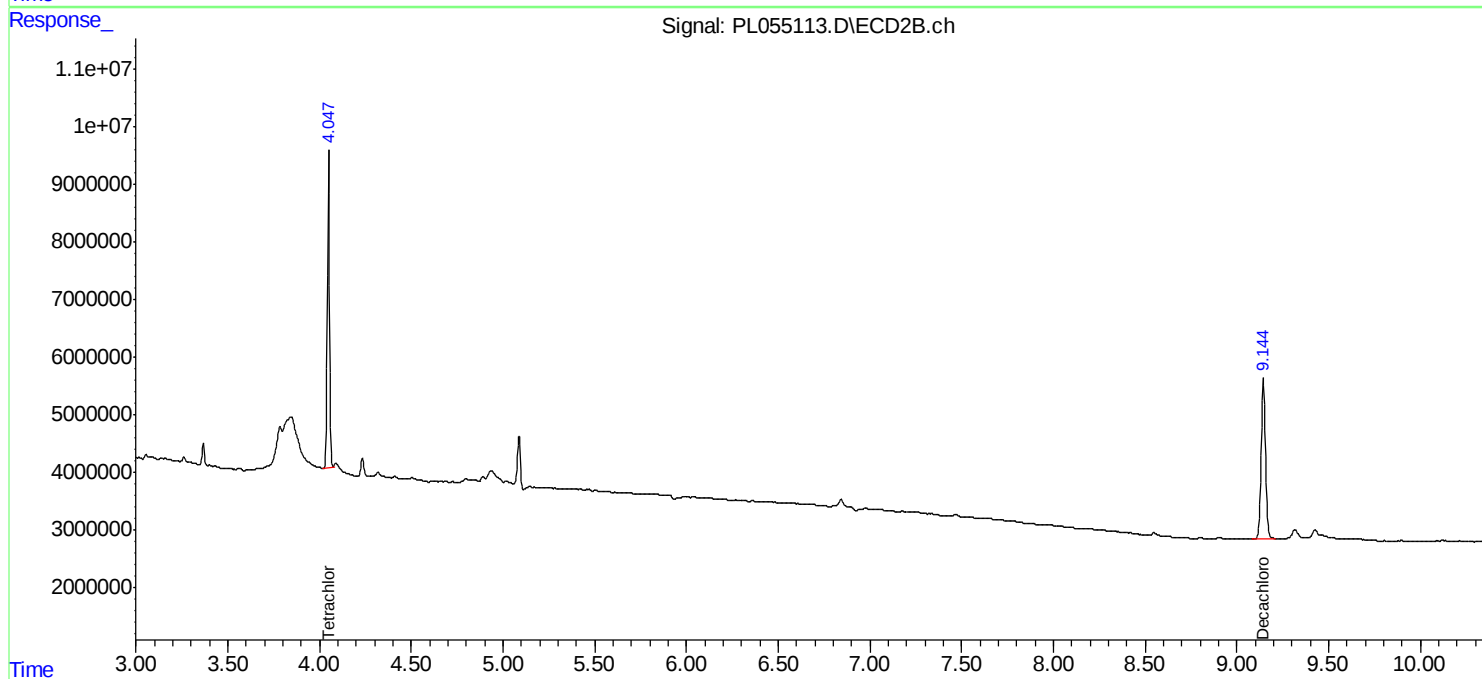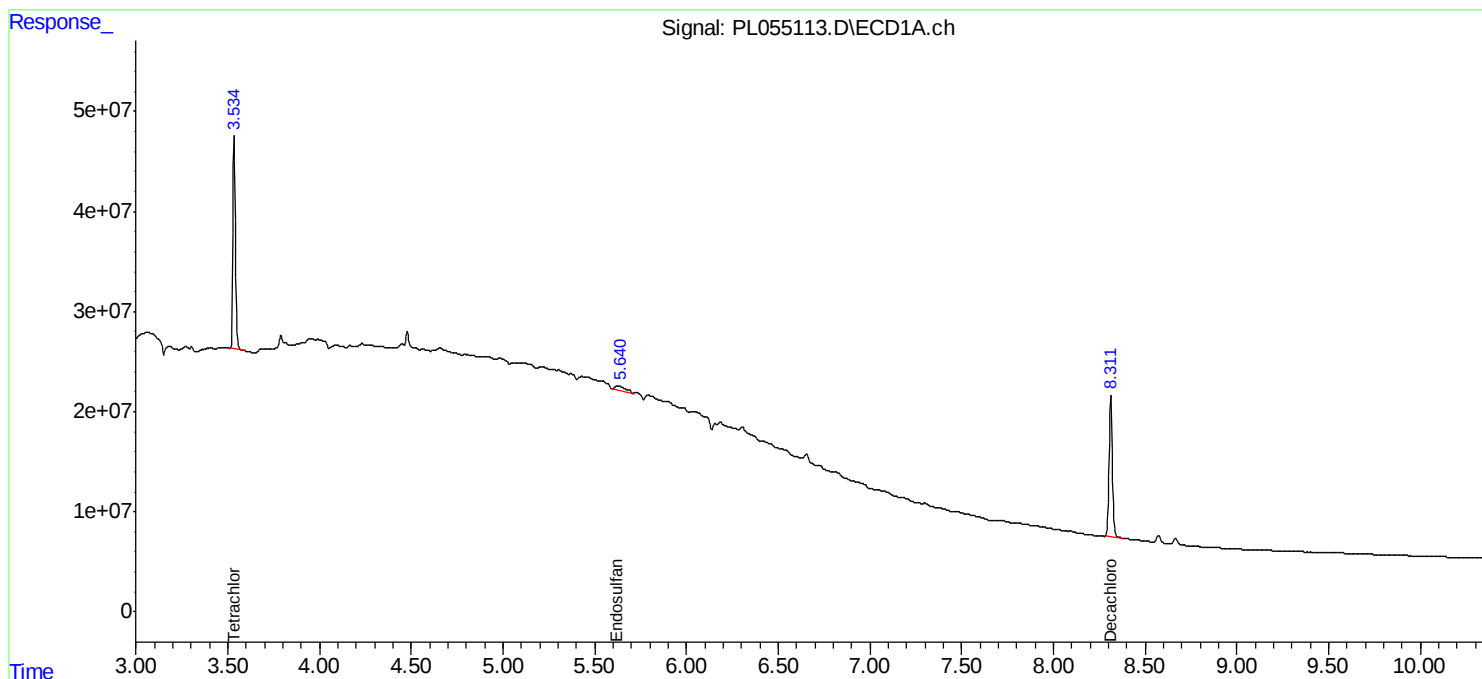


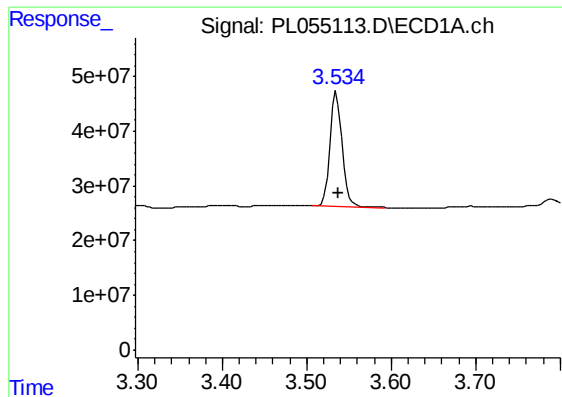

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 209617683
Conc: 18.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1A-COMP

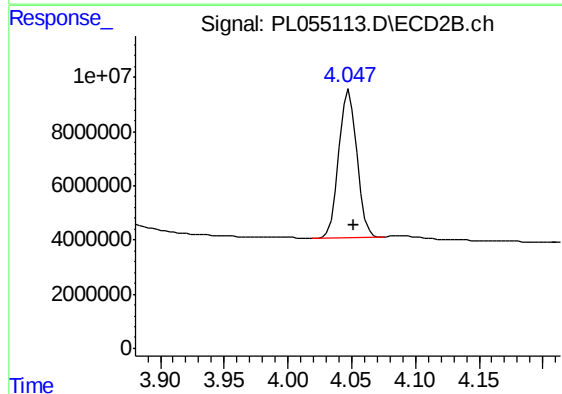


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: -0.003 min
Response: 53931594
Conc: 21.13 ng/ml

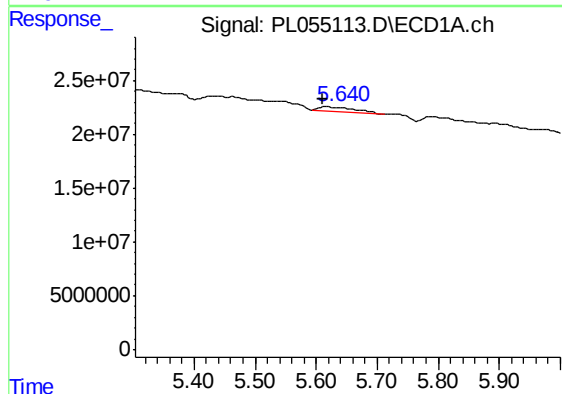


#9 Endosulfan I

R.T.: 5.616 min
Delta R.T.: 0.005 min
Response: 18867330
Conc: 1.38 ng/ml

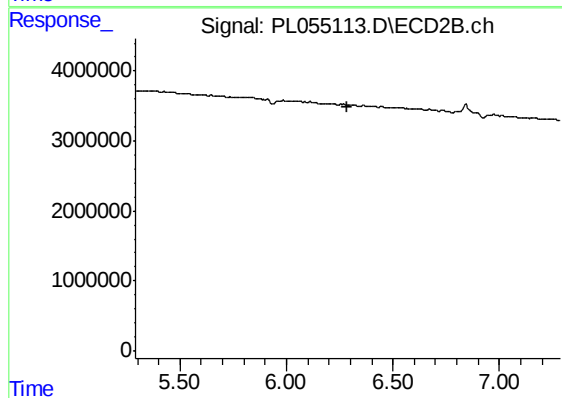

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

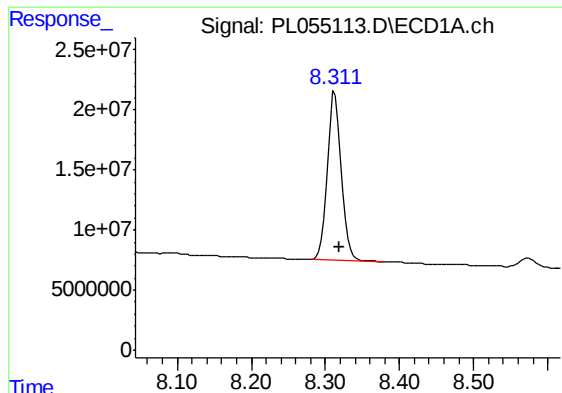

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: -0.006 min
Response: 189257883
Conc: 19.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1A-COMP

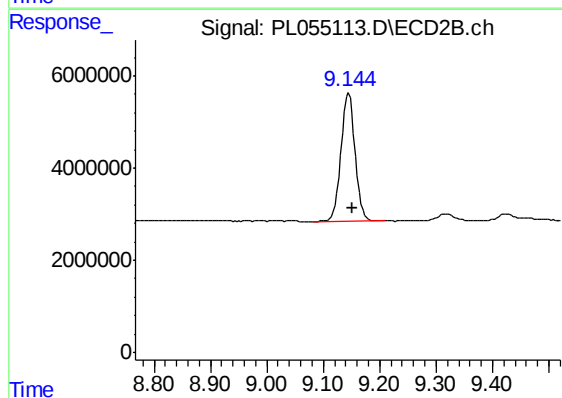

#28 Decachlorobiphenyl

R.T.: 9.145 min
Delta R.T.: -0.006 min
Response: 48720140
Conc: 20.32 ng/ml