

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121922\
 Data File : PL079777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2022 17:01
 Operator : AR\AJ
 Sample : PB149651TB
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB149651TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 20:38:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	2.563	42444185	52701713	18.789	19.361
28)	SA Decachlor...	8.765	7.629	35799251	43950824	18.433	18.708
Target Compounds							
3)	MA gamma-BHC...	4.133f	3.394f	71165	99139	0.022	0.025
5)	MB Aldrin	0.000	3.958	0	59421	N.D.	0.016 #
6)	B beta-BHC	4.314	0.000	458175	0	0.324	N.D. #
8)	B Heptachlo...	5.464	4.488f	636404	65061	0.223	0.019 #
10)	B gamma-Chl...	0.000	4.736f	0	224790	N.D.	0.066 #
13)	MA Dieldrin	0.000	5.080	0	110715	N.D.	0.033 #
19)	B Endosulfa...	0.000	6.054	0	163598	N.D.	0.058 #
25)	Chlordane-3	0.000	4.736f	0	224790	N.D.	0.672 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121922\
Data File : PL079777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2022 17:01
Operator : AR\AJ
Sample : PB149651TB
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB149651TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 20:38:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

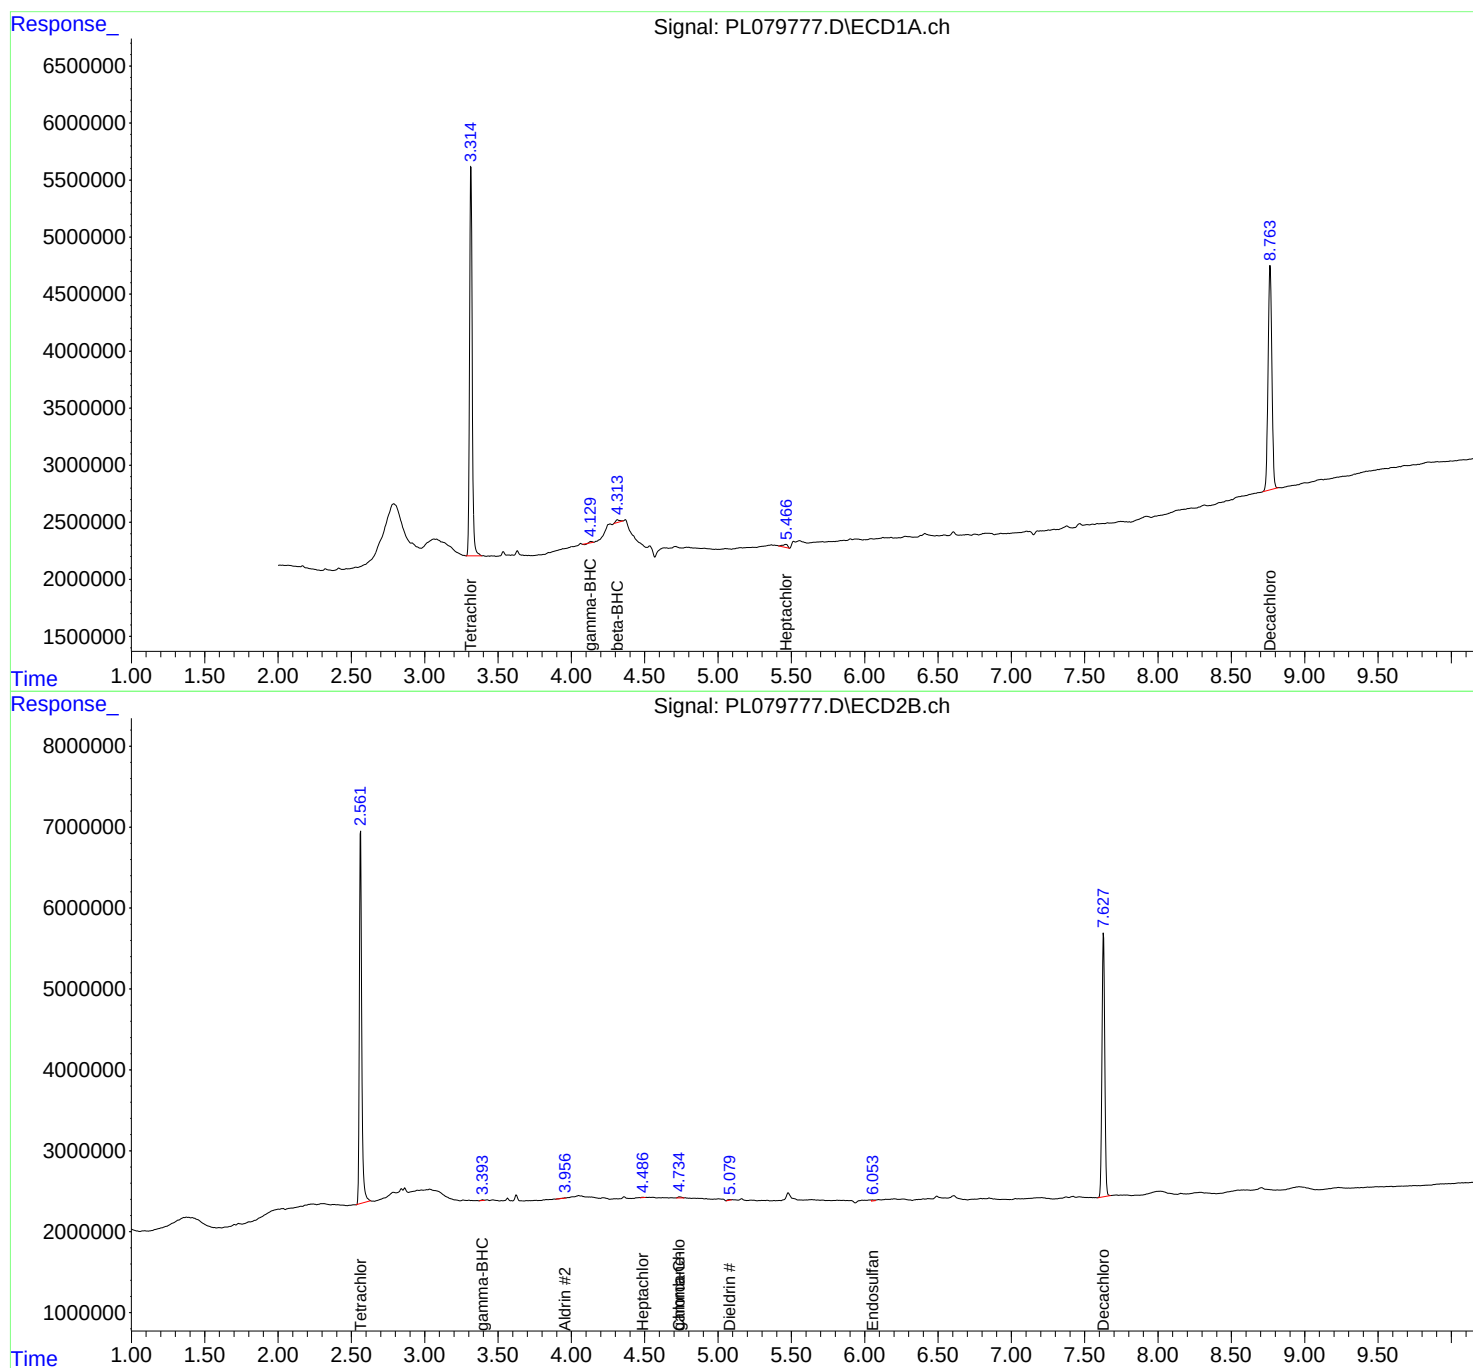


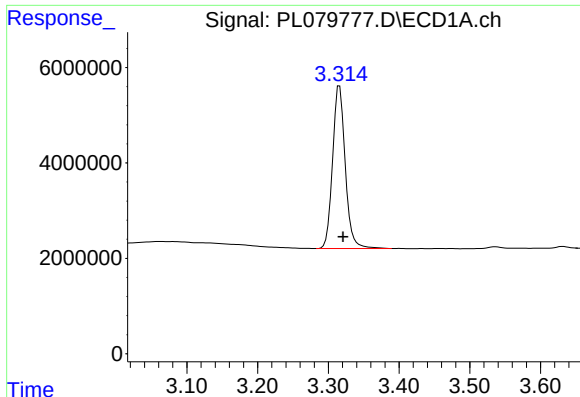

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.005 min
Response: 42444185
Conc: 18.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB149651TB

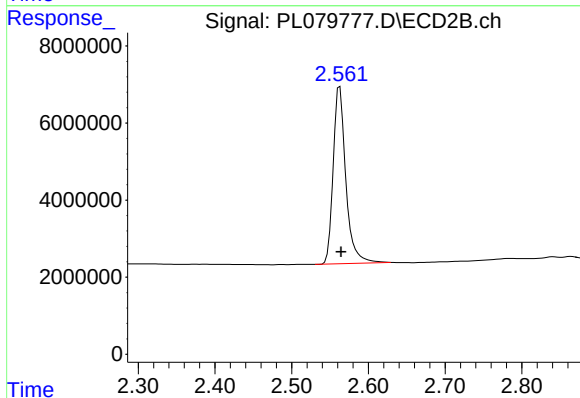


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: -0.002 min
Response: 52701713
Conc: 19.36 ng/ml

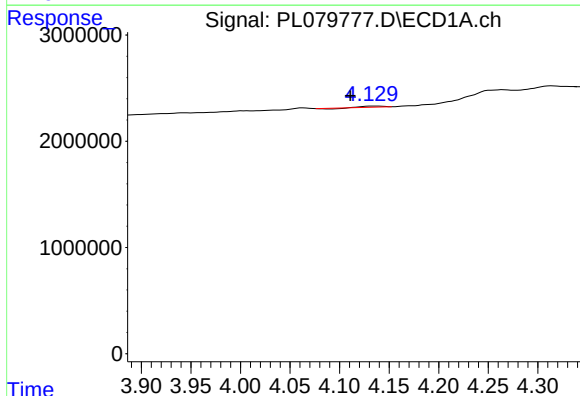


#3 gamma-BHC (Lindane)

R.T.: 4.133 min
Delta R.T.: 0.022 min
Response: 71165
Conc: 0.02 ng/ml

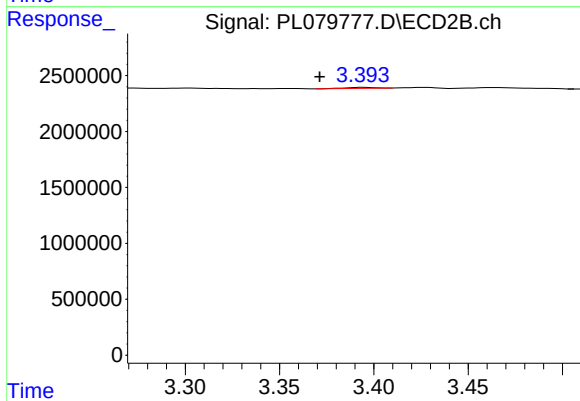

#3 gamma-BHC (Lindane)


R.T.: 3.394 min
Delta R.T.: 0.023 min
Response: 99139
Conc: 0.03 ng/ml

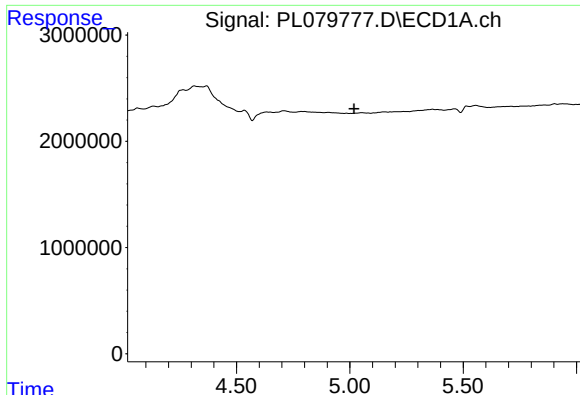

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.019 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB149651TB

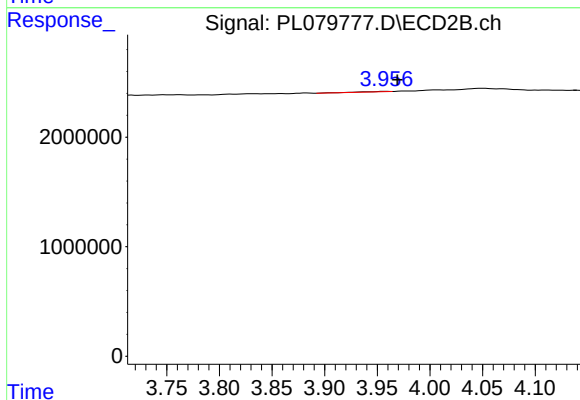


#5 Aldrin

R.T.: 3.958 min
Delta R.T.: -0.012 min
Response: 59421
Conc: 0.02 ng/ml

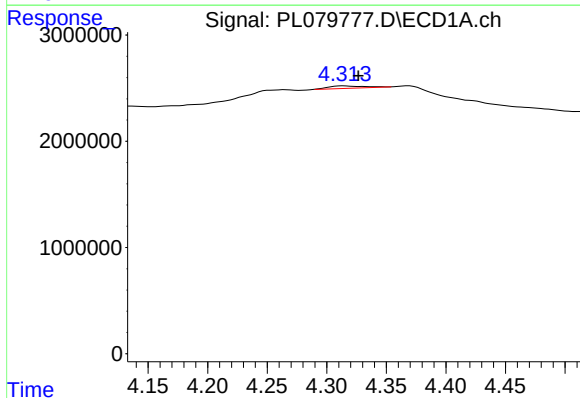


#6 beta-BHC

R.T.: 4.314 min
Delta R.T.: -0.012 min
Response: 458175
Conc: 0.32 ng/ml

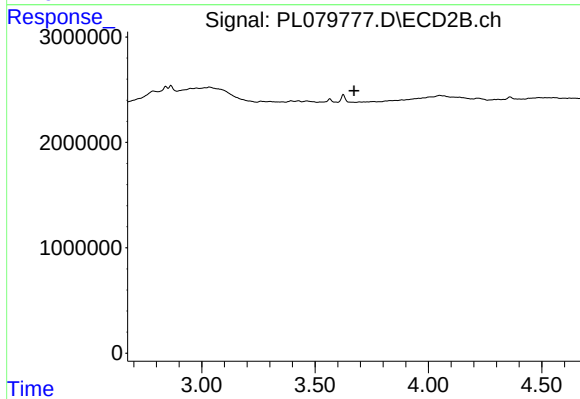

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 3.672 min
Response: 0
Conc: N.D.

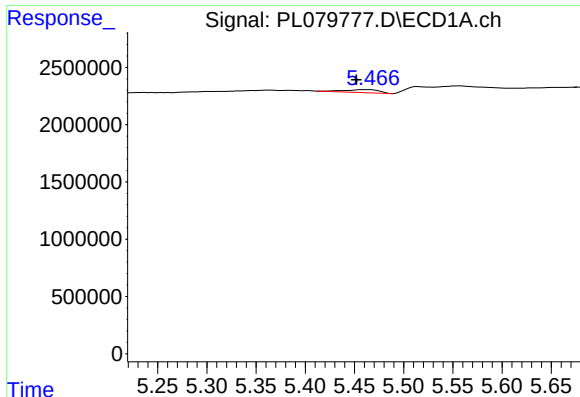

#8 Heptachlor epoxide


R.T.: 5.464 min
Delta R.T.: 0.012 min
Response: 636404
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB149651TB

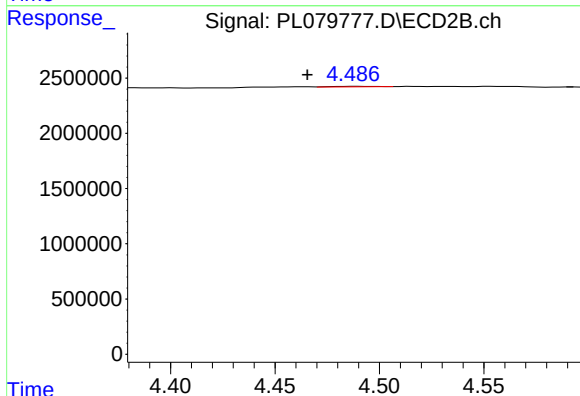


#8 Heptachlor epoxide

R.T.: 4.488 min
Delta R.T.: 0.023 min
Response: 65061
Conc: 0.02 ng/ml

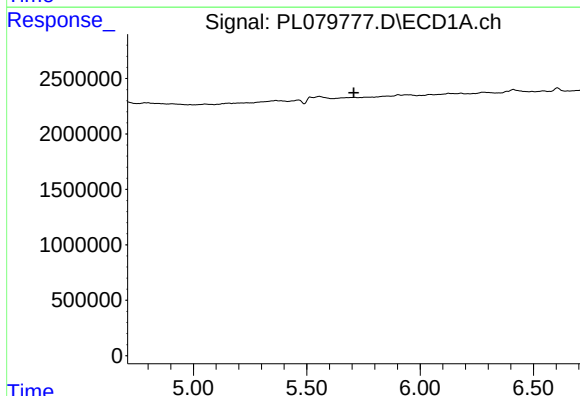


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.708 min
Response: 0
Conc: N.D.

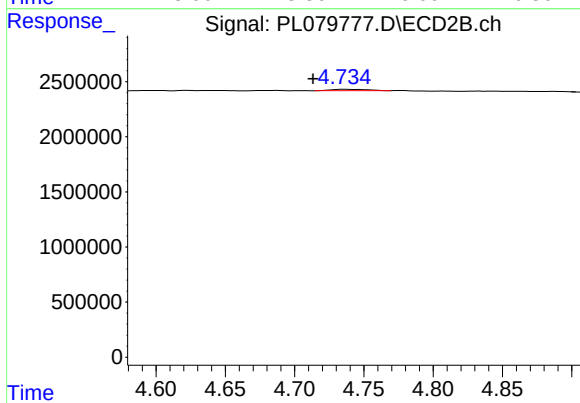

#10 gamma-Chlordane


R.T.: 4.736 min
Delta R.T.: 0.022 min
Response: 224790
Conc: 0.07 ng/ml

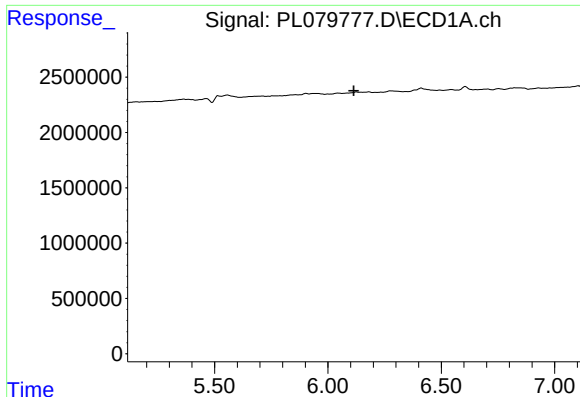

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB149651TB

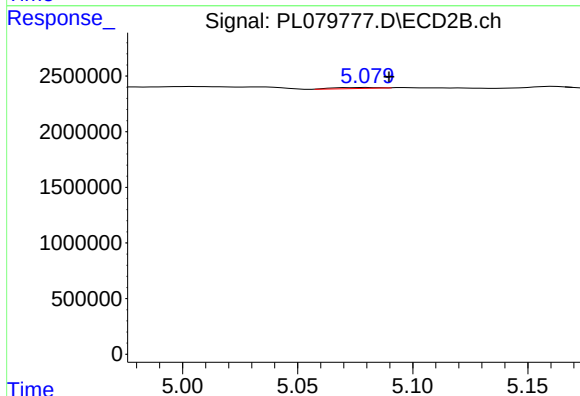


#13 Dieldrin

R.T.: 5.080 min
Delta R.T.: -0.010 min
Response: 110715
Conc: 0.03 ng/ml

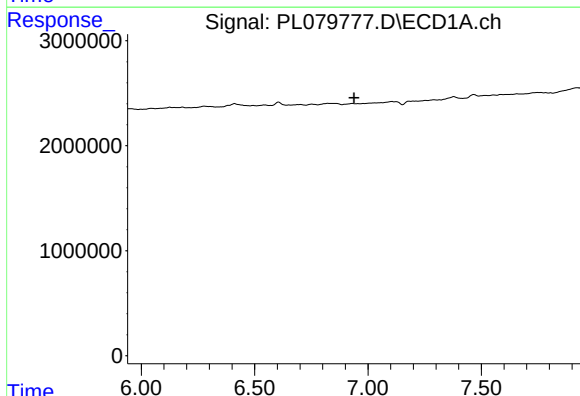


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.939 min
Response: 0
Conc: N.D.

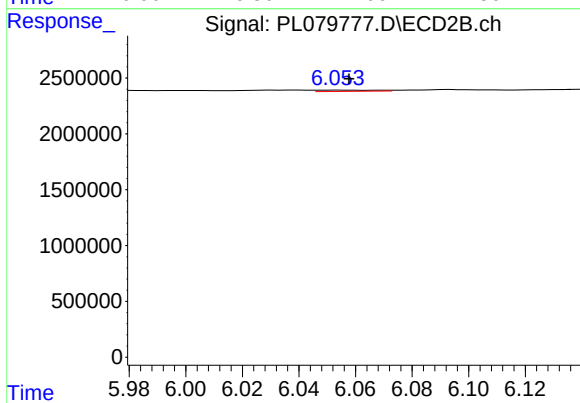

#19 Endosulfan Sulfate


R.T.: 6.054 min
Delta R.T.: -0.004 min
Response: 163598
Conc: 0.06 ng/ml

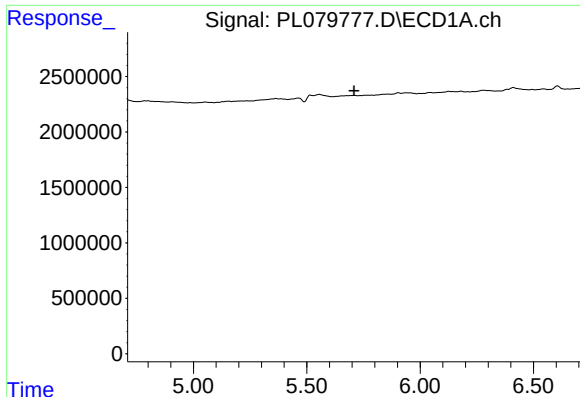

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.709 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB149651TB

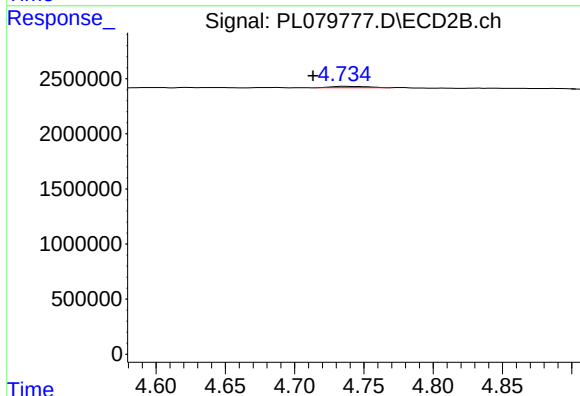


#25 Chlordane-3

R.T.: 4.736 min
Delta R.T.: 0.022 min
Response: 224790
Conc: 0.67 ng/ml

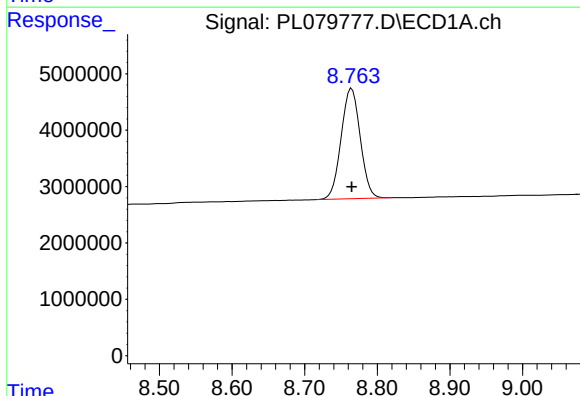

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 35799251
Conc: 18.43 ng/ml

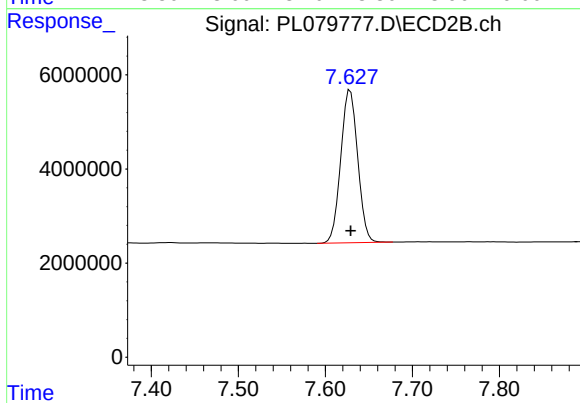

#28 Decachlorobiphenyl

R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 43950824
Conc: 18.71 ng/ml