

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL1121922\
 Data File : PL079779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2022 17:29
 Operator : AR\AJ
 Sample : N6023-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WASTE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 20:39:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	2.563	44376656	53463548	19.644	19.641
28)	SA Decachlor...	8.764	7.628	34589105	42329452	17.810	18.018
Target Compounds							
2)	A alpha-BHC	3.750f	0.000	361250	0	0.105	N.D. #
5)	MB Aldrin	0.000	3.954f	0	316189	N.D.	0.085 #
8)	B Heptachlo...	5.458	4.476	2781945	211941	0.974	0.063 #
10)	B gamma-Chl...	0.000	4.720	0	656364	N.D.	0.194 #
13)	MA Dieldrin	6.119	5.085	380810	458729	0.139	0.136
15)	B Endosulfa...	6.548f	5.631f	270720	416048	0.120	0.149
19)	B Endosulfa...	0.000	6.046	0	166460	N.D.	0.059 #
23)	Chlordane-1	0.000	3.514	0	520698	N.D.	4.896 #
25)	Chlordane-3	0.000	4.720	0	656364	N.D.	1.963 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121922\
Data File : PL079779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2022 17:29
Operator : AR\AJ
Sample : N6023-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WASTE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 20:39:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

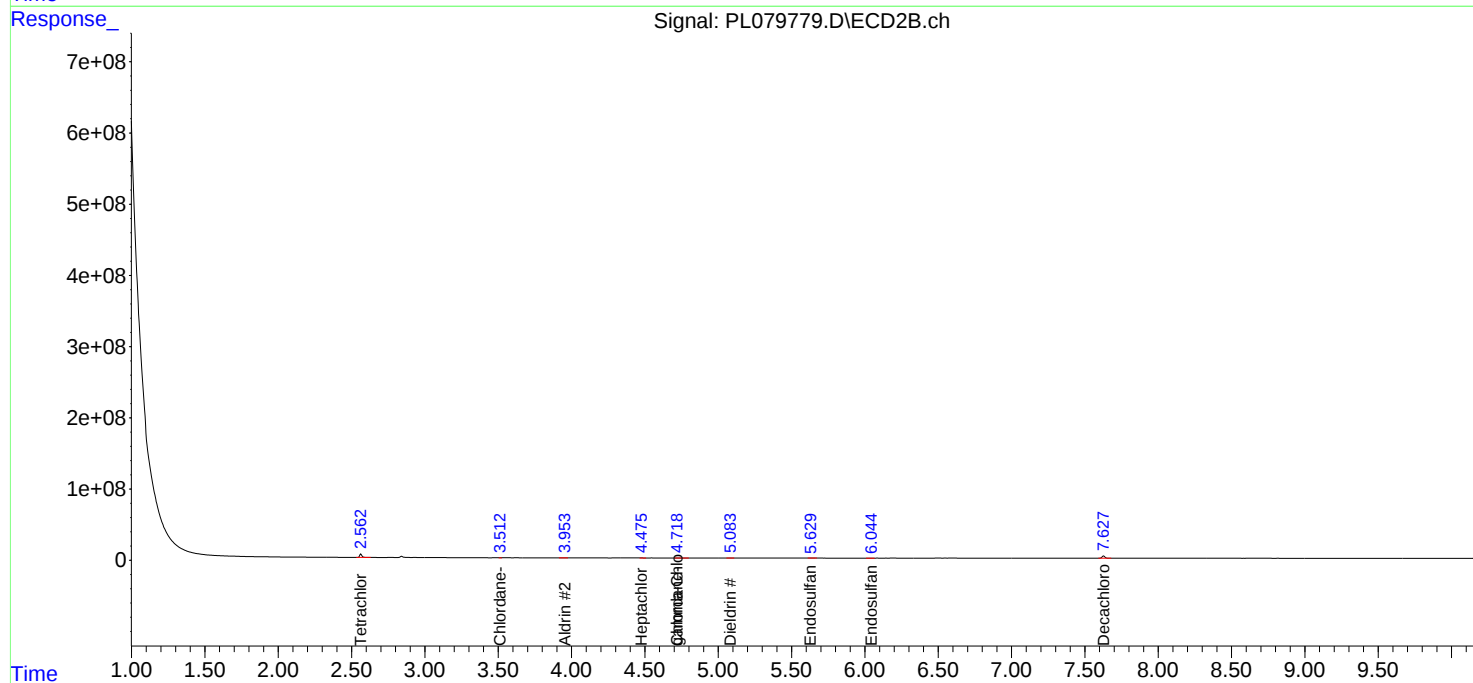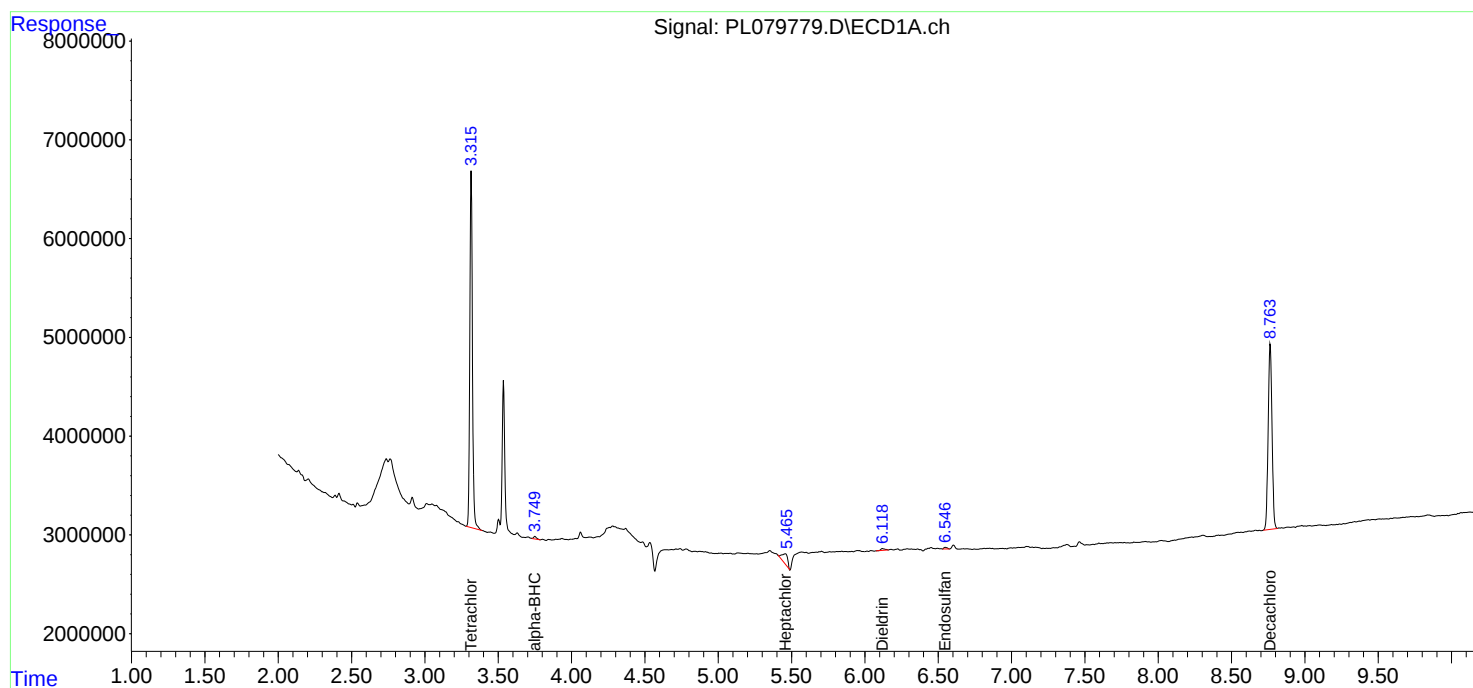


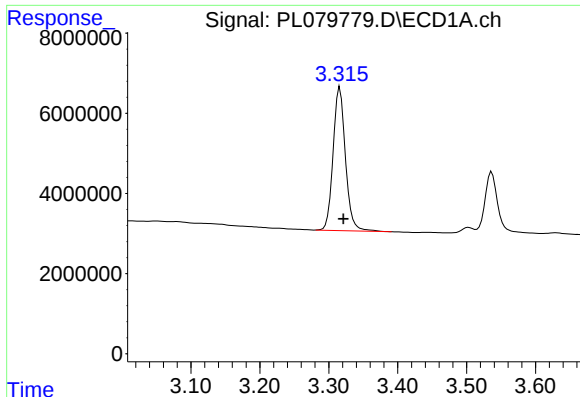

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.005 min
Response: 44376656
Conc: 19.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
WASTE

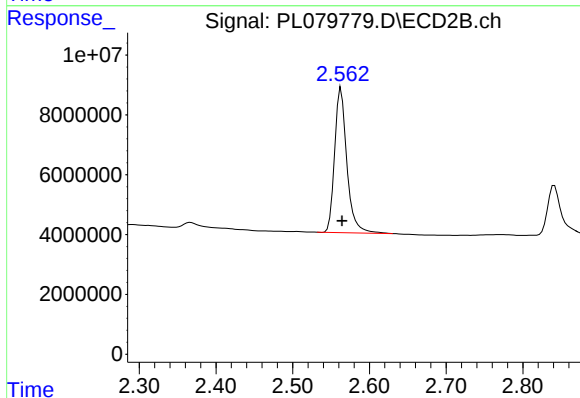


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: -0.001 min
Response: 53463548
Conc: 19.64 ng/ml

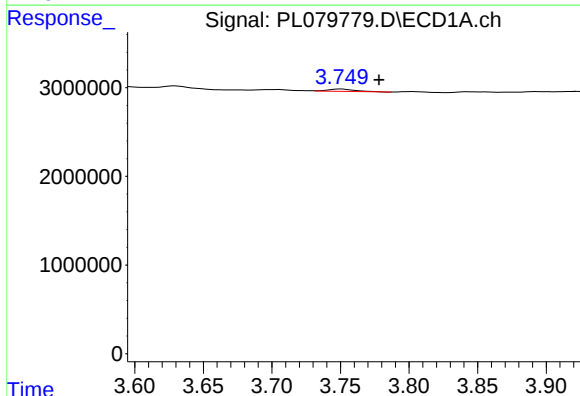


#2 alpha-BHC

R.T.: 3.750 min
Delta R.T.: -0.028 min
Response: 361250
Conc: 0.11 ng/ml

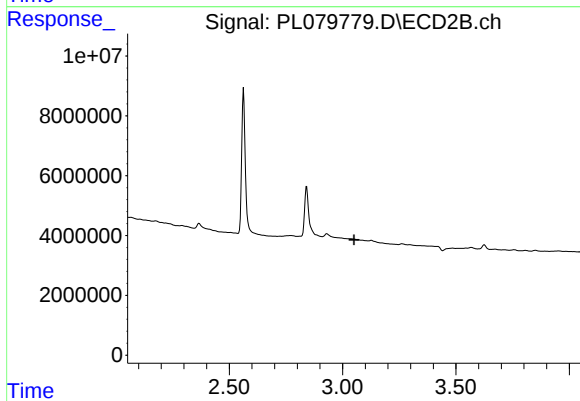

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.051 min
Response: 0
Conc: N.D.

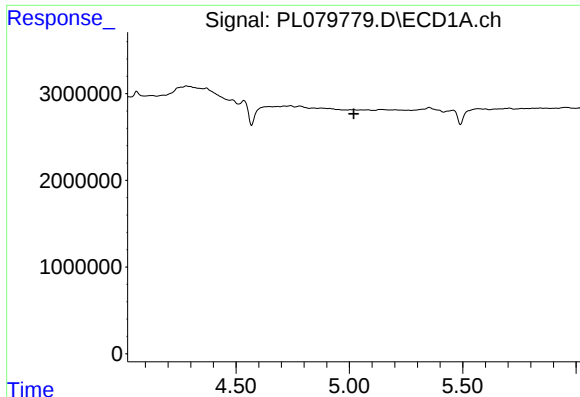

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.019 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WASTE

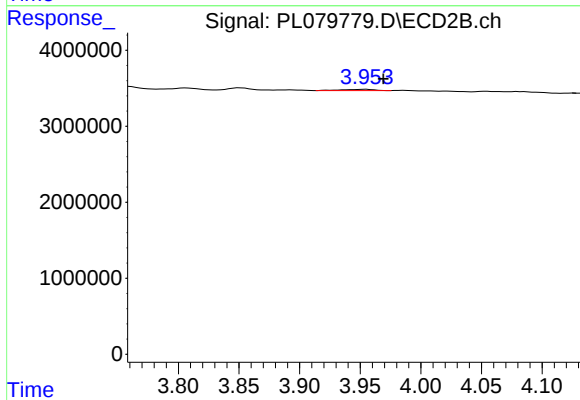


#5 Aldrin

R.T.: 3.954 min
Delta R.T.: -0.015 min
Response: 316189
Conc: 0.09 ng/ml

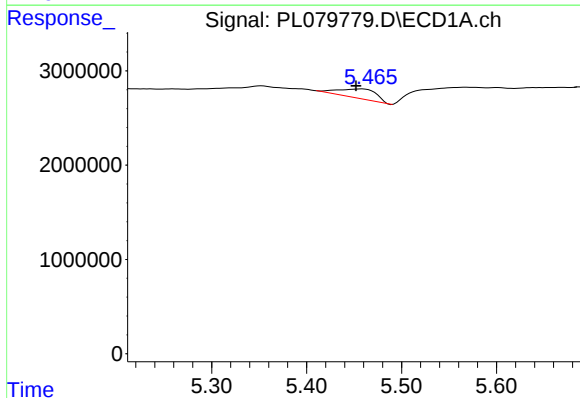


#8 Heptachlor epoxide

R.T.: 5.458 min
Delta R.T.: 0.006 min
Response: 2781945
Conc: 0.97 ng/ml

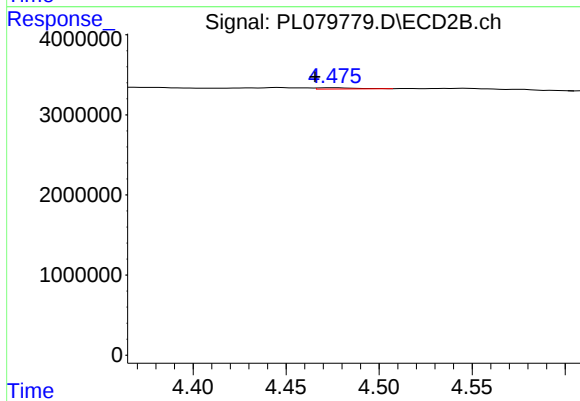

#8 Heptachlor epoxide


R.T.: 4.476 min
Delta R.T.: 0.011 min
Response: 211941
Conc: 0.06 ng/ml

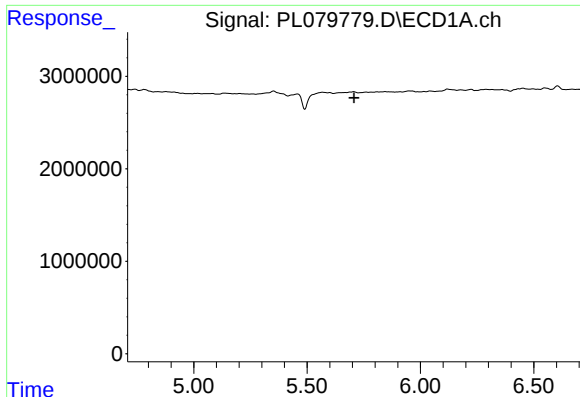

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WASTE

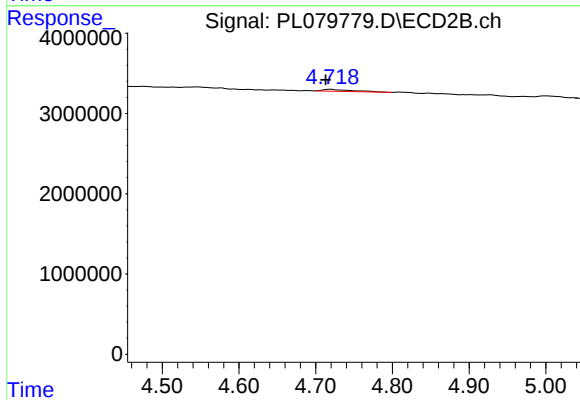


#10 gamma-Chlordane

R.T.: 4.720 min
Delta R.T.: 0.006 min
Response: 656364
Conc: 0.19 ng/ml

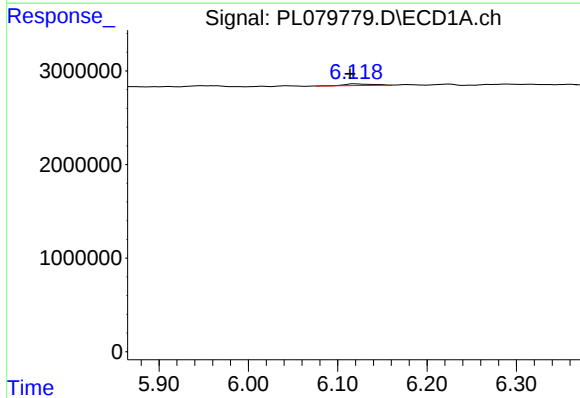


#13 Dieldrin

R.T.: 6.119 min
Delta R.T.: 0.005 min
Response: 380810
Conc: 0.14 ng/ml

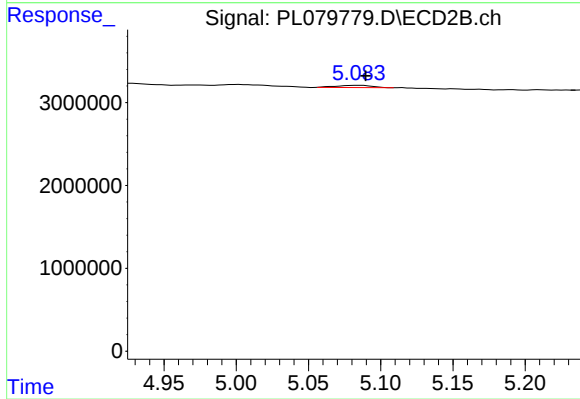

#13 Dieldrin


R.T.: 5.085 min
Delta R.T.: -0.005 min
Response: 458729
Conc: 0.14 ng/ml

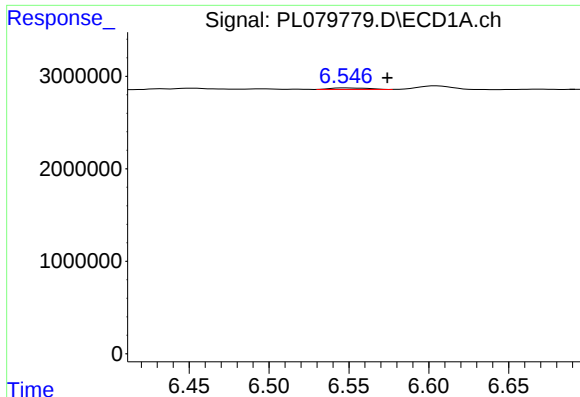

#15 Endosulfan II


R.T.: 6.548 min
Delta R.T.: -0.026 min
Response: 270720
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
WASTE

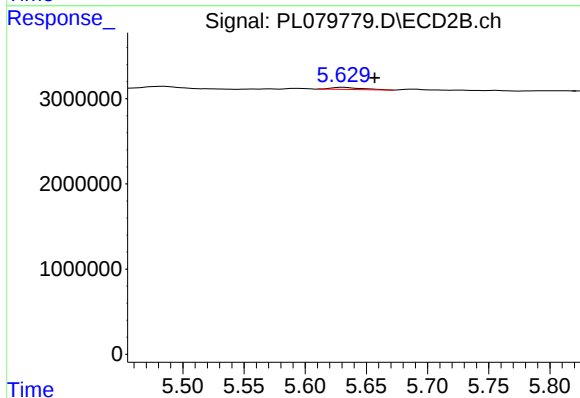


#15 Endosulfan II

R.T.: 5.631 min
Delta R.T.: -0.026 min
Response: 416048
Conc: 0.15 ng/ml

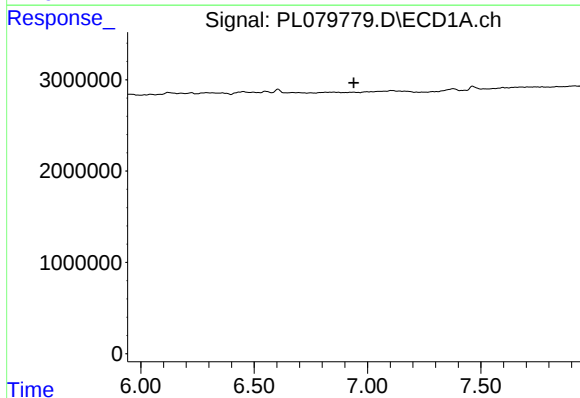


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.939 min
Response: 0
Conc: N.D.

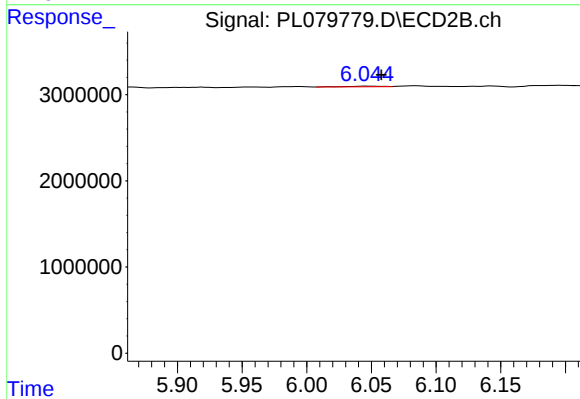

#19 Endosulfan Sulfate


R.T.: 6.046 min
Delta R.T.: -0.012 min
Response: 166460
Conc: 0.06 ng/ml

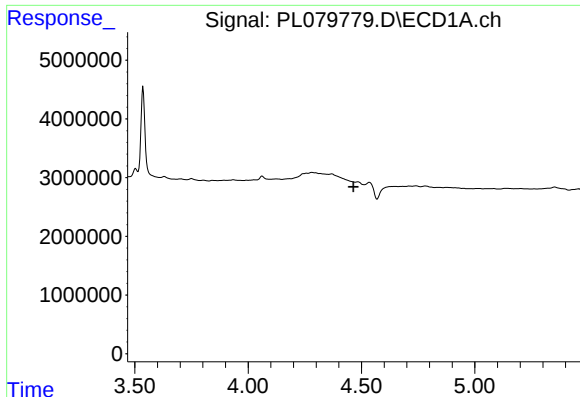

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WASTE

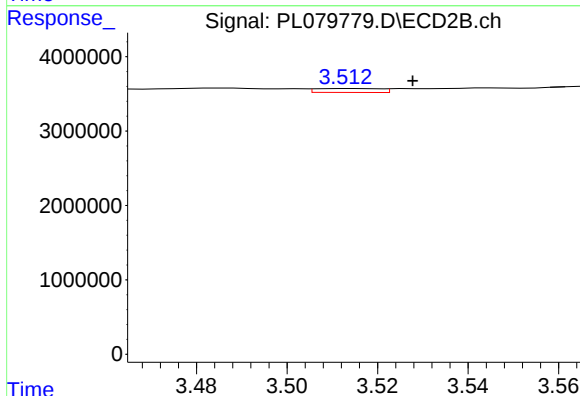


#23 Chlordane-1

R.T.: 3.514 min
Delta R.T.: -0.013 min
Response: 520698
Conc: 4.90 ng/ml

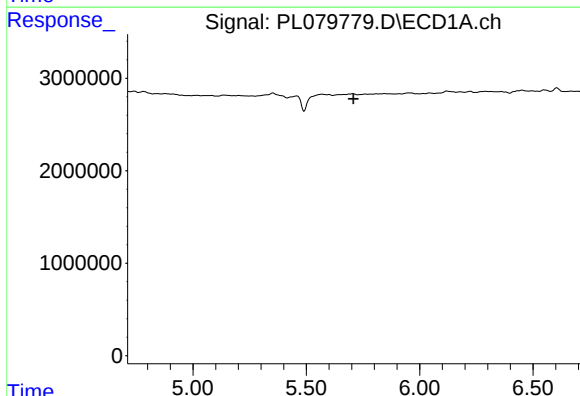


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.709 min
Response: 0
Conc: N.D.

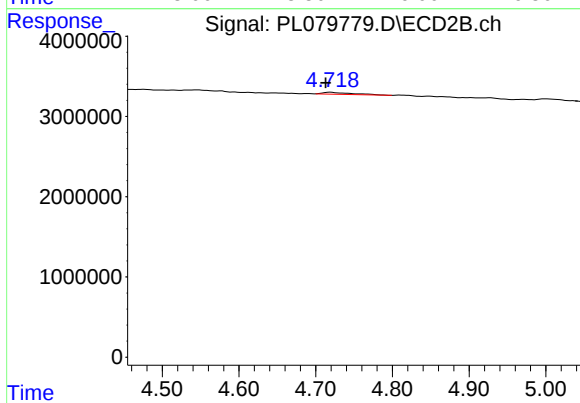

#25 Chlordane-3


R.T.: 4.720 min
Delta R.T.: 0.006 min
Response: 656364
Conc: 1.96 ng/ml

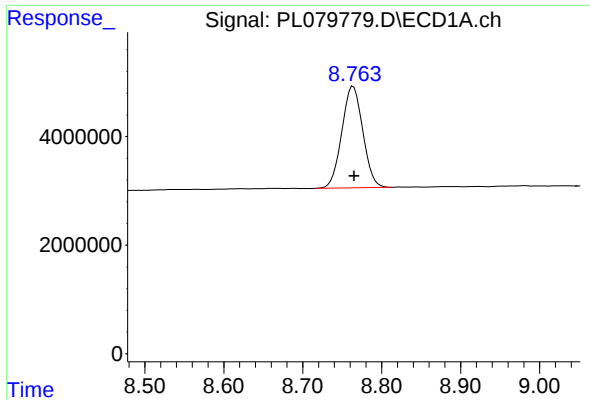

#28 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: -0.001 min
Response: 34589105
Conc: 17.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
WASTE

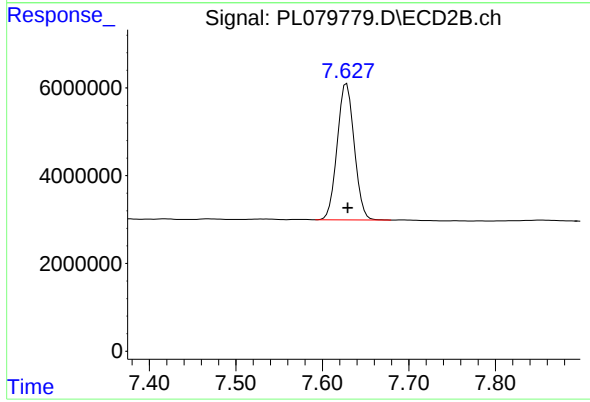

#28 Decachlorobiphenyl

R.T.: 7.628 min
Delta R.T.: 0.000 min
Response: 42329452
Conc: 18.02 ng/ml