

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121922\
 Data File : PL079766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2022 13:51
 Operator : AR\AJ
 Sample : N6097-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FVSUB-TP1-COMP-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 20:29:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	2.563	26507414	31968528	11.734	11.744
28)	SA Decachlor...	8.765	7.629	19908290	24468732	10.251	10.415
Target Compounds							
11)	B alpha-Chl...	5.786	4.771	2666649	1922609	0.925	0.574 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121922\
Data File : PL079766.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2022 13:51
Operator : AR\AJ
Sample : N6097-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FVSUB-TP1-COMP-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 20:29:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

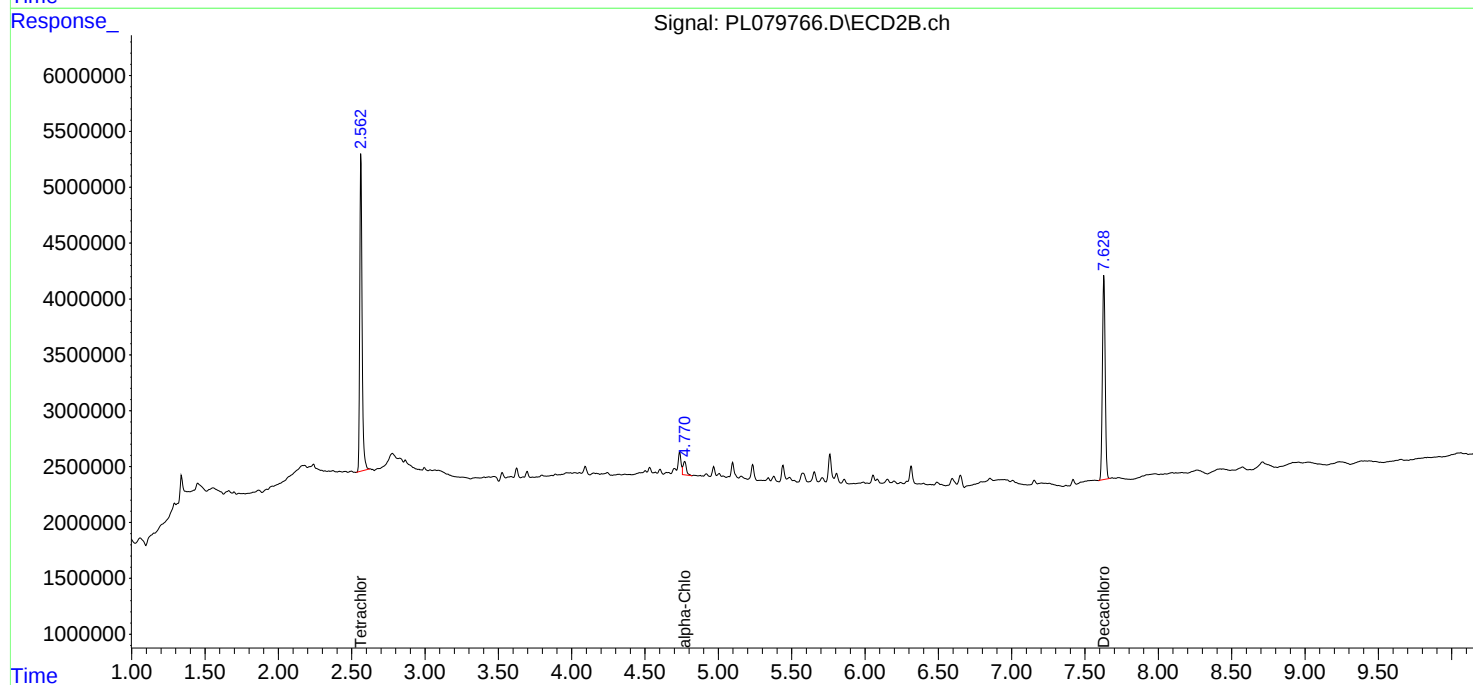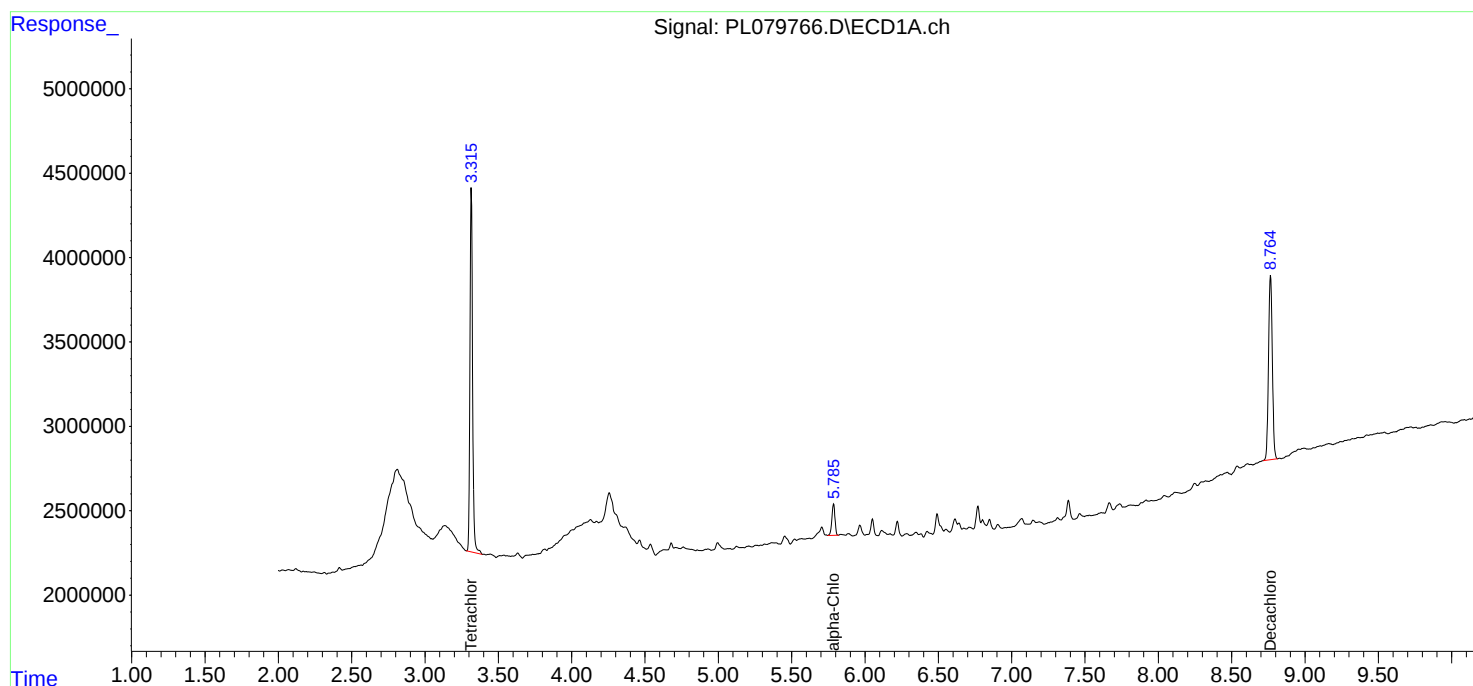


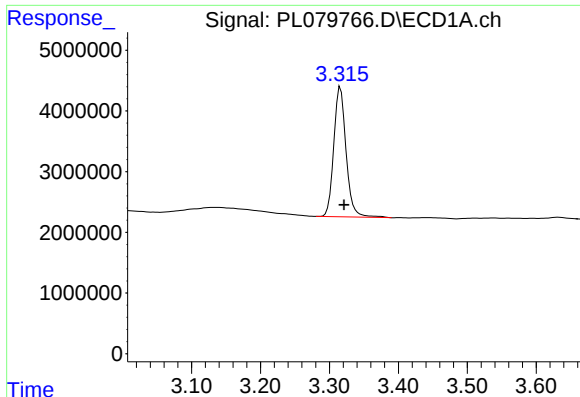

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.005 min
Response: 26507414
Conc: 11.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
FVSUB-TP1-COMP-01

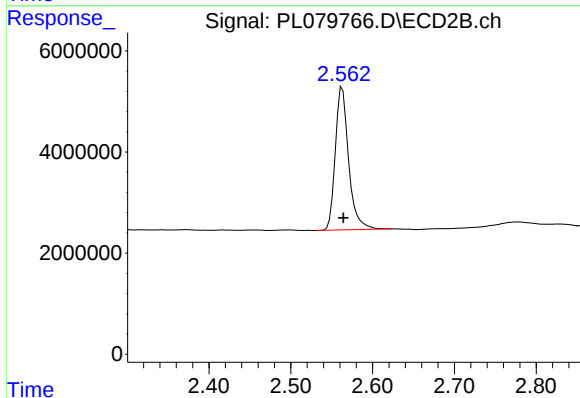


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: -0.001 min
Response: 31968528
Conc: 11.74 ng/ml

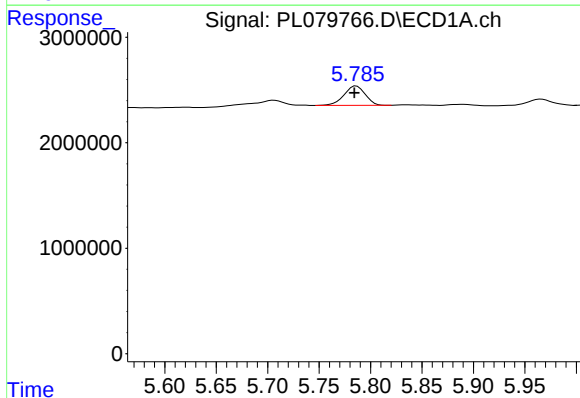


#11 alpha-Chlordane

R.T.: 5.786 min
Delta R.T.: 0.002 min
Response: 2666649
Conc: 0.93 ng/ml

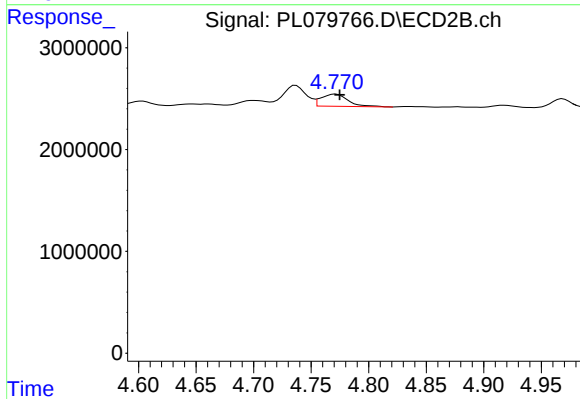

#11 alpha-Chlordane


R.T.: 4.771 min
Delta R.T.: -0.004 min
Response: 1922609
Conc: 0.57 ng/ml

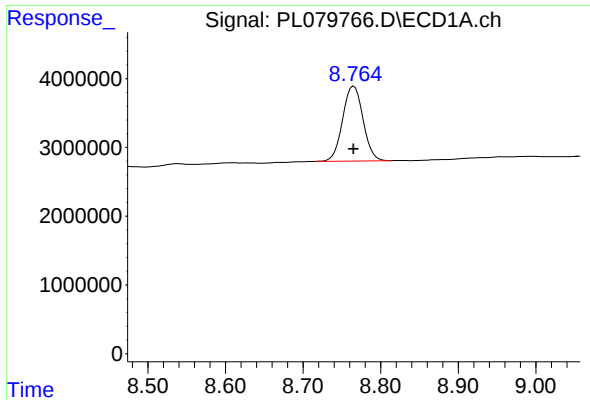

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 19908290
Conc: 10.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
FVSUB-TP1-COMP-01

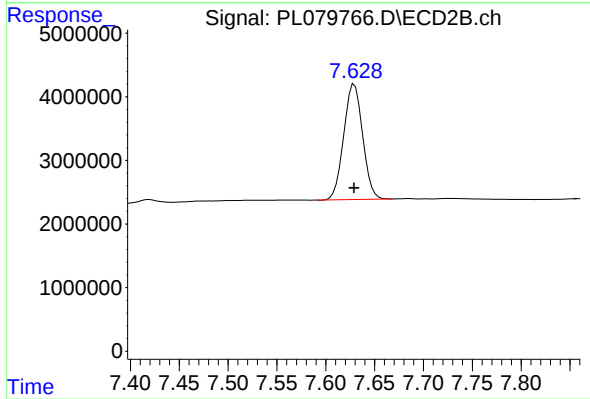

#28 Decachlorobiphenyl

R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 24468732
Conc: 10.42 ng/ml