

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121924\
 Data File : PL093447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 18:15
 Operator : AR\AJ
 Sample : P5330-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/20/2024
 Supervised By : Ankita Jodhani 12/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 21:54:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 15:18:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.538	2.775	38767271	42186019	14.916	14.628
28) SA Decachlor...	9.051	7.911	32368580	47635040	18.618	16.676
Target Compounds						
17) MA 4,4'-DDT	7.020	6.031	793507	1328407	0.412m	0.449m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121924\
Data File : PL093447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 18:15
Operator : AR\AJ
Sample : P5330-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/20/2024
Supervised By : Ankita Jodhani 12/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 21:54:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 15:18:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

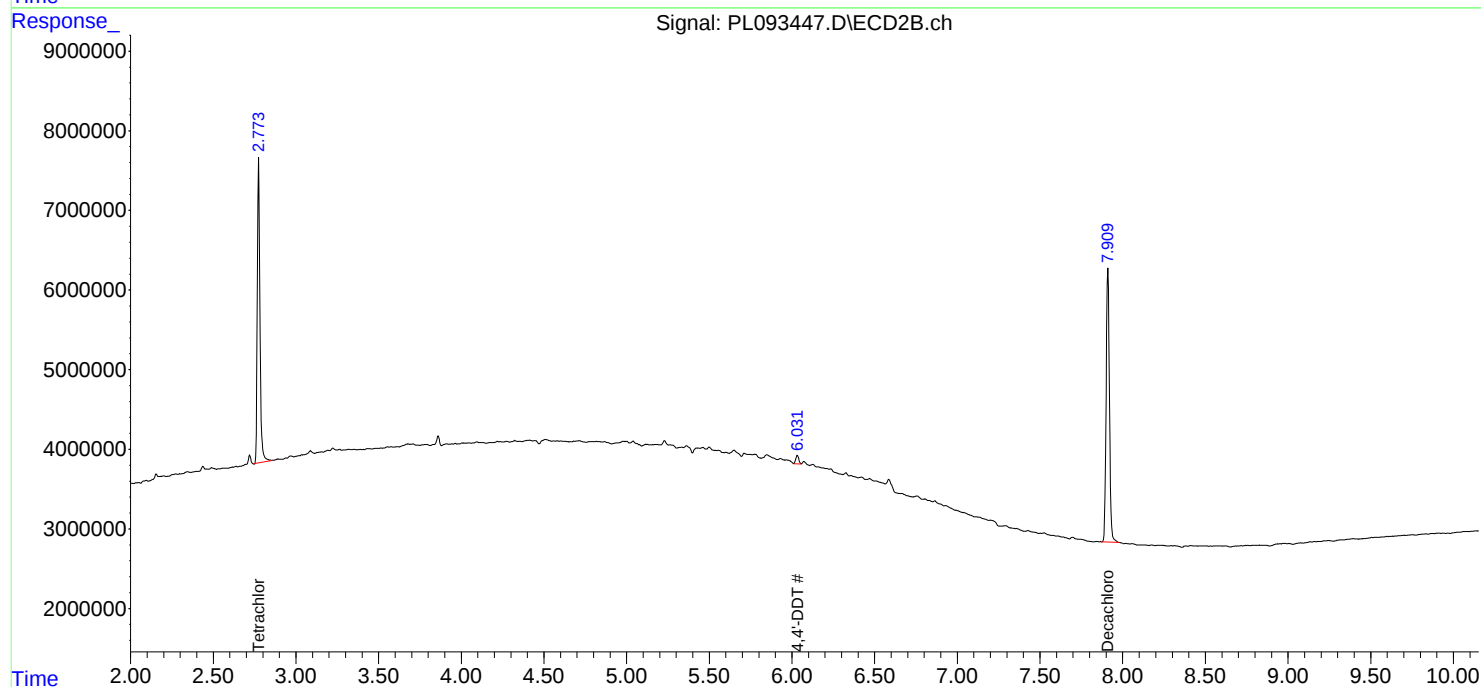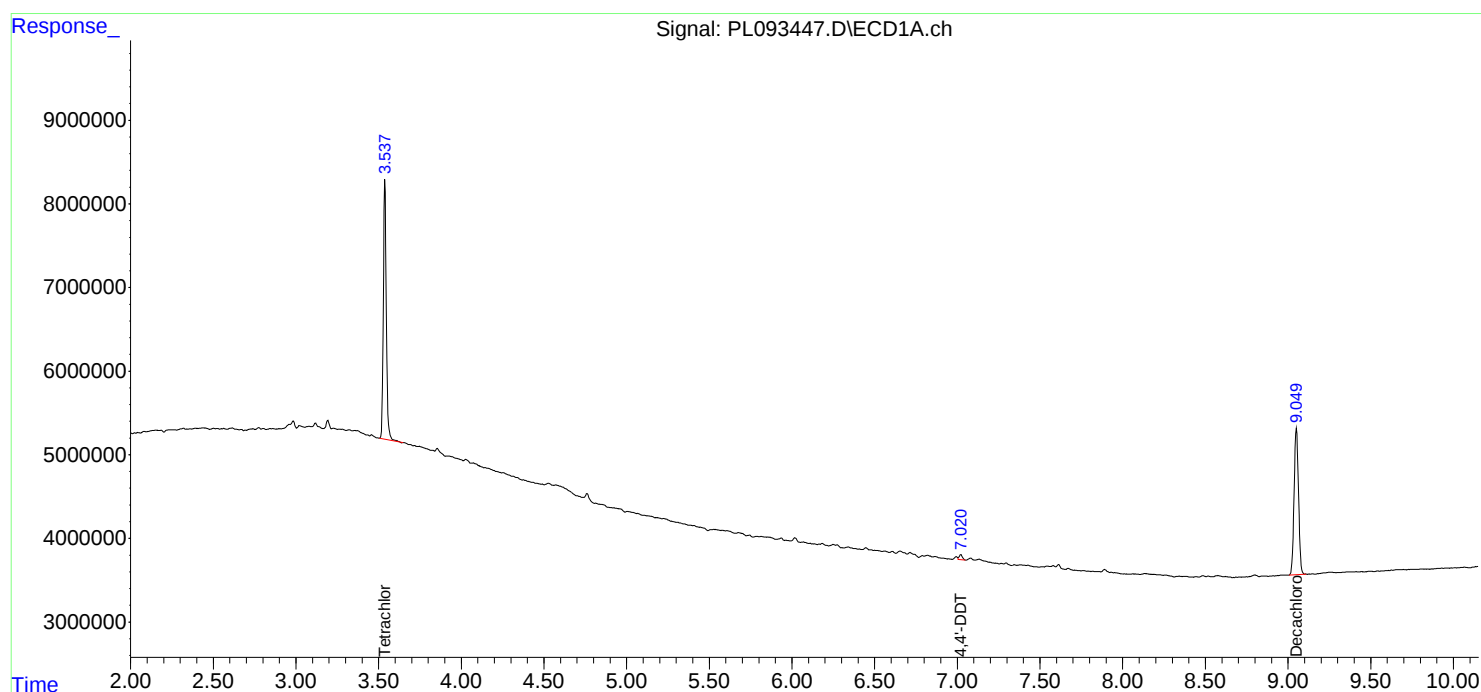

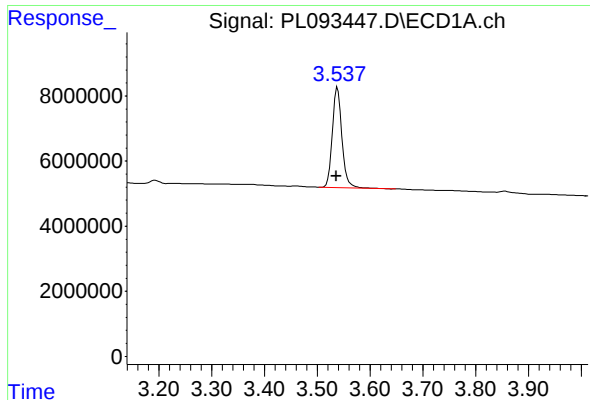


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.002 min
Response: 38767271
Conc: 14.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/20/2024
Supervised By :Ankita Jodhani 12/20/2024

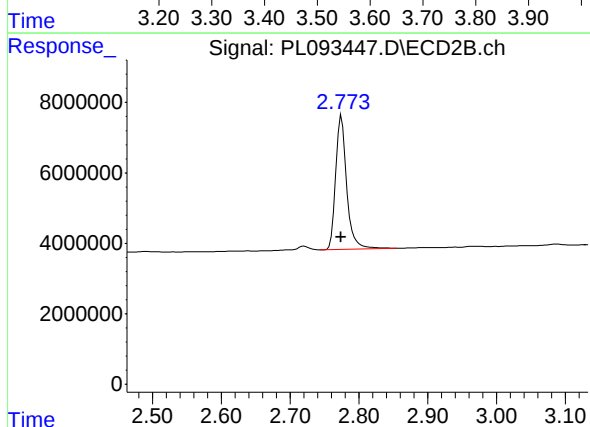


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 42186019
Conc: 14.63 ng/ml

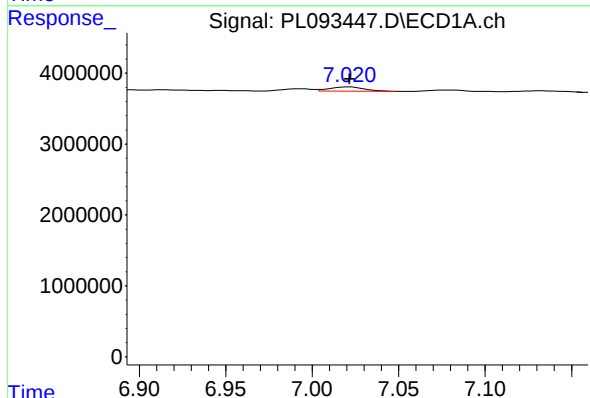


#17 4,4'-DDT

R.T.: 7.020 min
Delta R.T.: -0.002 min
Response: 793507
Conc: 0.41 ng/ml m

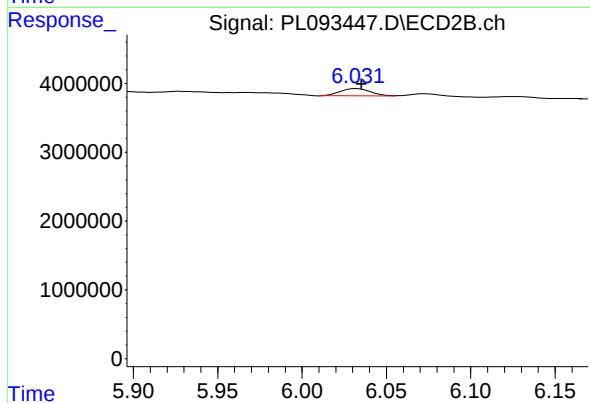

#17 4,4'-DDT

R.T.: 6.031 min
Delta R.T.: -0.004 min
Response: 1328407
Conc: 0.45 ng/ml m

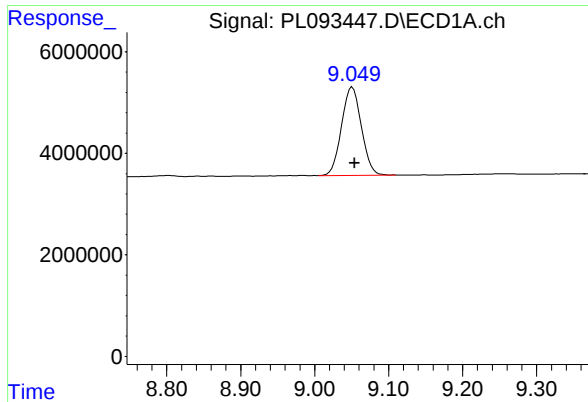


#28 Decachlorobiphenyl

R.T.: 9.051 min
Delta R.T.: -0.003 min
Response: 32368580
Conc: 18.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/20/2024
Supervised By :Ankita Jodhani 12/20/2024

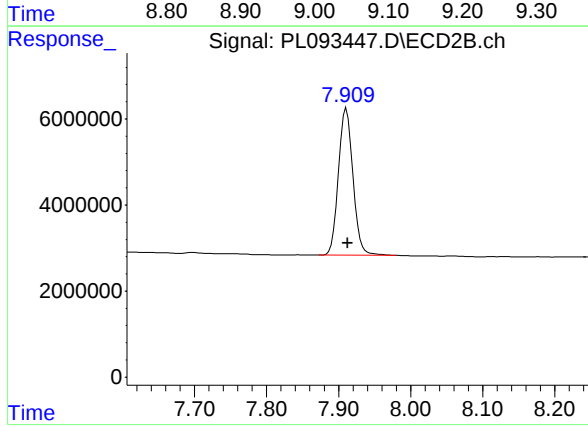

#28 Decachlorobiphenyl

R.T.: 7.911 min
Delta R.T.: -0.002 min
Response: 47635040
Conc: 16.68 ng/ml