

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121924\
 Data File : PL093448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 18:28
 Operator : AR\AJ
 Sample : P5339-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-06-12182024

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/20/2024
 Supervised By :Ankita Jodhani 12/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 21:54:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 15:18:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.773	34458637	38756887	13.259m	13.438m
28) SA Decachlor...	9.051	7.910	29432476	40891626	16.929	14.316

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121924\
Data File : PL093448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 18:28
Operator : AR\AJ
Sample : P5339-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-06-12182024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/20/2024
Supervised By : Ankita Jodhani 12/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time : Dec 19 21:54:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 15:18:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

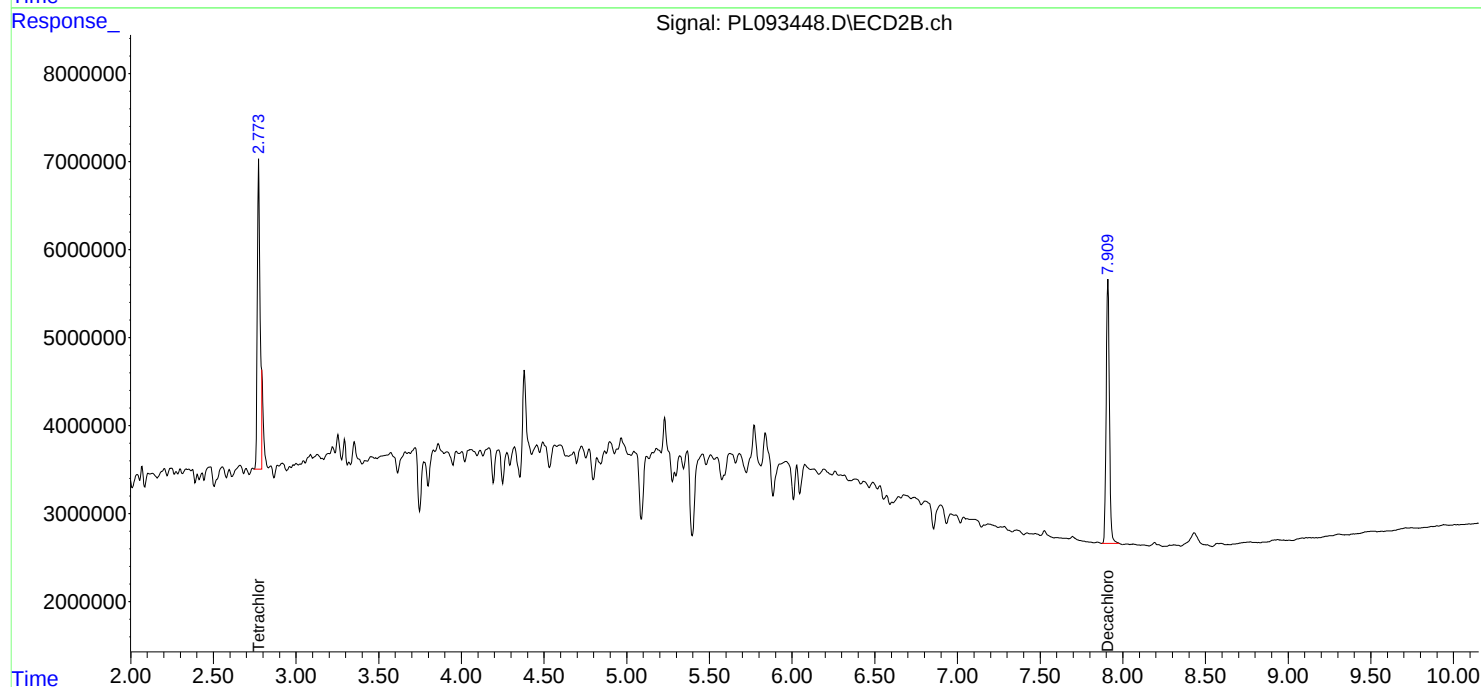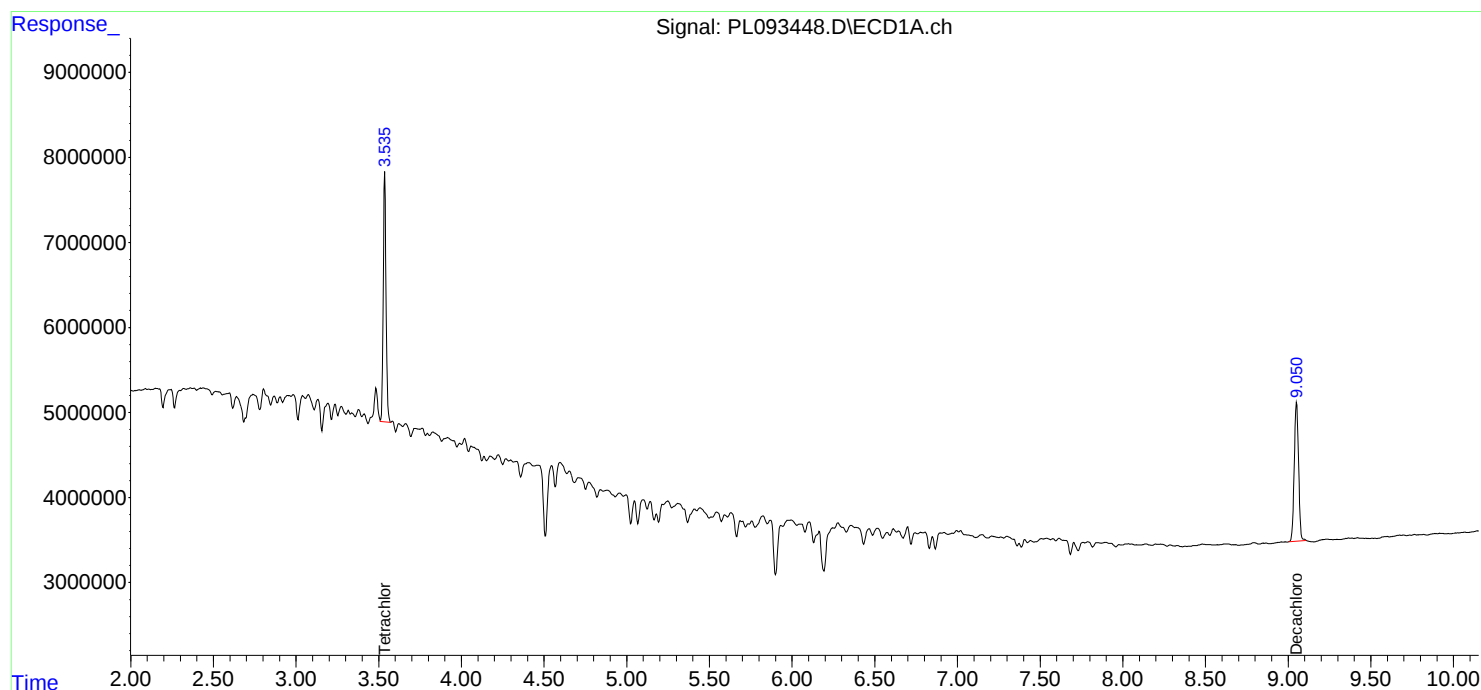

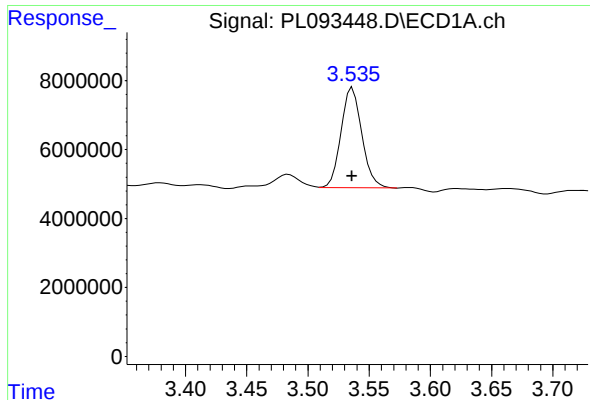


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 34458637
Conc: 13.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-06-12182024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/20/2024
Supervised By :Ankita Jodhani 12/20/2024

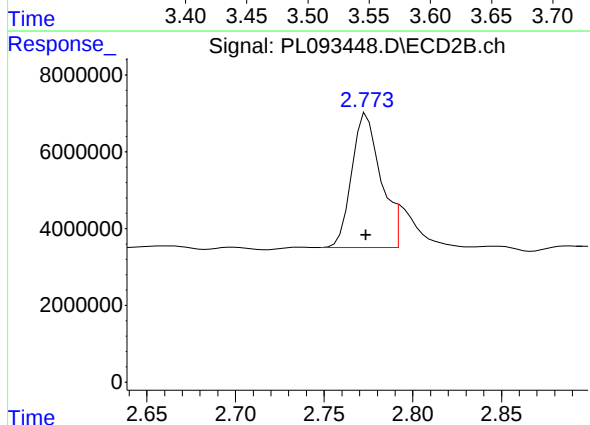


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 38756887
Conc: 13.44 ng/ml m

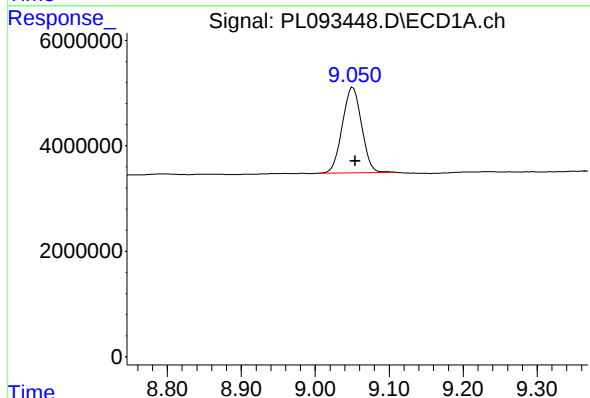

#28 Decachlorobiphenyl

R.T.: 9.051 min
Delta R.T.: -0.003 min
Response: 29432476
Conc: 16.93 ng/ml

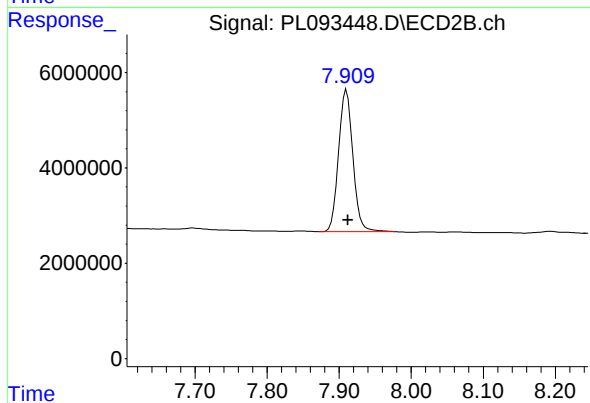

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.002 min
Response: 40891626
Conc: 14.32 ng/ml