

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121924\
 Data File : PL093458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 21:10
 Operator : AR\AJ
 Sample : P5342-03 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HT2651

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/20/2024
 Supervised By : Ankita Jodhani 12/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 10:06:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 15:18:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.791f	2292936	11550474	0.882m	4.005m#
28) SA Decachlor...	9.049	7.911	4069891	7846012	2.341m	2.747

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121924\
Data File : PL093458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 21:10
Operator : AR\AJ
Sample : P5342-03 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HT2651


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/20/2024
Supervised By : Ankita Jodhani 12/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 10:06:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 15:18:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

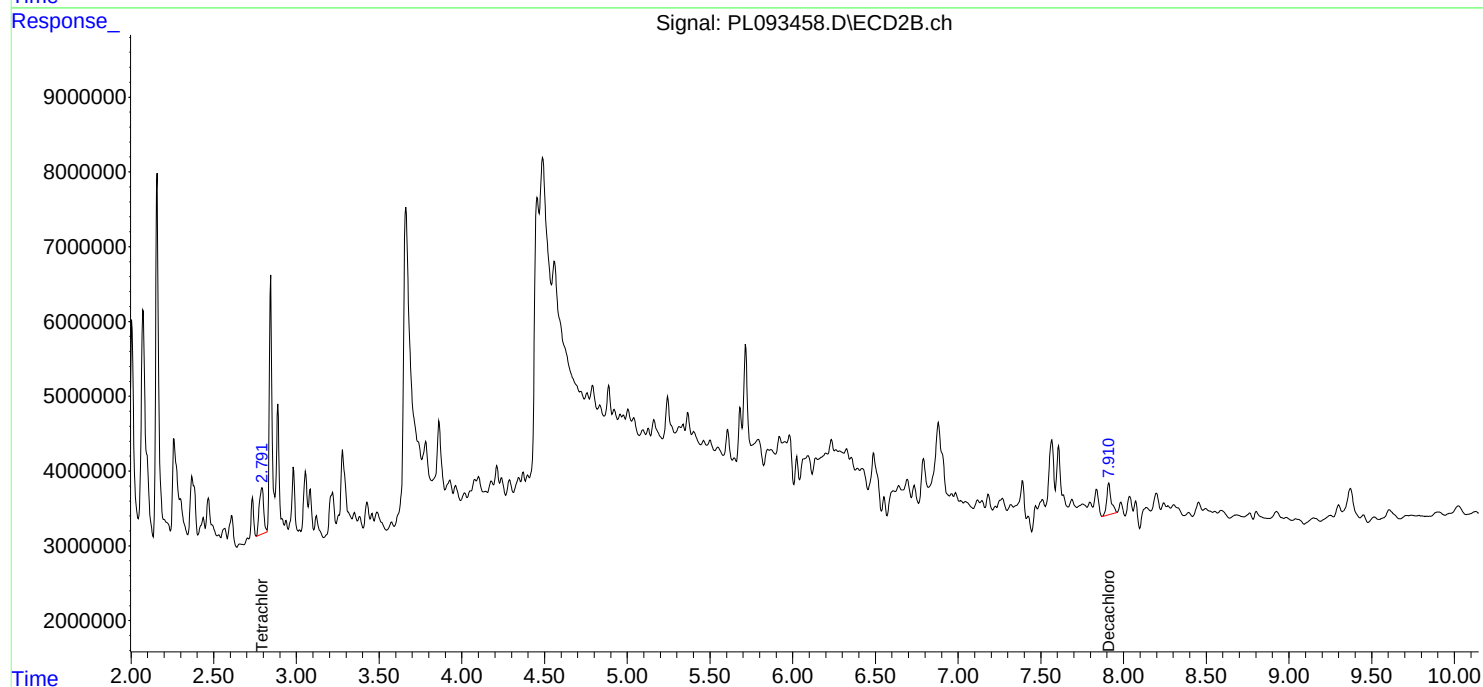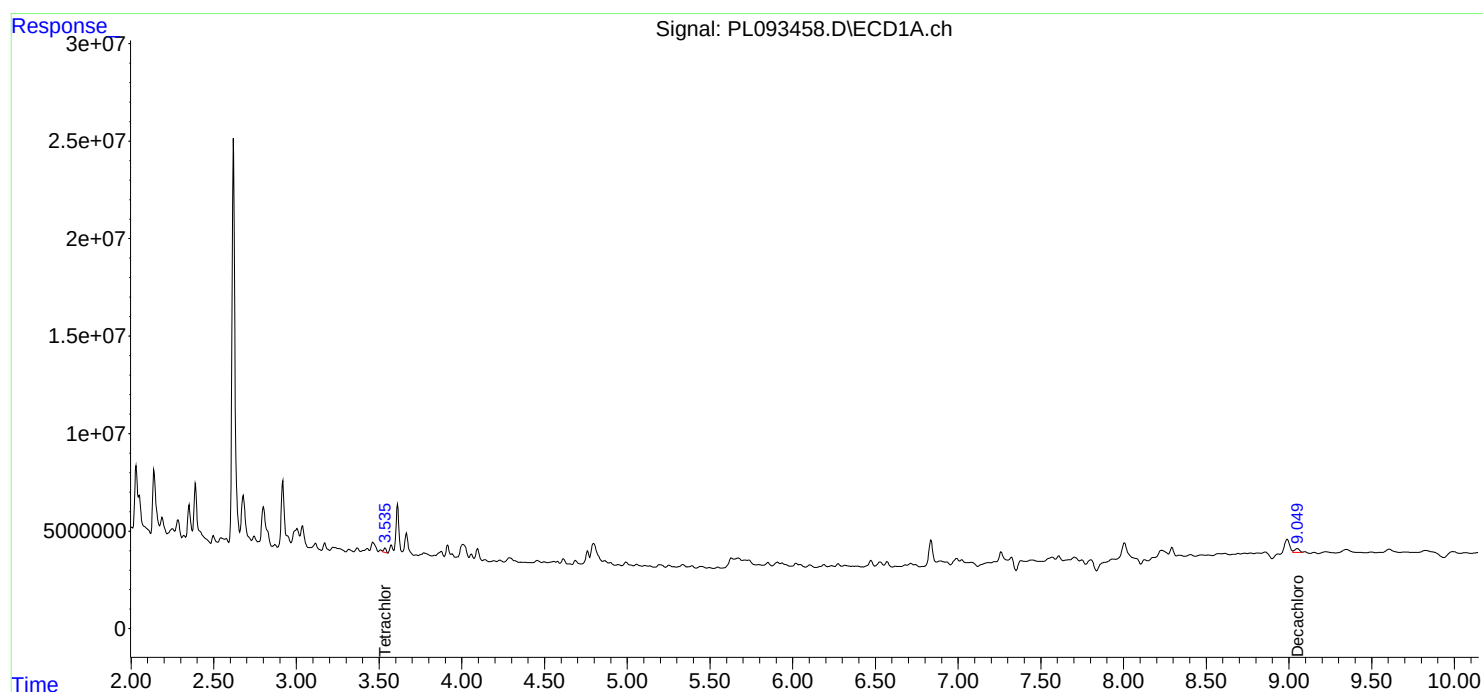

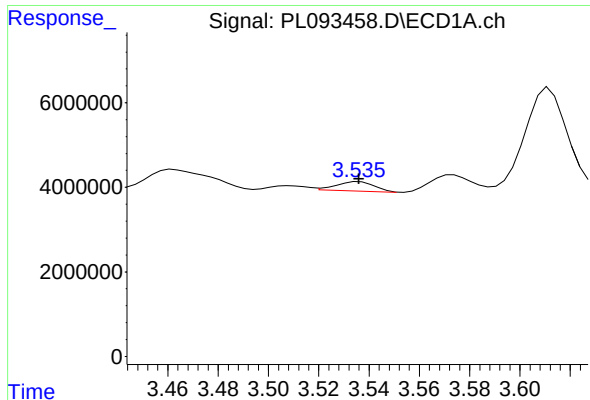


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.001 min
Response: 2292936
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
HT2651


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/20/2024
Supervised By :Ankita Jodhani 12/20/2024

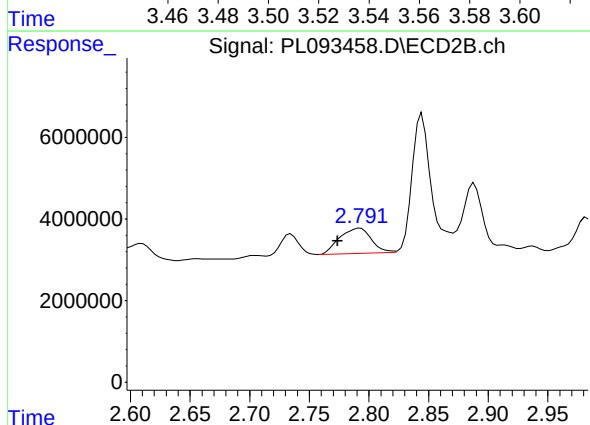


#1 Tetrachloro-m-xylene

R.T.: 2.791 min
Delta R.T.: 0.018 min
Response: 11550474
Conc: 4.00 ng/ml m

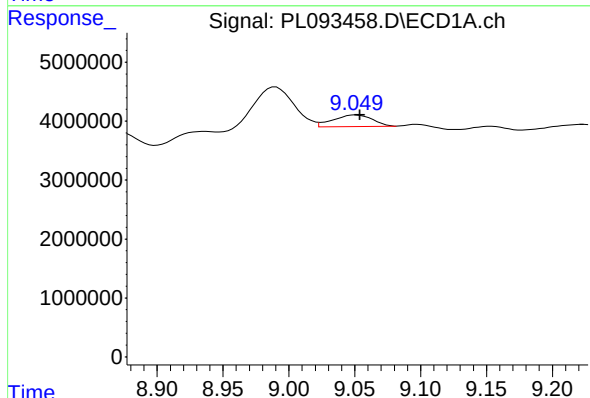

#28 Decachlorobiphenyl

R.T.: 9.049 min
Delta R.T.: -0.005 min
Response: 4069891
Conc: 2.34 ng/ml m

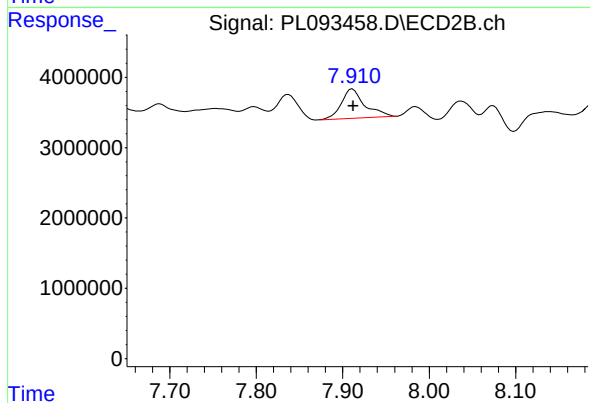

#28 Decachlorobiphenyl

R.T.: 7.911 min
Delta R.T.: -0.001 min
Response: 7846012
Conc: 2.75 ng/ml