

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122018\
 Data File : PL043339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2018 15:46
 Operator : AJ\SJ
 Sample : J6465-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 01:02:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.099	146.0E6	74863151	23.812	25.258
28)	SA Decachlor...	8.199	9.227	118.5E6	50289709	18.148	19.279
Target Compounds							
6)	B beta-BHC	4.396f	0.000	2957063	0	0.802	N.D. #
8)	B Heptachlo...	5.109f	6.001	2044058	3390675	0.258	0.894 #
9)	A Endosulfan I	5.452f	6.342	2612554	2199767	0.357	0.648 #
10)	B gamma-Chl...	5.452f	6.234	2612554	-244739	0.324	N.D. #
11)	B alpha-Chl...	5.452	6.306	2612554	550257	0.329	0.153 #
14)	MA Endrin	6.067f	0.000	761089	0	0.106	N.D. #
16)	A 4,4'-DDD	6.067f	0.000	761089	0	0.134	N.D. #
23)	Chlordane-1	4.375	0.000	2780739	0	10.349	N.D. #
25)	Chlordane-3	5.452	6.234	2612554	-244739	3.144	N.D. #
26)	Chlordane-4	5.452	6.306	2612554	550257	3.455	0.964 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122018\
Data File : PL043339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2018 15:46
Operator : AJ\SJ
Sample : J6465-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 01:02:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

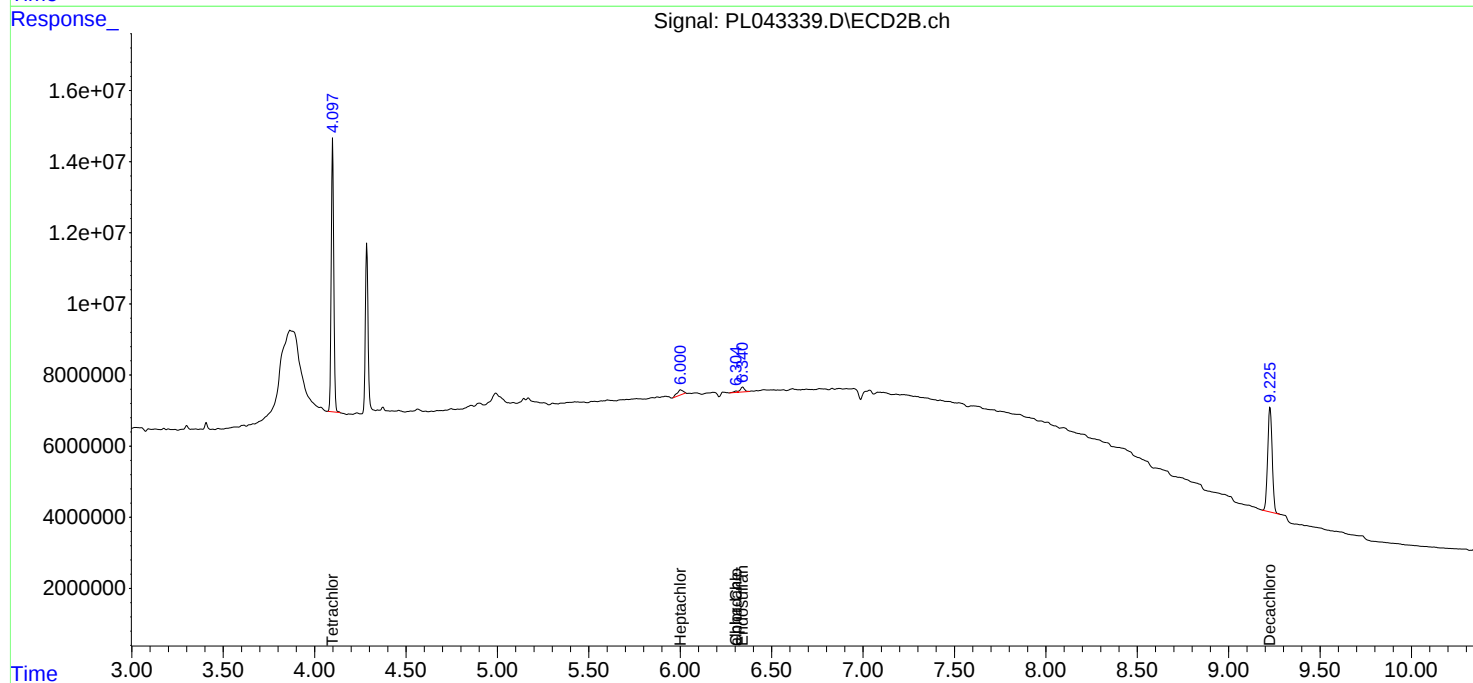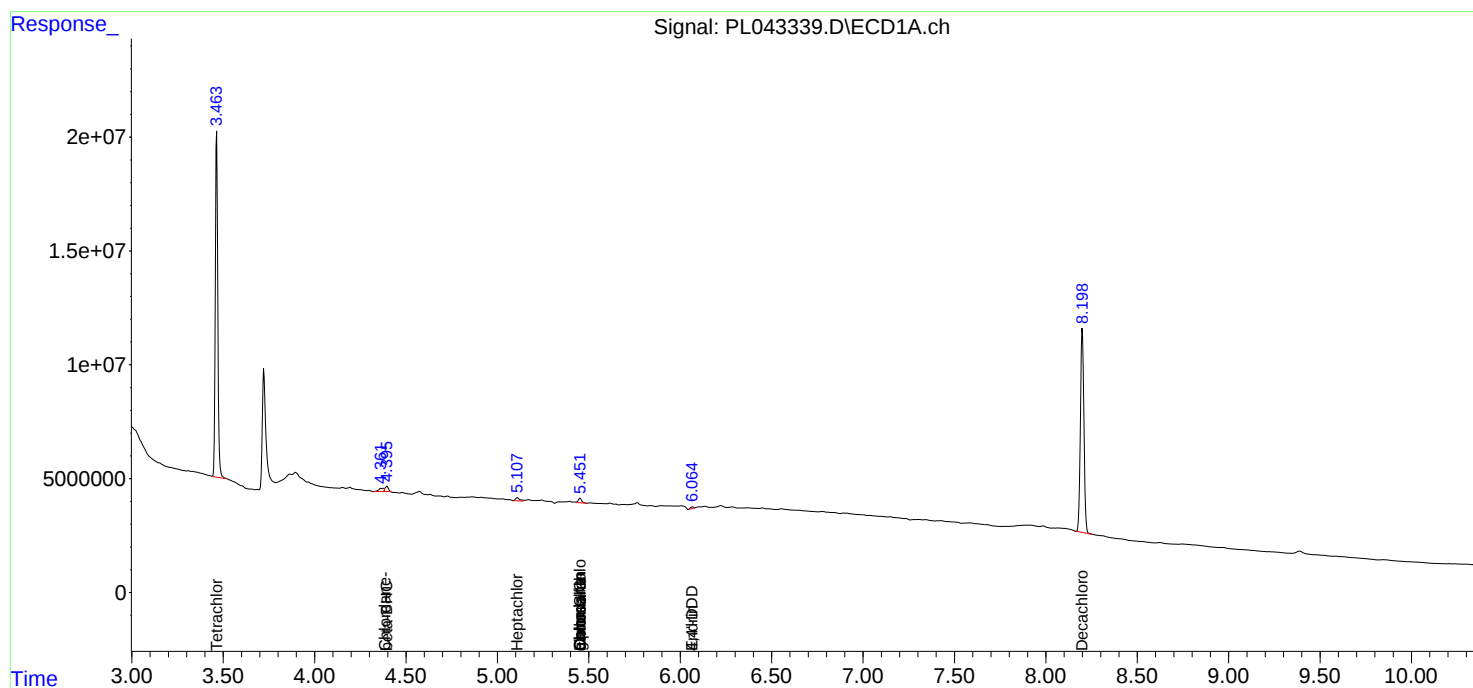


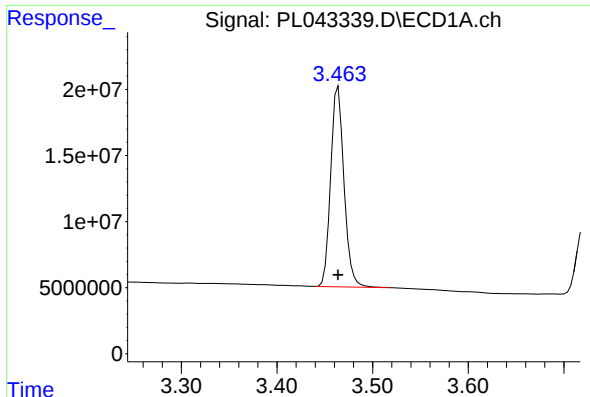

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 146038740
Conc: 23.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

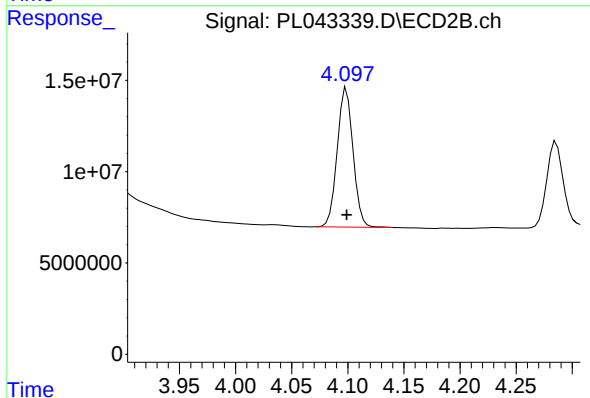


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 74863151
Conc: 25.26 ng/ml

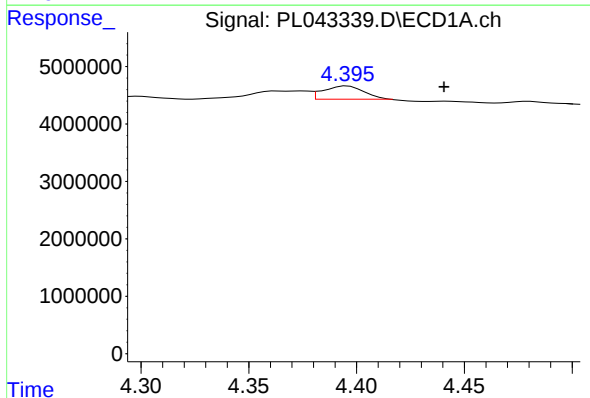


#6 beta-BHC

R.T.: 4.396 min
Delta R.T.: -0.045 min
Response: 2957063
Conc: 0.80 ng/ml

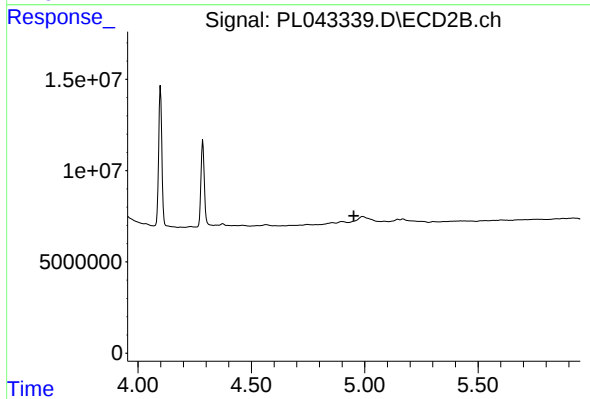

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

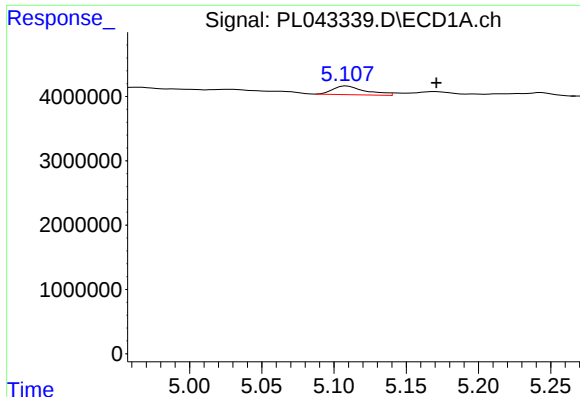

#8 Heptachlor epoxide


R.T.: 5.109 min
Delta R.T.: -0.062 min
Response: 2044058
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

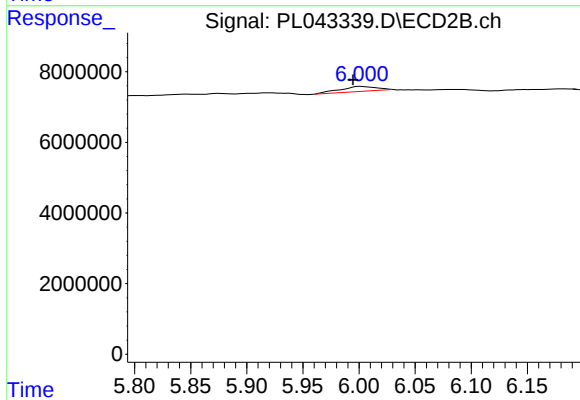


#8 Heptachlor epoxide

R.T.: 6.001 min
Delta R.T.: 0.007 min
Response: 3390675
Conc: 0.89 ng/ml

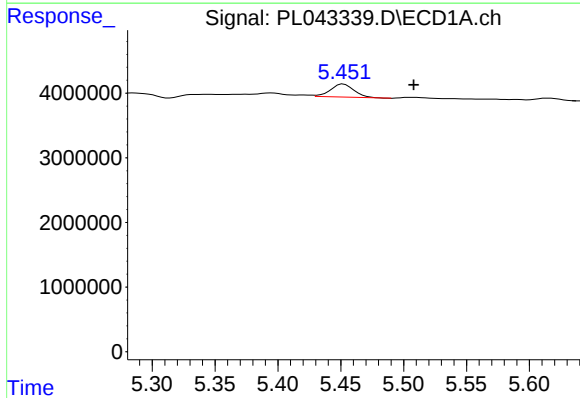


#9 Endosulfan I

R.T.: 5.452 min
Delta R.T.: -0.056 min
Response: 2612554
Conc: 0.36 ng/ml

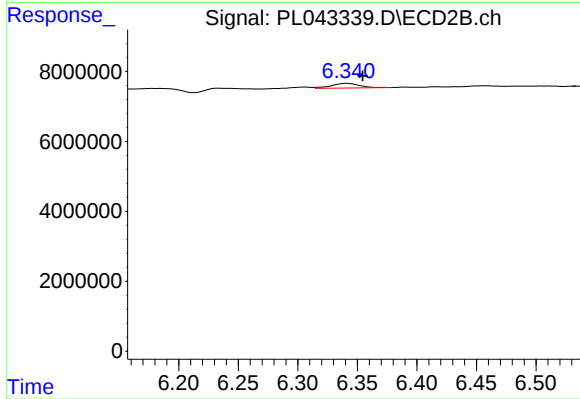

#9 Endosulfan I


R.T.: 6.342 min
Delta R.T.: -0.013 min
Response: 2199767
Conc: 0.65 ng/ml

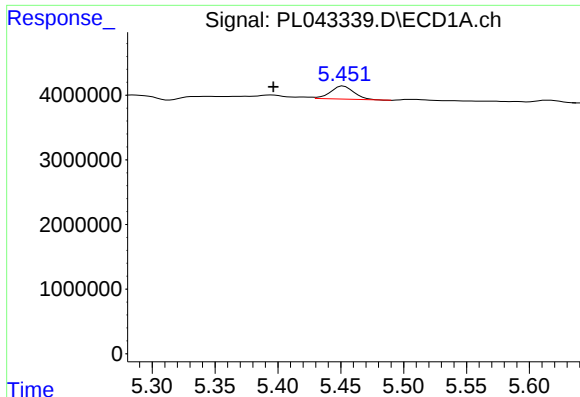

#10 gamma-Chlordane


R.T.: 5.452 min
Delta R.T.: 0.056 min
Response: 2612554
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

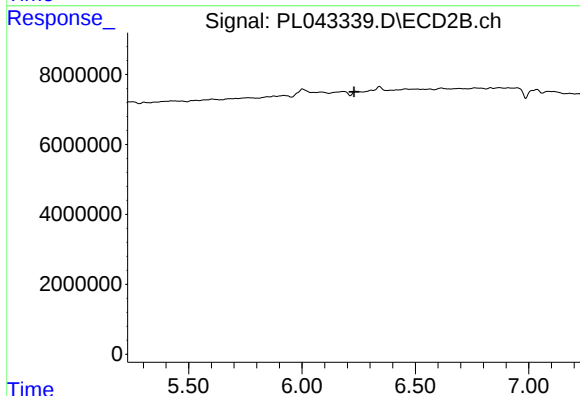


#10 gamma-Chlordane

R.T.: 6.234 min
Delta R.T.: 0.005 min
Response: -244739
Conc: N.D.

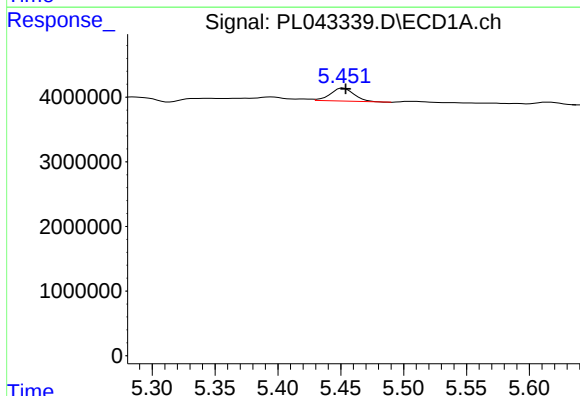


#11 alpha-Chlordane

R.T.: 5.452 min
Delta R.T.: -0.002 min
Response: 2612554
Conc: 0.33 ng/ml

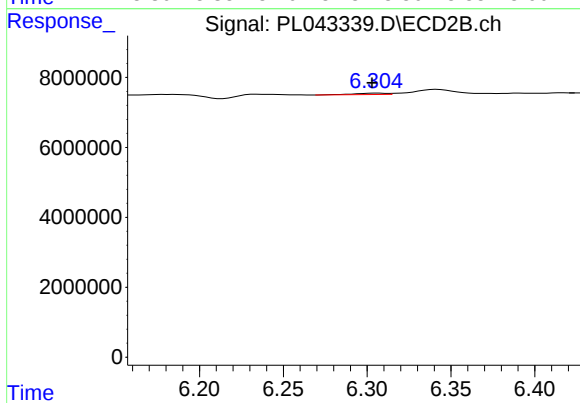

#11 alpha-Chlordane


R.T.: 6.306 min
Delta R.T.: 0.003 min
Response: 550257
Conc: 0.15 ng/ml

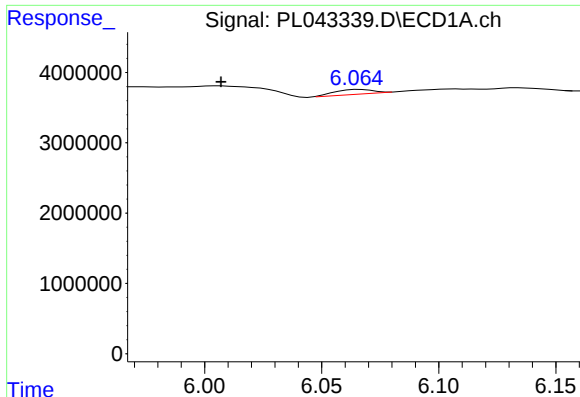

#14 Endrin


R.T.: 6.067 min
Delta R.T.: 0.060 min
Response: 761089
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

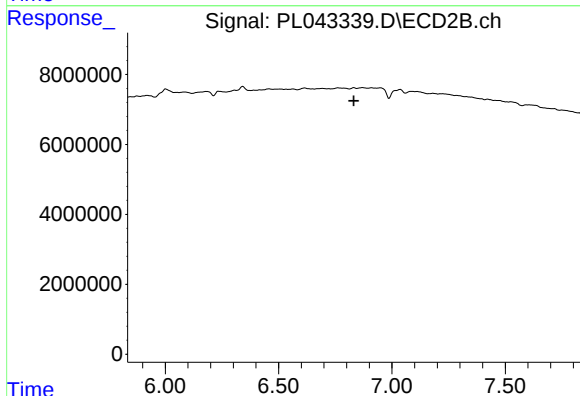


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

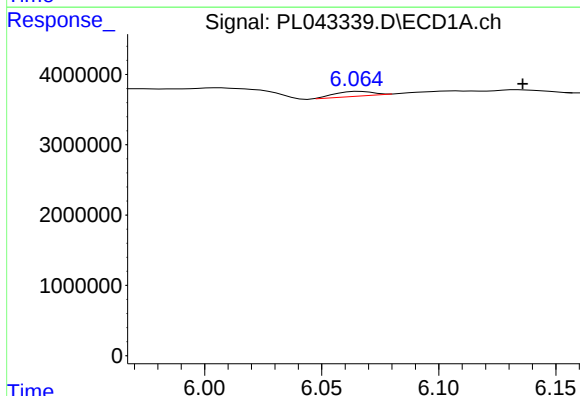


#16 4,4'-DDD

R.T.: 6.067 min
Delta R.T.: -0.069 min
Response: 761089
Conc: 0.13 ng/ml

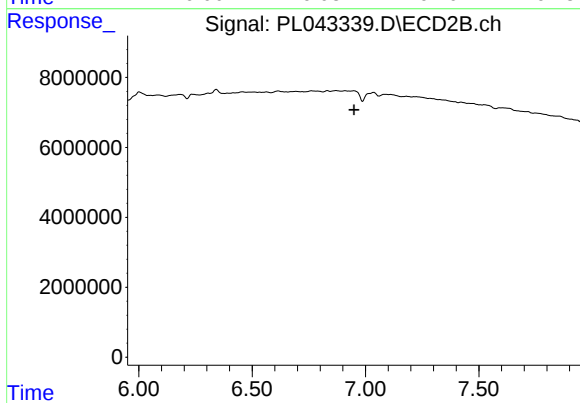

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

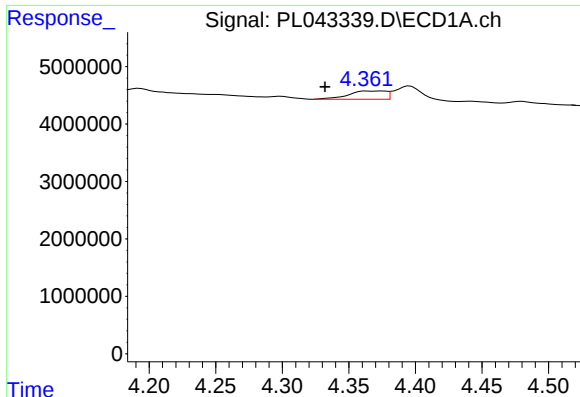

#23 Chlordane-1


R.T.: 4.375 min
Delta R.T.: 0.043 min
Response: 2780739
Conc: 10.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

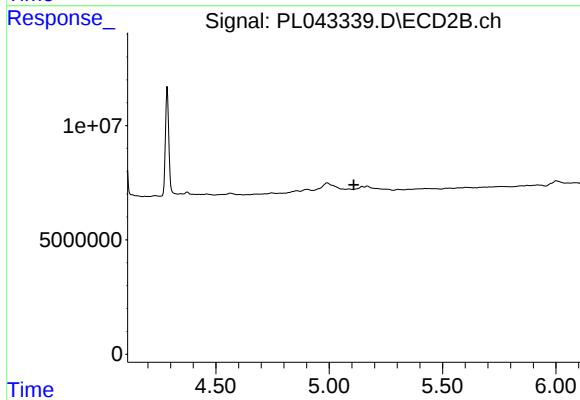


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

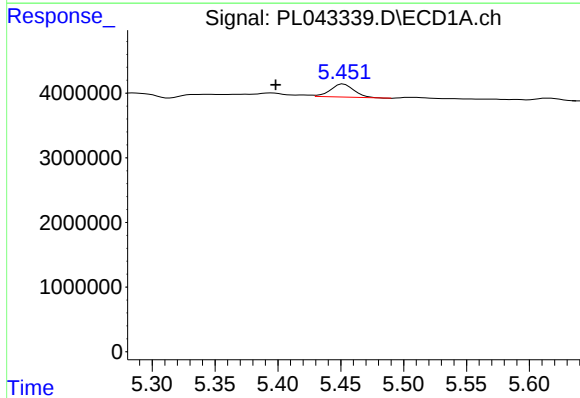


#25 Chlordane-3

R.T.: 5.452 min
Delta R.T.: 0.054 min
Response: 2612554
Conc: 3.14 ng/ml

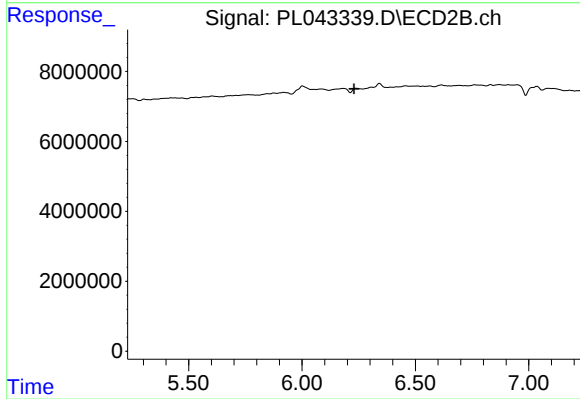

#25 Chlordane-3


R.T.: 6.234 min
Delta R.T.: 0.004 min
Response: -244739
Conc: N.D.

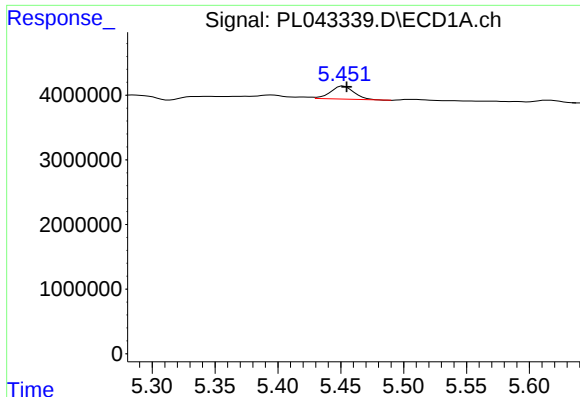

#26 Chlordane-4


R.T.: 5.452 min
Delta R.T.: -0.003 min
Response: 2612554
Conc: 3.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

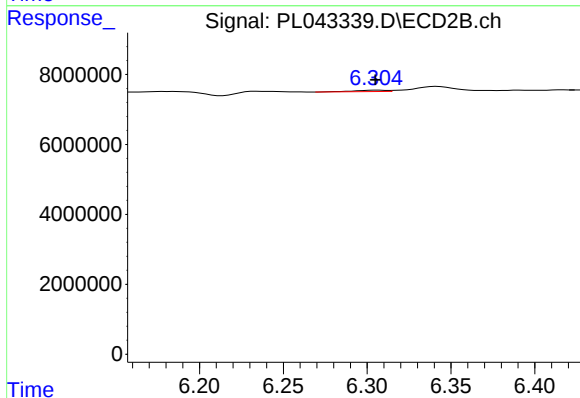


#26 Chlordane-4

R.T.: 6.306 min
Delta R.T.: 0.001 min
Response: 550257
Conc: 0.96 ng/ml

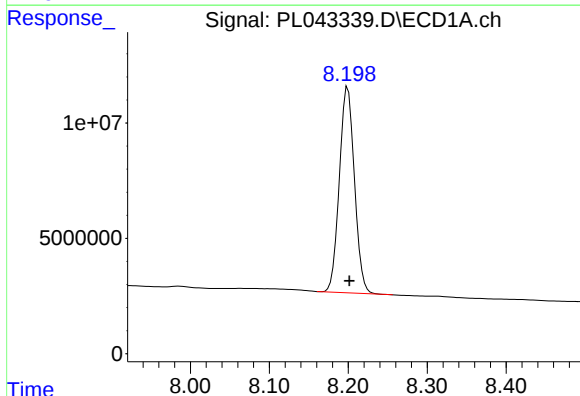

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: -0.002 min
Response: 118505336
Conc: 18.15 ng/ml

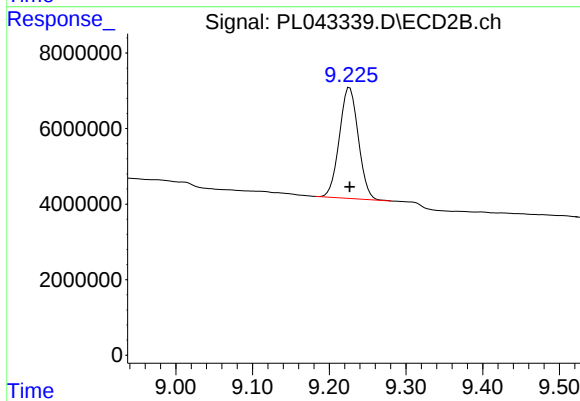

#28 Decachlorobiphenyl

R.T.: 9.227 min
Delta R.T.: 0.000 min
Response: 50289709
Conc: 19.28 ng/ml