

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122019\
 Data File : PL055128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2019 01:48
 Operator : SG\AJ
 Sample : K6107-01 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 12:10:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:58:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.048	46081953	11177269	3.961	4.380
28)	SA Decachlor...	8.312	9.146	30435980	8264869	3.178	3.447
Target Compounds							
6)	B beta-BHC	0.000	4.905	0	6541656	N.D.	4.645 #
8)	B Heptachlo...	5.261	5.920	33482987	10363969	2.214	4.149 #
9)	A Endosulfan I	5.628f	0.000	28794181	0	2.112	N.D. #
10)	B gamma-Chl...	5.480f	0.000	25351584	0	1.672	N.D. #
11)	B alpha-Chl...	5.555	0.000	5974245	0	0.405	N.D. #
23)	Chlordane-1	4.447f	0.000	2661628	0	6.202	N.D. #
25)	Chlordane-3	5.480f	0.000	25351584	0	18.810	N.D. #
26)	Chlordane-4	5.555	0.000	5974245	0	5.388	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122019\
Data File : PL055128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2019 01:48
Operator : SG\AJ
Sample : K6107-01 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 12:10:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:58:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

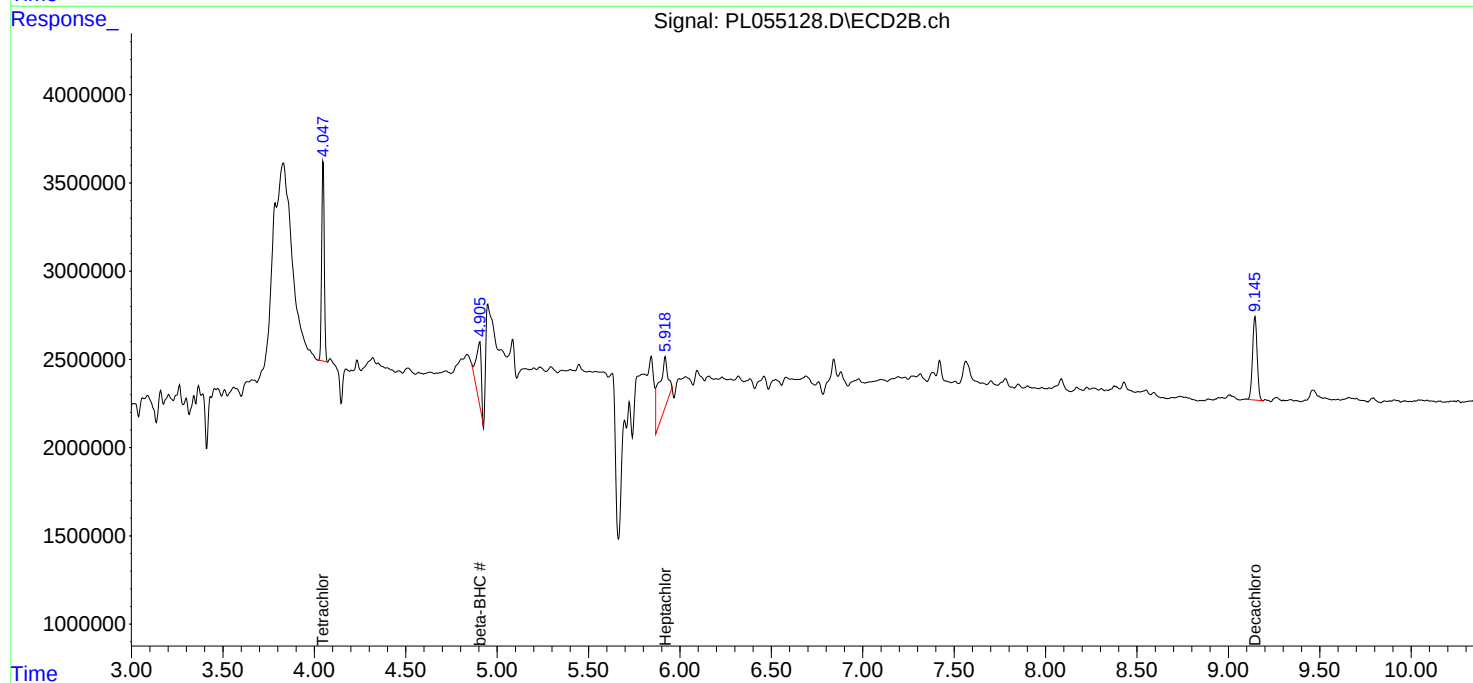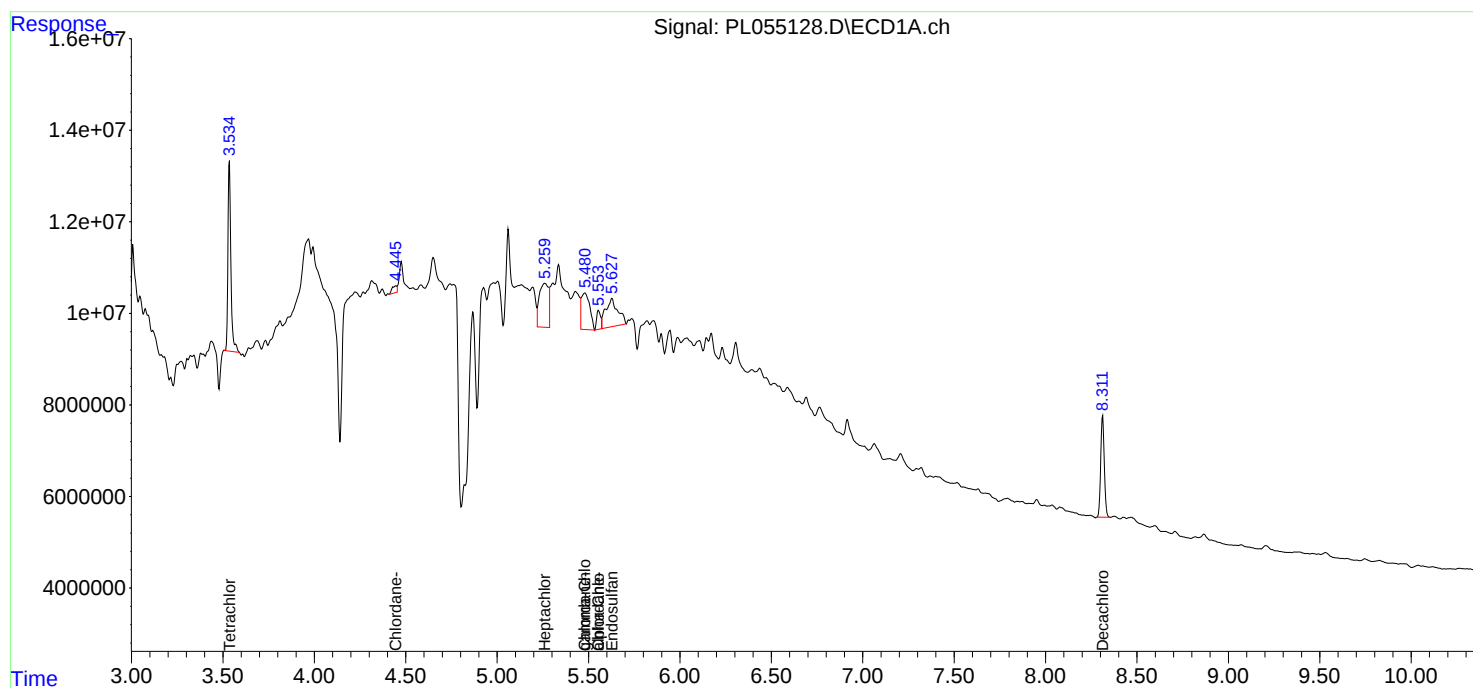


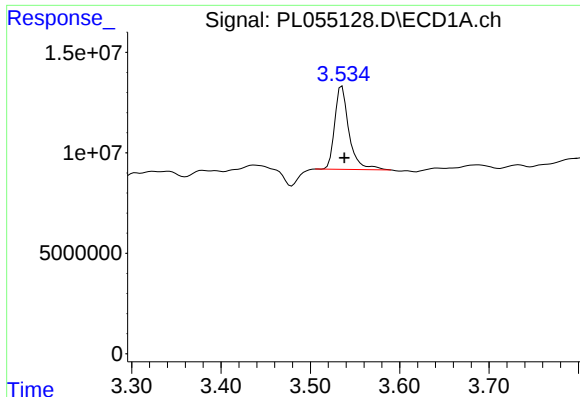

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 46081953
Conc: 3.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

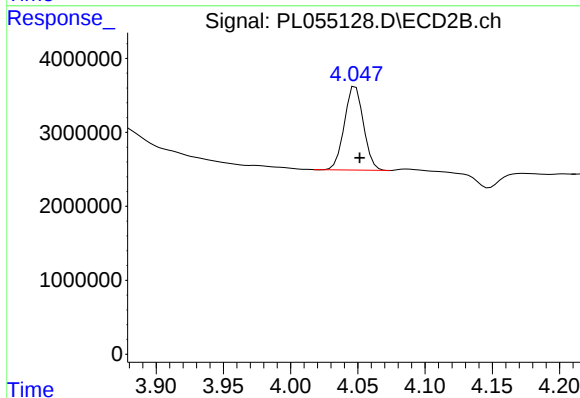


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: -0.003 min
Response: 11177269
Conc: 4.38 ng/ml

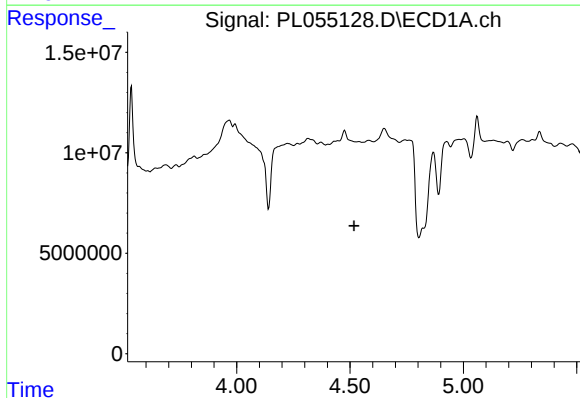


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.518 min
Response: 0
Conc: N.D.

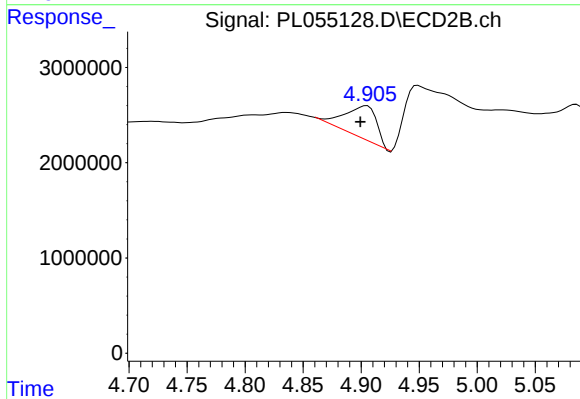

#6 beta-BHC


R.T.: 4.905 min
Delta R.T.: 0.006 min
Response: 6541656
Conc: 4.65 ng/ml

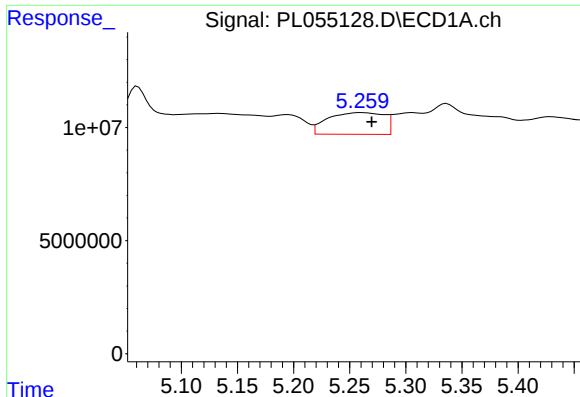

#8 Heptachlor epoxide


R.T.: 5.261 min
Delta R.T.: -0.009 min
Response: 33482987
Conc: 2.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

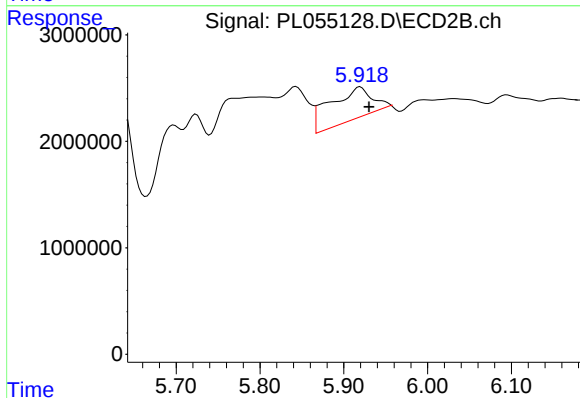


#8 Heptachlor epoxide

R.T.: 5.920 min
Delta R.T.: -0.010 min
Response: 10363969
Conc: 4.15 ng/ml

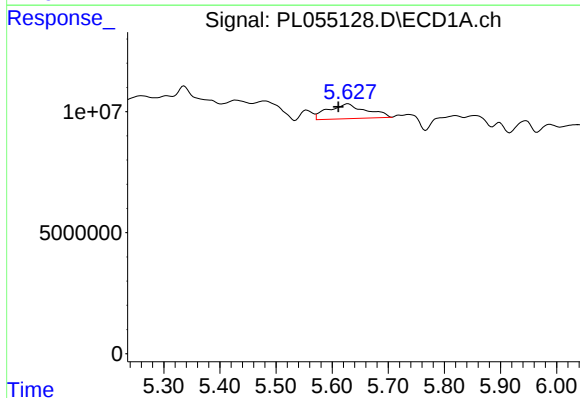


#9 Endosulfan I

R.T.: 5.628 min
Delta R.T.: 0.017 min
Response: 28794181
Conc: 2.11 ng/ml

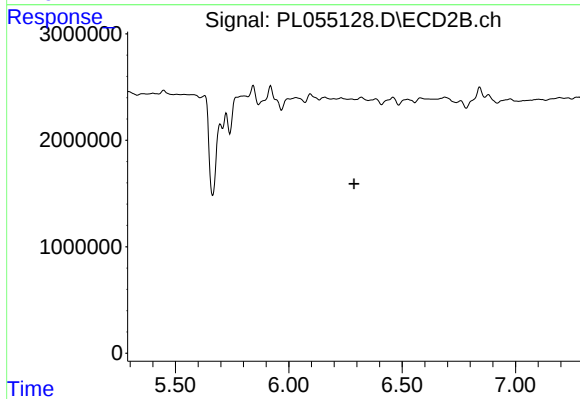

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.288 min
Response: 0
Conc: N.D.

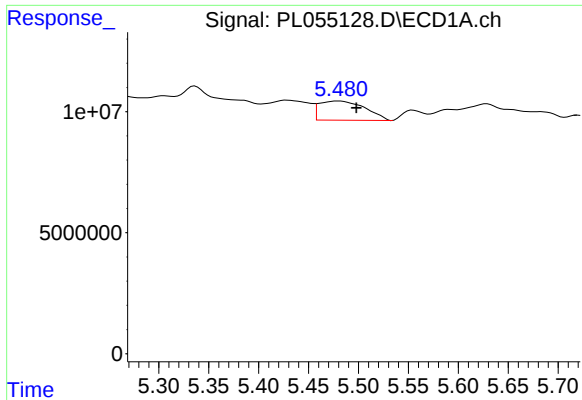

#10 gamma-Chlordane


R.T.: 5.480 min
Delta R.T.: -0.018 min
Response: 25351584
Conc: 1.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

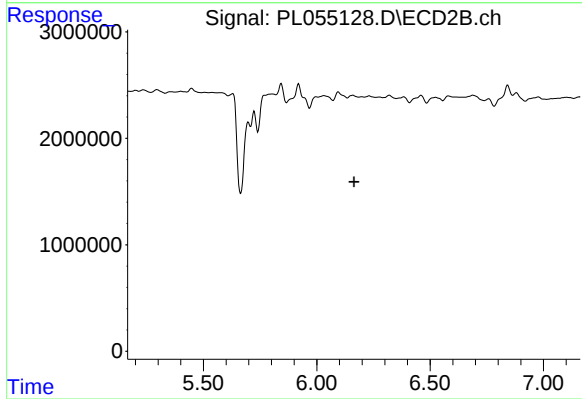


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

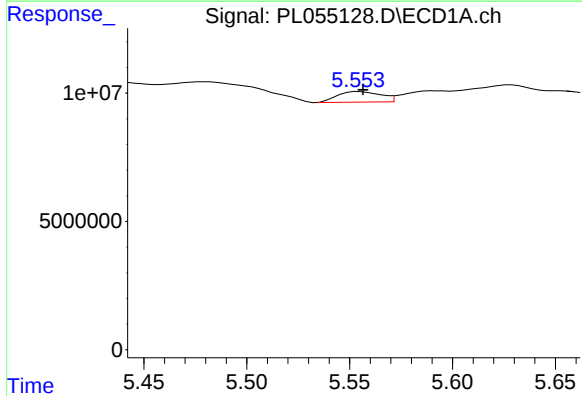


#11 alpha-Chlordane

R.T.: 5.555 min
Delta R.T.: -0.002 min
Response: 5974245
Conc: 0.41 ng/ml

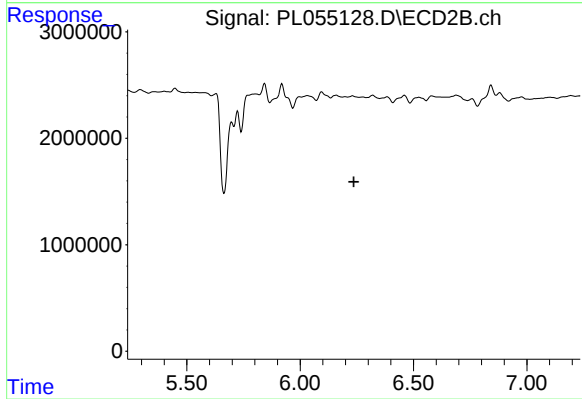

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

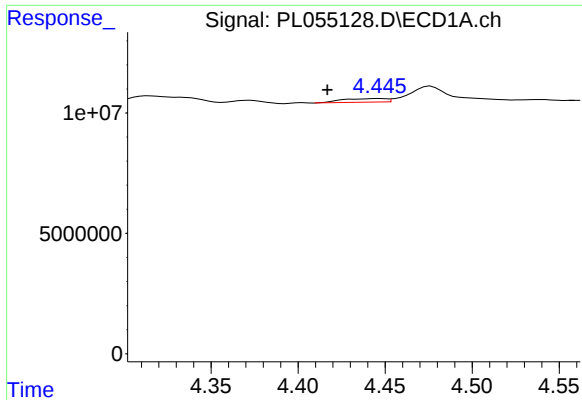

#23 Chlordane-1


R.T.: 4.447 min
Delta R.T.: 0.030 min
Response: 2661628
Conc: 6.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

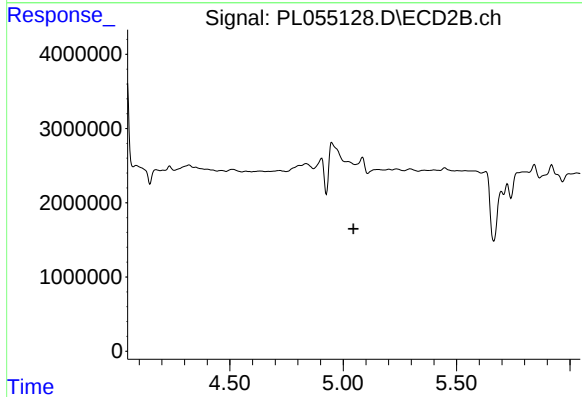


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.046 min
Response: 0
Conc: N.D.

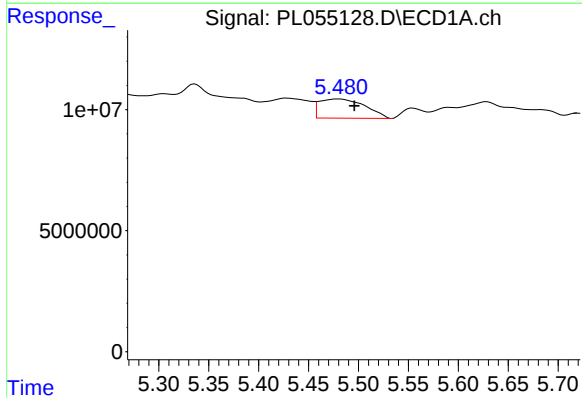


#25 Chlordane-3

R.T.: 5.480 min
Delta R.T.: -0.016 min
Response: 25351584
Conc: 18.81 ng/ml

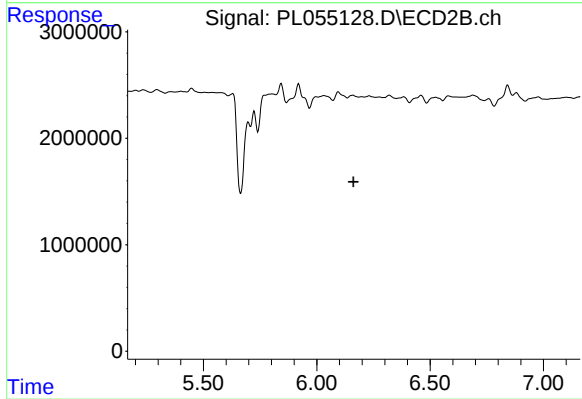

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.163 min
Response: 0
Conc: N.D.

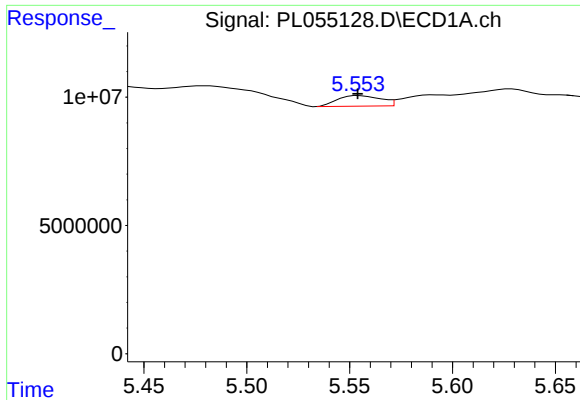

#26 Chlordane-4


R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 5974245
Conc: 5.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

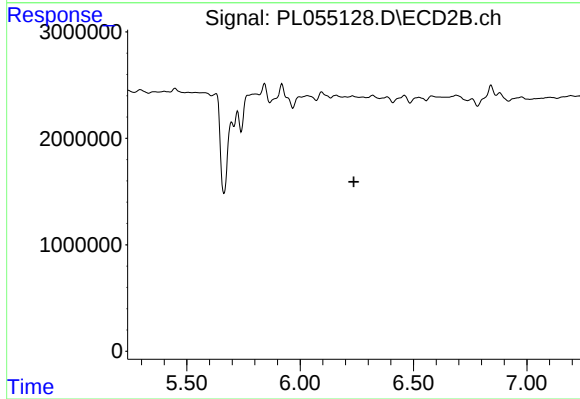


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

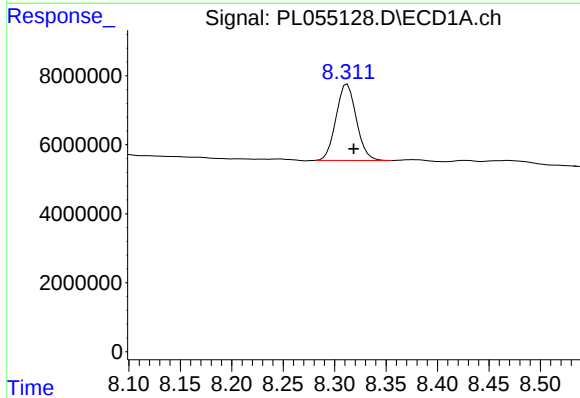

#28 Decachlorobiphenyl

R.T.: 8.312 min
Delta R.T.: -0.006 min
Response: 30435980
Conc: 3.18 ng/ml

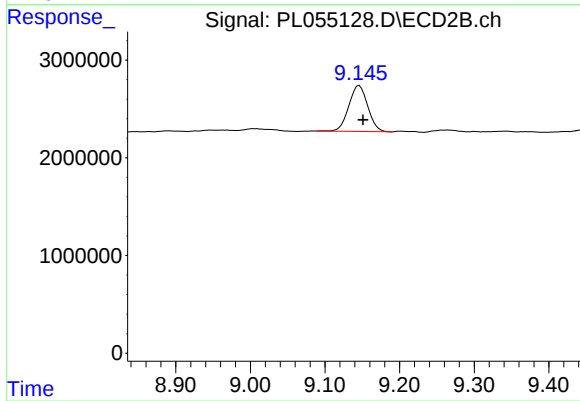

#28 Decachlorobiphenyl

R.T.: 9.146 min
Delta R.T.: -0.005 min
Response: 8264869
Conc: 3.45 ng/ml