

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122019\
 Data File : PL055131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2019 02:30
 Operator : SG\AJ
 Sample : K6370-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 12:10:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 18 14:58:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.049	104.7E6	29222897	9.004	11.452 #
28)	SA Decachlor...	8.313	9.146	1008.2E6	261.8E6	105.281	109.210
Target Compounds							
7)	B delta-BHC	0.000	5.087f	0	2391037	N.D.	0.897 #
8)	B Heptachlo...	0.000	5.920	0	3515074	N.D.	1.407 #
16)	A 4,4'-DDD	0.000	6.882	0	62352513	N.D.	32.474 #
17)	MA 4,4'-DDT	6.466	7.207f	129.4E6	19277564	12.348	9.730
18)	B Endrin al...	6.573f	7.108	378.8E6	8357018	38.252	4.263 #
19)	B Endosulfa...	6.760	0.000	60540886	0	5.653	N.D. #
21)	B Endrin ke...	7.282f	0.000	296.3E6	0	27.257	N.D. #
22)	Mirex	0.000	8.274f	0	211.0E6	N.D.	122.064 #
27)	Chlordane-5	0.000	7.050	0	1539647	N.D.	20.373 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122019\
Data File : PL055131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2019 02:30
Operator : SG\AJ
Sample : K6370-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 12:10:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Dec 18 14:58:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

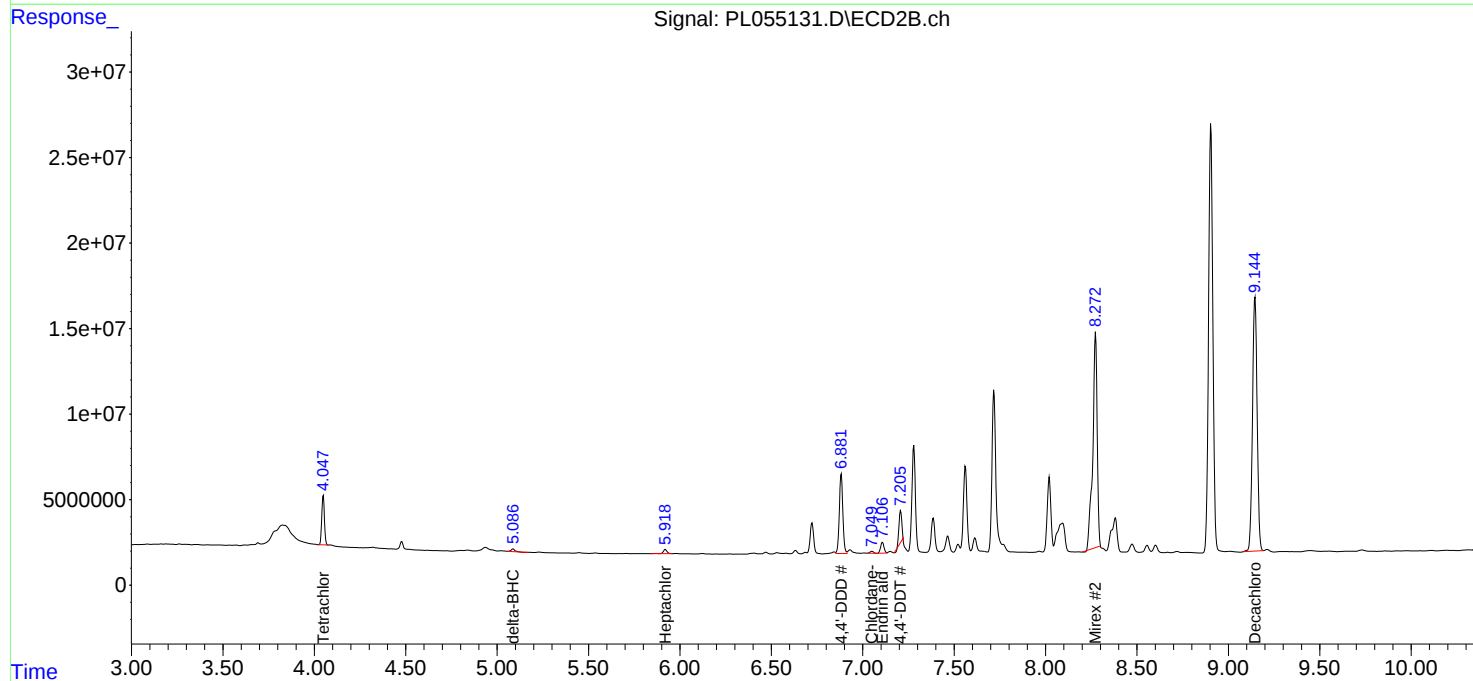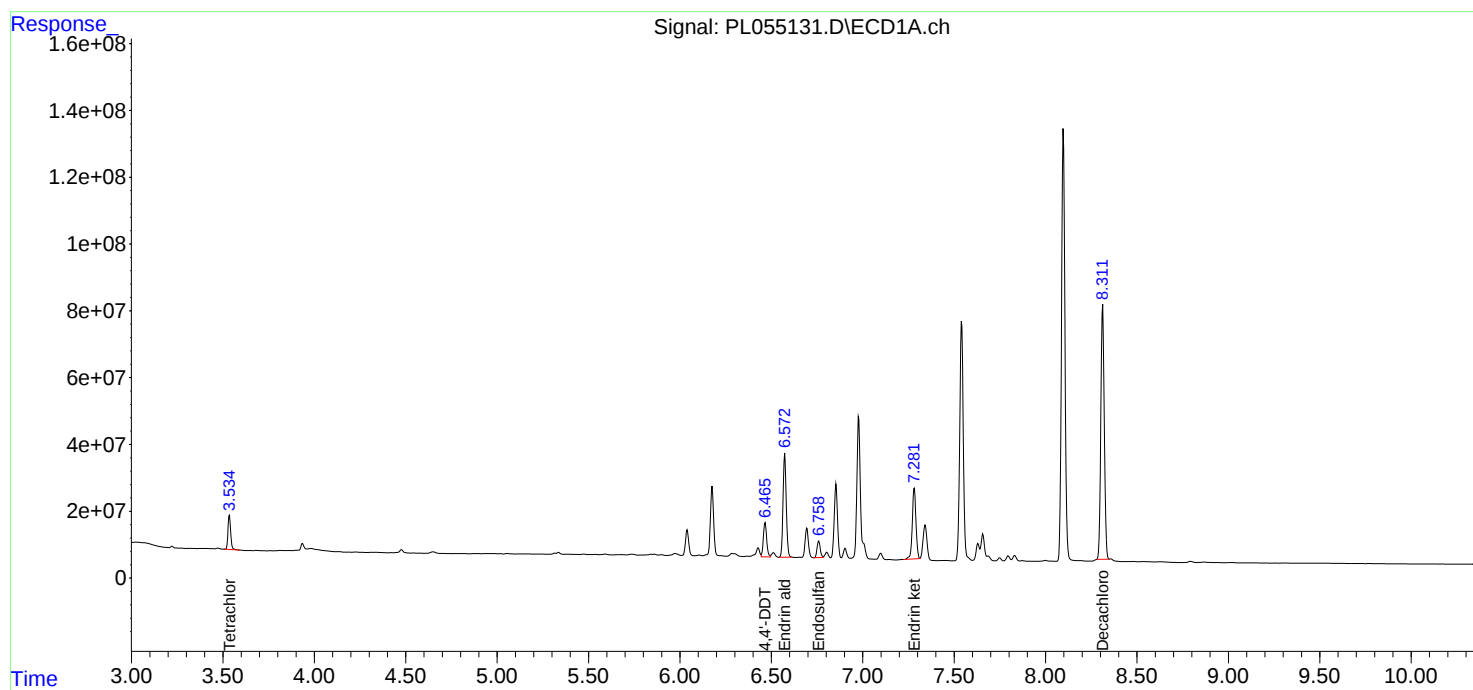


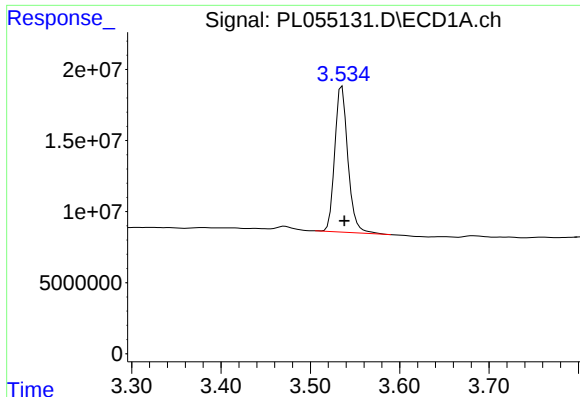

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 104749655
Conc: 9.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

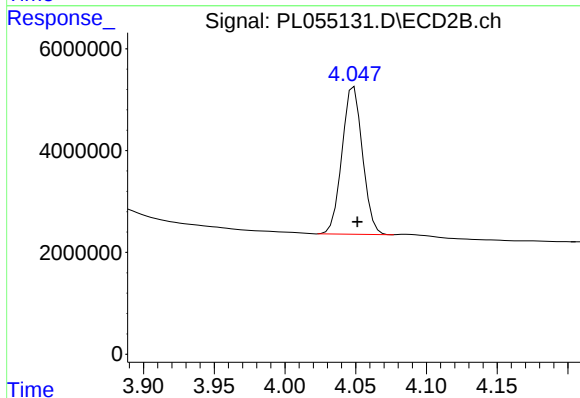


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.003 min
Response: 29222897
Conc: 11.45 ng/ml

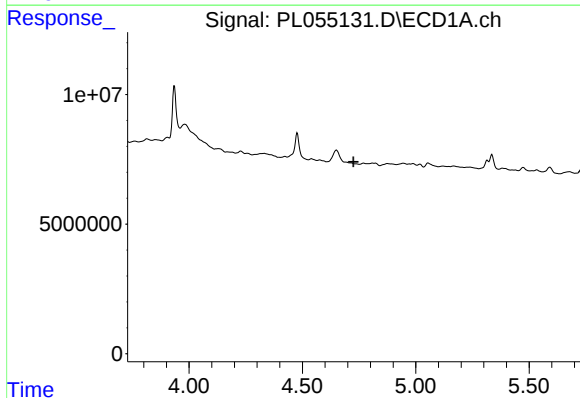


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

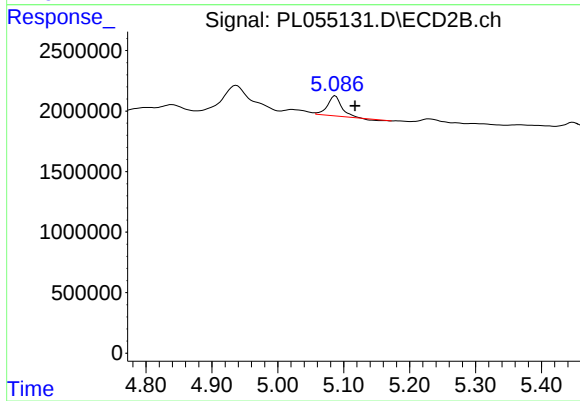

#7 delta-BHC


R.T.: 5.087 min
Delta R.T.: -0.030 min
Response: 2391037
Conc: 0.90 ng/ml

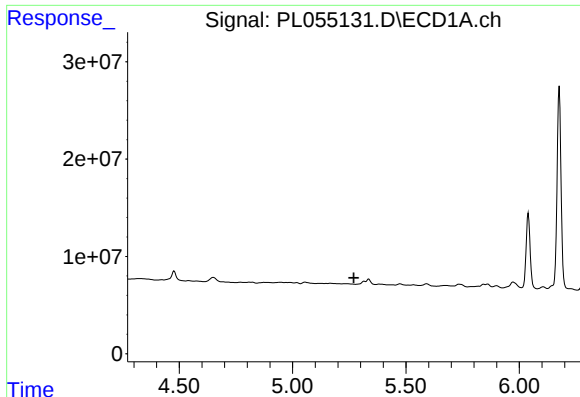

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.270 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

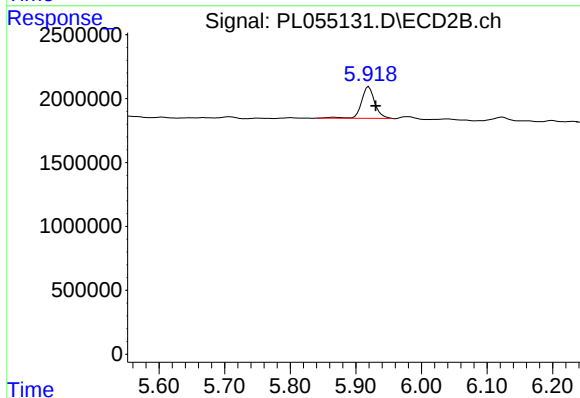


#8 Heptachlor epoxide

R.T.: 5.920 min
Delta R.T.: -0.010 min
Response: 3515074
Conc: 1.41 ng/ml

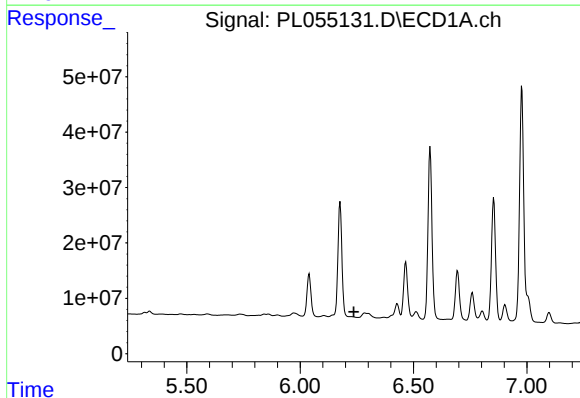


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

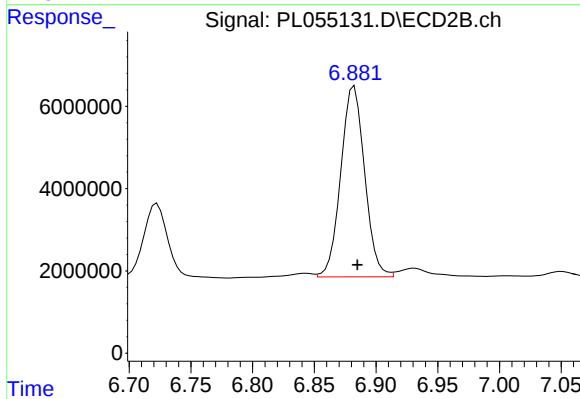

#16 4,4'-DDD


R.T.: 6.882 min
Delta R.T.: -0.003 min
Response: 62352513
Conc: 32.47 ng/ml

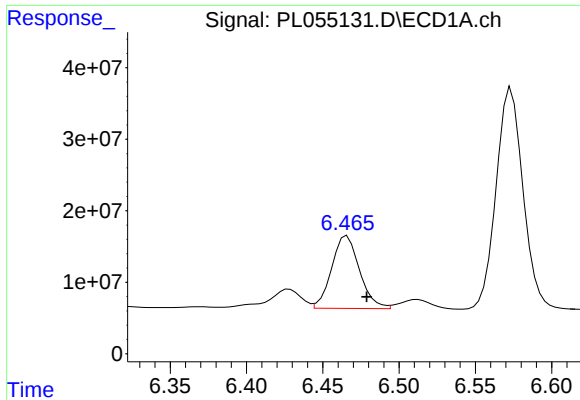

#17 4,4'-DDT


R.T.: 6.466 min
Delta R.T.: -0.013 min
Response: 129363578
Conc: 12.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

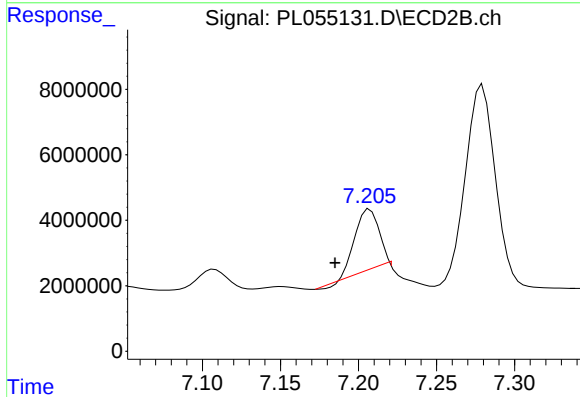


#17 4,4'-DDT

R.T.: 7.207 min
Delta R.T.: 0.022 min
Response: 19277564
Conc: 9.73 ng/ml

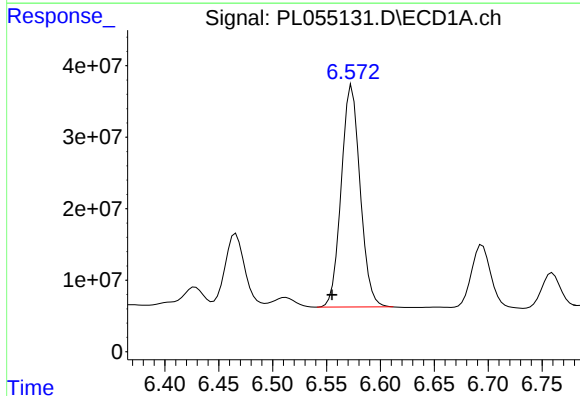


#18 Endrin aldehyde

R.T.: 6.573 min
Delta R.T.: 0.018 min
Response: 378802567
Conc: 38.25 ng/ml

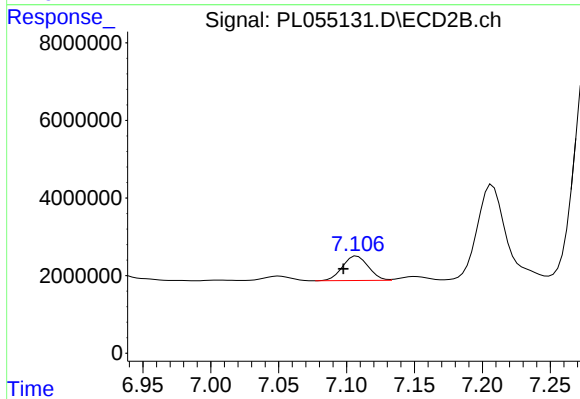

#18 Endrin aldehyde


R.T.: 7.108 min
Delta R.T.: 0.010 min
Response: 8357018
Conc: 4.26 ng/ml

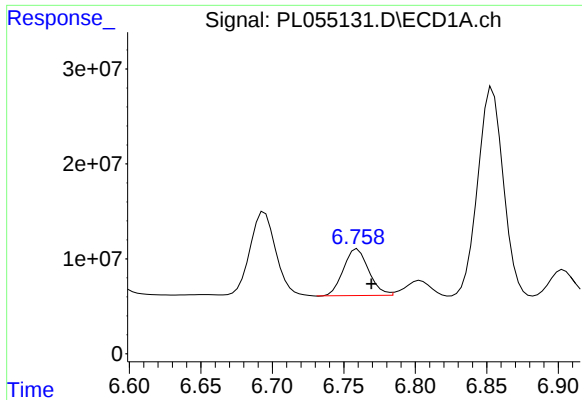

#19 Endosulfan Sulfate


R.T.: 6.760 min
Delta R.T.: -0.010 min
Response: 60540886
Conc: 5.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

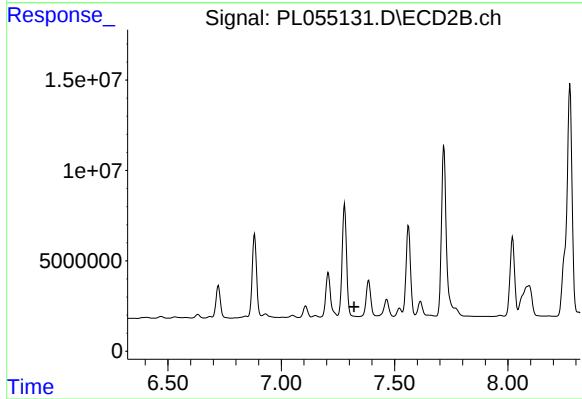


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.322 min
Response: 0
Conc: N.D.

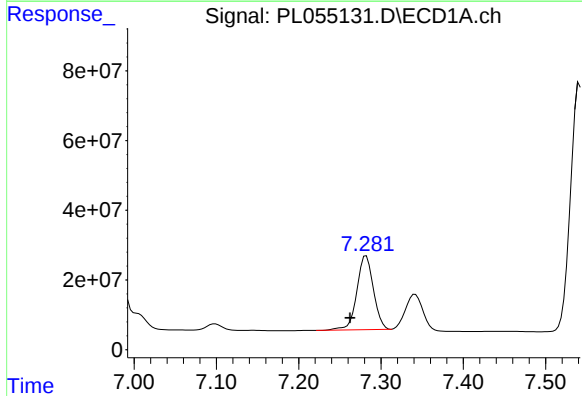


#21 Endrin ketone

R.T.: 7.282 min
Delta R.T.: 0.019 min
Response: 296259427
Conc: 27.26 ng/ml

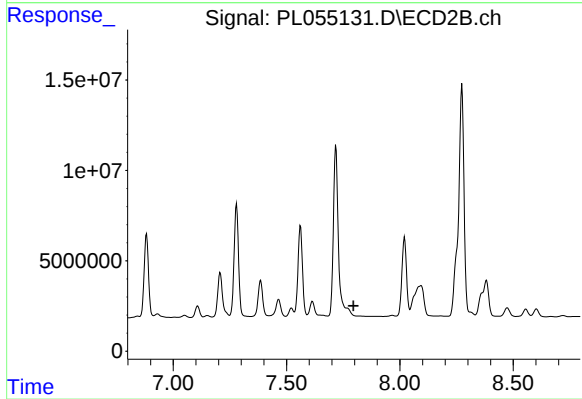

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.796 min
Response: 0
Conc: N.D.

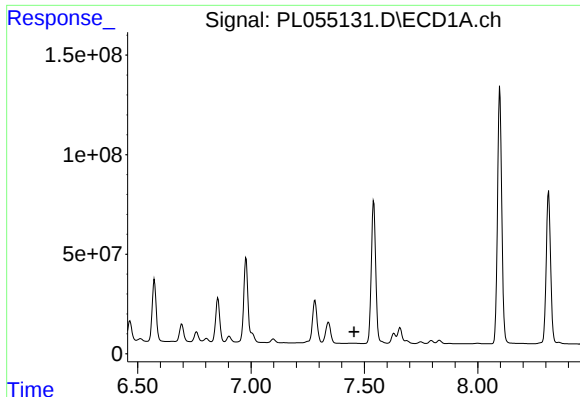

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

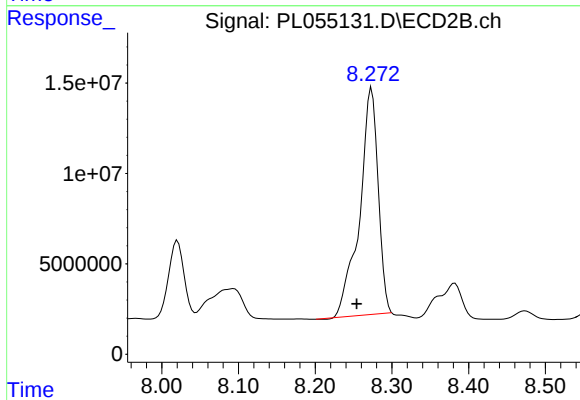


#22 Mirex

R.T.: 8.274 min
Delta R.T.: 0.019 min
Response: 210966452
Conc: 122.06 ng/ml

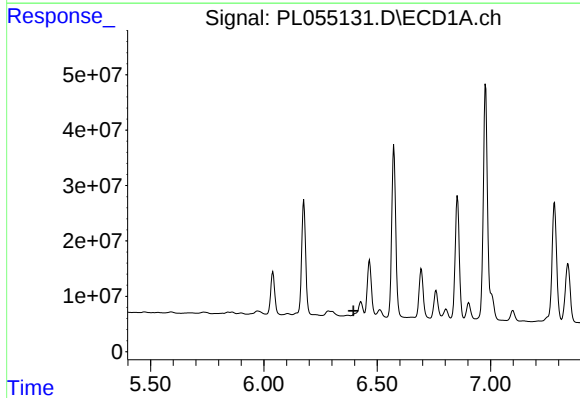


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

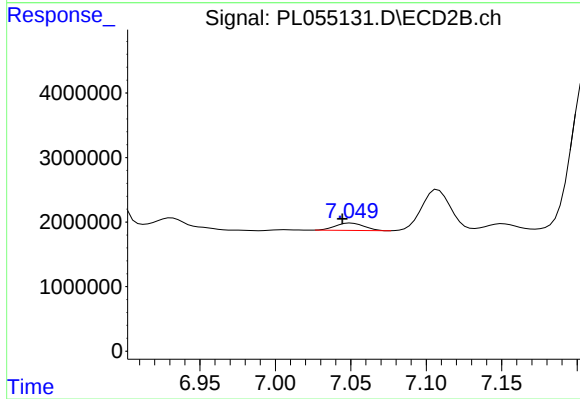

#27 Chlordane-5


R.T.: 7.050 min
Delta R.T.: 0.006 min
Response: 1539647
Conc: 20.37 ng/ml

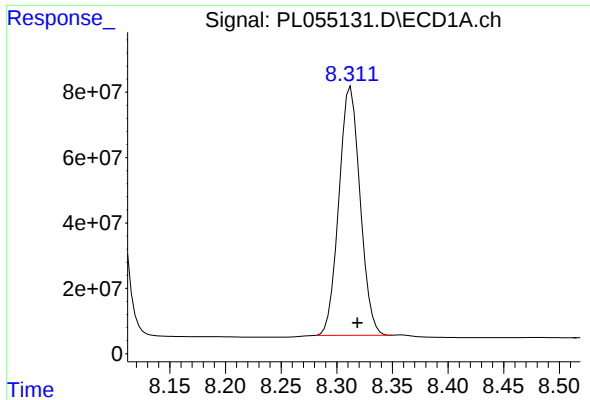

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: -0.006 min
Response: 1008186020
Conc: 105.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

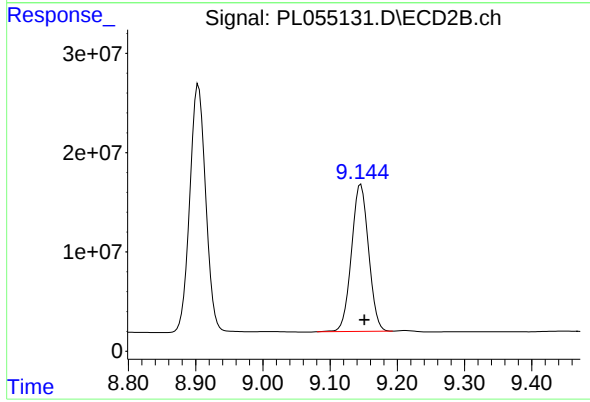

#28 Decachlorobiphenyl

R.T.: 9.146 min
Delta R.T.: -0.005 min
Response: 261823679
Conc: 109.21 ng/ml