

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122021\
 Data File : PL071531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2021 11:03
 Operator : AR\AJ
 Sample : PB141548BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 13:35:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.563	5.500	9338070	23000819	19.701	19.307
28)	SA Decachlor...	10.323	11.389	15039259	22761500	22.636	20.950
Target Compounds							
5)	MB Aldrin	0.000	7.472f	0	140311	N.D.	0.096 #
7)	B delta-BHC	0.000	7.021f	0	2197710	N.D.	1.438 #
8)	B Heptachlo...	0.000	7.930f	0	240834	N.D.	0.180 #
9)	A Endosulfan I	0.000	8.367	0	53271	N.D.	0.044 #
10)	B gamma-Chl...	0.000	8.233	0	198153	N.D.	0.153 #
14)	MA Endrin	0.000	8.878	0	157195	N.D.	0.155 #
23)	Chlordane-1	0.000	6.900f	0	492193	N.D.	10.708 #
24)	Chlordane-2	0.000	7.472	0	140311	N.D.	2.975 #
25)	Chlordane-3	0.000	8.233	0	198153	N.D.	1.132 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122021\
Data File : PL071531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2021 11:03
Operator : AR\AJ
Sample : PB141548BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 13:35:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

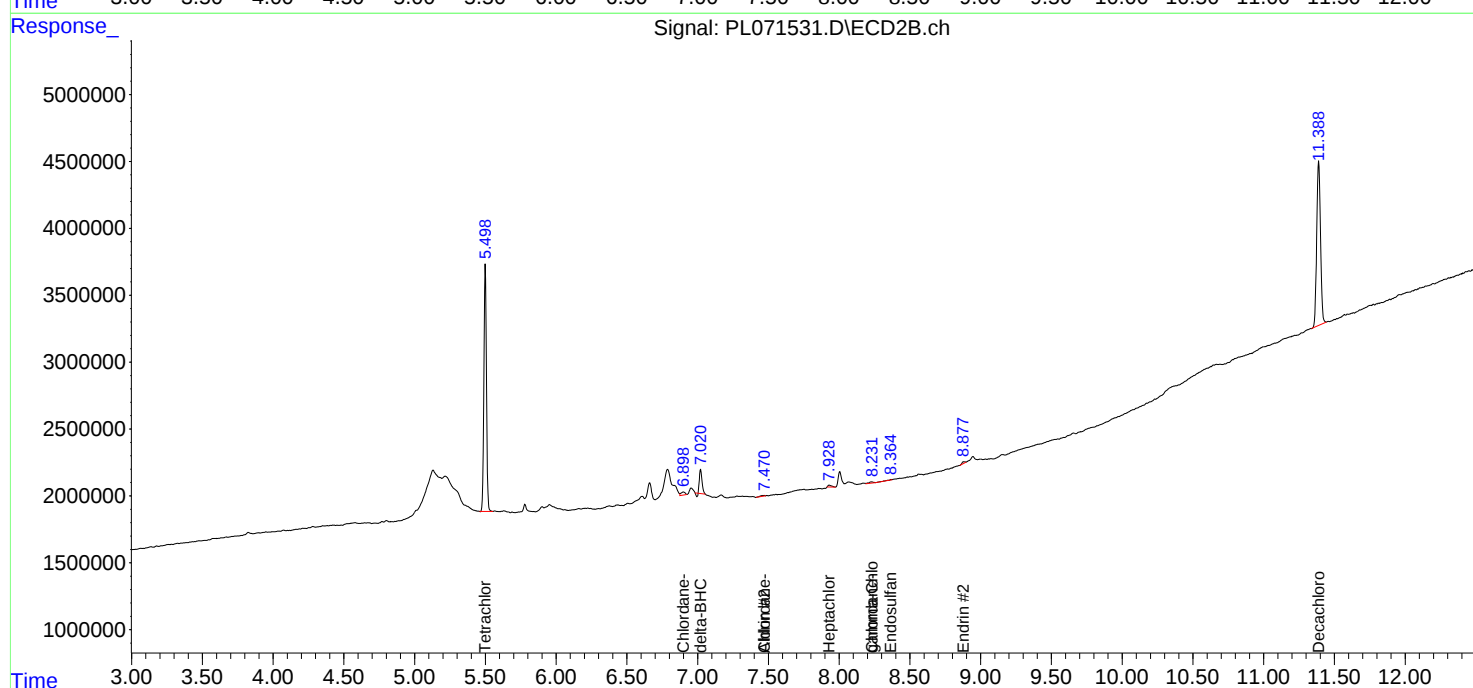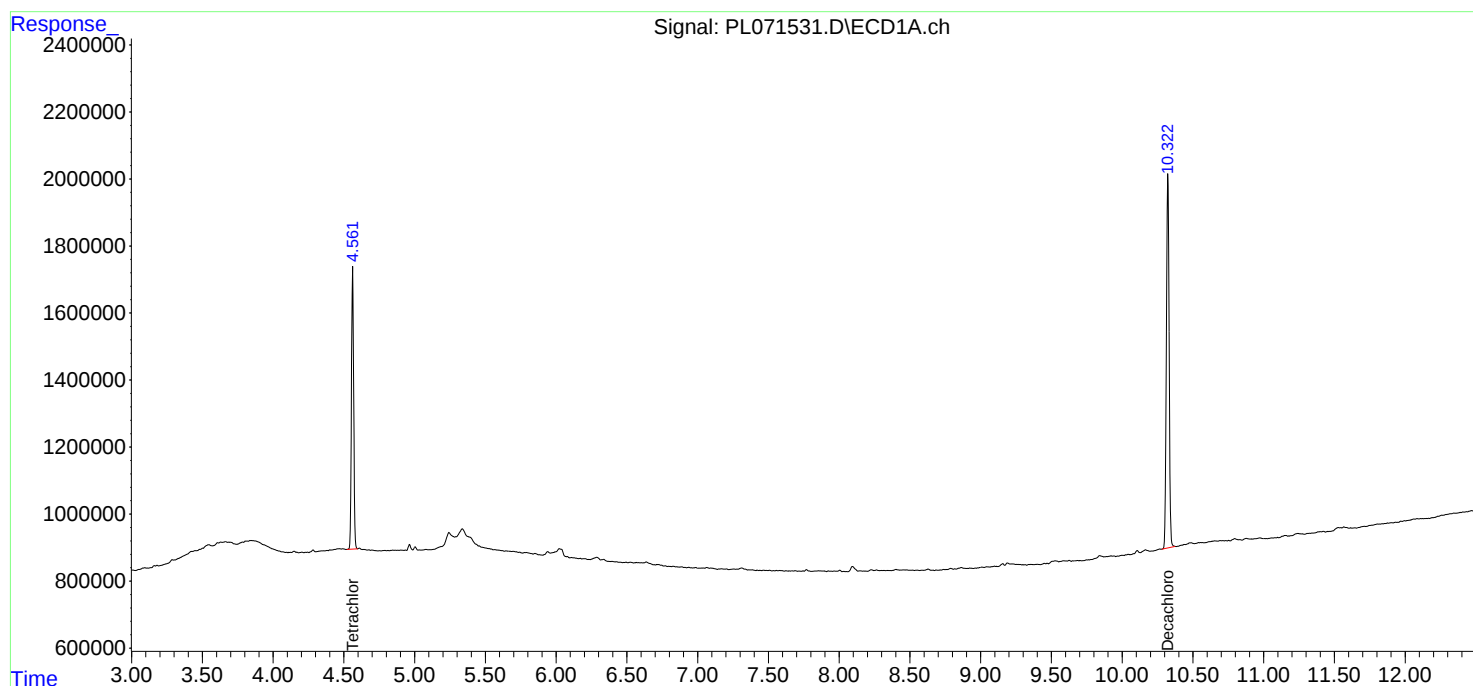


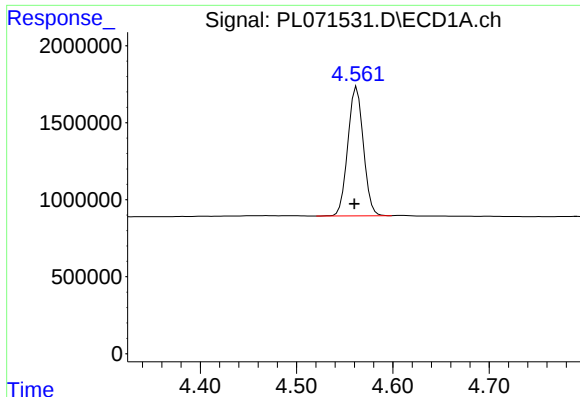

#1 Tetrachloro-m-xylene


R.T.: 4.563 min
Delta R.T.: 0.003 min
Response: 9338070
Conc: 19.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

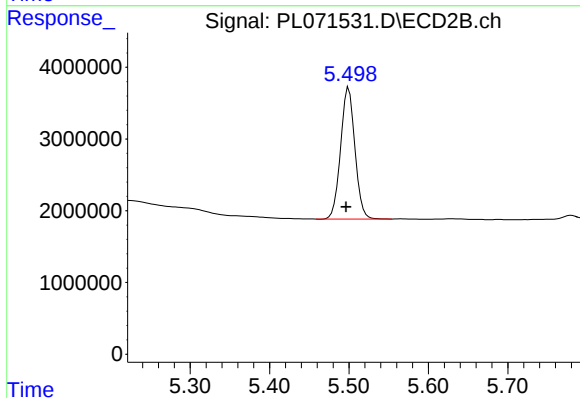


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: 0.003 min
Response: 23000819
Conc: 19.31 ng/ml

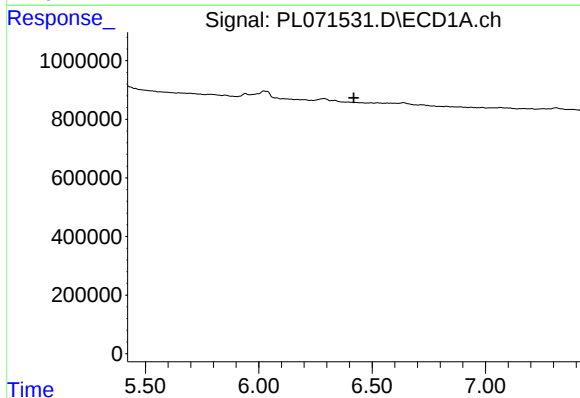


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.419 min
Response: 0
Conc: N.D.

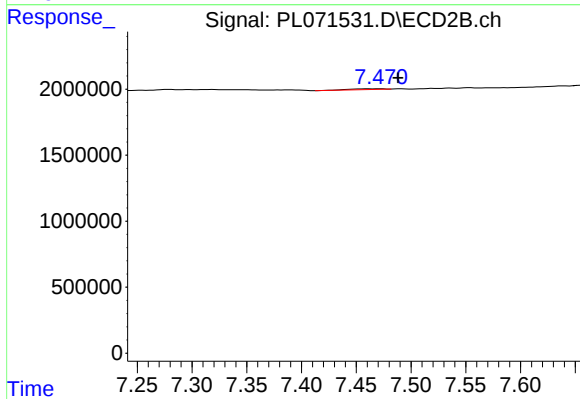

#5 Aldrin


R.T.: 7.472 min
Delta R.T.: -0.017 min
Response: 140311
Conc: 0.10 ng/ml

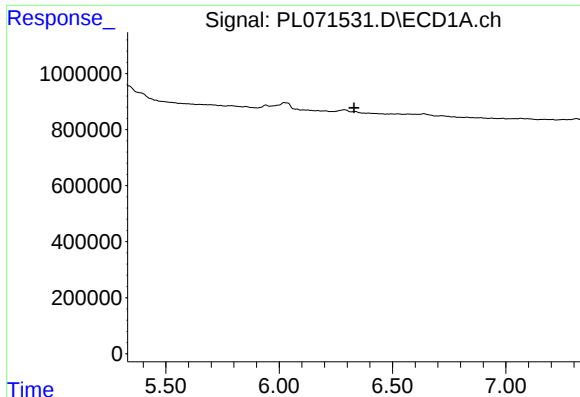

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

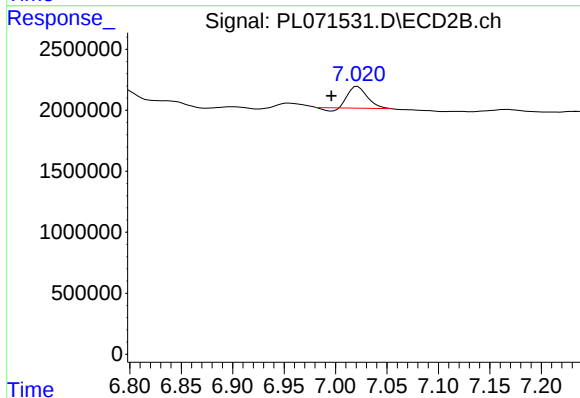


#7 delta-BHC

R.T.: 7.021 min
Delta R.T.: 0.025 min
Response: 2197710
Conc: 1.44 ng/ml

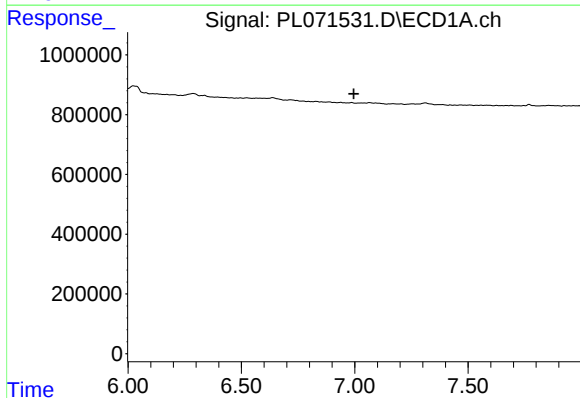


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.996 min
Response: 0
Conc: N.D.

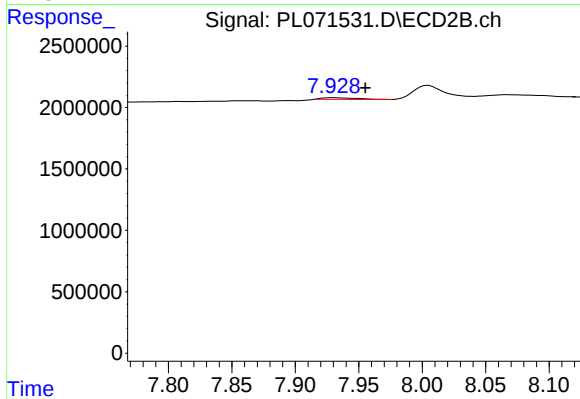

#8 Heptachlor epoxide


R.T.: 7.930 min
Delta R.T.: -0.025 min
Response: 240834
Conc: 0.18 ng/ml

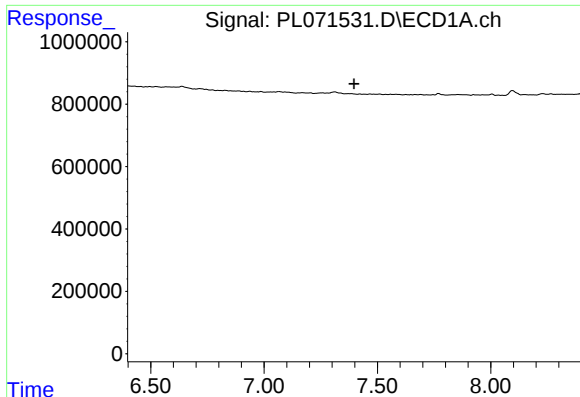

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

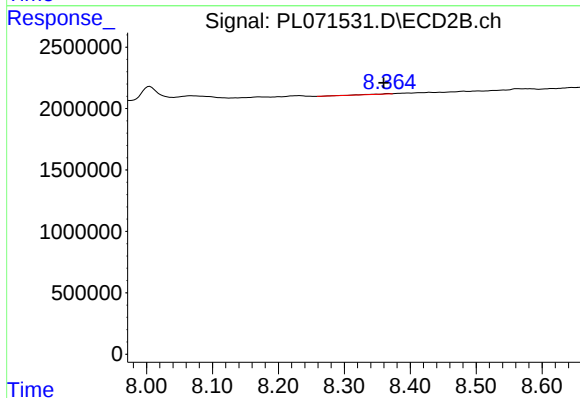


#9 Endosulfan I

R.T.: 8.367 min
Delta R.T.: 0.007 min
Response: 53271
Conc: 0.04 ng/ml

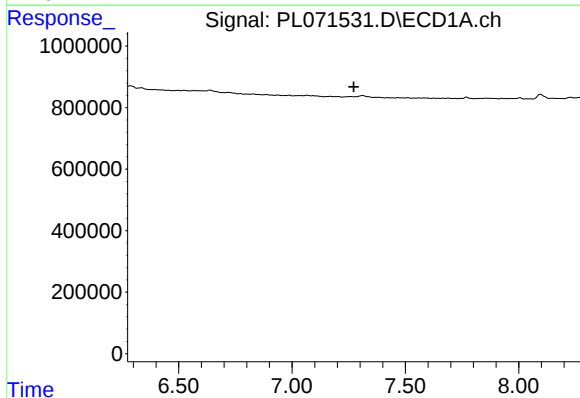


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.273 min
Response: 0
Conc: N.D.

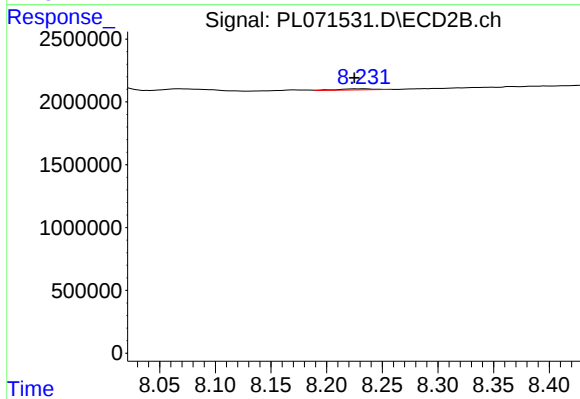

#10 gamma-Chlordane


R.T.: 8.233 min
Delta R.T.: 0.008 min
Response: 198153
Conc: 0.15 ng/ml

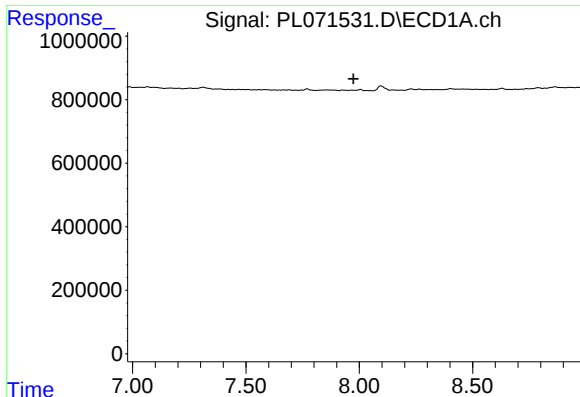

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 7.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

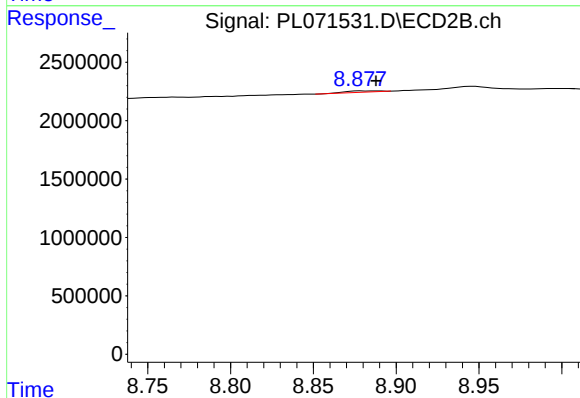


#14 Endrin

R.T.: 8.878 min
Delta R.T.: -0.010 min
Response: 157195
Conc: 0.16 ng/ml

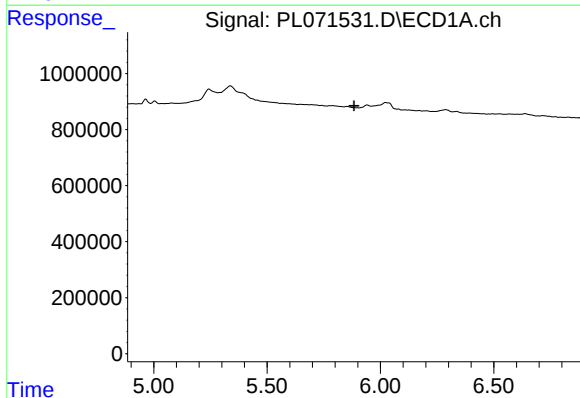


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.884 min
Response: 0
Conc: N.D.

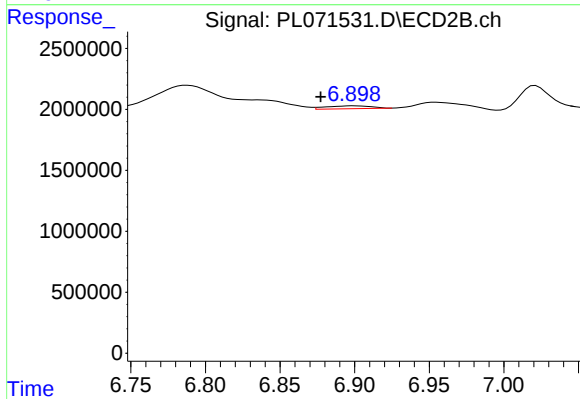

#23 Chlordane-1


R.T.: 6.900 min
Delta R.T.: 0.023 min
Response: 492193
Conc: 10.71 ng/ml

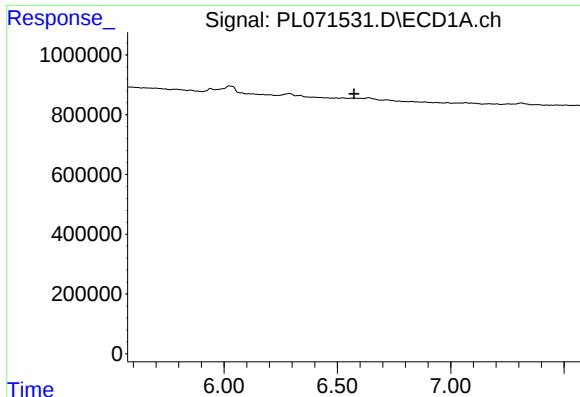

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

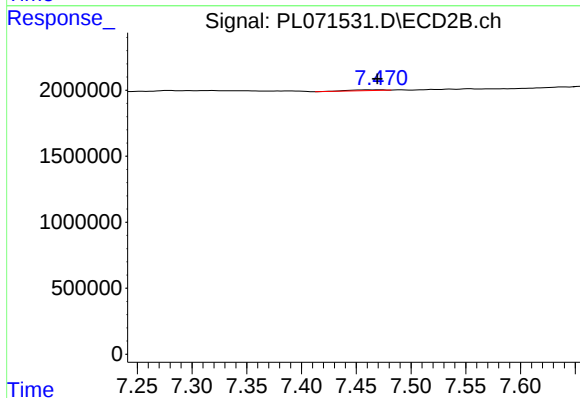


#24 Chlordane-2

R.T.: 7.472 min
Delta R.T.: 0.002 min
Response: 140311
Conc: 2.98 ng/ml

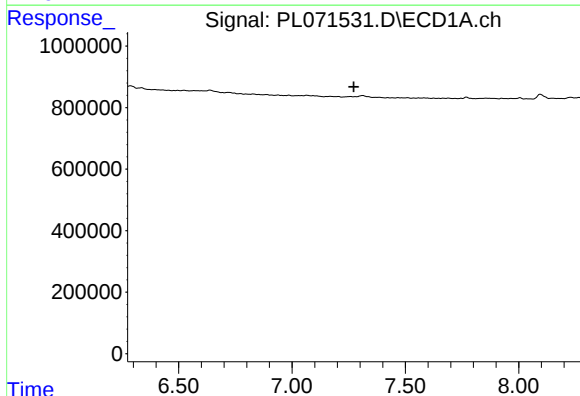


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.272 min
Response: 0
Conc: N.D.

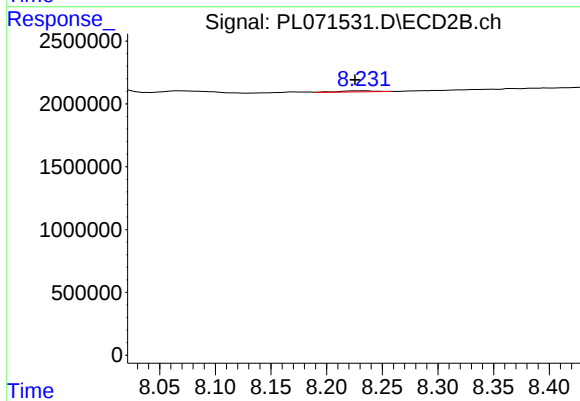

#25 Chlordane-3


R.T.: 8.233 min
Delta R.T.: 0.007 min
Response: 198153
Conc: 1.13 ng/ml

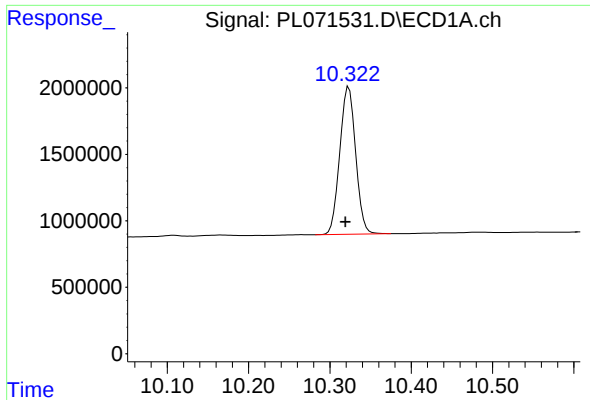

#28 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: 0.004 min
Response: 15039259
Conc: 22.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

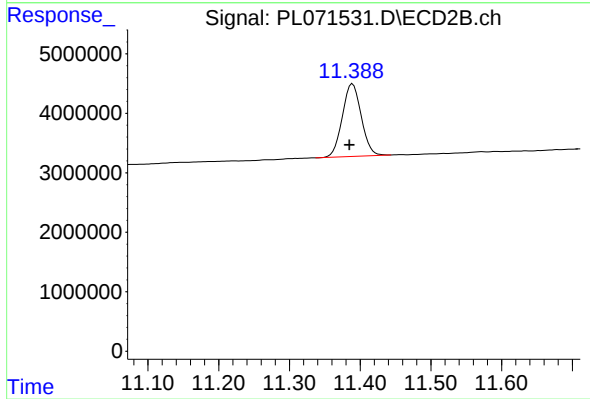

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: 0.004 min
Response: 22761500
Conc: 20.95 ng/ml