

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
 Data File : PL079792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 15:01
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 03:50:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 21 03:48:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	2.562	45483131	55499271	20.696	20.907
28)	SA Decachlor...	8.762	7.627	40485567	51735625	21.828	21.552
Target Compounds							
2)	A alpha-BHC	3.776	3.048	31701888	46503883	9.404	10.760
3)	MA gamma-BHC...	4.109	3.369	31275723	40428740	9.789	10.323
4)	MA Heptachlor	0.000	3.670f	0	19322692	N.D.	4.760 #
5)	MB Aldrin	0.000	3.950f	0	20515	N.D.	0.005 #
6)	B beta-BHC	4.324	3.670	14892948	19322692	10.871	12.742
8)	B Heptachlo...	0.000	4.455	0	738564	N.D.	0.212 #
9)	A Endosulfan I	5.854f	4.853f	181943	483660	0.070	0.144 #
11)	B alpha-Chl...	5.756f	4.746f	372273	802643	0.134	0.234 #
12)	B 4,4'-DDE	0.000	4.971	0	172813	N.D.	0.054 #
13)	MA Dieldrin	0.000	5.080	0	316256	N.D.	0.091 #
14)	MA Endrin	6.342	5.358	118.3E6	139.9E6	49.753	49.219
15)	B Endosulfa...	6.600f	0.000	1424435	0	0.585	N.D. #
16)	A 4,4'-DDD	6.492	5.519	1555413	1734054	0.793	0.681
17)	MA 4,4'-DDT	6.800	5.765	237.2E6	286.4E6	105.932	105.699
18)	B Endrin al...	6.704	5.835	2217449	6293460	1.246	2.805 #
19)	B Endosulfa...	0.000	6.051	0	135848	N.D.	0.047 #
20)	A Methoxychlor	7.285	6.342	311.9E6	346.6E6	264.643	244.451
21)	B Endrin ke...	7.422	6.551	4682789	8318032	1.918	2.605 #
23)	Chlordane-1	0.000	3.507f	0	1021665	N.D.	9.781 #
26)	Chlordane-4	5.756f	4.746f	372273	802643	0.776	2.208 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
Data File : PL079792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 15:01
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 03:50:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
Quant Title : GC Extractables
QLast Update : Wed Dec 21 03:48:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

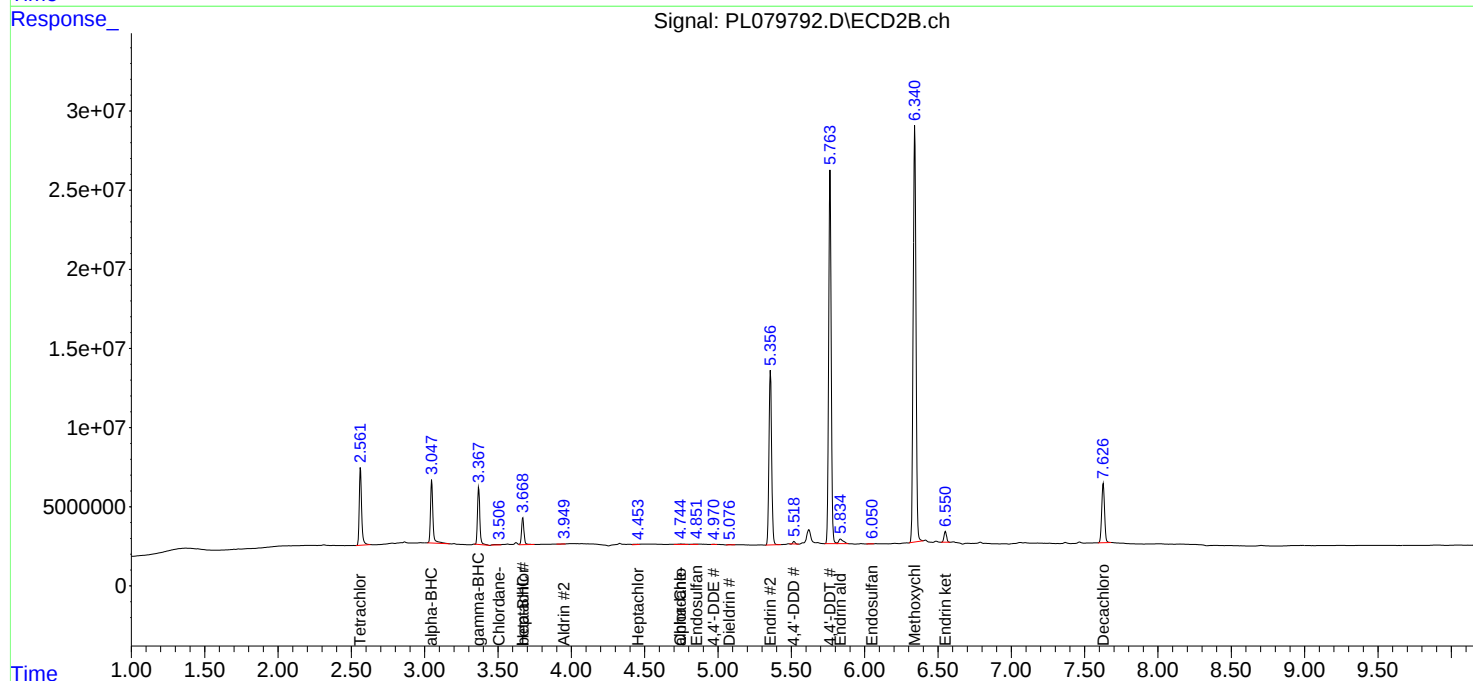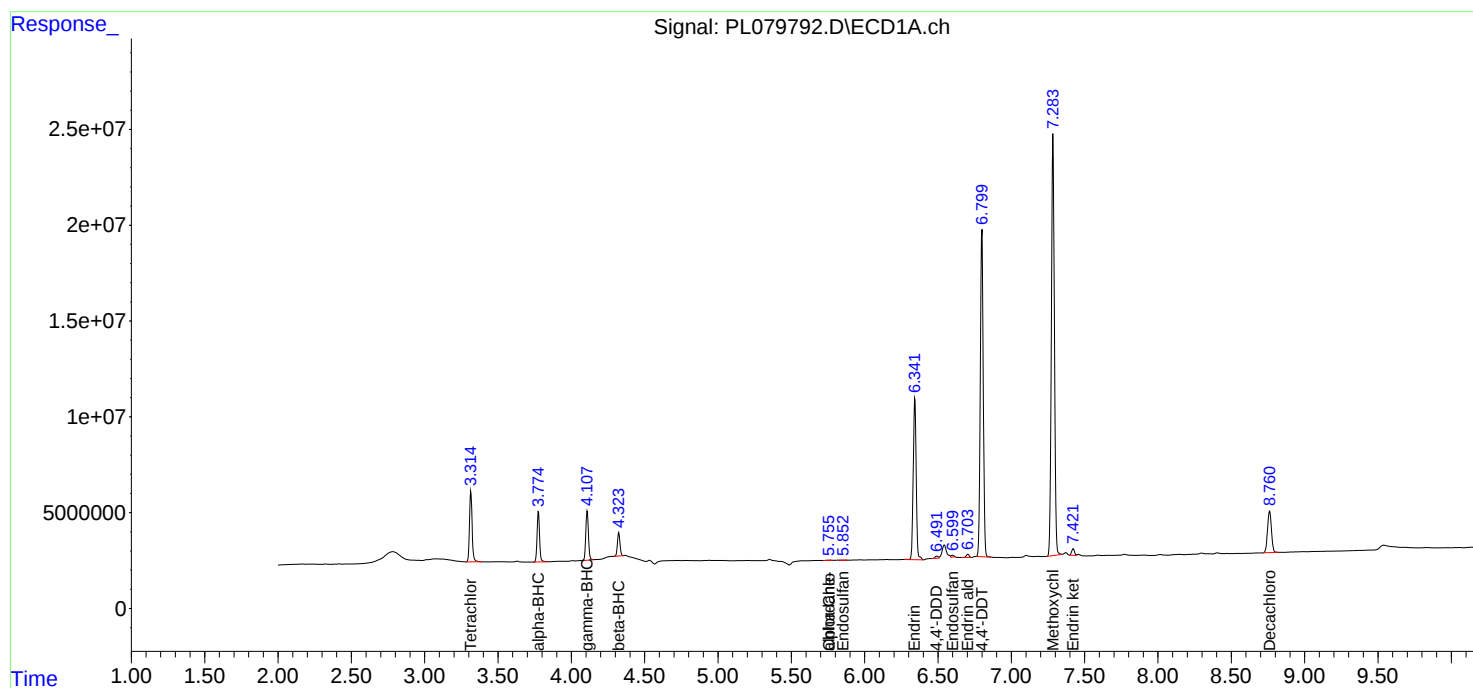


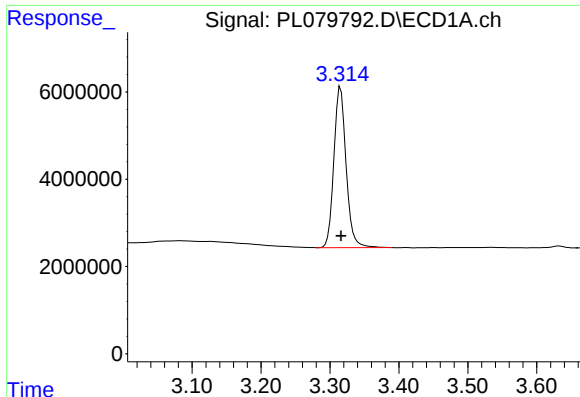

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 45483131
Conc: 20.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

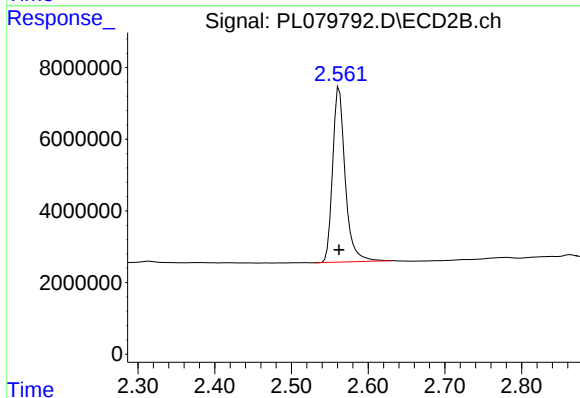


#1 Tetrachloro-m-xylene

R.T.: 2.562 min
Delta R.T.: 0.000 min
Response: 55499271
Conc: 20.91 ng/ml

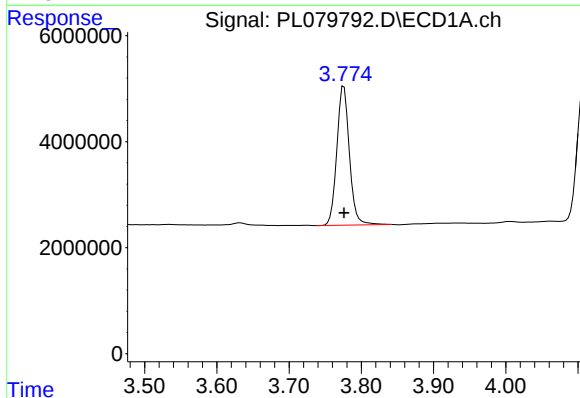


#2 alpha-BHC

R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 31701888
Conc: 9.40 ng/ml

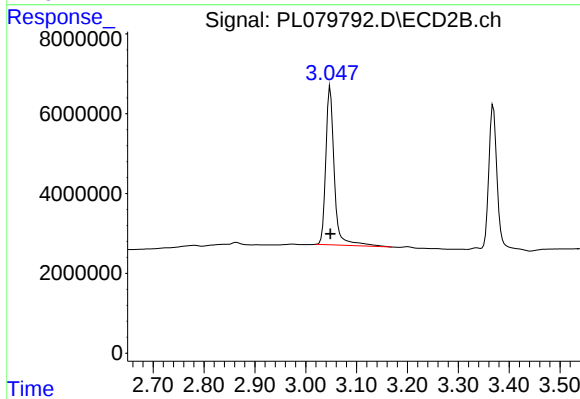

#2 alpha-BHC


R.T.: 3.048 min
Delta R.T.: 0.000 min
Response: 46503883
Conc: 10.76 ng/ml

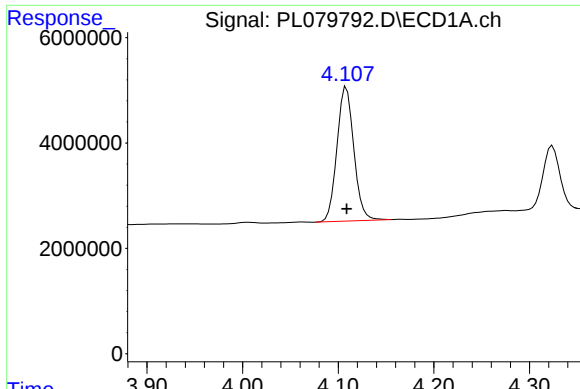

#3 gamma-BHC (Lindane)


R.T.: 4.109 min
Delta R.T.: 0.000 min
Response: 31275723
Conc: 9.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

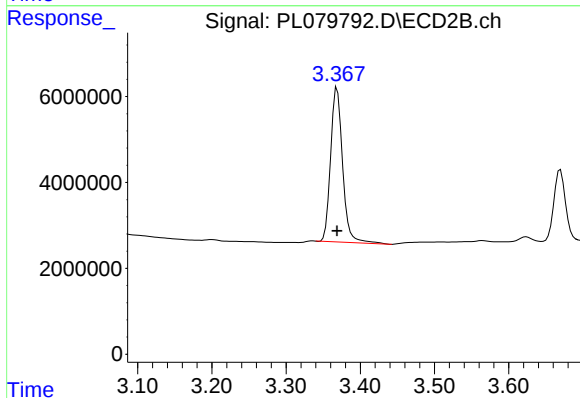


#3 gamma-BHC (Lindane)

R.T.: 3.369 min
Delta R.T.: 0.000 min
Response: 40428740
Conc: 10.32 ng/ml

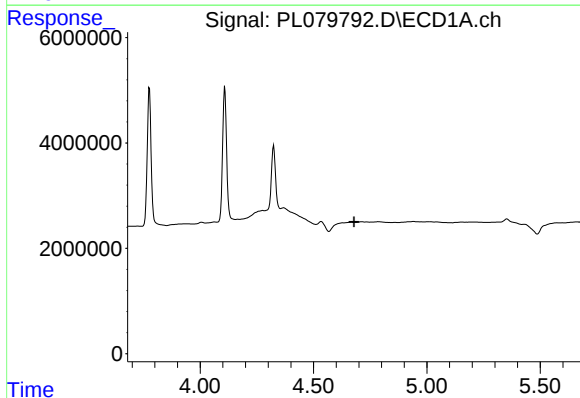


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.679 min
Response: 0
Conc: N.D.

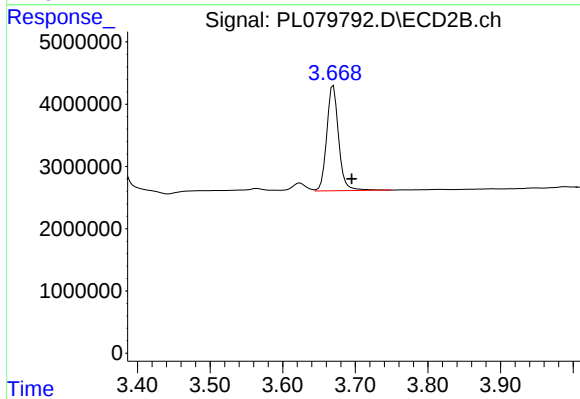

#4 Heptachlor


R.T.: 3.670 min
Delta R.T.: -0.025 min
Response: 19322692
Conc: 4.76 ng/ml

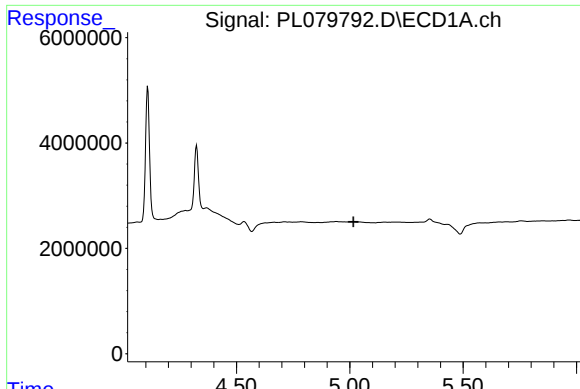

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.017 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

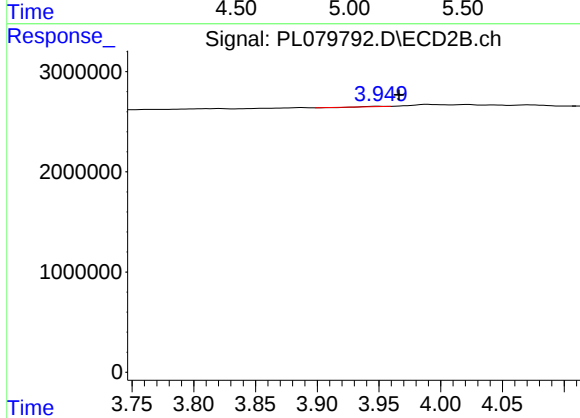


#5 Aldrin

R.T.: 3.950 min
Delta R.T.: -0.016 min
Response: 20515
Conc: 0.01 ng/ml

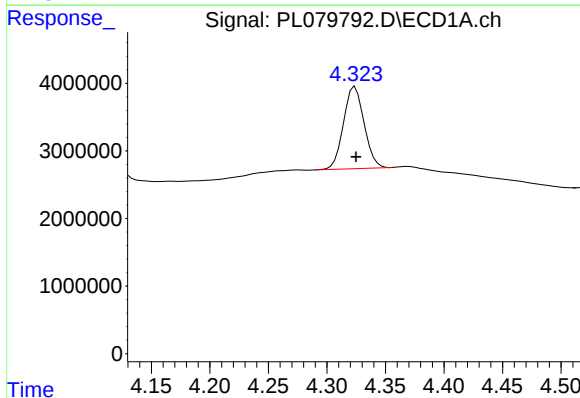


#6 beta-BHC

R.T.: 4.324 min
Delta R.T.: 0.000 min
Response: 14892948
Conc: 10.87 ng/ml

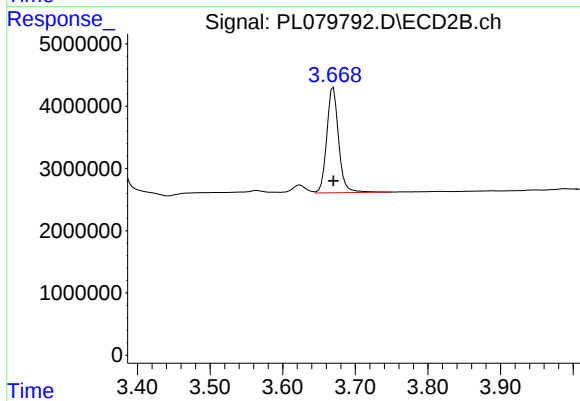

#6 beta-BHC


R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 19322692
Conc: 12.74 ng/ml

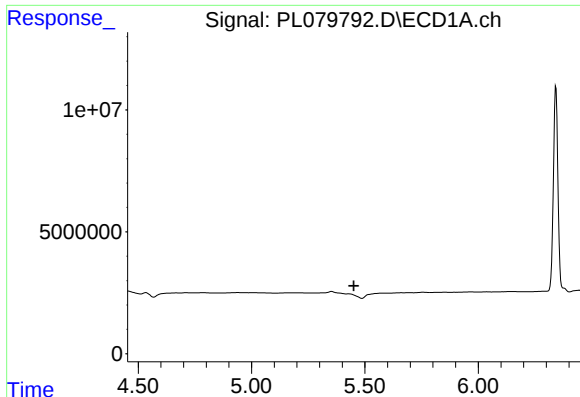

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.450 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

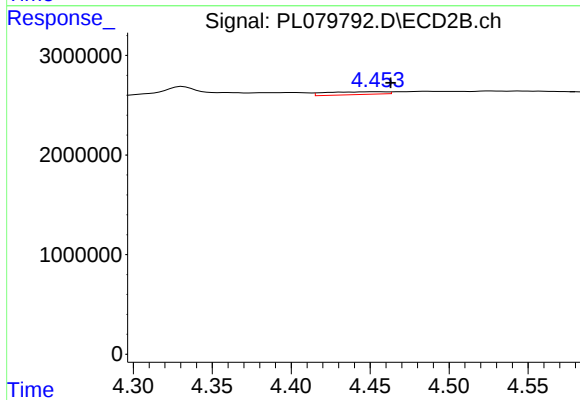


#8 Heptachlor epoxide

R.T.: 4.455 min
Delta R.T.: -0.008 min
Response: 738564
Conc: 0.21 ng/ml

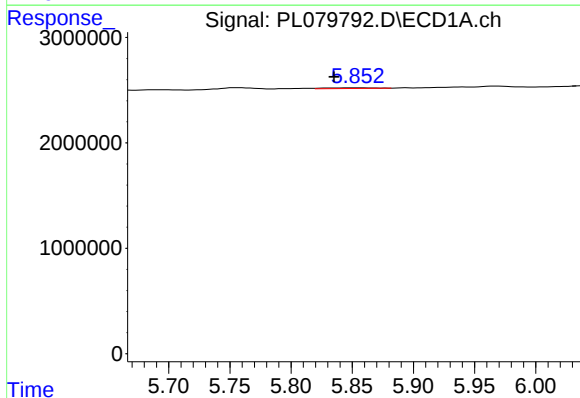


#9 Endosulfan I

R.T.: 5.854 min
Delta R.T.: 0.018 min
Response: 181943
Conc: 0.07 ng/ml

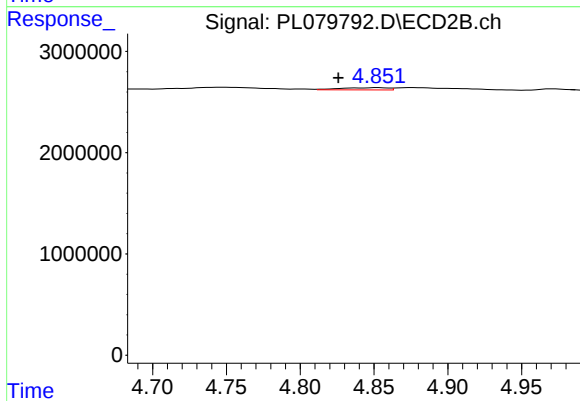

#9 Endosulfan I


R.T.: 4.853 min
Delta R.T.: 0.027 min
Response: 483660
Conc: 0.14 ng/ml

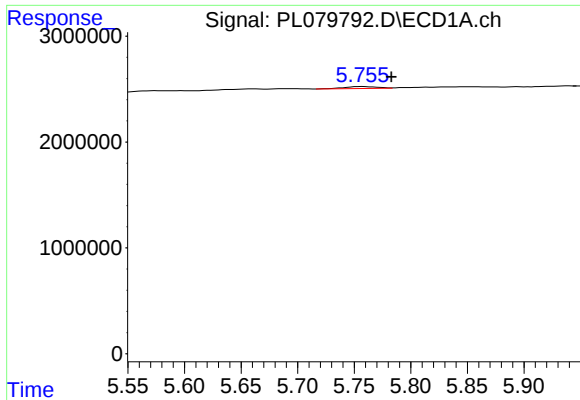

#11 alpha-Chlordane


R.T.: 5.756 min
Delta R.T.: -0.027 min
Response: 372273
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

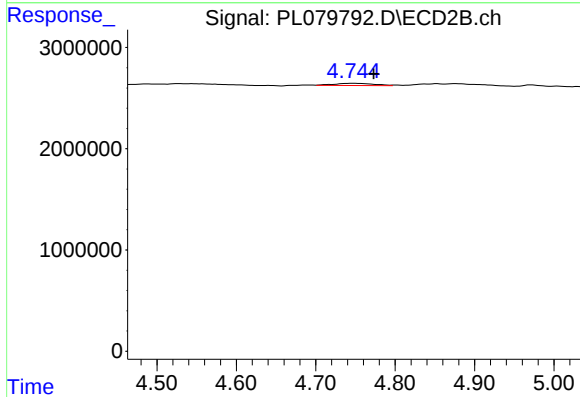


#11 alpha-Chlordane

R.T.: 4.746 min
Delta R.T.: -0.027 min
Response: 802643
Conc: 0.23 ng/ml

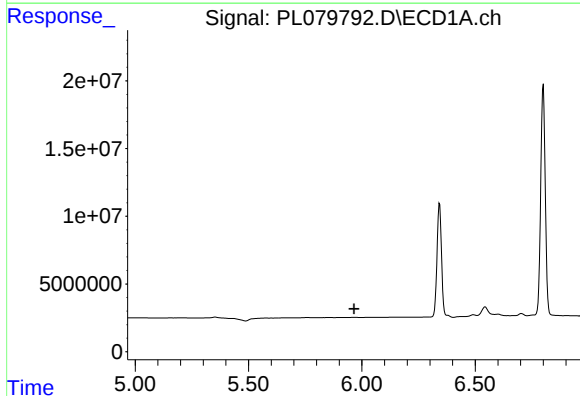


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.966 min
Response: 0
Conc: N.D.

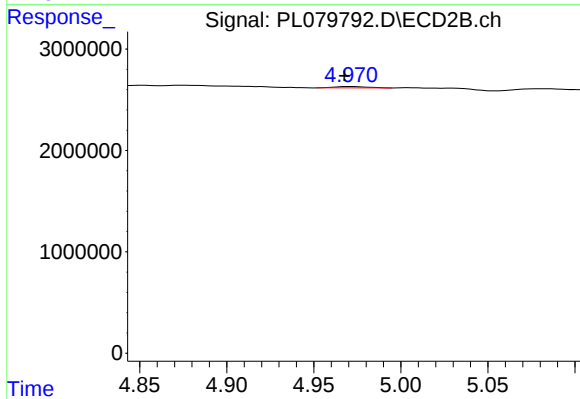

#12 4,4'-DDE


R.T.: 4.971 min
Delta R.T.: 0.004 min
Response: 172813
Conc: 0.05 ng/ml

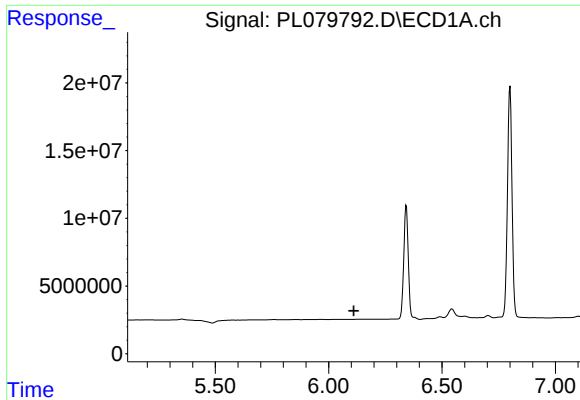

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

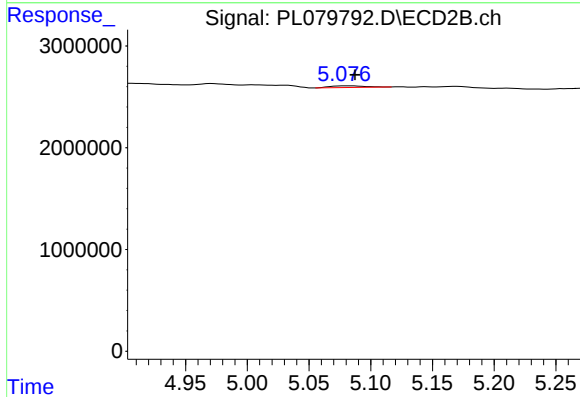


#13 Dieldrin

R.T.: 5.080 min
Delta R.T.: -0.008 min
Response: 316256
Conc: 0.09 ng/ml

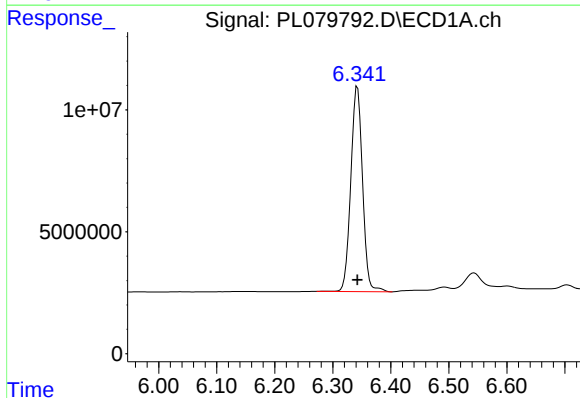


#14 Endrin

R.T.: 6.342 min
Delta R.T.: 0.000 min
Response: 118258881
Conc: 49.75 ng/ml

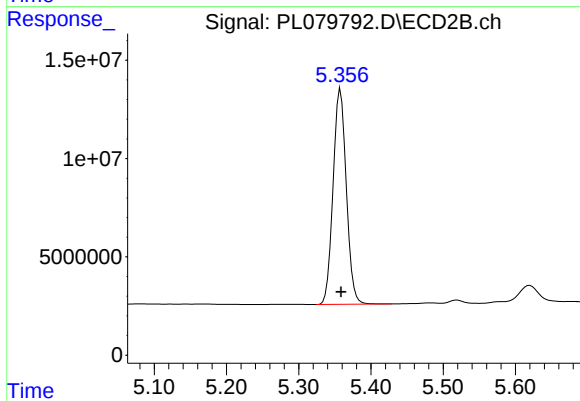

#14 Endrin


R.T.: 5.358 min
Delta R.T.: 0.000 min
Response: 139889627
Conc: 49.22 ng/ml

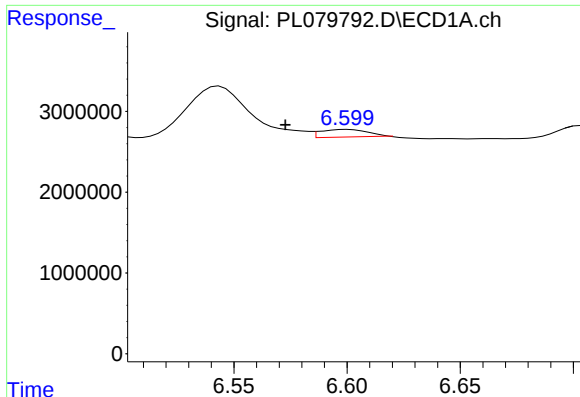

#15 Endosulfan II


R.T.: 6.600 min
Delta R.T.: 0.027 min
Response: 1424435
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

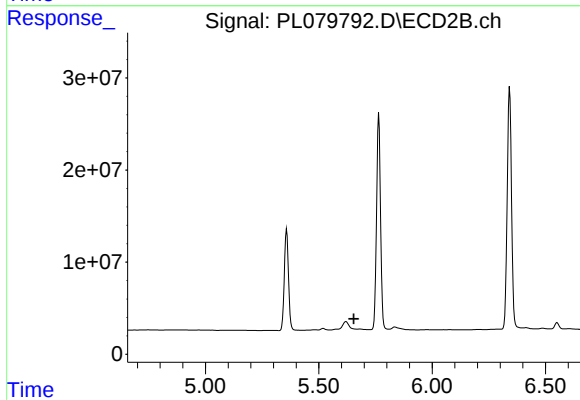


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.655 min
Response: 0
Conc: N.D.

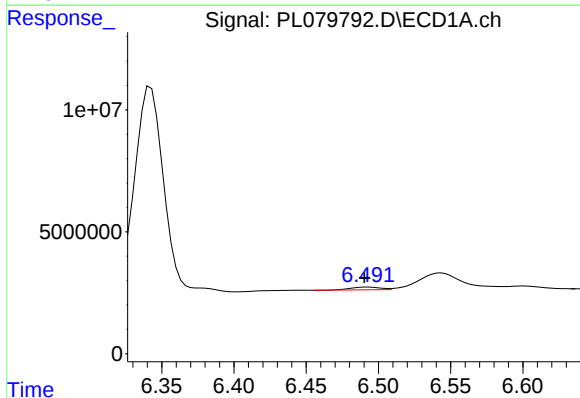


#16 4,4'-DDD

R.T.: 6.492 min
Delta R.T.: 0.002 min
Response: 1555413
Conc: 0.79 ng/ml

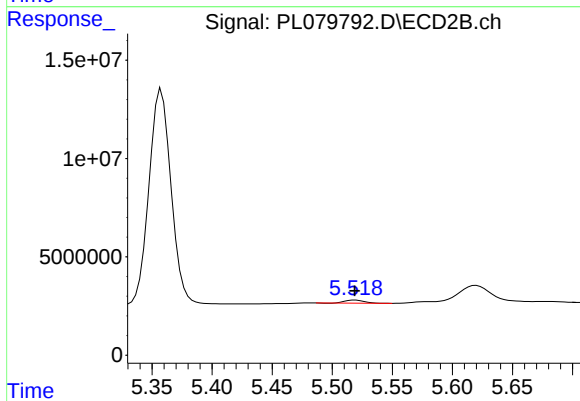

#16 4,4'-DDD


R.T.: 5.519 min
Delta R.T.: 0.000 min
Response: 1734054
Conc: 0.68 ng/ml

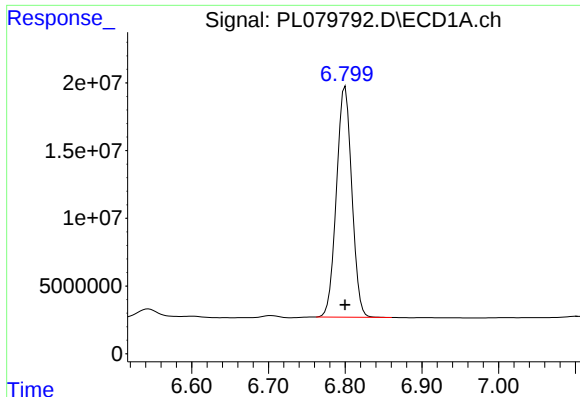

#17 4,4'-DDT


R.T.: 6.800 min
Delta R.T.: 0.000 min
Response: 237155590
Conc: 105.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

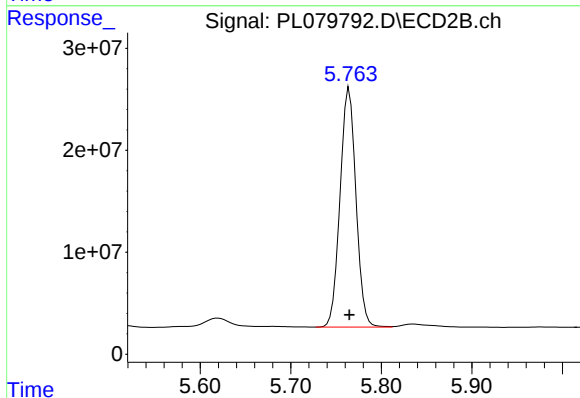


#17 4,4'-DDT

R.T.: 5.765 min
Delta R.T.: 0.000 min
Response: 286351897
Conc: 105.70 ng/ml

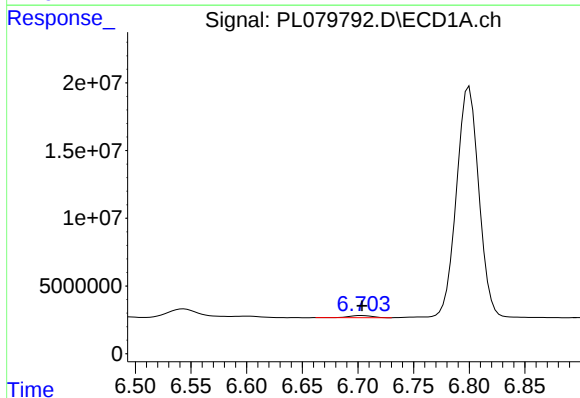


#18 Endrin aldehyde

R.T.: 6.704 min
Delta R.T.: 0.000 min
Response: 2217449
Conc: 1.25 ng/ml

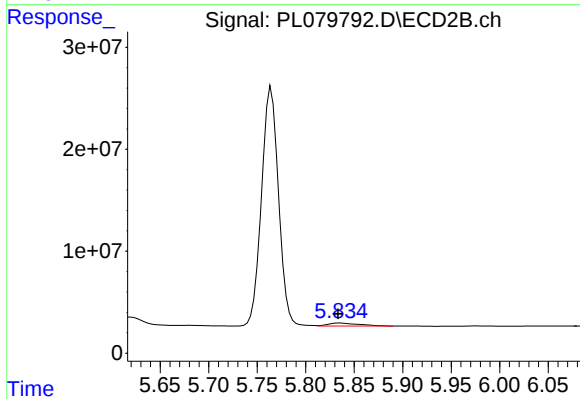

#18 Endrin aldehyde


R.T.: 5.835 min
Delta R.T.: 0.002 min
Response: 6293460
Conc: 2.81 ng/ml

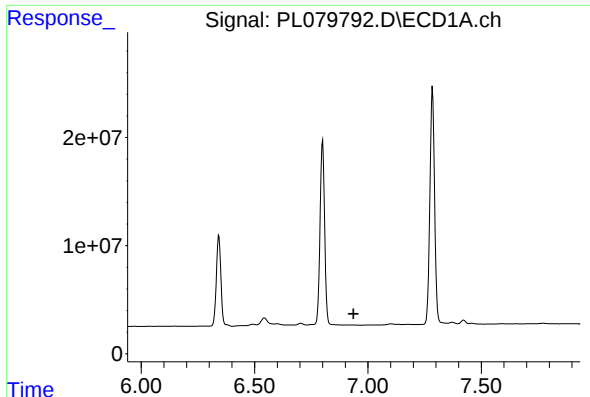

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

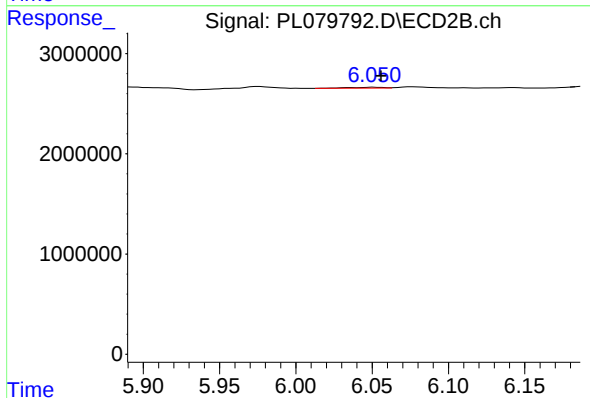


#19 Endosulfan Sulfate

R.T.: 6.051 min
Delta R.T.: -0.005 min
Response: 135848
Conc: 0.05 ng/ml

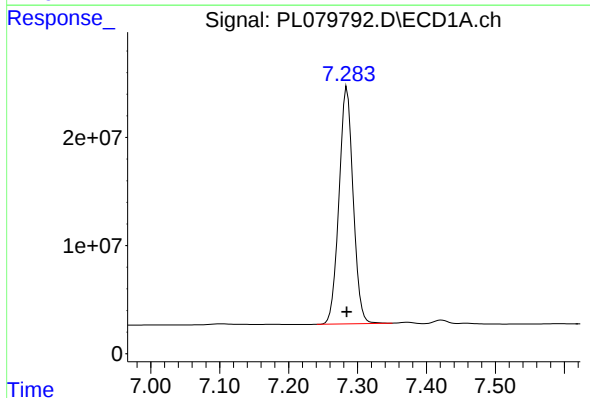


#20 Methoxychlor

R.T.: 7.285 min
Delta R.T.: 0.000 min
Response: 311940016
Conc: 264.64 ng/ml

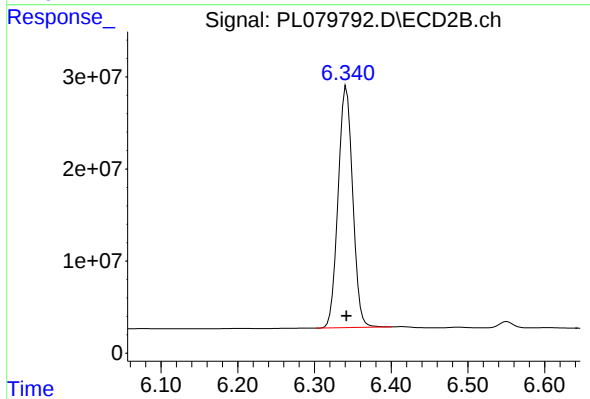

#20 Methoxychlor


R.T.: 6.342 min
Delta R.T.: 0.000 min
Response: 346646495
Conc: 244.45 ng/ml

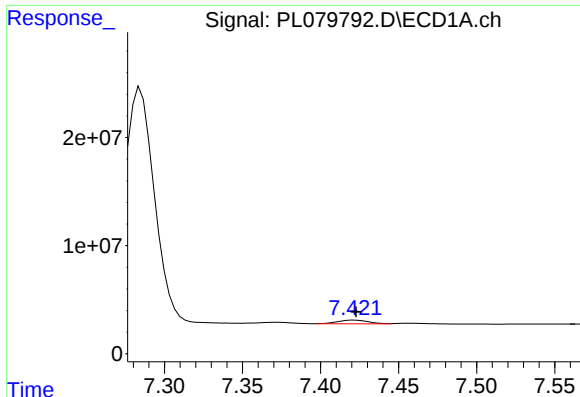

#21 Endrin ketone


R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 4682789
Conc: 1.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

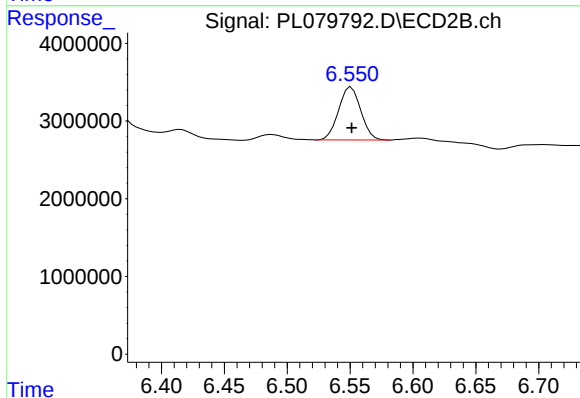


#21 Endrin ketone

R.T.: 6.551 min
Delta R.T.: 0.000 min
Response: 8318032
Conc: 2.60 ng/ml

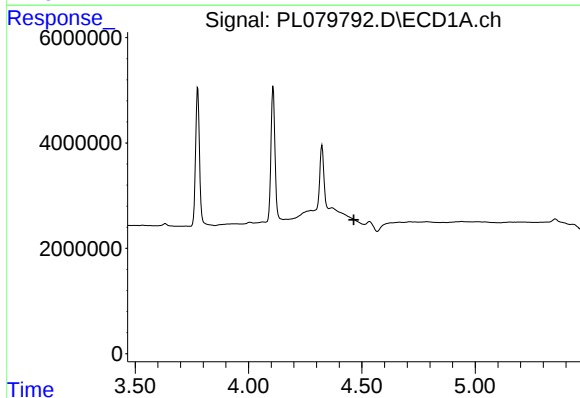


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.464 min
Response: 0
Conc: N.D.

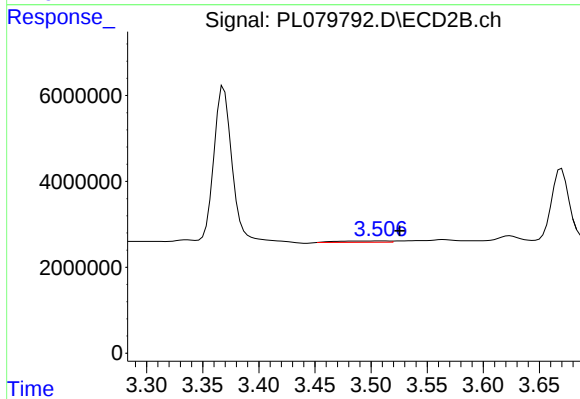

#23 Chlordane-1


R.T.: 3.507 min
Delta R.T.: -0.018 min
Response: 1021665
Conc: 9.78 ng/ml

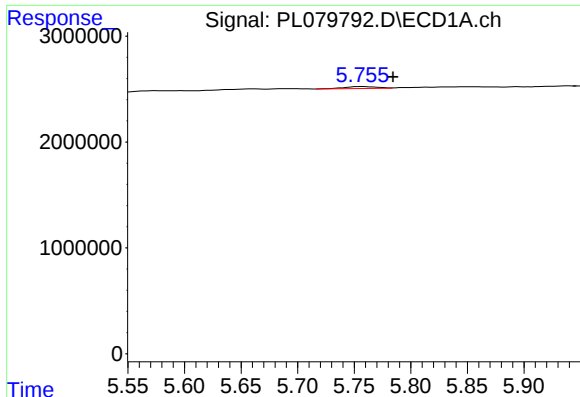

#26 Chlordane-4


R.T.: 5.756 min
Delta R.T.: -0.028 min
Response: 372273
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

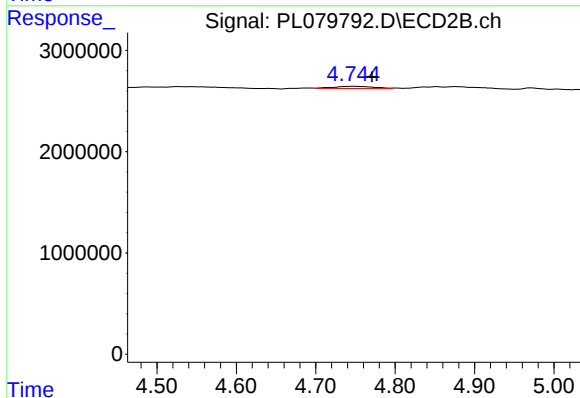


#26 Chlordane-4

R.T.: 4.746 min
Delta R.T.: -0.025 min
Response: 802643
Conc: 2.21 ng/ml

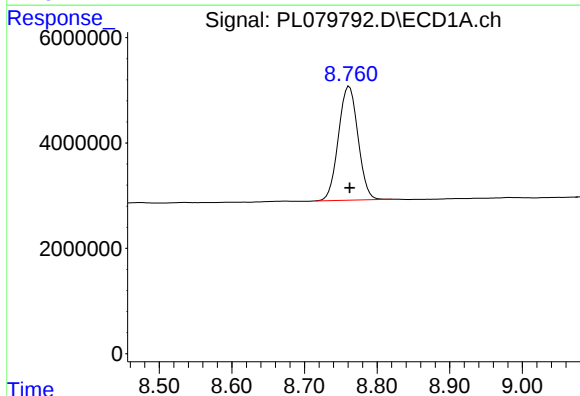

#28 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: 0.000 min
Response: 40485567
Conc: 21.83 ng/ml

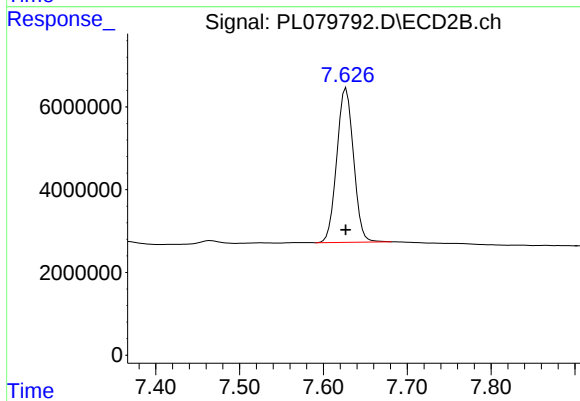

#28 Decachlorobiphenyl

R.T.: 7.627 min
Delta R.T.: 0.000 min
Response: 51735625
Conc: 21.55 ng/ml