

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
 Data File : PL079803.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 17:34
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 01:46:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 21 01:39:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	2.561	10490350	16329114	4.920	5.175
28)	SA Decachlor...	8.764	7.628	9759090	13242533	5.291	5.570
Target Compounds							
23)	Chlordane-1	4.464	3.526	4210087	5774072	45.977	55.291
24)	Chlordane-2	4.998	4.092	5504237	6399964	54.826	56.047
25)	Chlordane-3	5.707	4.712	19515518	17313787	49.572	51.135
26)	Chlordane-4	5.785	4.772	24173746	19012718	50.385	52.461
27)	Chlordane-5	6.640	5.433	3041892	4192991	38.238	45.029



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
Data File : PL079803.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 17:34
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 01:46:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
Quant Title : GC Extractables
QLast Update : Wed Dec 21 01:39:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

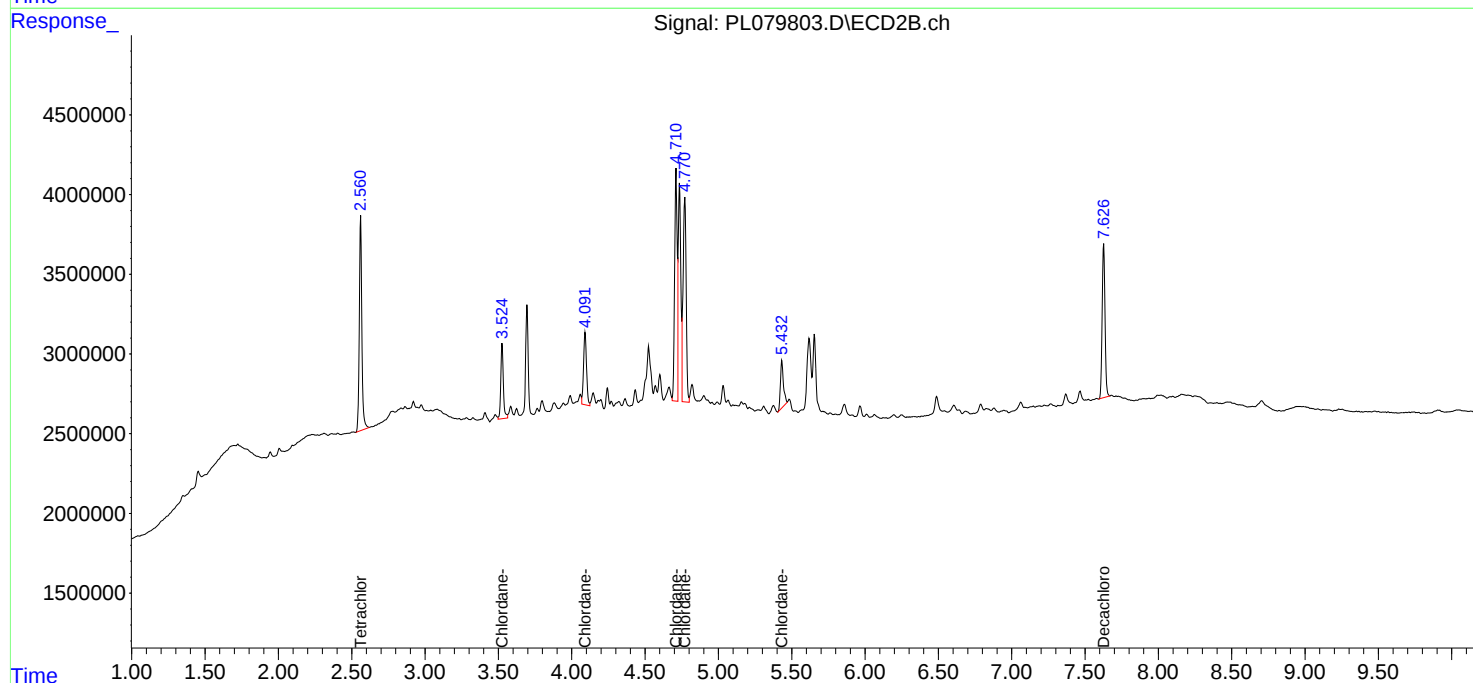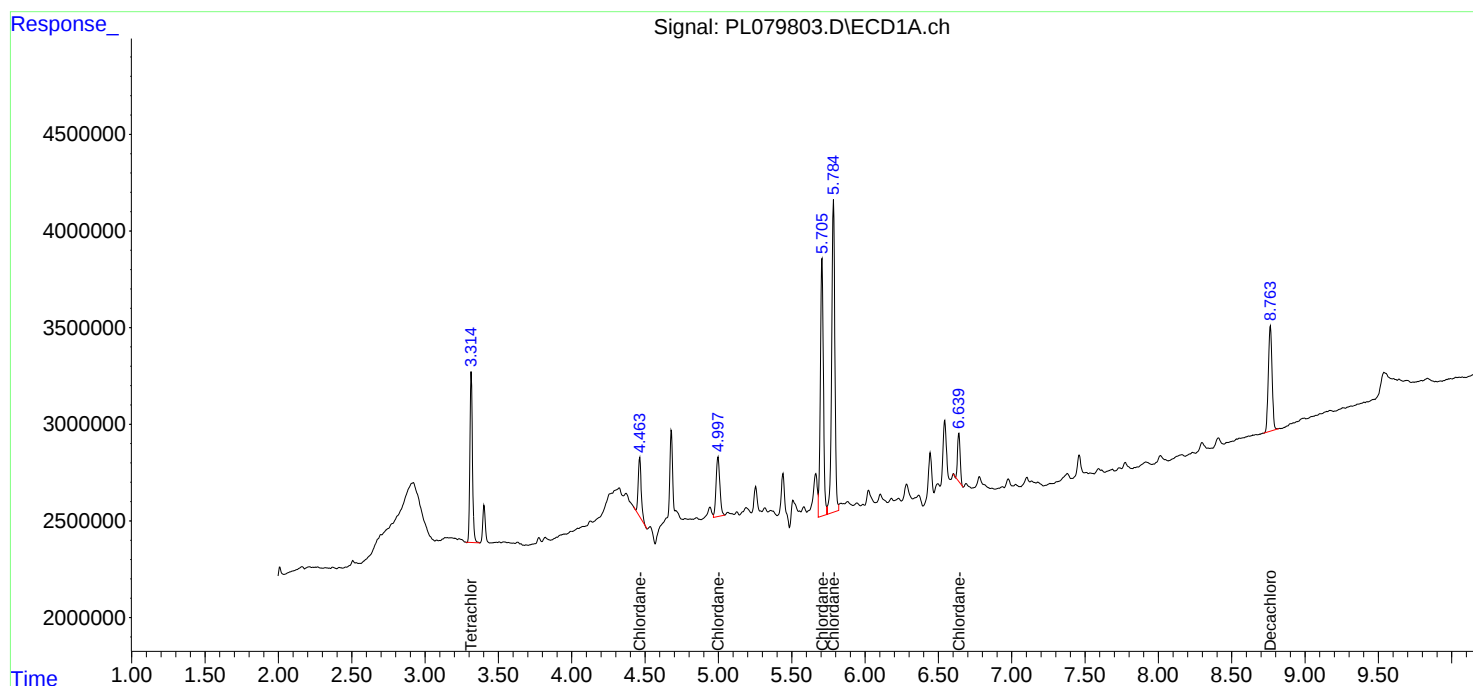


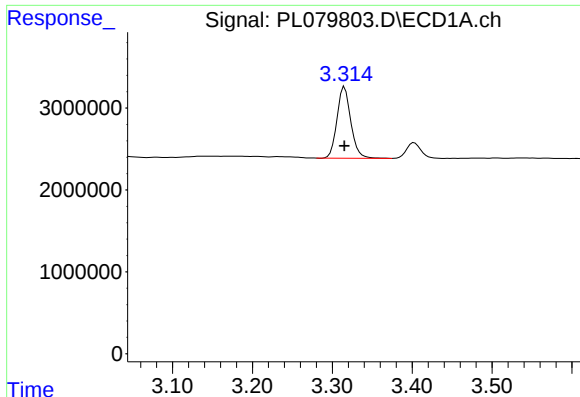

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 10490350
Conc: 4.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

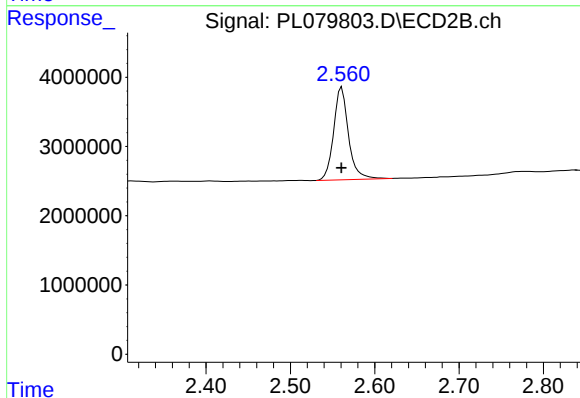


#1 Tetrachloro-m-xylene

R.T.: 2.561 min
Delta R.T.: 0.000 min
Response: 16329114
Conc: 5.18 ng/ml

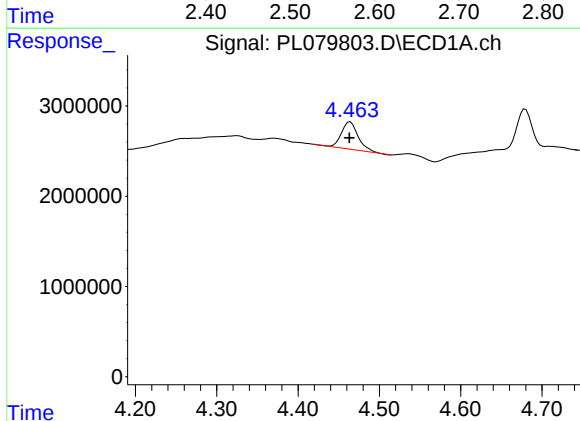


#23 Chlordane-1

R.T.: 4.464 min
Delta R.T.: 0.001 min
Response: 4210087
Conc: 45.98 ng/ml

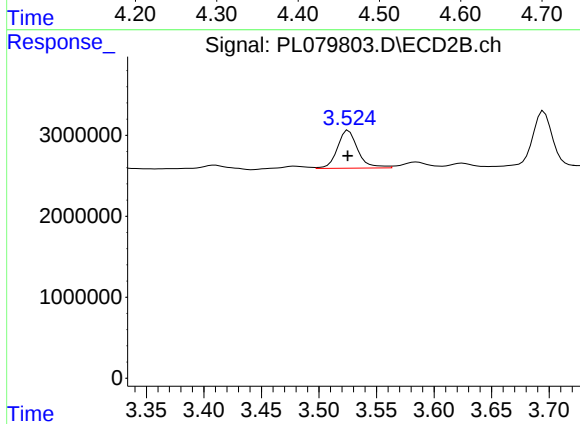

#23 Chlordane-1


R.T.: 3.526 min
Delta R.T.: 0.000 min
Response: 5774072
Conc: 55.29 ng/ml

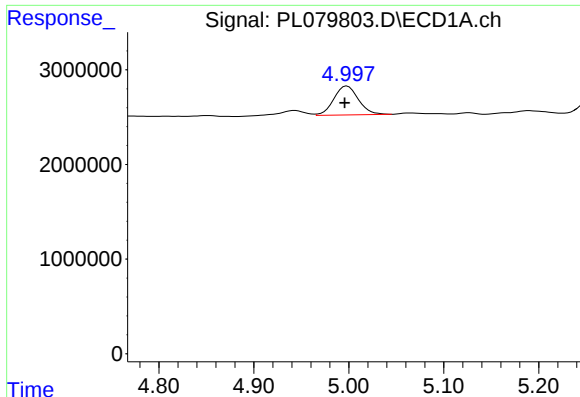

#24 Chlordane-2


R.T.: 4.998 min
Delta R.T.: 0.002 min
Response: 5504237
Conc: 54.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

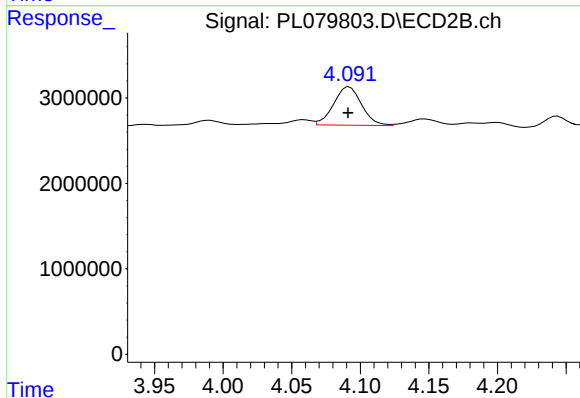


#24 Chlordane-2

R.T.: 4.092 min
Delta R.T.: 0.001 min
Response: 6399964
Conc: 56.05 ng/ml

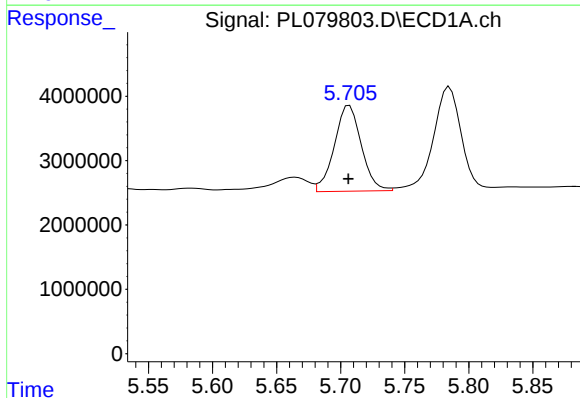


#25 Chlordane-3

R.T.: 5.707 min
Delta R.T.: 0.000 min
Response: 19515518
Conc: 49.57 ng/ml

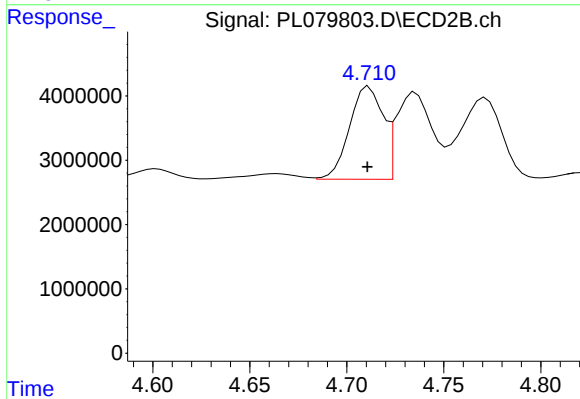

#25 Chlordane-3


R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 17313787
Conc: 51.14 ng/ml

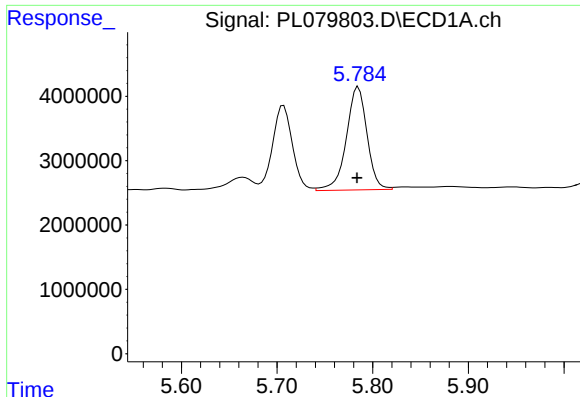

#26 Chlordane-4


R.T.: 5.785 min
Delta R.T.: 0.001 min
Response: 24173746
Conc: 50.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

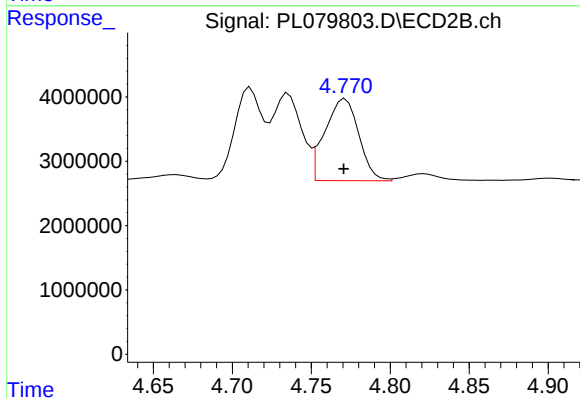


#26 Chlordane-4

R.T.: 4.772 min
Delta R.T.: 0.000 min
Response: 19012718
Conc: 52.46 ng/ml

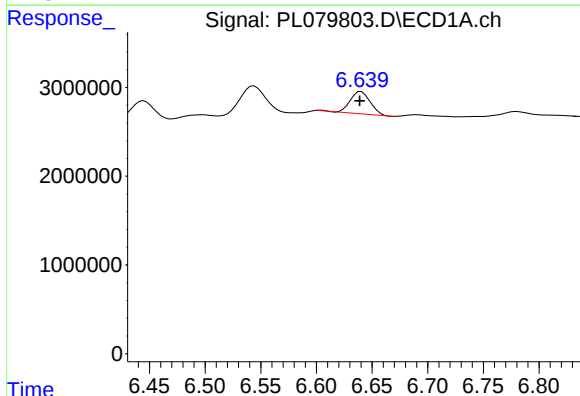


#27 Chlordane-5

R.T.: 6.640 min
Delta R.T.: 0.001 min
Response: 3041892
Conc: 38.24 ng/ml

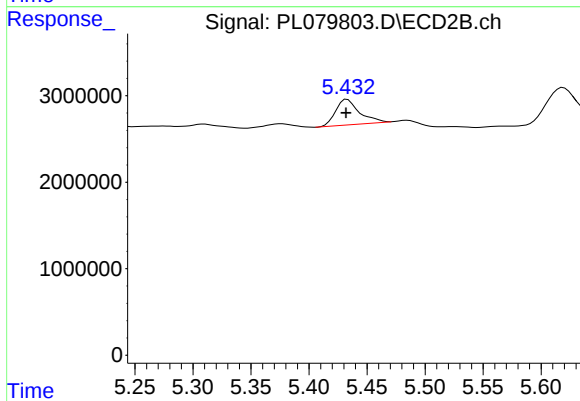

#27 Chlordane-5


R.T.: 5.433 min
Delta R.T.: 0.001 min
Response: 4192991
Conc: 45.03 ng/ml

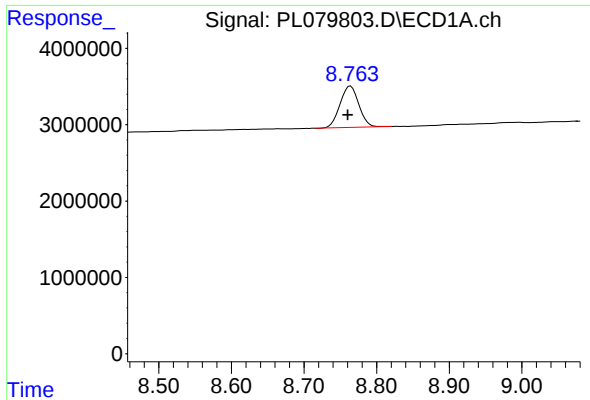

#28 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: 0.004 min
Response: 9759090
Conc: 5.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

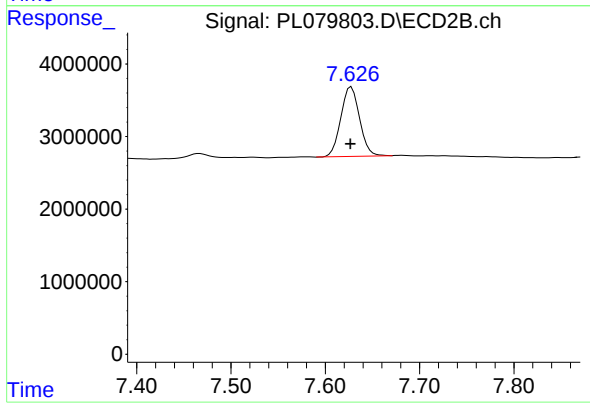

#28 Decachlorobiphenyl

R.T.: 7.628 min
Delta R.T.: 0.000 min
Response: 13242533
Conc: 5.57 ng/ml